

Test Laboratory: The name of your organization

D1900V2 SN5d043_031604

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d043

Ambient temperature = 23.5 deg. C; Liquid temperature = 22.0 deg. C

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.45$ mho/m; $\epsilon_r = 39.5$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 - SN3021; ConvF(5.1, 5.1, 5.1); Calibrated: 7/29/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn500; Calibrated: 12/23/2003
- Phantom: SAM 1; Type: SAM 1; Serial: 1185
- Measurement SW: DASY4, V4.2 Build 37; Postprocessing SW: SEMCAD, V1.8 Build 109

d=10mm; Pin=250mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm

Reference Value = 90.2 V/m; Power Drift = 0.0 dB

Maximum value of SAR (measured) = 11.2 mW/g


d=10mm; Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm

Reference Value = 90.2 V/m; Power Drift = 0.0 dB

Maximum value of SAR (measured) = 11.3 mW/g

Peak SAR (extrapolated) = 18.1 W/kg

SAR(1 g) = 10 mW/g; SAR(10 g) = 5.22 mW/g

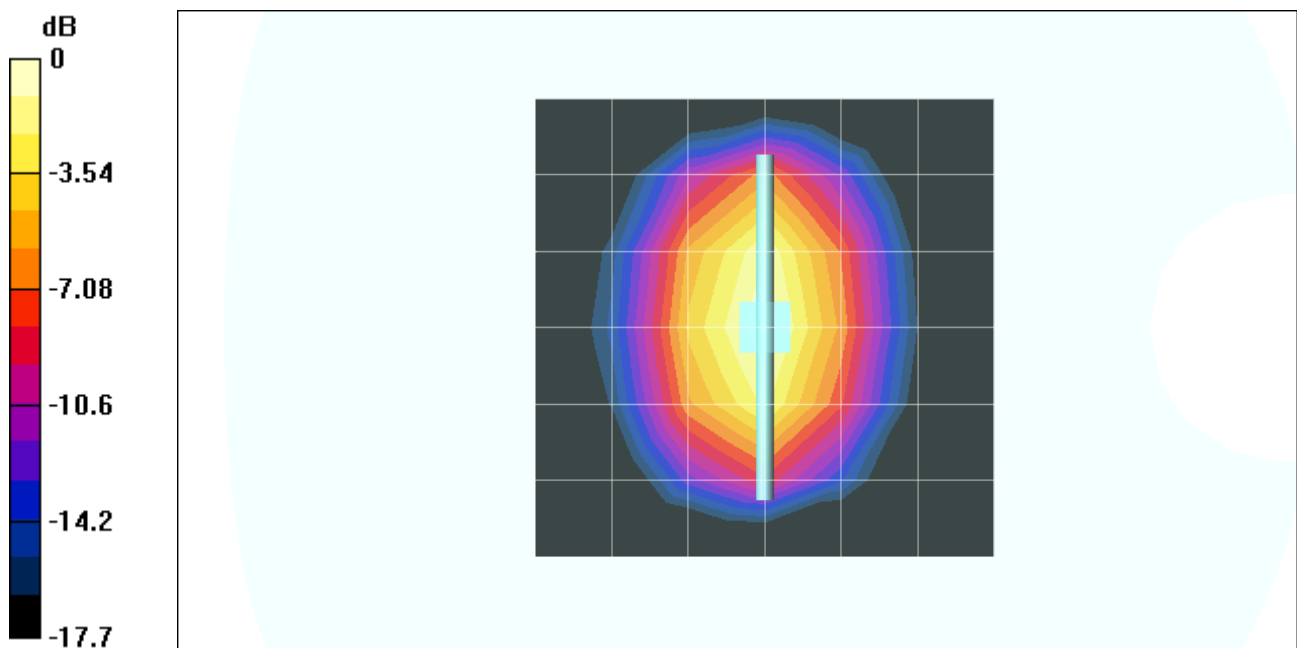

0 dB = 11.3mW/g

Test Laboratory: The name of your organization

D1900V2 SN5d043_031604

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d043

DASY4 Configuration:

- Probe: ES3DV2 - SN3021; ConvF(5.1, 5.1, 5.1); Calibrated: 7/29/2003
- Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE3 Sn500; Calibrated: 12/23/2003
- Phantom: SAM 1; Type: SAM 1; Serial: 1185
- Measurement SW: DASY4, V4.2 Build 37; Postprocessing SW: SEMCAD, V1.8 Build 109

d=10mm; Pin=250mW/Z Scan (1x1x51): Measurement grid: dx=20mm, dy=20mm, dz=2mm

Reference Value = 90.2 V/m; Power Drift = 0.0 dB

Maximum value of SAR (measured) = 11.7 mW/g

