




INTERNAL PHOTO OF SAMPLE -1

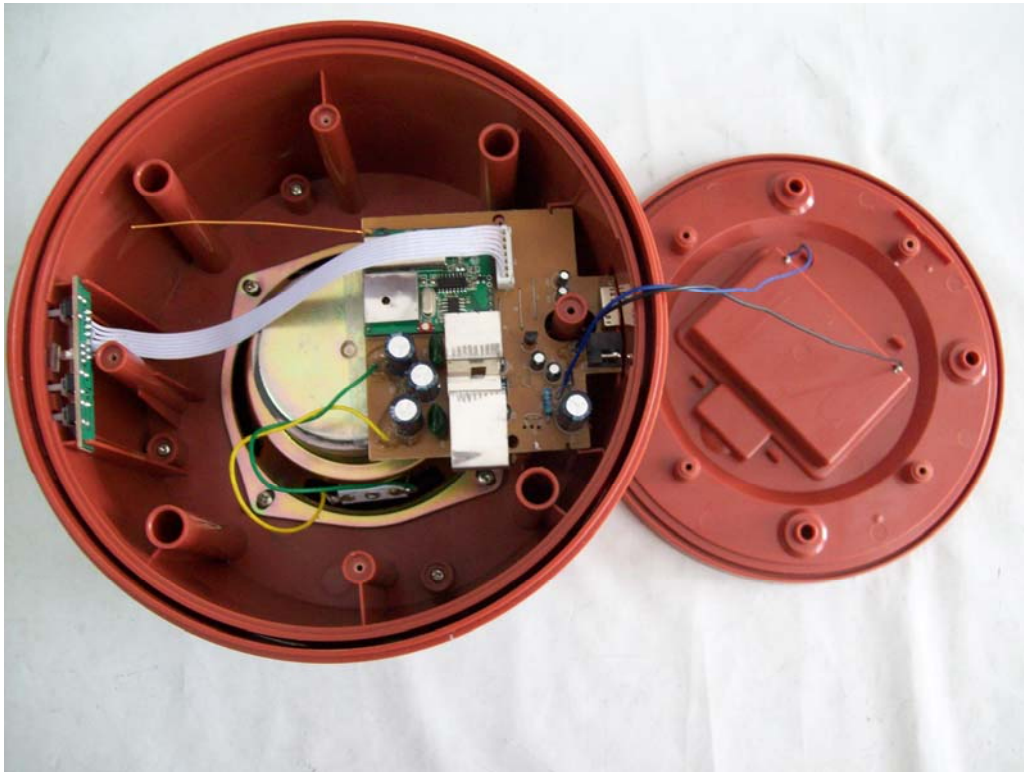


INTERNAL PHOTO OF SAMPLE -2

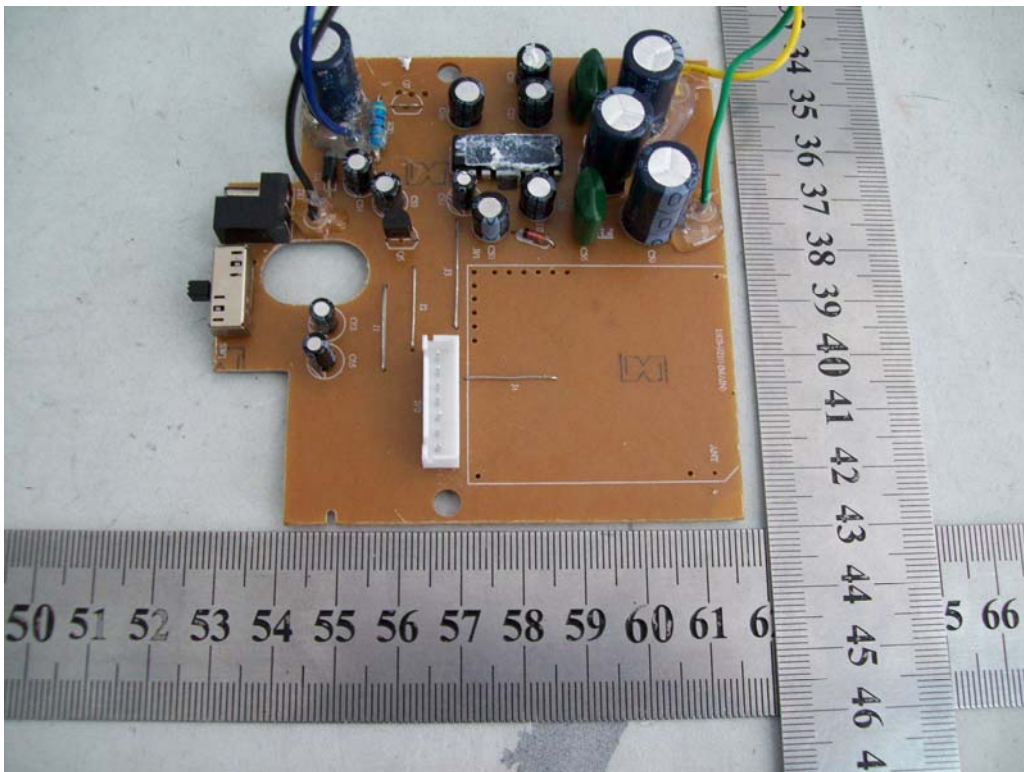

INTERNAL PHOTO OF SAMPLE -3

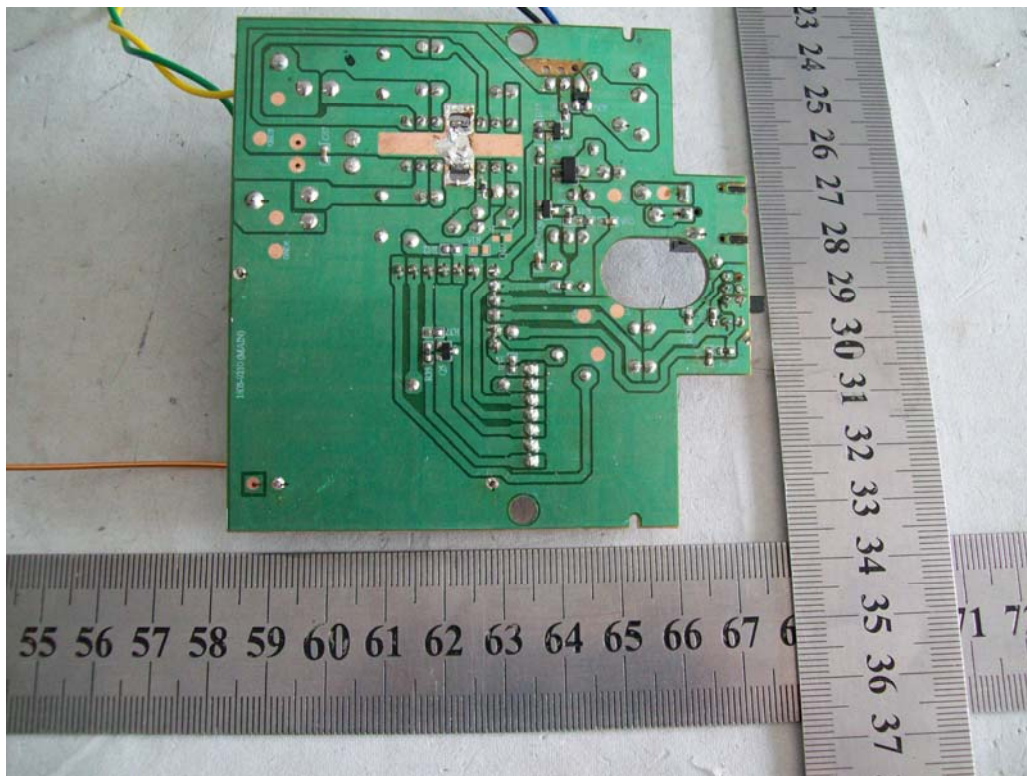


INTERNAL PHOTO OF SAMPLE -4

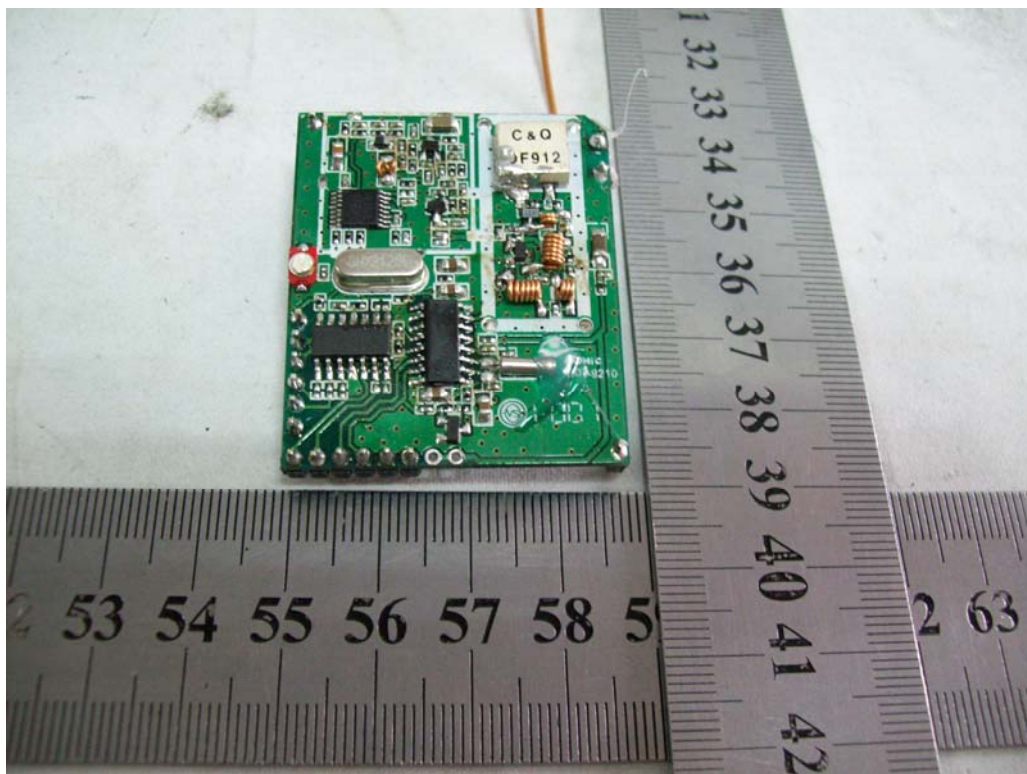




INTERNAL PHOTO OF SAMPLE - 5

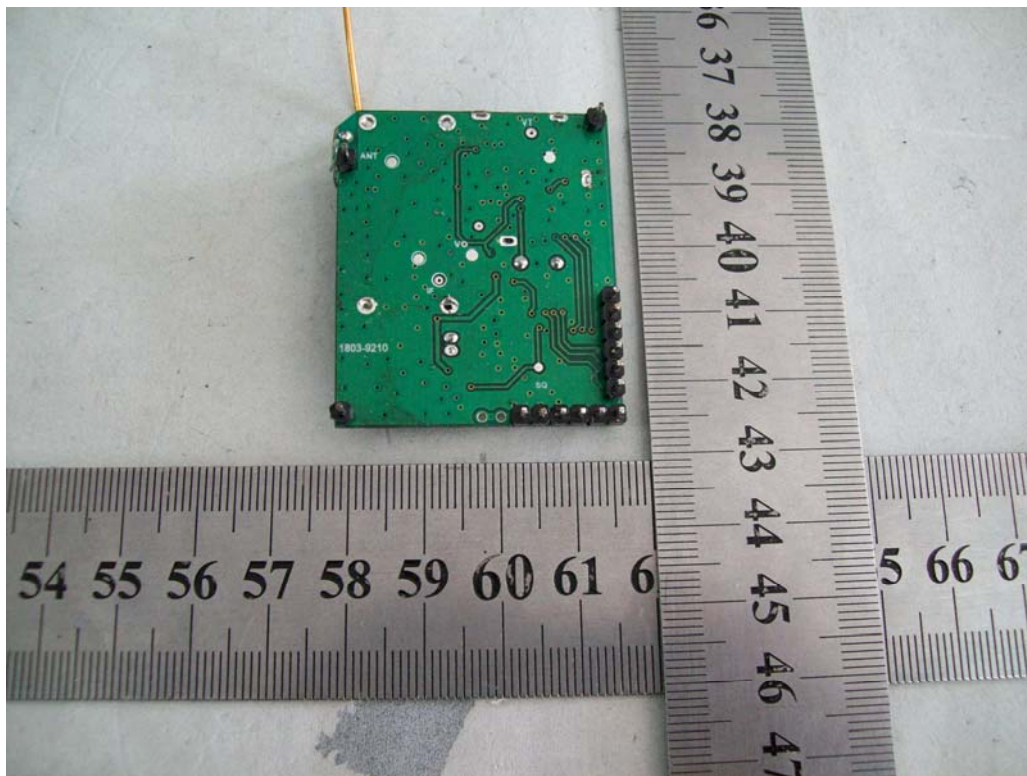

INTERNAL PHOTO OF THE ADAPTER -1

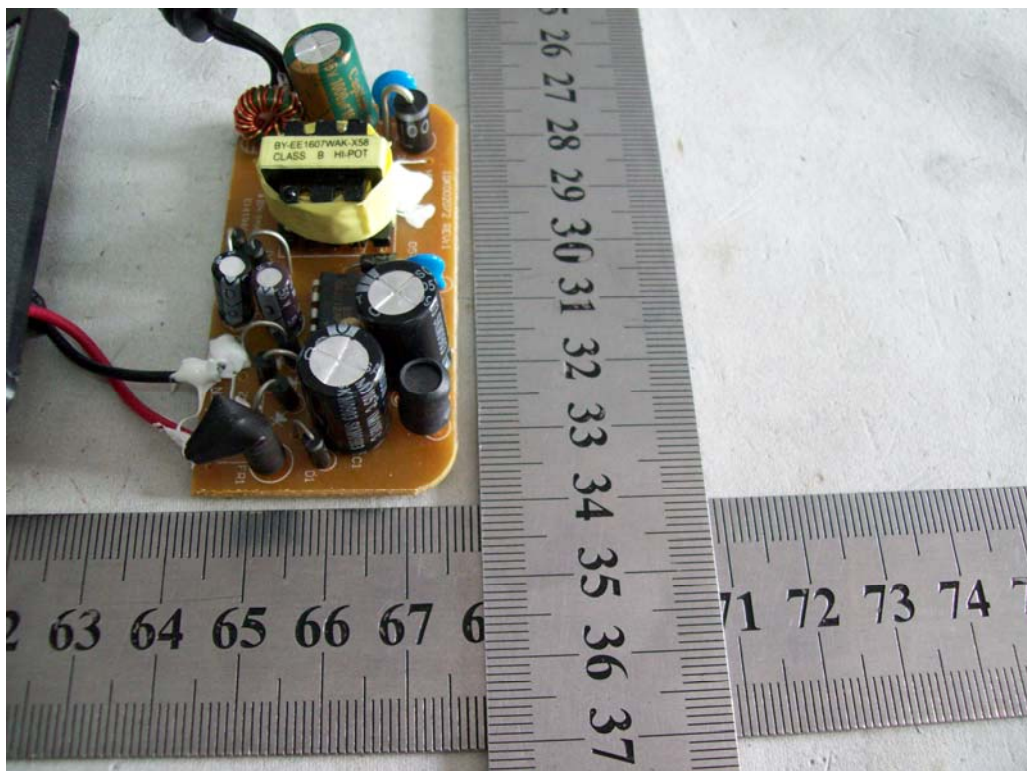

INTERNAL PHOTO OF THE ADAPTER-2

