

Telian Corporation, Model No: FTD8500
 FCC ID: NPQFTD8500


APPENDIX A - E-Field Probe Calibration Data

Calibration Laboratory of
 Schmid & Partner
 Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland

Client

ITS / ETL

CALIBRATION CERTIFICATE

Object(s)	ET3DV6 - SN:1785		
Calibration procedure(s)	QA CAL-01.v2 Calibration procedure for dosimetric E-field probes		
Calibration date:	July 28, 2003		
Condition of the calibrated item	In Tolerance (according to the specific calibration document)		
<p>This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p>			
Model Type	ID #	Cal Data (Calibrated by, Certificate No.)	Scheduled Calibration
RF generator HP 8684C	US3642U01700	4-Aug-99 (SPEAG, in house check Aug-02)	In house check: Aug-05
Power sensor E4412A	MY41495277	2-Apr-03 (METAS, No. 252-0250)	Apr-04
Power sensor HP 8481A	MY41092180	18-Sep-02 (Agilent, No. 20020918)	Sep-03
Power meter EPM E4419B	GB41293874	2-Apr-03 (METAS, No. 252-0250)	Apr-04
Network Analyzer HP 8753E	US37390585	18-Oct-01 (Agilent, No. 24BR1033101)	In house check: Oct 03
Fluke Process Calibrator Type 702	SN: 6295803	3-Sep-01 (ELCAL, No. 2360)	Sep-03
Calibrated by:	Name Nico Vetterli	Function Technician	Signature 
Approved by:	Katja Pokovic	Laboratory Director	
Date issued: July 28, 2003			
<p>This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.</p>			

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 1 245 9700, Fax +41 1 245 9779
info@speag.com, http://www.speag.com

Probe ET3DV6

SN:1785

Manufactured: May 28, 2003
Last calibration: July 28, 2003

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

ET3DV6 SN:1785

July 28, 2003

DASY - Parameters of Probe: ET3DV6 SN:1785

Sensitivity in Free Space

Diode Compression

NormX	1.70 $\mu\text{V}/(\text{V}/\text{m})^2$	DCP X	97	mV
NormY	1.70 $\mu\text{V}/(\text{V}/\text{m})^2$	DCP Y	97	mV
NormZ	1.63 $\mu\text{V}/(\text{V}/\text{m})^2$	DCP Z	97	mV

Sensitivity in Tissue Simulating Liquid

Head 900 MHz $\epsilon_r = 41.5 \pm 5\%$ $\sigma = 0.97 \pm 5\% \text{ mho/m}$

Valid for f=800-1000 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	6.6 $\pm 9.5\% \text{ (k=2)}$	Boundary effect:	
ConvF Y	6.6 $\pm 9.5\% \text{ (k=2)}$	Alpha	0.42
ConvF Z	6.6 $\pm 9.5\% \text{ (k=2)}$	Depth	2.27

Head 1800 MHz $\epsilon_r = 40.0 \pm 5\%$ $\sigma = 1.40 \pm 5\% \text{ mho/m}$

Valid for f=1710-1910 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	5.2 $\pm 9.5\% \text{ (k=2)}$	Boundary effect:	
ConvF Y	5.2 $\pm 9.5\% \text{ (k=2)}$	Alpha	0.49
ConvF Z	5.2 $\pm 9.5\% \text{ (k=2)}$	Depth	2.55

Boundary Effect

Head 900 MHz Typical SAR gradient: 5 % per mm

Probe Tip to Boundary		1 mm	2 mm
SAR _{be} [%]	Without Correction Algorithm	9.1	5.1
SAR _{be} [%]	With Correction Algorithm	0.2	0.4

Head 1800 MHz Typical SAR gradient: 10 % per mm

Probe Tip to Boundary		1 mm	2 mm
SAR _{be} [%]	Without Correction Algorithm	12.8	8.6
SAR _{be} [%]	With Correction Algorithm	0.2	0.1


Sensor Offset

Probe Tip to Sensor Center	2.7	mm
Optical Surface Detection	1.7 ± 0.2	mm

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

ET3DV6 SN:1785



July 28, 2003

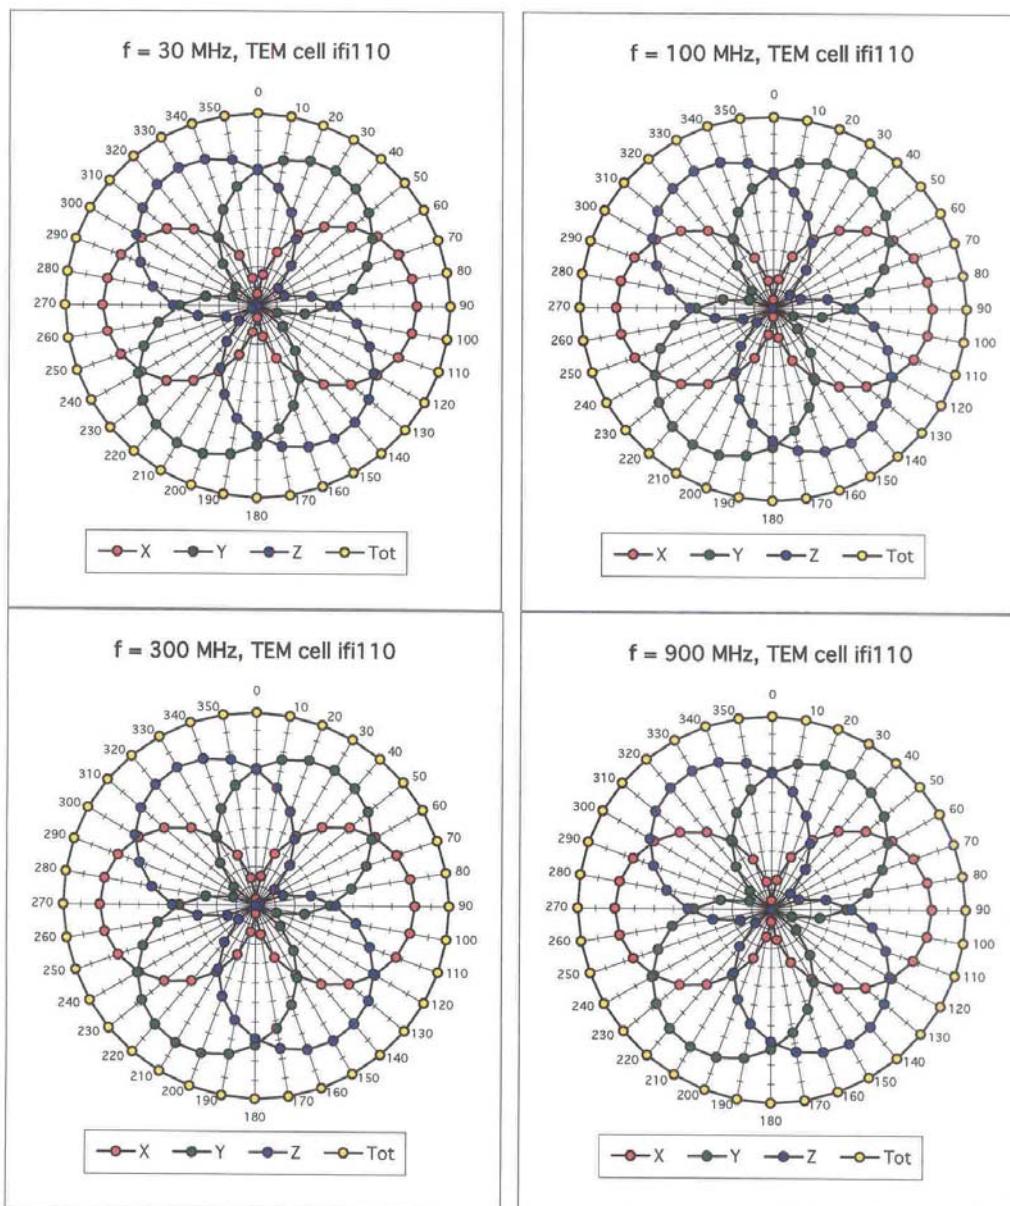Receiving Pattern (ϕ), $\theta = 0^\circ$ 

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

ET3DV6 SN:1785

July 28, 2003

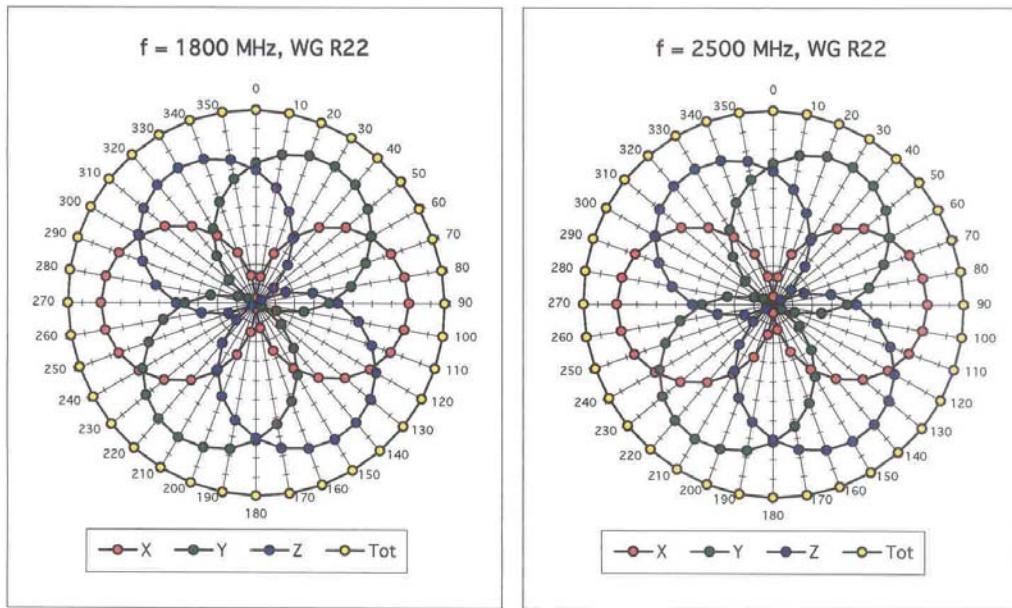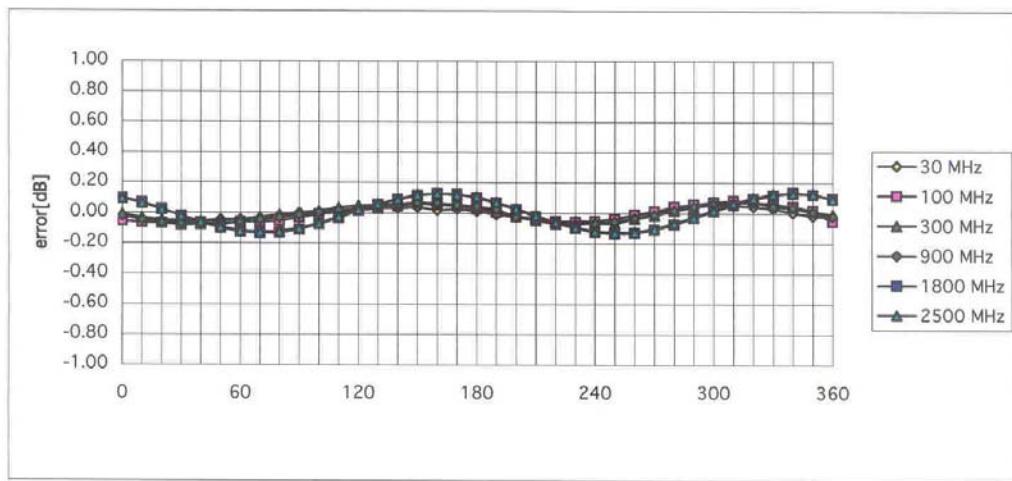Isotropy Error (ϕ), $\theta = 0^\circ$ 


Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

ET3DV6 SN:1785

July 28, 2003

Frequency Response of E-Field

(TEM-Cell:ifi110, Waveguide R22)

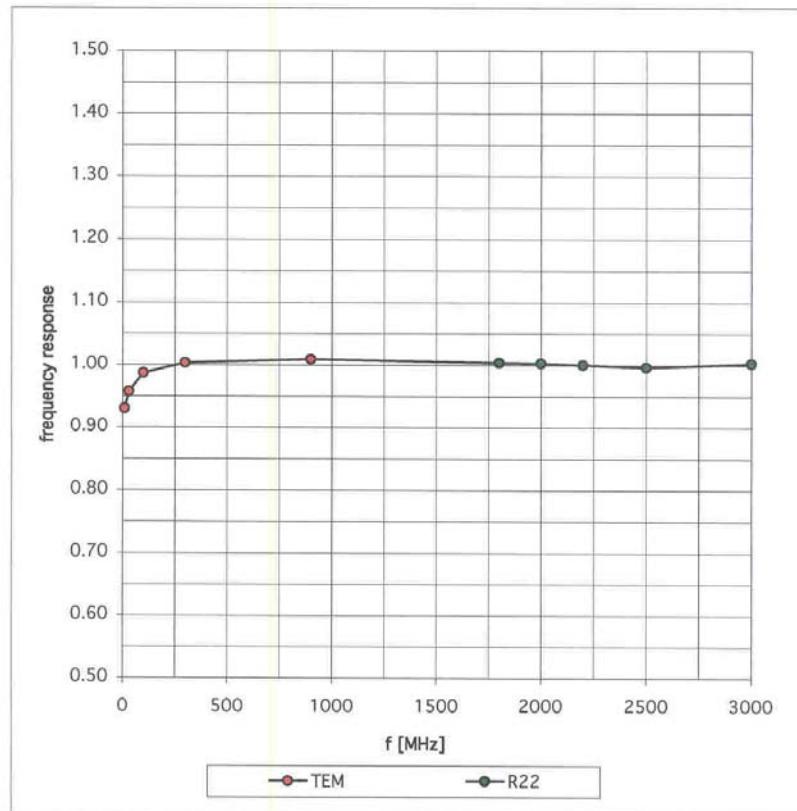



Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

ET3DV6 SN:1785

July 28, 2003

Dynamic Range $f(\text{SAR}_{\text{brain}})$

(Waveguide R22)

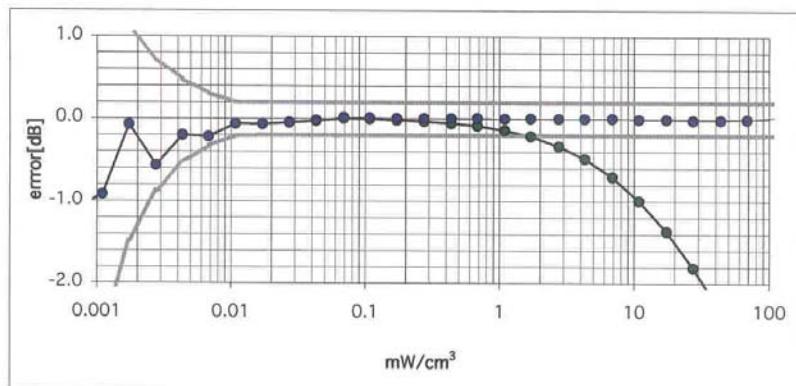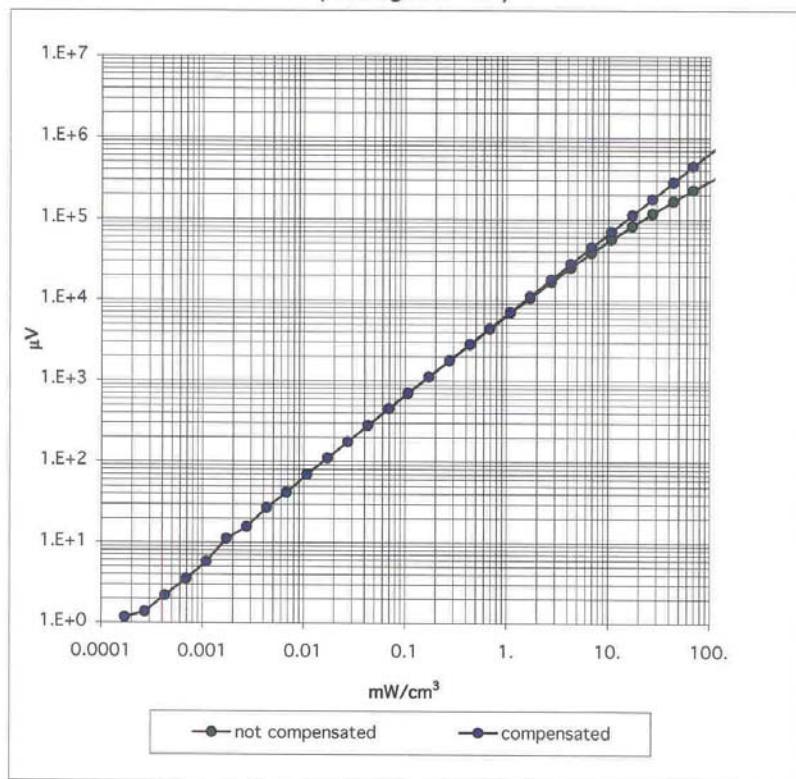


Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

ET3DV6 SN:1785

July 28, 2003

Conversion Factor Assessment

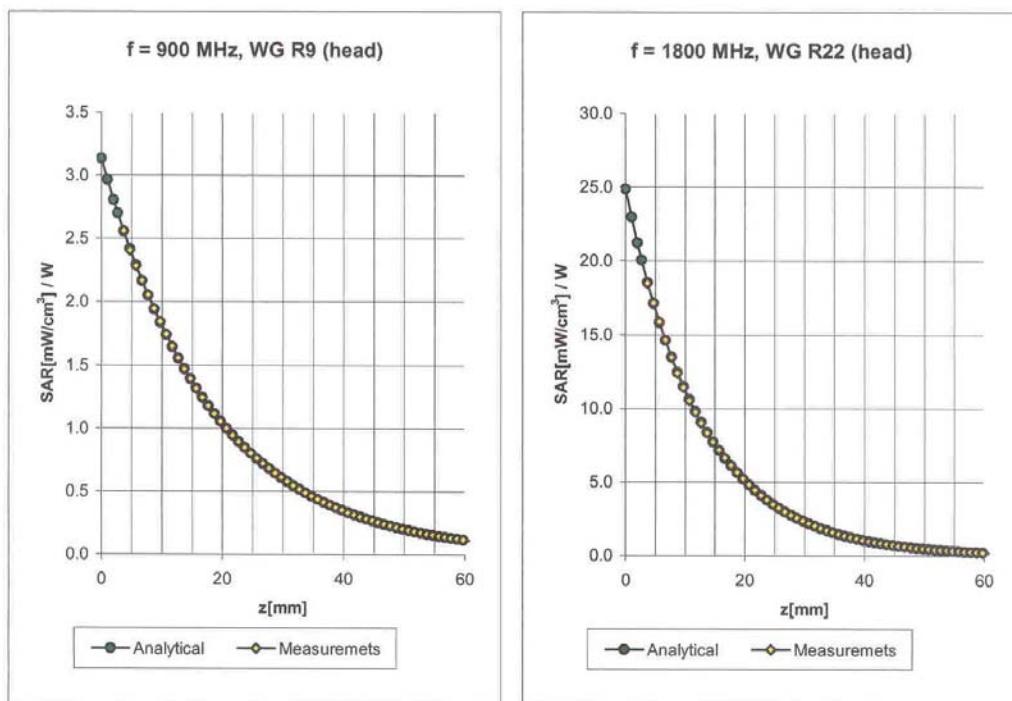

Head

900 MHz

 $\epsilon_r = 41.5 \pm 5\%$ $\sigma = 0.97 \pm 5\% \text{ mho/m}$

Valid for f=800-1000 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X

6.6 $\pm 9.5\%$ (k=2)

Boundary effect:

ConvF Y

6.6 $\pm 9.5\%$ (k=2)

Alpha

0.42

ConvF Z

6.6 $\pm 9.5\%$ (k=2)

Depth

2.27

Head

1800 MHz

 $\epsilon_r = 40.0 \pm 5\%$ $\sigma = 1.40 \pm 5\% \text{ mho/m}$

Valid for f=1710-1910 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X

5.2 $\pm 9.5\%$ (k=2)

Boundary effect:

ConvF Y

5.2 $\pm 9.5\%$ (k=2)

Alpha

0.49

ConvF Z

5.2 $\pm 9.5\%$ (k=2)

Depth


2.55

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

ET3DV6 SN:1785

July 28, 2003

Conversion Factor Assessment

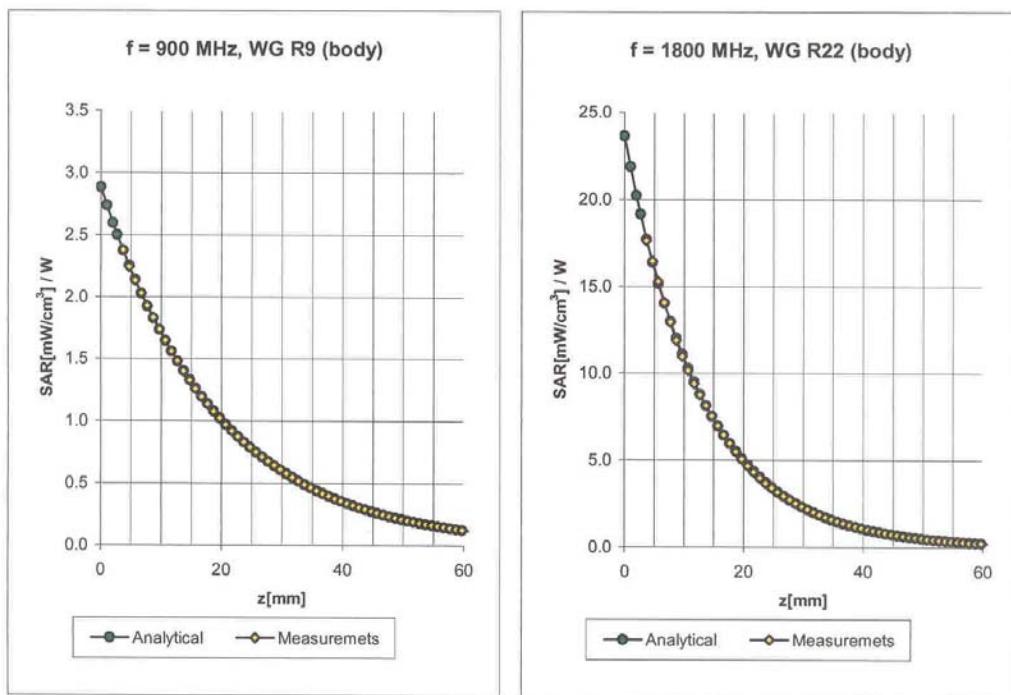

Body

900 MHz

 $\epsilon_r = 55.0 \pm 5\%$ $\sigma = 1.05 \pm 5\% \text{ mho/m}$

Valid for f=855-945 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X

6.3 $\pm 8.9\% \text{ (k=2)}$

Boundary effect:

ConvF Y

6.3 $\pm 8.9\% \text{ (k=2)}$

Alpha

0.43

ConvF Z

6.3 $\pm 8.9\% \text{ (k=2)}$

Depth

2.32

Body

1800 MHz

 $\epsilon_r = 53.3 \pm 5\%$ $\sigma = 1.52 \pm 5\% \text{ mho/m}$

Valid for f=1710-1890 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X

4.9 $\pm 8.9\% \text{ (k=2)}$

Boundary effect:

ConvF Y

4.9 $\pm 8.9\% \text{ (k=2)}$

Alpha

0.55

ConvF Z

4.9 $\pm 8.9\% \text{ (k=2)}$

Depth


2.70

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

ET3DV6 SN:1785

July 28, 2003

Conversion Factor Assessment

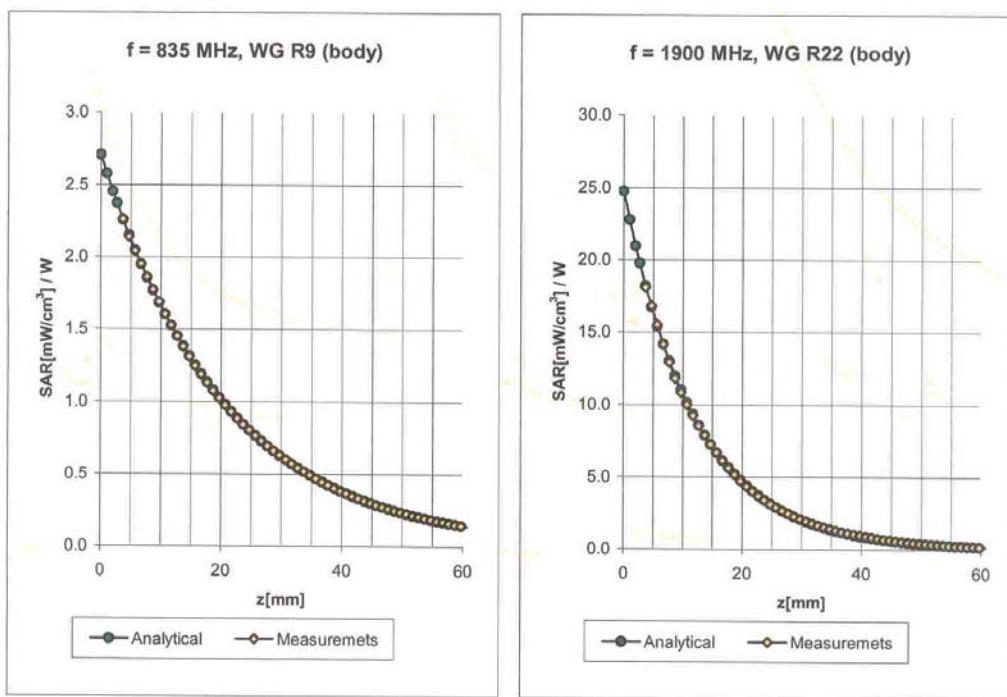

Body

835 MHz

 $\epsilon_r = 55.2 \pm 5\%$ $\sigma = 0.97 \pm 5\% \text{ mho/m}$

Valid for f=793-877 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X

6.3 $\pm 8.9\%$ (k=2)

Boundary effect:

ConvF Y

6.3 $\pm 8.9\%$ (k=2)

Alpha

0.45

ConvF Z

6.3 $\pm 8.9\%$ (k=2)

Depth

2.17

Body

1900 MHz

 $\epsilon_r = 53.3 \pm 5\%$ $\sigma = 1.52 \pm 5\% \text{ mho/m}$

Valid for f=1805-1995 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X

4.7 $\pm 8.9\%$ (k=2)

Boundary effect:

ConvF Y

4.7 $\pm 8.9\%$ (k=2)

Alpha

0.61

ConvF Z

4.7 $\pm 8.9\%$ (k=2)

Depth


2.46

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

ET3DV6 SN:1785

July 28, 2003

Conversion Factor Assessment

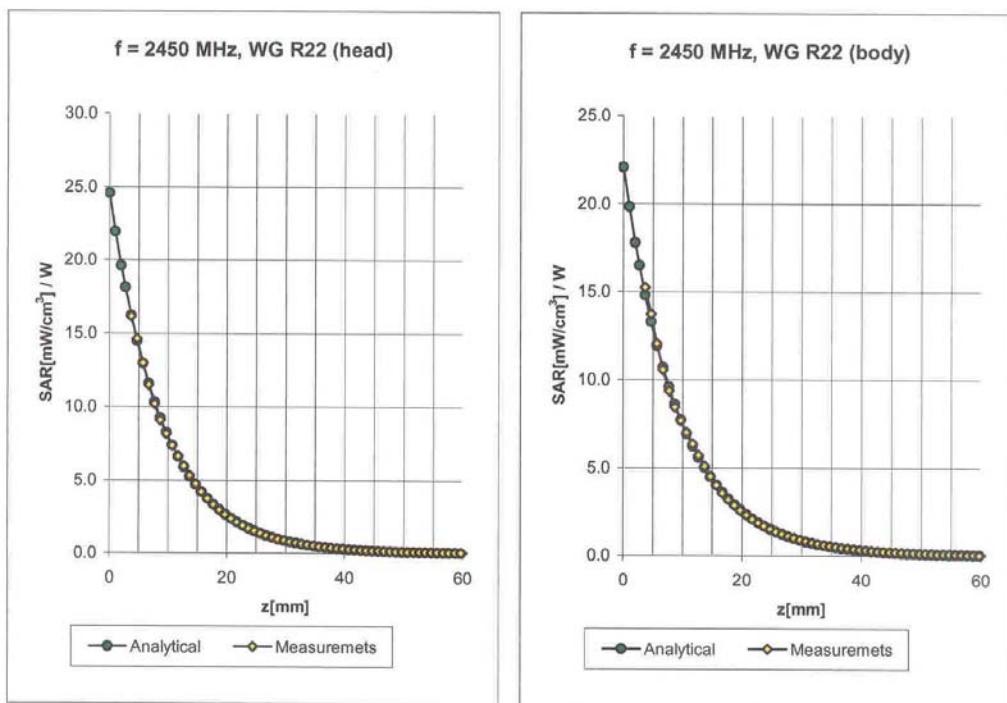

Head 2450 MHz $\epsilon_r = 39.2 \pm 5\%$ $\sigma = 1.80 \pm 5\% \text{ mho/m}$

Valid for f=2400-2500 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	4.8 $\pm 8.9\%$ (k=2)	Boundary effect:
ConvF Y	4.8 $\pm 8.9\%$ (k=2)	Alpha 1.01
ConvF Z	4.8 $\pm 8.9\%$ (k=2)	Depth 1.83

Body 2450 MHz $\epsilon_r = 52.7 \pm 5\%$ $\sigma = 1.95 \pm 5\% \text{ mho/m}$

Valid for f=2400-2500 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C


ConvF X	4.4 $\pm 8.9\%$ (k=2)	Boundary effect:
ConvF Y	4.4 $\pm 8.9\%$ (k=2)	Alpha 1.05
ConvF Z	4.4 $\pm 8.9\%$ (k=2)	Depth 1.66

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

ET3DV6 SN:1785

July 28, 2003

Conversion Factor Assessment

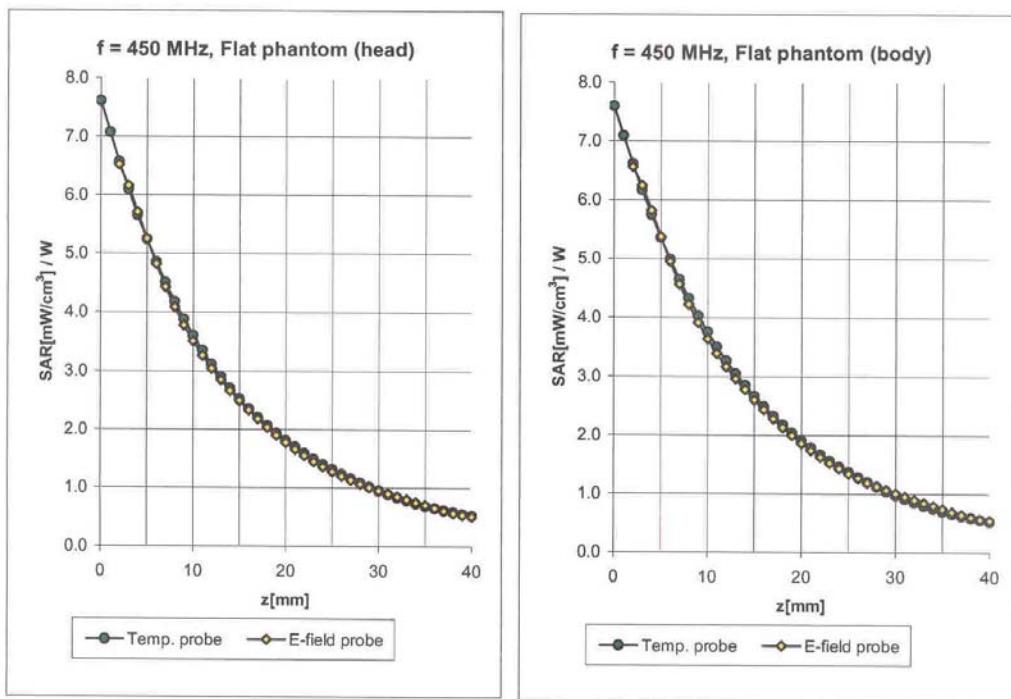

Head 450 MHz $\epsilon_r = 43.5 \pm 5\%$ $\sigma = 0.87 \pm 5\% \text{ mho/m}$

Valid for f=400-500 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	7.0 $\pm 15.5\%$ (k=2)	Boundary effect:
ConvF Y	7.0 $\pm 15.5\%$ (k=2)	Alpha 0.40
ConvF Z	7.0 $\pm 15.5\%$ (k=2)	Depth 2.22

Body 450 MHz $\epsilon_r = 56.7 \pm 5\%$ $\sigma = 0.94 \pm 5\% \text{ mho/m}$

Valid for f=400-500 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C


ConvF X	6.5 $\pm 15.5\%$ (k=2)	Boundary effect:
ConvF Y	6.5 $\pm 15.5\%$ (k=2)	Alpha 0.43
ConvF Z	6.5 $\pm 15.5\%$ (k=2)	Depth 2.36

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

ET3DV6 SN:1785

July 28, 2003

Deviation from Isotropy in HSL

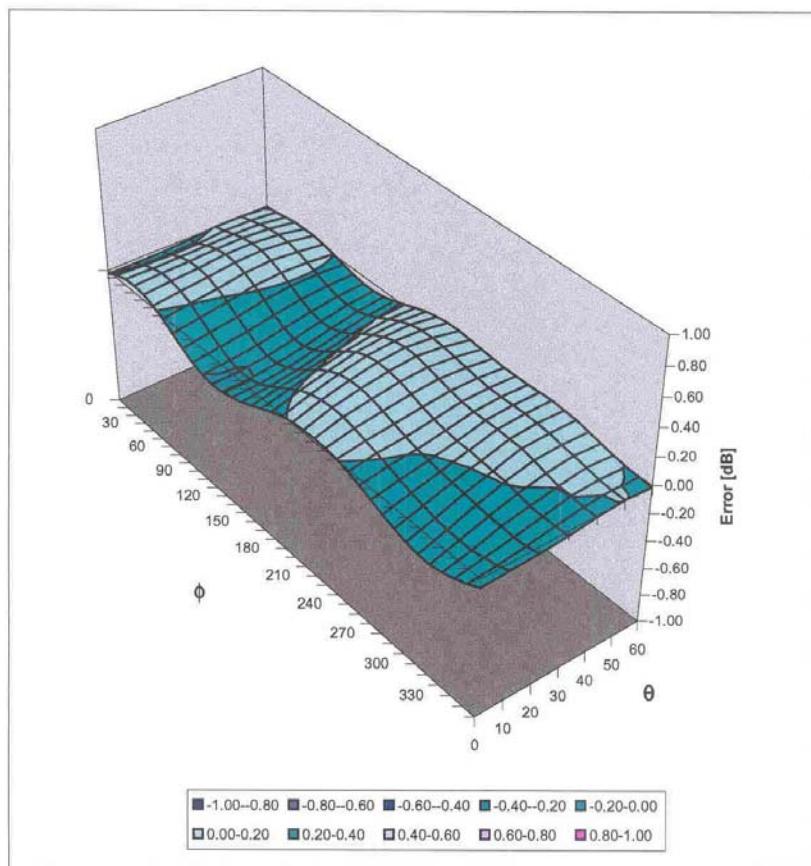Error (θ, ϕ), $f = 900$ MHz

Telian Corporation, Model No: FTD8500

FCC ID: NPQFTD8500

APPENDIX B – 900 MHz Dipole Calibration Certificate

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

900 MHz System Validation Dipole

Type:

D900V2

Serial Number:

013

Place of Calibration:

Zurich

Date of Calibration:

December 19, 2002

Calibration Interval:

24 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:

D. Vello

Approved by:

Heinz Kuhn

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

**Schmid & Partner
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

DASY

Dipole Validation Kit

Type: D900V2

Serial: 013

Manufactured: July 1997

Calibrated: December 19, 2002

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with head simulating solution of the following electrical parameters at 900 MHz:

Relative Dielectricity	42.4	± 5%
Conductivity	0.97 mho/m	± 5%

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.5 at 900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was 250mW ± 3 %. The results are normalized to 1W input power.

2. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the advanced extrapolation are:

averaged over 1 cm³ (1 g) of tissue: **10.6 mW/g**

averaged over 10 cm³ (10 g) of tissue: **6.72 mW/g**

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay: **1.418 ns** (one direction)
Transmission factor: **0.994** (voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

Feedpoint impedance at 900 MHz: **Re{Z} = 50.3 Ω**

Im {Z} = 0.7 Ω

Return Loss at 900 MHz **-41.9 dB**

4. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

5. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

6. Power Test

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

Date/Time: 12/19/02 11:57:16

Test Laboratory: SPEAG, Zurich, Switzerland
File Name: SN013_SN1507_HSL900_191202.da4



DUT: Dipole 900 MHz Type & Serial Number: D900V2 - SN013
Program: Dipole Calibration; Pin = 250 mW; d = 15 mm

Communication System: CW-900; Frequency: 900 MHz; Duty Cycle: 1:1
Medium: HSL 900 MHz ($\sigma = 0.97 \text{ mho/m}$, $\epsilon = 42.44$, $\rho = 1000 \text{ kg/m}^3$)
Phantom section: FlatSection


DASY4 Configuration:

- Probe: ET3DV6 - SN1507; ConvF(6.5, 6.5, 6.5); Calibrated: 1/24/2002
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 - SN410; Calibrated: 7/18/2002
- Phantom: SAM 4.0 - TP:1006
- Software: DASY4, V4.0 Build 51

Area Scan (81x81x1): Measurement grid: dx=15mm, dy=15mm
Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm
Reference Value = 56.5 V/m
Peak SAR = 4.03 mW/g
SAR(1 g) = 2.66 mW/g; SAR(10 g) = 1.68 mW/g
Power Drift = -0.003 dB

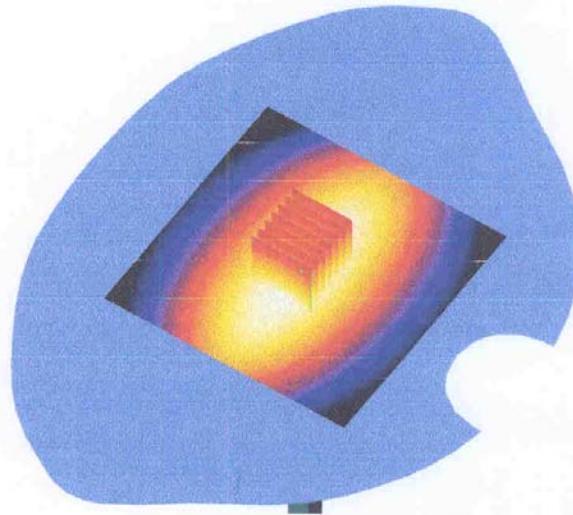

Telian Corporation, Model No: FTD8500
FCC ID: NPQFTD8500

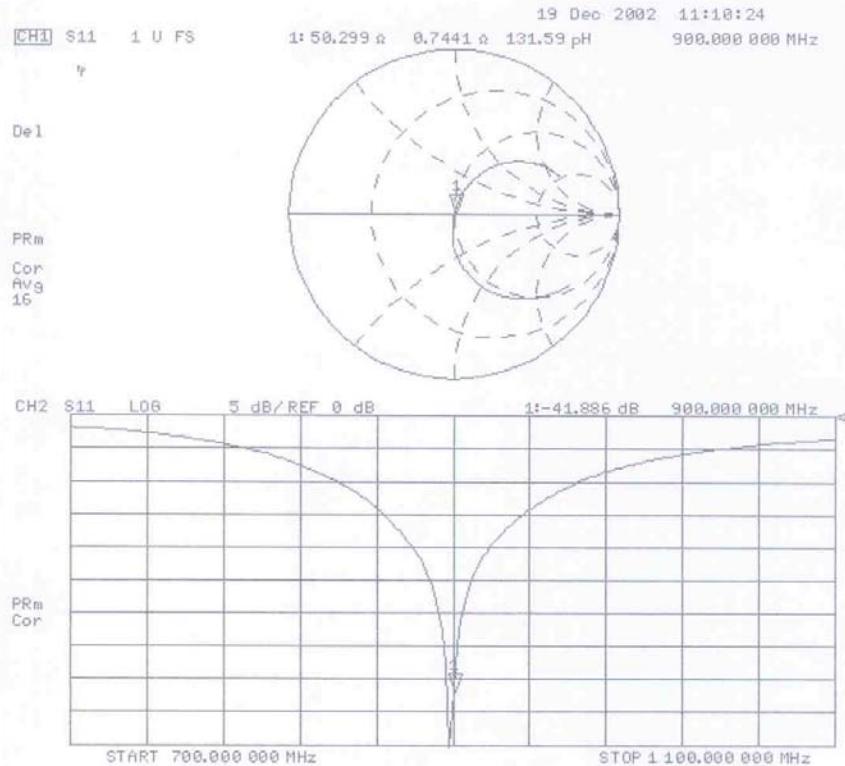

Telian Corporation, Model No: FTD8500

FCC ID: NPQFTD8500

APPENDIX C – Phantom Certificate**Schmid & Partner
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Certificate of conformity / First Article Inspection

Item	SAM Twin Phantom V4.0
Type No	QD 000 P40 BA
Series No	TP-1002 and higher
Manufacturer / Origin	Untersee Composites Hauptstr. 69 CH-8559 Fruthwilen Switzerland

Tests

The series production process used allows the limitation to test of first articles.

Complete tests were made on the pre-series Type No. QD 000 P40 AA, Serial No. TP-1001 and on the series first article Type No. QD 000 P40 BA, Serial No. TP-1006. Certain parameters have been retested using further series units (called samples).

Test	Requirement	Details	Units tested
Shape	Compliance with the geometry according to the CAD model.	IT'IS CAD File (*)	First article, Samples
Material thickness	Compliant with the requirements according to the standards	2mm +/- 0.2mm in specific areas	First article, Samples
Material parameters	Dielectric parameters for required frequencies	200 MHz – 3 GHz Relative permittivity < 5 Loss tangent < 0.05.	Material sample TP 104-5
Material resistivity	The material has been tested to be compatible with the liquids defined in the standards	Liquid type HSL 1800 and others according to the standard.	Pre-series, First article

Standards

- [1] CENELEC EN 50361
- [2] IEEE P1528-200x draft 6.5
- [3] IEC PT 62209 draft 0.9

(*) The IT'IS CAD file is derived from [2] and is also within the tolerance requirements of the shapes of [1] and [3].

Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of SAR measurements specified in standard [1] and draft standards [2] and [3].

Date

18.11.2001

Signature / Stamp