

## Additional Conversion Factors for Dosimetric E-Field Probe

Type:

**ET3DV6**

Serial Number:

**1702**

Place of Assessment:

**Zurich**

Date of Assessment:


**February 20, 2004**

Probe Calibration Date:

**February 17, 2004**

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Assessed by:



### Dosimetric E-Field Probe ET3DV6 SN:1702

Conversion factor ( $\pm$  standard deviation)

450 MHz                  ConvF                  7.7  $\pm$  8%

$\epsilon_r = 43.5 \pm 5\%$   
 $\sigma = 0.87 \pm 5\%$  mho/m  
(head tissue)

450 MHz                  ConvF                  7.6  $\pm$  8%

$\epsilon_r = 56.7 \pm 5\%$   
 $\sigma = 0.94 \pm 5\%$  mho/m  
(body tissue)

**Client**      **Digital EM (Dymstec)**

**CALIBRATION CERTIFICATE**

**Object(s)**      **D450V2 - SN: 1011**

**Calibration procedure(s)**      **QA CAL-15.v2**  
**Calibration procedure for dipole validation kits below 800 MHz**

**Calibration date:**      **May 5, 2003**



**Condition of the calibrated item**      **In Tolerance (according to the specific calibration document)**

This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.

**Calibration Equipment used (M&TE critical for calibration)**

Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
RF generator HP 8684C	US3642U01700	4-Aug-99 (SPEAG, in house check Aug-02)	In house check: Aug-05
Power sensor E4412A	MY41495277	2-Apr-03 (METAS, No 252-0250)	Apr-04
Power sensor HP 8481A	MY41092180	18-Sep-02 (Agilent, No. 20020918)	Sep-03
Power meter EPM E4419B	GB41293874	2-Apr-03 (METAS, No 252-0250)	Apr-04
Network Analyzer HP 8753E	US38432426	3-May-00 (Agilent, No. 8702K064602)	In house check: May 03
Fluke Process Calibrator Type 702	SN: 6295803	3-Sep-01 (ELCAL, No.2360)	Sep-03

	Name	Function	Signature
Calibrated by:	Katja Pokovic	Laboratory Director	
Approved by:	Niels Kuster	Quality Manager	

Date issued: May 5, 2003

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.



# DASY

## Dipole Validation Kit

Type: D450V2

Serial: 1011

Manufactured: November 18, 2002

Calibrated: May 3, 2003

## 1. Measurement Conditions

The measurements were performed in the 6mm thick flat phantom filled with head simulating liquid of the following electrical parameters at 450 MHz:

Relative Dielectricity	<b>45.3</b>	$\pm 5\%$
Conductivity	<b>0.87 mho/m</b>	$\pm 5\%$

The DASY3 System (Software version 3.1d) with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 7.4 at 450 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center of the flat phantom and the dipole was oriented parallel to the longer side of the phantom. The standard measuring distance was 15mm from dipole center to the liquid surface including the 6mm thick phantom shell. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 20mm was aligned with the dipole. The 5x5x7 fine cube was chosen for cube integration. Probe isotropy errors were cancelled by measuring the SAR with normal and 90° turned probe orientations and averaging.

The dipole input power (forward power) was 397 mW  $\pm 3\%$ . The results are normalized to 1W input power.

## 2. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the advanced extrapolation are:

averaged over 1 cm <sup>3</sup> (1 g) of tissue:	<b>4.96 mW/g</b> $\pm 16.8\%$ (k=2) <sup>1</sup>
averaged over 10 cm <sup>3</sup> (10 g) of tissue:	<b>3.27 mW/g</b> $\pm 16.2\%$ (k=2) <sup>1</sup>

---

<sup>1</sup> validation uncertainty

### 3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:	<b>1.413 ns</b>	(one direction)
Transmission factor:	<b>0.998</b>	(voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

Feedpoint impedance at 450 MHz:	$\text{Re}\{Z\} = 53.5 \Omega$
---------------------------------	--------------------------------

	$\text{Im}\{Z\} = -8.5 \Omega$
--	--------------------------------

Return Loss at 450 MHz	<b>-21.0 dB</b>
------------------------	-----------------

### 4. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

### 5. Design



The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

### 6. Power Test

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

### Validation Dipole D450V2 SN:1011, d = 15 mm

Frequency: 450 MHz; Antenna Input Power: 397 [mW]  
Phantom Name: Calibration (6mm shell thickness), Grid Spacing: Dx = 20.0, Dy = 20.0, Dz = 10.0  
Probe: ET3DV6 - SN1507-Y2003; ConvF(7.40,7.40,7.40); Crest factor: 1.0; Head 450 MHz:  $\sigma = 0.87$  mho/m  $\epsilon_r = 45.3$  p = 1.00 g/cm<sup>3</sup>  
Cubes (2): Peak: 3.05 mW/g  $\pm$  0.02 dB, SAR (1g): 1.97 mW/g  $\pm$  0.02 dB, SAR (10g): 1.30 mW/g  $\pm$  0.01 dB, (Advanced extrapolation)  
Penetration depth: 12.6 (11.2, 14.3) [mm]

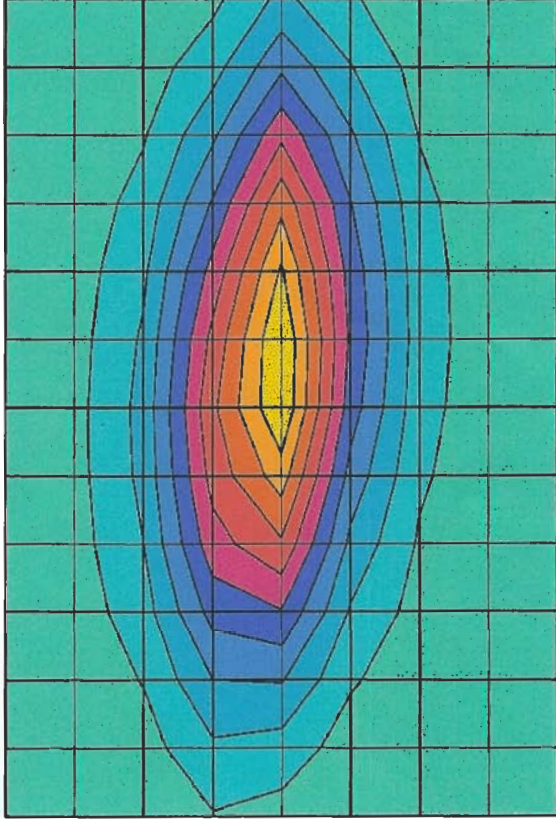
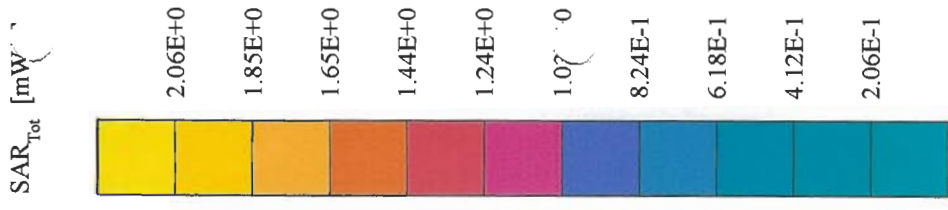


## Validation Dipole D450V2 SN:1011, d = 15 mm

Frequency: 450 MHz; Antenna Input Power: 397 [mW]

Phantom Name: Calibration (6mm shell thickness), Grid Spacing: Dx = 20.0, Dy = 20.0, Dz = 10.0

Probe: ET3DV6 - SN1507-Y2003; ConvF(7.40,7.40,7.40); Crest factor: 1.0; Head 450 MHz:  $\sigma = 0.87$  mho/m  $\epsilon_r = 45.3$   $\rho = 1.00$  g/cm<sup>3</sup>  
 Cubes (2): Peak: 3.32 mW/g  $\pm$  0.02 dB, SAR (1g): 2.07 mW/g  $\pm$  0.02 dB, SAR (10g): 1.34 mW/g  $\pm$  0.01 dB, (Worst-case extrapolation)  
 Penetration depth: 11.9 (10.3, 14.1) [mm]

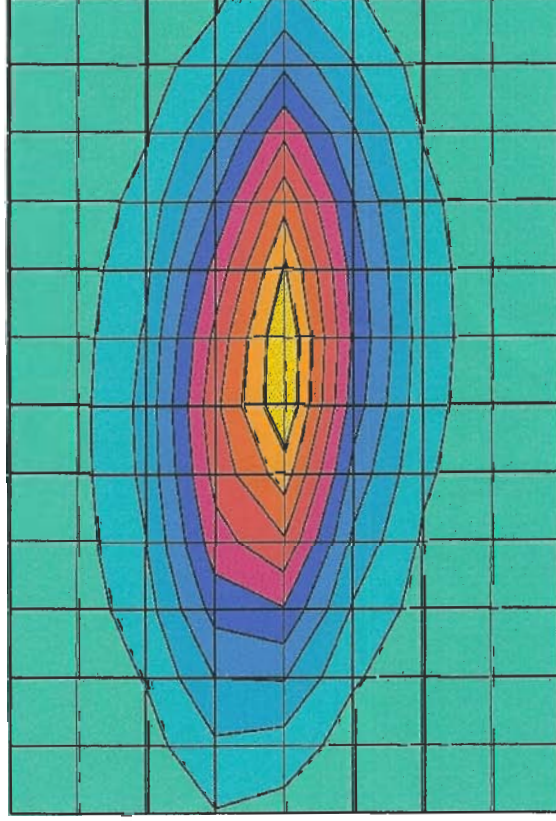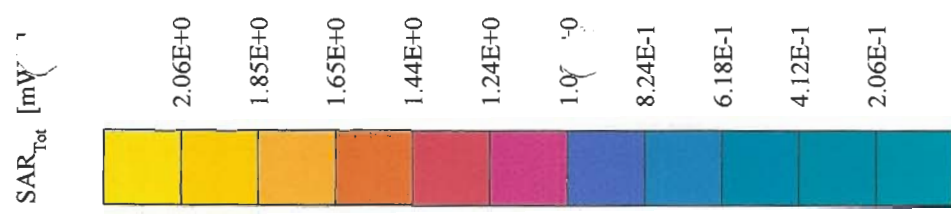



SN: 1011

3 May 2003 12:07:31


CH1 S11 1 U FS 1: 53.527  $\Omega$  -8.5332  $\Omega$  41.447 pF 450.000 000 MHz

De1

Cor

Avg  
16

↑

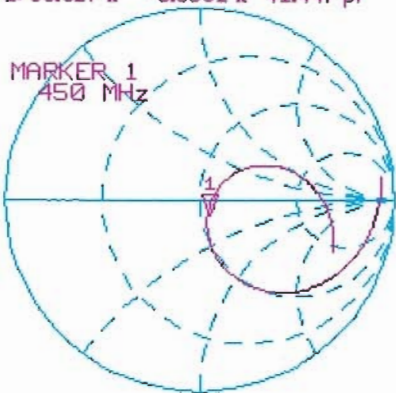


CH2 S11 LOG 5 dB/REF -15 dB 1: -21.022 dB 450.000 000 MHz

Cor

Avg  
16

↑

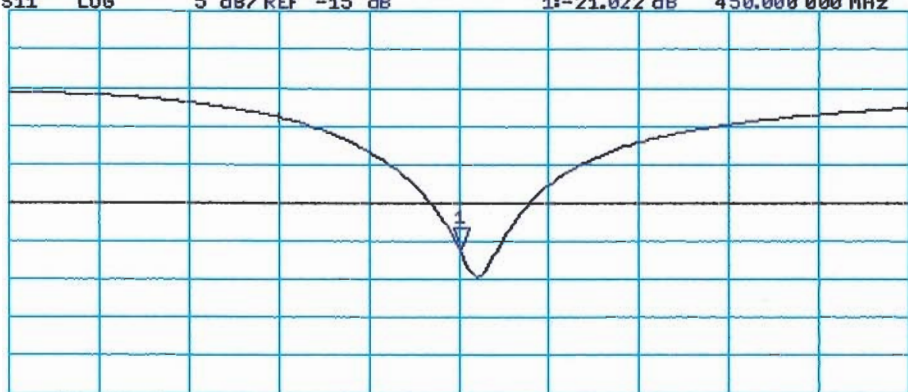

CENTER 450.000 000 MHz

SPAN 400.000 000 MHz