

## System Check\_Head\_835MHz

**DUT: D835V2-SN:4d091**

Communication System: ; Frequency: 835.0

Medium: HSL. Medium parameters used:  $f= 835.0$  MHz;  $\sigma= 0.930$  S/m;  $\epsilon_r = 40.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(10.57, 10.57, 10.57); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.481 W/kg; SAR (10g) = 0.317 W/kg;

**Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm):** Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.07 dB

SAR (1g) = 0.454 W/kg; SAR (10g) = 0.302 W/kg;

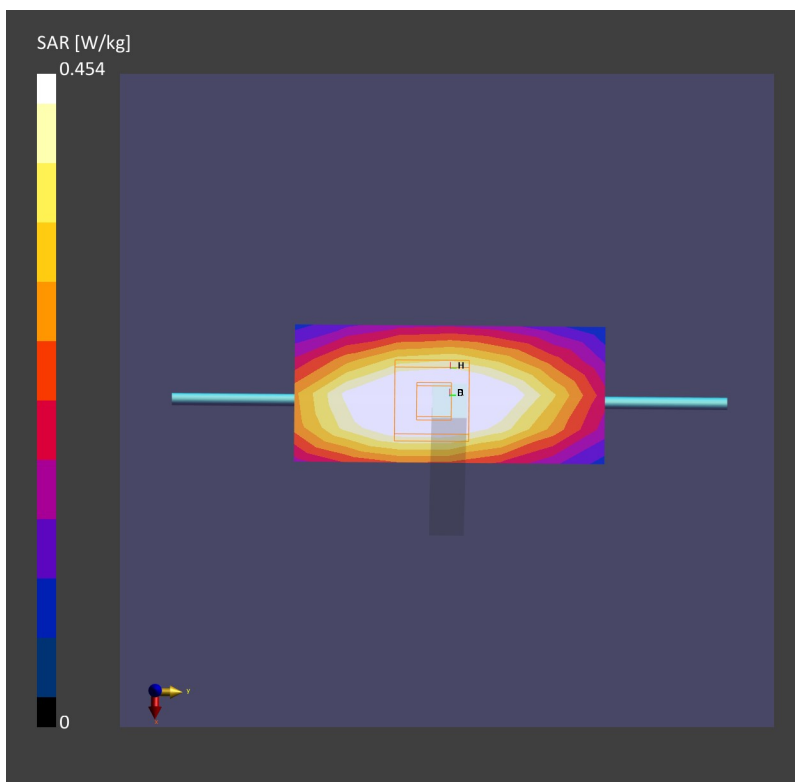

## System Check\_Head\_2450MHz

**DUT: D2450V2-SN:1040**

Communication System: ; Frequency: 2450.0

Medium: HSL. Medium parameters used:  $f= 2450.0$  MHz;  $\sigma= 1.84$  S/m;  $\epsilon_r = 39.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.25, 8.25, 8.25); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 96.0 mm):** Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.50 W/kg; SAR (10g) = 1.16 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = 0.08 dB

SAR (1g) = 2.50 W/kg; SAR (10g) = 1.17 W/kg;

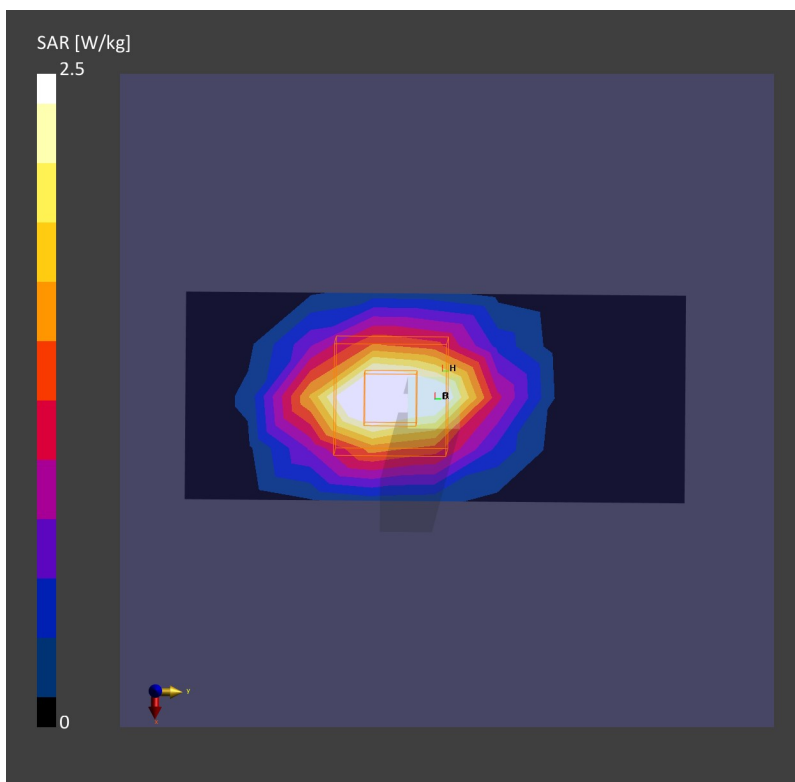

## System Check\_Head\_2600MHz

**DUT: D2600V2-SN:1061**

Communication System: ; Frequency: 2600.0

Medium: HSL. Medium parameters used:  $f= 2600.0$  MHz;  $\sigma= 2.01$  S/m;  $\epsilon_r = 40.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.99, 7.99, 7.99); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 96.0 mm):** Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.62 W/kg; SAR (10g) = 1.18 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = -0.01 dB

SAR (1g) = 2.67 W/kg; SAR (10g) = 1.20 W/kg;

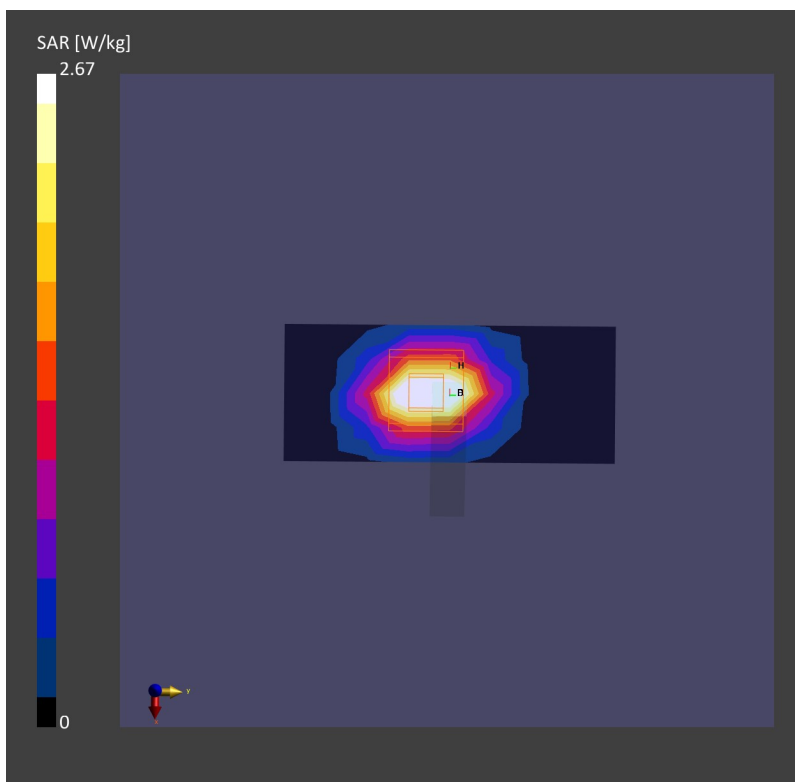

## System Check\_Head\_3500MHz

**DUT: D3500V2-SN:1037**

Communication System: ; Frequency: 3500.0

Medium: HSL. Medium parameters used:  $f= 3500.0$  MHz;  $\sigma= 2.81$  S/m;  $\epsilon_r = 39.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.45, 7.45, 7.45); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.03 W/kg; SAR (10g) = 1.19 W/kg;

**Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.17 W/kg; SAR (10g) = 1.25 W/kg;

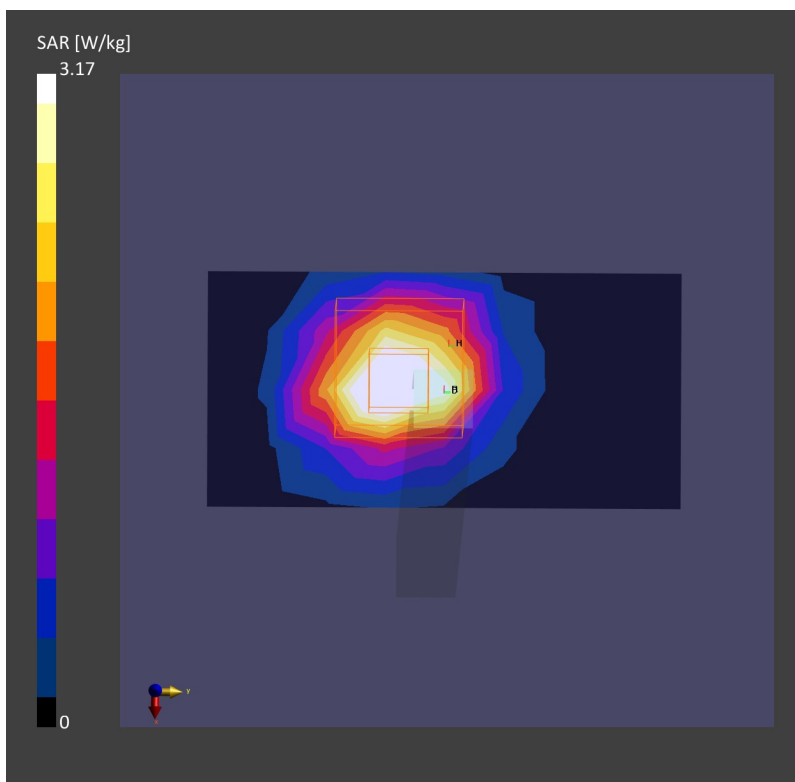

## System Check\_Head\_3700MHz

**DUT: D3700V2-SN:1008**

Communication System: ; Frequency: 3700.0

Medium: HSL. Medium parameters used:  $f= 3700.0$  MHz;  $\sigma= 3.00$  S/m;  $\epsilon_r = 38.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.3, 7.3, 7.3); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.21 W/kg; SAR (10g) = 1.23 W/kg;

**Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.39 W/kg; SAR (10g) = 1.26 W/kg;

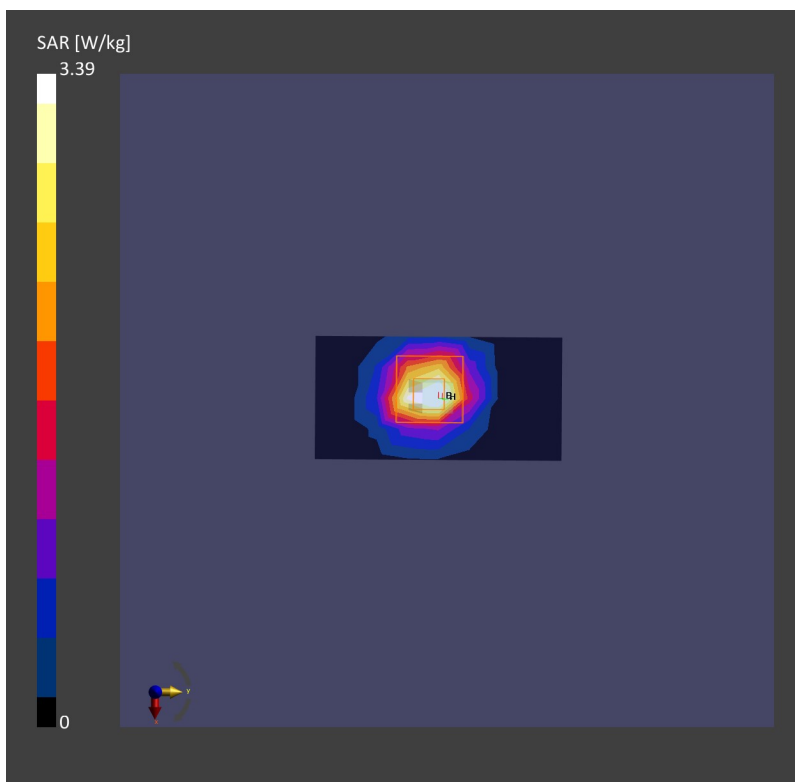

## System Check\_Head\_3900MHz

**DUT: D3900V2-SN:1048**

Communication System: ; Frequency: 3900.0

Medium: HSL. Medium parameters used:  $f= 3900.0$  MHz;  $\sigma= 3.19$  S/m;  $\epsilon_r = 38.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(6.66, 6.66, 6.66); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.26 W/kg; SAR (10g) = 1.22 W/kg;

**Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.46 W/kg; SAR (10g) = 1.28 W/kg;

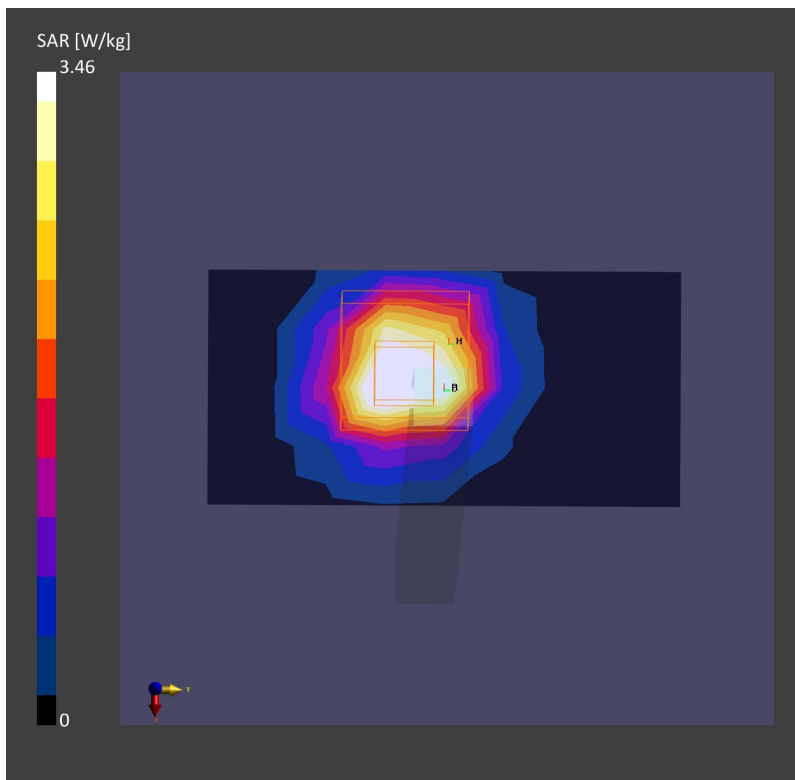

## System Check\_Head\_5250MHz

**DUT: D5GHzV2-SN:1113**

Communication System: ; Frequency: 5250.0

Medium: HSL. Medium parameters used:  $f= 5250.0$  MHz;  $\sigma= 4.64$  S/m;  $\epsilon_r = 36.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.65, 5.65, 5.65); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.30 W/kg; SAR (10g) = 0.998 W/kg;

**Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.04 dB

SAR (1g) = 3.79 W/kg; SAR (10g) = 1.09 W/kg;

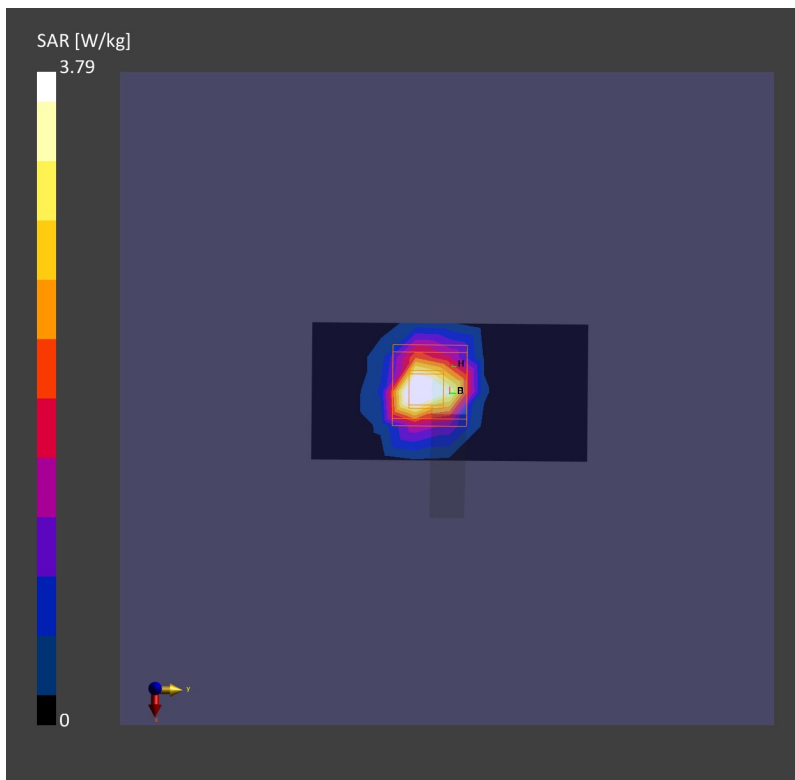

## System Check\_Head\_5600MHz

**DUT: D5GHzV2-SN:1113**

Communication System: ; Frequency: 5600.0

Medium: HSL. Medium parameters used:  $f= 5600.0$  MHz;  $\sigma= 4.98$  S/m;  $\epsilon_r = 35.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(4.9, 4.9, 4.9); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.72 W/kg; SAR (10g) = 1.11 W/kg;

**Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 4.15 W/kg; SAR (10g) = 1.20 W/kg;

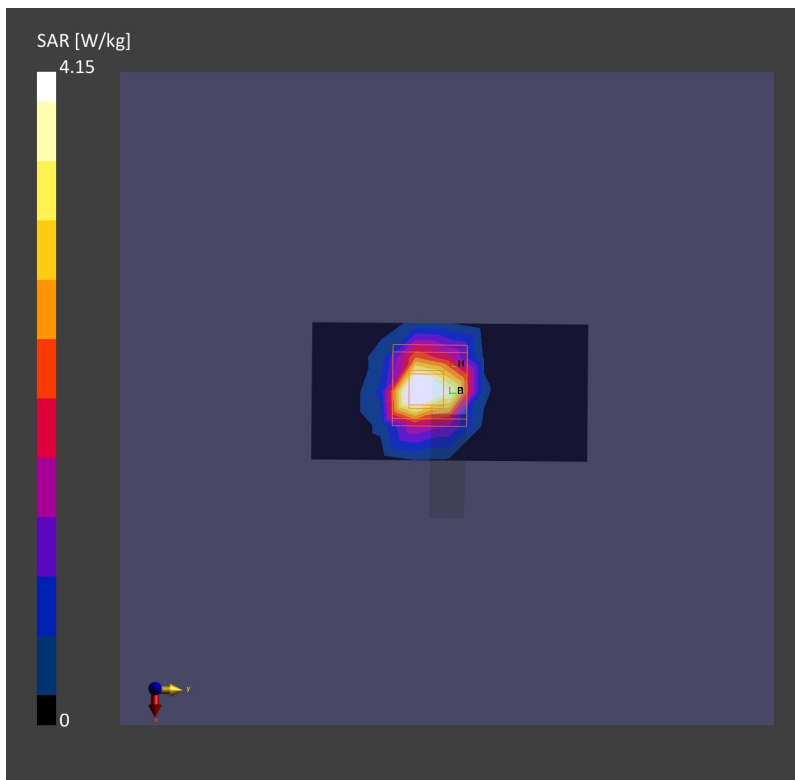



## System Check\_Head\_5750MHz

**DUT: D5GHzV2-SN:1113**

Communication System: ; Frequency: 5750.0

Medium: HSL. Medium parameters used:  $f= 5750.0$  MHz;  $\sigma= 5.21$  S/m;  $\epsilon_r = 35.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.1, 5.1, 5.1); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.32 W/kg; SAR (10g) = 0.990 W/kg;

**Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.77 W/kg; SAR (10g) = 1.08 W/kg;

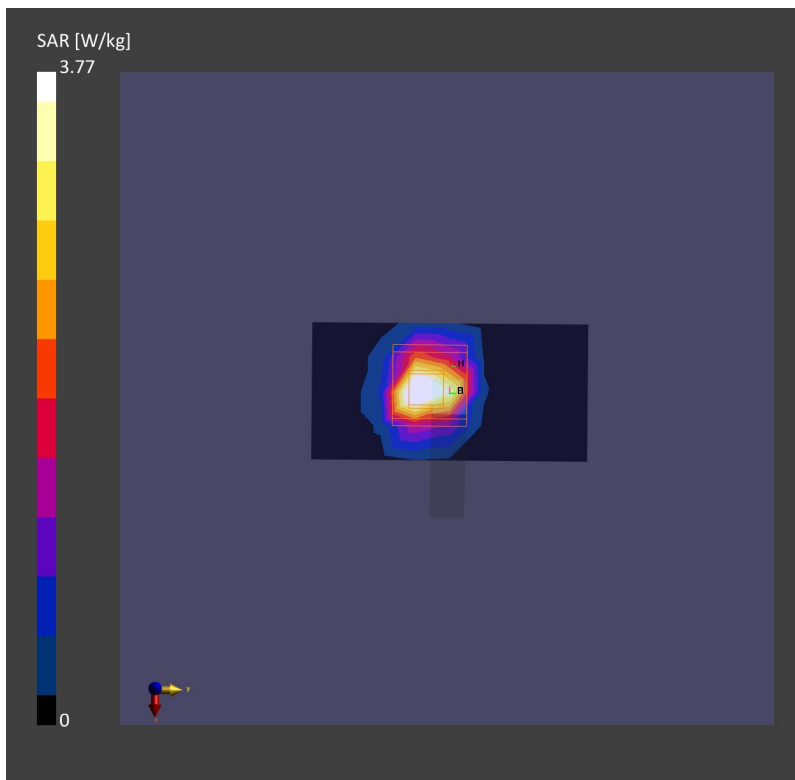

## System Check\_Head\_3500MHz

**DUT: D3500V2-SN:1037**

Communication System: ; Frequency: 3500.0

Medium: HSL. Medium parameters used:  $f= 3500.0$  MHz;  $\sigma= 2.79$  S/m;  $\epsilon_r = 39.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.45, 7.45, 7.45); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.01 W/kg; SAR (10g) = 1.18 W/kg;

**Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.18 W/kg; SAR (10g) = 1.24 W/kg;

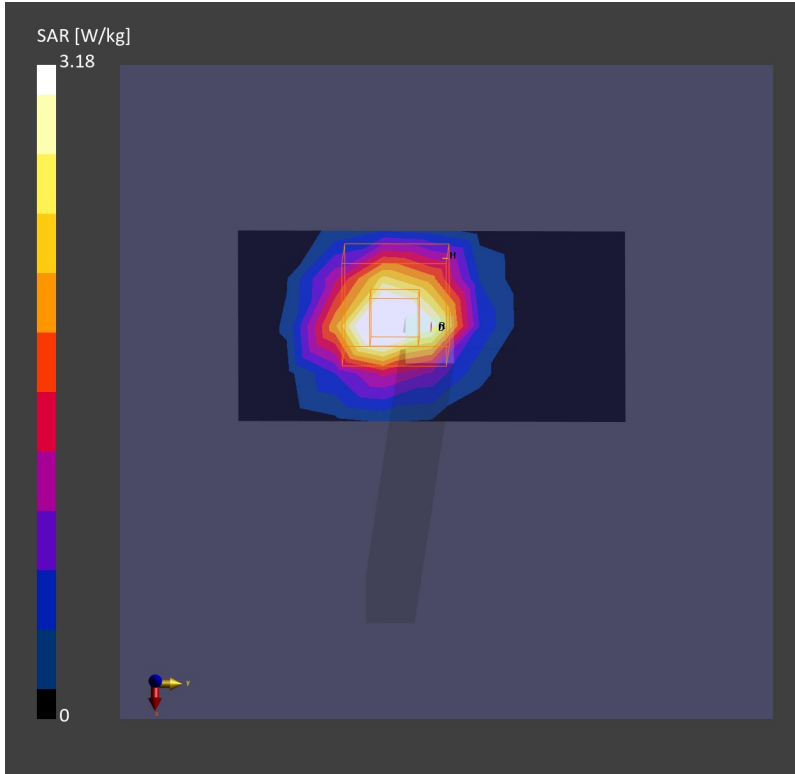

## System Check\_Head\_3900MHz

**DUT: D3900V2-SN:1048**

Communication System: ; Frequency: 3900.0

Medium: HSL. Medium parameters used:  $f= 3900.0$  MHz;  $\sigma= 3.18$  S/m;  $\epsilon_r = 38.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(6.66, 6.66, 6.66); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926

**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.27 W/kg; SAR (10g) = 1.22 W/kg;

**Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.06 dB

SAR (1g) = 3.49 W/kg; SAR (10g) = 1.28 W/kg;

