

System Check_Head_750MHz

DUT: D750V3-SN:1087

Communication System: ; Frequency: 750.0

Medium: HSL. Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.913$ S/m; $\epsilon_r = 41.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(10.95, 10.95, 10.95); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.408 W/kg; SAR (10g) = 0.273 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.07 dB

SAR (1g) = 0.409 W/kg; SAR (10g) = 0.273 W/kg;

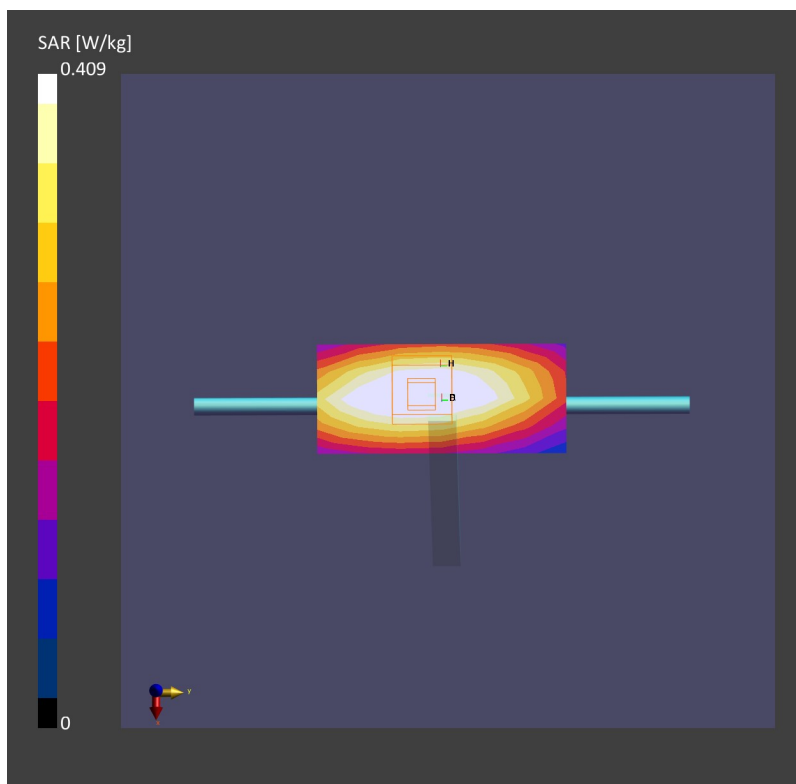

System Check_Head_835MHz

DUT: D835V2-SN:4d091

Communication System: ; Frequency: 835.0

Medium: HSL. Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.934$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(10.57, 10.57, 10.57); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.451 W/kg; SAR (10g) = 0.314 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.06 dB

SAR (1g) = 0.466 W/kg; SAR (10g) = 0.316 W/kg;

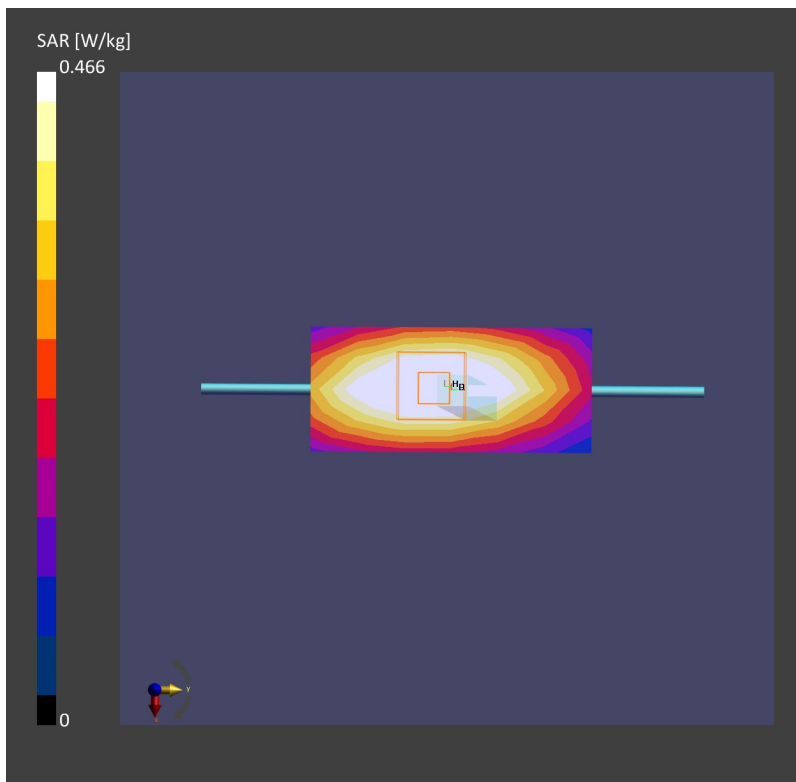

System Check_Head_2450MHz

DUT: D2450V2-SN:1040

Communication System: ; Frequency: 2450.000

Medium: HSL. Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.25, 8.25, 8.25); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.45 W/kg; SAR (10g) = 1.15 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = 0.01 dB

SAR (1g) = 2.57 W/kg; SAR (10g) = 1.19 W/kg;

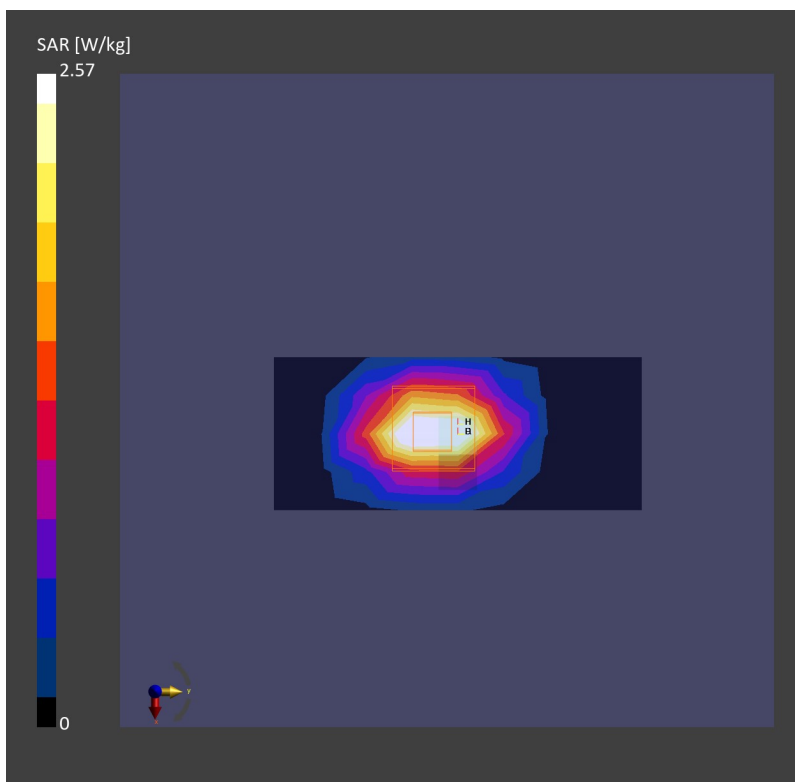

System Check_Head_2600MHz

DUT: D2600V2-SN:1061

Communication System: ; Frequency: 2600.0

Medium: HSL. Medium parameters used: $f = 2600.0$ MHz; $\sigma = 1.92$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.99, 7.99, 7.99); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.67 W/kg; SAR (10g) = 1.19 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = 0.03 dB

SAR (1g) = 2.79 W/kg; SAR (10g) = 1.23 W/kg;

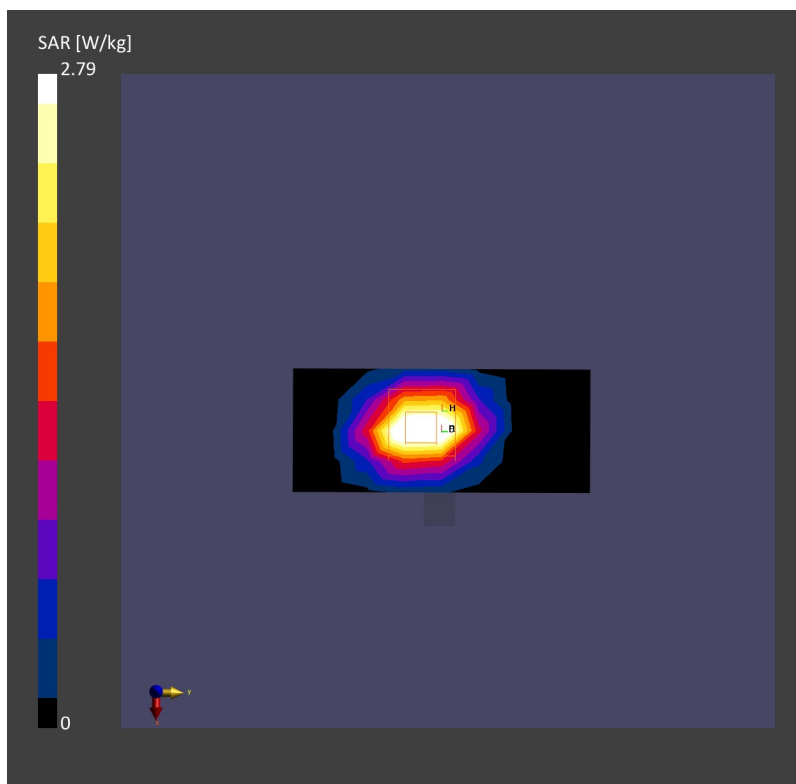

System Check_Head_3500MHz

DUT: D3500V2-SN:1037

Communication System: ; Frequency: 3500.0

Medium: HSL. Medium parameters used: $f = 3500.0$ MHz; $\sigma = 2.81$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.45, 7.45, 7.45); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.27 W/kg; SAR (10g) = 1.23 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 3.32 W/kg; SAR (10g) = 1.30 W/kg;

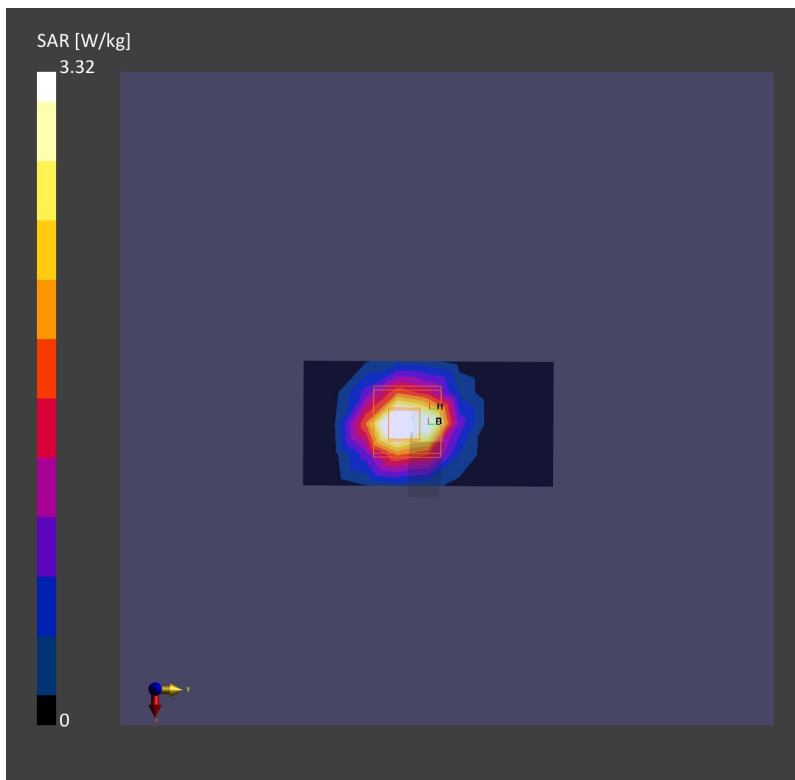

System Check_Head_3700MHz

DUT: D3700V2-SN:1008

Communication System: ; Frequency: 3700.000

Medium: HSL. Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.00$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.3, 7.3, 7.3); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELIV8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.05 W/kg; SAR (10g) = 1.15 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 3.12 W/kg; SAR (10g) = 1.16 W/kg;

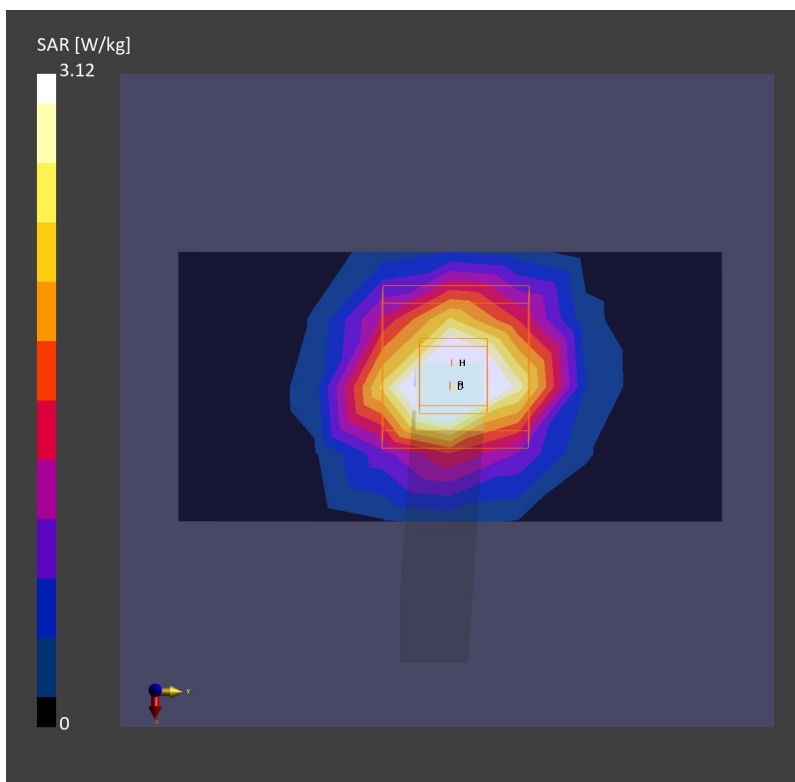

System Check_Head_3900MHz

DUT: D3900V2-SN:1048

Communication System: ; Frequency: 3900.000

Medium: HSL. Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.19$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(6.66, 6.66, 6.66); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.07 W/kg; SAR (10g) = 1.15 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.04 dB

SAR (1g) = 3.30 W/kg; SAR (10g) = 1.21 W/kg;

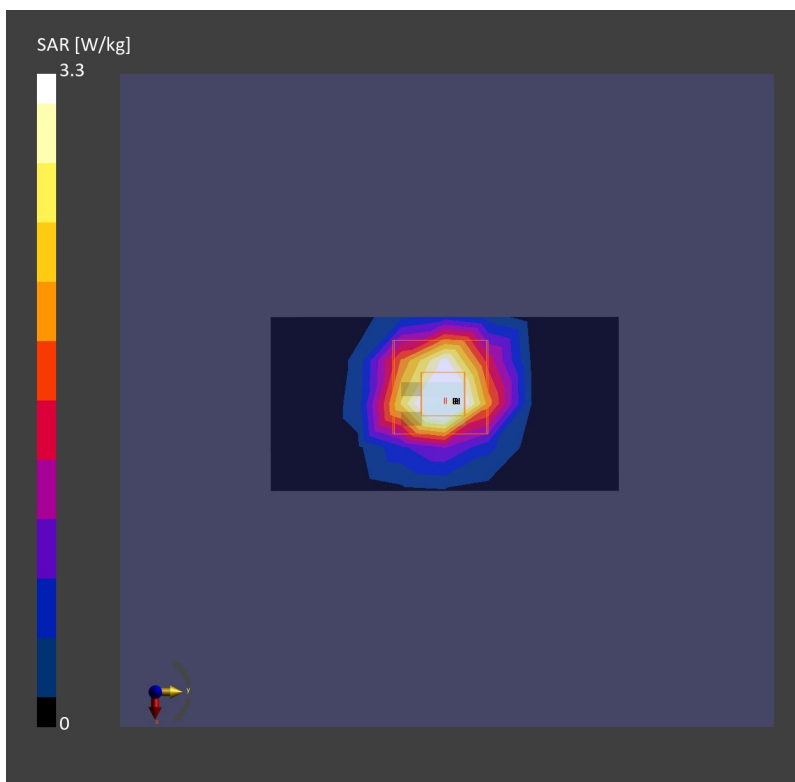

System Check_Head_5250MHz

DUT: D5GHzV2-SN:1113

Communication System: ; Frequency: 5250.000

Medium: HSL. Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.60$ S/m; $\epsilon_r = 35.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.65, 5.65, 5.65); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.66 W/kg; SAR (10g) = 1.05 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.86 W/kg; SAR (10g) = 1.15 W/kg;

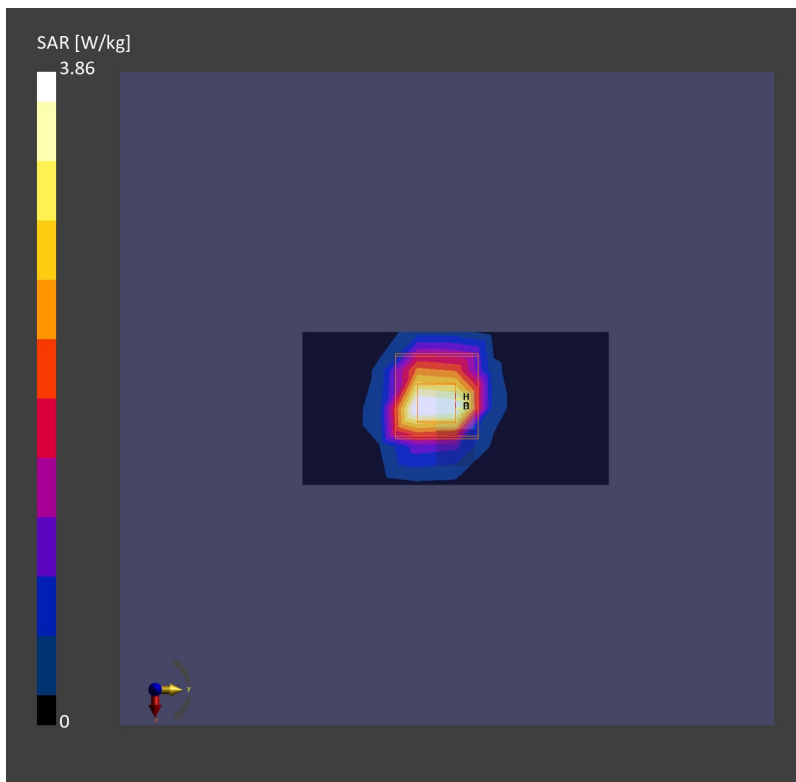

System Check_Head_5600MHz

DUT: D5GHzV2-SN:1113

Communication System: ; Frequency: 5600.000

Medium: HSL. Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.99$ S/m; $\epsilon_r = 35.4$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(4.9, 4.9, 4.9); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.59 W/kg; SAR (10g) = 1.11 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 4.18 W/kg; SAR (10g) = 1.19 W/kg;

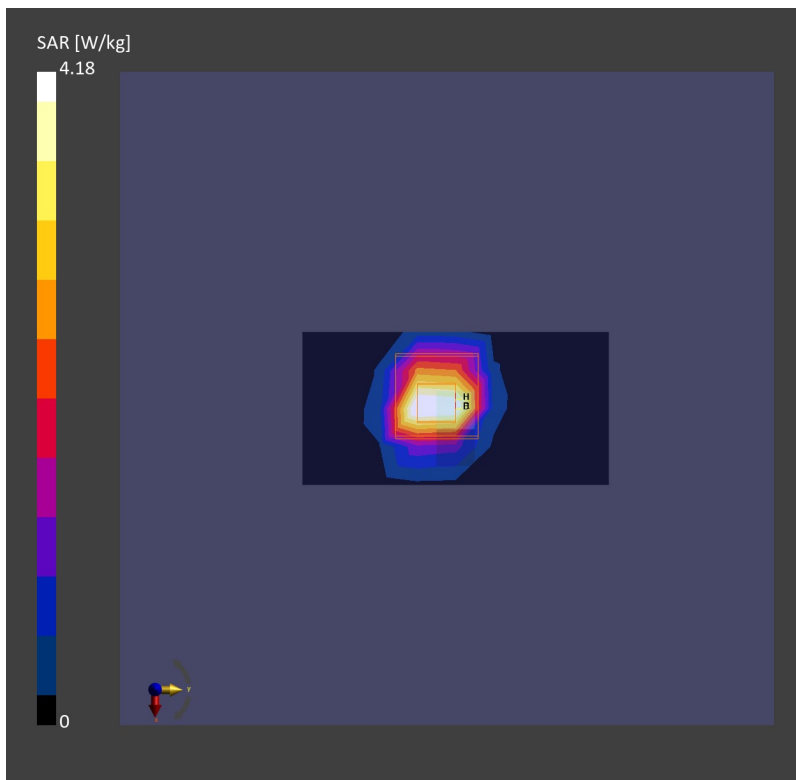

System Check_Head_5750MHz

DUT: D5GHzV2-SN:1113

Communication System: ; Frequency: 5750.000

Medium: HSL. Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.16$ S/m; $\epsilon_r = 35.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.1, 5.1, 5.1); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.65 W/kg; SAR (10g) = 0.997 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.04 dB

SAR (1g) = 3.97 W/kg; SAR (10g) = 1.14 W/kg;

