

System Check_Head_750MHz

DUT: D750V3-SN:1087

Communication System: ; Frequency: 750.0

Medium: HSL. Medium parameters used: $f= 750.0$ MHz; $\sigma= 0.890$ S/m; $\epsilon_r = 42.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(10.95, 10.95, 10.95); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.415 W/kg; SAR (10g) = 0.264 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.02 dB

SAR (1g) = 0.420 W/kg; SAR (10g) = 0.277 W/kg;

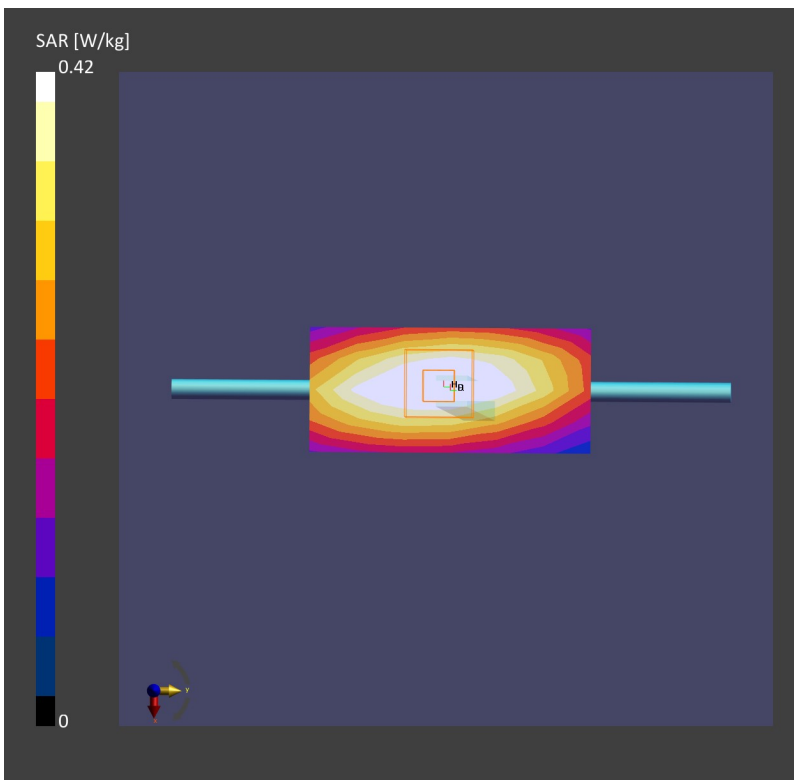

System Check_Head_835MHz

DUT: D835V2-SN:4d091

Communication System: ; Frequency: 835.0

Medium: HSL. Medium parameters used: $f= 835.0$ MHz; $\sigma= 0.912$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(10.57, 10.57, 10.57); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.447 W/kg; SAR (10g) = 0.292 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.01 dB

SAR (1g) = 0.466 W/kg; SAR (10g) = 0.307 W/kg;

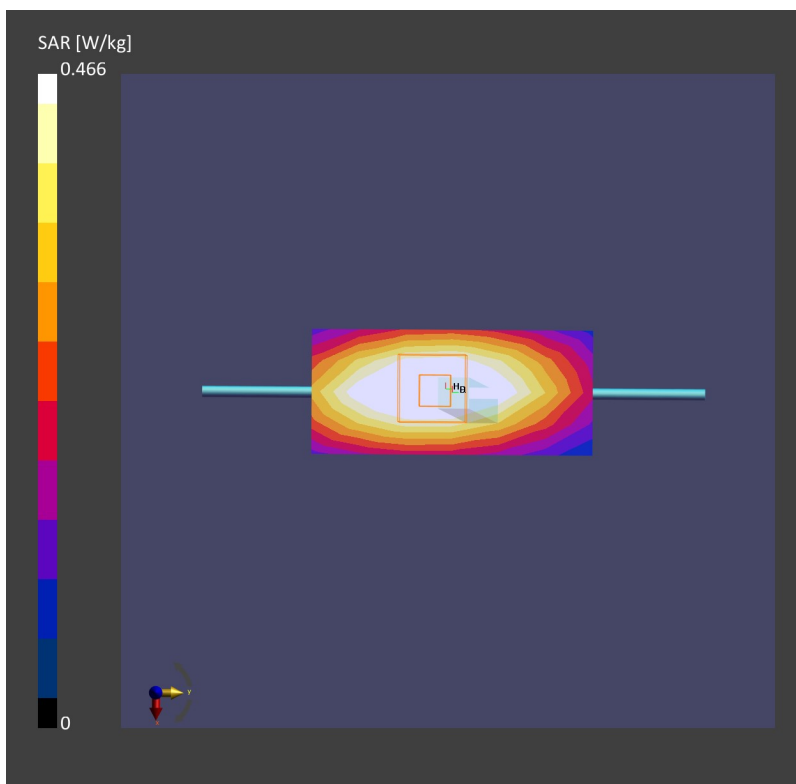

System Check_Head_1750MHz

DUT: D1750V2-SN:1090

Communication System: ; Frequency: 1750.0

Medium: HSL. Medium parameters used: $f= 1750.0$ MHz; $\sigma= 1.32$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(9.01, 9.01, 9.01); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.66 W/kg; SAR (10g) = 0.933 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.08 dB

SAR (1g) = 1.79 W/kg; SAR (10g) = 0.942 W/kg;

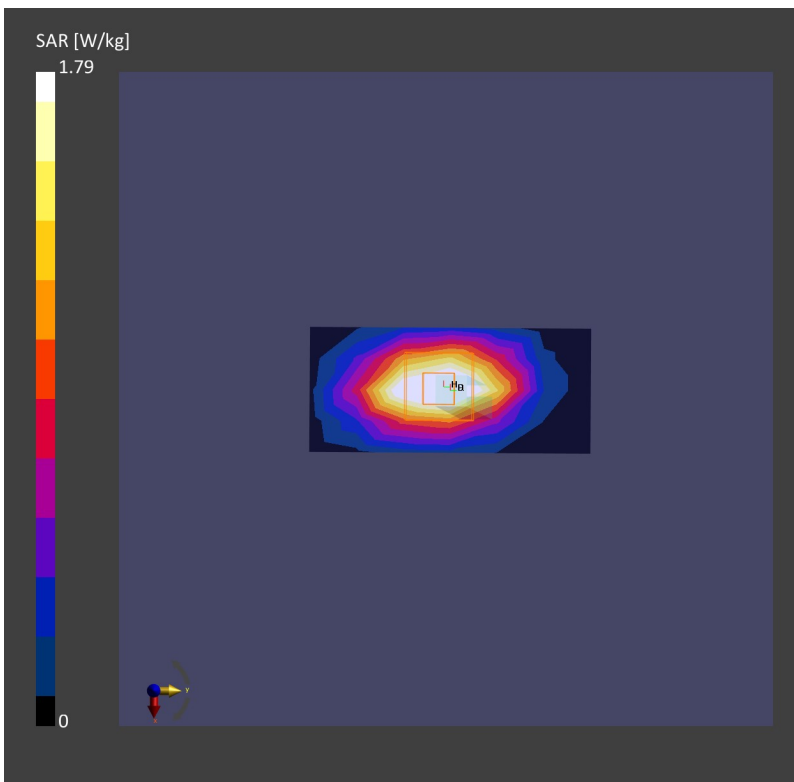

System Check_Head_1900MHz

DUT: D1900V2-SN:5d118

Communication System: ; Frequency: 1900.0

Medium: HSL. Medium parameters used: $f=1900.0$ MHz; $\sigma=1.40$ S/m; $\epsilon_r=40.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.58, 8.58, 8.58); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.84 W/kg; SAR (10g) = 0.978 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.03 dB

SAR (1g) = 1.96 W/kg; SAR (10g) = 0.998 W/kg;

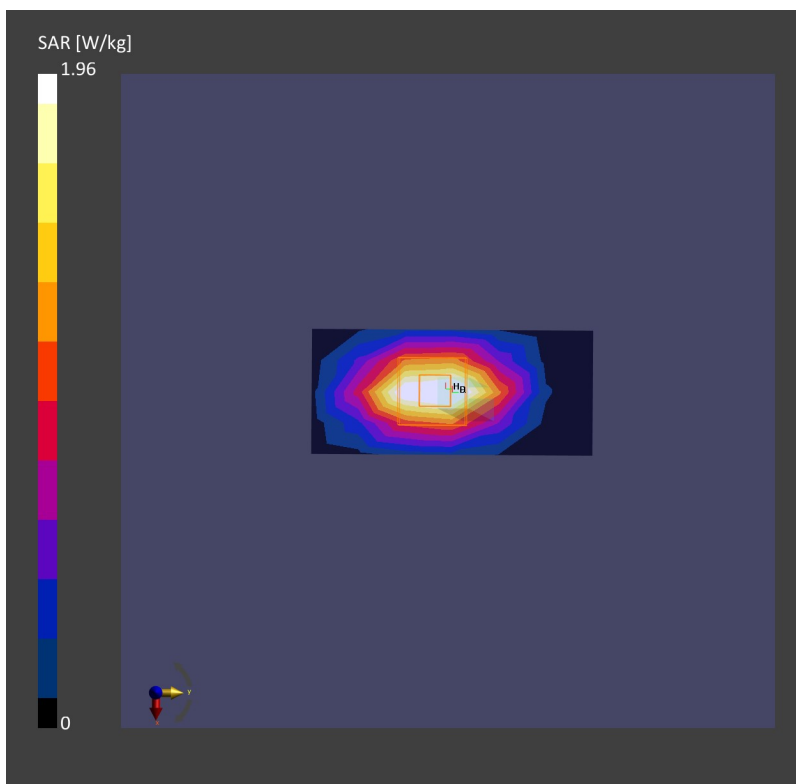

System Check_Head_2600MHz

DUT: D2600V2-SN:1061

Communication System: ; Frequency: 2600.0

Medium: HSL. Medium parameters used: $f= 2600.0$ MHz; $\sigma= 2.01$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.99, 7.99, 7.99); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.66 W/kg; SAR (10g) = 1.08 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = 0.04 dB

SAR(1 g) = 2.86 W/kg; SAR(10 g) = 1.26 W/kg;

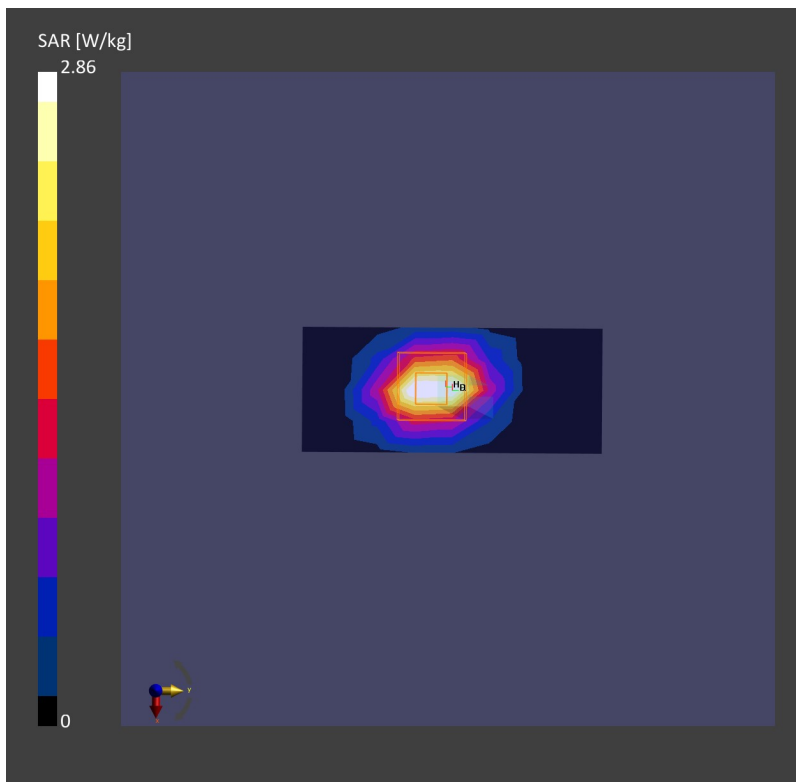

System Check_Head_3500MHz

DUT: D3500V2-SN:1037

Communication System: ; Frequency: 3500.0

Medium: HSL. Medium parameters used: $f= 3500.0$ MHz; $\sigma= 2.81$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.45, 7.45, 7.45); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.06 W/kg; SAR (10g) = 1.03 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.04 dB

SAR(1 g) = 3.32 W/kg; SAR(10 g) = 1.23 W/kg;

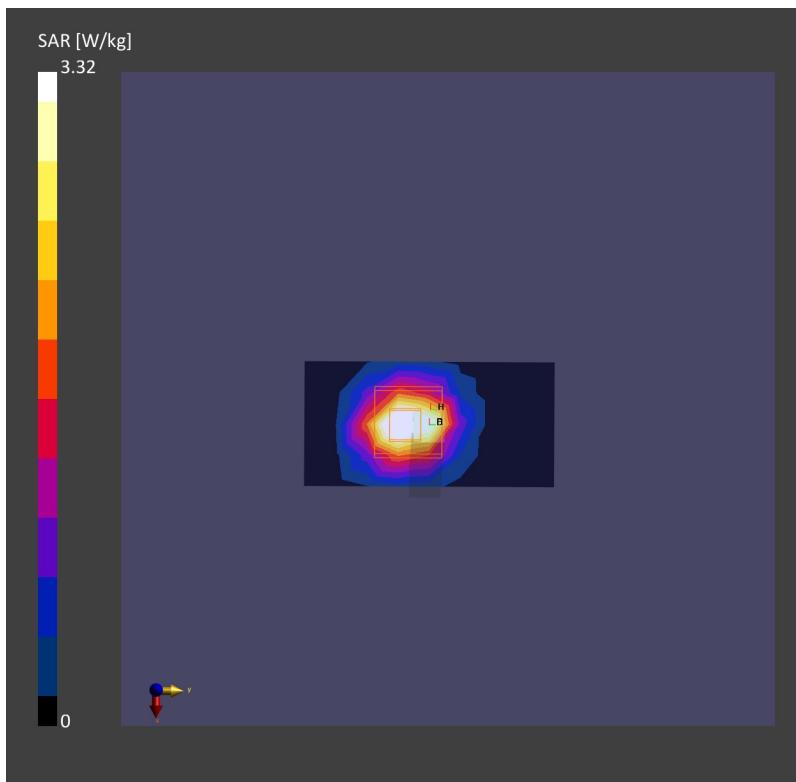

System Check_Head_3700MHz

DUT: D3700V2-SN:1008

Communication System: ; Frequency: 3700.0

Medium: HSL. Medium parameters used: $f= 3700.0$ MHz; $\sigma= 2.99$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.3, 7.3, 7.3); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.11 W/kg; SAR (10g) = 1.12 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.05 dB

SAR(1 g) = 3.36 W/kg; SAR(10 g) = 1.23 W/kg;

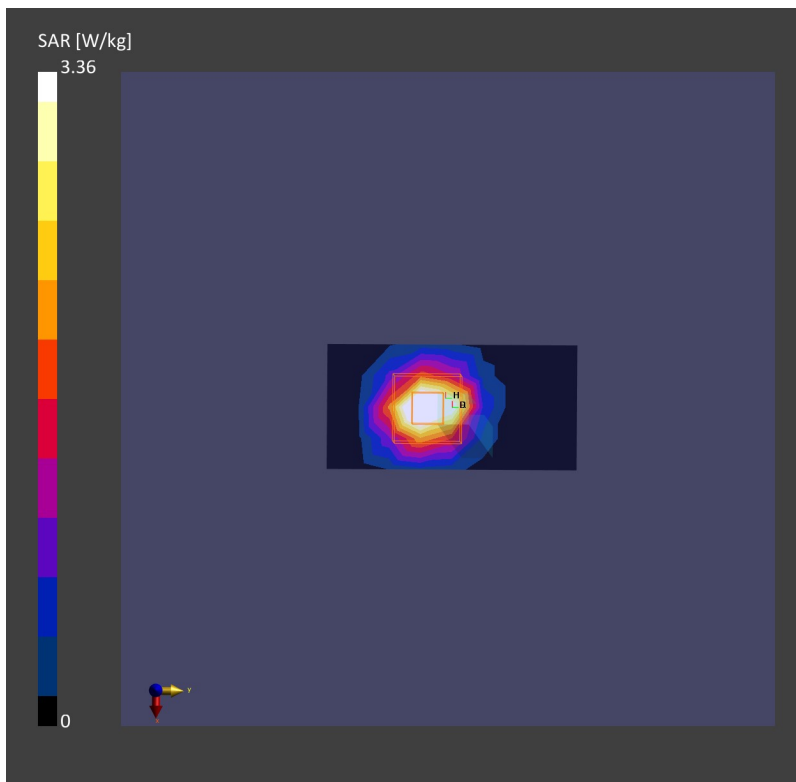

System Check_Head_3900MHz

DUT: D3900V2-SN:1048

Communication System: ; Frequency: 3900.0

Medium: HSL. Medium parameters used: $f= 3900.0$ MHz; $\sigma= 3.28$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(6.66, 6.66, 6.66); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.31 W/kg; SAR (10g) = 1.17 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR(1 g) = 3.52 W/kg; SAR(10 g) = 1.26 W/kg;

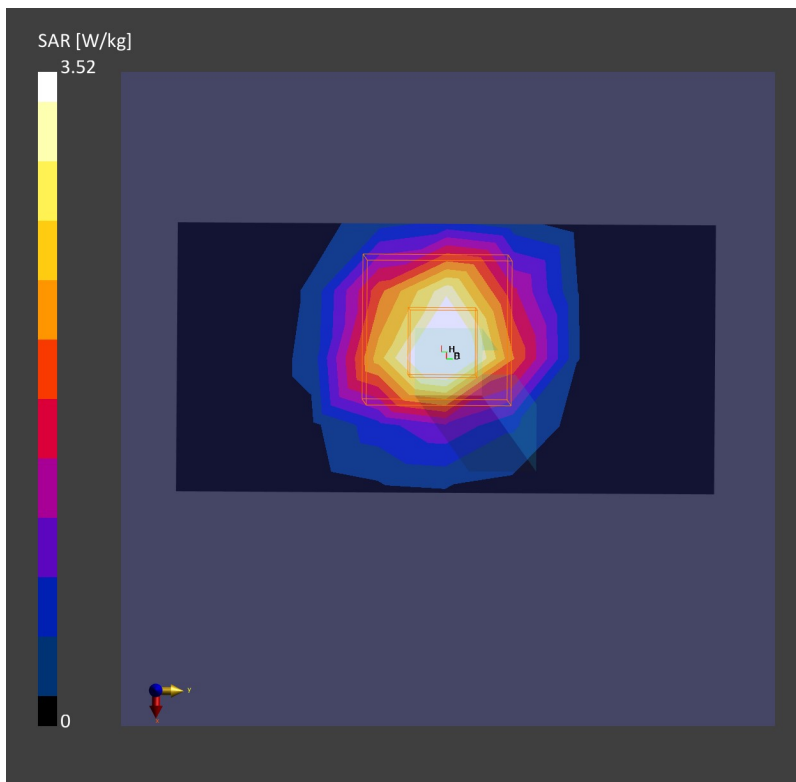

System Check_Head_2450MHz

DUT: D2450V2-SN:1040

Communication System: ; Frequency: 2450.0

Medium: HSL. Medium parameters used: $f= 2450.0$ MHz; $\sigma= 1.81$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.25, 8.25, 8.25); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.22 W/kg; SAR (10g) = 1.03 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = 0.03 dB

SAR (1g) = 2.48 W/kg; SAR (10g) = 1.14 W/kg;

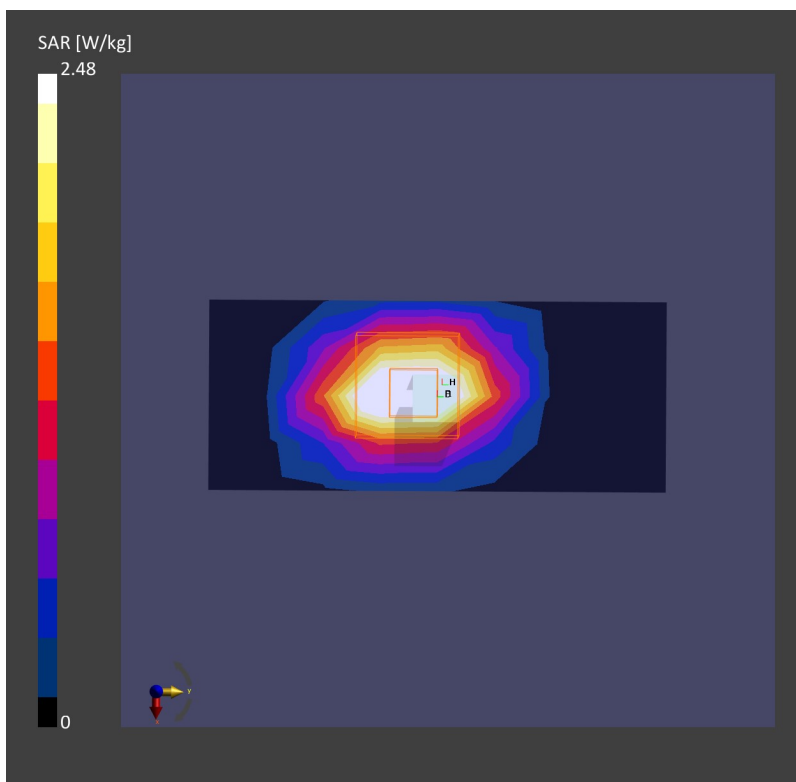

System Check_Head_5250MHz

DUT: D5GHzV2-SN:1113

Communication System: ; Frequency: 5250.0

Medium: HSL. Medium parameters used: $f= 5250.0$ MHz; $\sigma= 4.55$ S/m; $\epsilon_r = 36.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.65, 5.65, 5.65); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.75 W/kg; SAR (10g) = 0.986 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 3.92 W/kg; SAR (10g) = 1.11 W/kg;

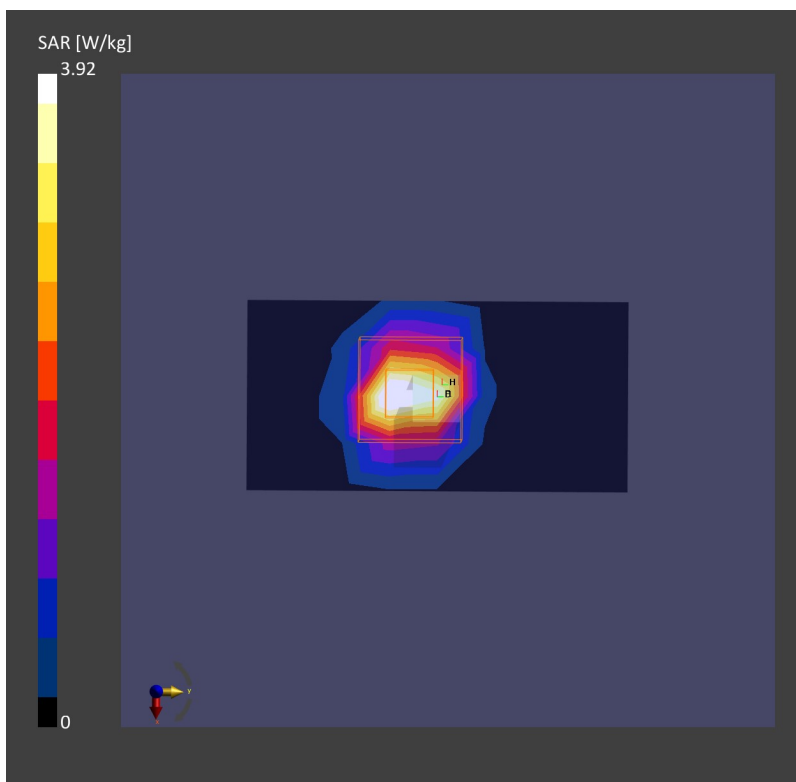

System Check_Head_5600MHz

DUT: D5GHzV2-SN:1113

Communication System: ; Frequency: 5600.0

Medium: HSL. Medium parameters used: $f= 5600.0$ MHz; $\sigma= 4.93$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(4.9, 4.9, 4.9); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.95 W/kg; SAR (10g) = 1.11 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 4.02 W/kg; SAR (10g) = 1.16 W/kg;

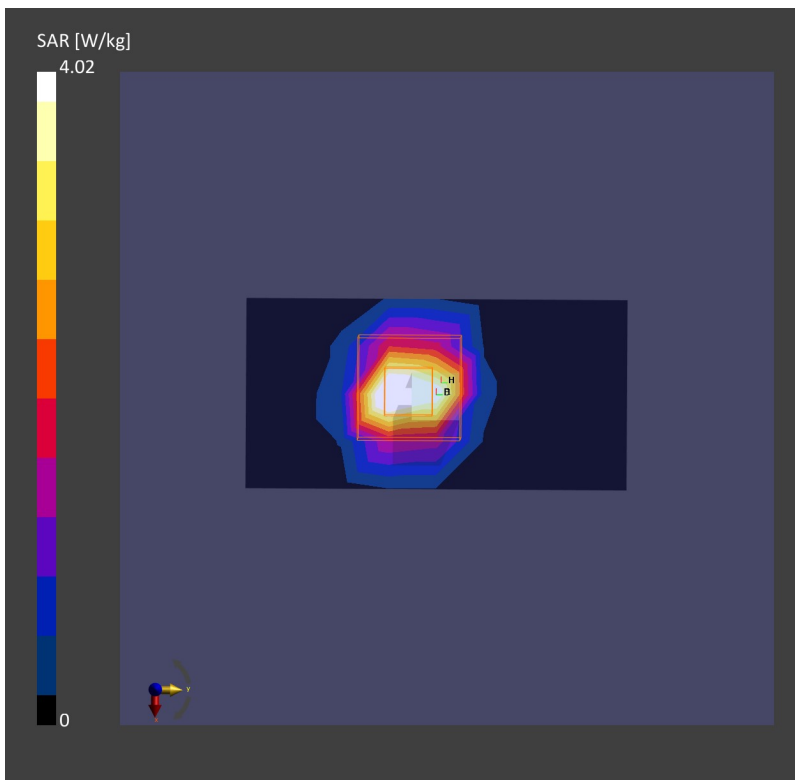

System Check_Head_5750MHz

DUT: D5GHzV2-SN:1113

Communication System: ; Frequency: 5750.0

Medium: HSL. Medium parameters used: $f= 5750.0$ MHz; $\sigma= 5.10$ S/m; $\epsilon_r = 35.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.1, 5.1, 5.1); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1279; Calibrated: 2022-10-26
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.86 W/kg; SAR (10g) = 1.02 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.08 dB

SAR (1g) = 4.00 W/kg; SAR (10g) = 1.15 W/kg;

