

System Check_Head_2450MHz

DUT:D2450V2 - SN:1040

Communication System: ; Frequency: 2450.0

Medium: MSL. Medium parameters used: $f= 2450.0$ MHz; $\sigma= 1.86$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7734; ConvF(7.98, 7.98, 7.98); Calibrated: 2022-06-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.03 W/kg; SAR (10g) = 0.989 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = 0.01 dB

SAR (1g) = 2.44 W/kg; SAR (10g) = 1.14 W/kg;

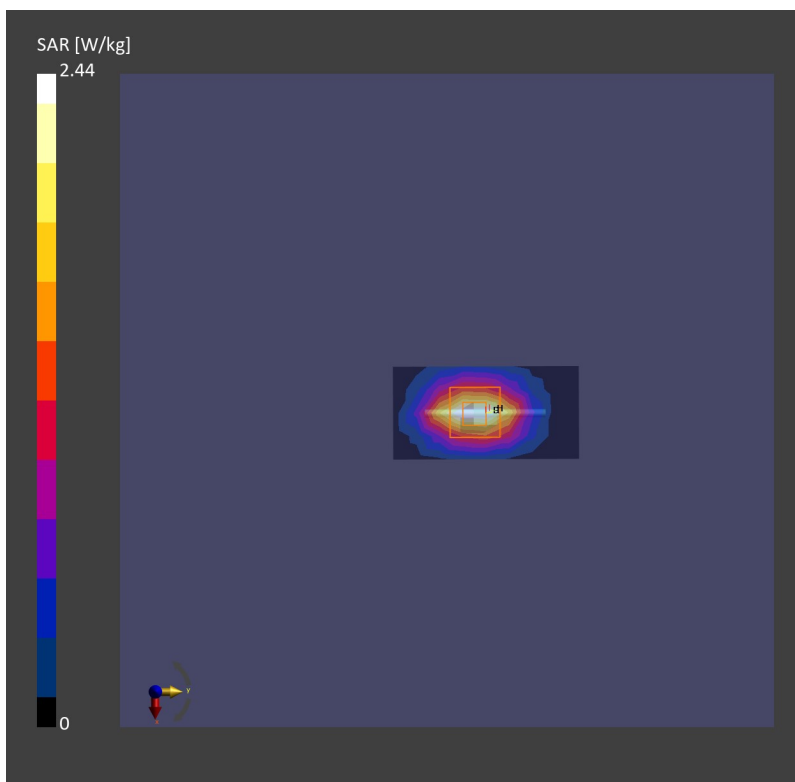

System Check_Head_5250MHz

DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5250.0

Medium: MSL. Medium parameters used: $f= 5250.0$ MHz; $\sigma= 4.60$ S/m; $\epsilon_r = 36.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7734; ConvF(5.76, 5.76, 5.76); Calibrated: 2022-06-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.19 W/kg; SAR (10g) = 0.967 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.84 W/kg; SAR (10g) = 1.09 W/kg;

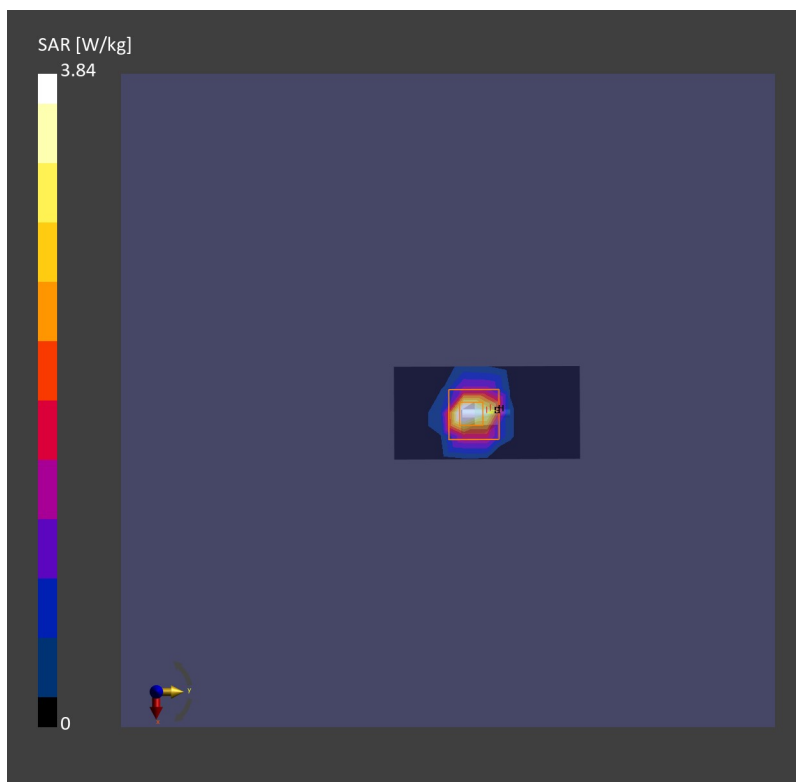

System Check_Head_5600MHz

DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5600.0

Medium: MSL. Medium parameters used: $f= 5600.0$ MHz; $\sigma= 4.99$ S/m; $\epsilon_r = 35.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7734; ConvF(5.01, 5.01, 5.01); Calibrated: 2022-06-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.53 W/kg; SAR (10g) = 1.06 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.05 dB

SAR (1g) = 3.93 W/kg; SAR (10g) = 1.14 W/kg;

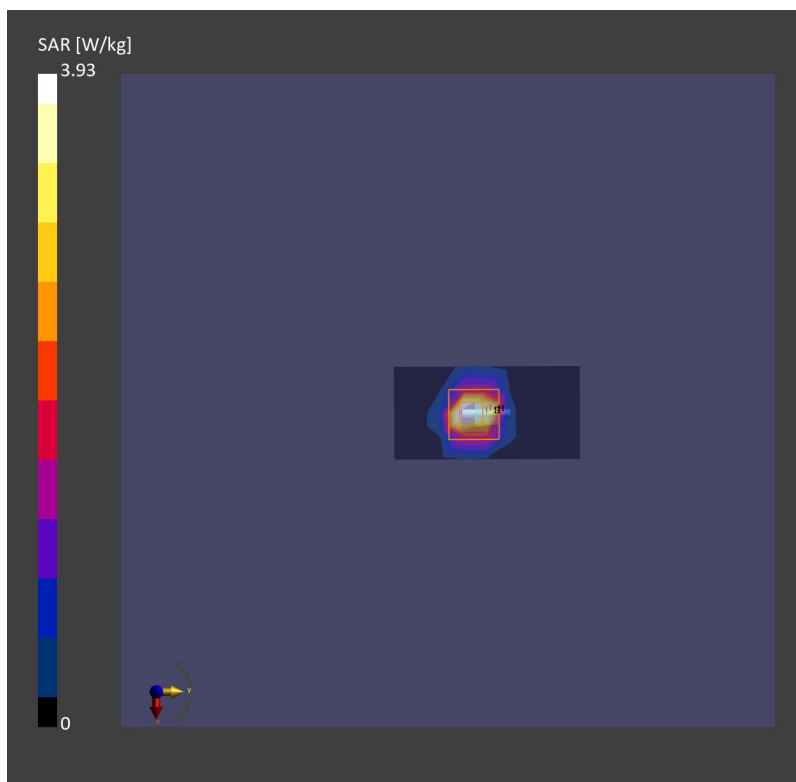

System Check_Head_5750MHz

DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5750.0

Medium: MSL. Medium parameters used: $f= 5750.0$ MHz; $\sigma= 5.17$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7734; ConvF(5.13, 5.13, 5.13); Calibrated: 2022-06-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.28 W/kg; SAR (10g) = 0.977 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.86 W/kg; SAR (10g) = 1.09 W/kg;

