




Appendix D


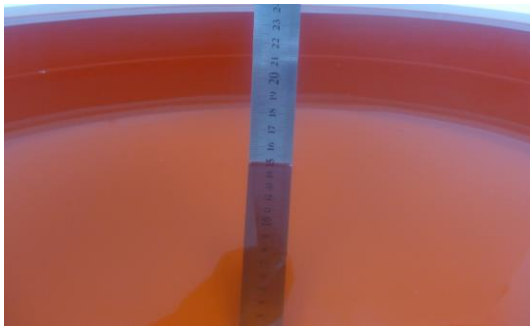
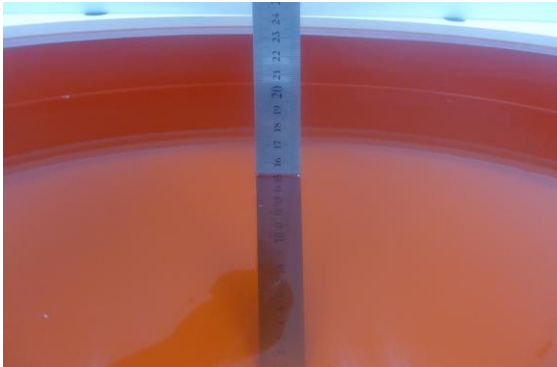

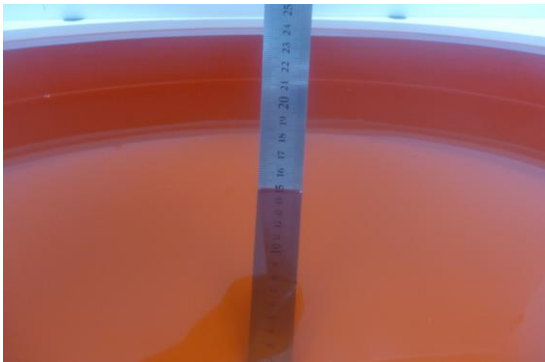
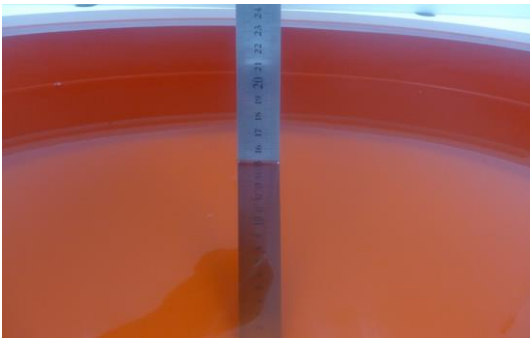
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

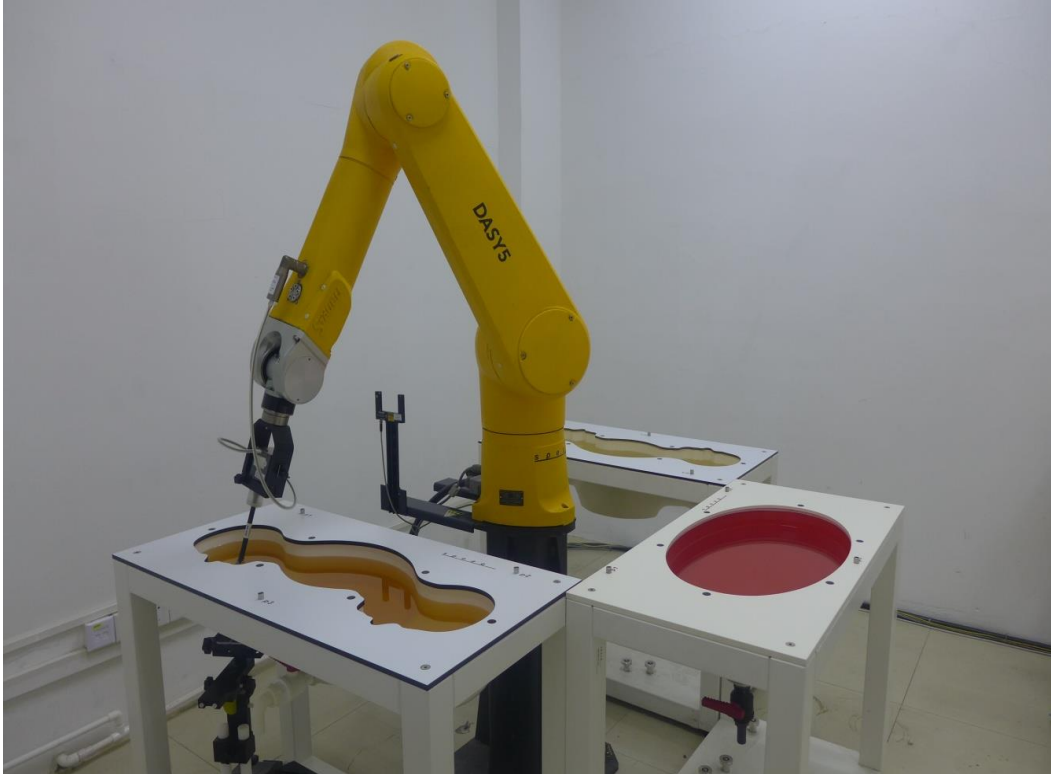





2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Head 1750
	
Photo 3: Tissue Simulant Liquid for Head 1950	Photo 4: Tissue Simulant Liquid for Head 2450
	
Photo 5: Tissue Simulant Liquid for Head 2600	Photo 6: Tissue Simulant Liquid for Head 5G
	

3. Photographs of EUT test position
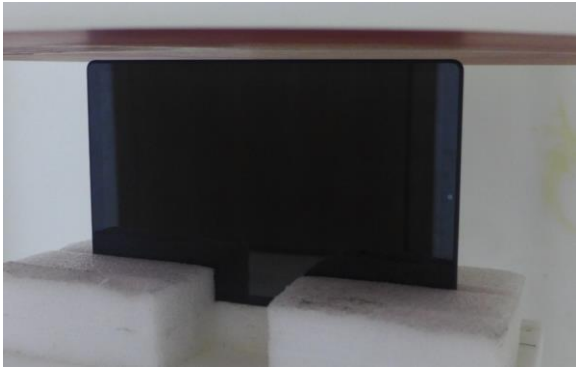
<p>Photo 7: Back side 0mm</p>	<p>Photo 8: Left side 0mm</p>
	
<p>Photo 9: Right side 0mm</p>	<p>Photo 10: Top side 0mm</p>
	
<p>Photo 11: Back side 18mm</p>	<p>Photo 12: Back side 19mm</p>
	

<p>Photo 13: Left side 7mm</p>	<p>Photo 14: Right side 16mm</p>
	
<p>Photo 15: Top side 19mm</p>	<p>Photo 16: Top side 21mm</p>
	

4. EUT Constructional Details

Photo 17: Front View	Photo 18: Back View
