



APPENDIX D: SYSTEM CERTIFICATE & CALIBRATION

D1: SAM PHANTOM

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Certificate of conformity / First Article Inspection

| | |
|-----------------------|--|
| Item | SAM Twin Phantom V4.0 |
| Type No | QD 000 P40 CA |
| Series No | TP-1150 and higher |
| Manufacturer / Origin | Untersee Composites Hauptstr. 69 CH-8559 Fruthwilen Switzerland |

Tests

The series production process used allows the limitation to test of first articles. Complete tests were made on the pre-series Type No. QD 000 P40 AA, Serial No. TP-1001 and on the series first article Type No. QD 000 P40 BA, Serial No. TP-1006. Certain parameters have been retested using further series units (called samples).

| Test | Requirement | Details | Units tested |
|----------------------|---|--|--------------------------------|
| Shape | Compliance with the geometry according to the CAD model. | IT'IS CAD File (*) | First article, Samples |
| Material thickness | Compliant with the requirements according to the standards | 2mm +/- 0.2mm in specific areas | First article, Samples |
| Material parameters | Dielectric parameters for required frequencies | 200 MHz – 3 GHz Relative permittivity < 5 Loss tangent < 0.05. | Material sample TP 104-5 |
| Material resistivity | The material has been tested to be compatible with the liquids defined in the standards | Liquid type HSL 1800 and others according to the standard. | Pre-series, First article |

Standards

- [1] CENELEC EN 50361
- [2] IEEE P1528-200x draft 6.5
- [3] IEC PT 62209 draft 0.9

(*) The IT'IS CAD file is derived from [2] and is also within the tolerance requirements of the shapes of [1] and [3].

Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of SAR measurements specified in standard [1] and draft standards [2] and [3].

Date 28.02.2002

Signature / Stamp

F. Bombault

**Schmid & Partner
Engineering AG**

Zeughausstrasse 43, CH-8004 Zurich
Tel. +41 1 245 97 00, Fax +41 1 245 97 79

Johannes Kofler



D2: DOSIMETRIC E-FIELD PROBE

IMPORTANT NOTICE

USAGE OF PROBES IN ORGANIC SOLVENTS

Diethylene Glycol Monobutyl Ether (the basis for liquids above 1 GHz), as many other organic solvents, is a very effective softener for synthetic materials. These solvents can cause irreparable damage to certain SPEAG products, except those which are explicitly declared as compliant with organic solvents.

Compatible Probes:

- ET3DV6
- ET3DV6R
- ES3DV2
- ER3DV6
- H3DV6

Important Note for ET3DV6 Probes:

The ET3DV6 probes shall not be exposed to solvents longer than necessary for the measurements and shall be cleaned daily after use with warm water and stored dry.

Client **Auden > Chunghwa Telecom**

CALIBRATION CERTIFICATE



Object(s) **ET3DV6 - SN:1790**
 Calibration procedure(s) **QA CAL-01.v2
Calibration procedure for dosimetric E-field probes**
 Calibration date: **August 29, 2003**
 Condition of the calibrated item **In Tolerance (according to the specific calibration document)**

This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.

Calibration Equipment used (M&TE critical for calibration)

| Model Type | ID # | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|-----------------------------------|--------------|---|------------------------|
| RF generator HP 8684C | US3642U01700 | 4-Aug-99 (SPEAG, in house check Aug-02) | In house check: Aug-05 |
| Power sensor E4412A | MY41495277 | 2-Apr-03 (METAS, No 252-0250) | Apr-04 |
| Power sensor HP 8481A | MY41092180 | 18-Sep-02 (Agilent, No. 20020918) | Sep-03 |
| Power meter EPM E4419B | GB41293874 | 2-Apr-03 (METAS, No 252-0250) | Apr-04 |
| Network Analyzer HP 8753E | US37390585 | 18-Oct-01 (Agilent, No. 24BR1033101) | In house check: Oct 03 |
| Fluke Process Calibrator Type 702 | SN: 6295803 | 3-Sep-01 (ELCAL, No.2360) | Sep-03 |

| | | | |
|----------------|---------------|---------------------|---|
| | Name | Function | Signature |
| Calibrated by: | Nico Vetterli | Technician |  |
| Approved by: | Katja Pokovic | Laboratory Director |  |

Date issued: August 28, 2003

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

Probe ET3DV6

SN:1790

Manufactured: May 28, 2003
Last calibration: August 29, 2003

Calibrated for DASYS Systems

(Note: non-compatible with DASYS2 system!)

DASY - Parameters of Probe: ET3DV6 SN:1790

Sensitivity in Free Space

| | | | | |
|-------|---|-------|-----------|----|
| NormX | 1.74 $\mu\text{V}/(\text{V}/\text{m})^2$ | DCP X | 96 | mV |
| NormY | 1.69 $\mu\text{V}/(\text{V}/\text{m})^2$ | DCP Y | 96 | mV |
| NormZ | 1.76 $\mu\text{V}/(\text{V}/\text{m})^2$ | DCP Z | 96 | mV |

Diode Compression

Sensitivity in Tissue Simulating Liquid

Head 900 MHz $\epsilon_r = 41.5 \pm 5\%$ $\sigma = 0.97 \pm 5\%$ mho/m

Valid for f=800-1000 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

| | | | |
|---------|------------------------------|------------------|-------------|
| ConvF X | 6.4 $\pm 9.5\%$ (k=2) | Boundary effect: | |
| ConvF Y | 6.4 $\pm 9.5\%$ (k=2) | Alpha | 0.48 |
| ConvF Z | 6.4 $\pm 9.5\%$ (k=2) | Depth | 2.13 |

Head 1800 MHz $\epsilon_r = 40.0 \pm 5\%$ $\sigma = 1.40 \pm 5\%$ mho/m

Valid for f=1710-1910 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

| | | | |
|---------|------------------------------|------------------|-------------|
| ConvF X | 5.1 $\pm 9.5\%$ (k=2) | Boundary effect: | |
| ConvF Y | 5.1 $\pm 9.5\%$ (k=2) | Alpha | 0.49 |
| ConvF Z | 5.1 $\pm 9.5\%$ (k=2) | Depth | 2.70 |

Boundary Effect

Head 900 MHz Typical SAR gradient: 5 % per mm

| | | | |
|-----------------------|------------------------------|-------------|-------------|
| Probe Tip to Boundary | | 1 mm | 2 mm |
| SAR _{be} [%] | Without Correction Algorithm | 9.4 | 5.2 |
| SAR _{be} [%] | With Correction Algorithm | 0.2 | 0.4 |





Head 1800 MHz Typical SAR gradient: 10 % per mm



| | | | |
|-----------------------|------------------------------|-------------|-------------|
| Probe Tip to Boundary | | 1 mm | 2 mm |
| SAR _{be} [%] | Without Correction Algorithm | 13.9 | 9.5 |
| SAR _{be} [%] | With Correction Algorithm | 0.2 | 0.1 |

Sensor Offset


| | | |
|----------------------------|---------------------------------|----|
| Probe Tip to Sensor Center | 2.7 | mm |
| Optical Surface Detection | 1.6 \pm 0.2 | mm |

Receiving Pattern (ϕ), $\theta = 0^\circ$

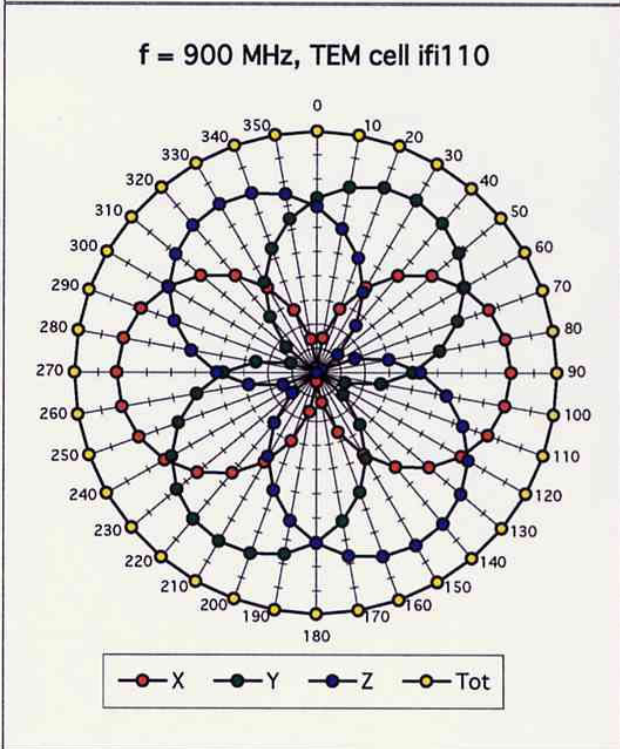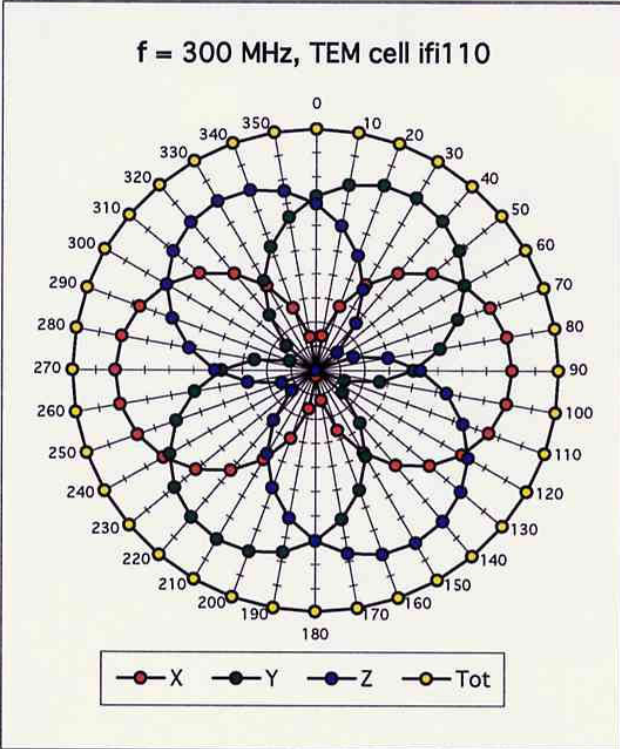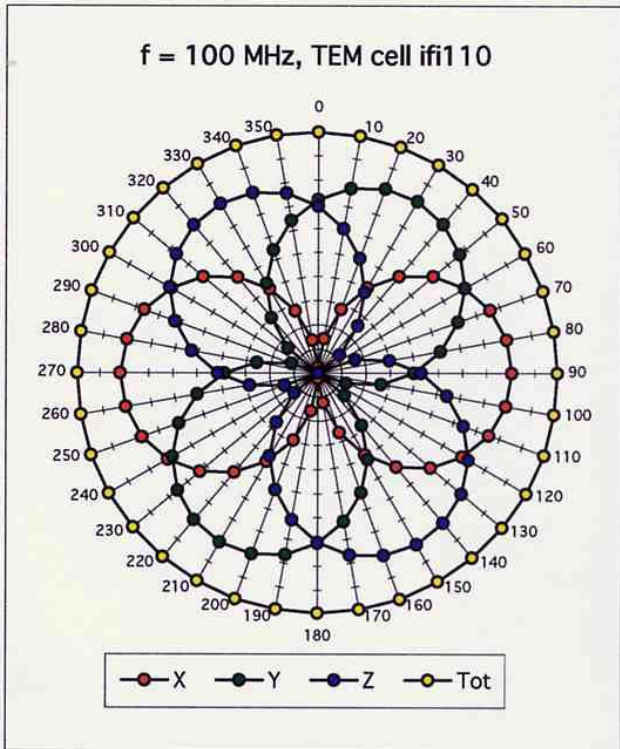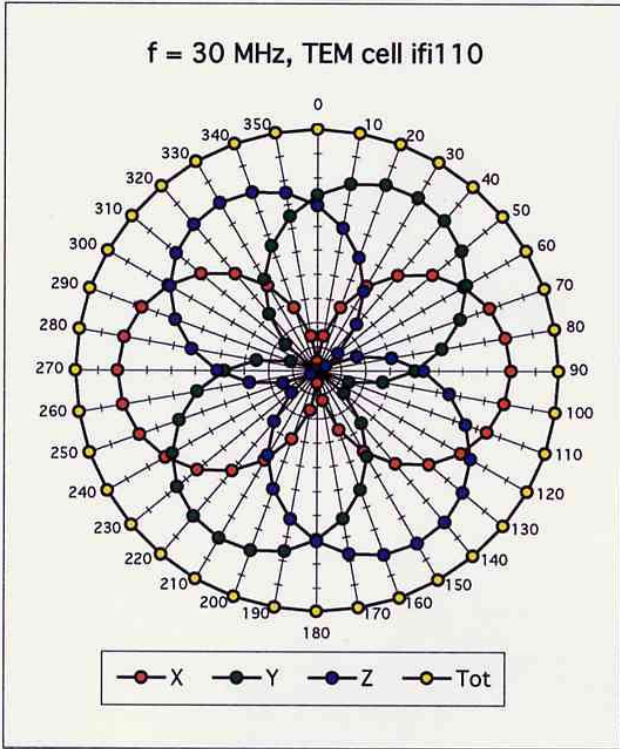

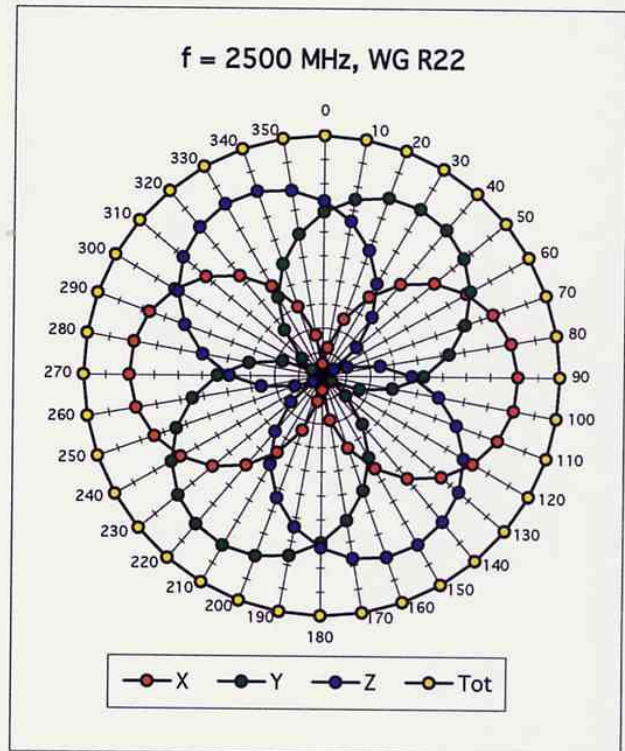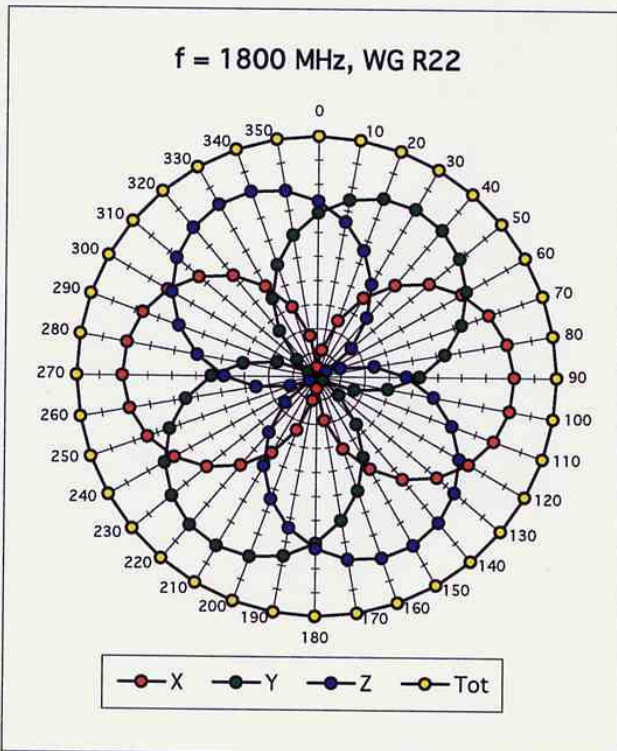


Isotropy Error (ϕ), $\theta = 0^\circ$

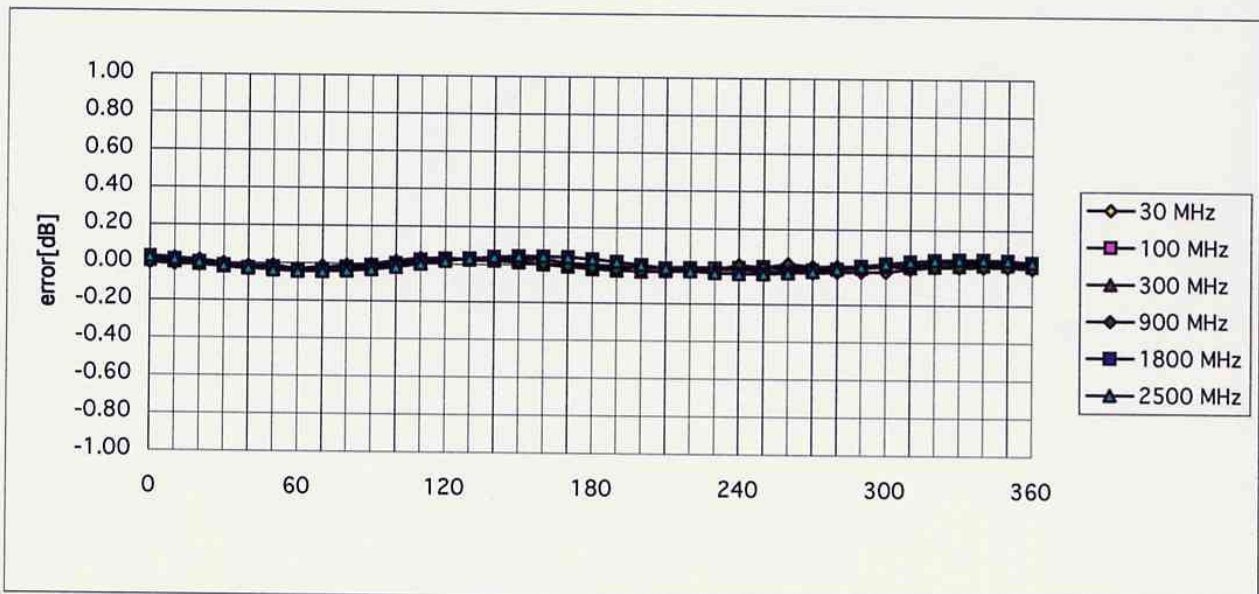

Frequency Response of E-Field

(TEM-Cell:ifi110, Waveguide R22)

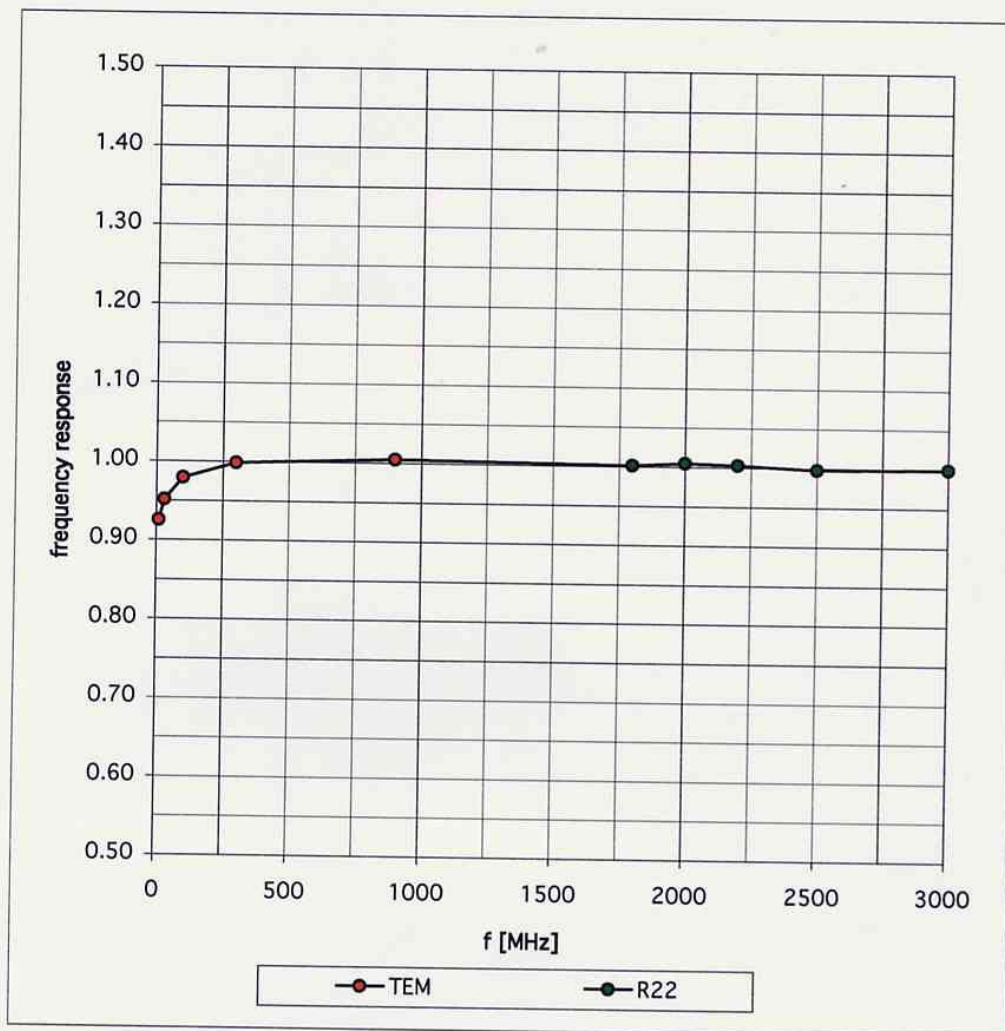

Dynamic Range f(SAR_{brain})

(Waveguide R22)

