


As noted in the Technical Report, the FCC identifier and label will not be placed on the device itself for two reasons: (i) the Capsule is so small that placing the label on it impracticable; and (ii) given that the M2A will always be within its packaging or inside the patient, except for the brief moment between when the package is opened and the device is ingested, having the label on the Capsule would be of little use. Therefore, consistent with 47 C.F.R. § 2.925(e) and the accompanying note ("a device intended to be implanted within the body of a . . . person would probably require an alternate method of identification"), the Applicant proposes, as an alternative method of affixing the label, to affix it to the Capsule's packaging as shown below and in the User's Manual, which is provided as a separate attachment accompanying the application.

The Capsule comes in packages of ten (10) in an M2A 10 Pak Capsule Case:



The label on the side of the M2A™ 10-Pak is as follows:

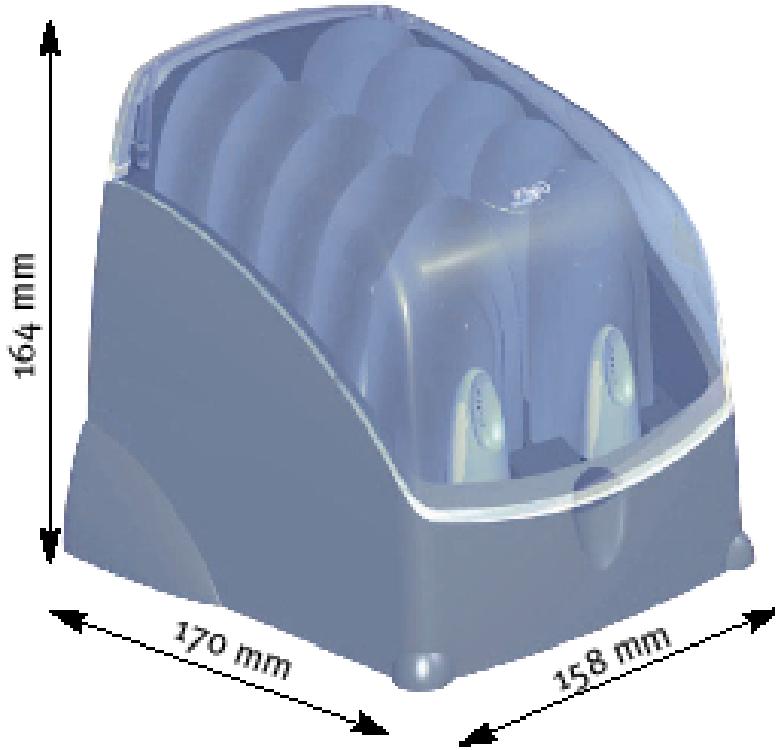