


1. Test Setup Photo


1. Test Setup Photo

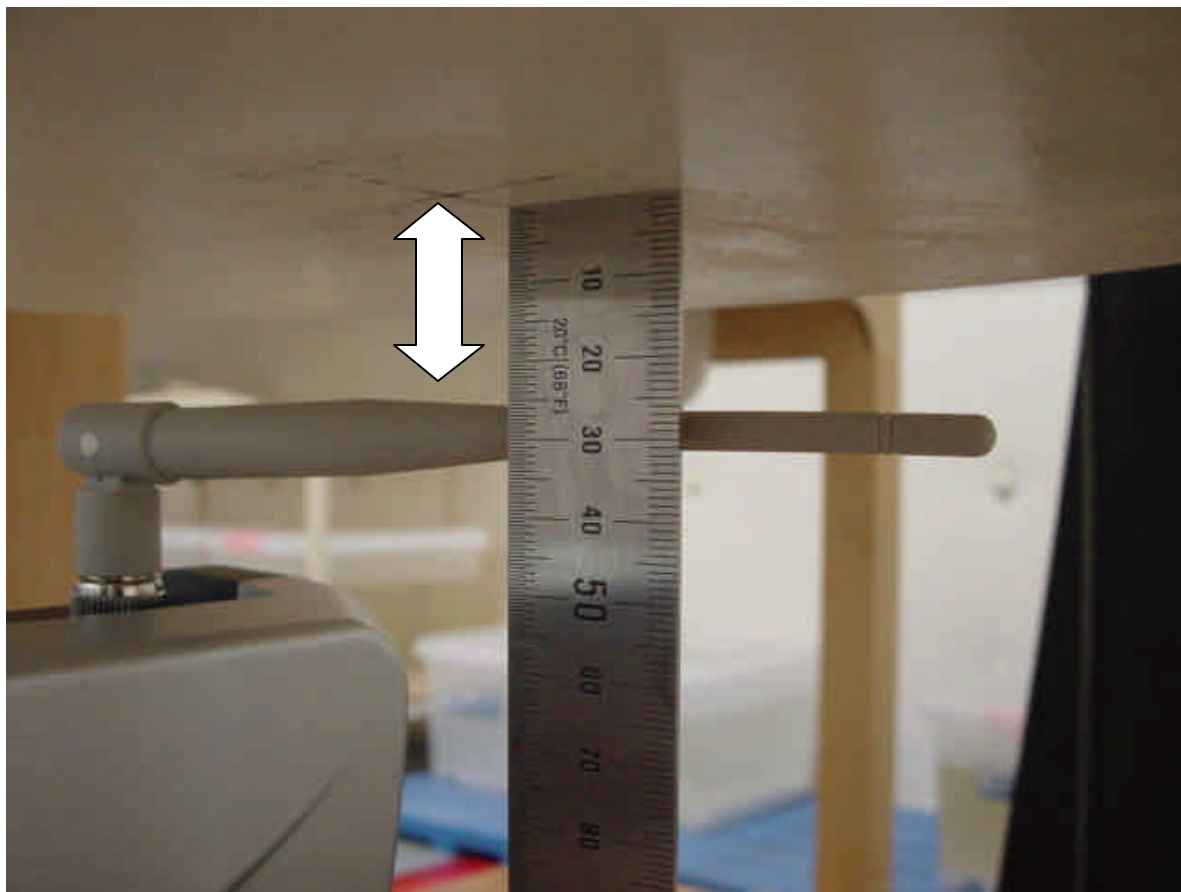

[Distance of 25 mm from the EUT]

Test Setup Photo

[1900MHz Body Tissue Liquid Depth : 15cm]

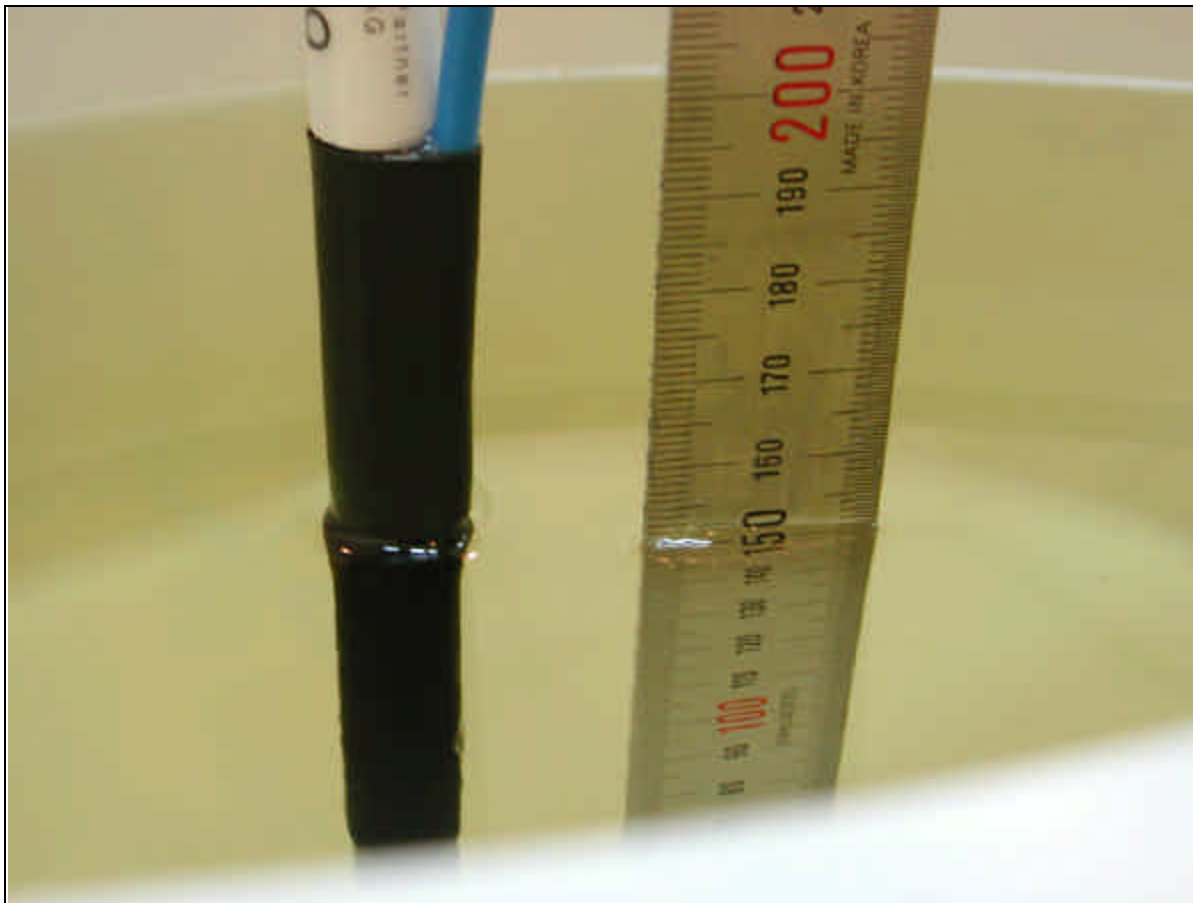

Test Setup Photo (Validation)