

FCC SAR TEST REPORT

Test File No : F690501/RF-SAR002266-A1

Equipment Under Test	Blood Glucose Meter
Model No.	GM01CAB
Alternative Model	GM01CAD
Applicant	i-SENS, Inc.
Address of Applicant	43, Banpo-daero 28-gil, Seocho-gu, Seoul, 137-873 Koera
FCC ID	OELGM01CAB
Device Category	Portable Device
Exposure Category	General Population/Uncontrolled Exposure
Standards	FCC 47 CFR Part 2 (2.1093) IEEE 1528, 2003 ANSI/IEEE C95.1, C95.3
Date of Test(s)	2015-02-26
Date of Issue	2015-04-09

In the configuration tested, the EUT complied with the standards specified above.

Remarks:

This report details the results of the testing carried out on one sample, the results contained in this test report do not relate to other samples of the same product. The manufacturer should ensure that all products in series production are in conformity with the product sample detailed in this report. This report may only be reproduced and distributed in full. If the product in this report is used in any configuration other than that detailed in the report, the manufacturer must ensure the new system complies with all relevant standards. Any mention of SGS Korea Co., Ltd. or testing done by SGS Korea Co., Ltd. in connection with distribution or use of the product described in this report must be approved by SGS Korea Co., Ltd. in writing.



**Report prepared by /
Minhyuk Han
Test Engineer**



**Approved by /
Jongwon Ma
Technical Manager**

Revision history

Revision	Date of issue	Revisions	Revised By
-	April, 06, 2015	Initial issue	Minhyuk Han
A1	April, 09, 2015	Updated Report - Corrected typo, Changed highest report SAR values	Minhyuk Han

Contents

1. TESTING LABORATORY	5
2. DETAILS OF MANUFACTURER	5
3. DESCRIPTION OF EUT(S)	5
4. THE HIGHEST REPORTED SAR VALUES	5
5. TEST METHODOLOGY	6
6. TESTING ENVIRONMENT	6
7. SPECIFIC ABSORPTION RATE (SAR)	7
7.1 INTRODUCTION	7
7.2 SAR DEFINITION	7
7.3 TEST STANDARDS AND LIMITS	7
8. THE SAR MEASUREMENT SYSTEM	9
9. SYSTEM COMPONENTS	10
9.1 PROBE	10
9.2 SAM PHANTOM	10
9.3 DEVICE HOLDER	10
10. SAR MEASUREMENT PROCEDURES	11
10.1 NORMAL SAR MEASUREMENT PROCEDURE	11
11. DEFINITION OF REFERENCE	13
11.1 SAR EVALUATION PROCEDURES FOR UMPC MINI-TABLET DEVICES	13
11.2 DUT ANTENNA LOCATIONS	13
11.3 UMPC MINI-TABLET DEVICES SIDES FOR SAR TESTING CONFIGURATIONS	13
12. SAR SYSTEM VERIFICATION	14
13. TISSUE SIMULANT FLUID FOR THE FREQUENCY BAND	15
14. TEST SYSTEM VALIDATION	16
15. INSTRUMENTS LIST	17
16. FCC POWER MEASUREMENT PROCEDURES	18
17. MEASURED AND REPORTED SAR	18
18. NOMINAL AND MAXIMUM OUTPUT POWER SPECIFICATIONS	18
19. RF CONDUCTED POWER MEASUREMENT	19
19.1 WCDMA	19
19.1.1 OUTPUT POWER VERIFICATION	19
19.1.2 BODY SAR MEASUREMENTS	19
19.1.3 PROCEDURES USED TO ESTABLISH RF SIGNAL FOR SAR HSDPA DATA DEVICES	19
20. SAR DATA SUMMARY	21
20.1 WCDMA V BODY SAR	21



SGS Korea Co., Ltd.

4, LS-ro 182beon-gil, Gunpo-si, Gyeonggi-do, 435-040

Tel. 031-428-5700 / Fax. 031-427-2371

<http://www.sgsgroup.kr>

Page : 4 / 61

20.2 WCDMA II BODY SAR _____	21
21. SAR MEASUREMENT VARIABILITY _____	23
21.1 MEASUREMENT VARIABILITY _____	23
21.2 MEASUREMENT UNCERTAINTY _____	23
APPENDIXES LIST _____	24
APPENDIX A.1 VERIFICATION TEST PLOTS FOR 835 MHZ_BODY _____	25
APPENDIX A.2 VERIFICATION TEST PLOTS FOR 1900 MHZ_BODY _____	26
APPENDIX A.3 SAR TEST PLOTS FOR WCDMA V (BODY SAR) _____	27
APPENDIX A.4 SAR TEST PLOTS FOR WCDMA II (BODY SAR) _____	28
APPENDIX B.1 UNCERTAINTY ANALYSIS DASY5 #3 _____	29
APPENDIX C.1 CALIBRATION CERTIFICATE FOR PROBE (SN: 1782) _____	30
APPENDIX C.2 CALIBRATION CERTIFICATE FOR DAE _____	41
APPENDIX C.3 CALIBRATION CERTIFICATE FOR DIPOLE _____	46
-THE END- _____	61

1. Testing Laboratory

Company Name	SGS Korea Co., Ltd. (Gunpo Laboratory)
Address	Wireless Div. 4, LS-ro 182beon-gil, Gunpo-si, Gyeonggi-do, 435-040 Republic of Korea
Telephone	+82 +31 428 5700
FAX	+82 +31 427 2371
Homepage	All SGS services are rendered in accordance with the applicable SGS conditions of service available on request and accessible at http://www.sgs.com/en/Terms-and-Conditions.aspx

2. Details of Manufacturer

Applicant	i-SENS, Inc.
Address	43, Banpo-daero 28-gil, Seocho-gu, Seoul, 137-873 Koera
Contact Person	Hyunyoung Shin
Email	hyshin@i-sens.com
Phone No.	+82-2-910-0834

3. Description of EUT(s)

EUT Type	Blood Glucose Meter
Model	GM01CAB
Alternative Model	GM01CAD
IMEI Number	B2C800C00011
Mode of Operation	WCDMA850 / WCDMA1900
Duty Cycle	1 (WCDMA)
Body worn Accessory	None
Tx Frequency Range	WCDMA 850 (826.40 MHz ~ 846.60 MHz) WCDMA1900 (1852.4 MHz ~ 1907.6 MHz)

4. The Highest Reported SAR Values

Equipment Class	Band	Tx Frequency (MHz)	Reported 1g SAR (W/kg)
			Body-Worn
PCB	WCDMA850	826.40 ~ 846.60	0.80
	WCDMA1900	1850.40 ~ 1907.60	1.18
Simultaneous SAR per KDB 690783 D01v01r03			N/A

5. Test Methodology

ANSI C95.1-1999: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz. It specifies the maximum exposure limit of 1.6 W/kg as averaged over any 1 gram of tissue for portable devices being used within 20 cm of the user in the uncontrolled environment.

Test tests documented in this report were performed in accordance with IEEE Standard 1528-2003 & IEEE 1528a-2005 and the following published KDB procedures.

In additions;

<input checked="" type="checkbox"/>	KDB 865664 D01v01r03	SAR Measurement Requirements for 100 MHz to 6 GHz
<input checked="" type="checkbox"/>	KDB 447498 D01v05r02	Mobile and Portable Devices RF Exposure Procedures and Equipment Authorization Policies
<input type="checkbox"/>	KDB 447498 D02v02	SAR Measurement Procedures for USB Dongle Transmitters
<input type="checkbox"/>	KDB 248227 D01v01r02	SAR Measurement Procedures for 802.11a,b,g Transmitters
<input type="checkbox"/>	KDB 615223 D01v01	802.16e/WiMax SAR Measurement Guidance
<input type="checkbox"/>	KDB 616217 D04v01r01	SAR Evaluation Considerations for Laptop, Notebook, Netbook and Tablet Computers
<input type="checkbox"/>	KDB 643646 D01v01r01	SAR Test Reduction Considerations for Occupational PTT Radios
<input type="checkbox"/>	KDB 648474 D03v01r02	Evaluation and Approval Considerations for Handsets with Specific Wireless Charging Battery Covers
<input type="checkbox"/>	KDB 648474 D04v01r02	SAR Evaluation Considerations for Wireless Handsets
<input type="checkbox"/>	KDB 680106 D01v02	RF Exposure Considerations for Low Power Consumer Wireless Power Transfer Applications
<input checked="" type="checkbox"/>	KDB 941225 D01v03	3G SAR Measurement Procedures
<input type="checkbox"/>	KDB 941225 D05v02r03	SAR Evaluation Considerations for LTE Devices
<input type="checkbox"/>	KDB 941225 D06v02	SAR Evaluation Procedures for Portable Devices with Wireless Router Capabilities
<input checked="" type="checkbox"/>	KDB 941225 D07v01r01	SAR Evaluation Procedures for UMPC Mini-Tablet Devices

6. Testing Environment

Ambient temperature	18°C ~ 25°C
Relative humidity	30% ~ 70%
Liquid temperature of during the test	< ± 2°C
Ambient noise & Reflection	< 0.012 W/kg

7. Specific Absorption Rate (SAR)

7.1 Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled

7.2 SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density (ρ). The equation description is as below:

$$SAR = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dv} \right)$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$SAR = C \left(\frac{\delta T}{\delta t} \right)$$

Where: C is the specific heat capacity, δT is the temperature rise and δt is the exposure duration, or related to the electrical field in the tissue by

$$SAR = \frac{\sigma |E|^2}{\rho}$$

Where: σ is the conductivity of the tissue, ρ is the mass density of the tissue and E is the RMS electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.

7.3 Test Standards and Limits

According to FCC 47CFR §2.1093(d) The limits to be used for evaluation are based generally on criteria published by the American National Standards Institute (ANSI) for localized specific absorption rate ("SAR") in Section 4.2 of "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz," ANSI/IEEE C95.3-2003, Copyright 2003 by the Institute of Electrical and Electronics Engineers, Inc., New York, New York 10017. These criteria for SAR evaluation are similar to those recommended by the National Council on Radiation Protection and Measurements (NCRP) in "Biological Effects and Exposure Criteria for Radio frequency Electromagnetic Fields," NCRP Report No. 86, Section 17.4.5. Copyright NCRP, 1986, Bethesda, Maryland 20814. SAR is a measure of the rate of energy absorption due to exposure to an RF transmitting source. SAR values have been related to threshold levels for potential biological hazards. The criteria to be used are specified in paragraphs (d)(1) and (d)(2) of this section and shall apply for portable devices transmitting in the

frequency range from 100 kHz to 6 GHz. Portable devices that transmit at frequencies above 6 GHz are to be evaluated in terms of the MPE limits specified in § 1.1310 of this chapter. Measurements and calculations to demonstrate compliance with MPE field strength or power density limits for devices operating above 6 GHz should be made at a minimum distance of 5 cm from the radiating source.

(1) Limits for Occupational/Controlled exposure: 0.4 W/kg as averaged over the whole-body and spatial peak SAR not exceeding 8 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 20 W/kg, as averaged over an 10 grams of tissue (defined as a tissue volume in the shape of a cube). Occupational/Controlled limits apply when persons are exposed as a consequence of their employment provided these persons are fully aware of and exercise control over their exposure. Awareness of exposure can be accomplished by use of warning labels or by specific training or education through appropriate means, such as an RF safety program in a work environment.

(2) Limits for General Population/Uncontrolled exposure: 0.08 W/kg as averaged over the whole-body and spatial peak SAR not exceeding 1.6 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 4 W/kg, as averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube). General Population/Uncontrolled limits apply when the general public may be exposed, or when persons that are exposed as a consequence of their employment may not be fully aware of the potential for exposure or do not exercise control over their exposure. Warning labels placed on consumer devices such as cellular telephones will not be sufficient reason to allow these devices to be evaluated subject to limits for occupational/controlled exposure in paragraph (d)(1) of this section.

Human Exposure	Uncontrolled Environment General Population	Controlled Environment Occupational
Partial Peak SAR (Partial)	1.60 m W/g	8.00 m W/g
Partial Average SAR (Whole Body)	0.08 m W/g	0.40 m W/g
Partial Peak SAR (Hands/Feet/Ankle/Wrist)	4.00 m W/g	20.00 m W/g

1. The spatial Peak value of the SAR averaged over any 1g gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.
2. The spatial Average value of the SAR averaged over the whole body.
3. The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

8. The SAR Measurement System

A block diagram of the SAR measurement System is given in Fig. a. This SAR Measurement System uses a Computer-controlled 3-D stepper motor system (SPEAG DASY 5 professional system). The model ET3DV6 field probe is used to determine the internal electric fields. The SAR can be obtained from the equation $SAR = \sigma (|E_i|^2) / \rho$ where σ and ρ are the conductivity and mass density of the tissue-simulant.

The DASY 5 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Staubli TX family) with controller, teach pendant and software. An arm extension is for accommodating the data acquisition electronics (DAE).
- A dosimeter probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- Data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.

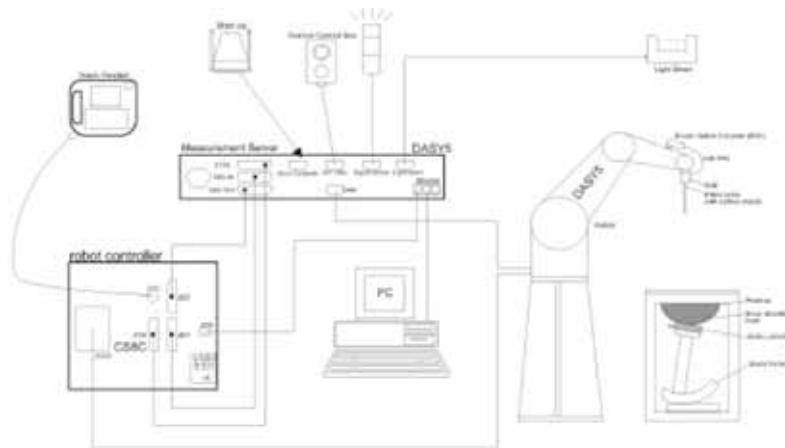



Fig a. The microwave circuit arrangement used for SAR system verification

- The Electro-optical converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection. The EOC is connected to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- A computer operating Windows7
- DASY 5 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM phantom enabling testing left-hand and right-hand usage.
- Tissue simulating liquid mixed according to the given recipes.
- Validation dipole kits allowing to validate the proper functioning of the system.

9. System Components

9.1 Probe

- Construction** : Symmetrical design with triangular core Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g. glycol).
- Calibration** : In air from 10 MHz to 2.5 GHz In brain simulating tissue (accuracy $\pm 8\%$)
- Frequency** : 10 MHz to >6 GHz; Linearity: ± 0.2 dB (30 MHz to 3 GHz)
- Directivity** : ± 0.2 dB in brain tissue (rotation around probe axis)
 ± 0.4 dB in brain tissue (rotation normal to probe axis)
- Dynamic Range** : 5 μ W/g to >100 mW/g; Linearity: ± 0.2 dB
- Dimensions** : Overall length: 330 mm
 Tip length: 16 mm
 Body diameter: 12 mm
 Tip diameter: 6.8 mm
 Distance from probe tip to dipole centers: 2.7 mm
- Application** : General dosimetry up to 3 GHz Compliance tests of mobile phone

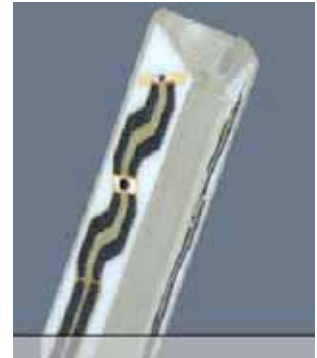

ET3DV6 E-Field Probe

NOTE:

- The Probe parameters have been calibrated by the SPEAG. Please reference "APPENDIX C" for the Calibration Certification Report.

9.2 SAM Phantom

- Construction** : The SAM Phantom is constructed of a fiberglass shell integrated in a wooden table. The shape of the shell is based on data from an anatomical study designed to determine the maximum exposure in at least 90 % of all users. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents the evaporation of the liquid. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot
- Shell Thickness** : 2.0 mm \pm 0.1 mm
- Filling Volume** : Approx. 25 liters



SAM Phantom

9.3 Device Holder

- Construction:** : In combination with the Twin SAM PhantomV4.0/V4.0C or Twin SAM, the Mounting Device (made from POM) enables the rotation of the mounted transmitter in spherical coordinates, whereby the rotation point is the ear opening. The devices can be easily and accurately positioned according to IEC, IEEE, CENELEC, FCC or other specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).



Device Holder

10. SAR Measurement Procedures

10.1 Normal SAR Measurement Procedure

Step 1: Power Reference Measurement

The Power Reference Measurement and Power Drift Measurements are for monitoring the power drift of the device under test in the batch process. The Minimum distance of probe sensors to surface determines the closest measurement point to phantom surface. The minimum distance of probe sensors to surface is 4 mm. This distance cannot be smaller than the Distance of sensor calibration points to probe tip as defined in the probe properties.

Step 2 and 3: Area Scan & Zoom Scan Procedures

The entire evaluation of the spatial peak values is performed within the Post-processing engine (SEMCAD). The system always gives the maximum values for the 1 g and 10 g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

1. The extraction of the measured data (grid and values) from the Zoom Scan.
2. The calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
3. The generation of a high-resolution mesh within the measured volume
4. The interpolation of all measured values from the measurement grid to the high-resolution grid
5. The extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
6. The calculation of the averaged SAR within masses of 1 g and 10 g.

Step 4: Power drift measurement

The Power Drift Measurement measures the field at the same location as the most recent power reference measurement within the same procedure, and with the same settings. The Power Drift Measurement gives the field difference in dB from the reading conducted within the last Power Reference Measurement. This allows a user to monitor the power drift of the device under test within a batch process. The measurement procedure is the same as Step 1.

< Area and Zoom Scan Resolutions per FCC KDB Publication 865664 D01v01r03 >


		≤ 3 GHz	> 3 GHz
Maximum distance from closest measurement point (geometric center of probe sensors) to phantom surface		5 ± 1 mm	½·δ·ln(2) ± 0.5 mm
Maximum probe angle from probe axis to phantom surface normal at the measurement location		30° ± 1°	20° ± 1°
Maximum area scan spatial resolution: Δx _{Area} , Δy _{Area}		≤ 2 GHz: ≤ 15 mm 2 – 3 GHz: ≤ 12 mm	3 – 4 GHz: ≤ 12 mm 4 – 6 GHz: ≤ 10 mm
		When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the above, the measurement resolution must be ≤ the corresponding x or y dimension of the test device with at least one measurement point on the test device.	
Maximum zoom scan spatial resolution: Δx _{Zoom} , Δy _{Zoom}		≤ 2 GHz: ≤ 8 mm 2 – 3 GHz: ≤ 5 mm*	3 – 4 GHz: ≤ 5 mm* 4 – 6 GHz: ≤ 4 mm*
Maximum zoom scan spatial resolution, normal to phantom surface	uniform grid: Δz _{Zoom} (n)	≤ 5 mm	3 – 4 GHz: ≤ 4 mm 4 – 5 GHz: ≤ 3 mm 5 – 6 GHz: ≤ 2 mm
	graded grid Δz _{Zoom} (1): between 1 st two points closest to phantom surface	≤ 4 mm	3 – 4 GHz: ≤ 3 mm 4 – 5 GHz: ≤ 2.5 mm 5 – 6 GHz: ≤ 2 mm
	Δz _{Zoom} (n>1): between subsequent points	≤ 1.5·Δz _{Zoom} (n-1)	
Minimum zoom scan volume	x, y, z	≥ 30 mm	3 – 4 GHz: ≥ 28 mm 4 – 5 GHz: ≥ 25 mm 5 – 6 GHz: ≥ 22 mm
<p>Note: δ is the penetration depth of a plane-wave at normal incidence to the tissue medium; see draft standard IEEE P1528-2011 for details.</p> <p>* When zoom scan is required and the <u>reported</u> SAR from the area scan based <i>1-g SAR estimation</i> procedures of KDB 447498 is ≤ 1.4 W/kg, ≤ 8 mm, ≤ 7 mm and ≤ 5 mm zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.</p>			

11. Definition of Reference

11.1 SAR Evaluation Procedures for UMPC Mini-Tablet Devices

This type of mini-tablets is normally optimized for mobile web access and multimedia use. The test procedures are applicable to devices with a display and overall diagonal dimension ≤ 20 cm (~7.9"). These devices are typically operated like a mini-tablet and are usually designed with certain UMPC features and operating characteristics; therefore, the term "UMPC Mini-Tablet" is used to identify the SAR test requirements for this category of devices. A composite test separation distance of 5 mm is applied to test UMPC mini-tablet transmitters and to maintain RF exposure conservativeness for the interactive operations associated with this type of devices.

11.2 DUT Antenna Locations

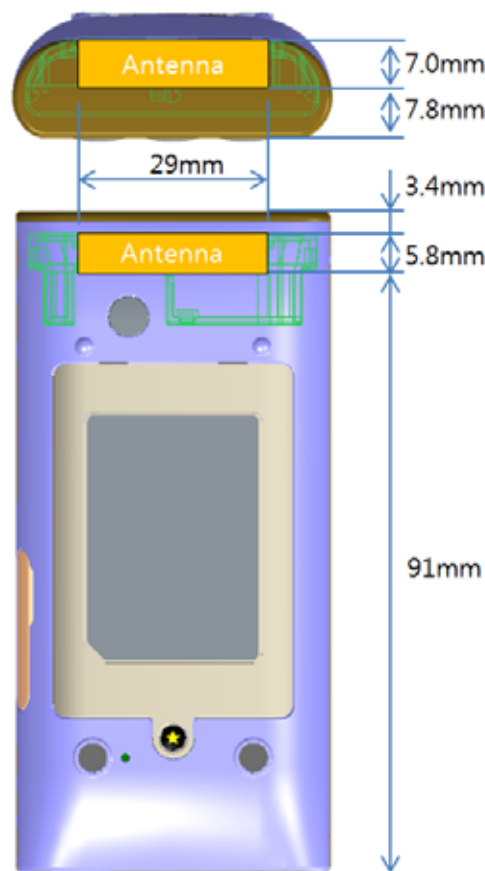

11.3 UMPC Mini-Tablet Devices sides for SAR Testing configurations

Mode	Rear	Front	Left Edge	Right Edge	Bottom	Top
WCDMA V	Yes	Yes	Yes	Yes	No	Yes
WCDMA II	Yes	Yes	Yes	Yes	No	Yes

Notes

Particular DUT edges were not required to be evaluated for Wireless Router SAR if the edges were greater than 2.5 cm from the transmitting antenna according to FCC Publication 941225 D06v01r01 guidance, page 2. The antenna document shows the distances between the transmit antennas and the edges of the device.

12. SAR System Verification

The microwave circuit arrangement for system verification is sketched in Fig. 9. The daily system accuracy verification occurs within the flat section of the SAM phantom. A SAR measurement was performed to see if the measured SAR was within +/- 10% from the target SAR values. These tests were done at 835 MHz, 1900 MHz. The tests were conducted on the same days as the measurement of the DUT. The obtained results from the system accuracy verification are displayed in the table 1. (SAR values are normalized to 1W forward power delivered to the dipole). During the tests, the ambient temperature of the laboratory was in the range $(22 \pm 2) ^\circ \text{C}$, the relative humidity was in the range $(55 \pm 5) \% \text{ R.H}$ and the liquid depth above the ear reference points was $\geq 15 \text{ cm} \pm 5 \text{ mm}$ (frequency $\leq 3 \text{ GHz}$) or $\geq 10 \text{ cm} \pm 5 \text{ mm}$ (frequency $> 3 \text{ GHz}$) in all the cases. It is seen that the system is operating within its specification, as the results are within acceptable tolerance of the reference values.

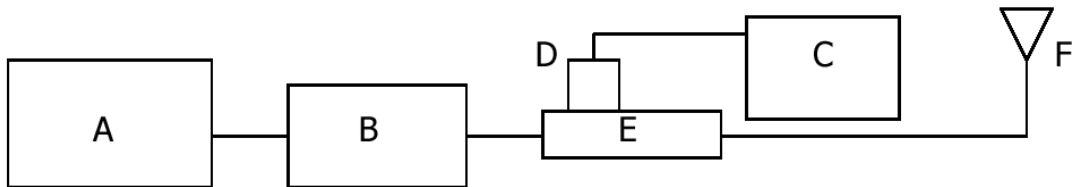


Fig 9. The microwave circuit arrangement used for SAR system verification

- A. Agilent Model E8247C Signal Generator
- B. EMPOWER Model 2001-BBS3Q7ECK Amplifier
- C. Agilent Model E4419B Power Meter
- D. Agilent Model 9300H Power Sensor
- E. Agilent Model 86205A Directional RF Bridges
- F. Reference dipole Antenna



Photo of the dipole Antenna

Verification Kit	Probe S/N	Tissue (MHz)	Target SAR 1 g from Standard (1 W)	Target SAR 10 g from Standard (1 W)	Normalized SAR 1 g (1 W)	Normalized SAR 10 g (1 W)	1g Deviation (%)	10g Deviation (%)	Date	Liquid Temp. (°C)
D835V2 SN:490	1782	835 Body	9.49	6.20	9.99	6.67	5.27	7.58	2015-03-11	22.0
D1900V2 SN:5d033	1782	1900 Body	40.6	21.3	39.4	21.4	-2.96	0.47	2015-03-10	21.9

Table1. Results system verification

13. Tissue Simulant Fluid for the Frequency Band

The dielectric properties for this simulant fluid were measured by using the Speag Model DAK-3.5 Dielectric Probe in conjunction with Agilent E5071C Network Analyzer(300 kHz - 6 GHz) by using a procedure detailed in Section V.

f (MHz)	Tissue type	Limits / Measured	Dielectric Parameters		
			Permittivity	Conductivity	Simulated Tissue Temp()
835	Body	Measured, 2015-03-11	55.71	0.95	22.0
		<i>Target Tissue Head</i>	55.2	0.97	
		Deviation (%)	0.92	-2.06	
1900	Body	Measured, 2015-03-10	51.24	1.53	21.9
		<i>Target Tissue Head</i>	53.30	1.52	
		Deviation (%)	-3.86	0.66	

The composition of the brain & muscle tissue simulating liquid

The following tissue formulations are provided for reference only as some of the parameters have not been thoroughly verified. The composition of ingredients may be modified accordingly to achieve the desired target tissue parameters required for routine SAR evaluation.

Ingredients (% by weight)	Frequency (MHz)									
	450		835		915		1900		2450	
Tissue Type	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body
Water	38.56	51.16	41.45	52.4	41.05	56.0	54.9	40.4	62.7	73.2
Salt (NaCl)	3.95	1.49	1.45	1.4	1.35	0.76	0.18	0.5	0.5	0.04
Sugar	56.32	46.78	56.0	45.0	56.5	41.76	0.0	58.0	0.0	0.0
HEC	0.98	0.52	1.0	1.0	1.0	1.21	0.0	1.0	0.0	0.0
Bactericide	0.19	0.05	0.1	0.1	0.1	0.27	0.0	0.1	0.0	0.0
Triton X-100	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	36.8	0.0
DGBE	0.0	0.0	0.0	0.0	0.0	0.0	44.92	0.0	0.0	26.7
Dielectric Constant	43.42	58.0	42.54	56.1	42.0	56.8	39.9	54.0	39.8	52.5
Conductivity (S/m)	0.85	0.83	0.91	0.95	1.0	1.07	1.42	1.45	1.88	1.78

Salt: 99 % Pure Sodium Chloride

Sugar: 98 % Pure Sucrose

Water: De-ionized, 16 MΩ⁺ resistivity

HEC: Hydroxyethyl Cellulose

DGBE: 99 % Di(ethylene glycol) butyl ether, [2-(2-butoxyethoxy)ethanol]

Triton X-100 (ultra pure): Polyethylene glycol mono [4-(1,1, 3, 3-tetramethylbutyl)phenyl]ether

Simulating Liquids for 5 GHz, Manufactured by SPEAG

Ingredients	(% by weight)
Water	78
Mineral Oil	11
Emulsifiers	9
Additives and Salt	2

14. Test System Validation

Per FCC KDB 865664 D01v01r03, SAR system validation status should be documented to confirm measurement accuracy. The SAR systems (including SAR probes, system components and software versions) used for this device were validated against its performance specifications prior to the SAR measurements. Reference dipoles were used with the require tissue-equivalent media for system validation, according to the procedures outlined in IEEE 1528-2003 and FCC KDB 865664 D01v01r03. Since frequency within the valid frequency range of the probe calibration point, using the system that normally operates with the probe for routine SAR measurements and according to the required tissue-equivalent media.

A tabulated summary of the system validation status including the validation date(s), measurement frequencies, SAR probe and tissue dielectric parameters has been included.

f (MHz)	Date	Probe S/N	Probe Cal point	Tissue Type	Dielectric Parameters		CW Validation			Modulated Validation		
					Permit tivity	Condu ctivity	Sensitivity	Probe Linearity	Probe Isotropy	Mod. Type	Duty Factor	PAR
835	2015-03-06	1782	835	Body	54.67	0.96	PASS	PASS	PASS	GMSK	PASS	N/A
1900	2015-03-07	1782	1900	Body	52.36	1.48	PASS	PASS	PASS	GMSK	PASS	N/A

< SAR System Validation Summary >

Note

All measurement were performed using probes calibrated for CW signal only. Modulations in the table above represent test configurations for which the measurement system has been validated per FCC KDB Publication 865664 D01v01r03. SAR system were validated for modulated signals with a periodic duty cycle, such as GMSK, or with a high peak to average ratio (>5 dB), such as OFDM according to KDB 865664 D01v01r03.

15. Instruments List

Test Platform	SPEAG DASY5 Professional				
Location	SGS Korea Co., Ltd. 4, LS-ro 182beon-gil, Gunpo-si, Gyeonggi-do, E&E Lab				
Manufacture	SPEAG				
Description	SAR Test System (Frequency range 300 MHz - 6 GHz)				
Software Reference	DASY5: V5.8 (1222) SEMCAD: V14.6.10 (7164)				
Hardware Reference					
Equipment	Type	Serial Number	Cal Date	Cal Interval	Cal Due
Robot	TX90XL	F13/5S7KC1/A/01	N/A	N/A	N/A
Phantom	SAM Phantom	TP-1821	N/A	N/A	N/A
Phantom	SAM Phantom	TP-1843	N/A	N/A	N/A
835 MHz System Validation Dipole	D835V2	490	2014-05-16	Biennial	2016-05-16
1900 MHz System Validation Dipole	D1900V2	5d033	2014-05-19	Biennial	2016-05-19
Dosimetric E-Field Probe	ET3DV6	1782	2015-02-24	Annual	2016-02-24
Data acquisition Electronics	DAE4	911	2015-02-20	Annual	2016-02-20
Network Analyzer	E5071C	MY46111535	2014-07-04	Annual	2015-07-04
Dielectric Assessment Kit	DAK-3.5	1107	2015-01-27	Annual	2016-01-27
Power Meter	E4419B	GB43311715	2014-06-25	Annual	2015-06-25
Power Sensor	E9300H	MY41495314	2014-07-02	Annual	2015-07-02
		MY41495307	2014-07-02	Annual	2015-07-02
Signal Generator	E8247C	MY43321024	2014-06-25	Annual	2015-06-25
Power Amplifier	2001-BBS3Q7ECK	1032 D/C 0336	2014-12-24	Annual	2015-12-24
Directional RF Bridges	86205A	MY31402302	2014-07-03	Annual	2015-07-03
LP Filter	LA-15N	N/A	2014-07-01	Annual	2015-07-01
LP Filter	LA-30N	N/A	2014-07-01	Annual	2015-07-01
Attenuator	8491B	50566	2014-07-01	Annual	2015-07-01
Hygro- Thermometer	98585	130188	2014-06-30	Annual	2015-06-30
Digital Thermometer	DTM3000	3027	2014-07-02	Annual	2015-07-02
Communication Tester	CMU200	109456	2014-06-30	Annual	2015-06-30

16. FCC Power Measurement Procedures

Power measurements were performed using a base station simulator under digital average power.

The handset was placed into a simulated call using a base station simulator in shielded chamber. SAR measurements were taken with a fully charged battery. In order to verify that the device was tested and maintained at full power, this was configured with the base station simulator. The SAR measurement Software calculates a reference point at the start and end of the test to check for power drifts. If conducted power deviations of more than 5 % occurred, the tests were repeated.

17. Measured and Reported SAR

Per FCC KDB Publication 447498 D01v05r02, When SAR is not measured at the maximum power level allowed for production units, the results must be scaled to the maximum tune-up tolerance limit according to the power applied to the individual channels tested to determine compliance. For simultaneous transmission, the measured aggregate SAR must be scaled according to the sum of the differences between the maximum tune-up tolerance and actual power used to test each transmitter. When SAR is measured at or scaled to the maximum tune-up tolerance limit, the results are referred to as reported SAR. Test highest reported SAR results are identified on the grant of equipment authorization according to procedures in KDB 690783 D01v01r03.

18. Nominal and Maximum Output Power Specifications

This device operates using the following maximum and nominal output power specifications. SAR values were scaled to the maximum allowed power to determine compliance per KDB Publication 447498 D01v05r02.

Mode / Band		Modulated Average (dBm)				
		3GPP WCDMA	3GPP HSDPA			
		Rel. 99	Rel. 5			
		RMC/AMR	Subtest 1	Subtest 2	Subtest 3	Subtest 4
WCDMA850	Maximum	24.0	24.0	24.0	23.5	23.5
	Nominal	23.5	23.5	23.5	23.0	23.0
WCDMA1900	Maximum	22.5	22.5	22.5	22.0	22.0
	Nominal	22.0	22.0	22.0	21.5	21.5
Tune-up Tolerance: -1.5 dB / + 0.5 dB						

19. RF Conducted Power Measurement

19.1 WCDMA

19.1.1 Output Power Verification

Maximum output power is measured on the High, Middle and Low channels for each applicable transmission band according to the general descriptions in section 5.2 of 3GPP TS 34.121, using the appropriate RMC or AMR with TPC (transmit power control) set to all “1s”.

19.1.2 Body SAR Measurements

SAR for body exposure configurations is measured using the 12.2 kbps RMC with the TPC bits all “1s”.

19.1.3 Procedures Used to Establish RF Signal for SAR HSDPA Data Devices

Body SAR is not required for handsets with HSDPA capabilities when the maximum average output of each RF channel with HSDPA active is less than ¼ dB higher than that measured without HSDPA using 12.2 kbps RMC and the maximum SAR for 12.2 kbps RMC is ≤ 75 % of the SAR limit. Otherwise, SAR is Measured for HSDPA, using an FRC with H-Set 1 in Sub-test 1 and a 12.2 kbps RMC configured in Test Loop Mode 1, using the highest body SAR configuration in 12.2 kbps RMC without HSDPA, on the maximum output channel with the body exposure configuration that results in the highest SAR in 12.2 kbps RMC for that RF channel.

Table 1

Sub-test	β_c	β_d	β_d (SF)	β_c/β_d	$\beta_{hs}^{(2)}$	CM (dB) ⁽²⁾
1	2/15	15/15	64	2/15	4/15	0.0
2	12/15 ⁽³⁾	15/15 ⁽³⁾	64	12/15 ⁽³⁾	24/15	1.0
3	15/15	8/15	64	15/8	30/15	1.5
4	15/15	4/15	64	15/4	30/15	1.5

Note 1: $\Delta_{ACK}, \Delta_{NACK}$ and $\Delta_{CQI} = 8 \Leftrightarrow A_{hs} = \beta_{hs}/\beta_c = 30/15 \Leftrightarrow \beta_{hs} = 30/15 \cdot \beta_c$
 Note 2: CM = 1 for $\beta_c/\beta_d = 12/15, \beta_{hs}/\beta_c = 24/15$.
 Note 3: For subtest 2 the β_c/β_d ratio of 12/15 for the TFC during the measurement period (TF1, TF0) is achieved by setting the signaled gain factors for the reference TFC (TF1, TF1) to $\beta_c = 11/15$ and $\beta_d = 15/15$.

3GPP Release Version	Mode	3GPP 34.121 Subtest	Cellular Band (dBm)			3GPP MPR(dB)
	Channel		4132	4183	4233	
99	WCDMA	12.2 kbps RMC	23.16	23.19	22.87	-
5	HSDPA	Subtest 1	23.13	23.13	22.86	0
5		Subtest 2	23.09	23.06	22.87	0
5		Subtest 3	23.12	23.11	22.70	-0.5
5		Subtest 4	23.08	23.04	22.70	-0.5
3GPP Release Version	Mode	3GPP 34.121 Subtest	PCS Band (dBm)			3GPP MPR(dB)
	Channel		9262	9400	9538	
99	WCDMA	12.2 kbps RMC	21.78	21.81	21.42	-
5	HSDPA	Subtest 1	21.34	21.86	21.39	0
5		Subtest 2	21.30	21.80	21.42	0
5		Subtest 3	21.19	21.71	21.35	-0.5
5		Subtest 4	21.20	21.78	21.33	-0.5

Note : WCDMA SAR was tested under RMC 12.2 kbps with HSPA inactive per KDB Publication 941225 D01v03. HSPA SAR was not required since the average output power of the HSPA subtests was not more than 0.25 dB higher than the RMC level and SAR was less than 1.2 W/kg

20. SAR Data Summary

20.1 WCDMA V Body SAR

EUT Position	Mode	Battery	Traffic Channel		Separation Distance (mm)	Power(dBm)		1-g SAR (W/kg)		Plot No
			Frequency (MHz)	Channel		Measured Power	Tune-Up Limit	Measured SAR	Scaled SAR	
Front	RMC	Standard	836.6	4183	5	23.19	24.00	0.342	0.412	-
Rear		Standard	836.6	4183	5	23.19	24.00	0.660	0.795	3
Left Edge		Standard	836.6	4183	5	23.19	24.00	0.504	0.607	-
Right Edge		Standard	836.6	4183	5	23.19	24.00	0.357	0.430	-
Top		Standard	836.6	4183	5	23.19	24.00	0.047	0.057	-
ANSI / IEEE C95.1 1992 – Safety Limit Spatial Peak Uncontrolled Exposure / General Population					Body 1.6 W/kg (mW/g) Averaged over 1 gram					

20.2 WCDMA II Body SAR

EUT Position	Mode	Battery	Traffic Channel		Separation Distance (mm)	Power(dBm)		1-g SAR (W/kg)		Plot No
			Frequency (MHz)	Channel		Measured Power	Tune-Up Limit	Measured SAR	Scaled SAR	
Front	RMC	Standard	1880.0	9400	5	21.81	22.50	0.374	0.438	-
Rear		Standard	1880.0	9400	5	21.81	22.50	0.698	0.818	-
Rear		Standard	1852.4	9262	5	21.78	22.50	1.000	1.180	4
Rear		Standard	1907.6	9538	5	21.42	22.50	0.657	0.842	-
Left Edge		Standard	1880.0	9400	5	21.81	22.50	0.418	0.490	-
Right Edge		Standard	1880.0	9400	5	21.81	22.50	0.214	0.251	-
Top		Standard	1880.0	9400	5	21.81	22.50	0.492	0.577	-
ANSI / IEEE C95.1 1992 – Safety Limit Spatial Peak Uncontrolled Exposure / General Population					Body 1.6 W/kg (mW/g) Averaged over 1 gram					

General Notes

1. The test data reported are the worst-case SAR values according to test procedures specified in IEEE 1528-2003, FCC KDB Publication 865664 D01v02r03 and FCC KDB Publication 447498 D01v05r02.
2. All modes of operation were investigated, and worst-case results are reported.
3. The EUT is tested 2nd hot-spot peak, if it is less than 2 dB below the highest peak.
4. The manufacturer has confirmed that the device(s) tested have the same physical, mechanical and thermal characteristics and are within operational tolerances expected for production units.
5. SAR results were scaled to the maximum allowed power to demonstrate compliance per FCC KDB Publication 447498 D01v05r02.
6. Device was tested using a fixed spacing for body-worn accessory testing. A separation distance of 10 mm was considered because the manufacturer has determined that there will be body-worn accessories available in the marketplace for users to support this separation distance.
7. Per FCC KDB Publication 648474 D04v01r02, body worn SAR was evaluated without a headset connected to the device. Since the standalone reported SAR was ≤ 1.2 W/kg, no additional body worn SAR evaluations using a headset cable were required.
8. Per FCC KDB Publication 865664 D01v01r03, variability SAR tests were performed when the measured SAR results for a frequency band were greater than 0.8 W/kg. Please see section 24 for variability analysis.

WCDMA Notes

1. WCDMA mode in Body SAR was tested under RMC 12.2 kbps with HSPA inactive per KDB Publication 941225 D01v03. HSPA SAR was not required since the average output power of the HSPA subtests was not more than 0.25 dB higher than the RMC level and SAR was less than 1.2 W/kg.
2. Per FCC KDB Publication 447498 D01v05r02, if the reported (scaled) SAR measured at the middle channel or highest output power channel for each test configuration is ≤ 0.8 W/kg then testing at the other channels is not required for such test configuration(s). When the maximum output power variation across the required test channels is $> \frac{1}{2}$ dB, instead of the middle channel, the highest output power channel must be used

21. SAR Measurement Variability

21.1 Measurement Variability

Per FCC KDB Publication 865664 D01v01r03, SAR measurement variability was assessed for each frequency band, which was determined by the SAR probe calibration point and tissue-equivalent medium used for the device measurements. When both head and body tissue-equivalent media were required for SAR measurements in a frequency band, the variability measurement procedures were applied to the tissue medium with the highest measured SAR, using the highest measured SAR configuration for that tissue-equivalent medium. These additional measurements were repeated after the completion of all measurements requiring the same head or body tissue-equivalent medium in a frequency band. The test device was returned to ambient conditions (normal room temperature) with the battery fully charged before it was re-mounted on the device holder for the repeated measurement(s) to minimize any unexpected variations in the repeated results.

SAR Measurement Variability was assessed using the following procedures for each frequency band:

- 1. When the original highest measured SAR is ≥ 0.80 W/kg, the measurement was repeated once.**
2. A second repeated measurement was performed only if the ratio of largest to smallest SAR for the original and first repeated measurements was > 1.20 or when the original or repeated measurement was ≥ 1.45 W/kg (~ 10% from the 1-g SAR limit).
3. A third repeated measurement was performed only if the original, first or second repeated measurement was ≥ 1.5 W/kg and the ratio of largest to smallest SAR for the original, first and second repeated measurements is > 1.20 .
4. Repeated measurements are not required when the original highest measured SAR is < 0.80 W/kg

Repeated SAR Measurement

Band	EUT Position	Mode	Battery	Traffic Channel		Distance (mm)	Measured 1 g SAR (W/kg)	1 st Repeated 1 g SAR (W/kg)	Deviation (%)
				Frequency (MHz)	Channel				
WCDMA II	Rear	RMC	Standard	1852.4	9262	5	1.00	1.01	1.00

21.2 Measurement Uncertainty

The measured SAR was < 1.5 W/kg for all frequency bands. Therefore, per KDB Publication 865664 D01v01r03, the extended measurement uncertainty analysis per IEEE 1528-2003 was not required.

Appendixes List

Appendix A	A.1 Verification Test Plots for 835 MHz A.2 Verification Test Plots for 1900 MHz A.3 SAR Test Plots for WCDMA V Band Body A.4 SAR Test Plots for WCDMA II Band Body
Appendix B	B.1 Uncertainty Analysis
Appendix C	C.1 Calibration certificate for Probe (SN: 1782) C.2 Calibration certificate for DAE C.3 Calibration certificate for Dipole

Appendix A.1 Verification Test Plots for 835 MHz_Body

Date: 2015-03-11

Test Laboratory : SGS Korea (Gunpo Laboratory)
 File Name: [835MHz Body Verification.da53:0](#)

Input Power : 100 mW

Ambient Temp : 23.2 °C Tissue Temp : 22.0 °C

DUT: Dipole 835 MHz D835V2; Type: D835V2; Serial: D835V2 - SN:490

Communication System: UID 0, CW (0); Frequency: 835 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 835$ MHz; $\sigma = 0.947$ S/m; $\epsilon_r = 55.714$; $\rho = 1000$ kg/m³
 Phantom section: Flat Section

DASY52 Configuration:


- Probe: ET3DV6 - SN1782; ConvF(5.97, 5.97, 5.97); Calibrated: 2015-02-24;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sr911; Calibrated: 2015-02-20
- Phantom: SAM (20deg probe tilt) with CRP v5.0_12_03; Type: QD000P40CD; Serial: TP:1821
- DASY52 52.8.8(1222)SEMCAD X 14.6.10(7331)

Verification/835MHz Body Verification/Area Scan (61x81x1): Interpolated grid:

$dx=1.500$ mm, $dy=1.500$ mm
 Maximum value of SAR (interpolated) = 1.08 W/kg

Verification/835MHz Body Verification/Zoom Scan (5x5x7)/Cube 0: Measurement grid:

$dx=8$ mm, $dy=8$ mm, $dz=5$ mm
 Reference Value = 34.61 V/m; Power Drift = -0.04 dB
 Peak SAR (extrapolated) = 1.41 W/kg
SAR(1 g) = 0.999 W/kg; SAR(10 g) = 0.667 W/kg
 Maximum value of SAR (measured) = 1.08 W/kg

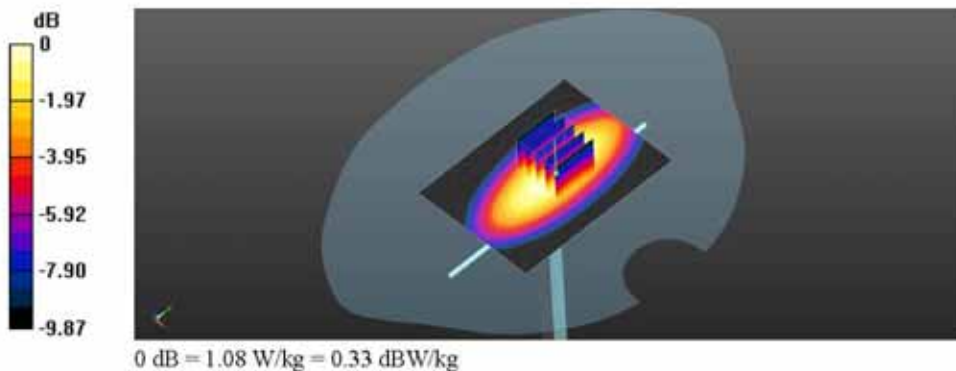

Appendix A.2 Verification Test Plots for 1900 MHz_Body

Date: 2015-03-10

Test Laboratory : SGS Korea (Gunpo Laboratory)
 File Name: [1900MHz Body Verification da53:0](#)

Input Power : 100 mW

Ambient Temp : 23.0 °C Tissue Temp : 21.9 °C

DUT: Dipole 1900 MHz D1900V2; Type: D1900V2; Serial: D1900V2 - SN:5d033


Communication System: UID 0, CW (0); Frequency: 1900 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 1900$ MHz; $\sigma = 1.526$ S/m; $\epsilon_r = 51.241$; $\rho = 1000$ kg/m³
 Phantom section: Flat Section

DASY52 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(4.67, 4.67, 4.67); Calibrated: 2015-02-24;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sr911; Calibrated: 2015-02-20
- Phantom: SAM (20deg probe tilt) with CRP v5.0_2014_12_03_Left; Type: QD000P40CD; Serial: TP1843
- DASY52 52.8.8(1222)SEMCAD X 14.6.10(7331)

Verification/1900MHz Body Verification/Area Scan (61x61x1): Interpolated grid:
 dx=1.500 mm, dy=1.500 mm
 Maximum value of SAR (interpolated) = 4.65 W/kg

Verification/1900MHz Body Verification/Zoom Scan (5x5x7)/Cube 0: Measurement
 grid: dx=8mm, dy=8mm, dz=5mm
 Reference Value = 58.16 V/m; Power Drift = -0.03 dB
 Peak SAR (extrapolated) = 6.32 W/kg
SAR(1 g) = 3.94 W/kg; SAR(10 g) = 2.14 W/kg
 Maximum value of SAR (measured) = 4.37 W/kg

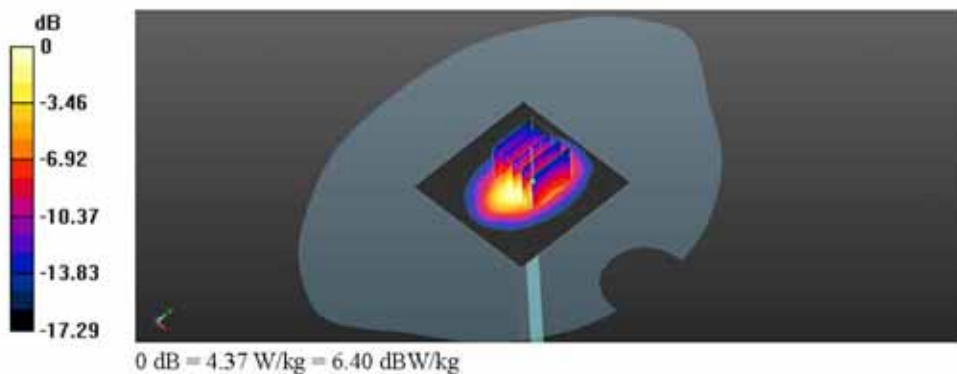

Appendix A.3 SAR Test Plots for WCDMA V (Body SAR)

Date: 2015-03-11

Test Laboratory : SGS Korea (Gunpo Laboratory)
 File Name: [WCDMA FDD V Rear_CH4183.da53:0](#)

Ambient Temp : 23.2 °C Tissue Temp : 22.0 °C

DUT: GM01CAB; Type: Blood Glucos Meter; Serial: B2C800C00011

Communication System: UID 0, WCDMA5 (0); Frequency: 836.6 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 837$ MHz; $\sigma = 0.95$ S/m; $\epsilon_r = 55.69$; $\rho = 1000$ kg/m³
 Phantom section: Flat Section


DASY52 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(5.97, 5.97, 5.97); Calibrated: 2015-02-24;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn911; Calibrated: 2015-02-20
- Phantom: SAM (20deg probe tilt) with CRP v5.0_12_03; Type: QD000P40CD; Serial: TP:1821
- DASY52 52.8.8(1222)SEMCAD X 14.6.10(7331)

Body/WCDMA FDD V_Rear_CH4183/Area Scan (71x91x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm
 Maximum value of SAR (interpolated) = 0.770 W/kg

Body/WCDMA FDD V_Rear_CH4183/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm
 Reference Value = 24.56 V/m; Power Drift = 0.01 dB
 Peak SAR (extrapolated) = 1.11 W/kg
SAR(1 g) = 0.660 W/kg; SAR(10 g) = 0.410 W/kg
 Maximum value of SAR (measured) = 0.714 W/kg

Body/WCDMA FDD V_Rear_CH4183/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm
 Reference Value = 24.56 V/m; Power Drift = 0.01 dB
 Peak SAR (extrapolated) = 0.778 W/kg
SAR(1 g) = 0.575 W/kg; SAR(10 g) = 0.404 W/kg
 Maximum value of SAR (measured) = 0.612 W/kg

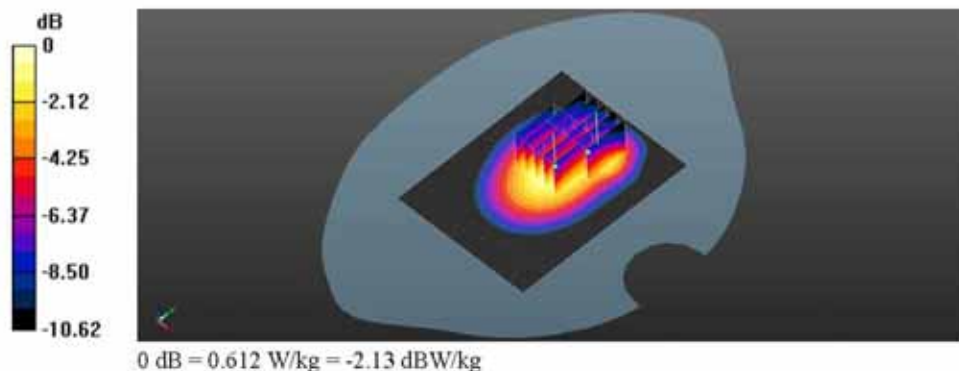

Appendix A.4 SAR Test Plots for WCDMA II (Body SAR)

Date: 2015-03-10

Test Laboratory : SGS Korea (Gunpo Laboratory)
 File Name: [WCDMA FDD II Rear_CH9262 Repeat Test.da53:0](#)

Ambient Temp : 23.0 °C Tissue Temp : 21.9 °C

DUT: GM01CAB; Type: Blood Glucos Meter; Serial: B2C800C00011

Communication System: UID 0, WCDMA2 (0); Frequency: 1852.4 MHz; Duty Cycle: 1:1
 Medium parameters used (interpolated): $f = 1852.4$ MHz; $\sigma = 1.475$ S/m; $\epsilon_r = 51.414$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY52 Configuration:
 - Probe: ET3DV6 - SN1782; ConvF(4.67, 4.67, 4.67); Calibrated: 2015-02-24;
 - Sensor-Surface: 4mm (Mechanical Surface Detection)
 - Electronics: DAE4 Sr911; Calibrated: 2015-02-20
 - Phantom: SAM (20deg probe tilt) with CRP v5.0_2014_12_03_Left, Type: QD000P40CD; Serial: TP1843
 - DASY52 52.8.8(1222)SEMCAD X 14.6.10(7331)

Body/WCDMA FDD II Rear_CH9262 Repeat Test/Area Scan (71x111x1):


Interpolated grid: dx=1.500 mm, dy=1.500 mm

Info: Interpolated medium parameters used for SAR evaluation.
 Maximum value of SAR (interpolated) = 1.21 W/kg

Body/WCDMA FDD II Rear_CH9262 Repeat Test/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: dx=8mm, dy=8mm, dz=5mm
 Reference Value = 15.53 V/m; Power Drift = -0.07 dB
 Peak SAR (extrapolated) = 1.63 W/kg
SAR(1 g) = 1.01 W/kg; SAR(10 g) = 0.573 W/kg

Info: Interpolated medium parameters used for SAR evaluation.
 Maximum value of SAR (measured) = 1.13 W/kg

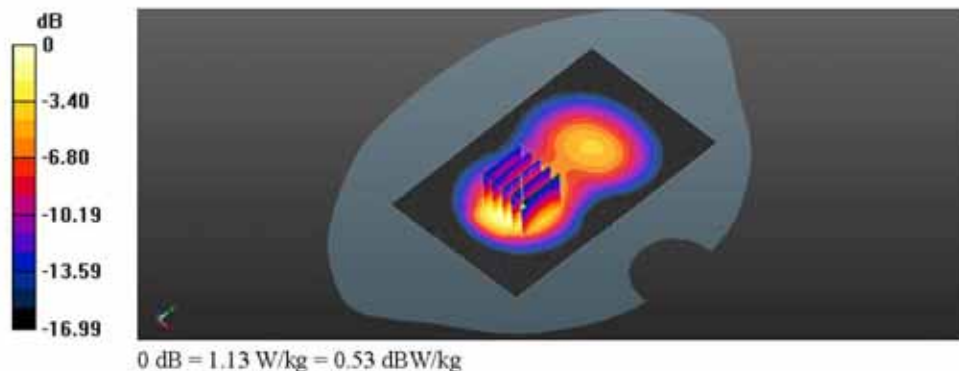

Appendix B.1 Uncertainty Analysis DASY5 #3

Measurement uncertainty for 300 MHz to 3 GHz averaged over 1 gram

a	b	c	d	e = f(d,k)	g	i =	k
						cxg/e	
Uncertainty Component	Section in	Tol	Prob .	Div.	Ci	lg	Vi
	IEEE 1528	(%)	Dist.		(1g)	ui (%)	(Veff)
Probe calibration	E.2.1	6.0	N	1	1	6.00	∞
Axial isotropy	E.2.2	4.7	R	1.73	0.71	1.92	∞
Hemispherical isotropy	E.2.2	9.6	R	1.73	0.71	3.92	∞
Boundary effect	E.2.3	1.0	R	1.73	1	0.58	∞
Linearity	E.2.4	4.7	R	1.73	1	2.71	∞
System detection limit	E.2.5	0.3	R	1.73	1	0.14	∞
Readout electronics	E.2.6	0.3	N	1	1	0.30	∞
Response time	E.2.7	0.5	R	1.73	1	0.29	∞
Integration time	E.2.8	2.6	R	1.73	1	1.50	∞
RF ambient Condition - Noise	E.6.1	3.0	R	1.73	1	1.73	∞
RF ambient Condition - reflections	E.6.1	3.0	R	1.73	1	1.73	∞
Probe Positiones	E.6.2	1.5	R	1.73	1	0.87	∞
Probe Positioning	E.6.3	2.9	R	1.73	1	1.67	∞
Max. SAR evaluation	E.5.2	1.0	R	1.73	1	0.58	∞
Test sample positioning	E.4.2	1.9	N	1	1	1.92	9
Device holder uncertainty	E.4.1	3.6	N	1	1	3.60	4
Output power variation -SAR drift measurement	6.6.3	5.0	R	1.73	1	2.89	∞
Phantom uncertainty	E.3.1	4.0	R	1.73	1	2.31	∞
Liquid conductivity - deviation from target values	E.3.2	5.0	R	1.73	0.64	1.85	∞
Liquid conductivity - measurement uncertainty	E.3.2	1.6	N	1	0.64	1.00	5
Liquid permittivity - deviation from target values	E.3.3	5.0	R	1.73	0.6	1.73	∞
Liquid permittivity - measurement uncertainty	E.3.3	1.2	N	1	0.6	0.75	4
Combined standard uncertainty				RSS		10.65	295
Expanded uncertainty (95% CONFIDENCE INTERVAL)				K=2		21.30	

Appendix C.1 Calibration certificate for Probe (SN: 1782)

**Calibration Laboratory of
 Schmid & Partner
 Engineering AG**
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
 Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **SGS (Dymstec)**

Certificate No: **ET3-1782_Feb15**

CALIBRATION CERTIFICATE

Object **ET3DV6 - SN:1782**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-23.v5, QA CAL-25.v6
 Calibration procedure for dosimetric E-field probes**

Calibration date: **February 24, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&E critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	03-Apr-14 (No. 217-01911)	Apr-15
Power sensor E4412A	MY41498067	03-Apr-14 (No. 217-01911)	Apr-15
Reference 3 dB Attenuator	SN: S5054 (3c)	03-Apr-14 (No. 217-01915)	Apr-15
Reference 20 dB Attenuator	SN: S5277 (20x)	03-Apr-14 (No. 217-01919)	Apr-15
Reference 30 dB Attenuator	SN: S5129 (30b)	03-Apr-14 (No. 217-01920)	Apr-15
Reference Probe ES3DV2	SN: 3013	30-Dec-14 (No. ES3-3013_Dec14)	Dec-15
DAE4	SN: 660	14-Jan-15 (No. DAE4-660_Jan15)	Jan-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-14)	In house check: Oct-15

Calibrated by:	Name Claudio Leubler	Function Laboratory Technician	Signature
Approved by:	Name Katja Pokovic	Function Technical Manager	Signature

Issued: February 25, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., θ = 0 is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- **NORM_{x,y,z}:** Assessed for E-field polarization θ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- **NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- **DCP_{x,y,z}:** DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- **PAR:** PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- **A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}:** A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- **ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- **Spherical isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- **Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- **Connector Angle:** The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

ET3DV6 – SN:1782

February 24, 2015

Probe ET3DV6

SN:1782

Manufactured: April 15, 2003
Calibrated: February 24, 2015

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

ET3DV6- SN:1782

February 24, 2015

DASY/EASY - Parameters of Probe: ET3DV6 - SN:1782

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	2.09	1.64	1.91	± 10.1 %
DCP (mV) ^B	96.5	99.0	97.0	

Modulation Calibration Parameters

UID	Communication System Name		A	B	C	D	VR	Unc ^E
			dB	dB $\sqrt{\mu\text{V}}$		dB	mV	(k=2)
0	CW	X	0.0	0.0	1.0	0.00	240.9	±3.8 %
		Y	0.0	0.0	1.0		249.3	
		Z	0.0	0.0	1.0		227.8	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

ET3DV6- SN:1782

February 24, 2015

DASY/EASY - Parameters of Probe: ET3DV6 - SN:1782

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
150	52.3	0.76	8.16	8.16	8.16	0.15	2.50	± 13.3 %
300	45.3	0.87	8.05	8.05	8.05	0.22	2.20	± 13.3 %
450	43.5	0.87	7.29	7.29	7.29	0.25	2.90	± 13.3 %
600	42.7	0.88	7.23	7.23	7.23	0.00	1.00	± 13.3 %
750	41.9	0.89	6.52	6.52	6.52	0.28	3.00	± 12.0 %
835	41.5	0.90	6.25	6.25	6.25	0.35	2.55	± 12.0 %
900	41.5	0.97	6.15	6.15	6.15	0.33	2.65	± 12.0 %
1640	40.3	1.29	5.63	5.63	5.63	0.80	2.09	± 12.0 %
1810	40.0	1.40	5.21	5.21	5.21	0.75	2.30	± 12.0 %
1900	40.0	1.40	5.11	5.11	5.11	0.80	2.09	± 12.0 %
2450	39.2	1.80	4.53	4.53	4.53	0.80	1.79	± 12.0 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

ET3DV6- SN:1782

February 24, 2015

DASY/EASY - Parameters of Probe: ET3DV6 - SN:1782

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
300	58.2	0.92	7.46	7.46	7.46	0.19	2.20	± 13.3 %
450	56.7	0.94	7.32	7.32	7.32	0.20	2.10	± 13.3 %
750	55.5	0.96	6.02	6.02	6.02	0.35	2.61	± 12.0 %
835	55.2	0.97	5.97	5.97	5.97	0.31	2.94	± 12.0 %
1900	53.3	1.52	4.67	4.67	4.67	0.80	2.48	± 12.0 %
2450	52.7	1.95	4.12	4.12	4.12	0.80	1.32	± 12.0 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

ET3DV6- SN:1782

February 24, 2015

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)


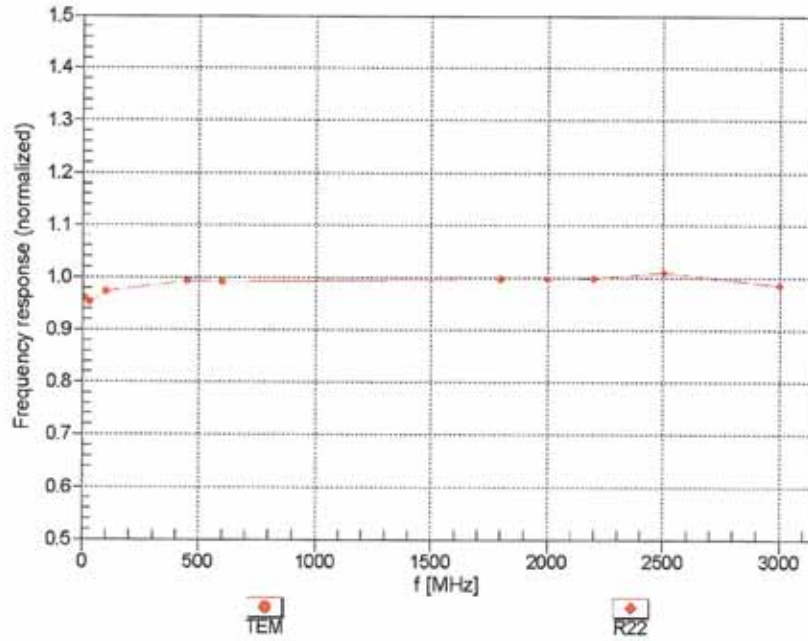


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

ET3DV6- SN:1782

February 24, 2015

Receiving Pattern (ϕ), $\theta = 0^\circ$

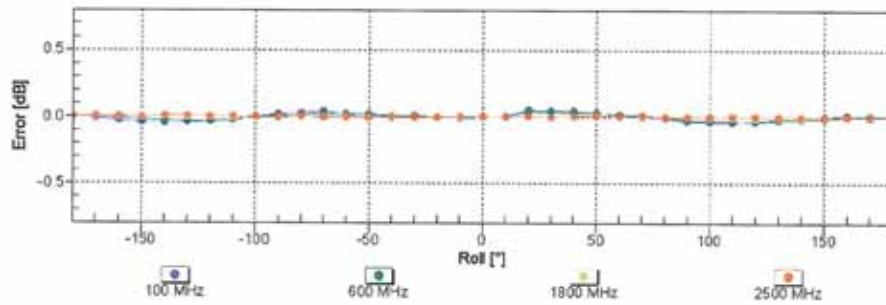
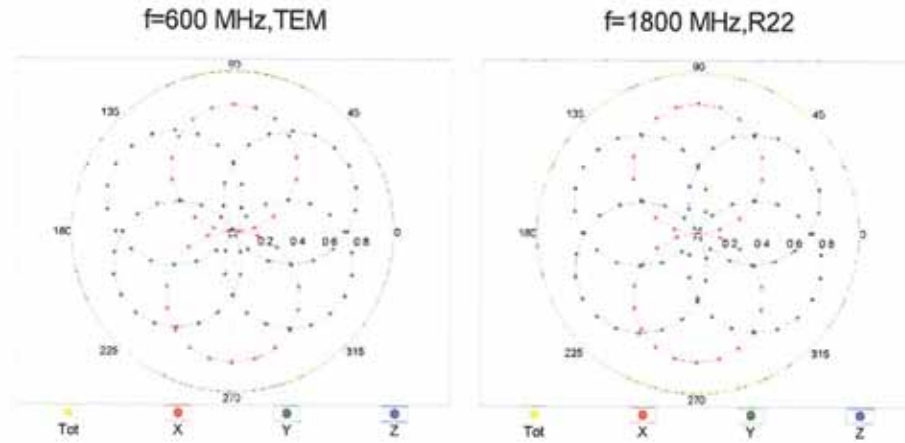


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

ET3DV6- SN:1782

February 24, 2015

Dynamic Range f(SAR_{head})
 (TEM cell , f_{eval}= 1900 MHz)

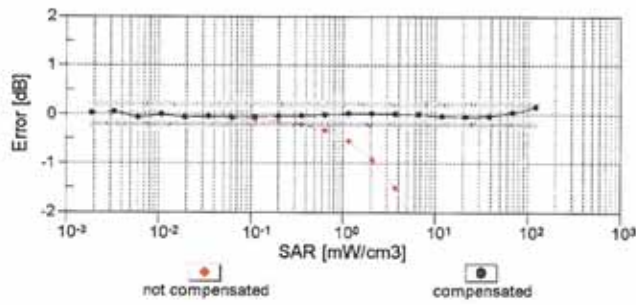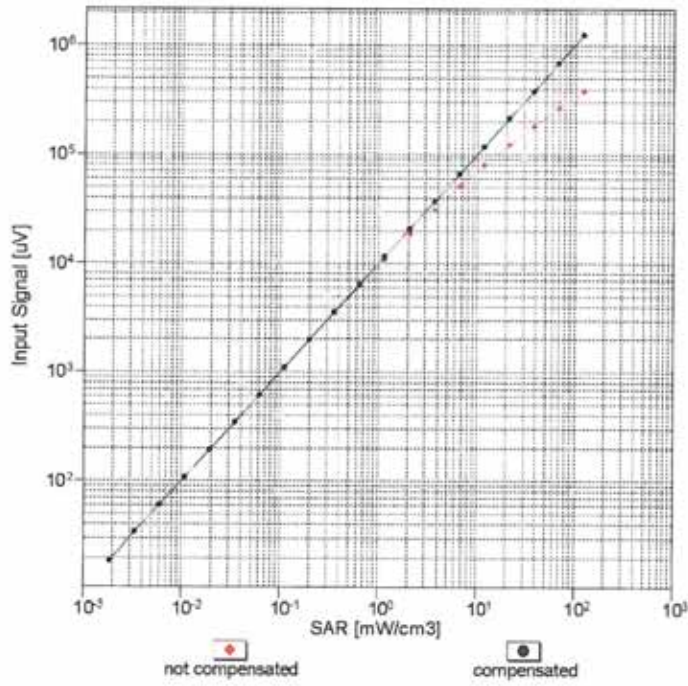


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

ET3DV6- SN:1782


February 24, 2015

Conversion Factor Assessment

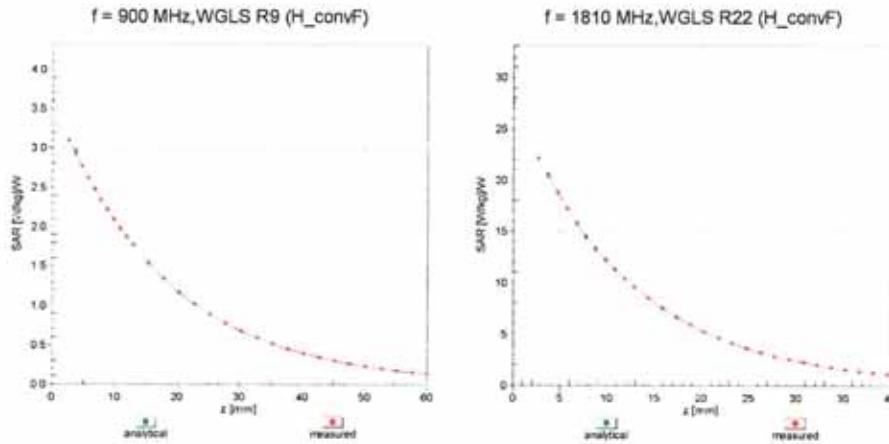

Deviation from Isotropy in Liquid

Error (ϕ, θ), $f = 900$ MHz

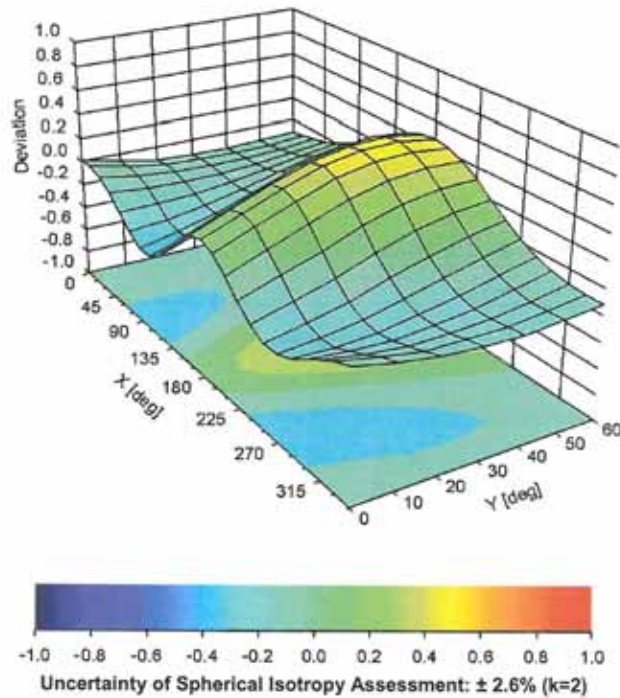

ET3DV6- SN:1782

February 24, 2015

DASY/EASY - Parameters of Probe: ET3DV6 - SN:1782

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-129.9
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	6.8 mm
Probe Tip to Sensor X Calibration Point	2.7 mm
Probe Tip to Sensor Y Calibration Point	2.7 mm
Probe Tip to Sensor Z Calibration Point	2.7 mm
Recommended Measurement Distance from Surface	4 mm

Appendix C.2 Calibration certificate for DAE

**Calibration Laboratory of
 Schmid & Partner
 Engineering AG**
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Dymstec**

Certificate No: **DAE4-911_Feb15**

CALIBRATION CERTIFICATE

Object: **DAE4 - SD 000 D04 BK - SN: 911**

Calibration procedure(s): **QA CAL-06.v29
 Calibration procedure for the data acquisition electronics (DAE)**

Calibration date: **February 20, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	03-Oct-14 (No:15573)	Oct-15
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	06-Jan-15 (in house check)	In house check: Jan-16
Calibrator Box V2.1	SE UMS 006 AA 1002	06-Jan-15 (in house check)	In house check: Jan-16

	Name	Function	Signature
Calibrated by:	Dominique Steffen	Technician	
Approved by:	Fin Bornholt	Deputy Technical Manager	

Issued: February 20, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary

DAE data acquisition electronics
Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- **DC Voltage Measurement:** Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- **Connector angle:** The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - **DC Voltage Measurement Linearity:** Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - **Common mode sensitivity:** Influence of a positive or negative common mode voltage on the differential measurement.
 - **Channel separation:** Influence of a voltage on the neighbor channels not subject to an input voltage.
 - **AD Converter Values with inputs shorted:** Values on the internal AD converter corresponding to zero input voltage
 - **Input Offset Measurement:** Output voltage and statistical results over a large number of zero voltage measurements.
 - **Input Offset Current:** Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - **Input resistance:** Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - **Low Battery Alarm Voltage:** Typical value for information. Below this voltage, a battery alarm signal is generated.
 - **Power consumption:** Typical value for information. Supply currents in various operating modes.

DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 μ V , full range = -100...+300 mV
 Low Range: 1LSB = 61nV , full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	405.170 \pm 0.02% (k=2)	404.879 \pm 0.02% (k=2)	404.758 \pm 0.02% (k=2)
Low Range	4.00112 \pm 1.50% (k=2)	3.96552 \pm 1.50% (k=2)	3.96381 \pm 1.50% (k=2)

Connector Angle

Connector Angle to be used in DASY system	230.5 $^{\circ}$ \pm 1 $^{\circ}$
---	-------------------------------------

Appendix (Additional assessments outside the scope of SCS108)

1. DC Voltage Linearity

High Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	200037.32	1.46	0.00
Channel X + Input	20004.28	0.78	0.00
Channel X - Input	-20004.64	1.68	-0.01
Channel Y + Input	200033.09	-1.68	-0.00
Channel Y + Input	20002.35	-1.20	-0.01
Channel Y - Input	-20008.45	-1.96	0.01
Channel Z + Input	200034.70	0.03	0.00
Channel Z + Input	20002.39	-1.05	-0.01
Channel Z - Input	-20004.67	1.87	-0.01

Low Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	1999.99	-0.06	-0.00
Channel X + Input	200.20	0.16	0.08
Channel X - Input	-199.85	0.08	-0.04
Channel Y + Input	1999.61	-0.30	-0.02
Channel Y + Input	198.82	-1.01	-0.50
Channel Y - Input	-200.06	0.06	-0.03
Channel Z + Input	1998.51	-1.46	-0.07
Channel Z + Input	198.92	-0.93	-0.46
Channel Z - Input	-201.66	-1.46	0.73

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	-10.84	-12.46
	- 200	15.93	14.84
Channel Y	200	20.13	19.14
	- 200	-20.31	-20.82
Channel Z	200	-20.75	-20.21
	- 200	17.28	17.42

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	0.34	-5.35
Channel Y	200	6.51	-	0.09
Channel Z	200	9.54	4.62	-

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15852	16154
Channel Y	15998	16109
Channel Z	16437	14961

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec
 Input 10MΩ

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (μV)
Channel X	0.94	-1.06	3.07	0.63
Channel Y	0.10	-1.29	1.79	0.60
Channel Z	-0.37	-2.17	1.01	0.56

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Appendix C.3 Calibration certificate for Dipole


**Calibration Laboratory of
 Schmid & Partner
 Engineering AG**
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**



Client **SGS (Dymstec)**

Certificate No: **D835V2-490_May14** 2014.6.2

CALIBRATION CERTIFICATE			
Object	D835V2 - SN: 490		
Calibration procedure(s)	QA CAL-05.v9 Calibration procedure for dipole validation kits above 700 MHz		
Calibration date:	May 16, 2014		
<p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p>			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	US37292783	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	MY41092317	09-Oct-13 (No. 217-01828)	Oct-14
Reference 20 dB Attenuator	SN: 5058 (20k)	03-Apr-14 (No. 217-01918)	Apr-15
Type-N mismatch combination	SN: 5047.2 / 06327	03-Apr-14 (No. 217-01921)	Apr-15
Reference Probe ES3DV3	SN: 3205	30-Dec-13 (No. ES3-3205_Dec13)	Dec-14
DAE4	SN: 601	30-Apr-14 (No. DAE4-601_Apr14)	Apr-15
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-16
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14
Calibrated by:	Name Claudio Leubler	Function Laboratory Technician	Signature
Approved by:	Name Katja Pokovic	Function Technical Manager	
			Issued: May 20, 2014
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	0.94 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.36 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.07 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.52 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	5.90 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	56.6 ± 6 %	1.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.45 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.49 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.59 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.20 W/kg ± 16.5 % (k=2)

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.9 Ω - 2.9 j Ω
Return Loss	- 30.4 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	45.3 Ω - 5.0 j Ω
Return Loss	- 22.9 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.392 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	May 19, 2003

DASY5 Validation Report for Head TSL

Date: 16.05.2014

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 490


Communication System: UID 0 - CW; Frequency: 835 MHz
 Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.94 \text{ S/m}$; $\epsilon_r = 40.2$; $\rho = 1000 \text{ kg/m}^3$
 Phantom section: Flat Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:


- Probe: ES3DV3 - SN3205; ConvF(6.22, 6.22, 6.22); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$
 Reference Value = 56.09 V/m; Power Drift = 0.03 dB
 Peak SAR (extrapolated) = 3.57 W/kg
SAR(1 g) = 2.36 W/kg; SAR(10 g) = 1.52 W/kg
 Maximum value of SAR (measured) = 2.78 W/kg

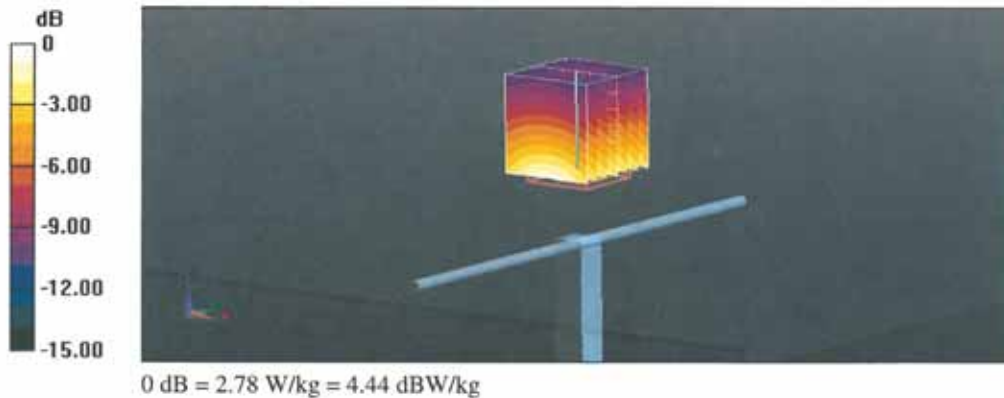

Impedance Measurement Plot for Head TSL

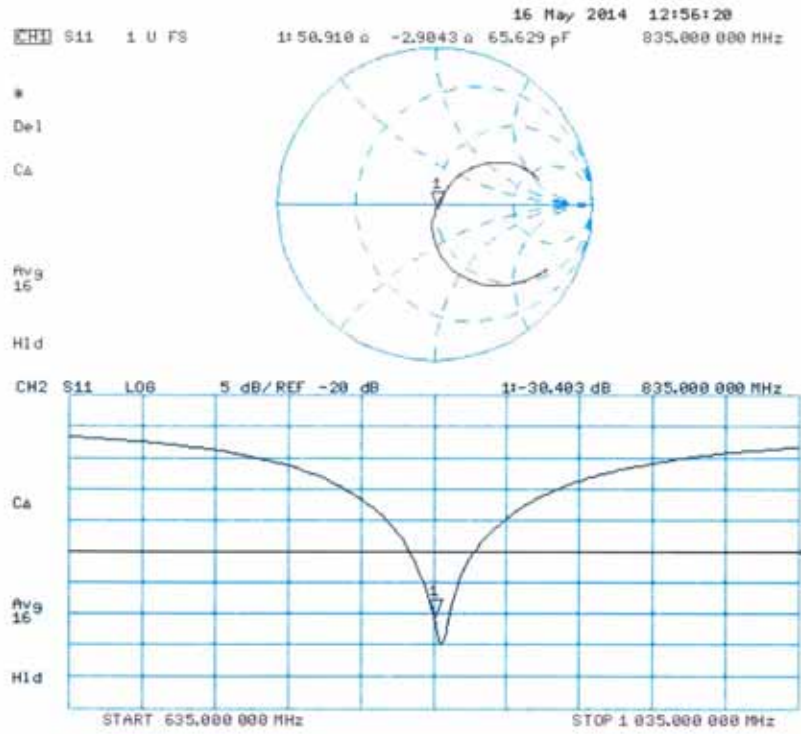

DASY5 Validation Report for Body TSL

Date: 15.05.2014

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 490


Communication System: UID 0 - CW; Frequency: 835 MHz
 Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 1.02 \text{ S/m}$; $\epsilon_r = 56.6$; $\rho = 1000 \text{ kg/m}^3$
 Phantom section: Flat Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:


- Probe: ES3DV3 - SN3205; ConvF(6.09, 6.09, 6.09); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$
 Reference Value = 55.12 V/m; Power Drift = -0.03 dB
 Peak SAR (extrapolated) = 3.64 W/kg
SAR(1 g) = 2.45 W/kg; SAR(10 g) = 1.59 W/kg
 Maximum value of SAR (measured) = 2.87 W/kg

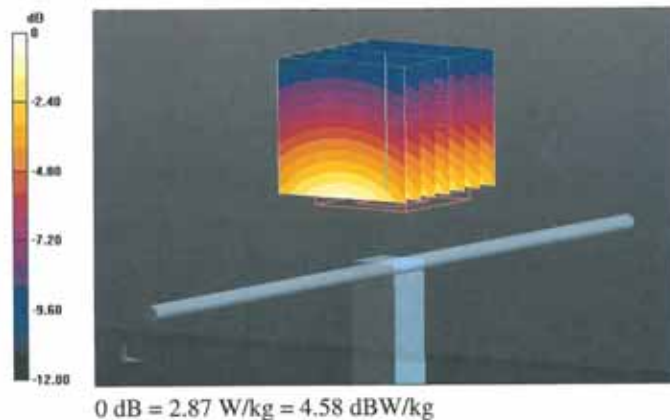

Impedance Measurement Plot for Body TSL

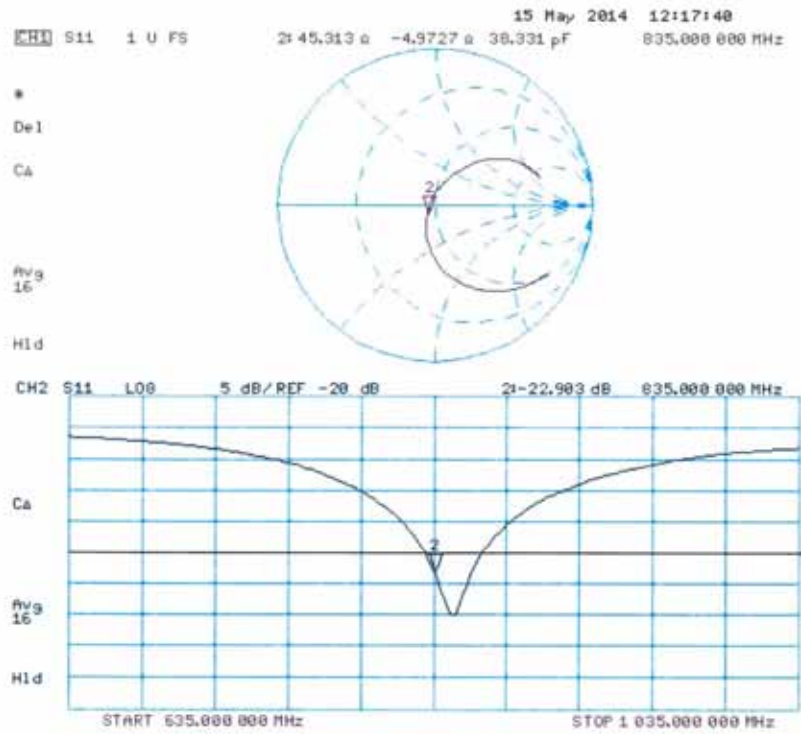

**Calibration Laboratory of
 Schmid & Partner
 Engineering AG**
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**



Client **SGS (Dymstec)**

Certificate No: **D1900V2-5d033_May14**

CALIBRATION CERTIFICATE

Object: **D1900V2 - SN: 5d033**

Calibration procedure(s): **QA CAL-05.v9
 Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **May 19, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	US37292783	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	MY41092317	09-Oct-13 (No. 217-01828)	Oct-14
Reference 20 dB Attenuator	SN: 5058 (20k)	03-Apr-14 (No. 217-01918)	Apr-15
Type-N mismatch combination	SN: 5047.2 / 06327	03-Apr-14 (No. 217-01921)	Apr-15
Reference Probe ES3DV3	SN: 3205	30-Dec-13 (No. ES3-3205_Dec13)	Dec-14
DAE4	SN: 601	30-Apr-14 (No. DAE4-601_Apr14)	Apr-15

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-16
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14

	Name	Function	Signature
Calibrated by:	Leif Klynsner	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: May 19, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of
Schmid & Partner
 Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.3 ± 6 %	1.37 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.99 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.3 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.24 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.1 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.5 ± 6 %	1.50 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.1 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	40.6 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.32 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.3 W/kg ± 16.5 % (k=2)

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.9 Ω + 1.5 j Ω
Return Loss	- 32.6 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	47.6 Ω + 1.9 j Ω
Return Loss	- 30.0 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.204 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	March 17, 2003

DASY5 Validation Report for Head TSL

Date: 19.05.2014

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d033

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 39.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(5.06, 5.06, 5.06); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 98.44 V/m; Power Drift = 0.02 dB


Peak SAR (extrapolated) = 18.3 W/kg

SAR(1 g) = 9.99 W/kg; SAR(10 g) = 5.24 W/kg

Maximum value of SAR (measured) = 12.6 W/kg

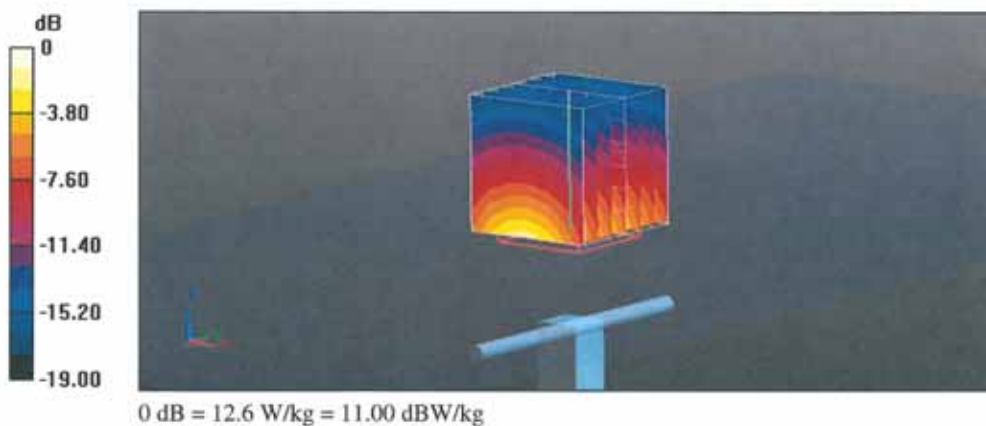

Impedance Measurement Plot for Head TSL

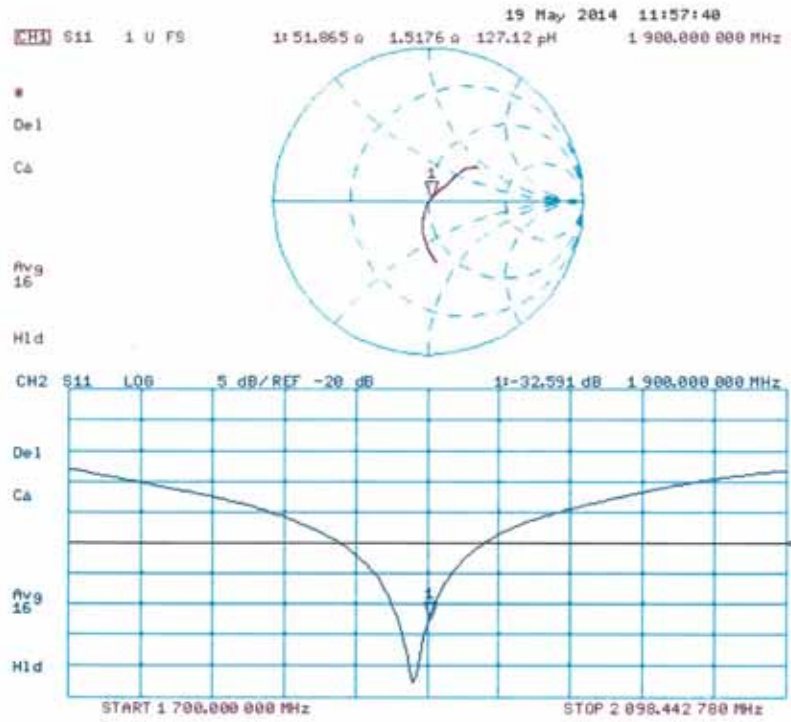

DASY5 Validation Report for Body TSL

Date: 16.05.2014

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d033


Communication System: UID 0 - CW; Frequency: 1900 MHz
 Medium parameters used: $f = 1900$ MHz; $\sigma = 1.5$ S/m; $\epsilon_r = 52.5$; $\rho = 1000$ kg/m³
 Phantom section: Flat Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:


- Probe: ES3DV3 - SN3205; ConvF(4.76, 4.76, 4.76); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 95.47 V/m; Power Drift = 0.02 dB
 Peak SAR (extrapolated) = 17.5 W/kg
SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.32 W/kg
 Maximum value of SAR (measured) = 12.6 W/kg

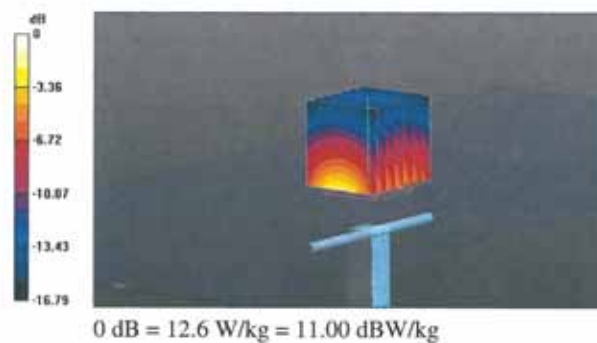

Impedance Measurement Plot for Body TSL

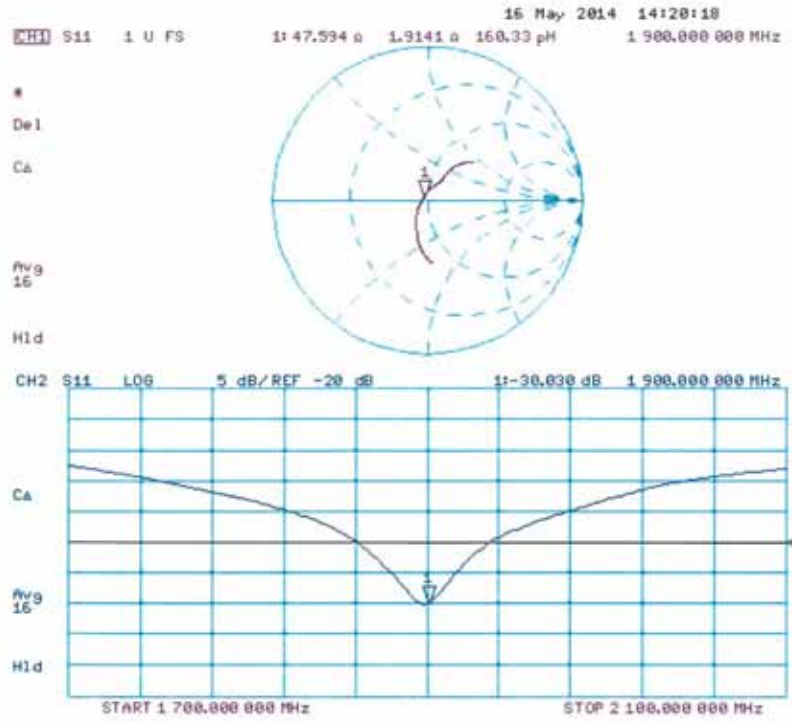

-THE END-