

**Order No.** : G-45-2015-00597  
**Applicant** : i-SENS, Inc.  
**Address** : 43, Banpo-daero 28-gil, Seocho-gu, Seoul, 137-873, Republic of Korea  
**Product** : Blood Glucose Meter  
**Model** : GM01CAB  
**Alt Model Name** : GM01CAD  
**Environment** : Temp. (21.5 ~ 22.7) °C, Humidity (28.0 ~ 32.0) %R.H.  
 Atmospheric Pressure (100.5 ~ 100.6) kPa  
**Standards** : FCC Part 15 Subpart B  
 FCC Part 18  
**Date of Receipt** : February 26, 2015  
**Date of Test** : March 30, 2015 ~ March 31, 2015  
**Date of Issue** : April 06, 2015  
**Test Result** : Compliance  
**Use of report** : Validation

The results shown in this test report refer only to the sample(s) tested unless otherwise stated.  
 This Test Report cannot be reproduced, except in full.

Affirmation	Tested by	Technical Manager
	Name : Jinho Seo (Signature)	Name : Paul Kang (Signature)

The above test report is the accredited test results by Korea Laboratory Accreditation Scheme, which signed the ILAC-MRA

**Accredited by KOLAS Republic of KOREA**  
**SGS Korea Co., Ltd. Gunpo Laboratory**  
 4, LS-ro 182beon-gil, Gunpo-si, Gyeonggi-do, 435-040 Korea

**Remarks :**

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at [www.sgs.com/terms\\_e-document.htm](http://www.sgs.com/terms_e-document.htm). The results shown in this test report refer only to the sample(s) tested unless otherwise stated. This Test Report cannot be reproduced, except in full

## Contents

1. General Information .....	3
1.1 Client Information .....	3
1.2 Test Laboratory .....	3
1.3 General Information of E.U.T.....	3
1.4 Operating Modes and Conditions .....	4
1.5 Auxiliary Equipments .....	4
1.6 Cable List .....	5
1.7 System Configurations .....	6
1.8 Test System Layout.....	6
1.9 Modifications .....	6
1.10 Applicable Standards for Testing.....	7
1.11 Summary of Test Results .....	7
2. Emission Test .....	8
2.1 Test Results .....	8
2.2 Test Method and Limits .....	8
2.2.1 Test Method .....	8
2.2.2 Test Limits .....	8
2.3 Conducted Emission .....	9
2.3.1 Test Equipments .....	9
2.3.2 Test Site .....	10
2.3.3 Environment Conditions .....	10
2.4 Radiated Emission .....	11
2.4.1 Test Equipments .....	11
2.4.2 Test Site .....	11
2.4.3 Environment Conditions .....	12
Appendix A: Conducted Emission.....	14
Appendix B: Radiated Emission (3 m Scan Data).....	15

## 1. General Information

### 1.1 Client Information

Applicant : i-SENS, Inc.  
 Address of Applicant : 43, Banpo-daero 28-gil, Seocho-gu, Seoul, 137-873, Republic of Korea

Manufacturer : i-SENS, Inc.  
 Address of Manufacturer : 43, Banpo-daero 28-gil, Seocho-gu, Seoul, 137-873, Republic of Korea

### 1.2 Test Laboratory

Name and Address : SGS Korea Co., Ltd.  
 Giheung 1 Laboratory : 35, Giheungdanji-ro 121beon-gil, Giheung-gu, Yongin-si, Gyeonggi-do, Republic of Korea  
 Giheung 2 Laboratory : 23, Giheungdanji-ro 24beon-gil, Giheung-gu, Yongin-si, Gyeonggi-do, Republic of Korea  
 Gunpo Laboratory : 4, LS-ro 182beon-gil, Gunpo-si, Gyeonggi-do, 435-040 Republic of Korea  
 Phone : + 82 31 428 5700  
 Fax : + 82 31 427 2370  
 e-mail : [paul.kang@sgs.com](mailto:paul.kang@sgs.com)

### 1.3 General Information of E.U.T.

Product Name	Blood Glucose Meter
Model Name	GM01CAB
Alt Model Name	GM01CAD
Model different	Model name is different in market
FCC ID	OELGM01CAB
Serial No.	B2C800C00012
H/W Version	V1.0.6
S/W Version	V64.52.3
EMI Classification	Class B
Internal Highest Frequency	20 MHz
Test Voltage	120 V 60 Hz

## 1.4 Operating Modes and Conditions

Operating mode	Operating condition
USB Data communication	USB Data communication with notebook computer.
Blood glucose measurement	Blood glucose measurement status.

## 1.5 Auxiliary Equipments

Description	Model	Serial No.	Manufacturer
Notebook Computer	LGE-DMLGX14(B)	008QTEQ024836	LG Electronics Co., Ltd.
LCD Monitor	S2740Lb	CN-DP7D0G-74261-352-05CL	DELL Inc.
USB Keyboard	WK590	HDJ2011000000	WINTEK
USB MOUSE	M-U0026	810-002147	Logitech
Wireless Router	WG602v4	-	NETGEAR

Note: Auxiliary equipments are declared according to FCC procedure.

## 1.6 Cable List


Start		END		Cable Spec.		
Name	I/O Port	Name	I/O Port	Length	Shield	Core
USB Data communication Mode						
EUT	USB	Notebook Computer	USB	0.5	Shield	-
Notebook Computer	USB	USB Keyboard	-	1.2	Unshield	-
	USB	USB Mouse	-	1.2	Unshield	-
	RGB	LCD Monitor	RGB	1.0	Unshield	-
	LAN	Wireless Router	LAN	1.5	Unshield	-
	DC IN	AC/DC Adapter	DC OUT	1.5	Unshield	-
AC/DC Adapter	AC IN	AC Source	-	1.2	Unshield	-
LCD Monitor	DC IN	AC/DC Adapter	DC OUT	1.0	Unshield	-
AC/DC Adapter	AC IN	AC Source	-	1.5	Unshield	-
Wireless Router	DC IN	Power supply	DC OUT	1.0	Unshield	-
Power supply	AC IN	AC Source	-	-	-	-
Blood glucose measurement Mode						
EUT	-	-	-	-	-	-

## 1.7 System Configurations


Description	Model	Serial No.	Manufacturer
Main Board	RGA2E0620-V2.0.0	141216	-
Display	-	-	-
Inner Battery	JHY403048 2.146Wh 580mAh3.7V	B2C800C00012	-

## 1.8 Test System Layout

<USB Data communication Mode>

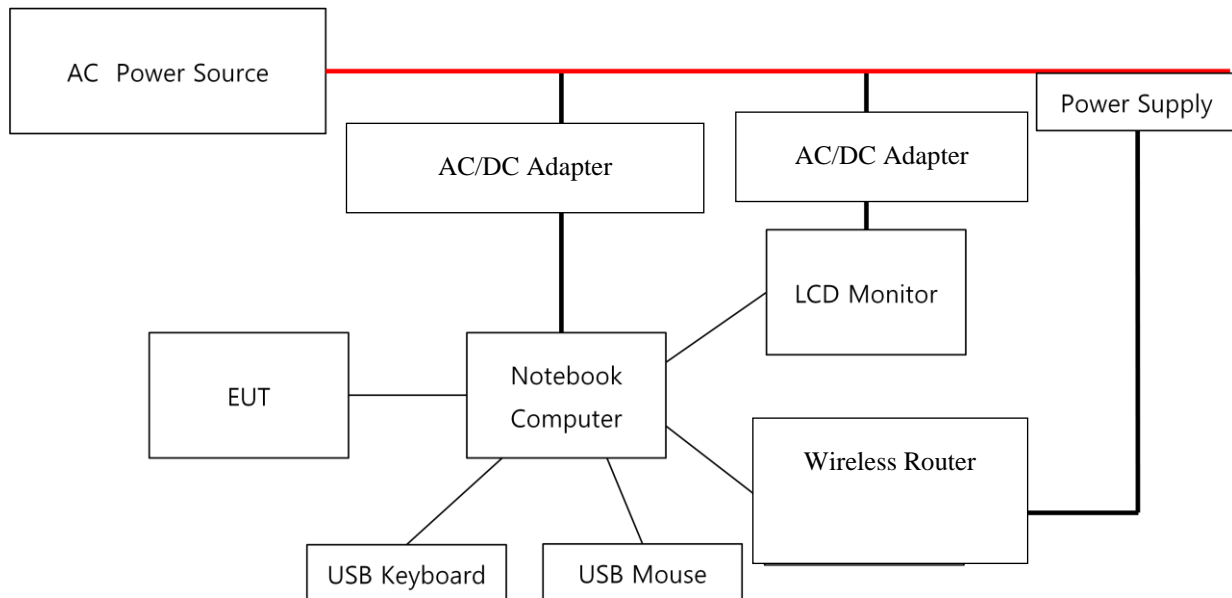

<Blood glucose measurement Mode>



## 1.9 Modifications

There was no modified item during the test.



# TEST REPORT



Report No. : F690501/RF-EMG005521 Page( 7 )/( 17 )

## 1.10 Applicable Standards for Testing

Standards	Status	Deviation
FCC Part 15 Subpart B FCC Part 18	Applicable	No Deviation

## 1.11 Summary of Test Results

Test Item	Basic Standards	Results
Conducted Emission	FCC Part 15 Subpart B, FCC Part 18 ANSI C63.4 : 2009, MD-5:1986	Complied
Radiated Emission	FCC Part 15 Subpart B, FCC Part 18 ANSI C63.4 : 2009, MD-5:1986	Complied

Note : Test methods of all test items are performed according to the basic standards in this table.

## EMISSION

### 2.1 Test Results

Test Items	Basic Standards	Test Results
Conducted Emission	FCC Part 15 Subpart B, FCC Part 18 ANSI C63.4 : 2009, MD-5:1986	<b>Complied</b>
Radiated Emission	FCC Part 15 Subpart B, FCC Part 18 ANSI C63.4 : 2009, MD-5:1986	<b>Complied</b>

### 2.2 Test Method and Limits

#### 2.2.1 Test Method

Test Items	Measuring Frequency Range	RBW	Measuring Distance
Conducted Emission	0.15 MHz ~ 30 MHz	9 kHz	-
Radiated Emission	9 kHz ~ 0.15 MHz	200 Hz	3 m
	0.15 MHz ~ 30 MHz	9 kHz	3 m
	30 MHz ~ 1 GHz	120 kHz	10 m & 3 m
	Above 1 GHz	9 kHz	3 m

Note : 10 m method of radiated emission measurement is only applied to Class A equipment over the frequency range of 30 MHz ~ 1 GHz. Except this, 3 m method is applied to Class B equipment over the frequency range of 30 MHz ~ 1 GHz and Class A and Class B equipment above 1 GHz.

#### 2.2.2 Test Limits

##### -Conducted Emission Limits

Frequency Range	Limits( dB( $\mu$ V) )		Class
	Quasi-peak	Average	
0.15 MHz ~ 0.5 MHz	79	66	<b>Class A</b>
0.5 MHz ~ 30 MHz	73	60	
0.15 MHz ~ 0.5 MHz	66 to 56	56 to 46	<b>Class B</b>
0.5 MHz ~ 5 MHz	56	46	
5 MHz ~ 30 MHz	60	50	

Note : The lower limit shall apply at the transition frequencies. The limit decreases linearly with the logarithm of the frequency in the range 0.15 MHz to 0.5 MHz.



### -Radiated Emission Limits in part 18

Frequency Range	Limits( dB( $\mu$ V/m) ) Average	Class
9 kHz ~ 400 MHz	63.5	<b>Miscellaneous device</b>

### -Radiated Emission Limits below 1 GHz in part 15

Frequency Range	Limits( dB( $\mu$ V/m) )	Class
	Quasi-peak	
30 MHz ~ 88 MHz	39.1	<b>Class A</b>
88 MHz ~ 216 MHz	43.5	
216 MHz ~ 960 MHz	46.4	
960 MHz ~ 1 GHz	49.5	
30 MHz ~ 88 MHz	40	<b>Class B</b>
88 MHz ~ 216 MHz	43.5	
216 MHz ~ 960 MHz	46	
960 MHz ~ 1 GHz	54	

### -Radiated Emission Limits above 1 GHz (3m method)

Frequency Range	Limits( dB( $\mu$ V/m) )		Class
	Average	Peak	
Above 1 GHz	59.5	79.5	<b>Class A</b>
Above 1 GHz	54	74	<b>Class B</b>

## 2.3 Conducted Emission

The initial preliminary exploratory scans were performed over the measuring frequency range(0.15 MHz to 30 MHz) using a max hold mode incorporating a Peak detector and Average detector and using the software of EMC32(Version 8.50.0 from R&S). The final test data was measured using a Quasi-Peak detector and Average detector.

### 2.3.1 Test Equipments

Description	Model No.	Manufacturer	S/N	Last Cal. Date
Two-Line V-Network	ENV216	R & S	100190	2014.12.25
Artificial Mains Networks	ESH2-Z5	R & S	100280	2014.04.04
Test Receiver	ESCI 7	R & S	100911	2014.01.07

Note : The calibration period of every equipment is 1 year.

### 2.3.2 Test Site

Shield Room in Gunpo Laboratory

### 2.3.3 Environment Conditions

Temperature : 22.4 °C ~ 22.7 °C

Humidity : 31.0 %R.H. ~ 32.0 %R.H.

Atmospheric Pressure : 100.5 kPa

**Test Date** : March 30, 2015

### USB Data Communication Mode

Freq. ( MHz )	Line (H/N)	Level ( dB $\mu$ V )		CL ( dB )	LISN ( dB )	Result ( dB $\mu$ V )		Limit ( dB $\mu$ V )		Margin ( dB )	
		Q/P	A/V			Q/P	A/V	Q/P	A/V	Q/P	A/V
0.19	N	42.0	25.9	0.0	9.7	51.7	35.6	63.9	53.9	12.2	18.3
0.20	H	43.0	24.4	0.0	9.6	52.6	34.0	63.6	53.6	11.0	19.6
0.26	H	32.7	15.4	0.0	9.6	42.3	25.0	61.4	51.4	19.1	26.4
0.33	H	25.6	10.1	0.0	9.6	35.2	19.7	59.5	49.5	24.3	29.8
11.08	N	19.8	13.2	0.1	9.8	29.7	23.1	60.0	50.0	30.3	26.9
24.09	N	19.5	12.1	0.2	9.9	29.7	22.3	60.0	50.0	30.3	27.7

Measurement Uncertainty :  $\pm 3.21$  dB (The confidential level is about 95%,  $k=2$ )

- Note :
- Line ( H ) : Hot
  - Line ( N ) : Neutral
  - CL: Cable Loss
  - LISN : LISN Factor
  - Result = Level + CL + LISN
  - Margin = Limit – Result

**See Appendix A (Conducted Emission)**

## 2.4 Radiated Emission

The initial preliminary exploratory scans were performed at 3 m distance over the measuring frequency range(9 kHz to 1 GHz) using a max hold mode incorporating a Peak detector and using the software of EP5RE(Version Ver3.10.20 from TOYO). The final test data was measured using a Quasi-Peak detector at 1 GHz at 3 m distance. at USB Communication mode and Average detector at Blood glucose measurement Mode. Measurements were made with the antenna positioned in both the horizontal and vertical planes of polarization. The antenna height was varied from 1 m to 4 m and the EUT was rotated 360° to find the maximum emitting point for each frequency.

### 2.4.1 Test Equipments

Description	Model No.	Manufacturer	S/N	Last Cal. Date
Bilog Antenna	VULB9163	SCHWARZBECK MESS- ELEKTRONIK	396	2014.06.16
Test Receiver	ESU26	R & S	100109	2014.06.16
Amplifier	8447F	HP	2944A03909	2014.08.27
Active Loop Antenna	FMZB1519	SCHWARZBECK	1519-039	2013.07.09

Note : Only the calibration period of Antennas is 2 years but the period of every equipment is 1 year.

### 2.4.2 Test Site

3 m Semi-Anechoic Chamber in Gunpo Laboratory

## 2.4.3 Environment Conditions

Temperature : 21.5 °C ~ 21.9 °C  
 Humidity : 28.0 %R.H. ~ 31.0 %R.H.  
 Atmospheric Pressure : 100.6 kPa

**Test Date** : March 31, 2015

### Blood Glucose measurement Mode

Freq. ( MHz )	Level ( dB $\mu$ V )	Pol. (H/V)	A ( ° )	H ( cm )	AF ( dB )	CL ( dB )	F/S ( dB $\mu$ V/m )	Limit ( dB $\mu$ V/m )	Margin ( dB )
9kHz~150kHz									
0.01	27.4	H	172	200	20.4	0.1	47.9	63.5	15.6
0.02	30.0	H	172	200	20.4	0.1	50.4	63.5	13.1
0.03	36.9	V	148	200	20.3	0.1	57.2	63.5	6.3
0.04	26.2	H	105	200	20.2	0.1	46.5	63.5	17.0
0.05	24.2	V	170	200	20.1	0.1	44.4	63.5	19.1
0.09	29.1	H	172	200	20.0	0.1	49.2	63.5	14.3
150kHz~30MHz									
0.19	22.1	H	176	200	20.0	0.1	42.2	63.5	21.3
0.24	20.8	V	340	200	20.0	0.1	40.9	63.5	22.6
0.57	21.2	H	20	200	20.2	0.1	41.5	63.5	22.0
5.03	19.6	V	223	200	20.2	0.3	40.0	63.5	23.5

Measurement Uncertainty (Horizontal) :  $\pm 3.59$  dB (The confidential level is about 95%,  $k=2$ )

Measurement Uncertainty (Vertical) :  $\pm 3.59$  dB (The confidential level is about 95%,  $k=2$ )

Note: • AF = Antenna Factor                      • CL = Cable Loss                      • F/S = Field Strength  
 • Pol.(H) = Horizontal                      • Pol.(V) = Vertical                      • Amp. = Amplifier Gain  
 • Margin = Limit – F/S  
 • A : Angle                                      • H : Height

### Blood Glucose measurement Mode

Freq. ( MHz )	Level ( dB $\mu$ V )	Pol. ( H/V )	A ( ° )	H ( cm )	AF ( dB )	CL ( dB )	Amp. ( dB )	F/S ( dB $\mu$ V/m )	Limit ( dB $\mu$ V/m )	Margin ( dB )
41.10	32.6	H	65	400	14.3	0.9	27.7	20.1	63.5	43.4
58.27	33.1	V	133	100	12.9	1.0	27.8	19.1	63.5	44.4
93.13	33.8	V	231	100	10.5	1.3	27.8	17.8	63.5	45.7
100.33	32.4	H	111	400	11.2	1.3	27.6	17.4	63.5	46.1
370.55	33.2	V	26	100	15.8	2.5	27.0	24.6	63.5	38.9
397.70	32.6	H	80	200	16.4	2.6	26.7	24.9	63.5	38.6

### USB Data Communication Mode

Freq. ( MHz )	Level ( dB $\mu$ V )	Pol. ( H/V )	A ( ° )	H ( cm )	AF ( dB )	CL ( dB )	Amp. ( dB )	F/S ( dB $\mu$ V/m )	Limit ( dB $\mu$ V/m )	Margin ( dB )
48.07	47.8	V	99	100	14.1	0.9	27.6	35.2	40.0	4.8
65.85	50.4	H	231	400	10.1	1.0	27.8	33.7	40.0	6.3
66.17	51.9	V	172	400	9.9	1.0	27.8	35.0	40.0	5.0
143.89	55.1	V	240	100	8.2	1.5	27.2	37.6	43.5	5.9
155.98	54.2	V	103	200	8.2	1.6	27.5	36.5	43.5	7.0
384.33	36.2	H	89	100	16.1	2.6	26.9	28.0	46.0	18.0

Measurement Uncertainty (Horizontal) :  $\pm 5.31$  dB (The confidential level is about 95%,  $k=2$ )


Measurement Uncertainty (Vertical) :  $\pm 5.71$  dB (The confidential level is about 95%,  $k=2$ )

Note: • AF = Antenna Factor                      • CL = Cable Loss                      • F/S = Field Strength  
          • Pol.(H) = Horizontal                      • Pol.(V) = Vertical                      • Amp. = Amplifier Gain  
          • Margin = Limit – F/S                      • F/S = Level + AF + CL – Amp.  
          • A : Angle                                      • H : Height


**See Appendix B (Radiated Emission)**

## Appendix A: Conducted Emission

### Neutral

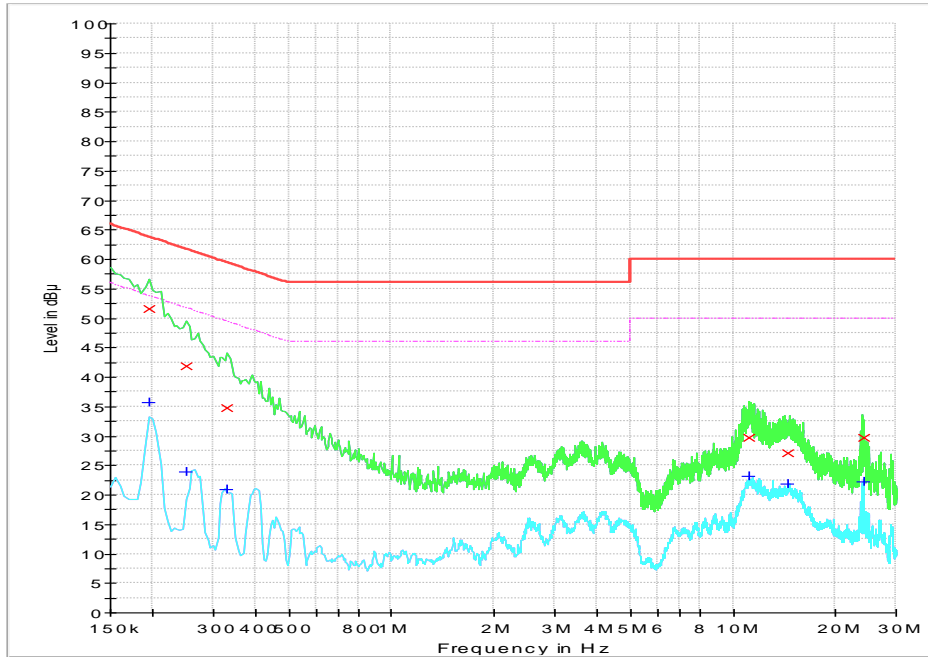


### Hot

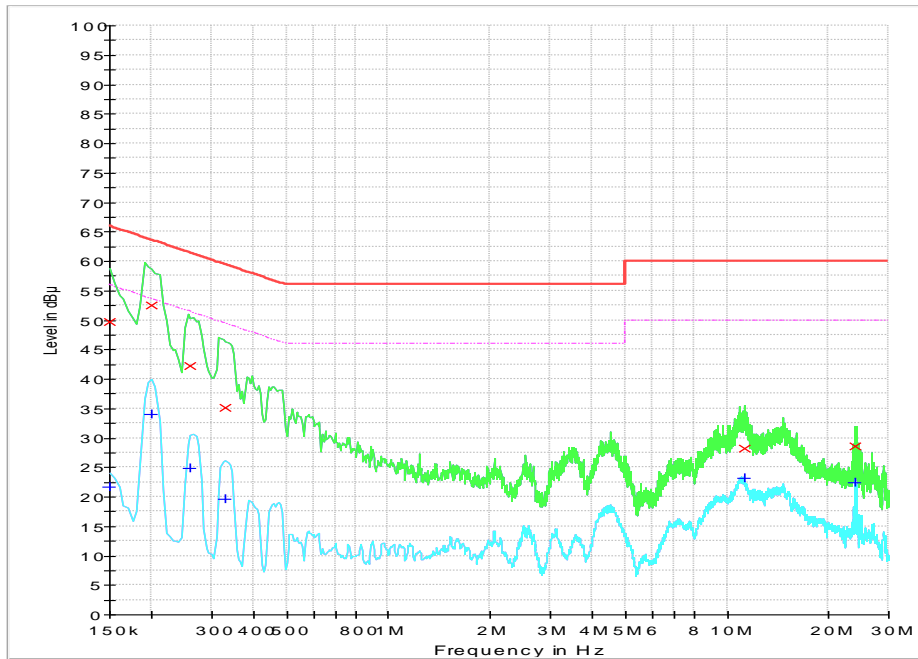


## Appendix B: Radiated Emission (3 m Scan Data)


### Blood Glucose measurement Mode Horizontal (9kHz ~ 150MHz)

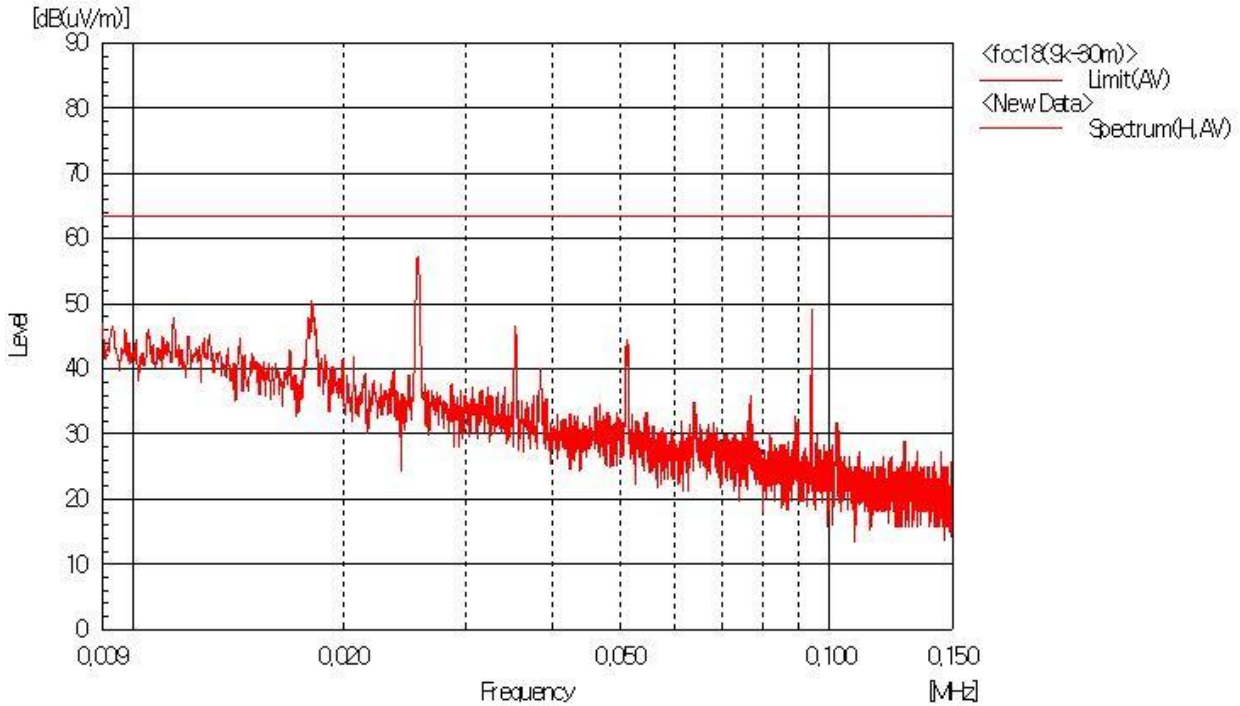


### Vertical(9kHz ~ 150MHz)

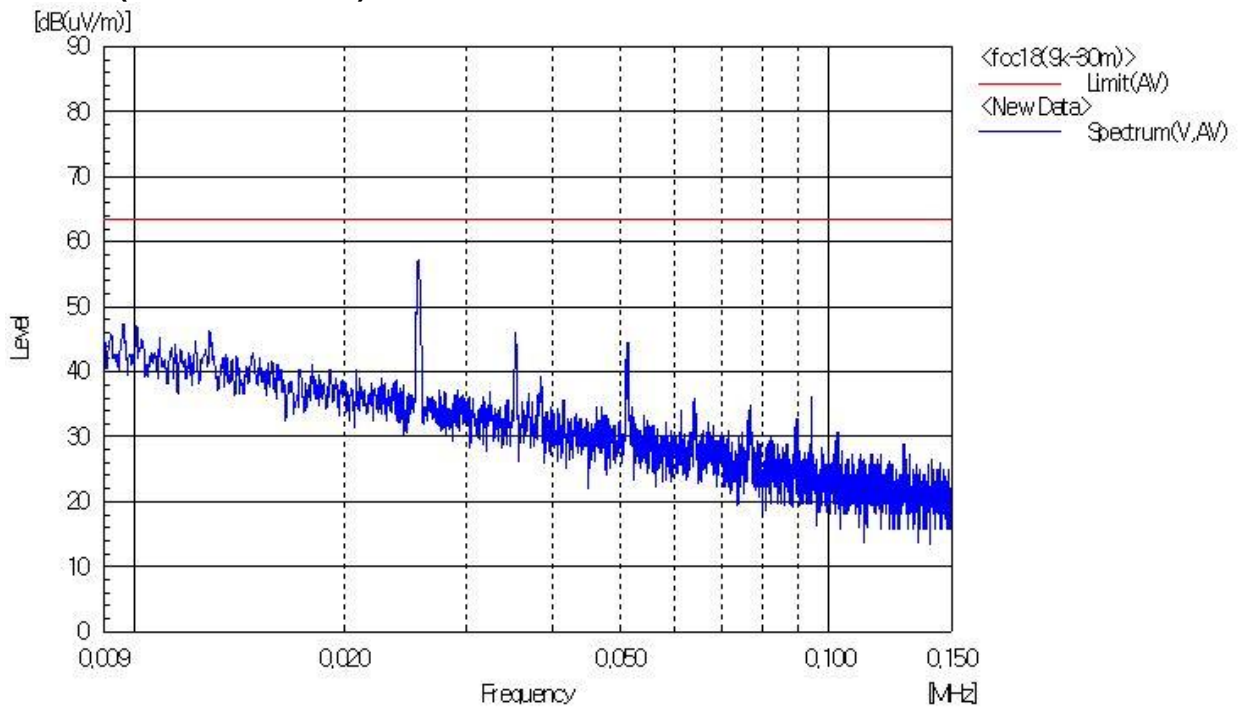

### Horizontal (150kHz ~ 30MHz)

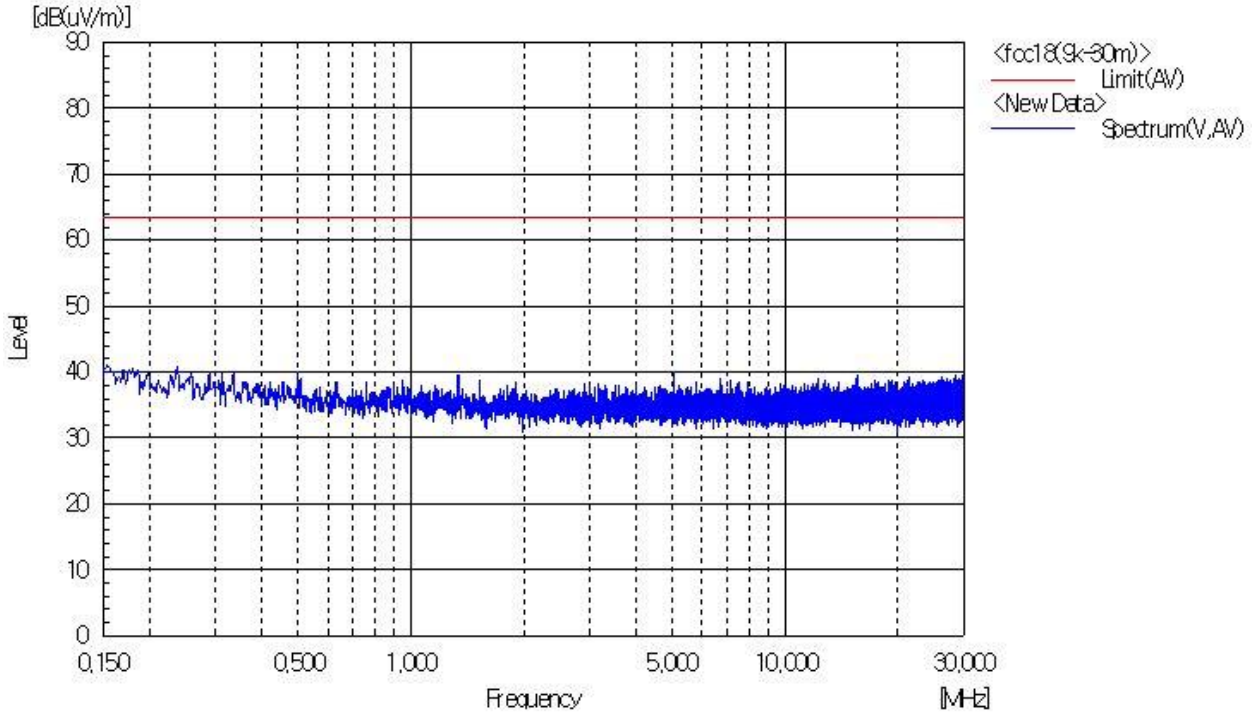


### Vertical(150kHz ~ 30MHz)

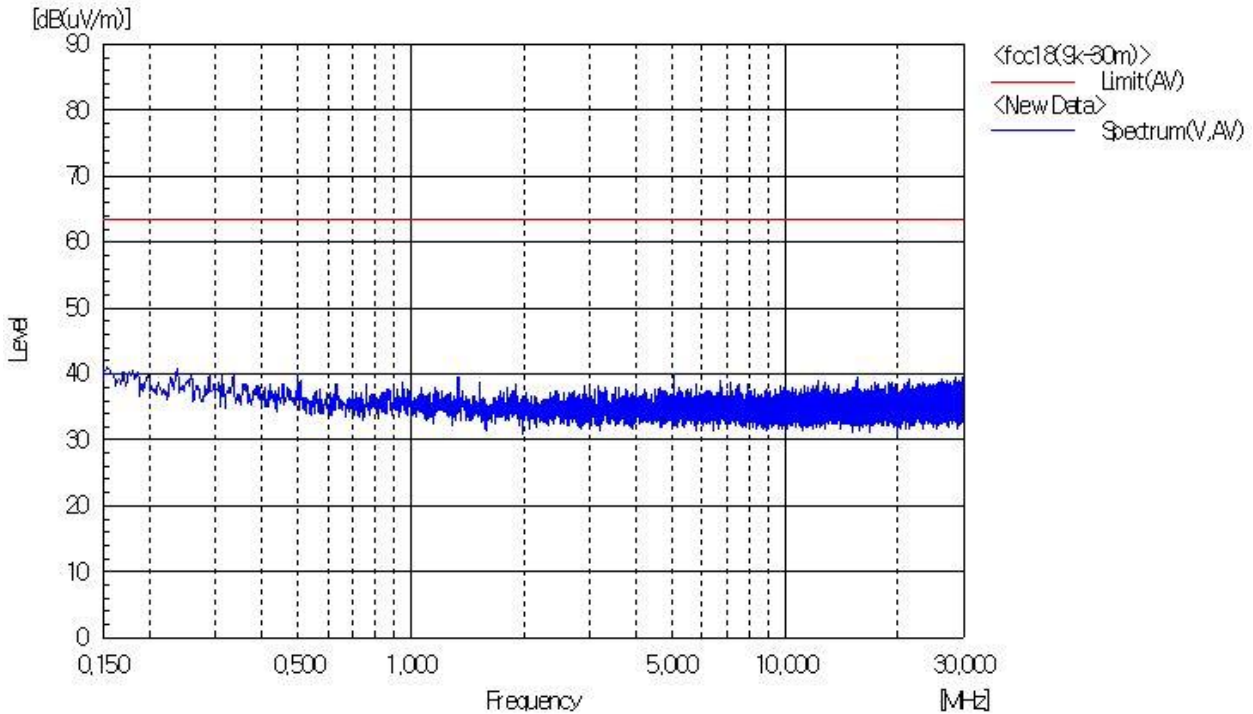



### Blood Glucose measurement Mode

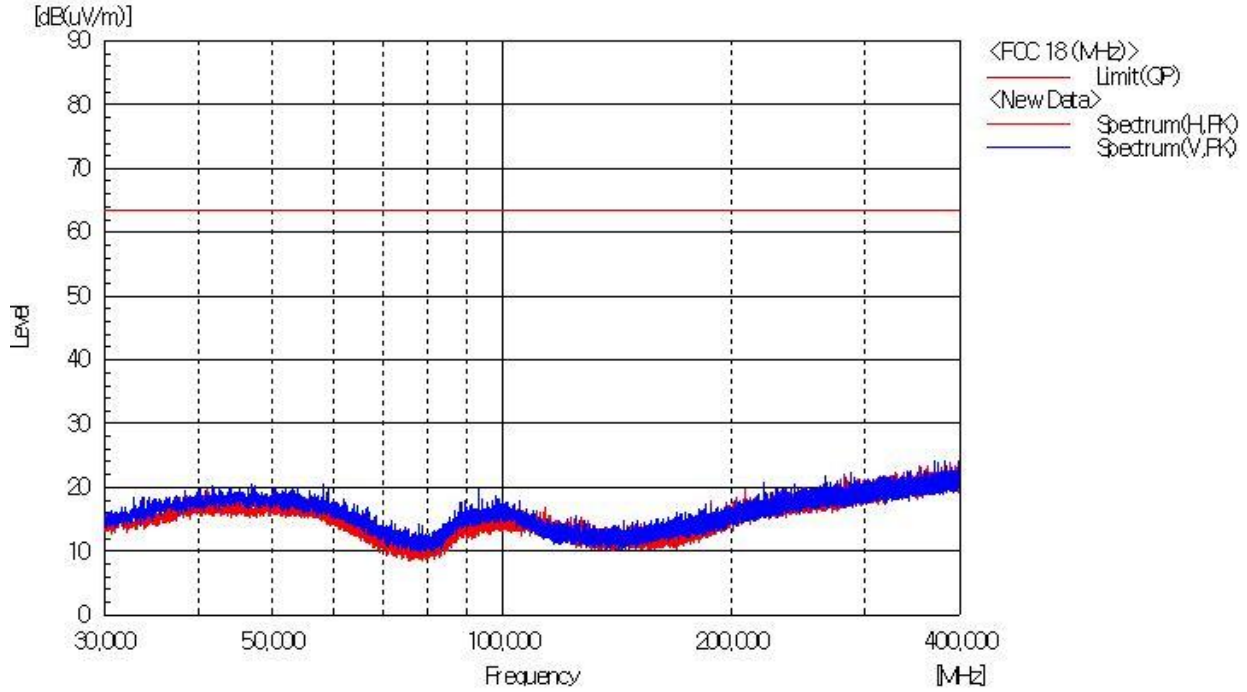

### USB Data Communication Mode

