


# LABELLING REQUIREMENTS

## Labelling Requirements

The sample label shown shall be *permanently affixed* at a conspicuous location on the device and be readily visible to the user at the time of purchase.

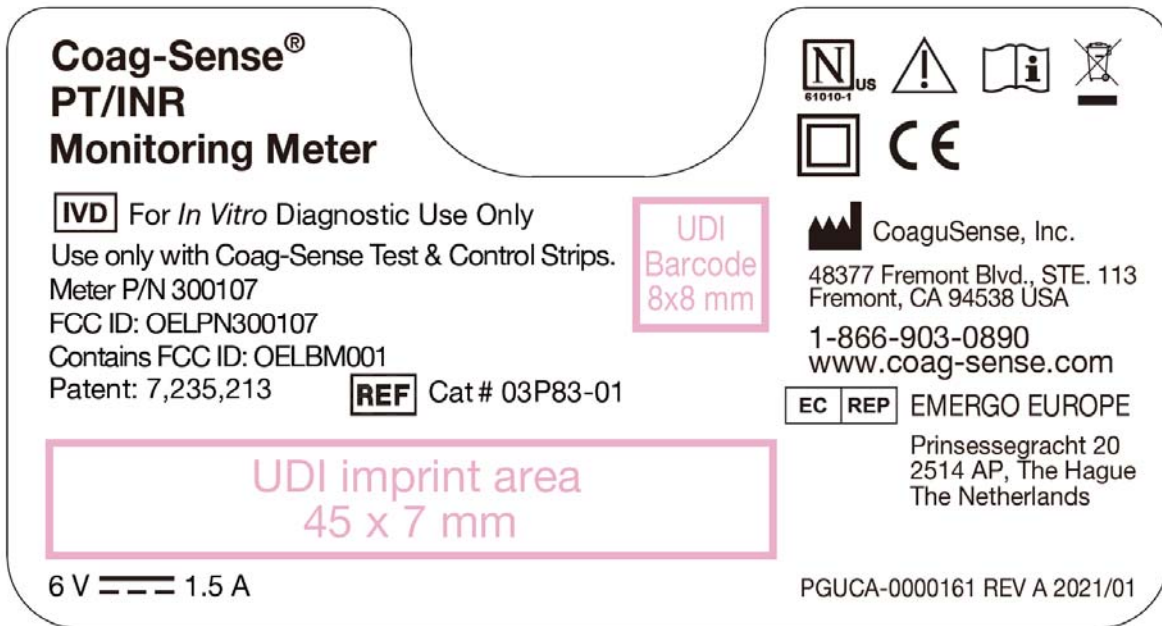


**Coag-Sense®  
PT/INR  
Monitoring Meter**




**IVD** For *In Vitro* Diagnostic Use Only  
Use only with Coag-Sense Test & Control Strips.  
Meter P/N 300107  
FCC ID: OELPN300107  
Contains FCC ID: OELBM001  
Patent: 7,235,213

**REF** Cat# 03P83-01

**UDI Barcode**  
8x8 mm

**UDI imprint area**  
45 x 7 mm

6 V  1.5 A


**N**<sub>US</sub>     
61010-1

**CE**

**CoaguSense, Inc.**  
48377 Fremont Blvd., STE. 113  
Fremont, CA 94538 USA  
1-866-903-0890  
www.coag-sense.com

**EC REP** EMERGO EUROPE  
Prinsessegracht 20  
2514 AP, The Hague  
The Netherlands

PGUCA-0000161 REV A 2021/01

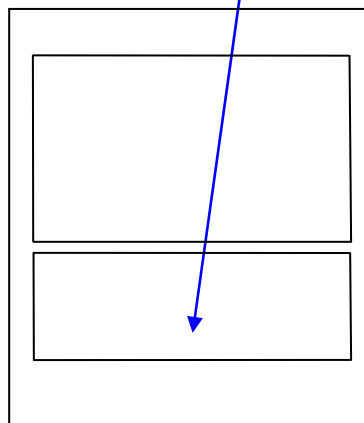

< Bottom >