

# Medtronic MiniMed

REVISED TEST REPORT FOR

**NGP Insulin Pump  
Model: MMT-1781KQ**

Tested to The Following Standards:

FCC Part 15 Subpart C Section(s)

**15.247  
(DTS 2400-2483.5 MHz)**

**Report No.: 99536-88A**

Date of issue: October 17, 2017



This test report bears the accreditation symbol indicating that the testing performed herein meets the test and reporting requirements of ISO/IEC 17025 under the applicable scope of EMC testing for CKC Laboratories, Inc.

We strive to create long-term, trust based relationships by providing sound, adaptive, customer first testing services. We embrace each of our customers' unique EMC challenges, not as an interruption to set processes, but rather as the reason we are in business.

## TABLE OF CONTENTS

Administrative Information .....	3
Test Report Information .....	3
Revision History .....	3
Report Authorization .....	3
Test Facility Information .....	4
Software Versions .....	4
Site Registration & Accreditation Information .....	4
Summary of Results .....	5
Modifications During Testing .....	5
Conditions During Testing .....	5
Equipment Under Test .....	6
General Product Information .....	7
FCC Part 15 Subpart C .....	8
15.247(a)(2) 6dB Bandwidth .....	8
15.247(b)(3) Output Power .....	12
15.247(e) Power Spectral Density .....	19
15.247(d) Radiated Emissions & Band Edge .....	27
Supplemental Information .....	46
Measurement Uncertainty .....	46
Emissions Test Details .....	46

## ADMINISTRATIVE INFORMATION

### Test Report Information

**REPORT PREPARED FOR:**

Medtronic MiniMed  
18000 Devonshire Street  
Northridge, CA 91325-1219

Representative: Greg Bowden  
Customer Reference Number: 4500117074

**DATE OF EQUIPMENT RECEIPT:****DATE(S) OF TESTING:****REPORT PREPARED BY:**

Terri Rayle  
CKC Laboratories, Inc.  
5046 Sierra Pines Drive  
Mariposa, CA 95338

Project Number: 99536

February 8, 2017

February 8-11, 2017

### Revision History

**Original:** Testing of the NGP Insulin Pump, Model: MMT-1781KQ to FCC Part 15 Subpart C Section(s) 15.247 (DTS 2400-2483.5 MHz).

**Revision A:** To replace the data in section 15.247(d) Radiated Emissions 1-26GHz due to incorrect transducer noted.

### Report Authorization

The test data contained in this report documents the observed testing parameters pertaining to and are relevant for only the sample equipment tested in the agreed upon operational mode(s) and configuration(s) as identified herein. Compliance assessment remains the client's responsibility. This report may not be used to claim product endorsement by A2LA or any government agencies. This test report has been authorized for release under quality control from CKC Laboratories, Inc.



**Steve Behm**  
**Director of Quality Assurance & Engineering Services**  
**CKC Laboratories, Inc.**

## Test Facility Information



Our laboratories are configured to effectively test a wide variety of product types. CKC utilizes first class test equipment, anechoic chambers, data acquisition and information services to create accurate, repeatable and affordable test results.

TEST LOCATION(S):  
CKC Laboratories, Inc.  
Canyon Park  
22116 23rd Drive S.E., Suite A  
Bothell, WA 98021

## Software Versions

CKC Laboratories Proprietary Software	Version
EMITest Emissions	5.03.02

## Site Registration & Accreditation Information

Location	CB #	TAIWAN	CANADA	FCC	JAPAN
Canyon Park Bothell, WA	US0081	SL2-IN-E- 1145R	3082C-1	US1022	A-0148

## SUMMARY OF RESULTS

**Standard / Specification: FCC Part 15 Subpart C - 15.247 (DTS) (2400-2483.5 MHz)**

Test Procedure	Description	Modifications	Results
15.247(a)(2)	6dB Bandwidth	NA	Pass
15.247(b)(3)	Output Power	NA	Pass
15.247(e)	Power Spectral Density	NA	Pass
15.247(d)	RF Conducted Emissions & Band Edge	NA	NA2
15.247(d)	Radiated Emissions & Band Edge	NA	Pass
15.207	AC Conducted Emissions	NA	NA1

NA = Not Applicable

NA1 = Not applicable because the EUT is only battery powered.

NA2 = Not applicable because the EUT does not have an antenna port.

### Modifications During Testing

This list is a summary of the modifications made to the equipment during testing.

Summary of Conditions
No modifications were made during testing.

**Modifications listed above must be incorporated into all production units.**

### Conditions During Testing

This list is a summary of the conditions noted to the equipment during testing.

Summary of Conditions
None

## EQUIPMENT UNDER TEST (EUT)

During testing, numerous configurations may have been utilized. The configurations listed below support compliance to the standard(s) listed in the Summary of Results section.

### Configuration 1

***Equipment Tested:***

Device	Manufacturer	Model #	S/N
NGP Insulin Pump (Jabil)	Medtronic MiniMed	MMT-1781KQ	NG0011690X

***Support Equipment:***

Device	Manufacturer	Model #	S/N
None			

### Configuration 2

***Equipment Tested:***

Device	Manufacturer	Model #	S/N
NGP Insulin Pump (Jabil)	Medtronic MiniMed	MMT-1781KQ	NG0011688X

***Support Equipment:***

Device	Manufacturer	Model #	S/N
None			

## General Product Information:

Product Information	Manufacturer-Provided Details
Equipment Type:	Stand-Alone Equipment
Type of Wideband System:	802.15.4
Operating Frequency Range:	2420MHz-2480MHz
Modulation Type(s):	O-QPSK
Maximum Duty Cycle:	23%
Number of TX Chains:	1
Antenna Type(s) and Gain:	Integral 0dBi
Beamforming Type:	None
Antenna Connection Type:	Integral
Nominal Input Voltage:	1.5V battery
Firmware / Software used for Test:	6x0G XTest PRM 2.5A (M969745DOC)

## FCC Part 15 Subpart C

### 15.247(a)(2) 6dB Bandwidth

Test Setup/Conditions			
Test Location:	Bothell Lab Bench	Test Engineer:	S. Pittsford
Test Method:	ANSI C63.10 (2013), KDB 558074 D01 DTS Meas Guidance v03r05 (04/08/2016)	Test Date(s):	2/10/2017
Configuration:	2		
Test Setup:	Frequency tested: 2420MHz, 2450MHz, 2480MHz Firmware power setting: Max Power EUT Firmware: 6x0G XTest PRM 2.5A(M969745DOC)  Duty Cycle: 100%  Test Mode: Continuously modulated Test Setup: EUT is set in a test fixture (nearfield probe connected to spectrum analyzer via a cable).		



Environmental Conditions			
Temperature (°C)	23.5	Relative Humidity (%):	30


Test Equipment					
Asset#	Description	Manufacturer	Model	Cal Date	Cal Due
02673	Spectrum Analyzer	Agilent	E4446A	2/3/2017	2/3/2019
P06867	Cable	Astrolab	32026-29080- 29080-84	10/16/2015	10/16/2017

Test Data Summary					
Frequency (MHz)	Antenna Port	Modulation	Measured (kHz)	Limit (kHz)	Results
2420	1	O-QPSK	1574	≥500	Pass
2450	1	O-QPSK	1586	≥500	Pass
2480	1	O-QPSK	1589	≥500	Pass



Plot(s)

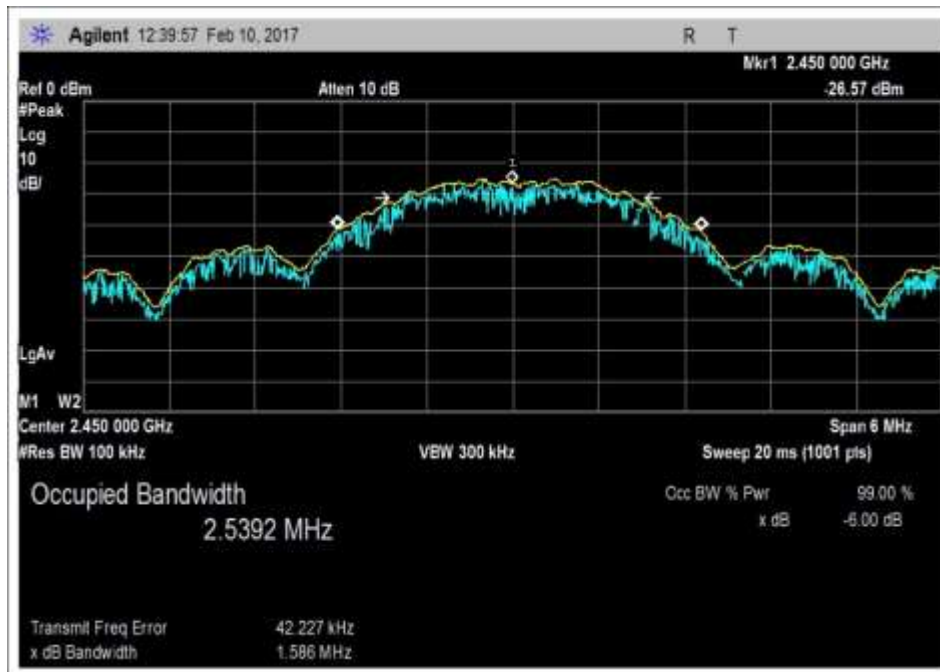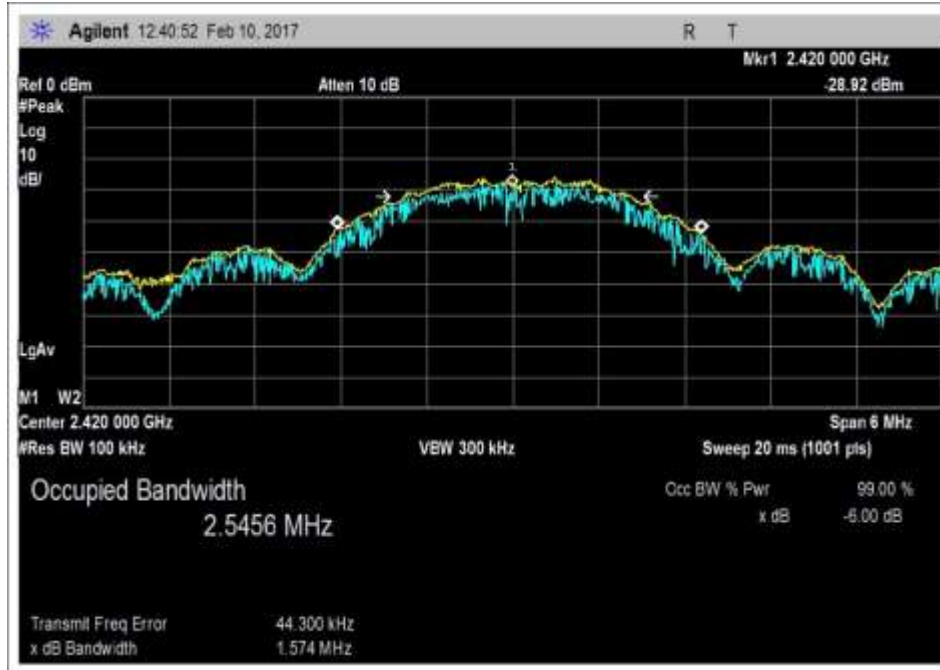

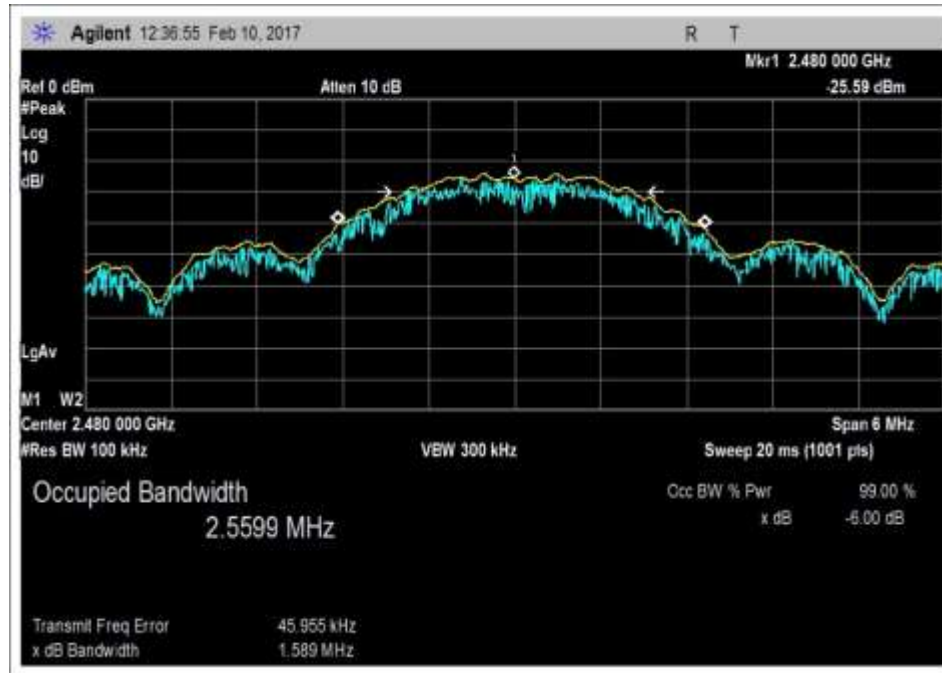

Test Setup Photo(s)



## 15.247(b)(3) Output Power

Test Setup / Conditions			
Test Location:	Bothell Lab C3	Test Engineer:	S. Pittsford
Test Method:	ANSI C63.10 (2013), KDB 558074 D01 DTS Meas Guidance v03r05 (04/08/2016)	Test Date(s):	2/11/2017
Configuration:	2		
Test Setup:	See Data Sheet.		

Environmental Conditions			
Temperature (°C)	22	Relative Humidity (%):	30

### Test Data Summary - Voltage Variations

This equipment is battery powered. Power output tests were performed using a fresh battery.

Power Output Test Data Summary - Radiated Measurement						
Measurement Option: RBW > DTS Bandwidth						
Frequency (MHz)	Modulation	Ant. Type / Gain (dBi)	Field Strength (dBuV/m @3m)	Calculated (dBm)	Limit (dBm)	Results
2420	O-QPSK	Integral 0dBi	91.4	-3.8	≤30	Pass
2450	O-QPSK	Integral 0dBi	92.2	-3.0	≤30	Pass
2480	O-QPSK	Integral 0dBi	91.4	-3.8	≤30	Pass

For fixed point-to-point antennas, the limit is calculated in accordance with 15.247(c)(1):  $Limit = 30 - Roundup\left(\frac{G-6}{3}\right)$

For directional beamforming antennas, the limit is calculated in accordance with 15.247(c)(2) and KDB 662911.

Conducted RF output power calculated in accordance with ANSI C63.10.

$$P(W) = \frac{(E \cdot d)^2}{30 G}$$

Or equivalently, in logarithmic form:

$$P(dBm) = E(dBuV/m) + 20LOG(d) - G - 104.77$$

**Test Setup / Conditions / Data**

Test Location: CKC Laboratories • 22116 23rd Dr. SE • Bothell, WA 98021 • (425) 402-1717  
 Customer: **Medtronic MiniMed**  
 Specification: **15.247(b) Power Output (2400-2483.5 MHz DTS)**  
 Work Order #: **99536** Date: 2/11/2017  
 Test Type: **Maximized Emissions** Time: 14:04:29  
 Tested By: Steven Pittsford Sequence#: 2  
 Software: EMITest 5.03.02

***Equipment Tested:***

Device	Manufacturer	Model #	S/N
Configuration 2			

***Support Equipment:***

Device	Manufacturer	Model #	S/N
Configuration 2			


***Test Conditions / Notes:***

Frequency tested: 2420MHz, 2450MHz, 2480MHz  
 Firmware power setting: Max Power  
 EUT Firmware: 6x0G XTest PRM 2.5A(M969745DOC)

Duty Cycle: 100%

Test Mode: Continuously modulated  
 Test Setup: The EUT is set 1.5 meters high on a Styrofoam table. X, Y and Z axis are investigated with the worst case reported.  
 EUT has a fresh battery installed

Medtronic MiniMed vO#: 99536 Sequence#: 2 Date: 2/11/2017  
 15.247(b) Power Output (2400-2483.5 MHz DTS) Test Distance: 3 Meters Vert

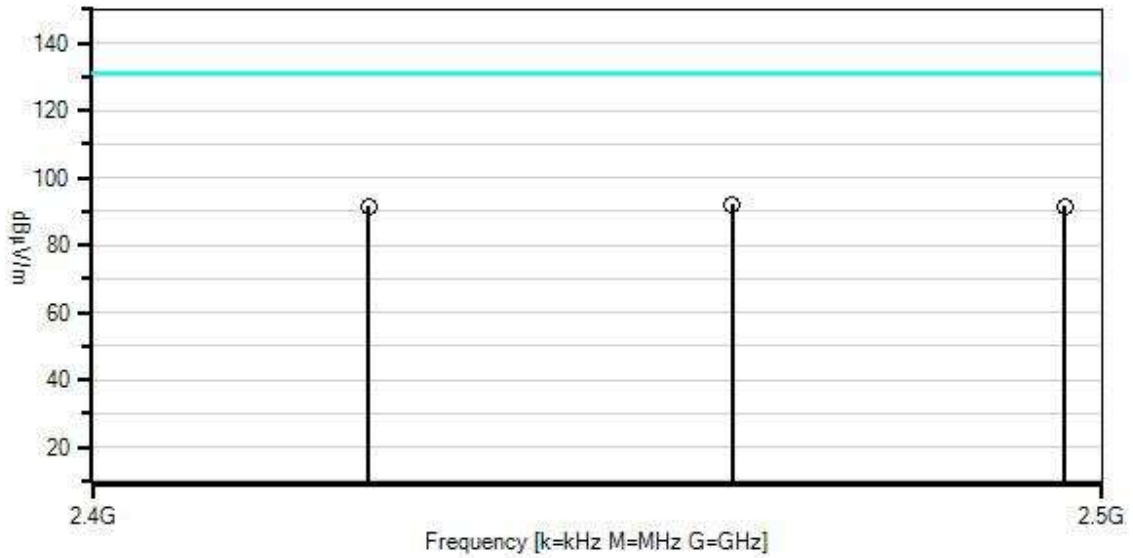

- Readings
  - × QP Readings
  - ▼ Ambient
  - Peak Readings
  - \* Average Readings
- 1 - 15.247(b) Power Output (2400-2483.5 MHz DTS)
- Software Version: 5.03.02

**Test Equipment:**

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
T2	ANP06540	Cable	Heliac	10/29/2015	10/29/2017
T3	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018
T4	AN03540	Preamp	83017A	4/30/2015	4/30/2017
T5	AN01467	Horn Antenna-ANSI C63.5 Calibration	3115	8/12/2015	8/12/2017
T6	ANP06935	Cable	32026-29801-29801-18	3/11/2016	3/11/2018


**Measurement Data:**



Reading listed by margin.

Test Distance: 3 Meters

#	Freq MHz	Rdng dB $\mu$ V	T1 T5 dB	T2 T6 dB	T3 dB	T4 dB	Dist Table	Corr dB $\mu$ V/m	Spec dB $\mu$ V/m	Margin dB	Polar Ant
1	2452.600M	95.1	+0.0 +27.7	+0.6 +0.4	+2.9	-34.5	+0.0	92.2	131.2	-39.0	Vert
2	2480.320M	94.3	+0.0 +27.7	+0.6 +0.4	+2.9	-34.5	+0.0	91.4	131.2	-39.8	Vert
3	2422.600M	94.5	+0.0 +27.7	+0.6 +0.4	+2.8	-34.6	+0.0	91.4	131.2	-39.8	Vert

**Plots**

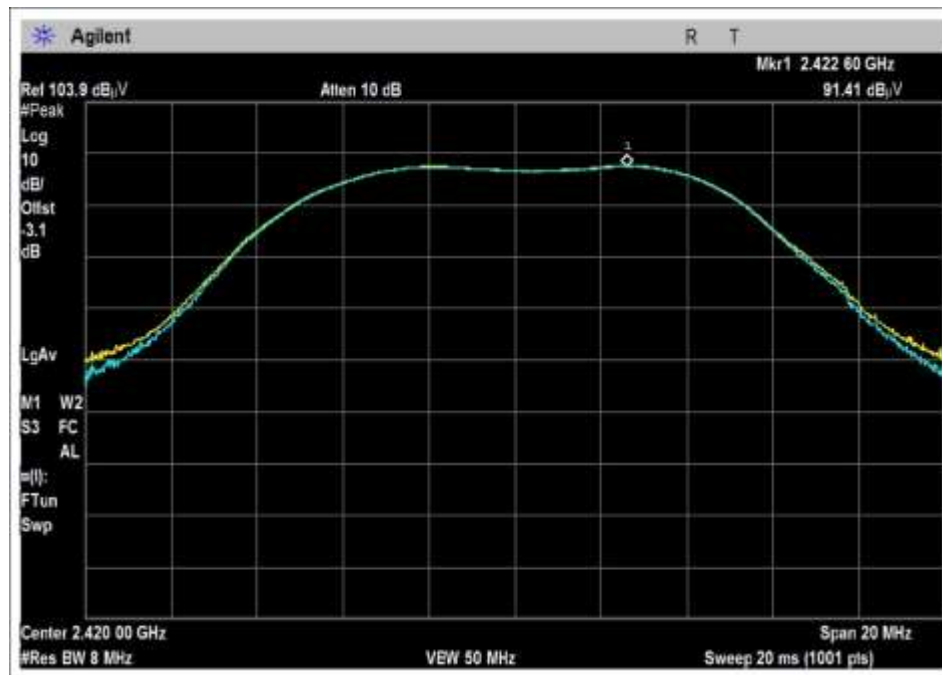

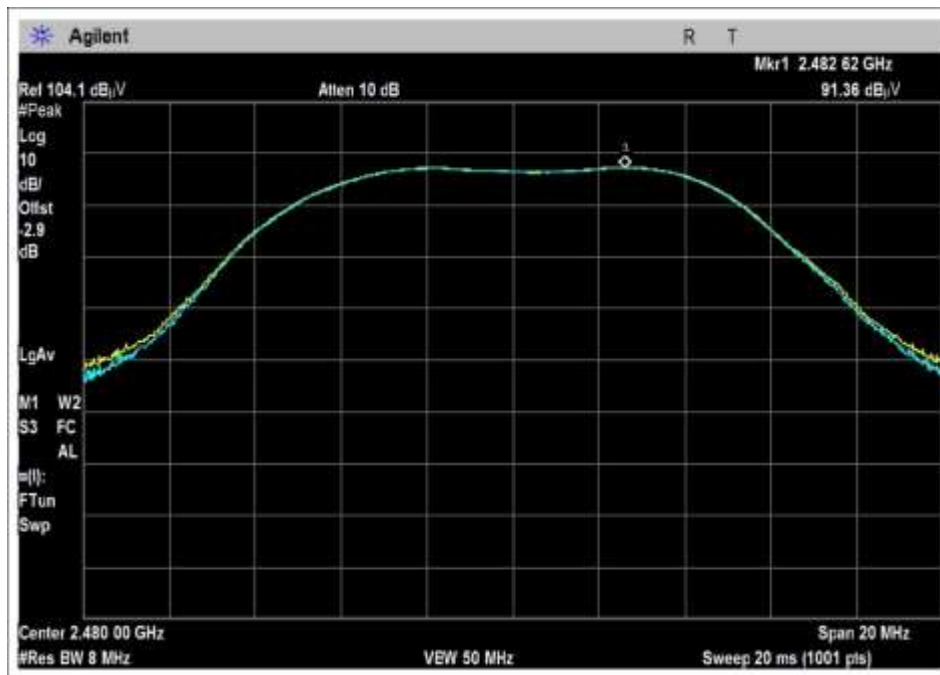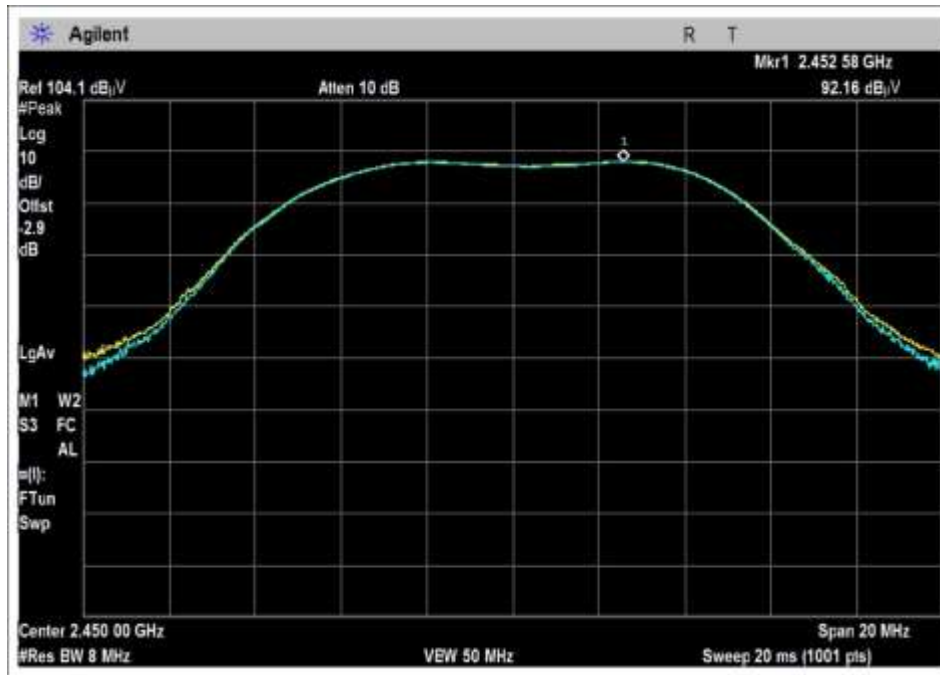



Test Setup Photo(s)



X AXIS



Y AXIS



Z AXIS

## 15.247(e) Power Spectral Density

Test Setup / Conditions / Data			
Test Location:	Bothell Lab C3	Test Engineer:	S. Pittsford
Test Method:	ANSI C63.10 (2013), KDB 558074 D01 DTS Meas Guidance v03r05 (04/08/2016)	Test Date(s):	2/11/2017
Configuration:	2		
Test Setup:	See data sheet.		

Environmental Conditions			
Temperature (°C)	2230	Relative Humidity (%):	

PSD Test Data Summary - Radiated Measurement						
Measurement Method: PKPSD						
Frequency (MHz)	Modulation	Ant. Type / Gain (dBi)	Field Strength (dBuV/m @3m)	Calculated (dBm/3kHz)	Limit (dBm/3kHz)	Results
2420	O-QPSK	Integral 0dBi	73.1	-22.1	≤8	Pass
2450	O-QPSK	Integral 0dBi	75.5	-19.7	≤8	Pass
2480	O-QPSK	Integral 0dBi	74.0	-21.2	≤8	Pass

Conducted RF output power calculated in accordance with ANSI C63.10.

$$P(W) = \frac{(E \cdot d)^2}{30 G}$$

Or equivalently, in logarithmic form:

$$P(dBm) = E(dBuV/m) + 20LOG(d) - G - 104.77$$

**Test Setup / Conditions / Data**

Test Location: CKC Laboratories • 22116 23rd Dr. SE • Bothell, WA 98021 • (425) 402-1717  
 Customer: **Medtronic MiniMed**  
 Specification: **15.247(e) Peak Power Spectral Density (2400-2483.5 MHz DTS)**  
 Work Order #: **99536** Date: 2/11/2017  
 Test Type: **Maximized Emissions** Time: 14:23:22  
 Tested By: Steven Pittsford Sequence#: 2  
 Software: EMITest 5.03.02

***Equipment Tested:***

Device	Manufacturer	Model #	S/N
Configuration 2			

***Support Equipment:***

Device	Manufacturer	Model #	S/N
Configuration 2			


***Test Conditions / Notes:***

Frequency tested: 2420MHz, 2450MHz, 2480MHz  
 Firmware power setting: Max Power  
 EUT Firmware: 6x0G XTest PRM 2.5A(M969745DOC)

Duty Cycle: 100%

Test Mode: Continuously modulated  
 Test Setup: The EUT is set 1.5 meters high on a Styrofoam table. X, Y and Z axis are investigated with the worst case reported.  
 EUT has a fresh battery installed

Medtronic MiniMed WO#: 99536 Sequence#: 2 Date: 2/11/2017  
 15.247(e) Peak Power Spectral Density (2400-2483.5 MHz DTS) Test Distance: 3 Meters Vert

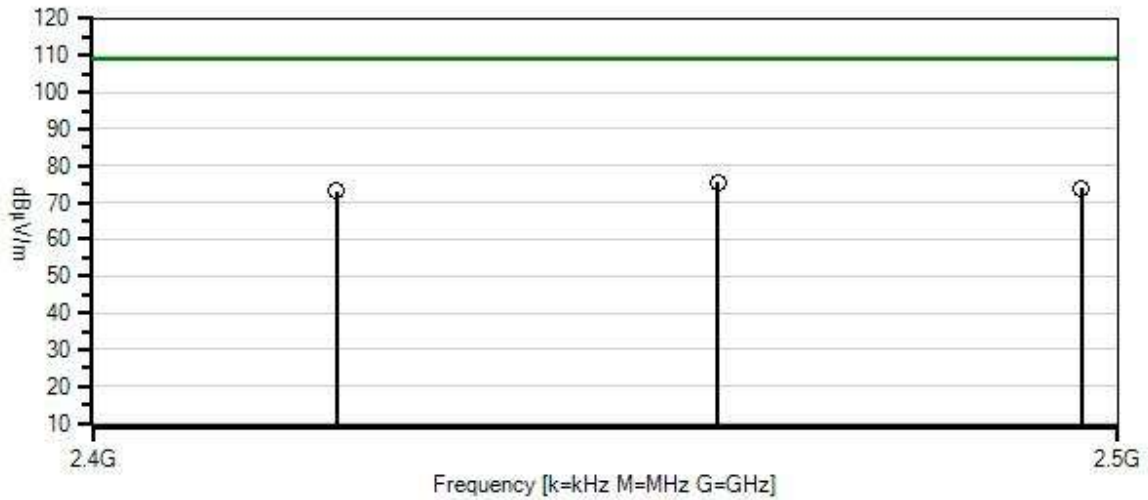

- Readings
- Peak Readings
- × QP Readings
- \* Average Readings
- ▼ Ambient
- Software Version: 5.03.02
- 1 - 15.247(e) Peak Power Spectral Density (2400-2483.5 MHz DTS)

**Test Equipment:**

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
T2	ANP06540	Cable	Heliac	10/29/2015	10/29/2017
T3	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018
T4	AN03540	Preamp	83017A	4/30/2015	4/30/2017
T5	AN01467	Horn Antenna- ANSI C63.5 Calibration	3115	8/12/2015	8/12/2017
T6	ANP06935	Cable	32026-29801- 29801-18	3/11/2016	3/11/2018


**Measurement Data:**


Reading listed by margin.

Test Distance: 3 Meters

#	Freq MHz	Rdng dB $\mu$ V	T1 dB	T2 dB	T3 dB	T4 dB	Dist Table	Corr dB $\mu$ V/m	Spec dB $\mu$ V/m	Margin dB	Polar Ant
1	2450.588M	78.4	+0.0 +27.7	+0.6 +0.4	+2.9	-34.5	+0.0	75.5	109.2	-33.7	Vert
2	2480.465M	76.9	+0.0 +27.7	+0.6 +0.4	+2.9	-34.5	+0.0	74.0	109.2	-35.2	Vert
3	2419.598M	76.2	+0.0 +27.7	+0.6 +0.4	+2.8	-34.6	+0.0	73.1	109.2	-36.1	Vert

Plot Data

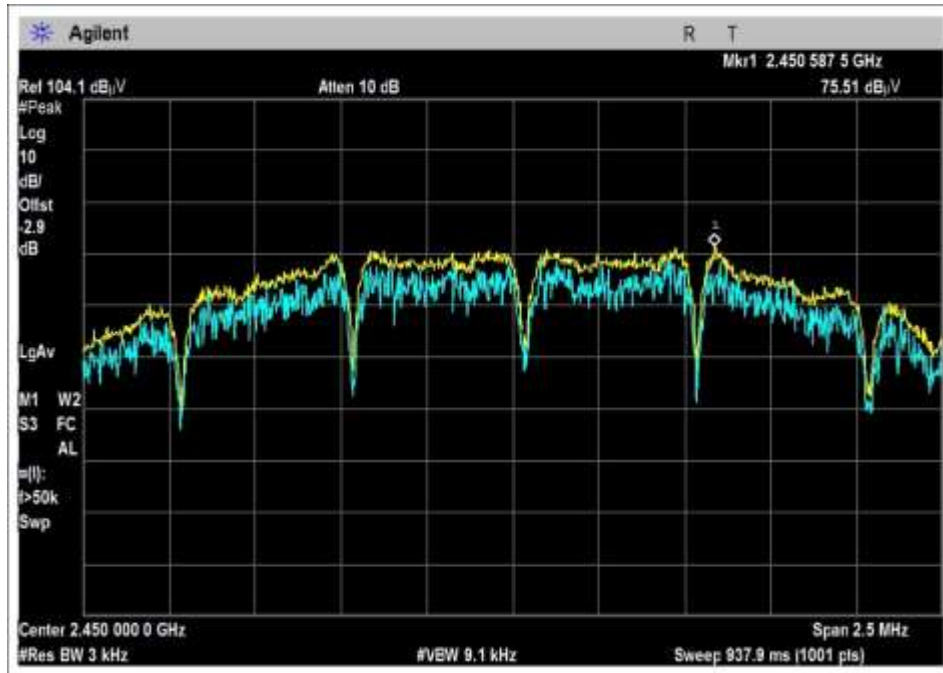

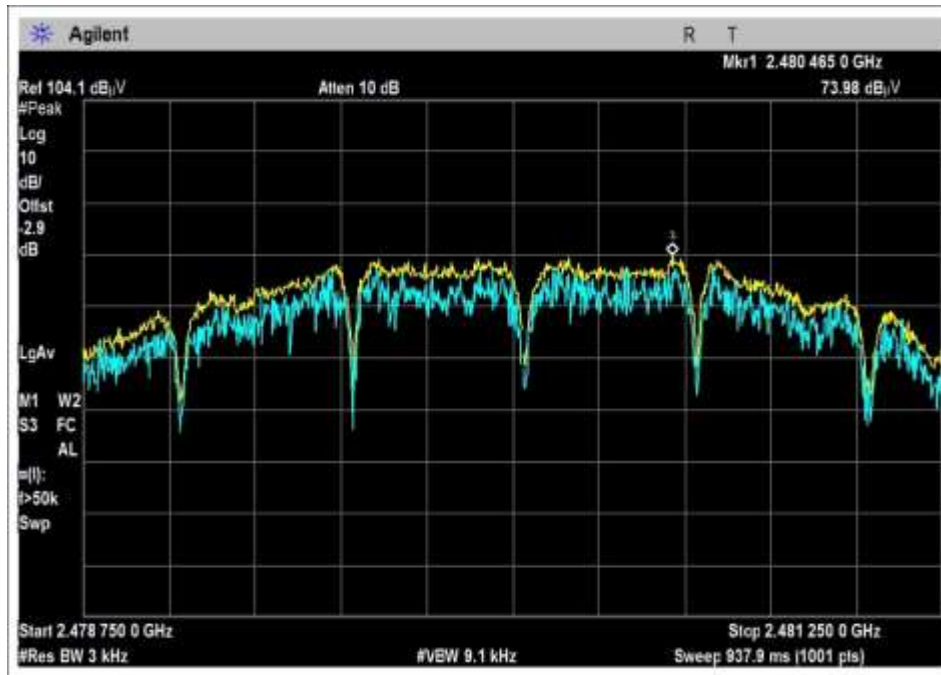

**Test Setup Photo(s)**







X AXIS



Y AXIS



Z AXIS

## 15.247(d) Radiated Emissions & Band Edge

### Test Setup/Conditions

Test Location:	Bothell Lab C3	Test Engineer:	M. Atkinson/S Pittsford
Test Method:	ANSI C63.10 (2013), KDB 558074 D01 DTS Meas Guidance v03r05 (04/08/2016)	Test Date(s):	2/8/2017 to 2/10/2017
Configuration:	1		

### Environmental Conditions

Temperature (°C)	22-23	Relative Humidity (%):	24-30
------------------	-------	------------------------	-------

See data sheets for test setup and test equipment.

### Test Setup / Conditions / Data

Test Location: CKC Laboratories • 22116 23rd Dr. SE • Bothell, WA 98021 • (425) 402-1717  
 Customer: **Medtronic MiniMed**  
 Specification: **15.247(d) / 15.209 Radiated Spurious Emissions**  
 Work Order #: **99536** Date: 2/8/2017  
 Test Type: **Maximized Emissions** Time: 11:22:00  
 Tested By: Michael Atkinson Sequence#: 1  
 Software: EMITest 5.03.02

#### *Equipment Tested:*

Device	Manufacturer	Model #	S/N
Configuration 1			

#### *Support Equipment:*

Device	Manufacturer	Model #	S/N
Configuration 1			

#### *Test Conditions / Notes:*


Frequency Range: 9kHz-1GHz  
 Frequency tested: 2420MHz, 2450MHz, 2480MHz  
 Firmware power setting: Max Power  
 EUT Firmware: 6x0G XTest PRM 2.5A(M969745DOC)

Duty Cycle: 100%

Test Mode: Continuously modulated

Test Setup:  
 The EUT is set 0.8 meters high on a Styrofoam table. X, Y and Z axis are investigated with the worst case reported.  
 EUT has a fresh battery installed

Medtronic MiniMed W/O#: 99536 Sequence#: 1 Date: 2/8/2017  
 15.247(d) / 15.209 Radiated Spurious Emissions Test Distance: 3 Meters Para

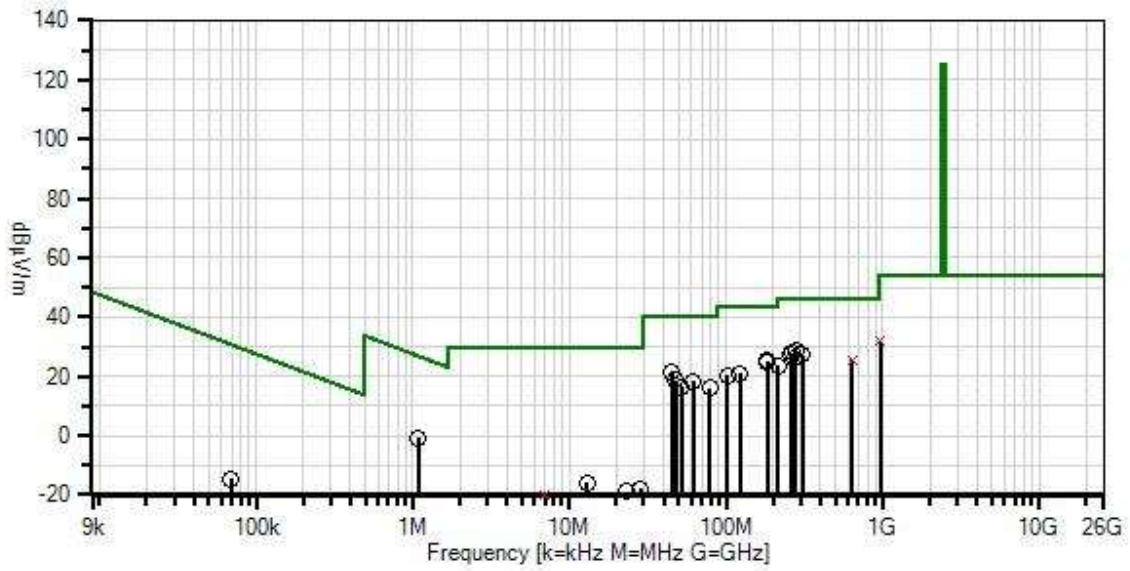

- Readings
  - × QP Readings
  - ▼ Ambient
  - 1 - 15.247(d) / 15.209 Radiated Spurious Emissions
  - Peak Readings
  - \* Average Readings
- Software Version: 5.03.02

**Test Equipment:**

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
T2	ANP06540	Cable	Heliac	10/29/2015	10/29/2017
T3	ANP05963	Cable	RG-214	2/15/2016	2/15/2018
T4	ANP05360	Cable	RG214	11/30/2016	11/30/2018
T5	AN02307	Preamp	8447D	2/15/2016	2/15/2018
T6	AN01991	Biconilog Antenna	CBL6111C	3/11/2016	3/11/2018
T7	ANP05657	Attenuator	PE7004-6	12/22/2015	12/22/2017
T8	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018
T9	AN00052	Loop Antenna	6502	4/8/2016	4/8/2018

**Measurement Data:**

Reading listed by margin.

Test Distance: 3 Meters

#	Freq MHz	Rdng dB $\mu$ V	T1	T2	T3	T4	Dist	Corr	Spec	Margin	Polar	
			T5	T6	T7	T8						
			T9					Table	dB $\mu$ V/m	dB $\mu$ V/m	dB	Ant
			dB	dB	dB	dB						
1	280.300M	33.7	+0.0 -27.0 +0.0	+0.2 +13.0	+1.6 +6.0	+1.0 +0.0	+0.0	28.5	46.0 Z-Axis	-17.5	Horiz	
2	268.600M	33.7	+0.0 -27.0 +0.0	+0.2 +12.7	+1.5 +6.0	+1.0 +0.0	+0.0	28.1	46.0 Z-Axis	-17.9	Horiz	
3	184.200M	35.0	+0.0 -27.3 +0.0	+0.2 +9.1	+1.4 +6.0	+0.8 +0.0	+0.0	25.2	43.5 Z-Axis	-18.3	Horiz	
4	45.005M	31.7	+0.0 -27.9 +0.0	+0.1 +10.8	+0.5 +6.0	+0.4 +0.0	+0.0	21.6	40.0 X-Axis	-18.4	Horiz	
5	260.900M	33.1	+0.0 -27.0 +0.0	+0.2 +12.6	+1.5 +6.0	+1.0 +0.0	+0.0	27.4	46.0 Z-Axis	-18.6	Vert	
6	308.400M	31.7	+0.0 -27.1 +0.0	+0.2 +13.7	+1.6 +6.0	+1.1 +0.0	+0.0	27.2	46.0 Z-Axis	-18.8	Horiz	
7	184.200M	34.3	+0.0 -27.3 +0.0	+0.2 +9.1	+1.4 +6.0	+0.8 +0.0	+0.0	24.5	43.5 Y-Axis	-19.0	Horiz	
8	276.400M	31.7	+0.0 -27.0 +0.0	+0.2 +12.9	+1.6 +6.0	+1.0 +0.0	+0.0	26.4	46.0 Y-Axis	-19.6	Vert	
9	215.300M	32.3	+0.0 -27.2 +0.0	+0.2 +10.0	+1.4 +6.0	+0.9 +0.0	+0.0	23.6	43.5 Z-Axis	-19.9	Horiz	

10	644.000M QP	23.1	+0.0 -28.1 +0.0	+0.3 +20.6	+2.1 +6.0	+1.7 +0.0	+0.0	25.7	46.0 Z-Axis	-20.3	Vert
^	644.000M	28.9	+0.0 -28.1 +0.0	+0.3 +20.6	+2.1 +6.0	+1.7 +0.0	+0.0	31.5	46.0 Z-Axis	-14.5	Vert
12	47.894M	30.0	+0.0 -27.9 +0.0	+0.1 +9.4	+0.6 +6.0	+0.4 +0.0	+0.0	18.6	40.0 X-Axis	-21.4	Vert
13	61.502M	33.1	+0.0 -27.8 +0.0	+0.1 +6.0	+0.7 +6.0	+0.4 +0.0	+0.0	18.5	40.0 X-Axis	-21.5	Vert
14	973.800M QP	22.4	+0.0 -27.1 +0.0	+0.4 +25.5	+2.5 +6.1	+2.2 +0.0	+0.0	32.0	54.0 Z-Axis	-22.0	Horiz
^	973.800M	28.3	+0.0 -27.1 +0.0	+0.4 +25.5	+2.5 +6.1	+2.2 +0.0	+0.0	37.9	54.0 Z-Axis	-16.1	Horiz
16	123.100M	29.0	+0.0 -27.6 +0.0	+0.1 +11.6	+1.2 +6.0	+0.6 +0.0	+0.0	20.9	43.5 Z-Axis	-22.6	Vert
17	102.789M	29.9	+0.0 -27.7 +0.0	+0.1 +10.3	+1.2 +6.0	+0.6 +0.0	+0.0	20.4	43.5 X-Axis	-23.1	Vert
18	52.300M	29.5	+0.0 -27.9 +0.0	+0.1 +7.8	+0.6 +6.0	+0.4 +0.0	+0.0	16.5	40.0 Z-Axis	-23.5	Vert
19	78.744M	29.6	+0.0 -27.8 +0.0	+0.1 +6.9	+0.8 +6.0	+0.5 +0.0	+0.0	16.1	40.0 X-Axis	-23.9	Vert
20	1.089M	29.3	+0.0 +0.0 +9.8	+0.0 +0.0	+0.0 +0.0	+0.0 +0.1	-40.0	-0.8	26.9 Z-Axis	-27.7	Para
21	12.905M	15.3	+0.0 +0.0 +8.8	+0.0 +0.0	+0.0 +0.0	+0.0 +0.2	-40.0	-15.7	29.5 X-Axis	-45.2	Para
22	69.000k	55.3	+0.0 +0.0 +10.2	+0.0 +0.0	+0.0 +0.0	+0.0 +0.0	-80.0	-14.5	30.8 Z-Axis	-45.3	Para
23	28.380M	15.7	+0.0 +0.0 +6.1	+0.0 +0.0	+0.0 +0.0	+0.0 +0.3	-40.0	-17.9	29.5 X-Axis	-47.4	GrdPe
24	23.102M	13.3	+0.0 +0.0 +7.4	+0.0 +0.0	+0.0 +0.0	+0.0 +0.3	-40.0	-19.0	29.5 Y-Axis	-48.5	Perp

25	6.997M	10.7	+0.0	+0.0	+0.0	+0.0	-40.0	-19.9	29.5	-49.4	Para
	QP		+0.0	+0.0	+0.0	+0.1			Z-Axis		
			+9.3								
^	6.997M	17.1	+0.0	+0.0	+0.0	+0.0	-40.0	-13.5	29.5	-43.0	Para
			+0.0	+0.0	+0.0	+0.1			Z-Axis		
			+9.3								
27	28.470M	12.9	+0.0	+0.0	+0.0	+0.0	-40.0	-20.7	29.5	-50.2	Para
			+0.0	+0.0	+0.0	+0.3			Z-Axis		
			+6.1								



Test Location: CKC Laboratories • 22116 23rd Dr SE • Bothell, WA 98021 • (425) 402-1717  
 Customer: **Medtronic MiniMed**  
 Specification: **15.247(d) / 15.209 Radiated Spurious Emissions**  
 Work Order #: **99536** Date: 2/8/2017  
 Test Type: **Radiated Scan** Time: 16:18:18  
 Tested By: Michael Atkinson Sequence#: 3  
 Software: EMITest 5.03.02

**Equipment Tested:**

Device	Manufacturer	Model #	S/N
Configuration 1			

**Support Equipment:**

Device	Manufacturer	Model #	S/N
Configuration 1			

**Test Conditions / Notes:**

Frequency Range: 1-26GHz  
 Frequency tested: 2420MHz, 2450MHz, 2480MHz  
 Firmware power setting: Max Power  
 EUT Firmware: 6x0G XTest PRM 2.5A(M969745DOC)

Duty Cycle: 100%

Test Mode: Continuously modulated

Test Setup:  
 The EUT is set 1.5 meters high on a Styrofoam table. X, Y and Z axis are investigated with the worst case reported.  
 EUT has a fresh battery installed.



Medtronic MiniMed WD#: 99536 Sequence#: 3 Date: 2/8/2017  
 15.247(d) / 15.209 Radiated Spurious Emissions Test Distance: 3 Meters Vert



— Readings  
 × QP Readings  
 ▼ Ambient  
 — 1 - 15.247(d) / 15.209 Radiated Spurious Emissions

○ Peak Readings  
 \* Average Readings  
 Software Version: 5.03.02

**Test Equipment:**

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
T2	ANP06540	Cable	Heliac	10/29/2015	10/29/2017
T3	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018
T4	AN03540	Preamp	83017A	4/30/2015	4/30/2017
T5	AN01467	Horn Antenna-ANSI C63.5 Calibration	3115	8/12/2015	8/12/2017
T6	ANP06935	Cable	32026-29801- 29801-18	3/11/2016	3/11/2018
T7	ANP06678	Cable	32026-29801- 29801-144	9/19/2016	9/19/2018
T8	ANP06957	Cable	32026-29094K- 29094K-72TC	9/19/2016	9/19/2018
T9	AN02742	Active Horn Antenna	AMFW-5F- 18002650-20- 10P	10/7/2016	10/7/2018

**Measurement Data:**

Reading listed by margin.

Test Distance: 3 Meters

#	Freq MHz	Rdng dB $\mu$ V	Reading listed by margin.				Dist Table	Corr dB $\mu$ V/m	Spec dB $\mu$ V/m	Margin dB	Polar Ant
			T1 T5 T9 dB	T2 T6 dB	T3 T7 dB	T4 T8 dB					
1	4899.300M	43.0	+0.0 +32.7 +0.0	+0.9 +0.5	+4.4 +0.0	-34.2 +0.0	+0.0	47.3	54.0 Mid	-6.7	Horiz
2	4959.900M	42.2	+0.0 +32.8 +0.0	+0.9 +0.5	+4.4 +0.0	-34.2 +0.0	+0.0	46.6	54.0 High	-7.4	Horiz
3	7351.100M	38.5	+0.0 +36.2 +0.0	+1.2 +0.6	+4.7 +0.0	-34.6 +0.0	+0.0	46.6	54.0 Mid	-7.4	Horiz
4	7260.600M	38.2	+0.0 +35.9 +0.0	+1.2 +0.6	+4.6 +0.0	-34.5 +0.0	+0.0	46.0	54.0 Low	-8.0	Horiz
5	12398.500 M	32.2	+0.0 +39.5 +0.0	+1.6 +0.9	+6.4 +0.0	-34.7 +0.0	+0.0	45.9	54.0 High	-8.1	Horiz
6	9667.000M	35.3	+0.0 +37.3 +0.0	+1.5 +0.7	+6.1 +0.0	-35.0 +0.0	+0.0	45.9	54.0 Low	-8.1	Horiz
7	7120.000M	38.4	+0.0 +35.4 +0.0	+1.2 +0.7	+4.4 +0.0	-34.4 +0.0	+0.0	45.7	54.0 Low	-8.3	Horiz
8	7438.500M	37.1	+0.0 +36.6 +0.0	+1.3 +0.6	+4.8 +0.0	-34.7 +0.0	+0.0	45.7	54.0 High	-8.3	Horiz
9	4843.000M	41.5	+0.0 +32.7 +0.0	+0.9 +0.5	+4.3 +0.0	-34.2 +0.0	+0.0	45.7	54.0 Low	-8.3	Horiz

10	4899.950M	41.2	+0.0 +32.7 +0.0	+0.9 +0.5 +0.0	+4.4 +0.0	-34.2 +0.0	+0.0	45.5	54.0 Mid	-8.5	Vert
11	4960.150M	40.9	+0.0 +32.8 +0.0	+0.9 +0.5 +0.0	+4.4 +0.0	-34.2 +0.0	+0.0	45.3	54.0 High	-8.7	Vert
12	4839.200M	40.4	+0.0 +32.7 +0.0	+0.9 +0.5 +0.0	+4.3 +0.0	-34.2 +0.0	+0.0	44.6	54.0 Low	-9.4	Vert
13	12100.600 M	31.1	+0.0 +39.3 +0.0	+1.5 +0.8 +0.0	+6.5 +0.0	-34.9 +0.0	+0.0	44.3	54.0 Low	-9.7	Horiz
14	12251.100 M	30.5	+0.0 +39.4 +0.0	+1.5 +0.8 +0.0	+6.6 +0.0	-34.8 +0.0	+0.0	44.0	54.0 Mid	-10.0	Horiz
15	4762.000M	38.9	+0.0 +32.7 +0.0	+0.9 +0.5 +0.0	+4.3 +0.0	-34.2 +0.0	+0.0	43.1	54.0	-10.9	Vert
16	9918.500M	32.3	+0.0 +37.2 +0.0	+1.3 +0.8 +0.0	+6.1 +0.0	-35.2 +0.0	+0.0	42.5	54.0 High	-11.5	Horiz
17	9680.600M	31.6	+0.0 +37.3 +0.0	+1.5 +0.7 +0.0	+6.1 +0.0	-35.0 +0.0	+0.0	42.2	54.0 Low	-11.8	Horiz
18	9801.100M	31.6	+0.0 +37.3 +0.0	+1.4 +0.7 +0.0	+6.1 +0.0	-35.1 +0.0	+0.0	42.0	54.0 Mid	-12.0	Horiz
19	2566.000M	42.3	+0.0 +28.0 +0.0	+0.6 +0.4 +0.0	+2.9 +0.0	-34.5 +0.0	+0.0	39.7	54.0	-14.3	Horiz
20	17151.100 M Ave	19.7	+0.0 +41.8 +0.0	+2.0 +1.0 +0.0	+8.7 +0.0	-34.4 +0.0	+0.0	38.8	54.0 Mid	-15.2	Horiz
^	17151.100 M	29.6	+0.0 +41.8 +0.0	+2.0 +1.0 +0.0	+8.7 +0.0	-34.4 +0.0	+0.0	48.7	54.0 Mid	-5.3	Horiz
22	16940.600 M Ave	20.0	+0.0 +41.3 +0.0	+2.1 +1.0 +0.0	+8.6 +0.0	-34.4 +0.0	+0.0	38.6	54.0 Low	-15.4	Horiz
^	16940.600 M	31.3	+0.0 +41.3 +0.0	+2.1 +1.0 +0.0	+8.6 +0.0	-34.4 +0.0	+0.0	49.9	54.0 Low	-4.1	Horiz

24	17358.500	18.4	+0.0	+2.0	+8.8	-34.5	+0.0	38.0	54.0	-16.0	Horiz
	M		+42.3	+1.0	+0.0	+0.0					
	Ave		+0.0						High		
^	17358.500	29.8	+0.0	+2.0	+8.8	-34.5	+0.0	49.4	54.0	-4.6	Horiz
	M		+42.3	+1.0	+0.0	+0.0					
			+0.0						High		
26	14520.600	21.7	+0.0	+1.8	+7.7	-34.9	+0.0	37.6	54.0	-16.4	Horiz
	M		+40.3	+1.0	+0.0	+0.0					
	Ave		+0.0						Low		
^	14520.600	33.4	+0.0	+1.8	+7.7	-34.9	+0.0	49.3	54.0	-4.7	Horiz
	M		+40.3	+1.0	+0.0	+0.0					
			+0.0						Low		
28	14701.100	22.2	+0.0	+1.8	+7.8	-34.9	+0.0	37.5	54.0	-16.5	Horiz
	M		+39.7	+0.9	+0.0	+0.0					
	Ave		+0.0						Mid		
^	14701.100	32.8	+0.0	+1.8	+7.8	-34.9	+0.0	48.1	54.0	-5.9	Horiz
	M		+39.7	+0.9	+0.0	+0.0					
			+0.0						Mid		
30	14878.557	21.9	+0.0	+1.8	+7.7	-34.9	+0.0	36.4	54.0	-17.6	Horiz
	M		+39.0	+0.9	+0.0	+0.0					
	Ave		+0.0						High		
^	14878.557	35.0	+0.0	+1.8	+7.7	-34.9	+0.0	49.5	54.0	-4.5	Horiz
	M		+39.0	+0.9	+0.0	+0.0					
			+0.0						High		
32	1252.000M	43.3	+0.0	+0.4	+2.1	-36.3	+0.0	34.0	54.0	-20.0	Horiz
			+24.2	+0.3	+0.0	+0.0					
			+0.0								
33	9019.000M	20.8	+0.0	+1.3	+6.0	-34.6	+0.0	32.0	54.0	-22.0	Horiz
	Ave		+37.8	+0.7	+0.0	+0.0			Low		
			+0.0								
^	9019.000M	36.9	+0.0	+1.3	+6.0	-34.6	+0.0	48.1	54.0	-5.9	Horiz
			+37.8	+0.7	+0.0	+0.0			Low		
			+0.0								
35	24200.000	25.6	+0.0	+0.0	+0.0	+0.0	+0.0	26.2	54.0	-27.8	Vert
	M		+0.0	+0.0	+8.5	+4.5					
	Ave		-12.4								
^	24200.000	38.2	+0.0	+0.0	+0.0	+0.0	+0.0	38.8	54.0	-15.2	Vert
	M		+0.0	+0.0	+8.5	+4.5					
			-12.4								
37	24500.000	25.1	+0.0	+0.0	+0.0	+0.0	+0.0	26.0	54.0	-28.0	Vert
	M		+0.0	+0.0	+8.6	+4.5					
	Ave		-12.2								
^	24500.000	38.5	+0.0	+0.0	+0.0	+0.0	+0.0	39.4	54.0	-14.6	Vert
	M		+0.0	+0.0	+8.6	+4.5					
			-12.2								
39	24800.000	24.0	+0.0	+0.0	+0.0	+0.0	+0.0	25.3	54.0	-28.7	Vert
	M		+0.0	+0.0	+8.6	+4.6					
	Ave		-11.9								
^	24800.000	37.2	+0.0	+0.0	+0.0	+0.0	+0.0	38.5	54.0	-15.5	Vert
	M		+0.0	+0.0	+8.6	+4.6					
			-11.9								

**Band Edge**

**Band Edge Summary**

Frequency (MHz)	Modulation	Ant. Type	Field Strength (dBuV/m @3m)	Limit (dBuV/m @3m)	Results
2390.0	O-QPSK	Integral 0dBi	26.1 (Ave)	<54	Pass
2390.0	O-QPSK	Integral 0dBi	38.9 (Peak)	<74	Pass
2400.0	O-QPSK	Integral 0dBi	27.0 (Ave)	<54	Pass
2400.0	O-QPSK	Integral 0dBi	39.9 (Peak)	<74	Pass
2483.5	O-QPSK	Integral 0dBi	48.8 (Ave)	<54	Pass
2483.5	O-QPSK	Integral 0dBi	59.3 (peak)	<74	Pass

**Test Setup / Conditions / Data**

Test Location: CKC Laboratories • 22116 23rd Dr. SE • Bothell, WA 98021 • (425) 402-1717  
 Customer: **Medtronic MiniMed**  
 Specification: **15.247(d) / 15.209 Radiated Spurious Emissions**  
 Work Order #: **99536** Date: 2/8/2017  
 Test Type: **Maximized Emissions** Time: 15:08:37  
 Tested By: Michael Atkinson Sequence#: 2  
 Software: EMITest 5.03.02

**Equipment Tested:**

Device	Manufacturer	Model #	S/N
Configuration 1			

**Support Equipment:**

Device	Manufacturer	Model #	S/N
Configuration 1			

**Test Conditions / Notes:**

Frequency tested: 2420MHz, 2480MHz  
 Firmware power setting: Max Power  
 EUT Firmware: 6x0G XTest PRM 2.5A(M969745DOC)

Duty Cycle: 100%

Test Mode: Continuously modulated

Test Setup:  
 The EUT is set 1.5 meters high on a Styrofoam table. X, Y and Z axis are investigated with the worst case reported.

Medtronic MiniMed W/O#: 99536 Sequence#: 2 Date: 2/8/2017  
15.247(d) / 15.209 Radiated Spurious Emissions Test Distance: 3 Meters Horiz



- Readings
- × QP Readings
- ▼ Ambient
- 1 - 15.247(d) / 15.209 Radiated Spurious Emissions

- Peak Readings
  - \* Average Readings
- Software Version: 5.03.02

**Test Equipment:**

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
T2	ANP06540	Cable	Heliac	10/29/2015	10/29/2017
	ANP05963	Cable	RG-214	2/15/2016	2/15/2018
	ANP05360	Cable	RG214	11/30/2016	11/30/2018
	AN02307	Preamp	8447D	2/15/2016	2/15/2018
	AN01991	Biconilog Antenna	CBL6111C	3/11/2016	3/11/2018
	ANP05657	Attenuator	PE7004-6	12/22/2015	12/22/2017
T3	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018
	AN00052	Loop Antenna	6502	4/8/2016	4/8/2018
T4	AN03540	Preamp	83017A	4/30/2015	4/30/2017
T5	AN01467	Horn Antenna-	3115	8/12/2015	8/12/2017
		ANSI C63.5 Calibration			
T6	ANP06935	Cable	32026-29801- 29801-18	3/11/2016	3/11/2018



**Measurement Data:**

Reading listed by margin.



Test Distance: 3 Meters


#	Freq MHz	Rdng dB $\mu$ V	T1 T5 dB	T2 T6 dB	T3 dB	T4 dB	Dist Table	Corr dB $\mu$ V/m	Spec dB $\mu$ V/m	Margin dB	Polar Ant
1	2483.500M	51.7	+0.0	+0.6	+2.9	-34.5	+0.0	48.8	54.0	-5.2	Horiz
	Ave		+27.7	+0.4							
^	2483.500M	62.2	+0.0	+0.6	+2.9	-34.5	+0.0	59.3	54.0	+5.3	Horiz
			+27.7	+0.4							
3	2400.000M	30.1	+0.0	+0.6	+2.8	-34.6	+0.0	27.0	54.0	-27.0	Horiz
	Ave		+27.7	+0.4							
^	2400.000M	43.0	+0.0	+0.6	+2.8	-34.6	+0.0	39.9	54.0	-14.1	Horiz
			+27.7	+0.4							
5	2390.000M	29.2	+0.0	+0.6	+2.8	-34.6	+0.0	26.1	54.0	-27.9	Horiz
	Ave		+27.7	+0.4							
^	2390.000M	42.0	+0.0	+0.6	+2.8	-34.6	+0.0	38.9	54.0	-15.1	Horiz
			+27.7	+0.4							
7	2655.000M	28.0	+0.0	+0.7	+3.0	-34.5	+0.0	26.0	54.0	-28.0	Horiz
	Ave		+28.4	+0.4							
^	2655.000M	40.3	+0.0	+0.7	+3.0	-34.5	+0.0	38.3	54.0	-15.7	Horiz
			+28.4	+0.4							

## Band Edge Plots

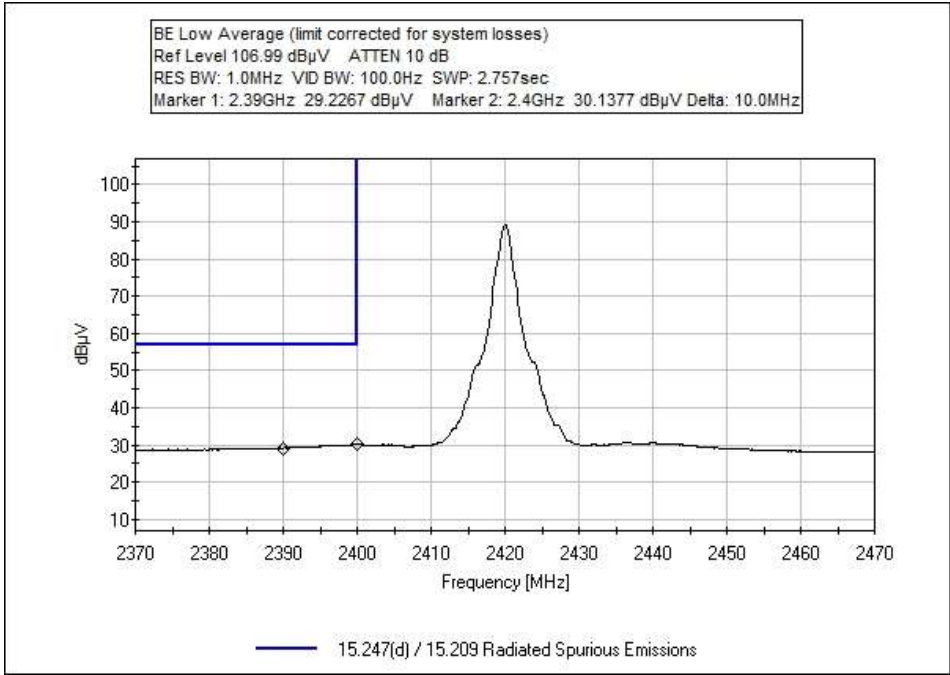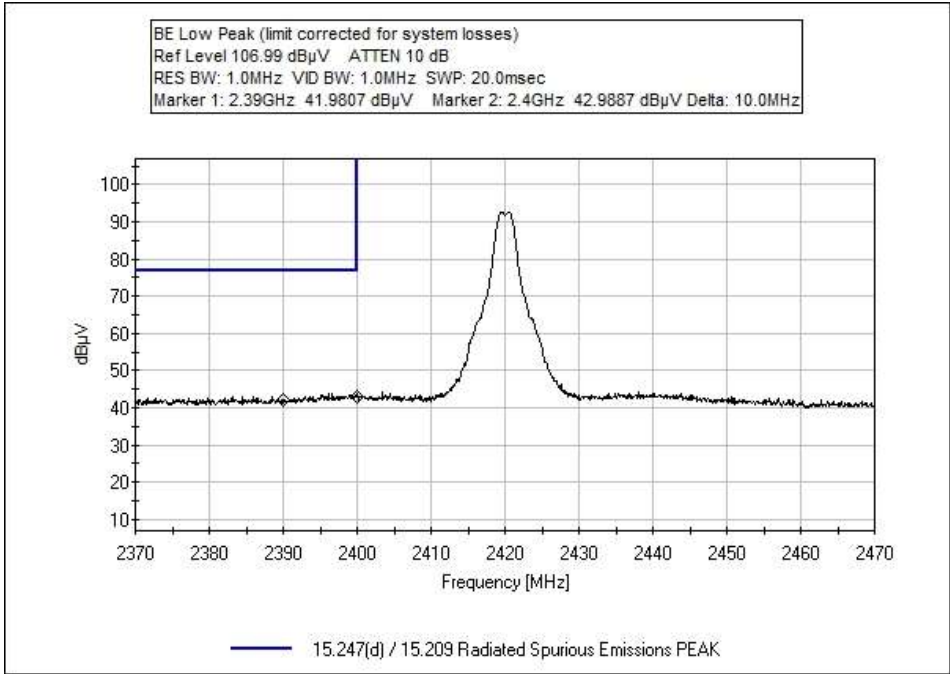



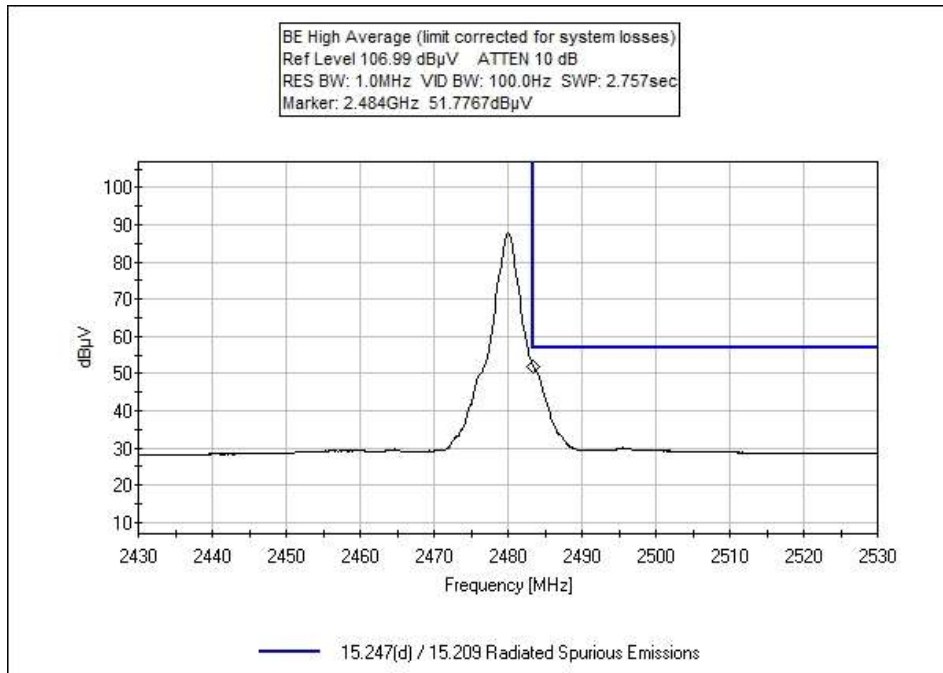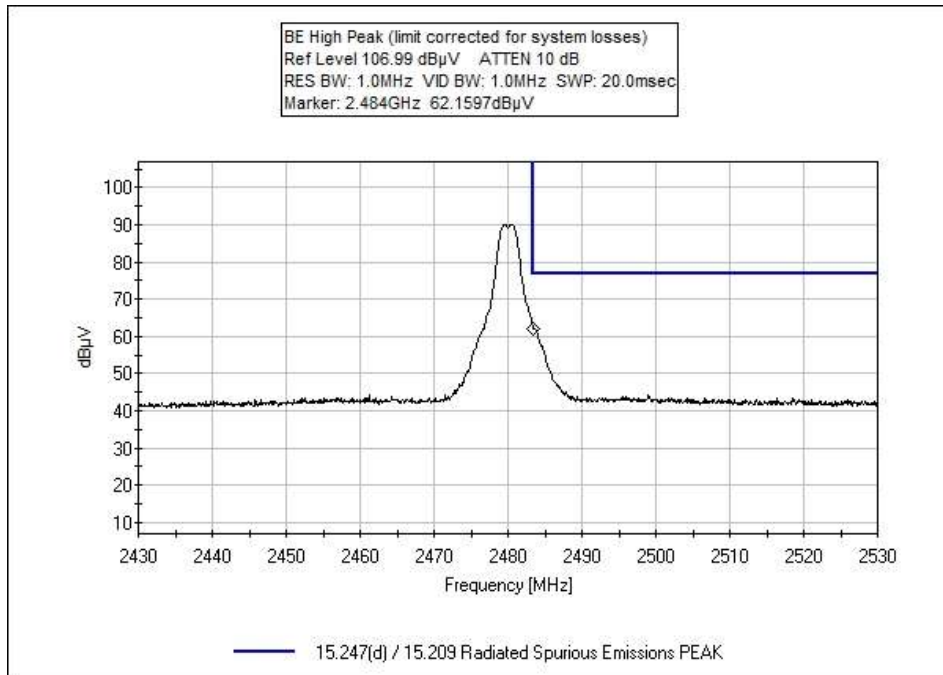

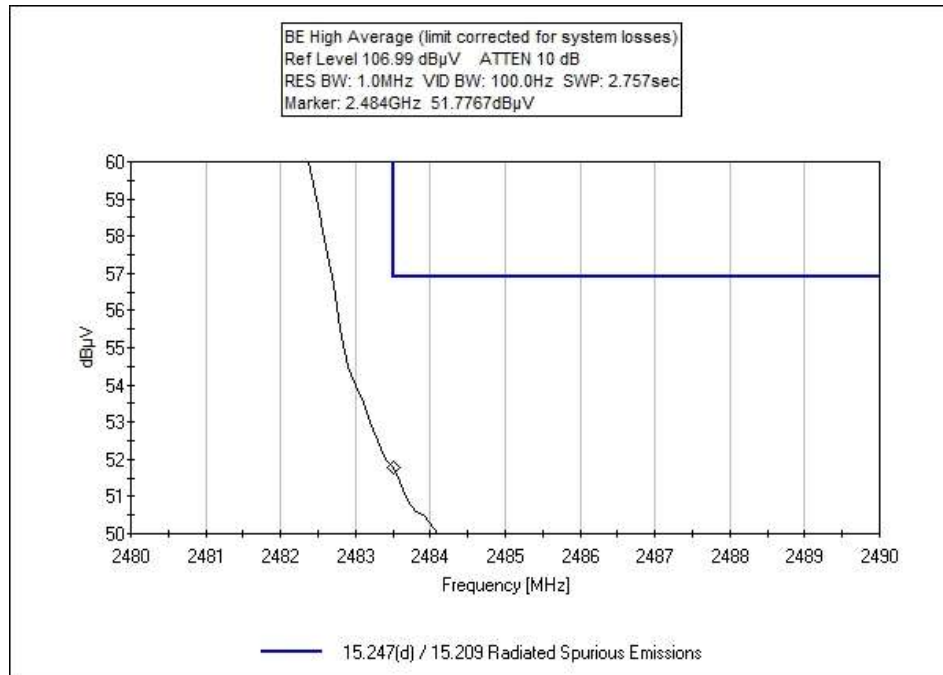

Test Setup Photo(s)



9KHz – 1GHz



1-26GHz



X AXIS



Y AXIS



Z AXIS

# SUPPLEMENTAL INFORMATION

## Measurement Uncertainty

Uncertainty Value	Parameter
4.73 dB	Radiated Emissions
3.34 dB	Mains Conducted Emissions
3.30 dB	Disturbance Power

Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k=2. Compliance is deemed to occur provided measurements are below the specified limits.

## Emissions Test Details

**TESTING PARAMETERS**

Unless otherwise indicated, the following configuration parameters are used for equipment setup: The cables were routed consistent with the typical application by varying the configuration of the test sample. Interface cables were connected to the available ports of the test unit. The effect of varying the position of the cables was investigated to find the configuration that produced maximum emissions. Cables were of the type and length specified in the individual requirements. The length of cable that produced maximum emissions was selected.

The equipment under test (EUT) was set up in a manner that represented its normal use, as shown in the setup photographs. Any special conditions required for the EUT to operate normally are identified in the comments that accompany the emissions tables.

The emissions data was taken with a spectrum analyzer or receiver. Incorporating the applicable correction factors for distance, antenna, cable loss and amplifier gain, the data was reduced as shown in the table below. The corrected data was then compared to the applicable emission limits. Preliminary and final measurements were taken in order to ensure that all emissions from the EUT were found and maximized.

**CORRECTION FACTORS**

The basic spectrum analyzer reading was converted using correction factors as shown in the highest emissions readings in the tables. For radiated emissions in dBμV/m, the spectrum analyzer reading in dBμV was corrected by using the following formula. This reading was then compared to the applicable specification limit. Individual measurements were compared with the displayed limit value in the margin column. The margin was calculated based on subtracting the limit value from the corrected measurement value; a positive margin represents a measurement exceeding the limit, while a negative margin represents a measurement less than the limit.

SAMPLE CALCULATIONS		
	Meter reading	(dBμV)
+	Antenna Factor	(dB/m)
+	Cable Loss	(dB)
-	Distance Correction	(dB)
-	Preamplifier Gain	(dB)
=	Corrected Reading	(dBμV/m)

**TEST INSTRUMENTATION AND ANALYZER SETTINGS**

The test instrumentation and equipment listed were used to collect the emissions data. A spectrum analyzer or receiver was used for all measurements. Unless otherwise specified, the following table shows the measuring equipment bandwidth settings that were used in designated frequency bands. For testing emissions, an appropriate reference level and a vertical scale size of 10 dB per division were used.

MEASURING EQUIPMENT BANDWIDTH SETTINGS PER FREQUENCY RANGE			
TEST	BEGINNING FREQUENCY	ENDING FREQUENCY	BANDWIDTH SETTING
CONDUCTED EMISSIONS	150 kHz	30 MHz	9 kHz
RADIATED EMISSIONS	9 kHz	150 kHz	200 Hz
RADIATED EMISSIONS	150 kHz	30 MHz	9 kHz
RADIATED EMISSIONS	30 MHz	1000 MHz	120 kHz
RADIATED EMISSIONS	1000 MHz	>1 GHz	1 MHz

**SPECTRUM ANALYZER/RECEIVER DETECTOR FUNCTIONS**

The notes that accompany the measurements contained in the emissions tables indicate the type of detector function used to obtain the given readings. Unless otherwise noted, all readings were made in the "positive peak" detector mode. Whenever a "quasi-peak" or "average" reading was recorded, the measurement was annotated with a "QP" or an "Ave" on the appropriate rows of the data sheets. In cases where quasi-peak or average limits were employed and data exists for multiple measurement types for the same frequency then the peak measurement was retained in the report for reference, however the numbering for the affected row was removed and an arrow or caret ("^") was placed in the far left-hand column indicating that the row above takes precedence for comparison to the limit. The following paragraphs describe in more detail the detector functions and when they were used to obtain the emissions data.

**Peak**

In this mode, the spectrum analyzer or receiver recorded all emissions at their peak value as the frequency band selected was scanned. By combining this function with another feature called "peak hold," the measurement device had the ability to measure intermittent or low duty cycle transient emission peak levels. In this mode, the measuring device made a slow scan across the frequency band selected and measured the peak emission value found at each frequency across the band.

**Quasi-Peak**

Quasi-peak measurements were taken using the quasi-peak detector when the true peak values exceeded or were within 2 dB of a quasi-peak specification limit. Additional QP measurements may have been taken at the discretion of the operator.

**Average**

Average measurements were taken using the average detector when the true peak values exceeded or were within 2 dB of an average specification limit. Additional average measurements may have been taken at the discretion of the operator. If the specification or test procedure requires trace averaging, then the averaging was performed using 100 samples or as required by the specification. All other average measurements are performed using video bandwidth averaging. To make these measurements, the test engineer reduces the video bandwidth on the measuring device until the modulation of the signal is filtered out. At this point the measuring device is set into the linear mode and the scan time is reduced.