



TESTING
CERT #803.01, 803.02, 803.05, 803.06

ADDENDUM TO MEDTRONIC MINIMED TEST REPORT FC09-003
FOR THE
MY SENTRY MONITOR, MMT-9101
FCC PART 15 SUBPART C SECTIONS 15.207, 15.209, 15.247, 15.249
& RSS-210 ISSUE 7
TESTING

DATE OF ISSUE: MARCH 25, 2009

PREPARED FOR:

Medtronic MiniMed
18000 Devonshire Street
Northridge, CA 91325-1219

PREPARED BY:

Mary Ellen Clayton
CKC Laboratories, Inc.
5046 Sierra Pines Drive
Mariposa, CA 95338

W.O. No.: 88416

Date of test: December 8-15, 2008

Report No.: FC09-003A

This report contains a total of 43 pages and may be reproduced in full only. Partial reproduction may only be done with the written consent of CKC Laboratories, Inc. The results in this report apply only to the items tested, as identified herein.

TABLE OF CONTENTS

Administrative Information	3
Approvals	3
Site File Registration Numbers	3
Summary of Results	4
Conditions During Testing.....	4
FCC 15.31(e) Voltage Variation.....	5
FCC 15.31(m) Number Of Channels	5
FCC 15.33(a) Frequency Ranges Tested	5
FCC 15.203 Antenna Requirements	5
EUT Operating Frequency	5
Equipment Under Test (EUT) Description	6
Equipment Under Test	6
Peripheral Devices	6
Report of Emissions Measurements.....	7
Testing Parameters.....	7
FCC 15.207 AC Conducted Emissions.....	9
FCC 15.247(b)(3) RF Power Output	16
FCC 15.247(d) OATS Radiated Spurious Emissions	18
FCC Part 15.247 Band Edge.....	21
FCC Part 15.247 Peak Power Spectral Density	24
FCC 15.249(a) RF Power Output	26
FCC 15.249(d) OATS Radiated Spurious Emissions	28
FCC Part 15.249 Block Edge.....	31
RSS-210 Occupied Bandwidth	34
Appendix A: Customer Information	38

ADMINISTRATIVE INFORMATION

DATE OF TEST: December 8-15, 2008

DATE OF RECEIPT: December 8, 2008

REPRESENTATIVE: Bob Vitti

MANUFACTURER:
Medtronic MiniMed
18000 Devonshire Street
Northridge, CA 91325-1219

TEST LOCATION:
CKC Laboratories, Inc.
5046 Sierra Pines Drive
Mariposa, CA 95338

TEST METHOD: ANSI C63.4 (2003), RSS-210 Issue 7 and RSS GEN Issue 2

PURPOSE OF TEST:

Original Report: To perform the testing of the My Sentry Monitor, MMT-9101 with the requirements for FCC Part 15 Subpart C Sections 15.207, 15.209, 15.247, 15.249 & RSS-210 devices.

Addendum A: To correct the low frequency stated in the test conditions, remove the duplicate 15.209 section, remove 15.247(e) plots, provide a new bandedge low channel plot, add clarification on the bandedge plots, fix the polarization on the RF power data sheet, and provide tables instead of tabular data for the peak power spectral density and RF power output data.

APPROVALS

QUALITY ASSURANCE:

TEST PERSONNEL:

Steve Behm, Director of Engineering Services



Mike Wilkinson, Senior EMC Engineer/Lab Manager

SITE FILE REGISTRATION NUMBERS

Location	Japan	Canada	FCC
Mariposa D	R-1827, C-1960 & T-276	3082A-2	784962

SUMMARY OF RESULTS

Test	Specification	Results
Conducted Emissions	FCC Part 15 Subpart C Section 15.207	Pass
Radiated Emissions	FCC Part 15 Subpart C Section 15.209	Pass
RF Output Power	FCC Part 15 Subpart C Sections 15.247(b)(3) & 15.249(a)	Pass
OATS Radiated Spurious Emissions	FCC Part 15 Subpart C Section 15.247(d) & 15.249(d)	Pass
Band Edge	FCC Part 15 Subpart C Section 15.247	Pass
Peak Power Spectral Density	FCC Part 15 Subpart C Section 15.247(e)	Pass
Block Edge	FCC Part 15 Subpart C Section 15.249	Pass
Occupied Bandwidth	RSS-210 Issue 7 and RSS GEN Issue 2	Pass

CONDITIONS DURING TESTING

No modifications to the EUT were necessary during testing.

FCC 15.31(e) Voltage Variations

FCC 15.31e was satisfied by measurement of the radiated signal level of the fundamental frequency component of the emission was performed with the supply voltage varied between 85% and 115% of the nominal rated supply voltage and no change was observed.

FCC 15.31(m) Number Of Channels

This device was tested on three channels.

FCC 15.33(a) Frequency Ranges Tested

15.207 Conducted Emissions: 150 kHz – 30 MHz

15.209/15.247 Radiated Emissions: 9 kHz – 10 GHz

FCC 15.203 Antenna Requirements

The antenna is an integral part of the EUT and is non-removable; therefore the EUT complies with Section 15.203 of the FCC rules.

EUT Operating Frequency

The EUT was operating at Zigbee 2400-2483.5 MHz Band and 916.5 MHz.

EQUIPMENT UNDER TEST (EUT) DESCRIPTION

The customer declares the EUT tested by CKC Laboratories was representative of a production unit.

EQUIPMENT UNDER TEST

My Sentry Monitor

Manuf: Medtronic MiniMed
Model: MMT-9101
Serial: M000102F

My Sentry Monitor Power Supply

Manuf: Specter Power
Model: AMDD-20050-2000
Serial: NA

PERIPHERAL DEVICES

The EUT was tested with the following peripheral device(s):

Remote Comlink

Manuf: Medtronic MiniMed
Model: MMT-7304NA
Serial: AB1907

Remote Computer

Manuf: Premio
Model: Premio Tower
Serial: CKC asset 1820

REPORT OF EMISSIONS MEASUREMENTS

TESTING PARAMETERS

TEMPERATURE AND HUMIDITY DURING TESTING

The temperature during testing was within +15°C and + 35°C.

The relative humidity was between 20% and 75%.

The cables were routed consistent with the typical application by varying the configuration of the test sample. Interface cables were connected to the available ports of the test unit. The effect of varying the position of the cables was investigated to find the configuration that produced maximum emissions. Cables were of the type and length specified in the individual requirements. The length of cable that produced maximum emissions was selected.

The equipment under test (EUT) was set up in a manner that represented its normal use, as shown in the setup photographs. Any special conditions required for the EUT to operate normally are identified in the comments that accompany the emissions tables.

The emissions data was taken with a spectrum analyzer or receiver. Incorporating the applicable correction factors for distance, antenna, cable loss and amplifier gain, the data was reduced as shown in the table below. The corrected data was then compared to the applicable emission limits. Preliminary and final measurements were taken in order to ensure that all emissions from the EUT were found and maximized.

CORRECTION FACTORS

The basic spectrum analyzer reading was converted using correction factors as shown in the highest emissions readings in the tables. For radiated emissions in dB μ V/m, the spectrum analyzer reading in dB μ V was corrected by using the following formula. This reading was then compared to the applicable specification limit.

SAMPLE CALCULATIONS		
	Meter reading	(dB μ V)
+	Antenna Factor	(dB)
+	Cable Loss	(dB)
-	Distance Correction	(dB)
-	Preamplifier Gain	(dB)
=	Corrected Reading	(dB μ V/m)

TEST INSTRUMENTATION AND ANALYZER SETTINGS

The test instrumentation and equipment listed were used to collect the emissions data. A spectrum analyzer or receiver was used for all measurements. The following table shows the measuring equipment bandwidth settings that were used in designated frequency bands. For testing emissions, an appropriate reference level and a vertical scale size of 10 dB per division were used. When conducted emissions testing was performed, a 10 dB external attenuator was used with internal offset correction in the analyzer.

SPECTRUM ANALYZER/RECEIVER DETECTOR FUNCTIONS

The notes that accompany the measurements contained in the emissions tables indicate the type of detector function used to obtain the given readings. Unless otherwise noted, all readings were made in the "Peak" mode. Whenever a "Quasi-Peak" or "Average" reading is listed as one of the highest readings, this is indicated as a "QP" or an "Ave" on the appropriate rows of the data sheets. The following paragraphs describe in more detail the detector functions and when they were used to obtain the emissions data.

Peak

In this mode, the spectrum analyzer/receiver readings were recorded all emissions at their peak value as the frequency band selected was scanned. By combining this function with another feature of the measuring device called "peak hold," the measuring device had the ability to measure transients or low duty cycle transient emission peak levels. In this mode the measuring device made a slow scan across the frequency band selected and measured the peak emission value found at each frequency across the band.

Quasi-Peak

When the true peak values exceeded or were within 2 dB of the specification limit, quasi-peak measurements were taken using the quasi-peak detector.

Average

For certain frequencies, average measurements may be made using the spectrum analyzer/receiver. To make these measurements, the test engineer reduces the video bandwidth on the measuring device until the modulation of the signal is filtered out. At this point the measuring device is set into the linear mode and the scan time is reduced.

FCC 15.207 AC CONDUCTED EMISSIONS

Test Setup Photos



Test Data Sheets

Test Location: CKC Laboratories, Inc. • 5046 Sierra Pines Dr. • Mariposa, CA 95338 • 209 966-5240

Customer: **Medtronic MiniMed**

Specification: **FCC 15.207 - AVE**

Work Order #: **88416**

Date: 12/15/2008

Test Type: **Conducted Emissions**

Time: 14:22:32

Equipment: **My Sentry Monitor**

Sequence#: 11

Manufacturer: Medtronic MiniMed

Tested By: Mike Wilkinson

Model: MMT-9101

120V 60Hz

S/N: M000102F

Test Equipment:

Function	S/N	Calibration Date	Cal Due Date	Asset #
Agilent E4446A SA	US44300407	01/03/2007	01/03/2009	02660
150kHz HP Filter TTE	G7754	01/22/2008	01/22/2010	02608
Site D Conducted Cable	N/A	03/06/2008	03/06/2010	CAB-SITE INT LISN 100k-30M
LISN, 8028-50-TS-24-BNC	8379276, 280	05/07/2007	05/07/2009	1248 & 1249

Equipment Under Test (* = EUT):

Function	Manufacturer	Model #	S/N
My Sentry Monitor*	Medtronic MiniMed	MMT-9101	M000102F
My Sentry Monitor Power Supply	Specter Power	AMDD-20050-2000	None

Support Devices:

Function	Manufacturer	Model #	S/N
----------	--------------	---------	-----

Test Conditions / Notes:

Standard used was FCC 15.207. EUT is set to transmit on Zigbee 2400-2483.5 MHz Band and 916.5 MHz. Frequency range investigated was: 150 kHz to 30 MHz. The temperature was 22°C and the humidity was 48%. RBW = 9 kHz 150 kHz-30 MHz.

Transducer Legend:

T1=CAB-SITED INT LISN 100k-30M	T2=Filter 150kHz HP AN02608
T3=LISN -280 - BK-AN1248	

Measurement Data:

Reading listed by margin.


Test Lead: Black

#	Freq MHz	Rdng dB μ V	T1 dB	T2 dB	T3 dB	dB	Dist Table	Corr dB μ V	Spec dB μ V	Margin dB	Polar Ant
1	1.613M	30.3	+11.5	+0.2	+0.2		+0.0	42.2	46.0	-3.8	Black
2	877.205k	29.8	+11.8	+0.3	+0.2		+0.0	42.1	46.0	-3.9	Black
3	1.507M	30.1	+11.6	+0.2	+0.2		+0.0	42.1	46.0	-3.9	Black
4	2.497M	30.2	+11.3	+0.1	+0.3		+0.0	41.9	46.0	-4.1	Black
5	1.362M	29.7	+11.6	+0.2	+0.2		+0.0	41.7	46.0	-4.3	Black

6	630.683k	29.0	+11.8	+0.3	+0.2	+0.0	41.3	46.0	-4.7	Black
7	867.025k	28.9	+11.8	+0.3	+0.2	+0.0	41.2	46.0	-4.8	Black
8	1.864M	29.2	+11.5	+0.2	+0.2	+0.0	41.1	46.0	-4.9	Black
9	1.762M	28.9	+11.5	+0.2	+0.2	+0.0	40.8	46.0	-5.2	Black
10	2.838M	29.0	+11.2	+0.1	+0.3	+0.0	40.6	46.0	-5.4	Black
11	3.012M	28.6	+11.2	+0.1	+0.3	+0.0	40.2	46.0	-5.8	Black
12	2.323M	28.2	+11.3	+0.2	+0.2	+0.0	39.9	46.0	-6.1	Black
13	1.251M	27.5	+11.7	+0.2	+0.2	+0.0	39.6	46.0	-6.4	Black
14	1.987M	27.6	+11.4	+0.2	+0.2	+0.0	39.4	46.0	-6.6	Black
15	608.140k	26.5	+11.8	+0.3	+0.2	+0.0	38.8	46.0	-7.2	Black
16	857.571k	26.5	+11.8	+0.3	+0.2	+0.0	38.8	46.0	-7.2	Black
17	744.855k	25.9	+11.8	+0.3	+0.2	+0.0	38.2	46.0	-7.8	Black
18	1.005M	25.7	+11.8	+0.2	+0.2	+0.0	37.9	46.0	-8.1	Black
19	3.531M	26.3	+11.1	+0.1	+0.3	+0.0	37.8	46.0	-8.2	Black
20	379.797k	27.4	+12.0	+0.2	+0.2	+0.0	39.8	48.3	-8.5	Black
21	2.242M	25.7	+11.3	+0.2	+0.2	+0.0	37.4	46.0	-8.6	Black
22	2.825M	25.8	+11.2	+0.1	+0.3	+0.0	37.4	46.0	-8.6	Black
23	3.284M	25.8	+11.1	+0.1	+0.3	+0.0	37.3	46.0	-8.7	Black
24	1.468M	18.6	+11.6	+0.2	+0.2	+0.0	30.6	46.0	-15.4	Black
	Ave									
^	1.468M	35.4	+11.6	+0.2	+0.2	+0.0	47.4	46.0	+1.4	Black
26	1.137M	17.3	+11.7	+0.2	+0.2	+0.0	29.4	46.0	-16.6	Black
	Ave									
^	1.137M	34.3	+11.7	+0.2	+0.2	+0.0	46.4	46.0	+0.4	Black

28	1.728M	16.5	+11.5	+0.2	+0.2	+0.0	28.4	46.0	-17.6	Black
Ave										
^	1.728M	34.5	+11.5	+0.2	+0.2	+0.0	46.4	46.0	+0.4	Black
30	2.472M	10.4	+11.3	+0.1	+0.3	+0.0	22.1	46.0	-23.9	Black
Ave										
^	2.472M	32.1	+11.3	+0.1	+0.3	+0.0	43.8	46.0	-2.2	Black

CKC Laboratories, Inc. Date: 12/15/2008 Time: 14:22:32 Medtronic MiniMed W/O#: 884416
 FCC 15.207 - AVE Test Lead: Black 120V 60Hz Sequence#: 11 Ext ATTN: (EXTATTN)

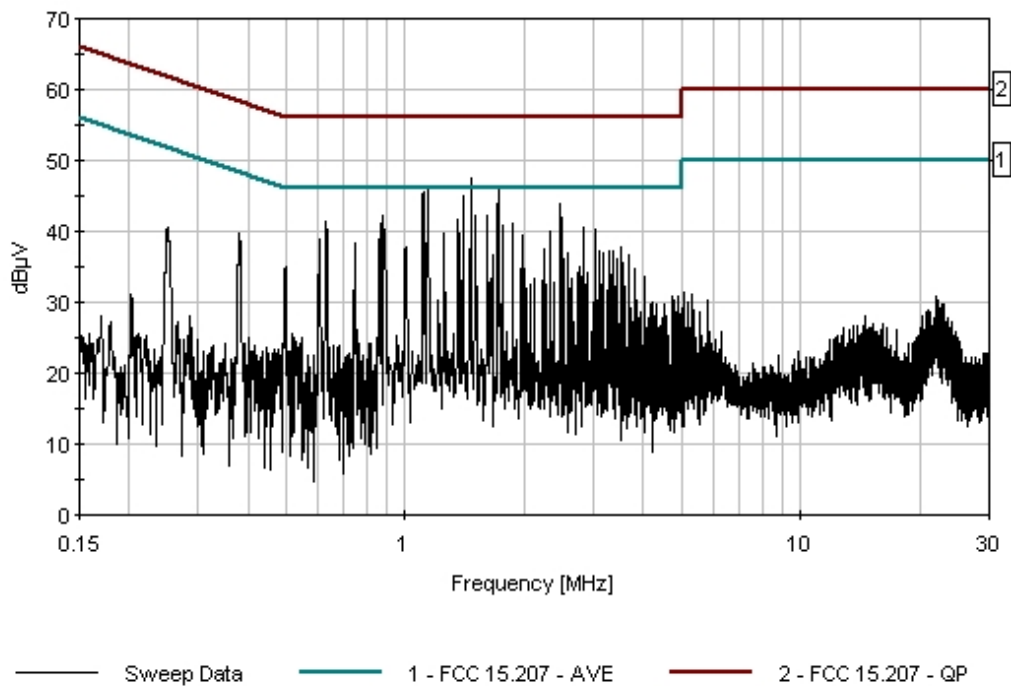

Test Location: CKC Laboratories, Inc. • 5046 Sierra Pines Dr. • Mariposa, CA 95338 • 209 966-5240

Customer: **Medtronic MiniMed**
 Specification: **FCC 15.207 - AVE**
 Work Order #: **88416**
 Test Type: **Conducted Emissions**
 Equipment: **My Sentry Monitor**
 Manufacturer: **Medtronic MiniMed**
 Model: **MMT-9101**
 S/N: **M000102F**

Date: 12/15/2008
 Time: 14:26:26
 Sequence#: 12
 Tested By: Mike Wilkinson
 120V 60Hz

Test Equipment:

Function	S/N	Calibration Date	Cal Due Date	Asset #
Agilent E4446A SA	US44300407	01/03/2007	01/03/2009	02660
150kHz HP Filter TTE	G7754	01/22/2008	01/22/2010	02608
Site D Conducted Cable	N/A	03/06/2008	03/06/2010	CAB-SITE INT LISN 100k-30M
LISN, 8028-50-TS-24-BNC	8379276, 280	05/07/2007	05/07/2009	1248 & 1249

Equipment Under Test (* = EUT):

Function	Manufacturer	Model #	S/N
My Sentry Monitor*	Medtronic MiniMed	MMT-9101	M000102F
My Sentry Monitor Power Supply	Specter Power	AMDD-20050-2000	None

Support Devices:

Function	Manufacturer	Model #	S/N
----------	--------------	---------	-----

Test Conditions / Notes:

Standard used was FCC 15.207. EUT is set to transmit on Zigbee 2400-2483.5 MHz Band and 916.5 MHz. Frequency range investigated was: 150 kHz to 30 MHz. The temperature was 22°C and the humidity was 48%. RBW = 9 kHz 150 kHz-30 MHz.

Transducer Legend:

T1=CAB-SITED INT LISN 100k-30M	T2=Filter 150kHz HP AN02608
T3=LISN -276 - WT-AN01248	

Measurement Data:

Reading listed by margin.


Test Lead: White

#	Freq MHz	Rdng dB μ V	T1 dB	T2 dB	T3 dB	Dist dB	Table	Corr dB μ V	Spec dB μ V	Margin dB	Polar Ant
1	626.319k	31.3	+11.8	+0.3	+0.1	+0.0		43.5	46.0	-2.5	White
2	1.383M	31.3	+11.6	+0.2	+0.2	+0.0		43.3	46.0	-2.7	White
3	877.205k	30.5	+11.8	+0.3	+0.2	+0.0		42.8	46.0	-3.2	White
4	2.485M	31.1	+11.3	+0.1	+0.3	+0.0		42.8	46.0	-3.2	White
5	1.494M	30.6	+11.6	+0.2	+0.2	+0.0		42.6	46.0	-3.4	White
6	1.638M	30.6	+11.5	+0.2	+0.2	+0.0		42.5	46.0	-3.5	White

7	605.230k	30.2	+11.8	+0.3	+0.1	+0.0	42.4	46.0	-3.6	White
8	1.851M	30.2	+11.5	+0.2	+0.2	+0.0	42.1	46.0	-3.9	White
9	2.999M	30.5	+11.2	+0.1	+0.3	+0.0	42.1	46.0	-3.9	White
10	865.570k	29.7	+11.8	+0.3	+0.2	+0.0	42.0	46.0	-4.0	White
11	1.349M	29.9	+11.6	+0.2	+0.2	+0.0	41.9	46.0	-4.1	White
12	2.302M	29.8	+11.3	+0.2	+0.2	+0.0	41.5	46.0	-4.5	White
13	1.745M	29.4	+11.5	+0.2	+0.2	+0.0	41.3	46.0	-4.7	White
14	1.970M	28.2	+11.4	+0.2	+0.2	+0.0	40.0	46.0	-6.0	White
15	1.243M	27.5	+11.7	+0.2	+0.2	+0.0	39.6	46.0	-6.4	White
16	3.012M	28.0	+11.2	+0.1	+0.3	+0.0	39.6	46.0	-6.4	White
17	3.157M	27.7	+11.2	+0.1	+0.3	+0.0	39.3	46.0	-6.7	White
18	2.566M	27.2	+11.3	+0.1	+0.3	+0.0	38.9	46.0	-7.1	White
19	741.945k	26.4	+11.8	+0.3	+0.1	+0.0	38.6	46.0	-7.4	White
20	1.953M	26.8	+11.4	+0.2	+0.2	+0.0	38.6	46.0	-7.4	White
21	852.480k	26.2	+11.8	+0.3	+0.2	+0.0	38.5	46.0	-7.5	White
22	2.740M	26.8	+11.2	+0.1	+0.3	+0.0	38.4	46.0	-7.6	White
23	3.263M	26.9	+11.1	+0.1	+0.3	+0.0	38.4	46.0	-7.6	White
24	3.335M	26.6	+11.1	+0.1	+0.3	+0.0	38.1	46.0	-7.9	White
25	1.120M	21.0	+11.7	+0.2	+0.2	+0.0	33.1	46.0	-12.9	White
	Ave									
^	1.120M	34.4	+11.7	+0.2	+0.2	+0.0	46.5	46.0	+0.5	White
27	1.451M	18.8	+11.6	+0.2	+0.2	+0.0	30.8	46.0	-15.2	White
	Ave									
^	1.451M	35.3	+11.6	+0.2	+0.2	+0.0	47.3	46.0	+1.3	White

29	1.711M	17.7	+11.5	+0.2	+0.2	+0.0	29.6	46.0	-16.4	White
Ave										
^	1.711M	35.5	+11.5	+0.2	+0.2	+0.0	47.4	46.0	+1.4	White
31	2.455M	10.0	+11.3	+0.1	+0.3	+0.0	21.7	46.0	-24.3	White
Ave										
^	2.455M	33.0	+11.3	+0.1	+0.3	+0.0	44.7	46.0	-1.3	White

CKC Laboratories, Inc. Date: 12/15/2008 Time: 14:26:26 Medtronic MiniMed WO#: 884416
 FCC 15.207 - AVE Test Lead: White 120V 60Hz Sequence#: 12 Ext ATTN: (EXTATTN)

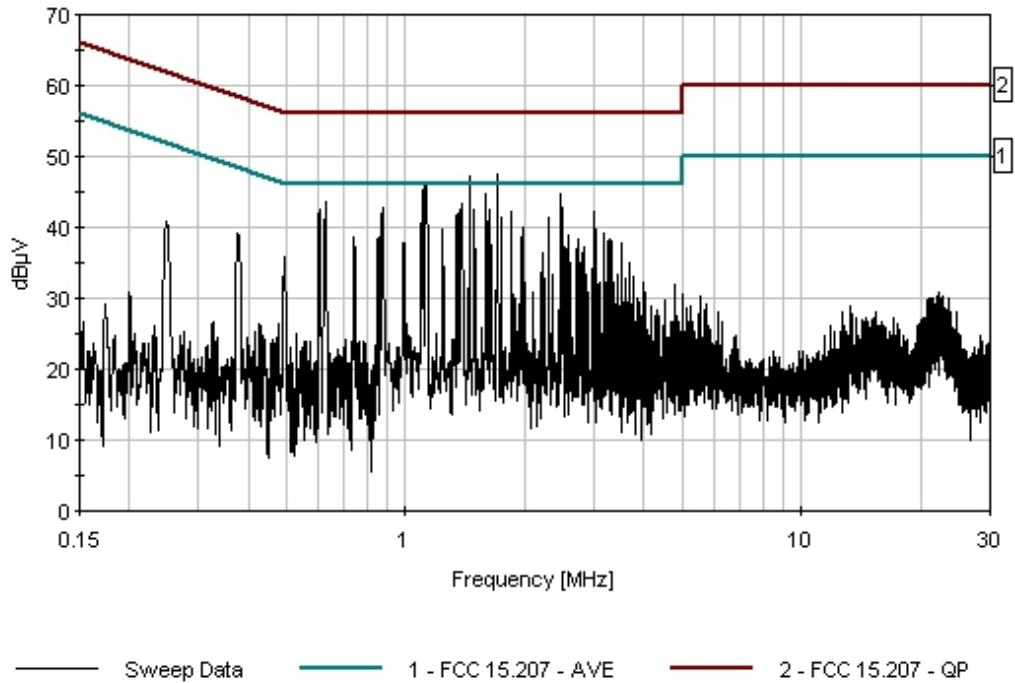

FCC 15.247(b)(3) RF POWER OUTPUT

Test Setup Photos



Test Data Sheet

Test Location: CKC Laboratories, Inc. • 5046 Sierra Pines Dr. • Mariposa, CA 95338 • 209 966-5240

Customer: **Medtronic MiniMed**

Specification: **15.247(b)(3)**

Work Order #: **884416**

Date: 12/9/2008

Test Type: **Maximized Emissions**

Time: 11:39:47

Equipment: **My Sentry Monitor**

Sequence#: 3

Manufacturer: Medtronic MiniMed

Tested By: Mike Wilkinson

Model: MMT9101

S/N: M000102F

Test Equipment:

Function	S/N	Calibration Date	Cal Due Date	Asset #
Agilent E4446A SA	US44300407	01/03/2007	01/03/2009	02660
Chase CBL6111C Bilog	2456	12/30/2006	12/30/2008	01991
EMCO 3115 Horn Antenna	9307-4085	03/17/2007	03/17/2009	00656
HP 8447D Preamp	1937A02604	03/14/2007	03/14/2009	00099
HP 8449B Preamp	3008A00301	12/13/2006	12/13/2008	2010
3M SITE CABLE 20GHZ	NA	03/06/2008	03/06/2010	SITED3M1
Cable 2' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03008
Cable 3' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03012
Cable 12' 40 GHz Astrolab	NA	07/03/2008	07/03/2010	AN05769
EMCO Loop Antenna	1074	05/01/2007	05/01/2009	00226

Equipment Under Test (* = EUT):

Function	Manufacturer	Model #	S/N
My Sentry Monitor*	Medtronic MiniMed	MMT9101	M000102F
My Sentry Monitor Power Supply	Specter Power	AMDD-20050-2000	None

Support Devices:

Function	Manufacturer	Model #	S/N
----------	--------------	---------	-----

Test Conditions / Notes:

Standard used was FCC 15.247. EUT is set to transmit continuously on Zigbee 2400-2483.5 MHz Band Low, Mid and High channels as indicated in the data sheet. Low Channel = 2405 MHz, Mid Channel = 2440 MHz, High Channel = 2475 MHz. Frequency range investigated was: Carrier. The temperature was 22°C and the humidity was 48%. RBW = 10 MHz . VBW = 3 x RBW.

Power Output

Frequency (MHz)	Field Strength (dBuV/m @3m)	Power (dBm)	Limit (dBm)	Comments
2405	116.4	19.076	30	Pass
2440	114.0	16.676	30	Pass
2475	111.1	13.776	30	Pass

Antenna gain used for calculation is 2.1 dBi.

Power formula used in accordance with KDB 558074

FCC 15.247(d) OATS RADIATED SPURIOUS EMISSIONS

Test Setup Photos



Test Data Sheets

Test Location: CKC Laboratories, Inc. • 5046 Sierra Pines Dr. • Mariposa, CA 95338 • 209 966-5240

Customer: **Medtronic MiniMed**
 Specification: **FCC 15.247 (d) / 15.209 / 15.205**
 Work Order #: **88416** Date: 12/10/2008
 Test Type: **Maximized Emissions** Time: 11:45:32
 Equipment: **My Sentry Monitor** Sequence#: 5
 Manufacturer: Medtronic MiniMed Tested By: Mike Wilkinson
 Model: MMT-9101
 S/N: M000102F

Test Equipment:

Function	S/N	Calibration Date	Cal Due Date	Asset #
Agilent E4446A SA	US44300407	01/03/2007	01/03/2009	02660
Chase CBL6111C Bilog	2456	12/30/2006	12/30/2008	01991
EMCO 3115 Horn Antenna	9307-4085	03/17/2007	03/17/2009	00656
HP 8447D Preamp	2727A05444	06/20/2008	06/20/2010	00062
Cable, HF	1067016	04/23/2007	04/23/2009	P04290
HP 8449B Preamp	3008A00301	12/13/2006	12/13/2008	2010
3M SITE CABLE 20GHZ	NA	03/06/2008	03/06/2010	SITED3M1
Cable 2' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03008
Cable 12' 40 GHz Astrolab	NA	07/03/2008	07/03/2010	AN05769
Cable 3' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03012
EMCO Loop Antenna	1074	05/01/2007	05/01/2009	00226
3.6 GHz HP Filter	None	05/15/2007	05/15/2009	01440

Equipment Under Test (* = EUT):

Function	Manufacturer	Model #	S/N
My Sentry Monitor*	Medtronic MiniMed	MMT-9101	M000102F
My Sentry Monitor Power	Specter Power	AMDD-20050-2000	None
Supply			

Support Devices:

Function	Manufacturer	Model #	S/N

Test Conditions / Notes:

Standard used was FCC 15.249, 15.209 and 15.205. EUT is set to transmit continuously on Zigbee 2400-2483.5 MHz Band Low, Mid and High channels as indicated in the data sheet. Low Channel = 2405 MHz, Mid Channel = 2440 MHz, High Channel = 2475 MHz. Frequency range investigated was: 9 kHz to 10 GHz. The temperature was 22°C and the humidity was 48%. RBW = 200 Hz 9 kHz-150kHz. RBW = 9 kHz 150 kHz-30 MHz RBW = 120 kHz 30-1000 MHz RBW = 1MHz 1000-10000 MHz VBW = 3 x RBW. Averaged measurements above 1.0 GHz include a 15.9 dB pulse modulation correction factor. See appendix in report for formula rationale.

Packet Width = 4ms

Total retries = 4

Duty Cycle = (4) * (4ms) / (100ms) = 0.16 * 100% = 16 % duty cycle

Correction factor = 20 log (16/100) = -15.92 dB.

Transducer Legend:

T1=Amp HF - AN02010	T2=ANT AN00656 900MHz-18.5GHz
T3=CAB-SITED3M1 9k - 20G	T4=CAB-AN05769-40GHZ-12FT
T5=CAB-AN03008-40GHZ-2FT	T6=CAB-AN03012-40GHZ-3FT
T7=FIL-AN01440-051407-3.5GHZ HP	T8=15.9dB dB15.35 Duty Cycle Correction

Measurement Data:

Reading listed by margin.

Test Distance: 3 Meters

#	Freq	Rdng	T1	T2	T3	T4	Dist	Corr	Spec	Margin	Polar
	MHz	dB μ V	T5	T6	T7	T8	Table	dB μ V/m	dB μ V/m	dB	Ant
1	4810.960M	52.4	-33.9	+32.5	+7.4	+3.0	+0.0	47.4	54.0	-6.6	Vert
	Ave		+0.6	+0.8	+0.5	-15.9			Low Channel		
^	4810.960M	61.2	-33.9	+32.5	+7.4	+3.0	+0.0	72.1	54.0	+18.1	Vert
			+0.6	+0.8	+0.5				Low Channel		
3	4878.940M	50.4	-34.1	+32.6	+7.4	+3.0	+0.0	45.3	54.0	-8.7	Vert
	Ave		+0.6	+0.8	+0.5	-15.9			Mid Channel		
^	4878.940M	57.3	-34.1	+32.6	+7.4	+3.0	+0.0	68.1	54.0	+14.1	Vert
			+0.6	+0.8	+0.5				Mid Channel		
5	4950.940M	48.2	-34.0	+32.7	+7.3	+3.1	+0.0	43.4	54.0	-10.6	Vert
	Ave		+0.6	+0.8	+0.6	-15.9			High Channel		
^	4950.940M	55.4	-34.0	+32.7	+7.3	+3.1	+0.0	66.5	54.0	+12.5	Vert
			+0.6	+0.8	+0.6	+0.0			High Channel		

FCC PART 15.247 BAND EDGE

Test Equipment

Function	S/N	Calibration Date	Cal Due Date	Asset #
Agilent E4446A SA	US44300407	01/03/2007	01/03/2009	02660
Cable, HF	1067016	04/23/2007	04/23/2009	P04290
Amp HF - S/N 301	3008A00301	11/13/2008	11/13/2010	02010
Antenna, Horn	4085	03/19/2007	03/19/2009	00656
Site D Rad Emiss-10m	N/A	03/06/2008	03/06/2010	CAB-SITED10M-9k-1G
3M SITE CABLE 20GHZ	NA	03/06/2008	03/06/2010	SITED3M1
Cable 2' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03008
Cable 12' 40 GHz Astrolab	NA	07/03/2008	07/03/2010	AN05769
Cable 3' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03012

Test Conditions

EUT is set to transmit continuously on Zigbee 2400-2483.5 MHz Band.


Test Setup Photos






Test Plots

FCC 15.247 BAND EDGE LOW CHANNEL

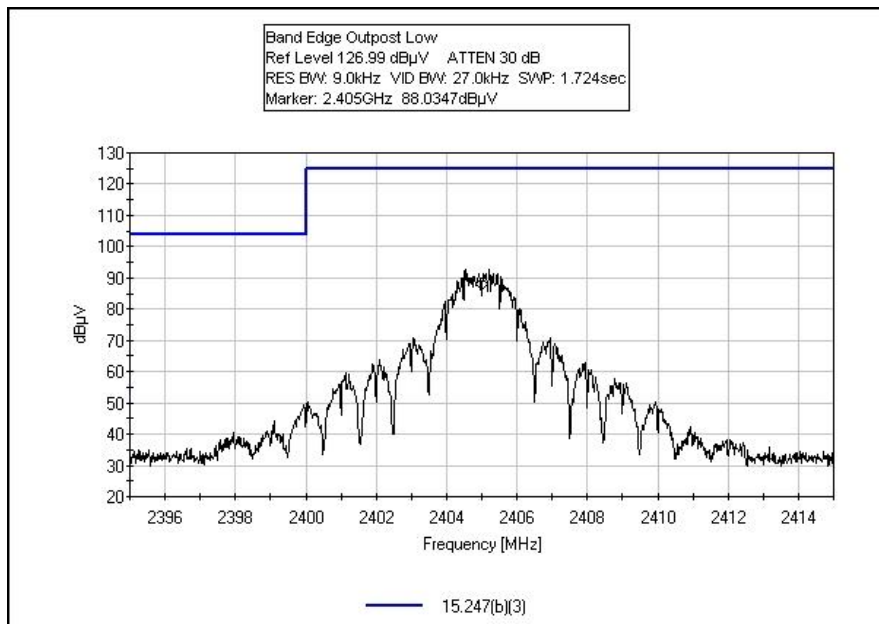

Note: Marker Delta Method used and includes the offset.

FCC 15.247 BAND EDGE HIGH CHANNEL

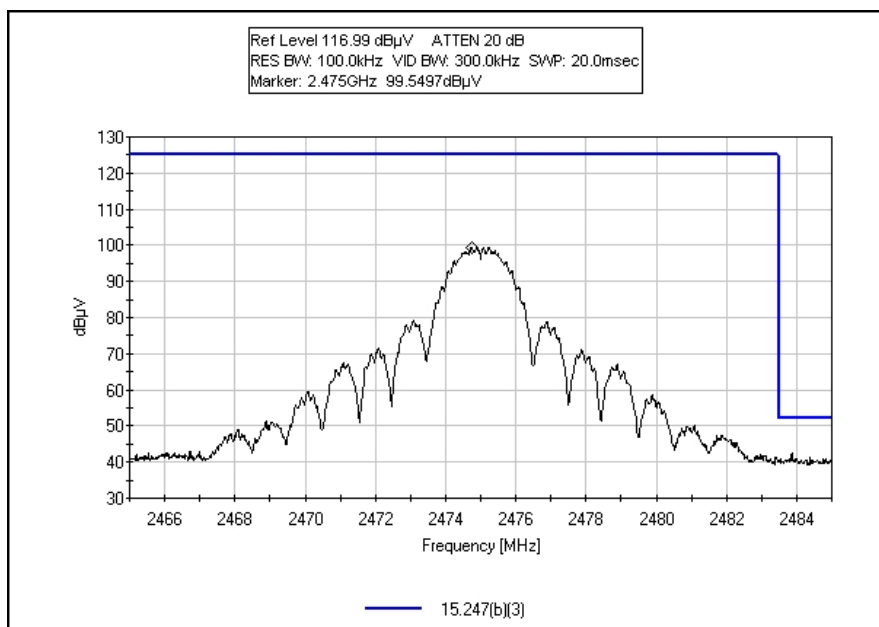

Note: Marker Delta Method used and includes the offset.

FCC PART 15.247 PEAK POWER SPECTRAL DENSITY

Test Setup Photos



Test Data Sheet

Test Location: CKC Laboratories, Inc. • 5046 Sierra Pines Dr. • Mariposa, CA 95338 • 209 966-5240

Customer: **Medtronic MiniMed**

Specification: **15.247(e)**

Work Order #: **884416**

Date: 12/9/2008

Test Type: **Maximized Emissions**

Time: 13:51:34

Equipment: **My Sentry Monitor**

Sequence#: 4

Manufacturer: Medtronic MiniMed

Tested By: Mike Wilkinson

Model: MMT9101

S/N: M000102F

Test Equipment:

Function	S/N	Calibration Date	Cal Due Date	Asset #
Agilent E4446A SA	US44300407	01/03/2007	01/03/2009	02660
Chase CBL6111C Bilog	2456	12/30/2006	12/30/2008	01991
EMCO 3115 Horn Antenna	9307-4085	03/17/2007	03/17/2009	00656
HP 8447D Preamp	1937A02604	03/14/2007	03/14/2009	00099
HP 8449B Preamp	3008A00301	12/13/2006	12/13/2008	2010
3M SITE CABLE 20GHZ	NA	03/06/2008	03/06/2010	SITED3M1
Cable 2' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03008
Cable 12' 40 GHz Astrolab	NA	07/03/2008	07/03/2010	AN05769
Cable 3' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03012
EMCO Loop Antenna	1074	05/01/2007	05/01/2009	00226

Equipment Under Test (* = EUT):

Function	Manufacturer	Model #	S/N
My Sentry Monitor*	Medtronic MiniMed	MMT9101	M000102F
My Sentry Monitor Power Supply	Specter Power	AMDD-20050-2000	None

Support Devices:

Function	Manufacturer	Model #	S/N
----------	--------------	---------	-----

Test Conditions / Notes:

Standard used was FCC 15.247. EUT is set to transmit continuously on Zigbee 2400-2483.5 MHz Band Low, Mid and High channels as indicated in the data sheet. Low Channel = 2405 MHz, Mid Channel = 2440 MHz, High Channel = 2475 MHz. Frequency range investigated was: Carrier. The temperature was 22°C and the humidity was 48%. RBW = 3 kHz VBW = 3 x RBW.

Power spectral density

Frequency (MHz)	Field Strength (dBuV/m @3m)	Power (dBm)	Limit (dBm)	Comments
2405	95.5	-1.824	8	Pass
2440	94.3	-3.024	8	Pass
2475	90.5	-6.824	8	Pass

Antenna gain used for calculation is 2.1 dBi.

Power formula used in accordance with KDB 558074

FCC 15.249(a) RF POWER OUTPUT

Test Setup Photos



Test Data Sheet

Test Location: CKC Laboratories, Inc. • 5046 Sierra Pines Dr. • Mariposa, CA 95338 • 209 966-5240

Customer: **Medtronic MiniMed**
 Specification: **FCC 15.249 (a)**
 Work Order #: **88416** Date: 12/8/2008
 Test Type: **Maximized Emissions** Time: 13:22:07
 Equipment: **My Sentry Monitor** Sequence#: 1
 Manufacturer: Medtronic MiniMed Tested By: Mike Wilkinson
 Model: MMT-9101
 S/N: M000102F

Test Equipment:

Function	S/N	Calibration Date	Cal Due Date	Asset #
Agilent E4446A SA	US44300407	01/03/2007	01/03/2009	02660
Chase CBL6111C Bilog	2456	12/30/2006	12/30/2008	01991
HP 8447D Preamp	2727A05444	06/20/2008	06/20/2010	00062
Cable, HF	1067016	04/23/2007	04/23/2009	P04290
Site D Rad Emiss-10m	N/A	03/06/2008	03/06/2010	CAB-SITED10M-9k-1G
3M SITE CABLE 20GHZ	NA	03/06/2008	03/06/2010	SITED3M1
Cable 2' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03008
Cable 12' 40 GHz Astrolab	NA	07/03/2008	07/03/2010	AN05769
Cable 3' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03012

Equipment Under Test (* = EUT):

Function	Manufacturer	Model #	S/N
My Sentry Monitor*	Medtronic MiniMed	MMT-9101	M000102F
My Sentry Monitor Power Supply	Specter Power	AMDD-20050-2000	None

Support Devices:

Function	Manufacturer	Model #	S/N

Test Conditions / Notes:

Standard used was FCC 15.249. EUT is set to transmit continuously on 916.56 MHz. Frequency range investigated was: Carrier The temperature was 22° C and the humidity was 48%. RBW = 120 kHz VBW = 3 x RBW

Transducer Legend:

T1=AMP-AN00062-062008	T2=ANT AN01991 25-1000MHZ
T3=CAB-SITED3M1 9k - 20G	T4=CAB-AN05769-40GHZ-12FT
T5=CAB-AN03008-40GHZ-2FT	T6=CAB-AN03012-40GHZ-3FT

Measurement Data:

#	Freq MHz	Rdng dBμV	Reading listed by margin.				Test Distance: 3 Meters					
			T1 dB	T2 dB	T3 dB	T4 dB	Dist Table	Corr dBμV/m	Spec dBμV/m	Margin dB	Polar Ant	
1	916.560M	91.6	-29.6 +0.3	+23.0 +0.4	+2.7	+1.3	+0.0	89.7	93.9	-4.2	Vert	
2	916.560M	88.9	-29.6 +0.3	+23.0 +0.4	+2.7	+1.3	+0.0	87.0	93.9	-6.9	Hori	

FCC 15.249(d) OATS RADIATED SPURIOUS EMISSIONS

Test Setup Photos



Test Data Sheets

Test Location: CKC Laboratories, Inc. • 5046 Sierra Pines Dr. • Mariposa, CA 95338 • 209 966-5240

Customer: **Medtronic MiniMed**
 Specification: **FCC 15.249(d) / 15.209**
 Work Order #: **88416**
 Test Type: **Maximized Emissions**
 Equipment: **My Sentry Monitor**
 Manufacturer: Medtronic MiniMed
 Model: MMT-9101
 S/N: M000102F

Date: 12/8/2008
 Time: 16:07:23
 Sequence#: 2
 Tested By: Mike Wilkinson

Test Equipment:

Function	S/N	Calibration Date	Cal Due Date	Asset #
Agilent E4446A SA	US44300407	01/03/2007	01/03/2009	02660
Chase CBL6111C Bilog	2456	12/30/2006	12/30/2008	01991
EMCO 3115 Horn Antenna	9307-4085	03/17/2007	03/17/2009	00656
HP 8447D Preamp	2727A05444	06/20/2008	06/20/2010	00062
Cable, HF	1067016	04/23/2007	04/23/2009	P04290
HP 8449B Preamp	3008A00301	12/13/2006	12/13/2008	2010
Site D Rad Emiss-10m	N/A	03/06/2008	03/06/2010	CAB-SITED10M-9k-1G
3M SITE CABLE 20GHZ	NA	03/06/2008	03/06/2010	SITED3M1
Cable 2' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03008
Cable 12' 40 GHz Astrolab	NA	07/03/2008	07/03/2010	AN05769
Cable 3' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03012
EMCO Loop Antenna	1074	05/01/2007	05/01/2009	00226
1.5 GHz HP Filter	3643A00027	05/15/2007	05/15/2009	02116

Equipment Under Test (* = EUT):

Function	Manufacturer	Model #	S/N
My Sentry Monitor*	Medtronic MiniMed	MMT-9101	M000102F
My Sentry Monitor Power Supply	Specter Power	AMDD-20050-2000	None

Support Devices:

Function	Manufacturer	Model #	S/N
----------	--------------	---------	-----

Test Conditions / Notes:

Standard used was FCC 15.249. EUT is set to transmit continuously on 915.56 MHz. Frequency range investigated was: 9 kHz to 10 GHz The temperature was 22° C and the humidity was 48%. RBW = 200 Hz 9 kHz-150kHz. RBW = 9 kHz 150 kHz-30 MHz RBW = 120 kHz 30-1000 MHz RBW = 1MHz 1000-10000 MHz VBW = 3 x RBW.

Transducer Legend:

T1=AMP-AN00062-062008	T2=Amp HF - AN02010
T3=ANT AN01991 25-1000MHz	T4=ANT AN00656 900MHz-18.5GHz
T5=CAB-SITED3M1 9k - 20G	T6=CAB-AN05769-40GHZ-12FT
T7=CAB-AN03008-40GHZ-2FT	T8=CAB-AN03012-40GHZ-3FT
T9=1.5GHz HPF 02116	

Measurement Data: Reading listed by margin. Test Distance: 3 Meters

#	Freq MHz	Rdng dB μ V	Reading listed by margin.				Dist Table	Corr dB μ V/m	Spec dB μ V/m	Margin dB	Polar Ant
			T1 dB	T2 dB	T3 dB	T4 dB					
1	1831.112M	43.2	+0.0 +3.6 +0.7	-35.0 +1.8	+0.0 +0.4	+26.8 +0.5	+0.0	42.0	54.0	-12.0	Vert
2	31.992M	39.9	-30.9 +0.4	+0.0 +0.2	+18.0 +0.1	+0.0 +0.1	+0.0	27.8	40.0	-12.2	Vert
3	1833.116M	42.8	+0.0 +3.6 +0.7	-35.0 +1.8	+0.0 +0.4	+26.8 +0.5	+0.0	41.6	54.0	-12.4	Horiz
4	479.992M	29.6	-30.5 +1.9	+0.0 +0.9	+17.8 +0.2	+0.0 +0.3	+0.0	20.2	46.0	-25.8	Vert

FCC PART 15.249 BLOCK EDGE

Test Equipment

Function	S/N	Calibration Date	Cal Due Date	Asset #
Agilent E4446A SA	US44300407	01/03/2007	01/03/2009	02660
Chase CBL6111C Bilog	2456	12/30/2006	12/30/2008	01991
HP 8447D Preamp	2727A05444	06/20/2008	06/20/2010	00062
Cable, HF	1067016	04/23/2007	04/23/2009	P04290
Site D Rad Emiss-10m	N/A	03/06/2008	03/06/2010	CAB-SITED10M-9k-1G
3M SITE CABLE 20GHZ	NA	03/06/2008	03/06/2010	SITED3M1
Cable 2' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03008
Cable 12' 40 GHz Astrolab	NA	07/03/2008	07/03/2010	AN05769
Cable 3' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03012

Test Conditions

EUT is set to transmit continuously on 916.56 MHz.


Test Setup Photos





Test Plots

FCC 15.249 BLOCK EDGE

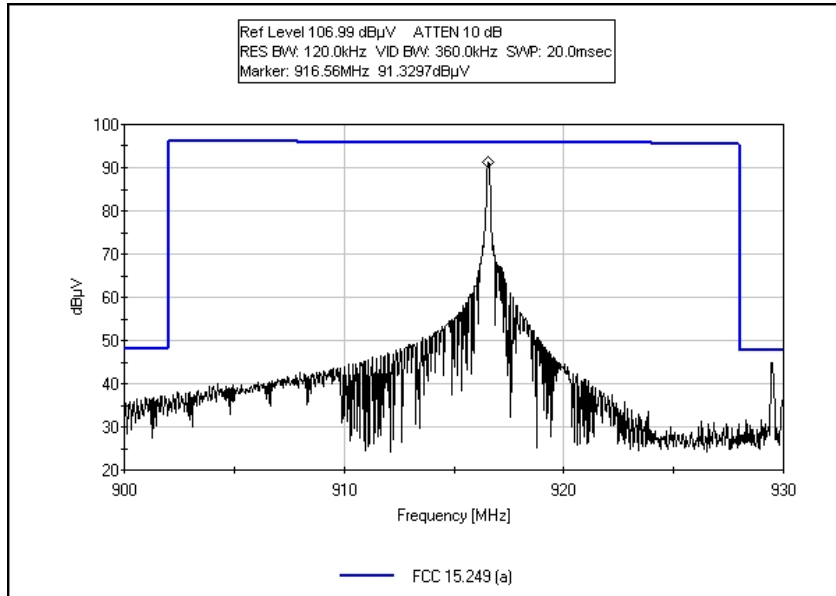

RSS-210 OCCUPIED BANDWIDTH

Test Equipment

Function	S/N	Calibration Date	Cal Due Date	Asset #
Agilent E4446A SA	US44300407	01/03/2007	01/03/2009	02660
Chase CBL6111C Bilog	2456	12/30/2006	12/30/2008	01991
HP 8447D Preamp	2727A05444	06/20/2008	06/20/2010	00062
Cable, HF	1067016	04/23/2007	04/23/2009	P04290
Amp HF - S/N 301	3008A00301	11/13/2008	11/13/2010	02010
Antenna, Horn	4085	03/19/2007	03/19/2009	00656
Site D Rad Emiss-10m	N/A	03/06/2008	03/06/2010	CAB-SITED10M-9k-1G
3M SITE CABLE 20GHZ	NA	03/06/2008	03/06/2010	SITED3M1
Cable 2' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03008
Cable 12' 40 GHz Astrolab	NA	07/03/2008	07/03/2010	AN05769
Cable 3' 40 GHz Astrolab	NA	01/15/2008	01/15/2010	AN03012

Test Conditions

EUT is set to transmit continuously on Zigbee 2400-2483.5 MHz Band and on 916.56 MHz.


Test Setup Photos






Test Plots


RSS-210 OCCUPIED BANDWIDTH LOW CHANNEL

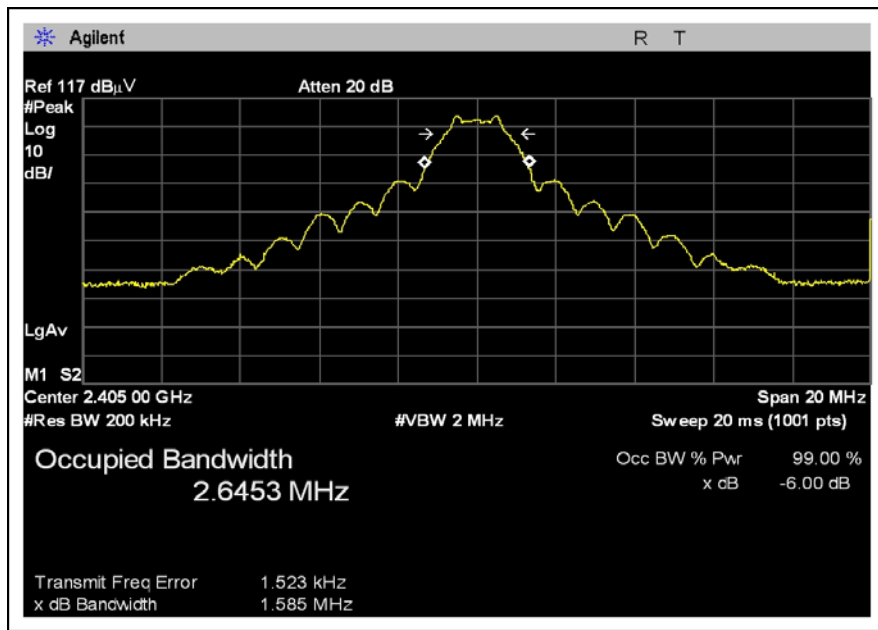


RSS-210 OCCUPIED BANDWIDTH MID CHANNEL

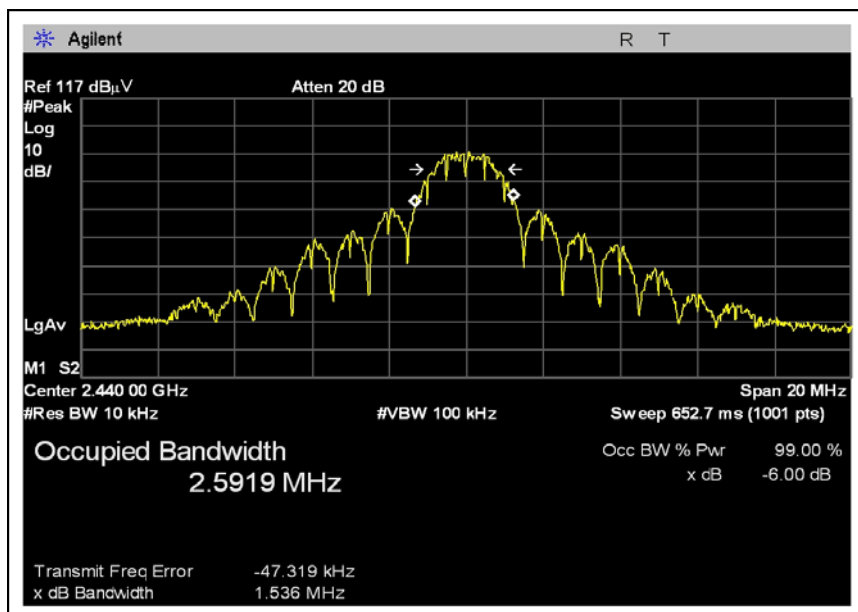

RSS-210 OCCUPIED BANDWIDTH HIGH CHANNEL

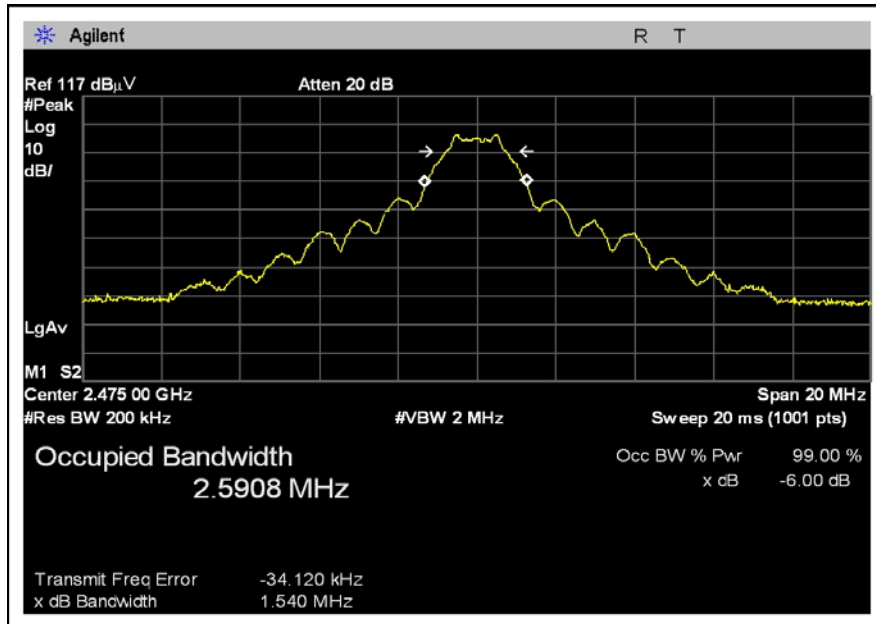

FCC 15.249 OCCUPIED BANDWIDTH 916.56 MHz

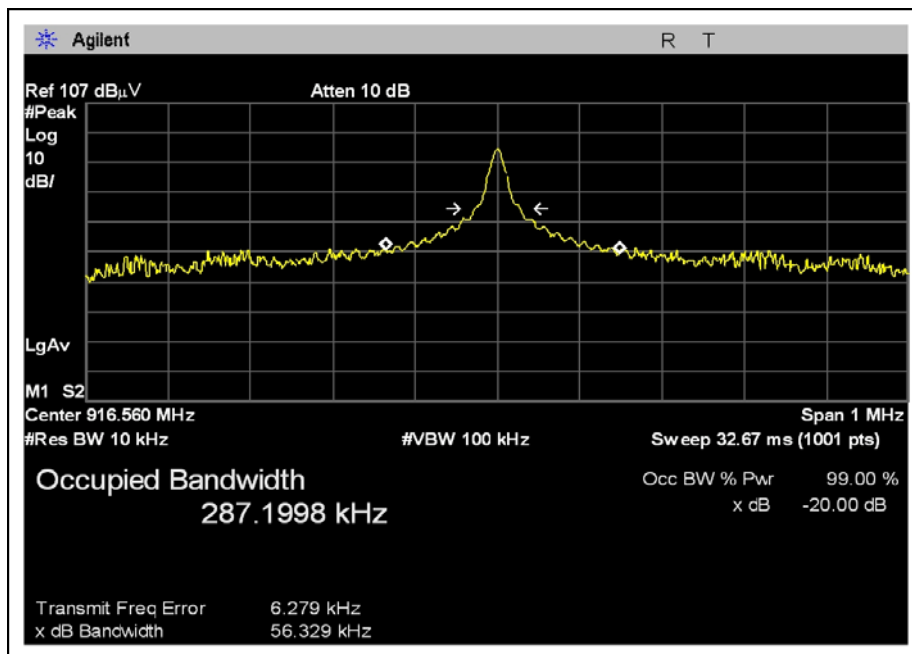

APPENDIX A: CUSTOMER INFORMATION

To CKC,

I've attached a document describing the Zigbee settings used in each of our devices. This document also describes how those settings affect the duty cycle calculation.

Using the settings and calculation from that document, the worst-case duty cycle calculations are as follows:

Packet width (ms) was measured as 3.73ms by CKC (see attached waveform), which matched the readings taken by Medtronic. To account for measurement error and ensure a worst-case approach, I will use a packet width of 4.0 ms in my calculations.

MySentry Monitor (Using the equation from ES9821 section 6.1, settings from 5.1) :

Packet Width = 4ms

Total retries = 4

Duty Cycle = $(4) * (4\text{ms}) / (100\text{ms}) = 0.16 * 100\% = 16\%$ duty cycle

Correction factor = $20 \log (16/100) = -15.92$ dB.

MySentry Repeater (Using the equation from ES9821 section 6.2, settings from 5.2) :


Packet Width = 4ms

Total retries = $(2) * (1) = 2$

Duty Cycle = $(2) * (4\text{ms}) / (100\text{ms}) = 0.08 * 100\% = 8\%$ duty cycle

Correction factor = $20 \log (8/100) = -21.94$ dB.

Mike Ivey (Medtronic MiniMed)

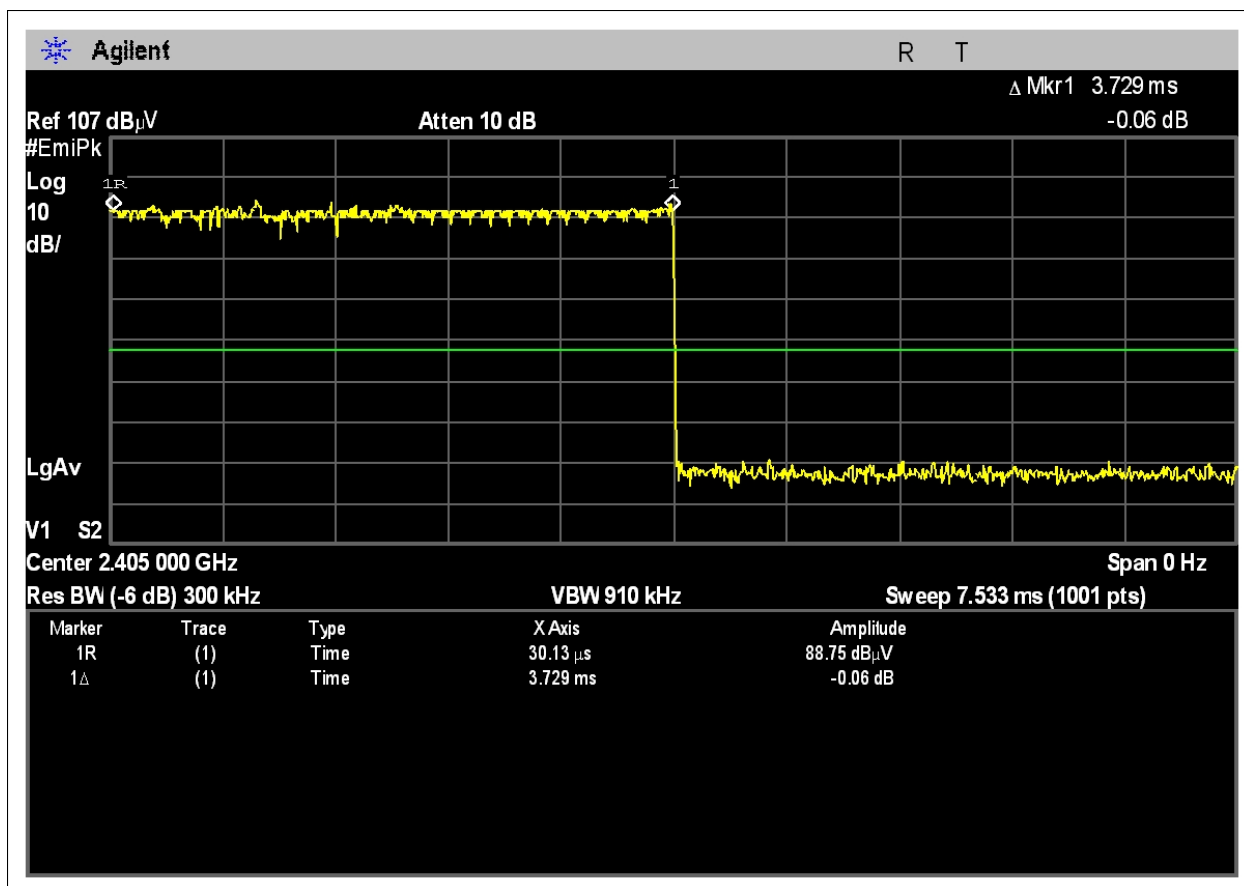

1.0 PURPOSE:

This document specifies settings for the Aerocomm ZB2430 Zigbee module used in MySentry Monitor (MMT-9101) and MySentry Outpost (MMT-9102). The settings are loaded into the EEPROM of the Zigbee Module. The calculations section specifies how these settings impact the worst case duty cycle during a 100ms window. This calculation is needed to provide a correction factor during FCC testing.

2.0 SCOPE:

This document contains settings for both the MySentry Monitor (MMT-9101) and MySentry Outpost (MMT-9102). These settings are used in the software to satisfy requirements outlined in Software Requirements Specifications **ES9700** and **ES9699**.

3.0 DEFINITIONS:

Zigbee Module Aerocomm ZB2430
EEProm Non-volatile memory which stores persistent device settings

4.0 REFERENCE DOCUMENTS:


ES9699 MySentry Monitor Software Requirements Specification
ES9700 MySentry Outpost Software Requirements Specification

5.0 SPECIFICATIONS:

5.1 MySentry Monitor

* Values are module defaults unless indicated by a *.

Description	EEProm Address	Value
Channel Mask	0x30	0x03FFF800
End Device Poll Rate	0x34	0x03E8
Channel Number	0x40	0x0B
Baud Rate	0x42	0x06
Baud_M	0x43	0xFF
Baud_E	0x44	0xFF
Control 0	0x45	0x38
MAC Retries	0x4B	0x03
Transmit Attempts	0x4C	0x02
Broadcast Attempts	0x4D	0x04
Stale Limit	0x4F	0x32
Control 1	0x56	0x08*
Interface Timeout	0x58	0x04
RF Packet Size	0x5A	0x0054
CTS On	0x5C	0x01C0
CTS Off	0x5E	0x01B0
Power Control	0x63	0x00
Destination ID	0x76	0xFFFF*
PAN ID	0x78	Varies by unit SN*
API Control	0xC1	0xF8

	Save Date	Type	Document	Sheet	Ver.
	Dec. 10, 08	Z20	ES9821	2 of 3	A

5.2 MySentry Outpost

* Values are module defaults unless indicated by a *

Description	EEProm Address	Value
Channel Mask	0x30	0x03FFF800
End Device Poll Rate	0x34	0x03E8
Channel Number	0x40	0x0B
Baud Rate	0x42	0x06
Baud_M	0x43	0xFF
Baud_E	0x44	0xFF
Control 0	0x45	0x30*
MAC Retries	0x4B	0x01*
Transmit Attempts	0x4C	0x02
Broadcast Attempts	0x4D	0x02*
Stale Limit	0x4F	0x32
Control 1	0x56	0x08*
Interface Timeout	0x58	0x02*
RF Packet Size	0x5A	0x0054
CTS On	0x5C	0x01C0
CTS Off	0x5E	0x01B0
Power Control	0x63	0x00
Destination ID	0x76	0x0000
PAN ID	0x78	Assigned by monitor*
API Control	0xC1	0xF8*

6.0 CALCULATIONS:

6.1 MySentry Monitor

The coordinator operates only in broadcast mode. Using the data above, the worst case duty cycle for a 100ms period of Zigbee transmission can be calculated.

Total retries = <Broadcast Attempts>


Duty Cycle = <Total retries> * <Packet width (ms)> / 100 ms

6.2 MySentry Outpost

The repeater operates only in normal operation. Using the data above, the worst case duty cycle for a 100ms period of Zigbee transmission can be calculated.

Total retries = <MAX Retries> * <Transmit Attempts>

Duty Cycle = <Total retries> * <Packet width (ms)> / 100 ms

	Save Date	Type	Document	Sheet	Ver.
	Dec. 10, 08	Z20	ES9821	3 of 3	A