

US Tech Test Report:
FCC ID:
Test Report Number:
Issue Date:
Customer:
Model:

FCC Part 95 Permissive Change
OU507APFH-AP
21-0379
January 26, 2022
GE Medical Systems Information Technologies, Inc.
07APFH-AP

INTERNAL PHOTOGRAPHS



Figure 1. Main Board, Top

US Tech Test Report:
FCC ID:
Test Report Number:
Issue Date:
Customer:
Model:

FCC Part 95 Permissive Change
OU507APFH-AP
21-0379
January 26, 2022
GE Medical Systems Information Technologies, Inc.
07APFH-AP

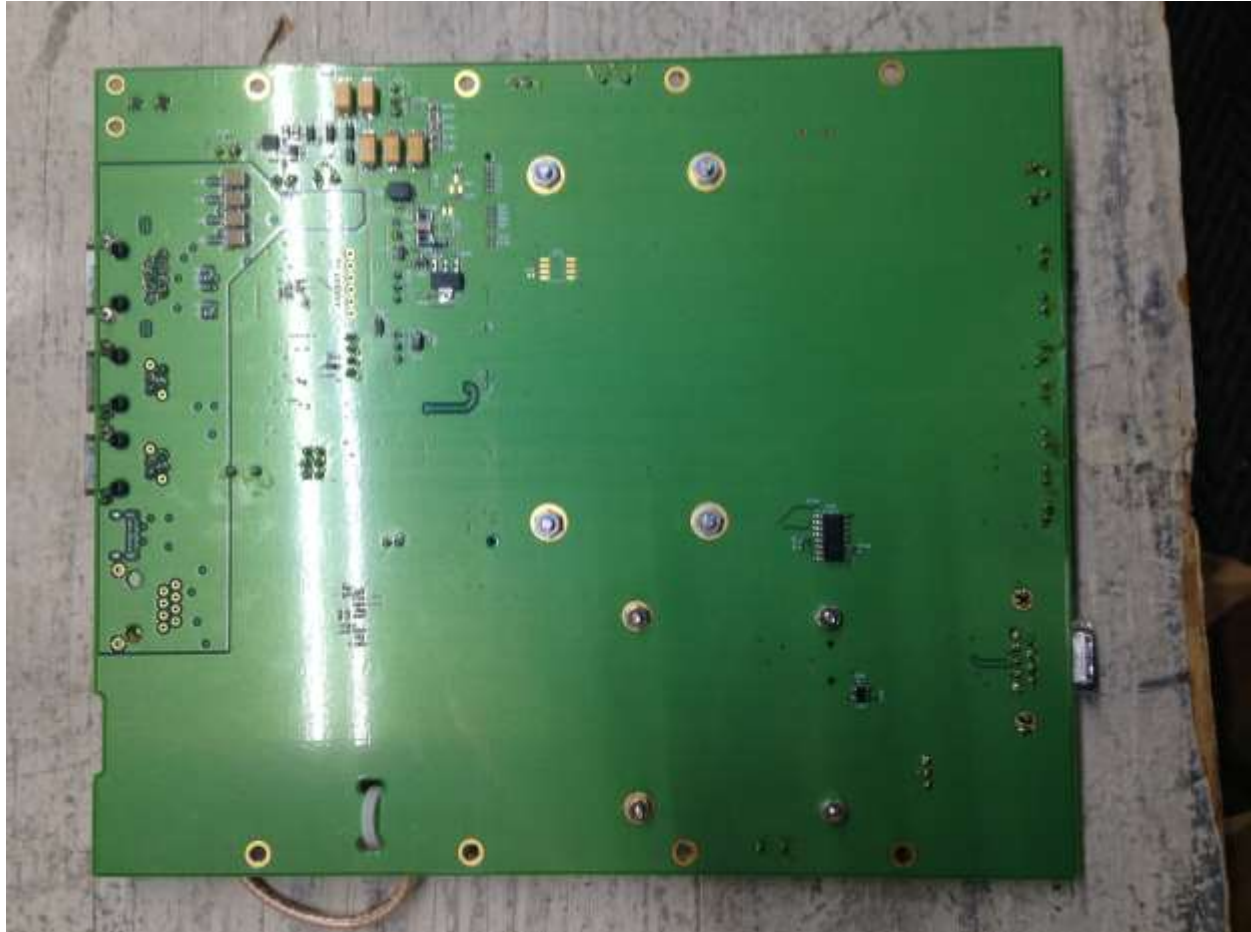


Figure 2. Main Board, Bottom

US Tech Test Report:
FCC ID:
Test Report Number:
Issue Date:
Customer:
Model:

FCC Part 95 Permissive Change
OU507APFH-AP
21-0379
January 26, 2022
GE Medical Systems Information Technologies, Inc.
07APFH-AP

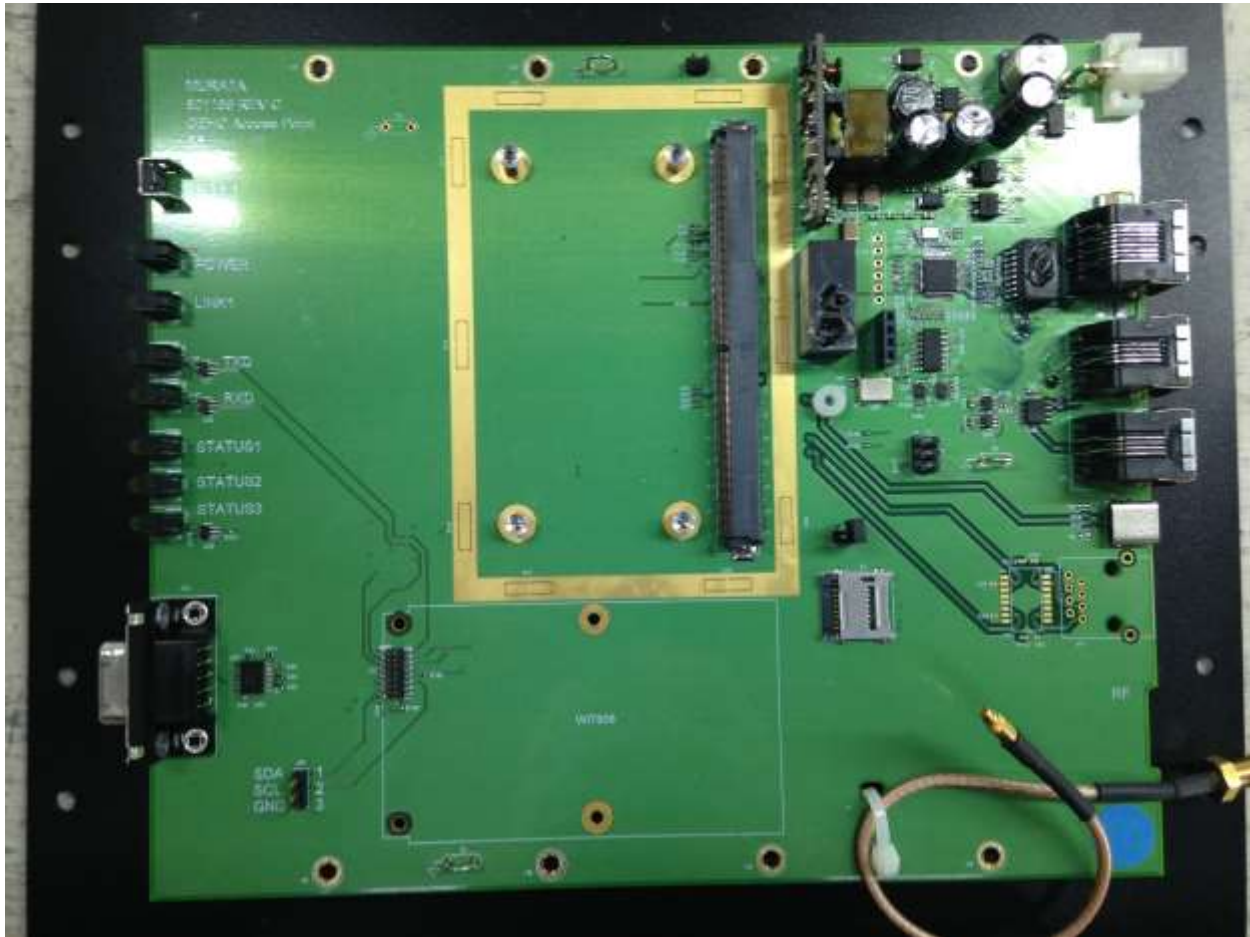


Figure 3. Modular PCBA Removed

US Tech Test Report:
FCC ID:
Test Report Number:
Issue Date:
Customer:
Model:

FCC Part 95 Permissive Change
OU507APFH-AP
21-0379
January 26, 2022
GE Medical Systems Information Technologies, Inc.
07APFH-AP

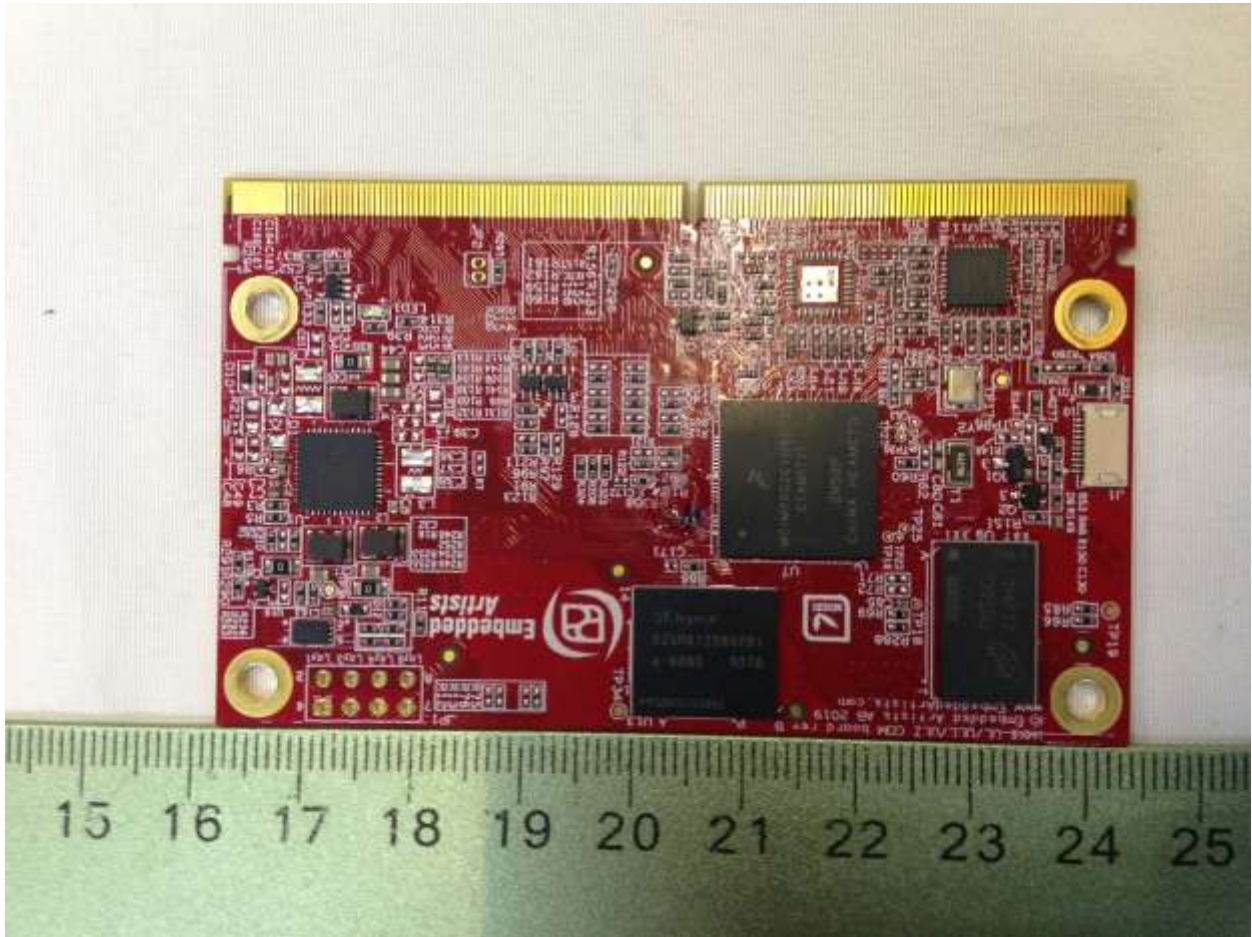


Figure 4. Embedded PCBA, Top

US Tech Test Report:
FCC ID:
Test Report Number:
Issue Date:
Customer:
Model:

FCC Part 95 Permissive Change
OU507APFH-AP
21-0379
January 26, 2022
GE Medical Systems Information Technologies, Inc.
07APFH-AP

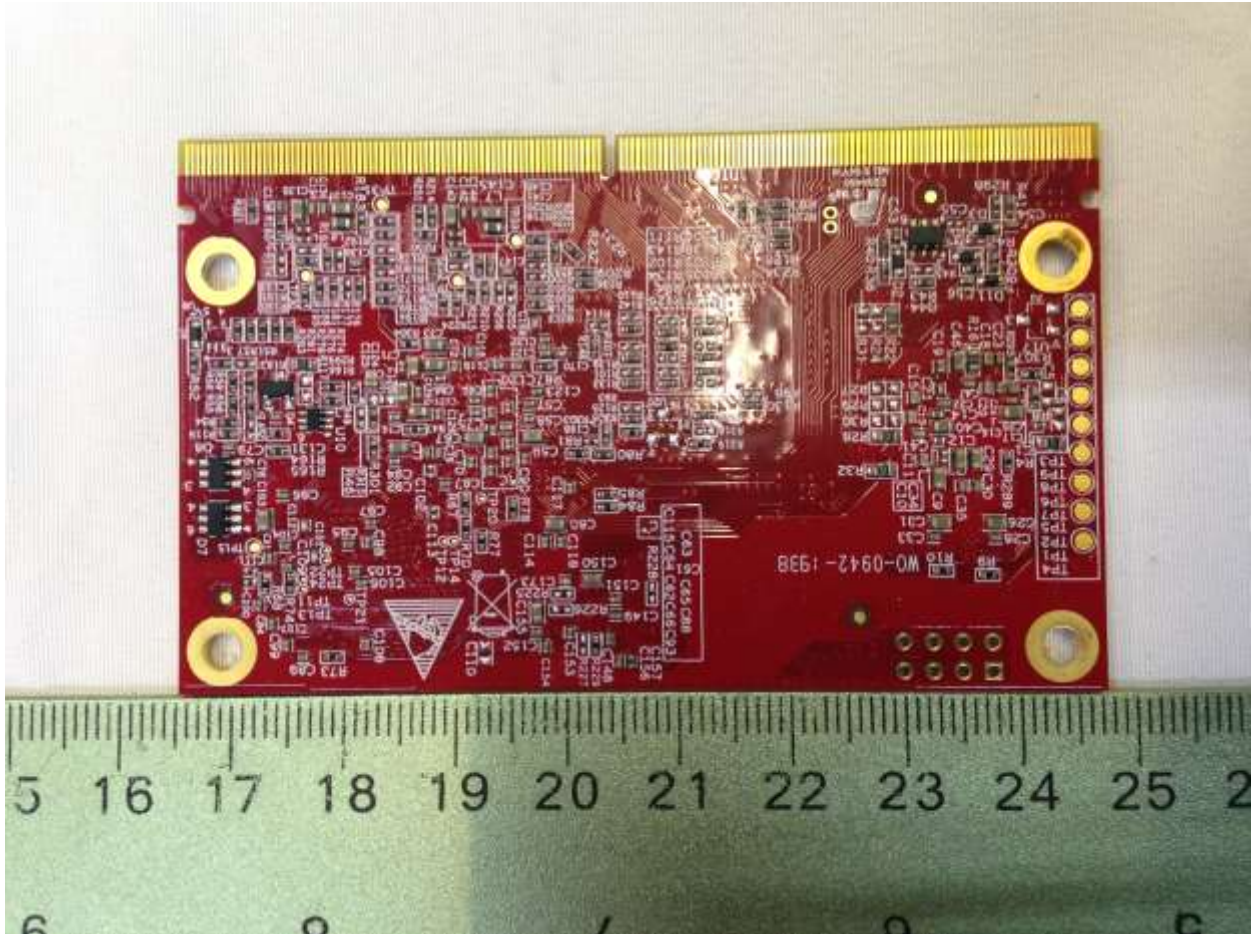


Figure 5. Embedded PCBA, Bottom

US Tech Test Report:
FCC ID:
Test Report Number:
Issue Date:
Customer:
Model:

FCC Part 95 Permissive Change
OU507APFH-AP
21-0379
January 26, 2022
GE Medical Systems Information Technologies, Inc.
07APFH-AP



Figure 6. Module with Shield, Top

US Tech Test Report:
FCC ID:
Test Report Number:
Issue Date:
Customer:
Model:

FCC Part 95 Permissive Change
OU507APFH-AP
21-0379
January 26, 2022
GE Medical Systems Information Technologies, Inc.
07APFH-AP

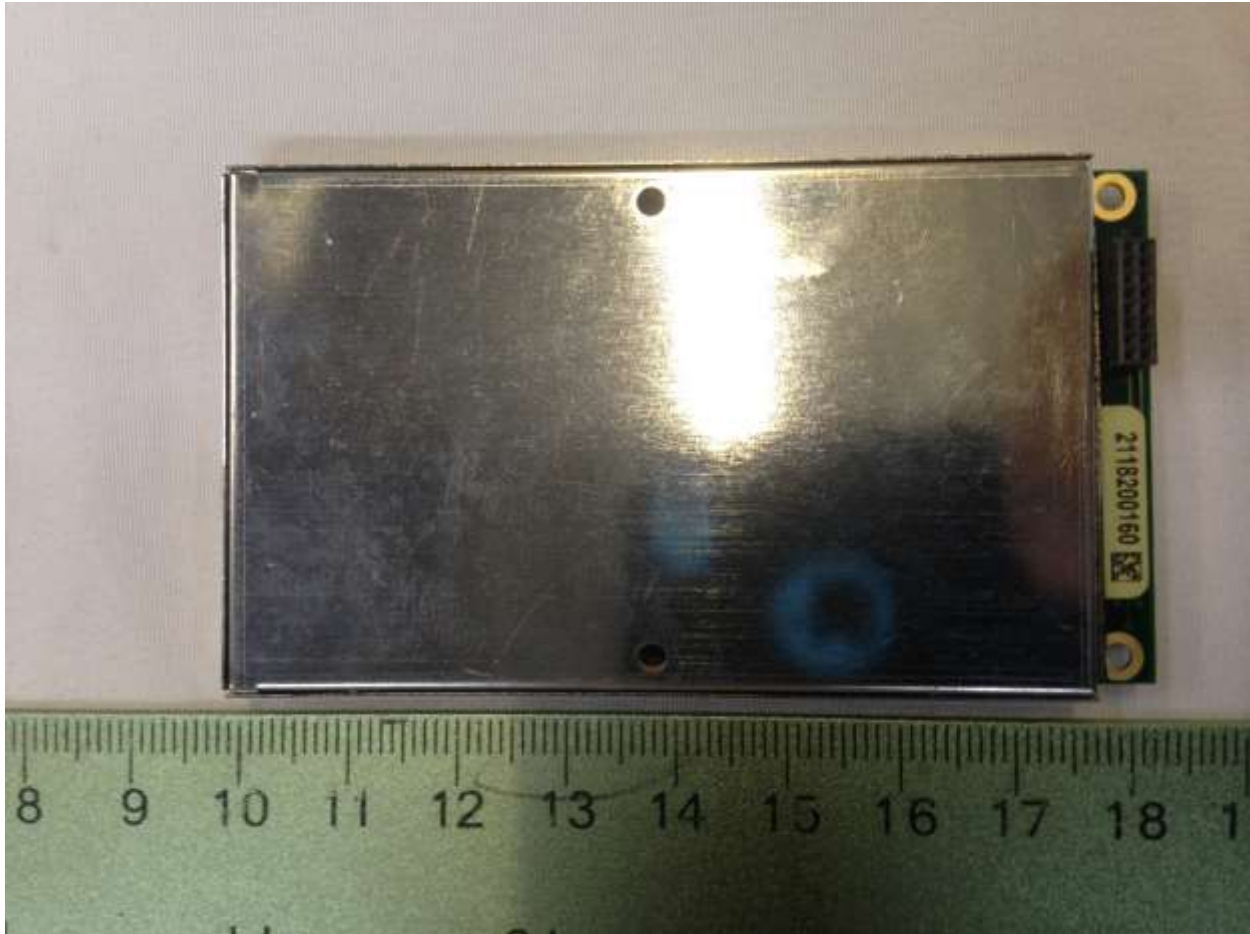


Figure 7. Module with Shield, Bottom

US Tech Test Report:
FCC ID:
Test Report Number:
Issue Date:
Customer:
Model:

FCC Part 95 Permissive Change
OU507APFH-AP
21-0379
January 26, 2022
GE Medical Systems Information Technologies, Inc.
07APFH-AP



Figure 8. Module with Shield Removed, Top

US Tech Test Report:
FCC ID:
Test Report Number:
Issue Date:
Customer:
Model:

FCC Part 95 Permissive Change
OU507APFH-AP
21-0379
January 26, 2022
GE Medical Systems Information Technologies, Inc.
07APFH-AP

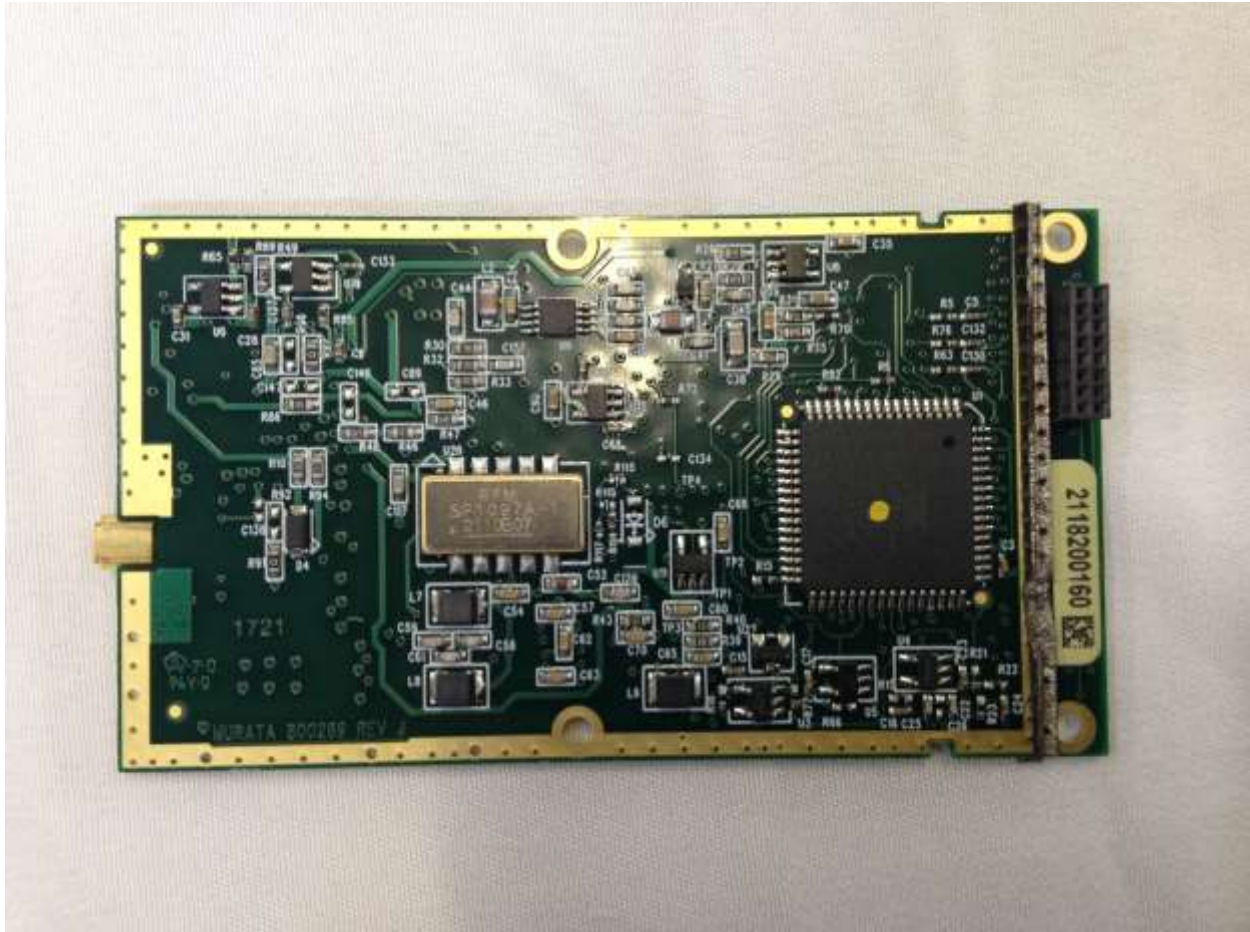


Figure 9. Module with Shield Removed, Bottom