

NOTES:

TOP PLOT: OCCUPIED BANDWIDTH, FCC 2.1049
 BOTTOM PLOT: EXEMPTION FROM TECHNICAL STANDARDS, FCC 90.2.17(b)
 AND RF POWER OUTPUT FCC 2.1046

MEAS TYPE:
 Radiated Prescan
 Radiated Final
 Conducted
 Disturbance Power
 Other *SEE NOTES*

ANTENNA/COUPLER:

- 9124 Bicon
- 3146 Log Per
- 3106 Horn
- 3109 Bicon
- 3115 Horn
- CBL6112B Bilog
- CBL6140 X-Wing
- MDS-21 Clamp
- NSLK 8126 LISN
- NNB-4/63TL LISN
- NNB-4/200X LISN
- N/A

POLARIZATION:

- Horizontal
- Vertical
- NA

DISTANCE:

- 3 Meter
- 10 Meter
- Meter
- NA


LOCATION:

- OATS
- Semi-Anechoic
- Shielded Room
- Factory Floor
- Other



PLOTTER

18:18:10 OCT 11, 2000
 GE MEDICAL SYSTEMS MODEL 340 OCCUPIED BANDWIDTH
 REF 120.0 dBμV #AT 10 dB PG -45.0 dB → 45 dB ADDED ATTENUATION

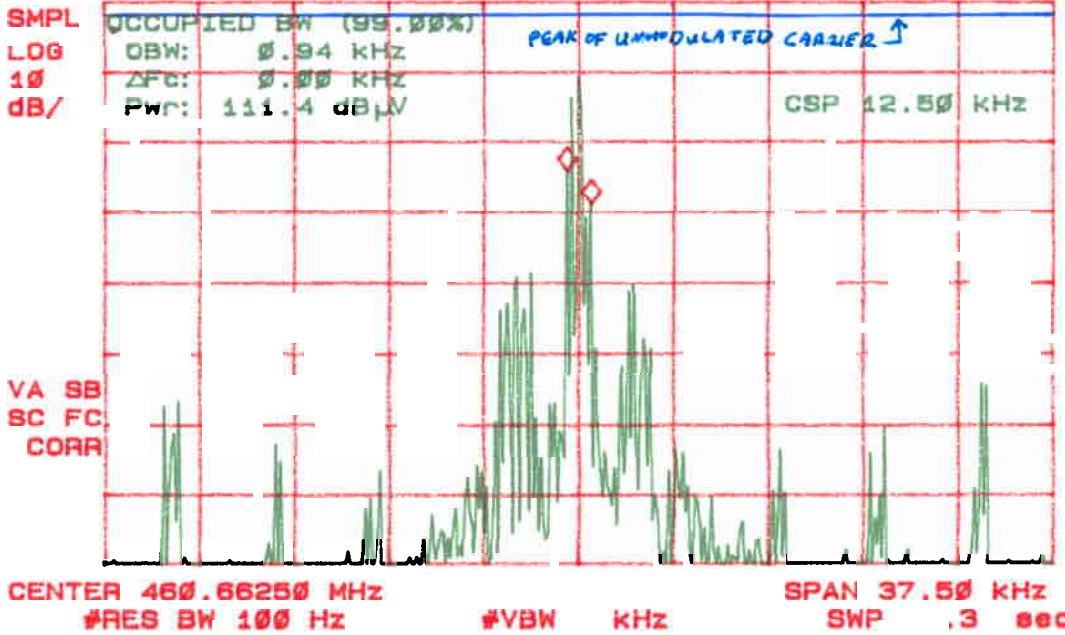

09:58:05 OCT 12, 2000
 GE MEDICAL SYSTEMS MODEL 340 MKR 460.6630 MHz
 REF 130.0 dBμV #AT 10 dB PG -45.0 dB 117.90 dBμV = 12.3mW

