

Guangdong Transtek Medical Electronics Co., Ltd.

广东乐心医疗电子股份有限公司

Document Name: 文件名称:	User manual
Document No 文件编号:	LS-IFU-LS802-Ga
Rev.: 版本号:	A/0
Page: 页码:	共28页


Prepared 编制	Reviewed 审核	Approved 批准
<i>Celia Li</i>	<i>Ada Liang</i>	<i>Jerry Fan</i>

◆ Revision History 修订履历

NO.	Date 日期	Update Description 变更描述	Prepared 编制	Reviewed 审核	Approved 批准
A/0	2024/04/17	Initial release	李鑫 Celia Li	梁桂英 Ada Liang	范佳龙 Jerry Fan

User Manual

Blood Pressure Monitor
LS802-Ga

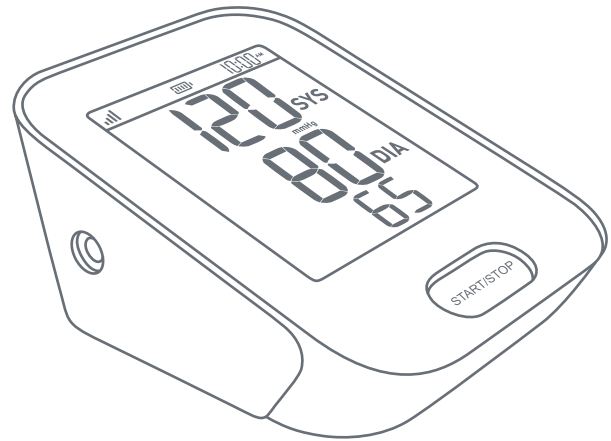

Guangdong Transtek Medical Electronics Co., Ltd.
Zone A, No.105, Dongli Road, Torch Development District,
528437 Zhongshan, Guangdong, China

version: A/0

TeleCuff Gen 1

技术要求:

- 1、黏合不可露胶
- 2、保持印刷面板上的清洁
- 3、注意套印的准确性
- 4、表面处理不可爆开
- 5、结构工艺以结构受控图为准
- 6、颜色参考:

广东乐心医疗电子股份有限公司

2022-03-31

受控文件

产品型号	LS802-Ga	材质	105g哑粉纸	零件名称	
产品名称	血压计	尺寸	210*145mm (折后105*145 mm)	5BF00204B-LS802-Ga说明书-A0	
对应结构图纸	-	印色	CMYK		
	比例	1:1	表面处理	零件图号	
	单位	mm	设计		
Transtek 广东乐心医疗电子股份有限公司		审核		共 15 张	第 1 张
		批准		版 本	A/0

TABLE OF CONTENTS

INTRODUCTION	3
General Description	
Indications for Use	
Measurement Principle	
Safety Information	
Display and Symbols	
Name of Each Part	
Contents/Product Includes	
BEFORE YOU START	10
The Choice of Power Supply	
Installing and Replacing the Batteries	
MEASUREMENT	12
Applying the cuff	
Taking a Measurement	
INFORMATION FOR USER	15
Tips for measurement	
Maintenances	
ABOUT BLOOD PRESSURE	17
What are systolic pressure and diastolic pressure?	
What is the standard blood pressure classification?	
Irregular heartbeat detector	
Why does my blood pressure fluctuate throughout the day?	
Why do I get a different blood pressure at home compared to the hospital?	
Is the result the same if measuring on the right arm?	
TROUBLESHOOTING	20
SPECIFICATIONS	21
AUTHORIZED COMPONENT	22
CONTACT INFORMATION	22
EMC GUIDANCE	23
SPECIFICATIONS FOR 4G	27
FCC STATEMENT	28

INTRODUCTION

General Description

Thank you for choosing this arm type Blood Pressure Monitor (LS802-Ga). It is equipped with the following key features. Please read this manual to know how to use your Blood Pressure Monitor safely and correctly. Keep the manual well for future reference.



Indications for Use

This Blood Pressure Monitor is intended for use in measuring blood pressure and pulse rate in patients with arm circumferences from 16 ~ 36 cm (6 1/8 ~ 14 1/8 inch), 22 ~ 42 cm (8 3/4 ~ 16 1/2 inch), 22 ~ 45 cm (8 3/4 ~ 17 3/4 inch) or 40 ~ 52cm (15 3/4 ~ 20 1/2 inch).

Cuff model AC1636-01, arm circumference range is 16 ~ 36cm (6 1/8 ~ 14 1/8 inch), which is intended for children older than 3 years old or adults without conditions of diabetes, pregnancy, or pre-eclampsia.

Cuff model AC2245-021, arm circumference range is 22 ~ 45cm (8 3/4 ~ 17 3/4 inch), which is intended for adult population or those who with conditions of diabetes, pregnancy, or pre-eclampsia.

Cuff model AC2242-41 and cuff model AC4052-04, arm circumference range are 22 ~ 42cm (8 3/4 ~ 16 1/2 inch), and 40 ~ 52cm (15 3/4 ~ 20 1/2 inch) respectively, which are intended for adults without conditions of diabetes, pregnancy, or pre-eclampsia.

It is intended indoor use only.

Measurement Principle

This product uses the Oscillometric Measuring method to detect blood pressure. Before every measurement, the unit establishes a "zero pressure" equivalent to the atmospheric pressure. Then it starts inflating the arm cuff, meanwhile, the unit detects pressure oscillations generated by beat-to-beat pulsatile, which is used to determine the systolic and diastolic pressure, and also pulse rate.

INTRODUCTION

Safety Information

The symbols below might be in the user manual, labeling or other component. They are the requirement of standard and using.

	Refer to instruction manual/booklet To signify that the instruction manual/ booklet must be read.		Type BF applied part
	Consult instructions for use or consult electronic instructions for use		Serial Number
	Direct Current		Polarity of d.c. power connector
	Class II Equipment		For indoor use only
	Batch code		Manufacturer
	Date of manufacture		Temperature limit
	Atmospheric pressure limitation		Humidity limitation
	General symbol for recovery/recyclable		
	MR Unsafe To identify an item which poses unacceptable risks to the patient, medical staff or other persons within the MR environment.		
	Caution Indicates that caution is necessary when operating the device or control close to where the symbol is placed, or that the current situation needs operator awareness or operator action in order to avoid undesirable consequences.		
	The symbol indicates that the product should not be discarded as unsorted waste but must be sent to separate collection facilities for recovery and recycling.		

INTRODUCTION

Precaution

- * **Blood Pressure Monitor is intended to be operated by adults, including medical staffs and lay persons. Adult patients could also be intended users or operators.**
- * This device is intended for indoor, home use and is not intended for self-use in public areas.
- * This device is portable, but it is not intended for use during patient transport.
- * This device is not suitable for continuous monitoring during medical emergencies or operations.
- * This device is intended for non-invasive measuring and monitoring of arterial blood pressure. It is not intended for use on extremities other than the arm, or for any purpose other than obtaining a blood pressure measurement.
- * This device is for patients who are at or over 3 years old. Do not use this device on neonates or infants.
- * Consult with your physician before using this monitor if you suffer from the following conditions: common arrhythmias such as premature ventricular beats or atrial fibrillation; peripheral arterial disease, implantation with electrical devices; undergoing intravascular therapy; arteriovenous shunt or mastectomy. Please note that any of these conditions may affect measurement readings, in addition to patient motion, trembling or shivering.
- * If you are taking medication, consult your physician to determine the proper time to measure your blood pressure.
- * This device may be used only for the intended use described in this manual, the manufacturer shall have no liability for any incidental, consequential, or special damages caused by misuse or abuse.
- * Please use the device under the environment which is provided in the user manual. Otherwise, the performance and lifetime of the device will be impacted and reduced.
- * The device may require up to 30 minutes to warm up / cool down from the minimum/ maximum storage temperature before it is ready for use.
- * The blood pressure monitor, its adapter, and the cuff are suitable for use within the patient environment.
- * Do not wash the cuff in a washing machine or dishwasher!
- * The device contains sensitive electronic components. To avoid measurement errors, avoid taking blood pressure measurements near a strong electromagnetic field radiated interference signal or electrical fast transient/burst signal.
- * Wireless communication equipment, such as wireless home network devices, mobile phones, cordless telephones and their base stations, walkie-talkies may cause interference that may affect the accuracy of measurements. A minimum distance of 1 foot (30 cm) should be kept from such devices during a measurement.
- * Please choose the appropriate cuff according to your arm circumference and physical health.

⚠ Caution

- * Do not attempt to repair the unit yourself if it malfunctions. Only have repairs carried out by authorized service centers.
- * It is recommended that the performance should be checked after repair, maintenance, and every two years of use, by retesting the requirements in limits of the error of the cuff pressure indication and air leakage (testing at least at 50 mmHg and 200 mmHg). Please contact manufacturer or distributor for authorized service personnel.
- * Store your device, cuff and adapter in a clean and dry place, protect it against extreme moisture, heat, lint, dust and direct sunlight. Never place any heavy objects on it.
- * Make sure the rubber tube of the cuff is not squeezed, stretched, or kinked during storage.
- * Dispose of accessories, detachable parts, and the device according to the local guidelines.

INTRODUCTION

Warning


- * **DO NOT self-diagnose the measurement results and start treatment by yourself. The measurement results given by this device is not a diagnosis. ALWAYS consult your doctor for evaluation of the results and treatment.**
- * **DO NOT adjust medication based on readings from this blood pressure monitor. Take medication as prescribed by your physician. ONLY a physician is qualified to diagnose and treat high blood pressure.**
- * **DO NOT** apply the cuff on an arm that has an intravenous drip or a blood transfusion attached.
- * **DO NOT** kink, fold, stretch, compress, or otherwise deform the tube during measuring, as the cuff pressure might continuously increase, which could prevent blood flow and result injury.
- * Taking blood pressure measurements too frequently could disrupt blood circulation and cause injuries.
- * **DO NOT** apply cuff to areas on patient where skin is delicate or damaged. Check cuff site frequently for irritation.
- * **DO NOT** place the cuff on the arm of a person whose arteries or veins are undergoing medical treatment, i.e. intra-vascular access or intra-vascular therapy or an arteriovenous (A-V) shunt, which could disrupt blood circulation and cause injuries.
- * **DO NOT** place the cuff on the arm on the same side of a mastectomy (especially when lymph nodes have been removed). It is recommended to take measurements on the unaffected side.
- * **DO NOT** wrap the cuff on the same arm to which another monitoring device is applied. One or both devices could temporarily stop functioning if you try to use them at the same time.
- * Warning: Please check (for example, by observation of the limb concerned) that the operation of the device does not result in prolonged impairment of patient blood circulation.
- * Warning: On the rare occasion of a fault causing the cuff to remain fully inflated during measurement, loosen and remove the cuff immediately. Prolonged high pressure applied to the arm (cuff pressure >300 mmHg or constant pressure >15 mmHg for more than 3 minutes) might lead to bruising and discolored skin.
- * **DO NOT** use this device with high-frequency (HF) surgical equipment at the same time.
- * This device is not used in conjunction with oxygen rich environments, not intended for use with flammable anaesthetics, not intended for use in conjunction with flammable agents.
- * Excessive cuff tube lengths could cause strangulation if you don't manage them properly.
- * **DO NOT** touch output of the batteries/adapter and the user simultaneously.
- * The power cord is considered the disconnect device for isolating this equipment from supply mains. **DO NOT** position the equipment so that it is difficult to reach or disconnect.
- * **DO NOT** use this device if you are allergic to polyester, nylon, or plastic.
- * Only use accessories approved by manufacturer. Using unapproved accessories might cause damage to the unit and injure users.
- * If you experience discomfort during a measurement, such as pain in the arm or other complaints, press the Power button immediately to release the air from the cuff.
- * **DO NOT** use the device while under maintenance, or being serviced.
- * Sensor degradation or looseness may reduce performance of device or cause other problems.
- * The air tube poses a risk of strangulation. Furthermore, the small parts of product and batteries present a choking hazard if swallowed. They should therefore always be kept away from infants/children.

Note

- * You can use this device to take your own measurement, no third-party operator is required.
- * Adapter is specified as a part of ME EQUIPMENT.
- * At the request of authorized service personnel, circuit diagrams, component part lists, descriptions, and calibration procedures will be made available by the manufacturer or distributor.
- * The expected lifetime of the cuff may vary by the frequency of washing, skin condition, and storage state.
- * Please report to the manufacturer and the competent authority of the Member State / the FDA in which you are established about any serious incident that has occurred in relation to this device.


INTRODUCTION

Display and Symbols

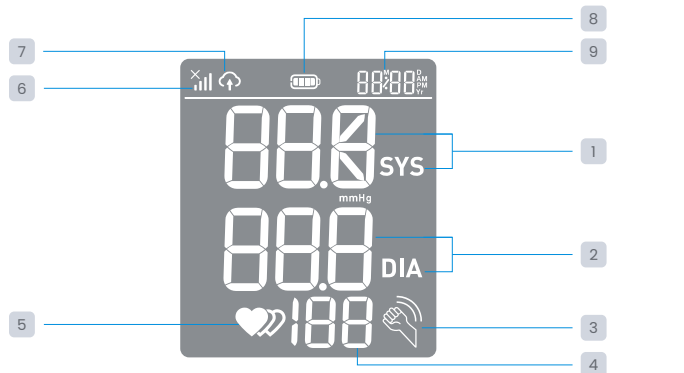


- 1 Systolic blood pressure reading
- 2 Diastolic blood pressure reading
- 3 Excessive body motion detector symbol
- 4 Pulse display
- 5 Heartbeat symbol / Irregular heartbeat
- 6 Signal indication
- 7 Data transmission indication
- 8 Battery symbol / Low battery symbol
- 9 Date / Time display

INTRODUCTION

SYMBOL	EXPLANATION	
1	Systolic blood pressure reading	
2	Diastolic blood pressure reading	
3		Excessive body motion detector symbol Appears when talking, moving, or shaking of the arm with the cuff on is detected during a measurement. NOTE: The measured blood pressure reading may not be accurate when this symbol is displayed with the reading.
4	Pulse display	
5		Heartbeat symbol Flashes when detected during the measurement.
		Irregular heartbeat symbol Appears when detected during a measurement. Refer to page 18 for more information.
6		Signal indication Indicates the signal situation in the communication process.
7		Data transmission indication Appears on the LCD display and flash when the measurement data is being sent. If the data transmission is a success, OK is shown.
8		Battery symbol / Low battery symbol Indicate the battery is low when both symbols  appear on the LCD display.
9	Date / Time display	

INTRODUCTION

Name of Each Part

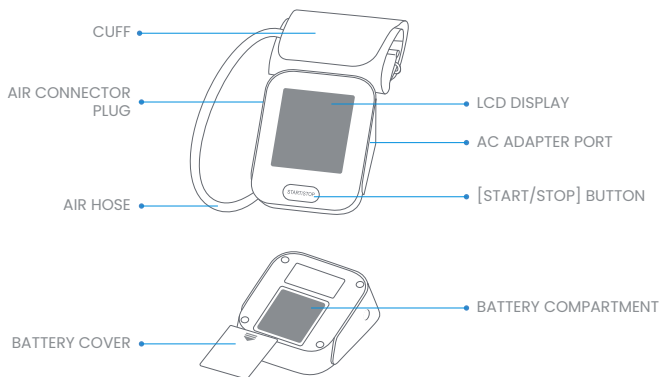

Contents/Product Includes

- 1 Pro Cellular Blood Pressure Monitor (LS802-Ga)
- 1 Cuff (Type BF applied part)
 - 16-36 cm (6 1/2 ~ 14 1/2 inch) upper arm cuff
 - 22-42 cm (8 3/4 ~ 16 1/2 inch) upper arm cuff
 - 22-45 cm (8 3/4 ~ 17 3/4 inch) upper arm cuff
 - 40-52 cm (15 3/4 ~ 20 1/2 inch) upper arm cuff
- 1 User Manual
- 1 Quick Start Guide
- 4 "AA" size batteries
- 1 AC Adapter (Optional!)


BEFORE YOU START

The Choice of Power Supply

1. DC 6V, 4 AA size batteries
2. AC adapter, 6V $\overline{\sim}$ 1A

Please use the AC adapter authorized by the manufacturer! (Optional)
Please unplug the adapter to depart from the using utility power, when you finish the measurement.

Four AA batteries could be installed inside the device even when the AC adapter is used to power the device, because the device will cut off the AA batteries power when detecting that the AC adapter is working to power the device.



CAUTION


In order to get the best effect and protect your monitor, please use the right batteries and special power adapter which complies with local safety standard.

Installing and Replacing the Batteries

- Slide off the battery cover.
- Install or replace 4 AA size batteries according to the polarity indications inside the battery compartment.
- Place back the battery cover.

Replace the batteries whenever the below happens

- Both symbols \perp and \square appear on the LCD display.
- The display dims.
- The display does not light up.





CAUTION

- New and used batteries, or different types of batteries shall not be used together.
- Remove batteries if the device is not likely to be used for some time.
- Do not heat or deform the batteries, or dispose of them in fire.
- Batteries should not be disposed of with household waste.
- Please check with your local authority for battery recycling advice.



BEFORE YOU START



Note :

When you insert or replace batteries into the device, the symbol  and  will display on the LCD alternately. This indicates that the device is searching and pairing with a mobile network.

You can long press the  button to end pairing and use the device.

If you manually cancel pairing, the device may take longer to send a measurement after use.



If successful, the symbol  will be shown on the LCD. You can then utilize the devices as normal by pressing the  button.



If unsuccessful, the monitor will power off automatically after several minutes.

MEASUREMENT

Applying the cuff

Only use a cuff that has been approved by the manufacturer for this device model. Before use, please confirm if it fits your arm circumference.




Choosing for cuff:

Cuff model AC1636-01, arm circumference range is 16 ~ 36cm (6 1/8 ~ 14 1/8 inch), which is intended for children older than 3 years old or adults without conditions of diabetes, pregnancy, or pre-eclampsia.

Cuff model AC2245-021, arm circumference range is 22 ~ 45cm (8 3/4 ~ 17 3/4 inch), which is intended for adult population or those who with conditions of diabetes, pregnancy, or pre-eclampsia.

Cuff model AC2242-41 and cuff model AC4052-04, arm circumference range are 22 ~ 42cm (8 3/4 ~ 16 1/2 inch), and 40 ~ 52cm (15 3/4 ~ 20 1/2 inch) respectively, which are intended for adults without conditions of diabetes, pregnancy, or pre-eclampsia.

1. Remove all jewelry, such as watches and bracelets from your left arm.
Note: If your doctor has diagnosed you with poor circulation in your left arm, use your right arm.
2. Roll or push up your sleeve to expose the skin. Make sure your sleeve is not too tight.
3. Hold your arm with palm facing up and tie the cuff on your upper arm, then align the air tube toward the center of your arm.
4. Make sure the bottom edge of the arm cuff 2~3 cm (0.8-1.2 inch) above the inside elbow. Then wrap the cuff securely.
Note: The cuff should be snug but not too tight. You should be able to insert one finger between the cuff and your arm.
5. Sit upright in a comfortable chair with your back against the backrest of the chair. Keep your feet flat and your legs uncrossed.
Place your arm resting comfortably on a flat table. The cuff worn on your arm should be placed at the same level as your right atrium of the heart.
6. Take 5-6 deep breaths and let's start measuring!



Helpful tips to help ensure an accurate reading

- Take the measurement in a silent room.
- Rest for 5 minutes before a measurement.
- Be relaxed, remain still and DO NOT talk while taking a measurement.
- For a meaningful comparison, try to measure under similar conditions. For example, take daily measurements at approximately the same time, on the same arm, or as directed by a physician.

MEASUREMENT

Taking a Measurement

1. When the monitor is off, press the **START/STOP** button to turn on, and then it will complete the whole measurement automatically.



LCD display



Adjust the zero point




Inflating and measuring



Display the measured result



MEASUREMENT

2. After the measurement, the data transmission starts. The symbol  will blink on the LCD.



If successful, the symbol  will disappear and the LCD will display **OK**.



Press the **START/STOP** button to turn off the device, otherwise it will power off automatically after about 1 minute.

If unsuccessful, an error message ("E5" or "E6" for example) will display on the LCD for about 1 minute and then the device will power off.



Note:
In the case of a data transmission failure (E5 or E6), up to 60 measurements are saved on the device and will be sent when a successful connection is achieved.






Tip:
You can press the **START/STOP** button to stop the measurement any time.



INFORMATION FOR USER

Tips for Measurement

Measurements may be inaccurate if taken in the following circumstances.

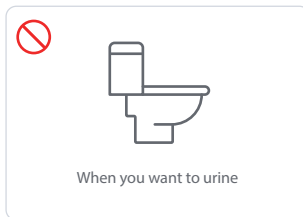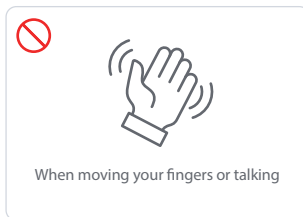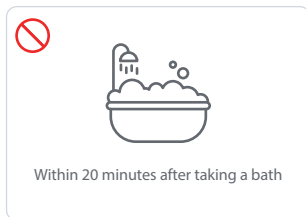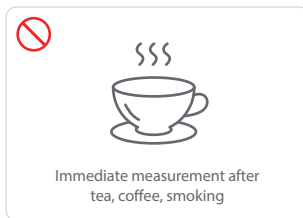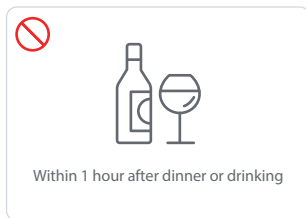

INFORMATION FOR USER

Maintenance

In order to get the best performance, please follow the instructions below.

1. Cleaning Process:

- Step 1: Before cleaning the monitor, make sure that the monitor is switched off and disconnected from the power line.
- Step 2: Clean the cuff with a soft cloth dampened with the soapy water. Until no visible contaminants remain.
- Step 3: Rinse the cuff and wipe off the cleaning solution with a fresh cloth or towel, dampened with tap water after cleaning until no visible cleaning agent remains.
- Step 4: Wipe off with a dry cloth to remove residual moisture.
- Step 5: Air dry the cuff thoroughly after cleaning.

2. Disinfection Process (Clean the monitor before disinfection):

- Step 1: Before disinfecting the monitor, make sure that the monitor is switched off and disconnected from the power line.
- Step 2: Disinfect the cuff with a soft cloth dampened with the 70% isopropanol during 3 minutes.
- Step 3: Rinse the cuff and wipe off the disinfection solution with a fresh cloth or towel, dampened with tap water after disinfecting until no visible disinfection agent remains.
- Step 4: Wipe off with a dry cloth to remove residual moisture.
- Step 5: Air dry the cuff thoroughly after disinfecting.

• Suggestion:



Frequency of Cleaning and Disinfection:

For single patient multiple use, it's recommended to clean the device surface once a month or whenever it's necessary.
For multiple patient multiple use, it's recommended to clean the device every time before and after usage. Maintenance procedures shall be taken as per instruction.

ABOUT BLOOD PRESSURE

What are systolic pressure and diastolic pressure?

When ventricles contract and pump blood out of the heart, the blood pressure reaches its maximum value in the cycle, which is called systolic pressure. When the ventricles relax, the blood pressure reaches its minimum value in the cycle, which is called diastolic pressure.



What is the standard blood pressure classification?

The following chart is the standard blood pressure classification published by American Heart Association (AHA).

This chart reflects blood pressure categories defined by American Heart Association.

Blood Pressure Category	Systolic mmHg (upper#)		Diastolic mmHg (lower#)
Normal	less than 120	and	less than 80
Elevated	120-129	and	less than 80
High Blood Pressure (Hypertension) Stage 1	130-139	or	80-89
High Blood Pressure (Hypertension) Stage 2	140 or higher	or	90 or higher
Hypertensive Crisis (Consult your doctor immediately)	Higher than 180	and/or	Higher than 120

ABOUT BLOOD PRESSURE


CAUTION

Only a physician can tell your normal BP range. Please contact a physician if your measuring result falls out of the range. Please note that only a physician can tell whether your blood pressure value has reached a dangerous point.

Irregular Pulse Rate Detector

An irregular pulse rate will be detected if there is an irregular pulse rhythm while measuring systolic and diastolic blood pressure. When measurements were performed, the monitor will record all pulse intervals and calculate the average. If two or more pulse intervals were recorded, and the difference between each interval and the average is larger than $\pm 25\%$ of the average; or if four or more pulse intervals were recorded, and the difference between each interval and the average is larger than $\pm 15\%$ of the average value, the irregular pulse symbol will be displayed along with measurement results.

CAUTION

The appearance of the IPR icon  indicates that a pulse irregularity consistent with an irregular pulse rate was detected during measurement. Usually this is NOT a cause for concern. However, if the symbol appears often, we recommend you seek medical advice. Please note that the irregular pulse rate detector results cannot be used directly for clinical judgement. Please seek medical advice from professionals before making any medical decisions.

ABOUT BLOOD PRESSURE

Why does my blood pressure fluctuate throughout the day?

1. Individual blood pressure varies multiple times everyday. It is also affected by the way you tie your cuff and your measurement position, so please take the measurement under the same conditions.
2. If the person takes medicine, the pressure will vary more.
3. Wait at least 3 minutes for another measurement.

Why do I get different blood pressure at home compared to the hospital?

The blood pressure is different even throughout the day due to weather, emotion, exercise etc. Also, there is the “white coat” effect, which means blood pressure usually increases in clinical settings.

Is the result the same if measuring on the right arm?

It is ok for both arms, but there will be some different results for different people. We suggest you measure the same arm every time.

Note:

What you need to pay attention to when you measure your blood pressure at home:

If the cuff is tied properly.

If the cuff is too tight or too loose.


If the cuff is tied on the upper arm.

If you feel anxious.

Taking 2-3 deep breaths before beginning will be better for measuring.

Advice: Relax yourself for 4-5 minutes until you calm down.

TROUBLE SHOOTING

PROBLEM	DISPLAY	CHECK THIS	REMEDY
No power or Low batteries	Display will not light up or  shows	Batteries are exhausted.	Replace with new batteries.
		Batteries are inserted incorrectly.	Insert the batteries correctly.
		AC adapter is inserted incorrectly.	Insert the AC adapter tightly.
Error message	E 1 shows	The cuff is not secure or abnormal inflation.	Refasten the cuff and then measure again.
	E 2 shows	The monitor detected motion,talking or the pulse is too weak while measuring.	Movement can affect the measurement.Relax for a moment and then measure again.
	E 3 shows	The measurement process does not detect the pulse signal.	Loosen the clothing on the arm and then measure again.
	E 4 shows	Not able to calculate, measurement failed.	Relax for a moment and then measure again.
	E 5 shows	Failed to communicate with the server.	Contact customer service.
	E 6 shows	No access to network.	Contact customer service.
	EExx,shows on the display.	A calibration error occurred.	Retake the measurement. If the problem persists, contact customer service for further assistance. Refer to the warranty for contact information and return instructions.
Warning message	out shows	Out of measurement range.	Relax for a moment. Refasten the cuff and then measure again. If the problem persists, contact your physician.

NOTE: If the product still does not work, contact the Customer Service. Under no circumstance should you disassemble or attempt to repair the unit by yourself.


SPECIFICATIONS

External dimensions	Approx. 154.3 mm × 121.5 mm × 68.1 mm
Display mode	Digital LCD V.A. 78 mm × 92 mm
Weight	Approx. 406 g (Excluding the batteries and cuff)
Measurement mode	Oscillographic testing mode
Mode of operation	Continuous operation
Measurement range	Rated cuff pressure: 0 mmHg ~ 299 mmHg (0 kPa ~ 39.9 kPa) Measurement pressure: SYS: 60 mmHg ~ 230 mmHg (8.0 kPa ~ 30.7 kPa) DIA: 40 mmHg ~ 130 mmHg (5.3 kPa ~ 17.3 kPa) Pulse value: (40~199) beat/minute
Accuracy	Pressure: 5°C ~ 40°C within ±3 mmHg (0.4 kPa) Pulse value: ±5%
Normal working condition	Temperature: +5°C to +40°C Relative humidity: 15% to 90%, non-condensing, but not requiring a water vapour partial pressure greater than 50 hPa Atmospheric pressure: 700 hPa to 1060 hPa
Storage condition & transportation condition	Temperature: -20°C to +60°C Relative humidity: ≤93%, non-condensing, at a water vapour pressure up to 50 hPa Atmospheric pressure: 500 hPa to 1060 hPa
Measurement perimeter of the upper arm	About 16 to 36 cm (6 ½ ~ 14 ½ inch), 22 to 42cm (8 ¾ ~ 16 ½ inch), 22 to 45cm (8 ¾ ~ 17 ½ inch) or 40 to 52cm (15 ¾ ~ 20 ½ inch).
Degree of protection	Type BF applied part
Device Classification	Battery Powered Mode: Internally Powered ME Equipment AC Adaptor Powered Mode: Class II ME Equipment
Protection against ingress of water	IP21, It means the device could protected against solid foreign objects of 12.5 mm and greater, and protect against vertically falling water drops.
Software Version	A01
Expected Lifetime	Device: 5 years or 10,000 measurements (may vary based on usage conditions) Cuff: 10,000 times Alkaline battery: About 200~300 times Adapter: About 20,000 hours

WARNING: No modification of this equipment is allowed.

AUTHORIZED COMPONENT

Please use the authorized adapter (Not included).

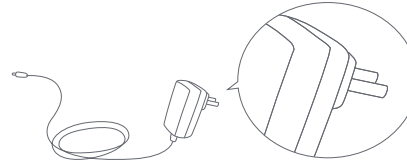

Adapter

Type: BLJ06L060100P-U

Input: 100~240V, 50-60Hz, 0.2A max

Output: 6V $\overline{\text{---}}$ 1000 mA

CONTACT INFORMATION

For more information about our products, please visit www.transtekcorp.com.

Manufactured by: Guangdong Transtek Medical Electronics Co., Ltd.

Company: Guangdong Transtek Medical Electronics Co., Ltd.

Address: Zone A, No.105, Dongli Road, Torch Development District,
528437 Zhongshan, Guangdong, China

EMC GUIDANCE

The ME EQUIPMENT or ME SYSTEM is suitable for home healthcare environments.

Essential performance:

Accuracy of measuring blood pressure and pulse rate

Measurement Range	Systolic pressure: 60-230 mmHg Diastolic pressure: 40-130 mmHg Pulse: 40-199 beats/minute
Accuracy	Pressure: ± 3 mmHg Pulse value: $\pm 5\%$

The Basis Safety of the Blood Pressure Monitor (LS802-Ga) is as following:
Deviation from normal operation that poses an unacceptable risk to the patient or operator.

Warning: Don't be near the active HF surgical equipment and the RF shielded room of an ME system for magnetic resonance imaging, where the intensity of EM disturbances is high.

Warning: Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.

Warning: Use of accessories, transducers and cables other than those specified or provided by the manufacturer of this equipment could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.

Warning: Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the equipment including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.

EMC GUIDANCE

Technical description:

1. All necessary instructions for maintaining BASIC SAFETY and ESSENTIAL PERFORMANCE with regard to electromagnetic disturbances for the expected lifetime.
2. Guidance and manufacturer's declaration–electromagnetic emissions and Immunity.

Table 1

Guidance and manufacturer's declaration - electromagnetic emissions	
Emissions test	Compliance
RF emissions CISPR 11	Group 1
RF emissions CISPR 11	Class B
Harmonic emissions IEC 61000-3-2	Class A
Voltage fluctuations/flicker emissions IEC 61000-3-3	Comply

Table 2

Guidance and manufacturer's declaration – electromagnetic Immunity		
Immunity Test	IEC 60601-1-2 Test level	Compliance level
Electrostatic discharge (ESD) IEC 61000-4-2	±8 kV contact ±2 kV, ±4 kV, ±8 kV, ±15 kV air	±8 kV contact ±2 kV, ±4 kV, ±8 kV, ±15 kV air
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV signal input/output 100 kHz repetition frequency	±2 kV for power supply lines NA 100 kHz repetition frequency
Surge IEC 61000-4-5	±0.5 kV, ±1 kV, differential mode ±0.5 kV, ±1 kV, ±2 kV common mode	±0.5 kV, ±1 kV differential mode N/A
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	0% UT ; 0,5 cycle. At 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315°. 0% UT ; 1 cycle and 70% UT ; 25/30 cycles; Single phase: at 0°. 0% UT ; 250 / 300 cycle	0% UT ; 0,5 cycle. At 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315°. 0% UT ; 1 cycle and 70% UT ; 25/30 cycles; Single phase: at 0°. 0% UT ; 250 / 300 cycle
Power frequency magnetic field IEC 61000-4-8	30 A/m 50 Hz / 60 Hz	30 A/m 50 Hz / 60 Hz
Conducted RF IEC 61000-4-6	3 V 0,15 MHz – 80 MHz 6 V in ISM and amateur radio bands between 0,15 MHz and 80 MHz 80% AM at 1 kHz	3 V 0,15 MHz – 80 MHz 6 V in ISM and amateur radio bands between 0,15 MHz and 80 MHz 80% AM at 1 kHz
Radiated RF IEC 61000-4-3	10 V/m 80 MHz – 2,7 GHz 80% AM at 1 kHz	10 V/m 80 MHz – 2,7 GHz 80% AM at 1 kHz

NOTE U_i is the a.c. mains voltage prior to application of the test level.

Table 3

Guidance and manufacturer's declaration – electromagnetic Immunity								
Radiated RF IEC 61000-4-3 (Test specifications for ENCLOSURE PORT IMMUNITY to RF wireless communications equipment)	Test Frequency (MHz)	Band (MHz)	Service	Modulation	Maximum Power (W)	Distance (m)	IEC 60601-1-2 Test Level (V/m)	Compliance level (V/m)
	385	380-390	TETRA 400	Pulse modulation 18 Hz	1.8	0.3	27	27
	450	430-470	GMR5 460, FRS 460	FM ± 5k Hz deviation 1 kHz sine	2	0.3	28	28
	710	704-787	LTE Band 13, 17	Pulse modulation 217 Hz	0.2	0.3	9	9
	745							
	780							
	810	800-960	GSM 800/900, TETRA 800, iDEN 820, CDMA 850, LTE Band 5	Pulse modulation 18 Hz	2	0.3	28	28
	870							
	930							
	1720	1700-1990	GSM 1800; CDMA 1900; GSM 1900; DECT; LTE Band 1, 3, 4, 25; UMTS	Pulse modulation 217 Hz	2	0.3	28	28
	1845							
	1970							
	2450	2400-2570	Bluetooth, WLAN, 802.11 b/g/n, RFID 2450, LTE Band 7	Pulse modulation 217 Hz	2	0.3	28	28
	5240	5100-5800	WLAN 802.11 a/n	Pulse modulation 217 Hz	0.2	0.3	9	9
5500								
5785								

SPECIFICATIONS FOR 4G

Specifications for 4G		
E-MTC	Supporting band:	Cat-M1: B2/4/12
	Transmitted frequency range	1850–1910MHz, 1710–1755MHz, 699–716MHz
	Transmitted power	20±2dBm
	Throughput	588–1119 kbps
	Latency	≤21ms
	Jitter	≤21ms
	PER	<10%
	Data Integrity	Data shall be transmitted correctly and completely
	Accessibility	Accessibility is high since 4G is broadband
<p>Remark:</p> <ol style="list-style-type: none"> 1.The Quality of Service (QoS) is considered as KPIs here. 2. For the Blood Pressure Monitor, the E-MTC is used to transmit the control data between the EUT and the controller,the manufacture considered 375~1119 kbps is a suitable throughput for the usage 3.The PER of the wireless system is normally less than 1%, for Semi-anechoic chamber, we considered the PER cannot be greater than 10%. 4. Use the wireless module which the EUT used as the test model,instead the EUT. 		

Warning

Failure to comply with the following warnings may cause cybersecurity issues.

DO NOT casually use the blood pressure monitor for others, as it may lead to leakage of personal measurement data.

DO NOT connect the blood pressure at places with poor network or wireless connectivity, as it may interrupt data upload and lead to deficient data.

FCC STATEMENT

FCC ID: OU9LS802GAM2

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Caution: The user is cautioned that changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

NOTE: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

FCC Radiation Exposure Statement:

This equipment complies with FCC radiation exposure limits set forth for an uncontrolled environment. This equipment should be installed and operated with minimum distance 20cm between the radiator and your body. This transmitter must not be co-located or operating in conjunction with any other antenna or transmitter.

FCC Responsible Party

Name: MIO LABS INC.
 Address: KCH, 575 Lexington Ave 14F New York, NY 10022
 Telephone: 301-910-0529
 E-mail: mio@transtekcorp.com