

FCC - TEST REPORT

Report Number : **64.790.18.00884.01** Date of Issue: 2018-06-20

Model : TMB-1490-BS

Product Type : Blood Pressure Monitor


Applicant : Guangdong Transtek Medical Electronics Co.,Ltd

Address : Zone A, No.105, Dongli Road, Torch Development District, 528437,
Zhongshan, Guangdong, China

Production Facility : Guangdong Transtek Medical Electronics Co.,Ltd

Address : Zone B, No.105, Dongli Road, Torch Development District, 528437,
Zhongshan, Guangdong, China

Test Result : **Positive** **Negative**



Total pages including Appendices : 33

TÜV SÜD Certification and Testing (China) Co., Ltd. Guangzhou Branch is a subcontractor to TÜV SÜD Product Service GmbH according to the principles outlined in ISO 17025.

TÜV SÜD Certification and Testing (China) Co., Ltd. Guangzhou Branch reports apply only to the specific samples tested under stated test conditions. Construction of the actual test samples has been documented. It is the manufacturer's responsibility to assure that additional production units of this model are manufactured with identical electrical and mechanical components. The manufacturer/importer is responsible to the Competent Authorities in Europe for any modifications made to the production units which result in non-compliance to the relevant regulations. TÜV SÜD Certification and Testing (China) Co., Ltd. Guangzhou Branch shall have no liability for any deductions, inferences or generalizations drawn by the client or others from TÜV SÜD Certification and Testing (China) Co., Ltd. Guangzhou Branch issued reports.

This report is the confidential property of the client. As a mutual protection to our clients, the public and ourselves, extracts from the test report shall not be reproduced except in full without our written approval.

1 Table of Contents

1	Table of Contents	2
2	Details about the Test Laboratory	3
3	Description of the Equipment Under Test	4
4	Summary of Test Standards	5
5	Summary of Test Results	6
6	General Remarks	7
7	Test Setups	8
8	Systems test configuration	9
9	Technical Requirement	10
9.1	Conducted peak output power	13
9.2	Power spectral density	16
9.3	6 dB Bandwidth and 99% Occupied Bandwidth	19
9.4	Spurious RF conducted emissions	22
9.5	Band edge	26
9.6	Spurious radiated emissions for transmitter	28
10	Test Equipment List	32
11	System Measurement Uncertainty	33



2 Details about the Test Laboratory

Details about the Test Laboratory

Test Site 1

Company name: TÜV SÜD Certification and Testing (China) Co., Ltd. Shenzhen Branch
Building 12 & 13, Zhiheng Wisdomland Business Park, Nantou Checkpoint
Road 2, Nanshan District
Shenzhen 518052
P.R. China

Telephone: 86 755 8828 6998
Fax: 86 755 828 5299

FCC Registration No.: 514049

3 Description of the Equipment Under Test

Product:	Blood Pressure Monitor
Model no.:	TMB-1490-BS
SN:	BS0337171200008D
FCC ID:	OU9TMB1490BS
Options and accessories:	N/A
Rating:	Battery:6.0VDC Power adapter:BLJ06L060100P-U Power adapter input:100-240V~ 50/60Hz,0.2A Max Power adapter output:6VDC,1000mA
RF Transmission Frequency:	2402MHz-2480MHz
No. of Operated Channel:	40
Modulation:	GFSK
Antenna Type:	Internal Antenna
Antenna Gain:	0.0dBi
Description of the EUT:	The Equipment Under Test (EUT) TMB-1490-BS is Blood Pressure Monitor operated at 2.402-2.48GHz

4 Summary of Test Standards

Test Standards	
FCC Part 15 Subpart C 10-1-2016 Edition	PART 15 - RADIO FREQUENCY DEVICES Subpart C - Intentional Radiators

All the test methods were according to KDB558074 D01 v01 DTS Measurement Guidance and ANSI C63.10 (2013).

5 Summary of Test Results

Technical Requirements					
FCC Part 15 Subpart C					
Test Condition		Test Site	Test Result		
			Pass	Fail	N/A
§15.207	Conducted emission AC power port	Site 1	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
§15.247 (b) (1)	Conducted peak output power	Site 1	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
§15.247(a)(1)	20dB bandwidth	---	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
§15.247(a)(1)	Carrier frequency separation	---	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
§15.247(a)(1)(iii)	Number of hopping frequencies	---	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
§15.247(a)(1)(iii)	Dwell Time	---	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
§15.247(a)(2)	6dB bandwidth and 99% Occupied Bandwidth	Site 1	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
§15.247(e)	Power spectral density	Site 1	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
§15.247(d)	Spurious RF conducted emissions	Site 1	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
§15.247(d)	Band edge	Site 1	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
§15.247(d) & §15.209	Spurious radiated emissions for transmitter	Site 1	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
§15.203	Antenna requirement	See note 1	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Note 1: N/A=Not Applicable.

Note 2: The EUT uses a Integrated antenna, which gain is 0.0dBi. In accordance to §15.203, it is considered sufficiently to comply with the provisions of this section.

6 General Remarks

This submittal(s) (test report) is intended for FCC ID: OU9TMB1490BS complies with Section 15.207, 15.209, 15.247 of the FCC Part 15, Subpart C rules.

TMB-1490-BS is Blood Pressure Monitor with Bluetooth 4.0. The TX and RX range is 2402MHz-2480MHz for 4.0.

SUMMARY:

All tests according to the regulations cited on page 5 were

- Performed
- **Not Performed**

The Equipment under Test


- **Fulfills** the general approval requirements.
- **Does not fulfill** the general approval requirements.

Testing Start Date: March 27, 2018

Testing End Date: May 31, 2018

- TÜV SÜD Certification and Testing (China) Co., Ltd. Guangzhou Branch -


Reviewed by:



Tony Liu




Prepared by:




Kevin Ouyang

7 Test Setups


7.1 AC Power Line Conducted Emission test setups

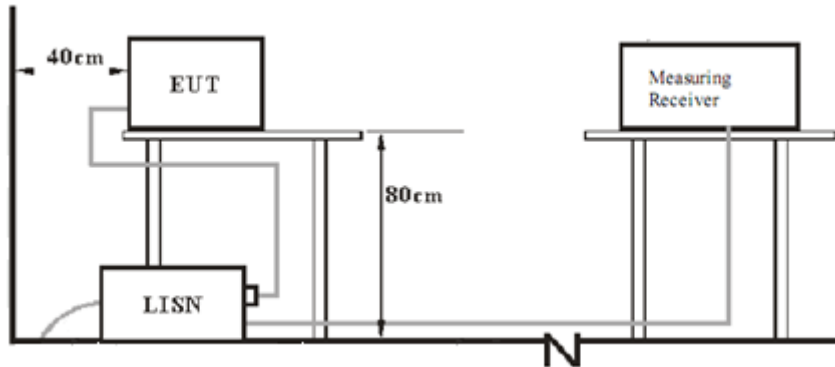

7.2 Radiated test setups

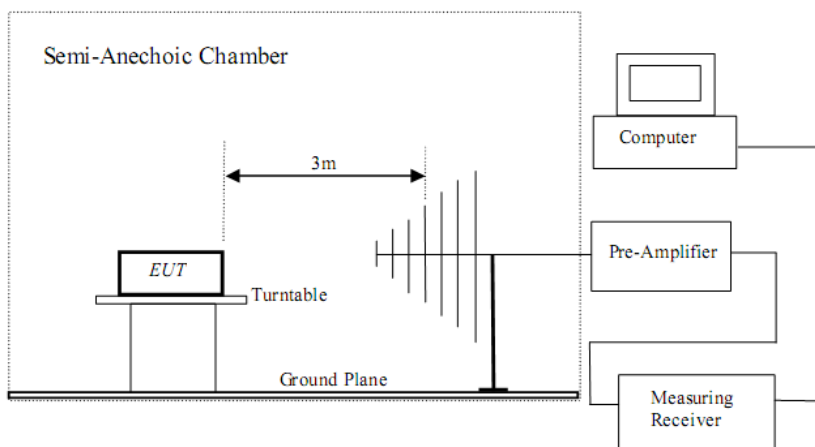

7.3 Conducted RF test setups



8 Systems test configuration

Auxiliary Equipment Used during Test:

DESCRIPTION	MANUFACTURER	MODEL NO.(SHIELD)	S/N(LENGTH)
Notebook	Lenovo	X220	---
Mobile phone	Huawei	P10	---
Non-Invasive Blood Pressure Simulator	---	FLUKE BP Pump 2	---

Test software: nRFgo Studio, which used to control the EUT in continues transmitting mode.

The system was configured to channel 0, 19, and 39 for the test.

9 Technical Requirement

9.1 Conducted Emission

Test Method

1. The EUT was placed on a table, which is 0.8m above ground plane
2. The power line of the EUT is connected to the AC mains through an Artificial Mains Network (A.M.N.).
3. Maximum procedure was performed to ensure EUT compliance
4. A EMI test receiver is used to test the emissions from both sides of AC line

Limit


According to §15.207, conducted emissions limit as below:

Frequency MHz	QP Limit dB μ V	AV Limit dB μ V
0.150-0.500	66-56*	56-46*
0.500-5	56	46
5-30	60	50

“*”: Decreasing linearly with logarithm of the frequency

Conducted Emission

Product Type : Blood pressure monitor
 M/N : TMB-1490-BS
 Operating Condition : EUT on with Bluetooth function on.
 Test Specification : Line
 Comment : AC 120V/60Hz

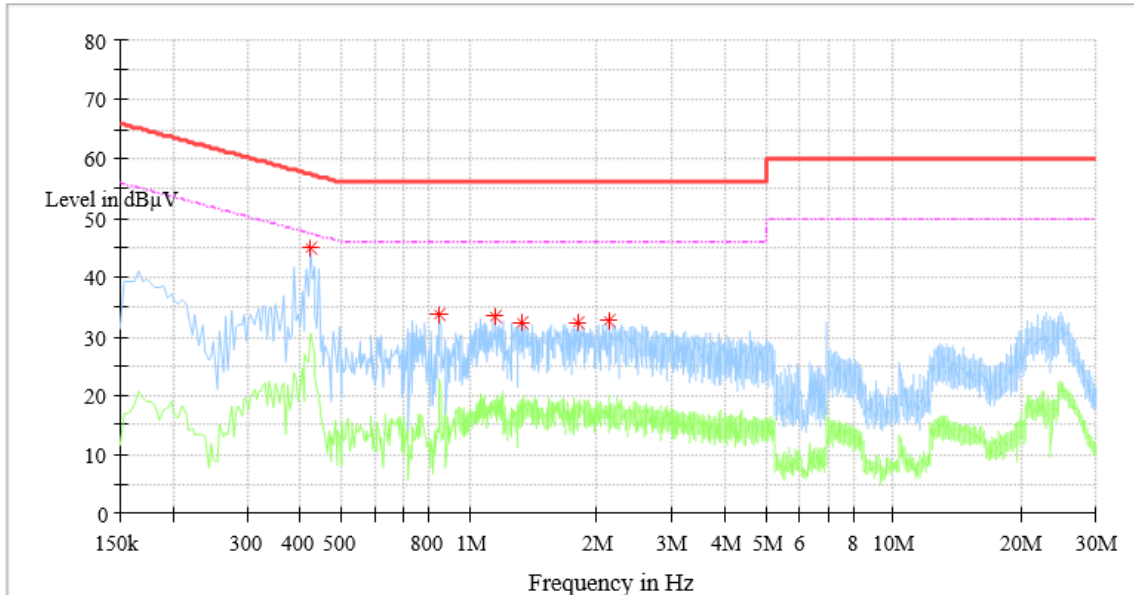


Final Result

Frequency (MHz)	QuasiPeak (dBμV)	Average (dBμV)	Limit (dBμV)	Margin (dB)	Line	Corr. (dB)
0.422000	45.07	---	57.41	12.33	L1	11.4
0.850000	33.66	---	56.00	22.34	L1	10.2
1.150000	33.35	---	56.00	22.65	L1	10.2
1.330000	32.43	---	56.00	23.57	L1	10.2
1.794000	32.37	---	56.00	23.63	L1	10.3
2.142000	32.71	---	56.00	23.29	L1	10.3

Conducted Emission

Product Type : Blood pressure monitor
 M/N : TMB-1490-BS
 Operating Condition : EUT on with Bluetooth function on.
 Test Specification : Neutral
 Comment : AC 120V/60Hz

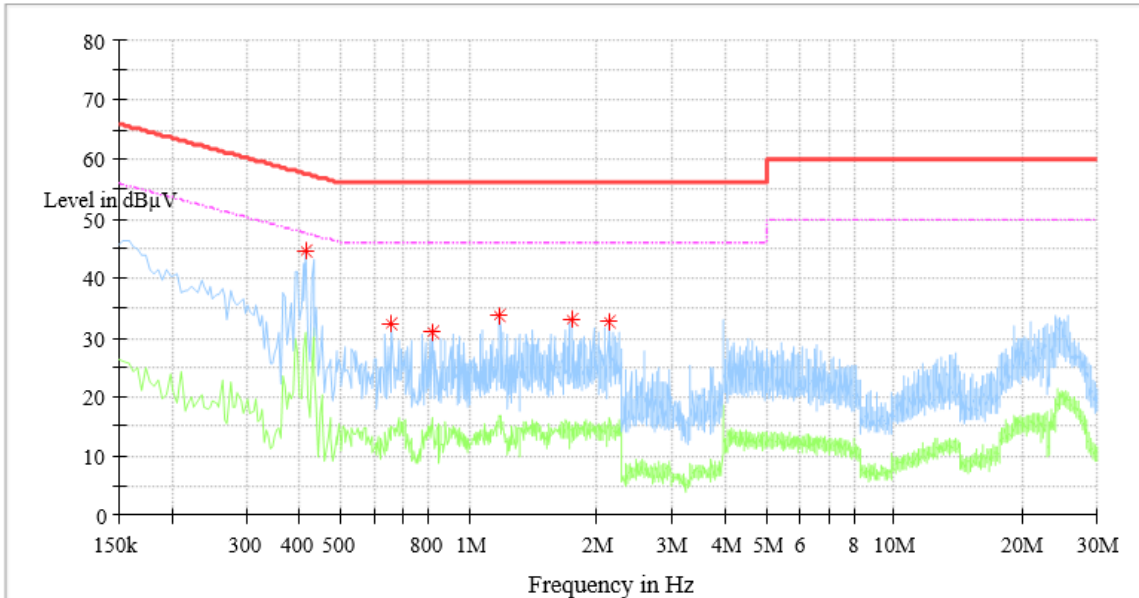

Final Result

Frequency (MHz)	QuasiPeak (dBµV)	Average (dBµV)	Limit (dBµV)	Margin (dB)	Line	Corr. (dB)
0.414000	44.54	---	57.57	13.03	N	10.3
0.658000	32.36	---	56.00	23.64	N	10.4
0.822000	31.00	---	56.00	25.00	N	10.4
1.178000	33.57	---	56.00	22.43	N	10.4
1.738000	32.92	---	56.00	23.08	N	10.4
2.142000	32.52	---	56.00	23.48	N	10.4

9.2 Conducted peak output power

Test Method

1. Use the following spectrum analyzer settings:
RBW > the 6 dB bandwidth of the emission being measured, VBW \geq 3RBW, Span \geq 3RBW
Sweep = auto, Detector function = peak, Trace = max hold.
2. Add a correction factor to the display.
3. Allow the trace to stabilize. Use the marker-to-peak function to set the marker to the peak of the emission. The indicated level is the peak output power.

Limits


According to §15.247 (b) (1), conducted peak output power limit as below:

Frequency Range MHz	Limit W	Limit dBm
2400-2483.5	≤ 1	≤ 30

Test result as below table


Frequency MHz	Conducted Peak Output Power dBm	Result
Bottom channel 2402MHz	-2.70	Pass
Middle channel 2440MHz	-1.73	Pass
Top channel 2480MHz	-0.82	Pass

Low channel 2402MHz

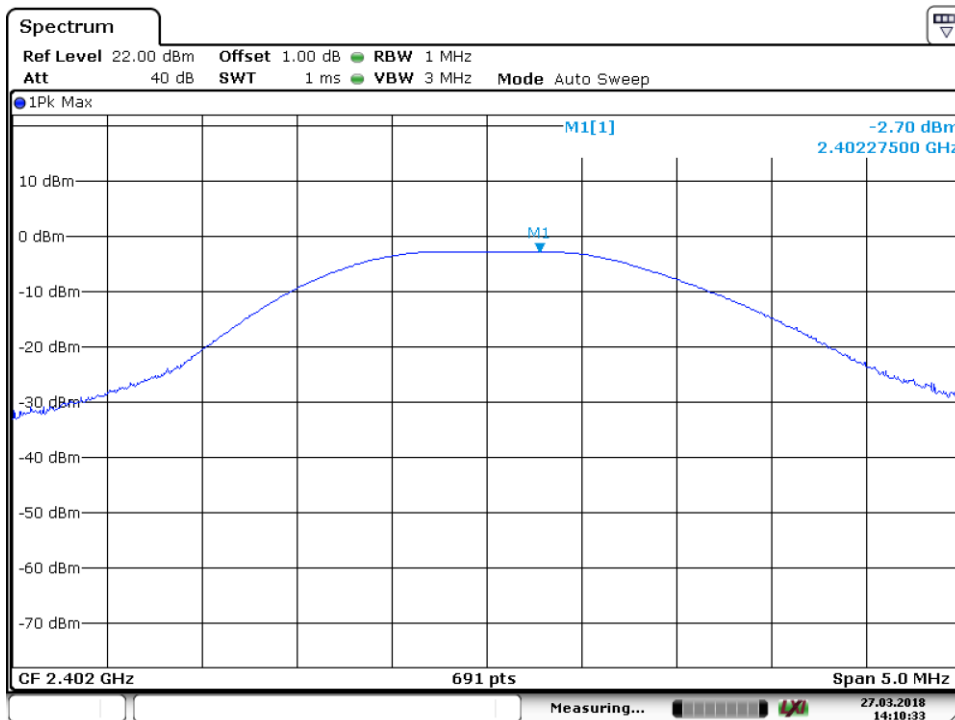


Date: 27.MAR.2018 14:10:33

Middle channel 2440MHz

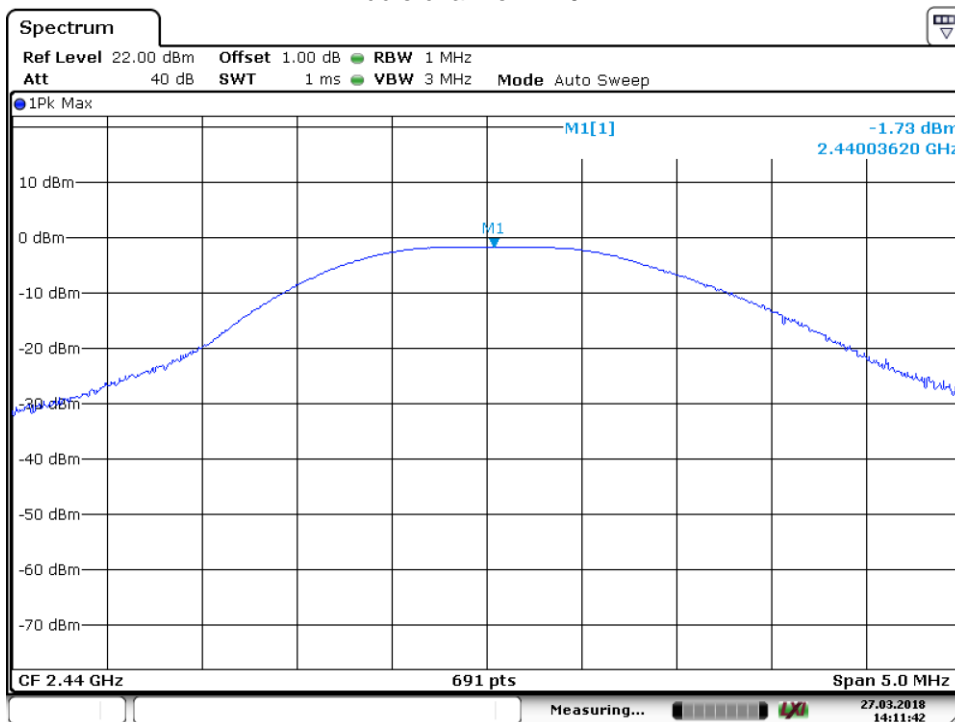

Date: 27.MAR.2018 14:11:42

High channel 2480MHz

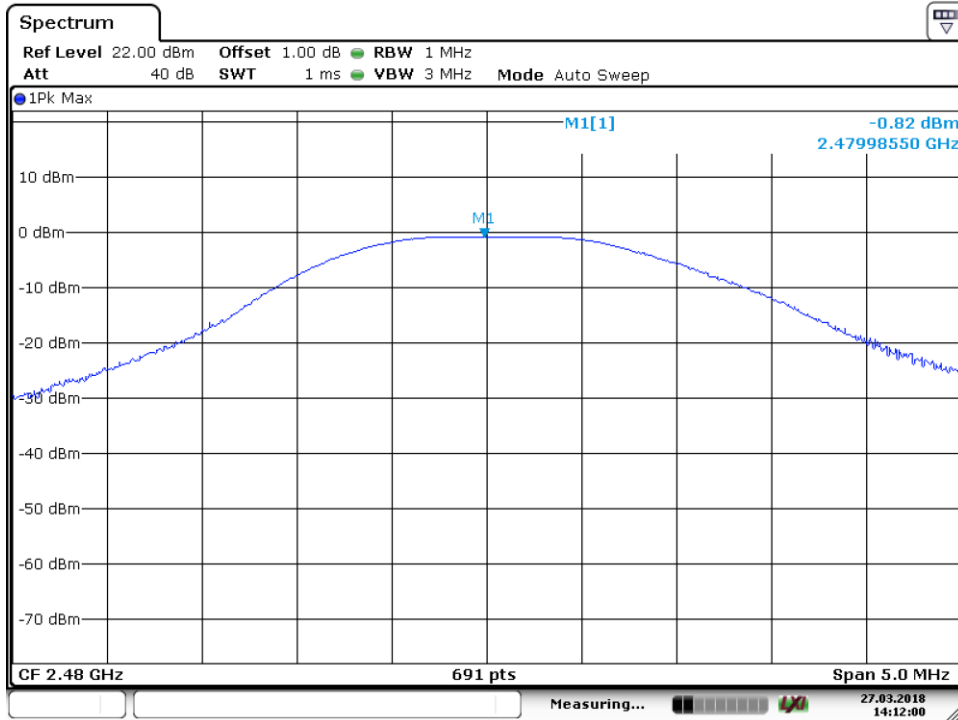

Date: 27.MAR.2018 14:12:00

9.3 Power spectral density

Test Method

This procedure shall be used if maximum peak conducted output power was used to demonstrate compliance:

1. Set analyzer center frequency to DTS channel center frequency. RBW=3kHz, VBW \geq 3RBW, Span=1.5 times DTS bandwidth, Detector=Peak, Sweep=auto, Trace= max hold.
2. Allow trace to fully stabilize, use the peak marker function to determine the maximum amplitude level within the RBW.
3. Repeat above procedures until other frequencies measured were completed.

Limit


Limit [dBm]

 ≤ 8

Test result


Frequency MHz	Power spectral density dBm	Result
Bottom channel 2402MHz	-16.54	Pass
Middle channel 2440MHz	-15.50	Pass
Top channel 2480MHz	-14.64	Pass

Low channel 2402MHz

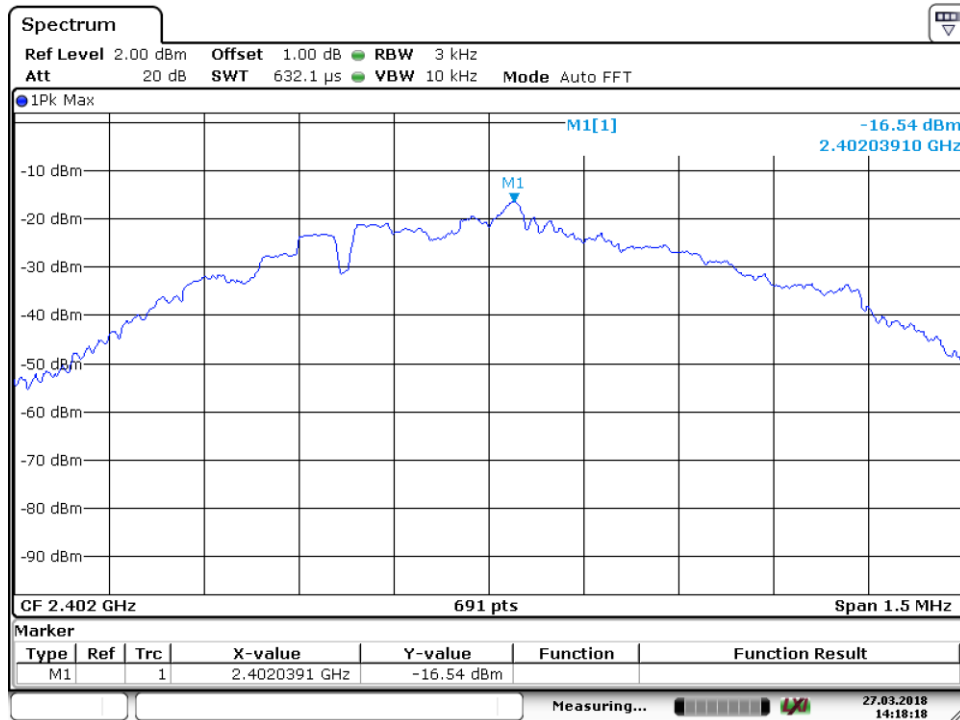


Date: 27. MAR.2018 14:18:18

Middle channel 2440MHz

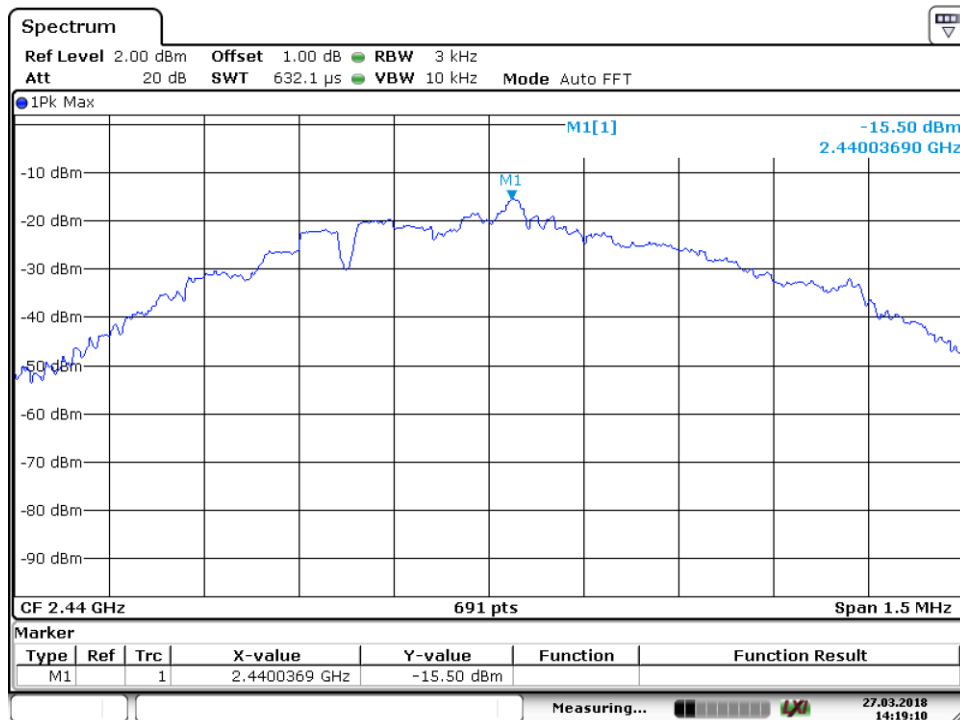

Date: 27. MAR.2018 14:19:10

High channel 2480MHz

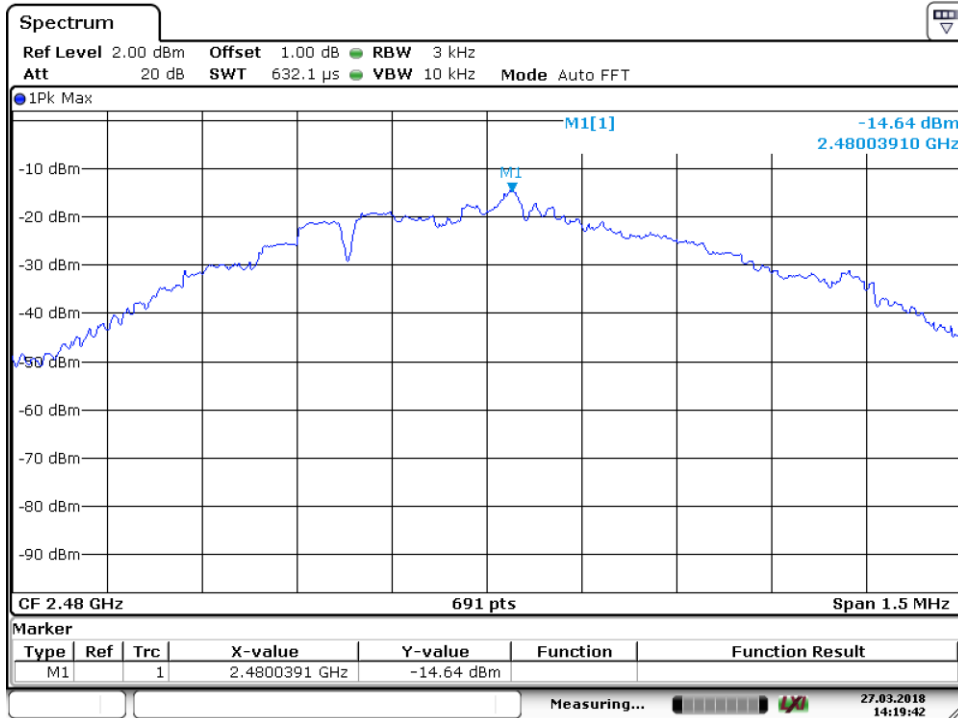

Date: 27.MAR.2018 14:19:42

9.4 6 dB Bandwidth and 99% Occupied Bandwidth

Test Method

1. Use the following spectrum analyzer settings:
RBW=100K, VBW \geq 3RBW, Sweep = auto, Detector function = peak, Trace = max hold
2. Use the automatic bandwidth measurement capability of an instrument, may be employed using the X dB bandwidth mode with X set to 6 dB, care shall be taken so that the bandwidth measurement is not influenced by any intermediate power nulls in the fundamental emission that might be \geq 6 dB.
3. Allow the trace to stabilize, record the X dB Bandwidth value.

Limit

Limit [kHz]


—————
≥500

Test result

Frequency MHz	6dB bandwidth kHz	99% bandwidth kHz	Result
Bottom channel 2402MHz	707.7	1150.51	Pass
Middle channel 2440MHz	703.3	1196.26	Pass
Top channel 2480MHz	703.3	1263.39	Pass


6 dB Bandwidth

Low channel 2402MHz

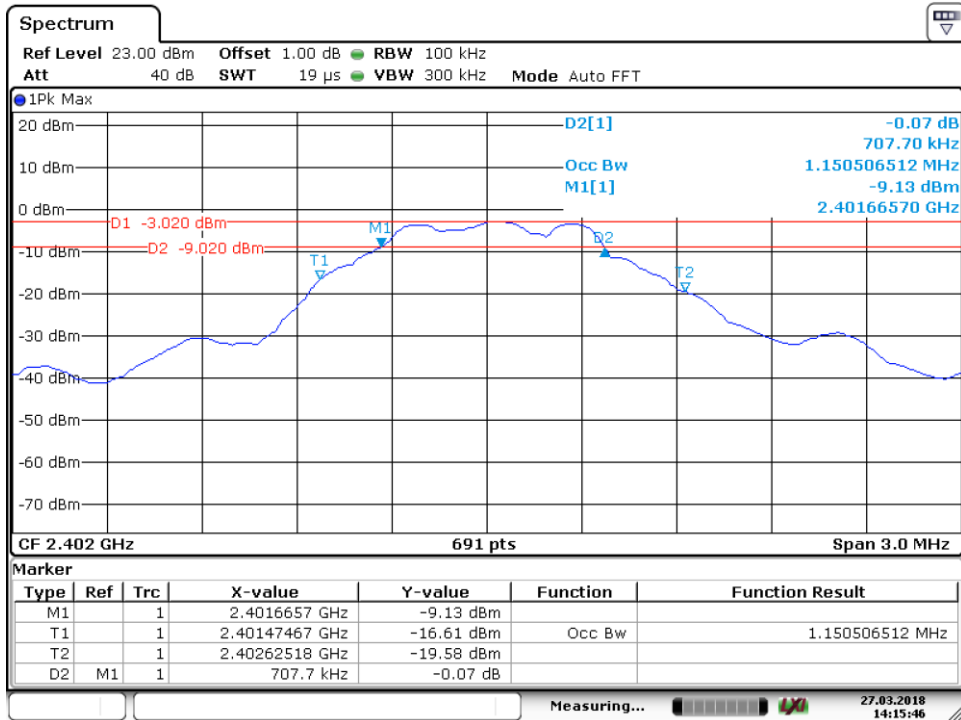


Date: 27. MAR.2018 14:15:47

Middle channel 2440MHz

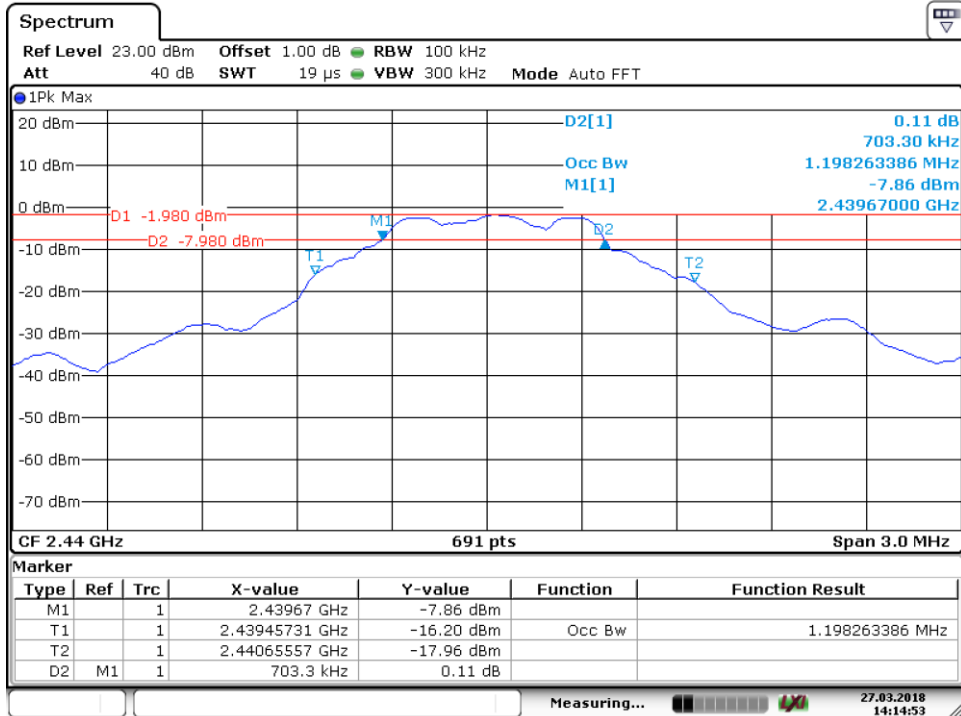

Date: 27. MAR.2018 14:14:53

High channel 2480MHz

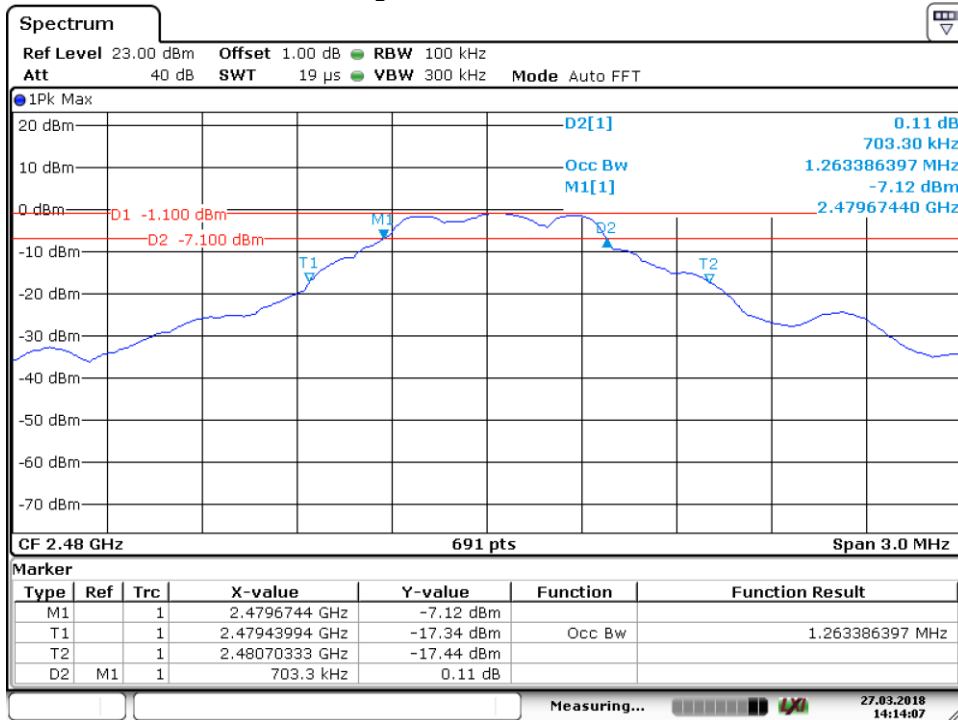

Date: 27.MAR.2018 14:14:07

9.5 Spurious RF conducted emissions

Test Method


1. Establish a reference level by using the following procedure:
 - a. Set RBW=100 kHz. VBW \geq 3RBW. Detector =peak, Sweep time = auto couple, Trace mode = max hold.
 - b. Allow trace to fully stabilize, use the peak marker function to determine the maximum PSD level.
2. Use the maximum PSD level to establish the reference level.
 - a. Set the center frequency and span to encompass frequency range to be measured.
 - b. Use the peak marker function to determine the maximum amplitude level. Ensure that the amplitude of all unwanted emissions outside of the authorized frequency band (excluding restricted frequency bands) are attenuated by at least the minimum requirements, report the three highest emissions relative to the limit.
3. Repeat above procedures until other frequencies measured were completed.

Limit


Frequency Range MHz	Limit (dBc)
30-25000	-20

Spurious RF conducted emissions

2402MHz

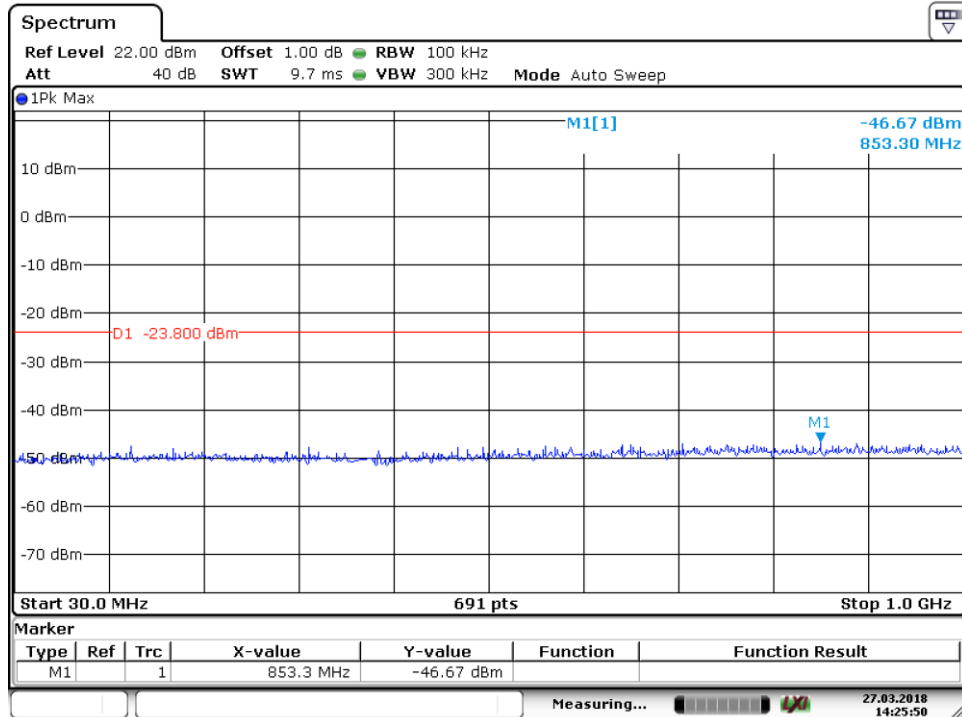


Date: 27. MAR.2018 14:25:50

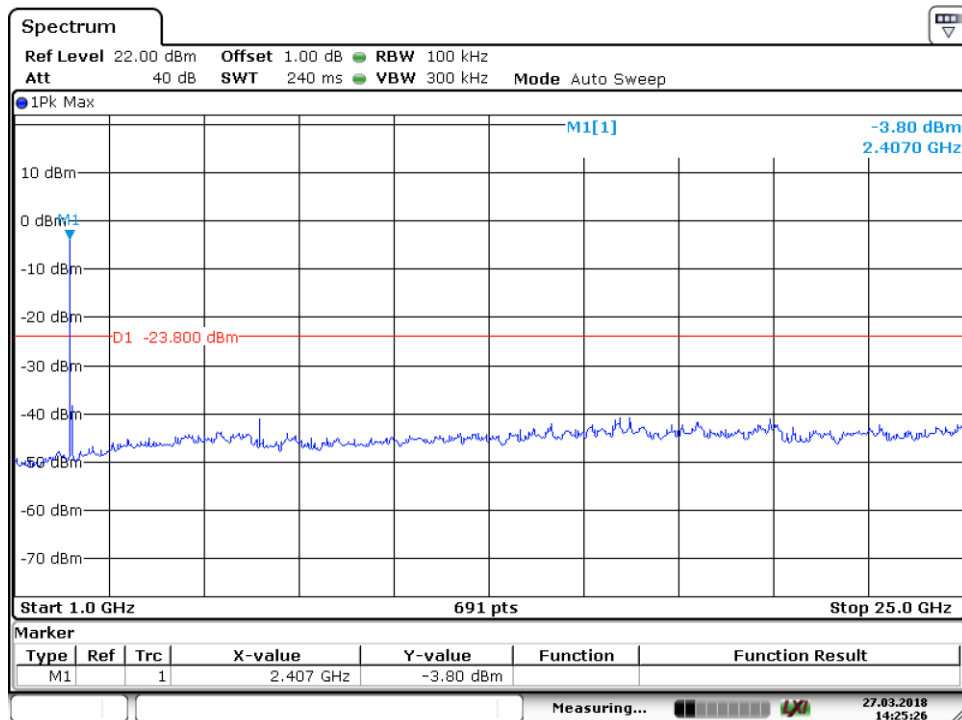


Date: 27. MAR.2018 14:25:26

2440MHz

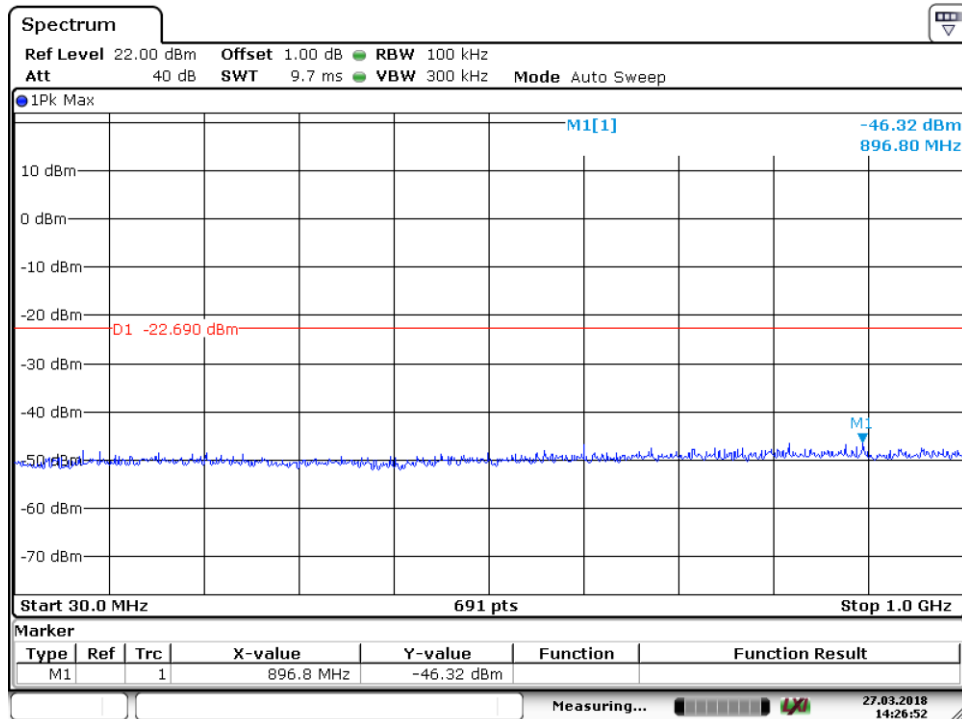


Date: 27.MAR.2018 14:26:53

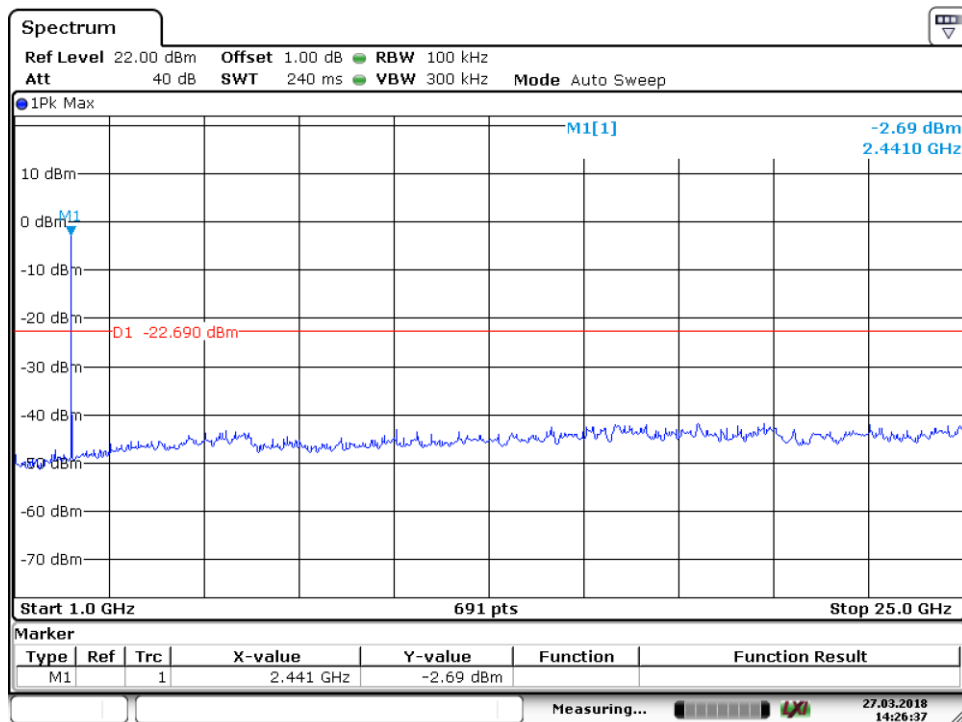


Date: 27.MAR.2018 14:26:37

2480MHz

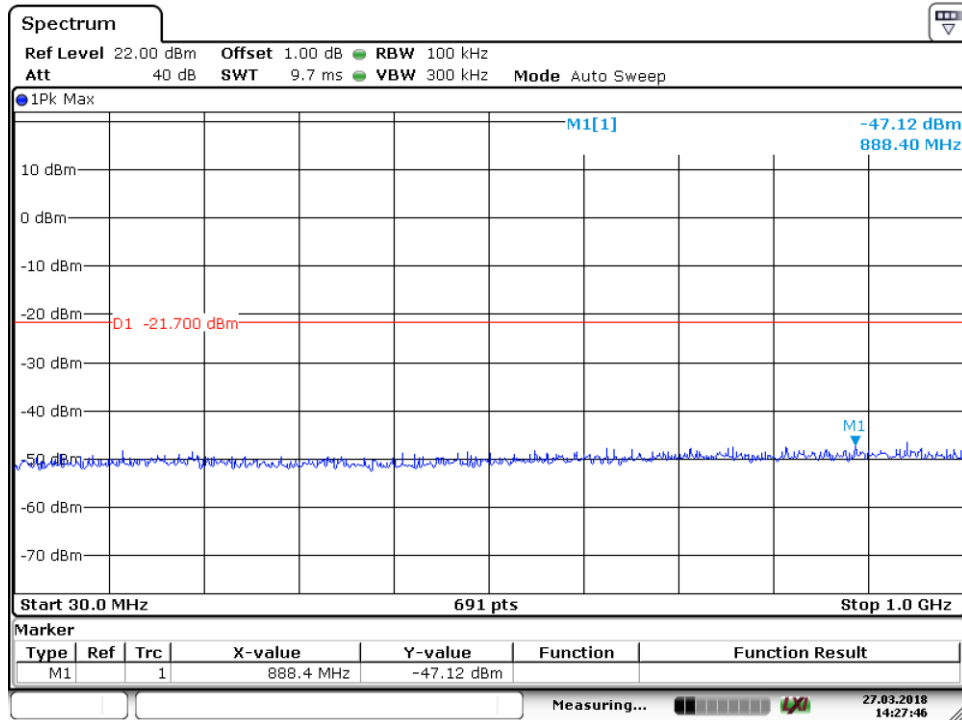

Date: 27.MAR.2018 14:27:46

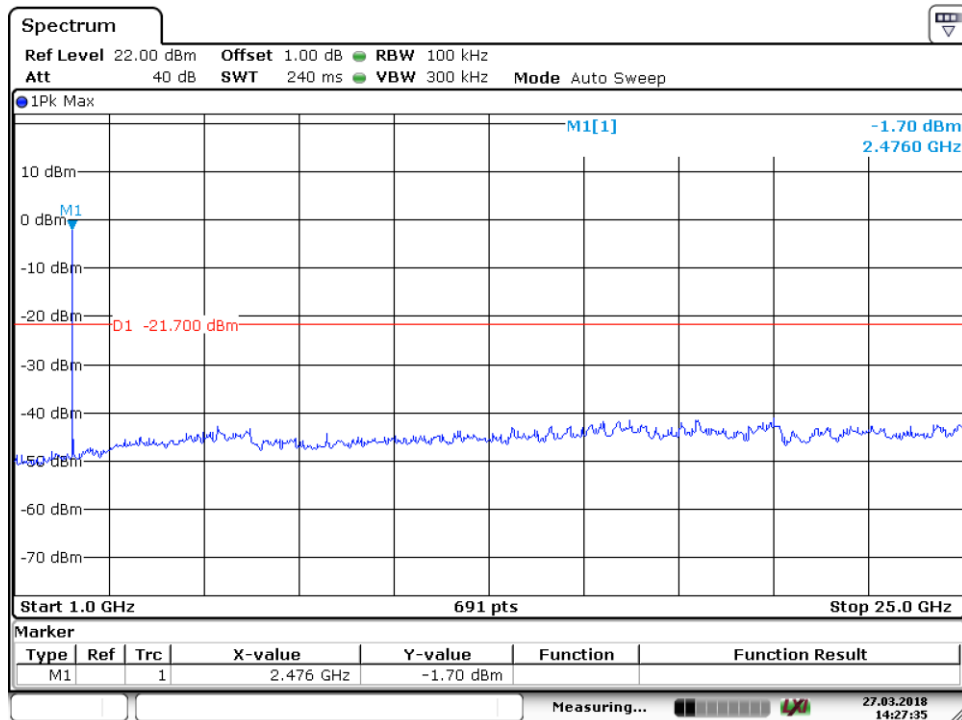

Date: 27.MAR.2018 14:27:35

9.6 Band edge

Test Method


- 1 Use the following spectrum analyzer settings:
Span = wide enough to capture the peak level of the in-band emission and all spurious
RBW = 100 kHz, VBW \geq RBW, Sweep = auto, Detector function = peak, Trace = max hold.
- 2 Allow the trace to stabilize, use the peak and delta measurement to record the result.
- 3 The level displayed must comply with the limit specified in this Section.

Limit

Frequency Range MHz	Limit (dBc)
30-25000	-20


Band edge testing

2402MHz

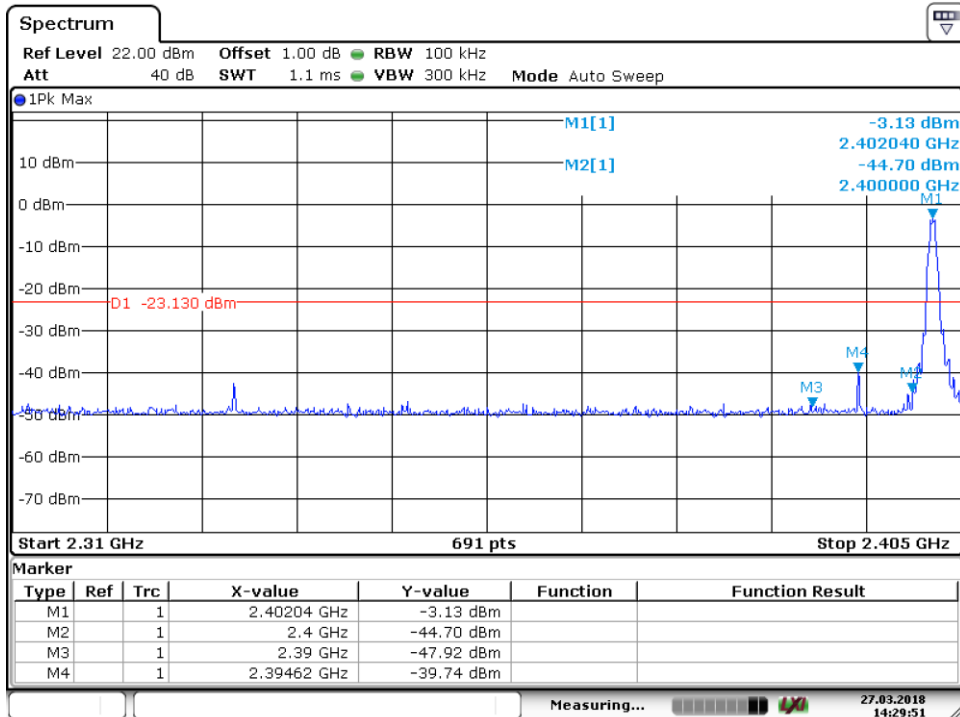

Date: 27.MAR.2018 14:29:51

2480MHz

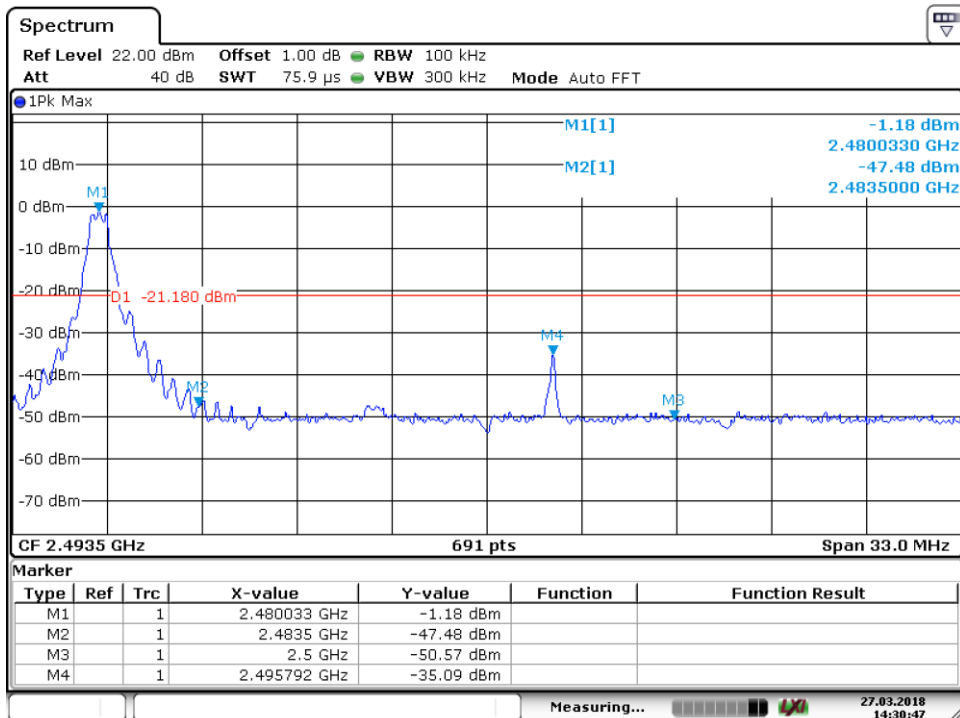

Date: 27.MAR.2018 14:30:47

9.7 Spurious radiated emissions for transmitter

Test Method

- 1: The EUT was placed on a turn table which is 1.5m above ground plane for above 1GHz and 0.8m above ground for below 1GHz at 3 meter chamber room for test. The table was rotated 360 degrees to determine the position of the highest radiation.
- 2: The EUT was set 3 meters away from the interference – receiving antenna, which was mounted on the top of a variable – height antenna tower.
- 3: The height of antenna is varied from one meter to four meters above the ground to determine the maximum value of the field strength. Both horizontal and vertical polarizations of the antenna are set to make the measurement.
- 4: For each suspected emission, the EUT was arranged to its worst case and then the antenna was tuned to heights from 1 meter to 4 meters and the rotatable table was turned from 0 degrees to 360 degrees to find the maximum reading.
- 5: Use the following spectrum analyzer settings According to C63.10:

For Above 1GHz

Span = wide enough to capture the peak level of the in-band emission and all spurious
RBW = 1MHz, VBW \geq RBW for peak measurement and VBW = 10Hz for average measurement, Sweep = auto, Detector function = peak, Trace = max hold.

For Below 1GHz

Use the following spectrum analyzer settings:

Span = wide enough to capture the peak level of the in-band emission and all spurious
RBW = 100 KHz, VBW \geq RBW for peak measurement, Sweep = auto, Detector function = peak, Trace = max hold.

Note:

- 1: The resolution bandwidth and video bandwidth of test receiver/spectrum analyzer is 120 KHz for Quasi-peak detection (QP) at frequency below 1GHz.
- 2: The resolution bandwidth of test receiver/spectrum analyzer is 1MHz and the video bandwidth is 3MHz for peak detection (PK) at frequency above 1GHz.
- 3: The resolution bandwidth of test receiver/spectrum analyzer is 1MHz and the video bandwidth is 3MHz for RMS Average ((duty cycle < 98%) for Average detection (AV) at frequency above 1GHz, then the measurement results was added to a correction factor ($20\log(1/\text{duty cycle})$).
- 4: The resolution bandwidth of test receiver/spectrum analyzer is 1MHz and the video bandwidth is 10Hz (duty cycle > 98%) for Average detection (AV) at frequency above 1GHz.

Limit

The radio emission outside the operating frequency band shall be at least 20 dB below that in the 100 kHz bandwidth within the band that contains the highest level of the desired power. Radiated emissions which fall in the restricted bands, as defined in section 15.205, must comply with the radiated emission limits specified in section 15.209.

Frequency MHz	Field Strength uV/m	Field Strength dB μ V/m	Detector
30-88	100	40	QP
88-216	150	43.5	QP
216-960	200	46	QP
960-1000	500	54	QP
Above 1000	500	54	AV
Above 1000	5000	74	PK

Spurious radiated emissions for transmitter

According to C63.10, if the peak (or quasi-peak) measured value complies with the average limit, it is unnecessary to perform an average measurement, so AV emission value did not show in below table if the peak value complies with average limit.

Transmitting spurious emission test result as below:

Below 1GHz

Frequency Band	Frequency	Emission Level	Polarization	Limit	Detector	Margin	Correct factor	Result
	MHz	dBuV/m		dBuV/m				
30-1000MHz	239.897222	41.13	H	46.00	QP	4.87	-27.3	Pass
	311.785000	38.99	H	46.00	QP	7.01	-24.1	Pass
	359.800000	34.38	H	46.00	QP	11.62	-23.8	Pass
	504.006667	31.25	H	46.00	QP	14.75	-21.6	Pass
	56.944444	31.14	V	40.00	QP	8.86	-25.9	Pass
	71.925556	27.37	V	40.00	QP	12.63	-30.9	Pass
	239.897222	37.33	V	46.00	QP	8.67	-27.7	Pass
	311.838889	37.21	V	46.00	QP	18.05	-15.0	Pass

Above 1GHz

Low channel 2402MHz Test Result

Frequency Band	Frequency	Emission Level	Polarization	Limit	Detector	Margin	Correct factor	Result
	MHz	dBuV/m		dBuV/m				
1000-25000MHz	1242.375000	30.99	H	74	PK	43.01	-12.2	Pass
	4803.750000	45.88	H	74	PK	28.12	2.5	Pass
	7206.093750	46.84	H	74	PK	27.16	5.2	Pass
	1244.375000	29.86	V	74	PK	44.14	-12.1	Pass
	4803.750000	47.26	V	74	PK	26.74	2.6	Pass
	7206.093750	43.15	V	74	PK	30.85	5.4	Pass

Middle channel 2440MHz Test Result

Frequency Band	Frequency	Emission Level	Polarization	Limit	Detector	Margin	Correct factor	Result
	MHz	dBuV/m		dBuV/m				
1000-25000MHz	1247.062500	30.18	H	74	PK	43.82	-12.2	Pass
	4879.687500	44.80	H	74	PK	29.20	2.5	Pass
	1255.125000	30.78	V	74	PK	43.22	-11.9	Pass
	4879.687500	48.45	V	74	PK	25.55	2.6	Pass

High channel 2480MHz Test Result

Frequency Band	Frequency	Emission Level	Polarization	Limit	Detector	Margin	Correct factor	Result
	MHz	dBuV/m		dBμV/m		dB	(dB)	
1000-25000MHz	1240.000000	32.85	H	74	PK	41.15	-12.2	Pass
	4959.843750	47.38	H	74	PK	26.62	2.7	Pass
	1240.000000	33.21	V	74	PK	40.79	-12.1	Pass
	4959.843750	47.84	V	74	PK	26.16	2.8	Pass

Remark:

- (1) "*" means the emission(s) appear within the restrict bands shall follow the requirement of section 15.205.
- (2) Data of measurement within this frequency range shown "--" in the table above means the reading of emissions are the noise floor or attenuated more than 10dB below the permissible limits or the field strength is too small to be measured.
- (3) Above 1GHz: Corrector factor = Antenna Factor + Cable Loss- Amplifier Gain
Below 1GHz: Corrector factor = Antenna Factor + Cable Loss

10 Test Equipment List

List of Test Instruments

Radiated Emission Test

Description	Manufacturer	Model no.	Serial no.	cal. due date
EMI Test Receiver	Rohde & Schwarz	ESR 26	101269	2018-7-14
Trilog Super Broadband Test Antenna	Schwarzbeck	VULB 9163	707	2018-7-14
Horn Antenna	Rohde & Schwarz	HF907	102294	2018-7-14
Pre-amplifier	Rohde & Schwarz	SCU 18	102230	2018-7-14
Signal Generator	Rohde & Schwarz	SMY01	839369/005	2018-7-7
Attenuator	Agilent	8491A	MY39264334	2018-7-7
3m Semi-anechoic chamber	TDK	9X6X6	----	2020-7-7
Test software	Rohde & Schwarz	EMC32	Version 9.15.00	N/A

Conducted Emission Test

Description	Manufacturer	Model no.	Serial no.	cal. due date
EMI Test Receiver	Rohde & Schwarz	ESR 3	101782	2018-7-14
LISN	Rohde & Schwarz	ENV4200	100249	2018-7-14
LISN	Rohde & Schwarz	ENV432	101318	2018-7-14
LISN	Rohde & Schwarz	ENV216	100326	2018-7-14
ISN	Rohde & Schwarz	ENY81	100177	2018-7-14
ISN	Rohde & Schwarz	ENY81-CA6	101664	2018-7-14
High Voltage Probe	Rohde & Schwarz	TK9420(VT9420)	9420-584	2018-7-14
RF Current Probe	Rohde & Schwarz	EZ-17	100816	2018-7-14
Attenuator	Shanghai Huaxiang	TS2-26-3	080928189	2018-7-7
Test software	Rohde & Schwarz	EMC32	Version9.15.00	N/A

TS8997 Test System

Description	Manufacturer	Model no.	Serial no.	cal. due date
Signal Generator	Rohde & Schwarz	SMB100A	108272	2018-7-7
Signal Analyzer	Rohde & Schwarz	FSV40	101030	2018-7-7
Vector Signal Generator	Rohde & Schwarz	SMU 200A	105324	2018-7-7
RF Switch Module	Rohde & Schwarz	OSP120/OSP-B157	101226/100851	2018-7-7
Power Splitter	Weinschel	1580	SC319	2018-7-7
10dB Attenuator	Weinschel	56-10	58764	2018-7-14
10dB Attenuator	R&S	DNF	DNF-001	2018-7-14
10dB Attenuator	R&S	DNF	DNF-002	2018-7-14
10dB Attenuator	R&S	DNF	DNF-003	2018-7-14
10dB Attenuator	R&S	DNF	DNF-004	2018-7-14
Test software	Rohde & Schwarz	EMC32	Version 9.26.01	N/A

11 System Measurement Uncertainty

For a 95% confidence level, the measurement expanded uncertainties for defined systems, in accordance with the recommendations of ISO 17025 were:

System Measurement Uncertainty	
Test Items	Extended Uncertainty
Uncertainty for Conducted Emission 150kHz-30MHz (for test using High Voltage Probe TK9420(VT9420))	2.92 dB
Uncertainty for Radiated Spurious Emission 25MHz-3000MHz	Horizontal: 4.98dB; Vertical: 5.06dB;
Uncertainty for Radiated Spurious Emission 3000MHz-18000MHz	Horizontal: 4.95dB; Vertical: 4.94dB;
Uncertainty for Radiated Spurious Emission 18000MHz-40000MHz	Horizontal: 5.14dB; Vertical: 5.12dB;
Uncertainty for Conducted RF test with TS 8997	Power level test involved: 2.06dB Frequency test involved: 1.16x10 ⁻⁷