

Test Laboratory: KWC

K33BIC04_E_Dipole_1880_121109

Communication System: CW-1880, Frequency: 1880 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section


DASY4 Configuration:

Probe: ER3DV6 - SN2282, ConvF(1, 1, 1), Calibrated: 8/14/2009
 Sensor-Surface: 0mm (Fix Surface),
 Electronics: DAE4 Sn530, Calibrated: 3/12/2009
 Measurement SW: DASY4, V4.7 Build 80
 Postprocessing SW: SEMCAD, V1.8 Build 186
Temperature: Room T = 21.8 +/- 1 deg C, Liquid T = 22.0 +/- 1 deg C

E Scan 1880 - measurement distance from the probe sensor center to CD1880 Dipole = 10mm/Hearing Aid

Compatibility Test (41x181x1): Measurement grid: dx=5mm, dy=5mm

Probe Modulation Factor = 1.00
 Device Reference Point: 0.000, 0.000, -6.30 mm
 Reference Value = 152.2 V/m; Power Drift = -0.017 dB
 Maximum value of Total (interpolated) = 135.7 V/m

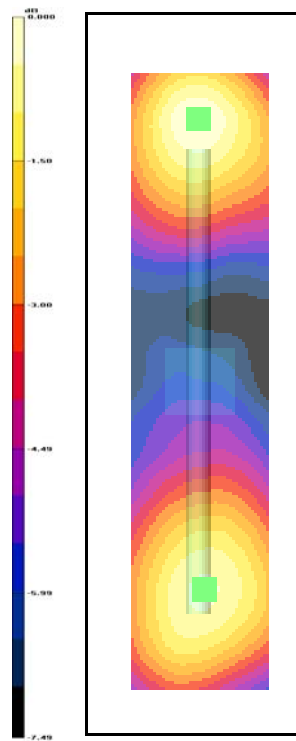

0 dB = 135.7V/m


Test Laboratory: KWC

K33BIC04_H3DV6_Dipole_1880_121109

Communication System: CW-1880, Frequency: 1880 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section
DASY4 Configuration:
 Probe: H3DV6 - SN6123, , Calibrated: 7/16/2009
 Sensor-Surface: 0mm (Fix Surface),
 Electronics: DAE4 Sn530, Calibrated: 3/12/2009
 Measurement SW: DASY4, V4.7 Build 80
 Postprocessing SW: SEMCAD, V1.8 Build 186
Temperature: Room T = 21.8 +/- 1 deg C, Liquid T = 22.0 +/- 1 deg C

H Scan - measurement distance from the probe sensor center to CD1880 Dipole = 10mm/Hearing Aid Compatibility Test (41x181x1):

Measurement grid: dx=5mm, dy=5mm
 Probe Modulation Factor = 1.00
 Device Reference Point: 0.000, 0.000, -6.30 mm
 Reference Value = 0.498 A/m; Power Drift = -0.077 dB
 Maximum value of Total (interpolated) = 0.466 A/m

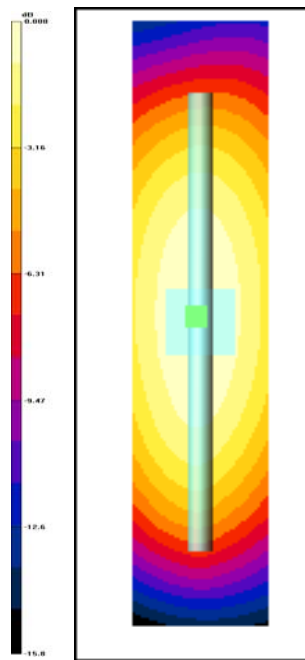

0 dB = 0.466A/m