

Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

CDMA 800 Channel 1013

Date: 01/13/2011

Communication System: CDMA_Triband, Frequency: 824.7 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2341 Probe: H3DV5 - SN6029, ConvF(1, 1, 1), Calibrated: 7/12/2010 Calibrated: 7/16/2010

Sensor-Surface: (Fix Surface),
 Electronics: DAE4 Sn527, Calibrated: 7/8/2010
 Measurement SW: DASY4, V4.7 Build 80
 Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 +/- 1 deg C, Liquid T = 22.0 +/- 1 deg C

CELL_1013/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 103.9 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 142.1 V/m; Power Drift = -0.185 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1 96.0 M4	Grid 2 102.2 M4	Grid 3 96.1 M4
Grid 4 97.4 M4	Grid 5 103.9 M4	Grid 6 98.2 M4
Grid 7 94.7 M4	Grid 8 100.1 M4	Grid 9 93.9 M4

CELL_1013/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.141 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.100 A/m; Power Drift = 0.012 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1 0.191 M4	Grid 2 0.132 M4	Grid 3 0.075 M4
Grid 4 0.191 M4	Grid 5 0.129 M4	Grid 6 0.077 M4
Grid 7 0.202 M4	Grid 8 0.141 M4	Grid 9 0.085 M4



Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

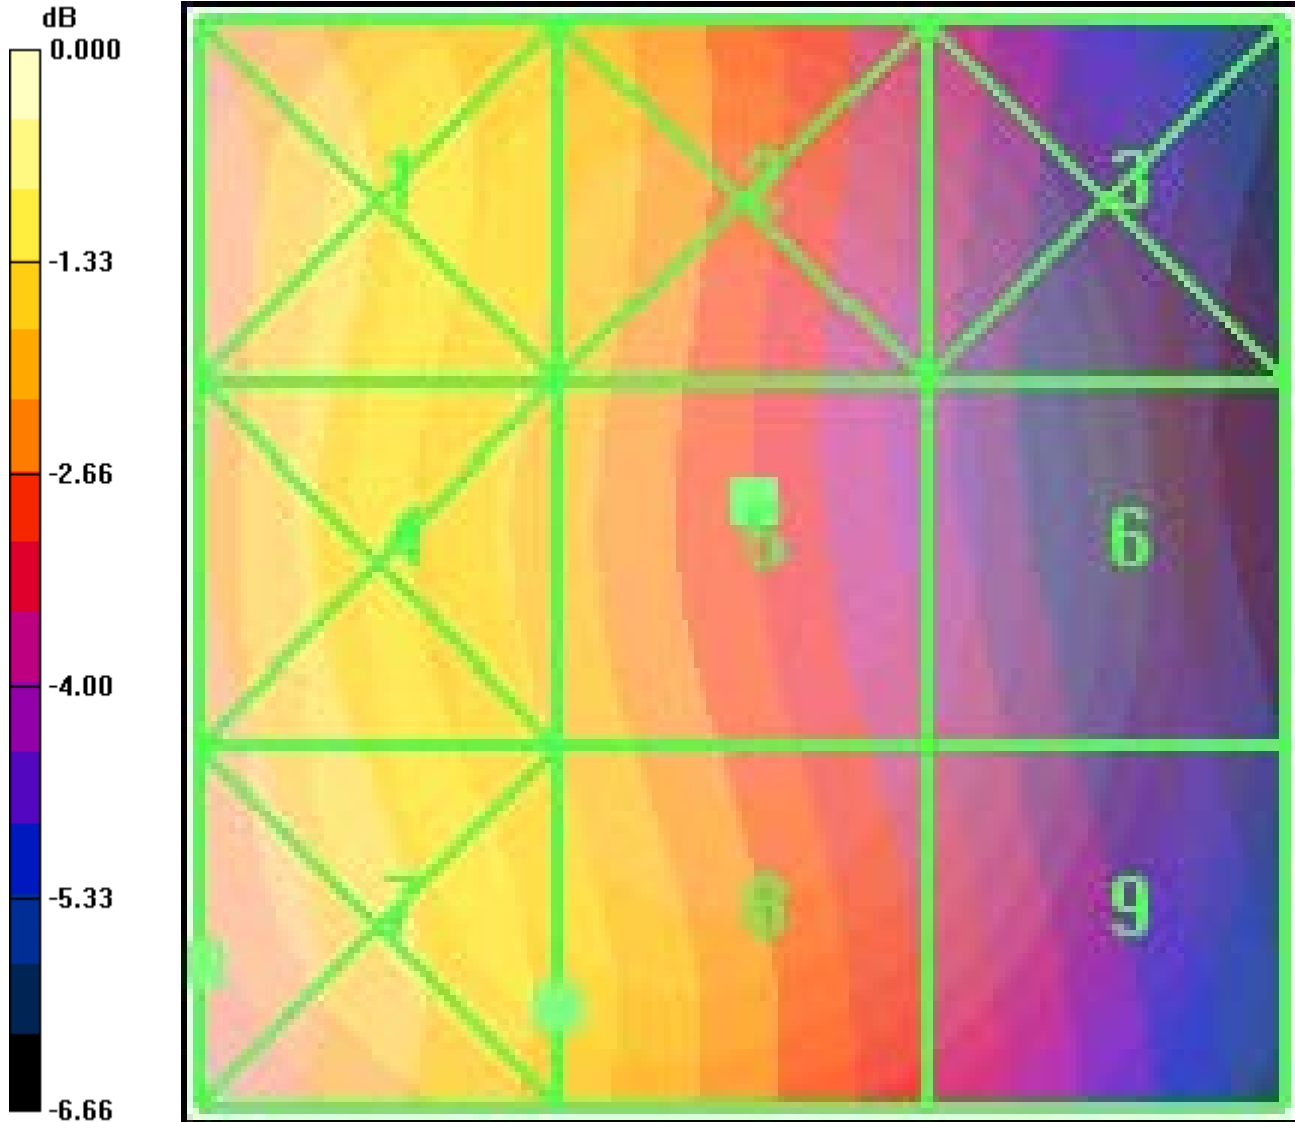

0 dB = 103.9V/m

Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

CDMA 800 Channel 383

Date: 01/13/2011

Communication System: CDMA_Triband, Frequency: 836.49 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2341 Probe: H3DV5 - SN6029, ConvF(1, 1, 1), Calibrated: 7/12/2010 Calibrated: 7/16/2010

Sensor-Surface: (Fix Surface),
 Electronics: DAE4 Sn527, Calibrated: 7/8/2010
 Measurement SW: DASY4, V4.7 Build 80
 Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8̄ 1 deg C, Liquid T = 22.0̄ 1 deg C

CELL_383/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 89.8 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 115.8 V/m; Power Drift = 0.152 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1 82.0 M4	Grid 2 88.4 M4	Grid 3 84.0 M4
Grid 4 83.2 M4	Grid 5 89.8 M4	Grid 6 85.7 M4
Grid 7 80.5 M4	Grid 8 86.3 M4	Grid 9 82.2 M4

CELL_383/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.111 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.076 A/m; Power Drift = -0.088 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1 0.159 M4	Grid 2 0.111 M4	Grid 3 0.068 M4
Grid 4 0.150 M4	Grid 5 0.101 M4	Grid 6 0.058 M4
Grid 7 0.154 M4	Grid 8 0.106 M4	Grid 9 0.064 M4



Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

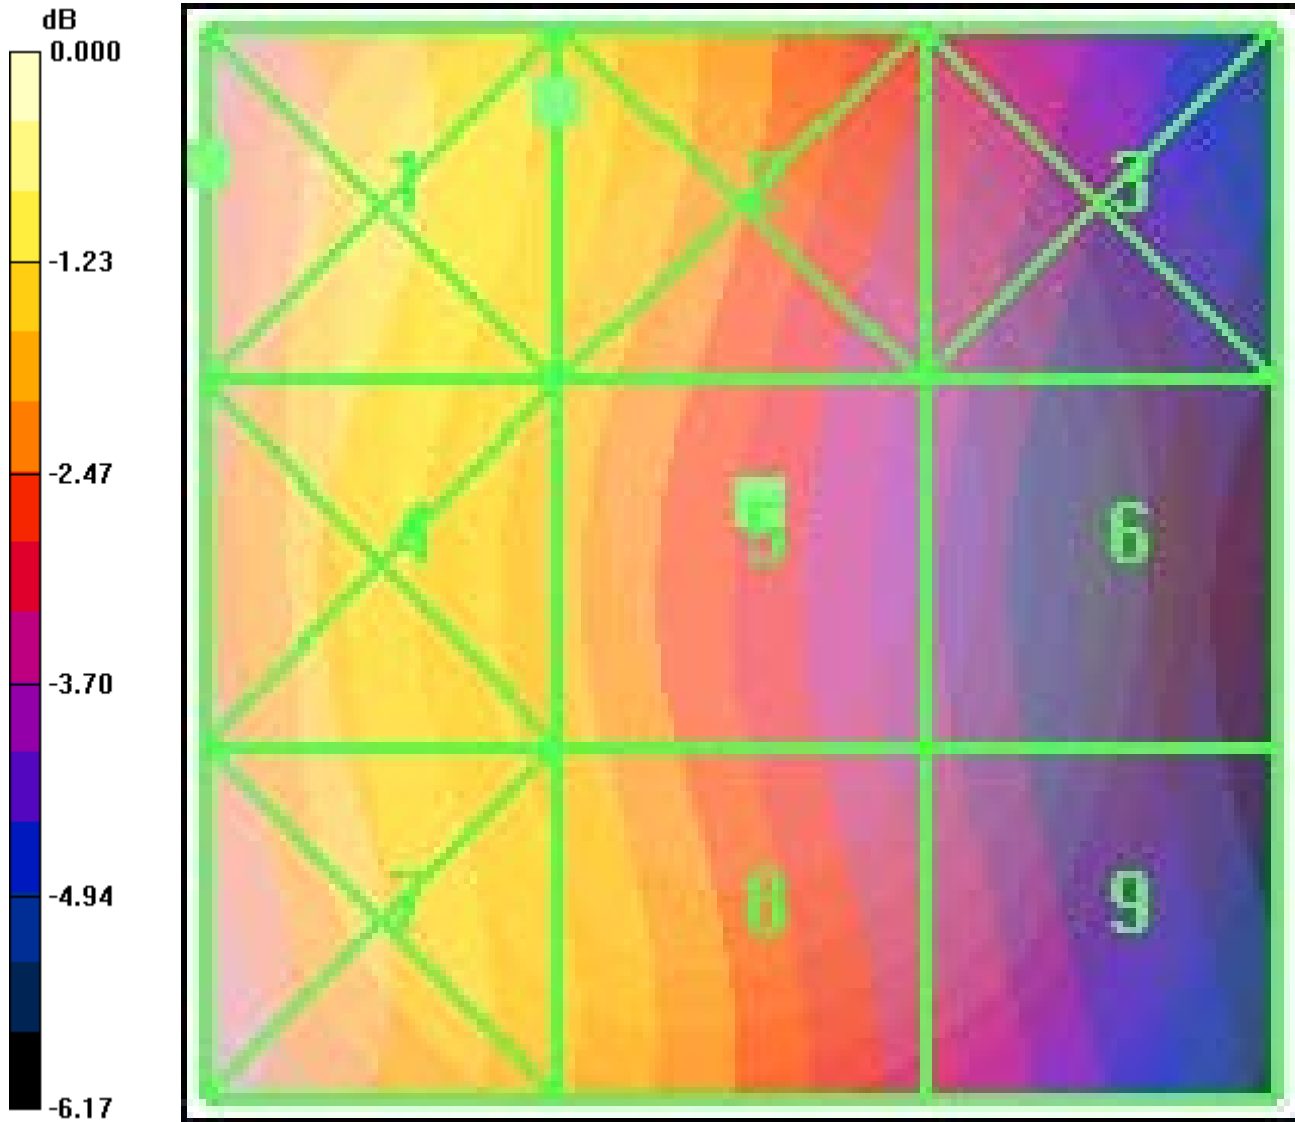

0 dB = 89.8V/m

Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

CDMA 800 Channel 777

Date: 01/13/2011

Communication System: CDMA_Triband, Frequency: 848.31 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2341 Probe: H3DV5 - SN6029, ConvF(1, 1, 1), Calibrated: 7/12/2010 Calibrated: 7/16/2010

Sensor-Surface: (Fix Surface),
 Electronics: DAE4 Sn527, Calibrated: 7/8/2010
 Measurement SW: DASY4, V4.7 Build 80
 Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 ± 1 deg C, Liquid T = 22.0 ± 1 deg C

CELL_777/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 76.6 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 103.5 V/m; Power Drift = 0.133 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1 70.4 M4	Grid 2 75.8 M4	Grid 3 72.7 M4
Grid 4 70.9 M4	Grid 5 76.6 M4	Grid 6 74.9 M4
Grid 7 67.5 M4	Grid 8 72.7 M4	Grid 9 69.6 M4

CELL_777/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.101 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.067 A/m; Power Drift = -0.026 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1 0.135 M4	Grid 2 0.089 M4	Grid 3 0.051 M4
Grid 4 0.133 M4	Grid 5 0.087 M4	Grid 6 0.052 M4
Grid 7 0.143 M4	Grid 8 0.101 M4	Grid 9 0.065 M4



Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

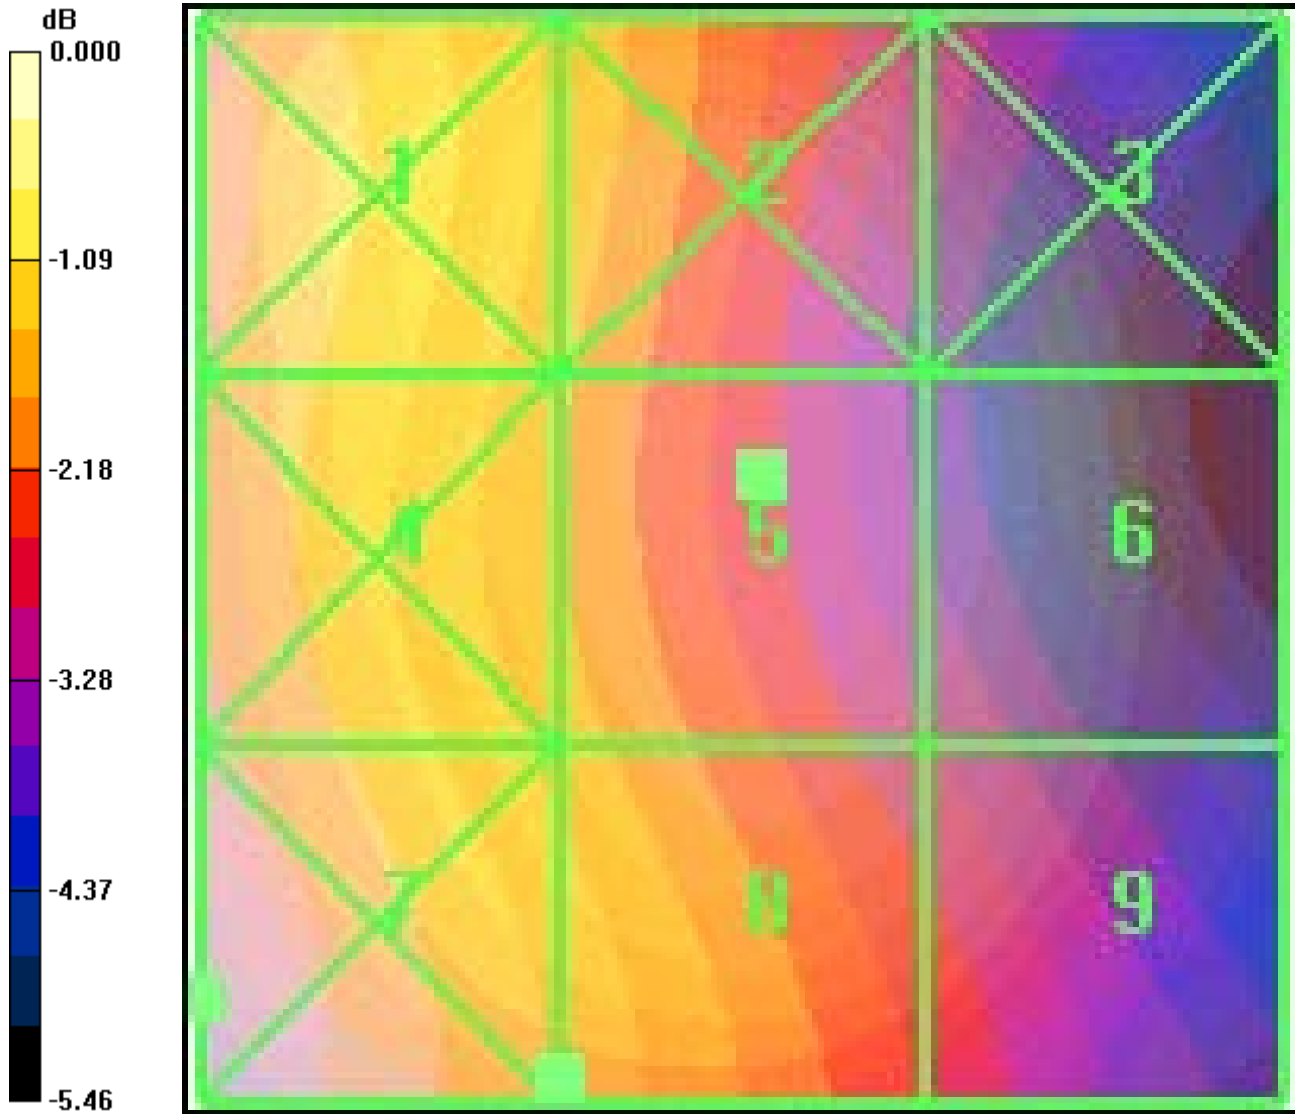


0 dB = 76.6V/m



Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

CDMA 800 Channel 1013 (360) E roll

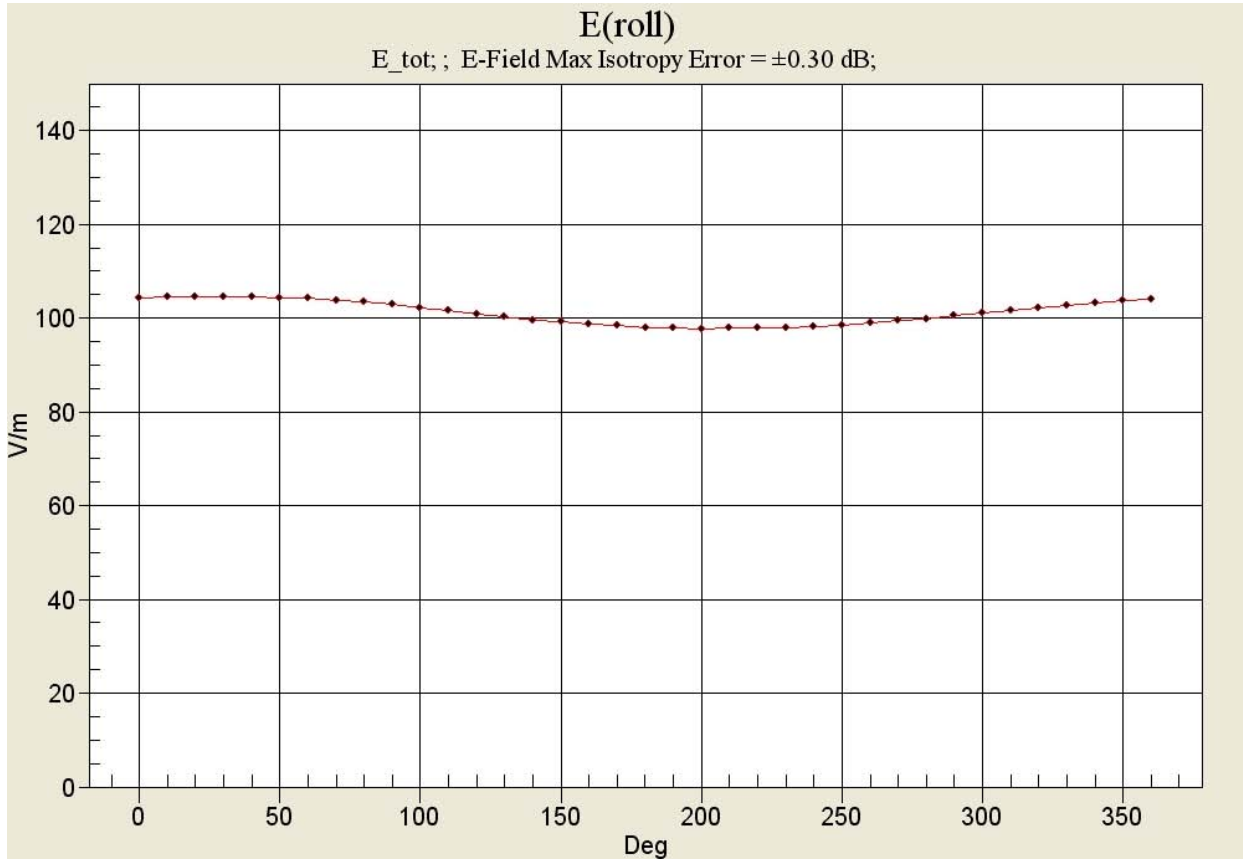

Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

CDMA 1700 Channel 25

Date: 01/13/2011

Communication System: CDMA_Triband, Frequency: 1711.25 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2341 Probe: H3DV5 - SN6029, ConvF(1, 1, 1), Calibrated: 7/12/2010 Calibrated: 7/16/2010

Sensor-Surface: (Fix Surface),

Electronics: DAE4 Sn527, Calibrated: 7/8/2010

Measurement SW: DASY4, V4.7 Build 80

Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8̄ 1 deg C, Liquid T = 22.0̄ 1 deg C

AWS_25/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 46.6 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 56.1 V/m; Power Drift = 0.019 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1 28.5 M4	Grid 2 38.7 M4	Grid 3 38.5 M4
Grid 4 39.6 M4	Grid 5 46.6 M4	Grid 6 45.5 M4
Grid 7 45.0 M4	Grid 8 47.3 M4	Grid 9 45.7 M4

AWS_25/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.118 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.095 A/m; Power Drift = 0.099 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1 0.116 M4	Grid 2 0.099 M4	Grid 3 0.072 M4
Grid 4 0.148 M4	Grid 5 0.118 M4	Grid 6 0.077 M4
Grid 7 0.166 M4	Grid 8 0.131 M4	Grid 9 0.083 M4



Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

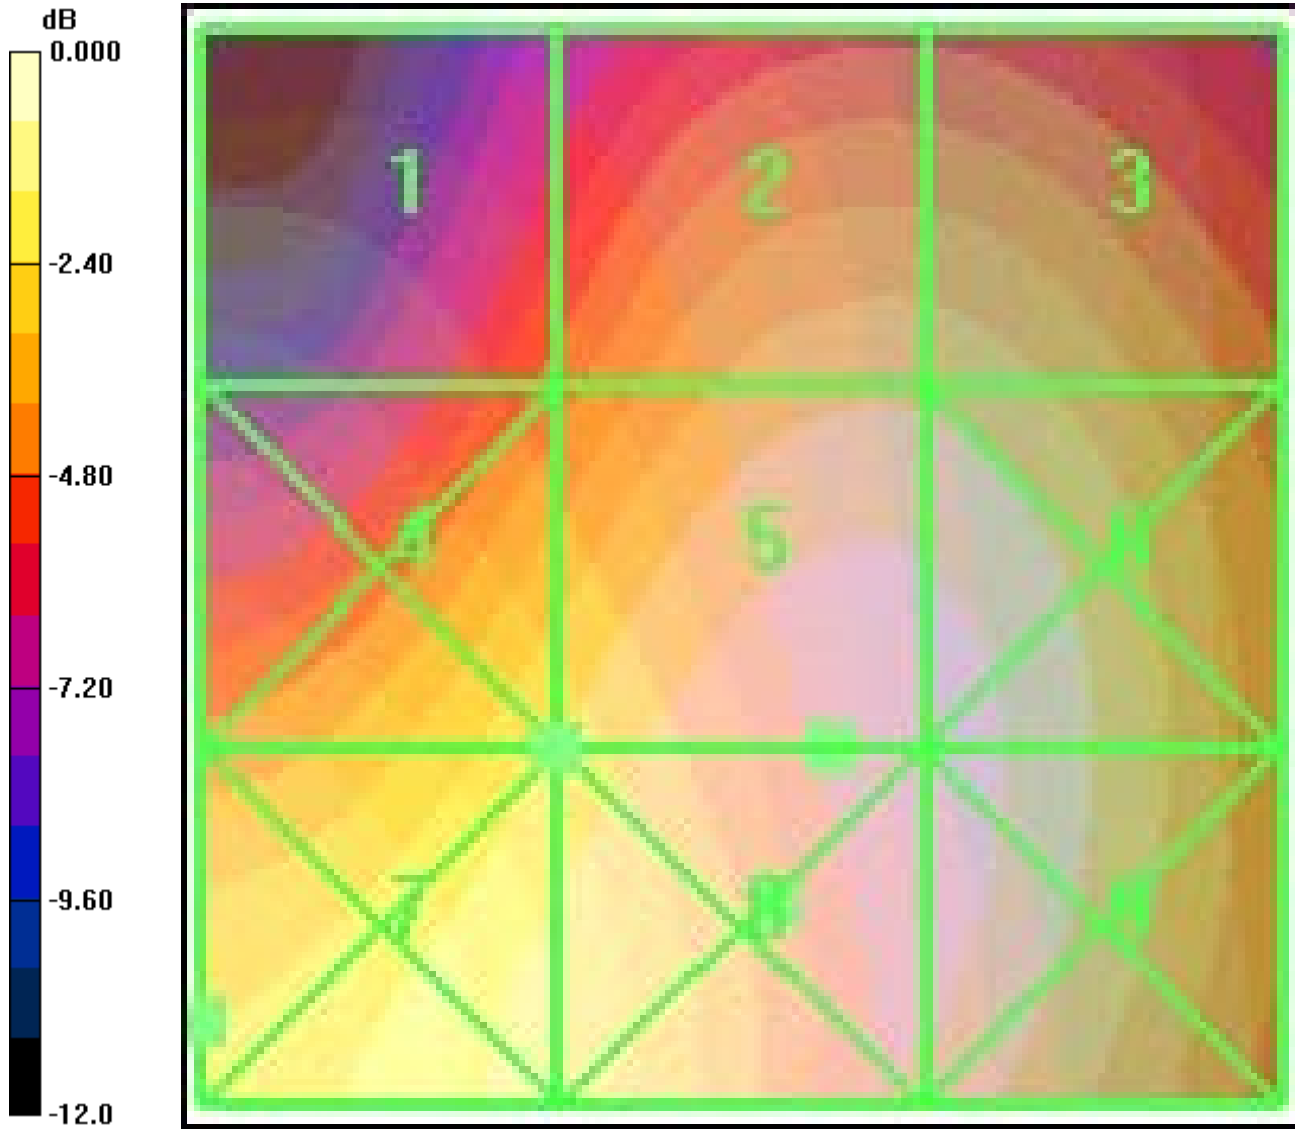

0 dB = 47.3V/m

Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

CDMA 1700 Channel 450

Date: 01/13/2011

Communication System: CDMA_Triband, Frequency: 1732.5 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2341 Probe: H3DV5 - SN6029, ConvF(1, 1, 1), Calibrated: 7/12/2010 Calibrated: 7/16/2010

Sensor-Surface: (Fix Surface),

Electronics: DAE4 Sn527, Calibrated: 7/8/2010

Measurement SW: DASY4, V4.7 Build 80

Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8̄ 1 deg C, Liquid T = 22.0̄ 1 deg C

AWS_450/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 56.8 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 67.1 V/m; Power Drift = -0.146 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1 34.2 M4	Grid 2 47.9 M4	Grid 3 47.9 M4
Grid 4 46.7 M4	Grid 5 56.8 M4	Grid 6 56.2 M4
Grid 7 52.3 M4	Grid 8 57.2 M4	Grid 9 56.4 M4

AWS_450/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.146 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.118 A/m; Power Drift = 0.127 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1 0.137 M4	Grid 2 0.121 M4	Grid 3 0.090 M4
Grid 4 0.174 M4	Grid 5 0.146 M4	Grid 6 0.101 M4
Grid 7 0.196 M3	Grid 8 0.166 M4	Grid 9 0.120 M4



Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

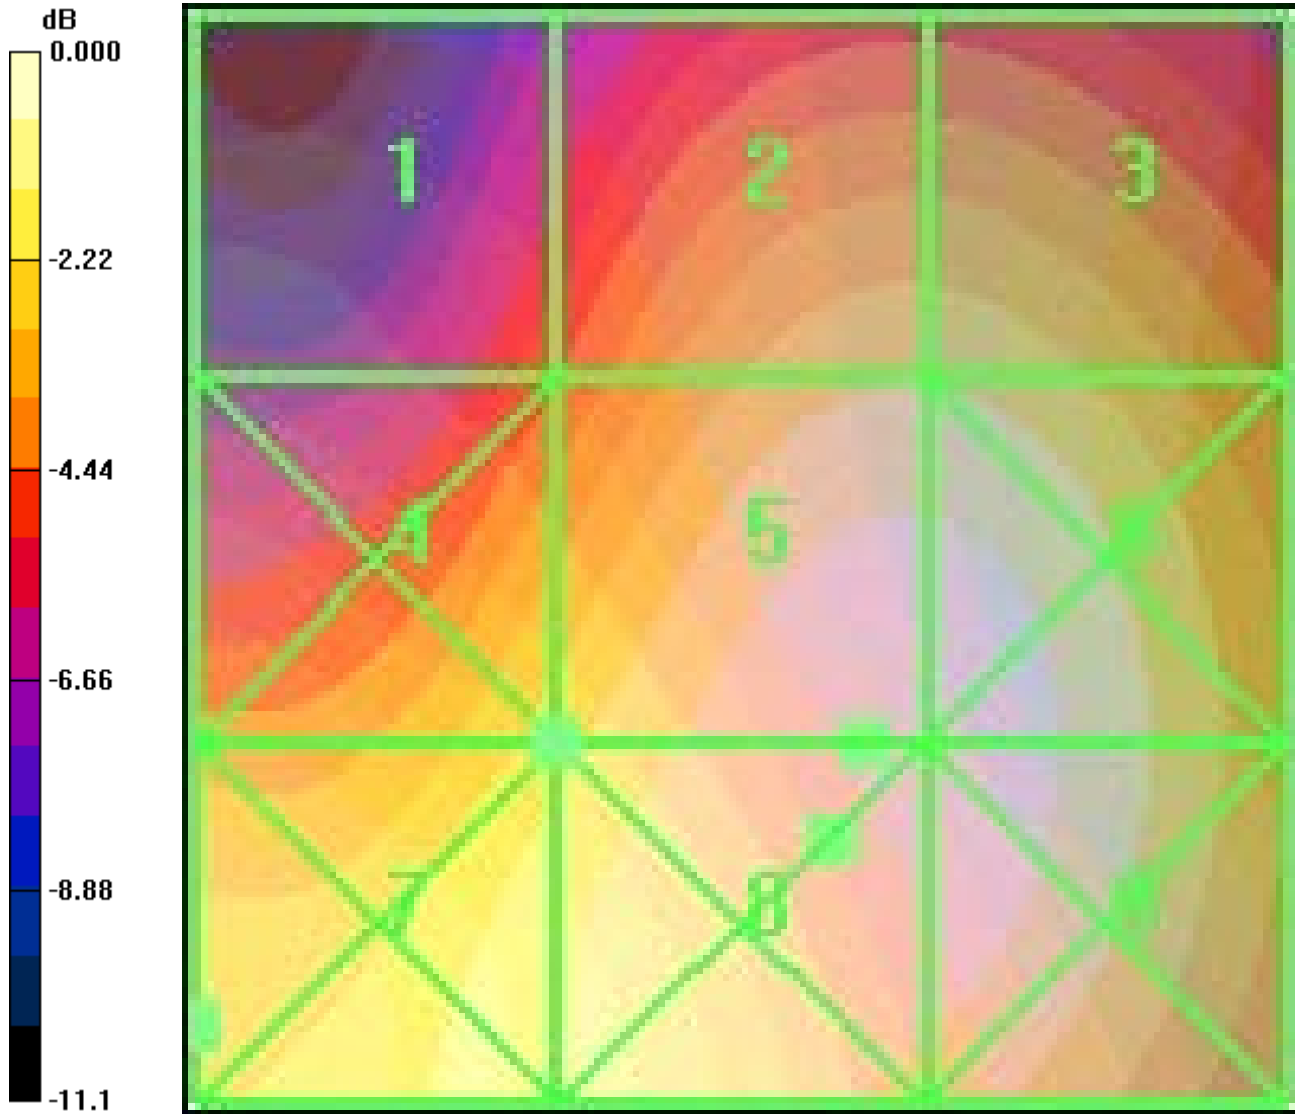

0 dB = 57.2V/m

Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

CDMA 1700 Channel 875

Date: 01/13/2011

Communication System: CDMA_Triband, Frequency: 1753.75 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2341 Probe: H3DV5 - SN6029, ConvF(1, 1, 1), Calibrated: 7/12/2010 Calibrated: 7/16/2010

Sensor-Surface: (Fix Surface),
 Electronics: DAE4 Sn527, Calibrated: 7/8/2010
 Measurement SW: DASY4, V4.7 Build 80
 Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 ± 1 deg C, Liquid T = 22.0 ± 1 deg C

AWS_875/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 56.7 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 69.0 V/m; Power Drift = -0.017 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1	Grid 2	Grid 3
36.2 M4	47.6 M4	47.3 M4
Grid 4	Grid 5	Grid 6
47.3 M4	56.7 M4	55.5 M4
Grid 7	Grid 8	Grid 9
50.2 M4	56.8 M4	55.5 M4

AWS_875/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.141 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.116 A/m; Power Drift = 0.095 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.141 M4	0.122 M4	0.086 M4
Grid 4	Grid 5	Grid 6
0.170 M4	0.140 M4	0.090 M4
Grid 7	Grid 8	Grid 9
0.182 M4	0.151 M4	0.097 M4




Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

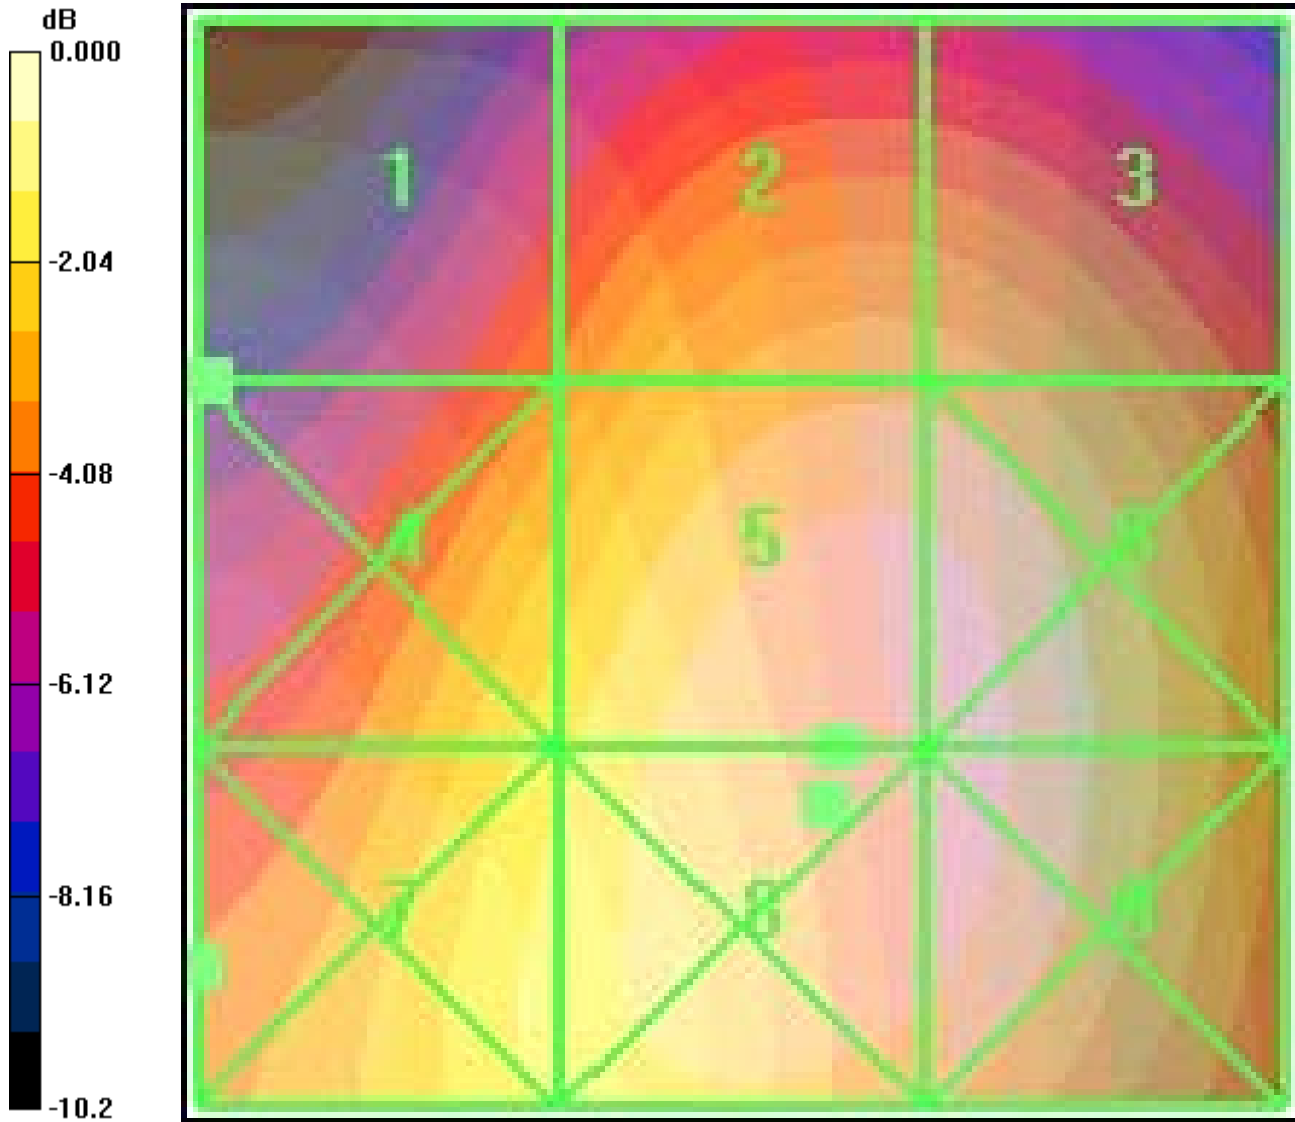

0 dB = 56.8V/m

CDMA 1700 Channel 450 (360) E roll

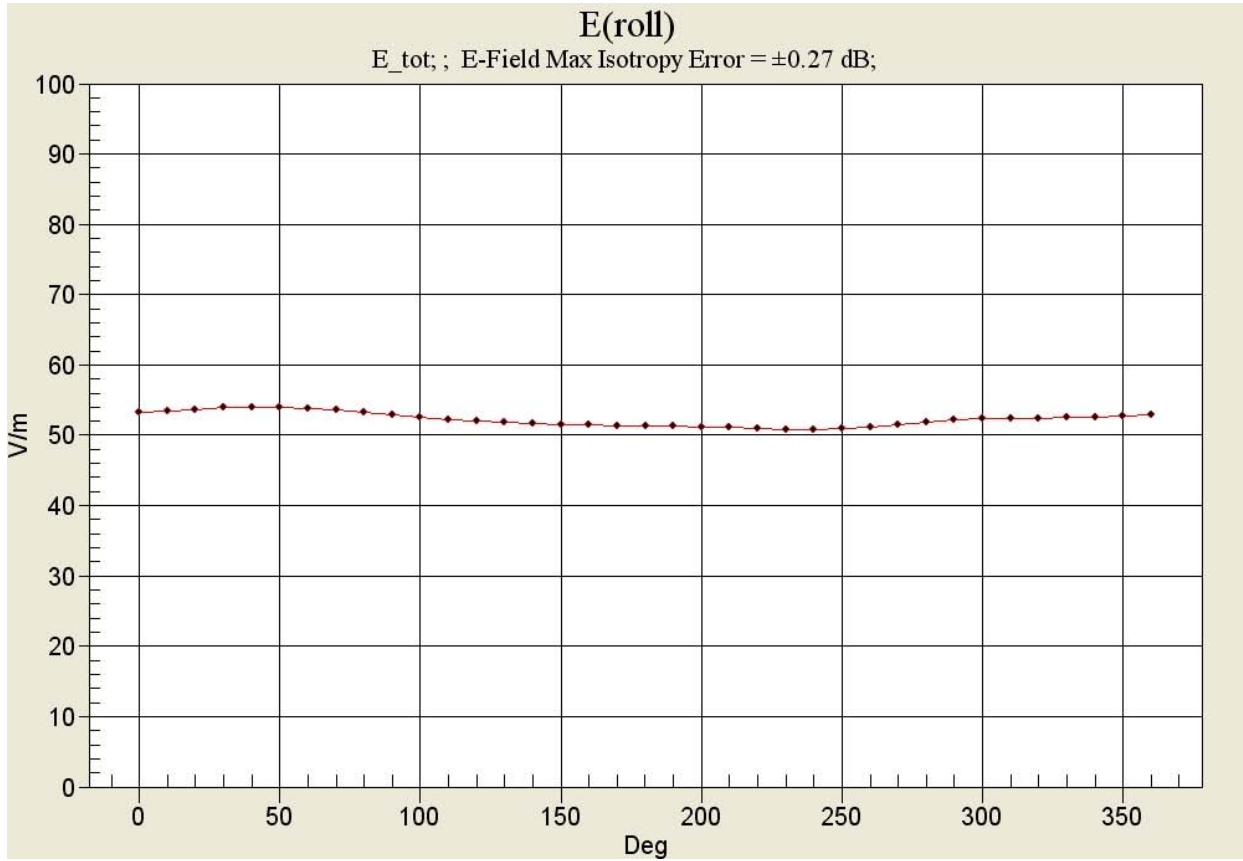

Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

CDMA 1900 Channel 25

Date: 01/13/2011

Communication System: CDMA_Triband, Frequency: 1850 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2341 Probe: H3DV5 - SN6029, ConvF(1, 1, 1), Calibrated: 7/12/2010 Calibrated: 7/16/2010

Sensor-Surface: (Fix Surface),
 Electronics: DAE4 Sn527, Calibrated: 7/8/2010
 Measurement SW: DASY4, V4.7 Build 80
 Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 ± 1 deg C, Liquid T = 22.0 ± 1 deg C

PCS_25/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 61.8 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 76.8 V/m; Power Drift = -0.115 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1 38.6 M4	Grid 2 55.6 M4	Grid 3 55.5 M4
Grid 4 47.4 M4	Grid 5 61.8 M4	Grid 6 61.5 M4
Grid 7 48.8 M4	Grid 8 61.6 M4	Grid 9 61.1 M4

PCS_25/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.188 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.149 A/m; Power Drift = -0.103 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1 0.184 M4	Grid 2 0.159 M4	Grid 3 0.104 M4
Grid 4 0.220 M3	Grid 5 0.188 M4	Grid 6 0.123 M4
Grid 7 0.230 M3	Grid 8 0.201 M3	Grid 9 0.135 M4



Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

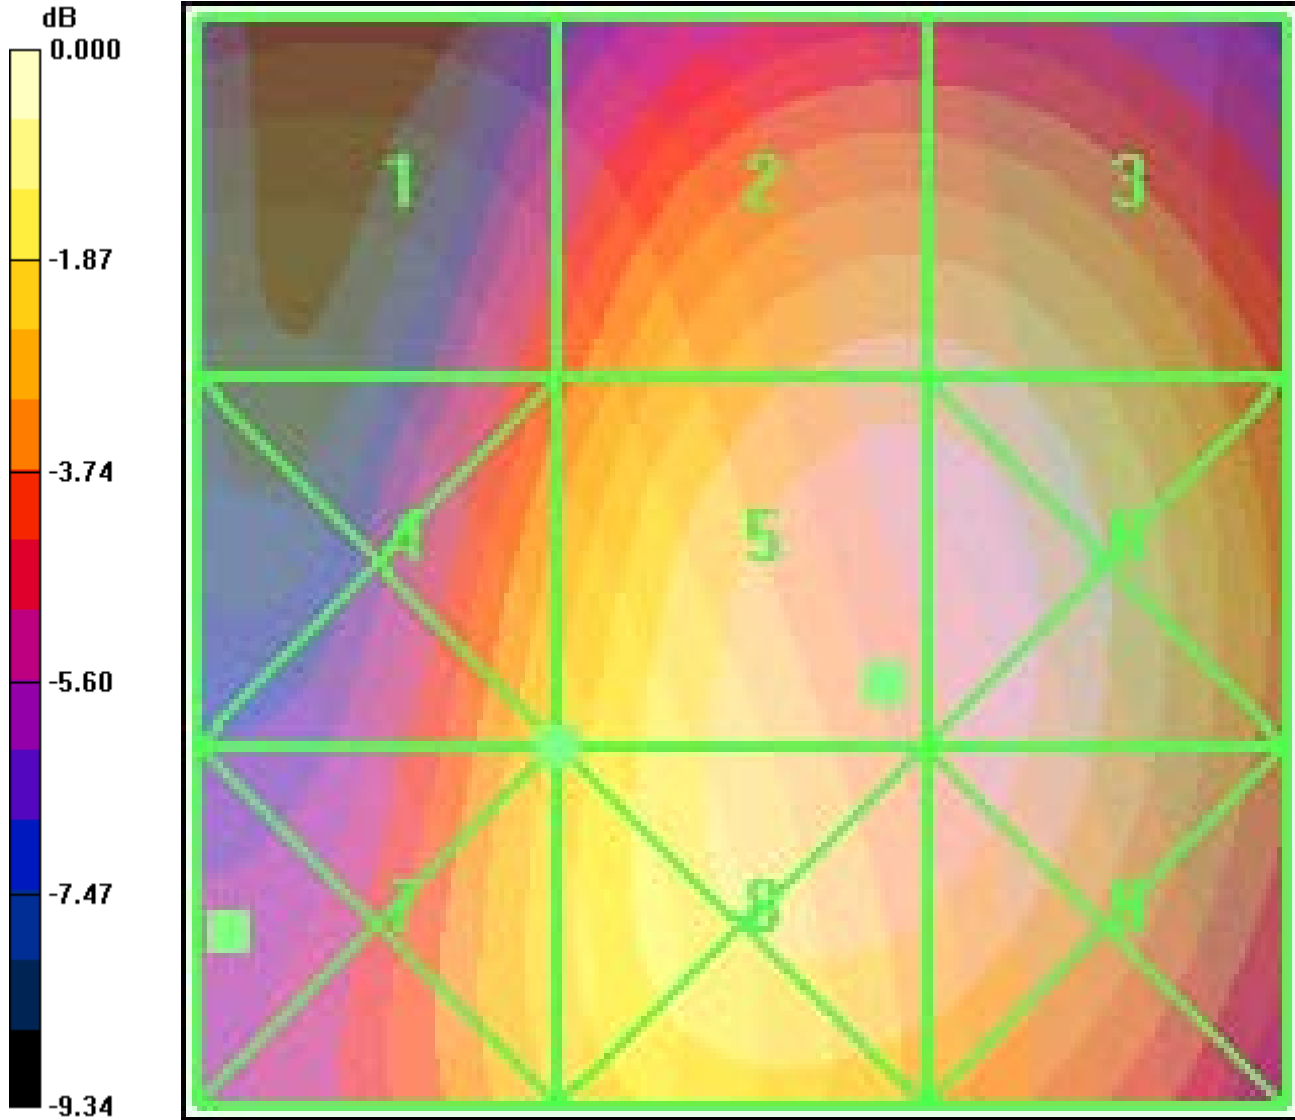

0 dB = 61.8V/m

Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

CDMA 1900 Channel 600

Date: 01/13/2011

Communication System: CDMA_Triband, Frequency: 1880 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2341 Probe: H3DV5 - SN6029, ConvF(1, 1, 1), Calibrated: 7/12/2010 Calibrated: 7/16/2010

Sensor-Surface: (Fix Surface),

Electronics: DAE4 Sn527, Calibrated: 7/8/2010

Measurement SW: DASY4, V4.7 Build 80

Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8̄ 1 deg C, Liquid T = 22.0̄ 1 deg C

PCS_600/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 61.0 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 73.9 V/m; Power Drift = -0.130 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1 35.9 M4	Grid 2 54.4 M4	Grid 3 54.4 M4
Grid 4 45.0 M4	Grid 5 61.0 M4	Grid 6 60.8 M4
Grid 7 47.6 M4	Grid 8 61.0 M4	Grid 9 60.7 M4

PCS_600/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.183 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.154 A/m; Power Drift = 0.085 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1 0.182 M4	Grid 2 0.161 M4	Grid 3 0.106 M4
Grid 4 0.207 M3	Grid 5 0.183 M4	Grid 6 0.122 M4
Grid 7 0.214 M3	Grid 8 0.192 M3	Grid 9 0.133 M4



Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

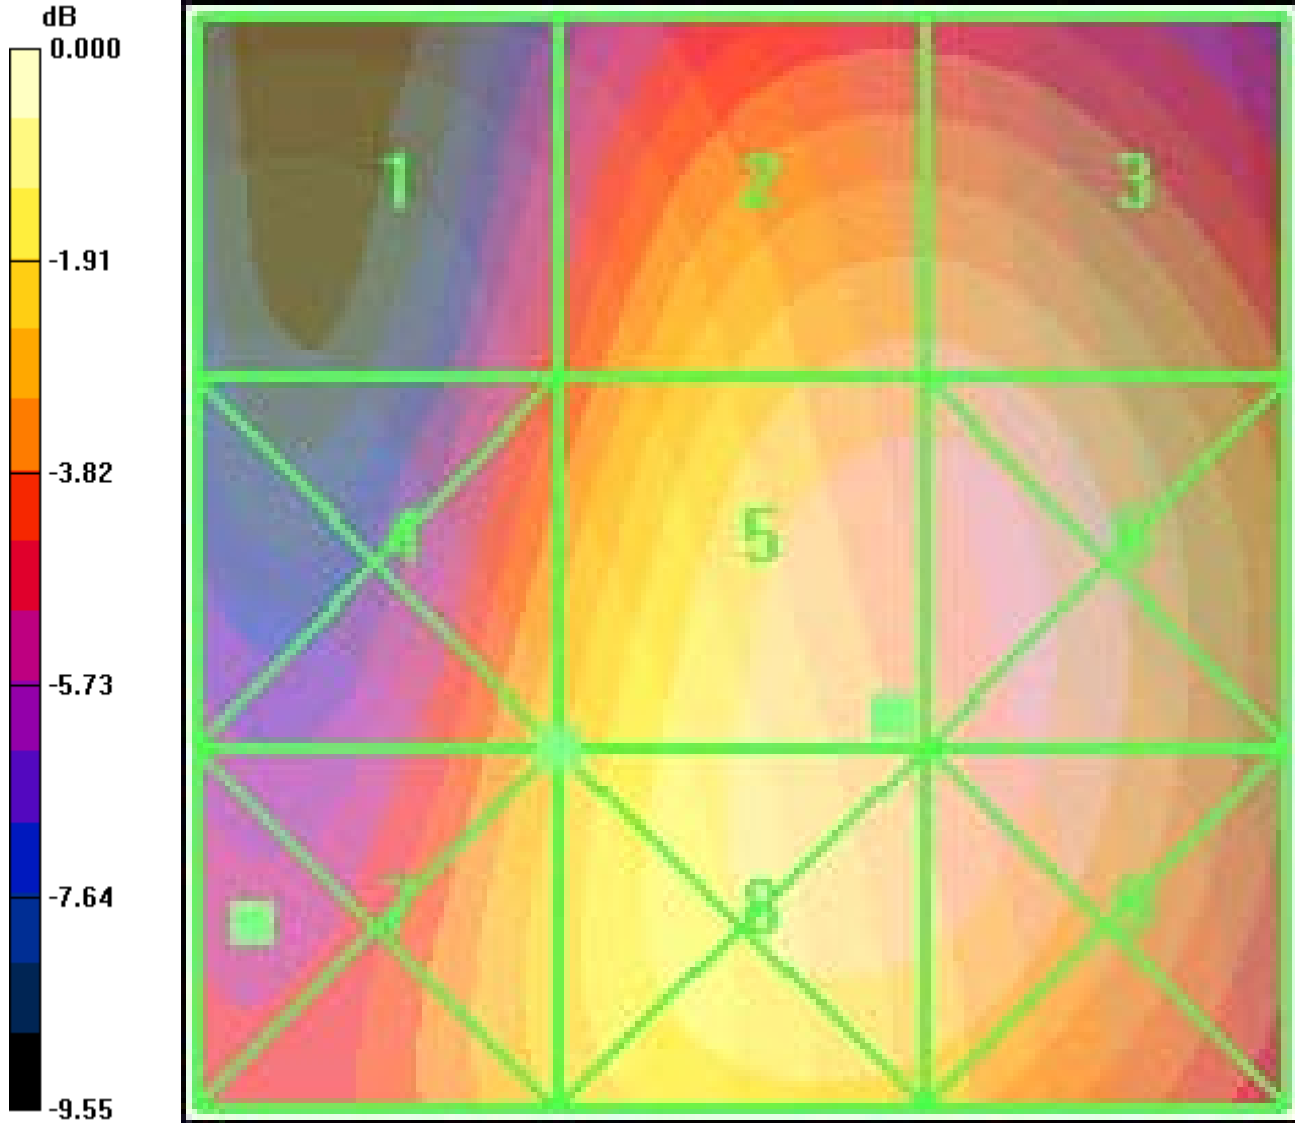

0 dB = 61.0V/m

Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

CDMA 1900 Channel 1175

Date: 01/13/2011

Communication System: CDMA_Triband, Frequency: 1910 MHz, Duty Cycle: 1:1
 Medium: Air, Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom: HAC Test Arch with AMCC, Phantom section: RF Section

DASY4 Configuration:

Probe: ER3DV6 - SN2341 Probe: H3DV5 - SN6029, ConvF(1, 1, 1), Calibrated: 7/12/2010 Calibrated: 7/16/2010

Sensor-Surface: (Fix Surface),
 Electronics: DAE4 Sn527, Calibrated: 7/8/2010
 Measurement SW: DASY4, V4.7 Build 80
 Postprocessing SW: SEMCAD, V1.8 Build 186

Temperature:

Room T = 21.8 ± 1 deg C, Liquid T = 22.0 ± 1 deg C

PCS_1175/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 60.6 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 68.2 V/m; Power Drift = -0.055 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1 35.1 M4	Grid 2 55.7 M4	Grid 3 56.0 M4
Grid 4 39.8 M4	Grid 5 60.6 M4	Grid 6 60.8 M4
Grid 7 42.0 M4	Grid 8 60.1 M4	Grid 9 60.2 M4

PCS_1175/Hearing Aid Compatibility Test (101x101x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.168 A/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, -6.30 mm

Reference Value = 0.144 A/m; Power Drift = -0.145 dB


Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1 0.162 M4	Grid 2 0.150 M4	Grid 3 0.104 M4
Grid 4 0.183 M4	Grid 5 0.168 M4	Grid 6 0.119 M4
Grid 7 0.189 M4	Grid 8 0.177 M4	Grid 9 0.132 M4



Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

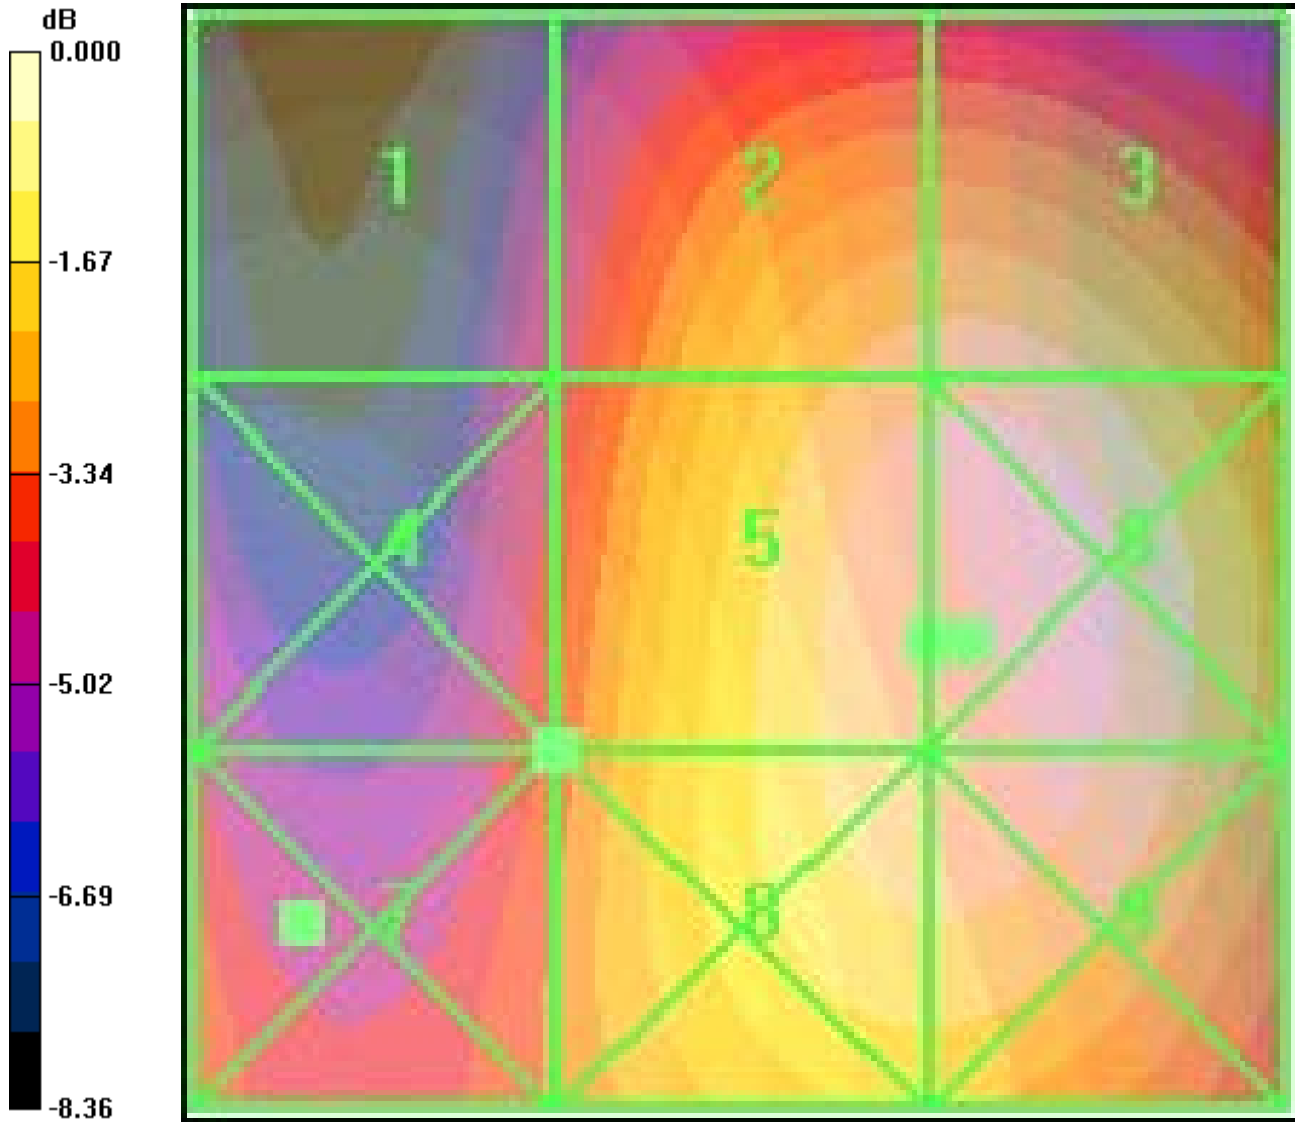

0 dB = 60.8V/m

Applicant	Kyocera
FCC ID:	OVF-K33BIC06
Report #:	CT-K33BIC-06B C2PC-20RFC-1210-R0

CDMA 1900 Channel 25 (360) E roll

