



Hearing Aid Compatibility

FCC 47 CFR section 20.19 Test Report

Single-Band Single-Mode CDMA Cellular Phone

FCC ID: OVFKWC-KX9D

Model: KX9D

STATEMENT OF CERTIFICATION

The data, data evaluation and equipment configuration represented herein are a true and accurate representation of the measurements of the sample's HAC RF emissions characteristics as of the dates and at the times of the test under the conditions herein specified.

STATEMENT OF COMPLIANCE

This product was tested in accordance with the measurement procedures specified in ANSI PC63.19-2005 and has been shown to be capable of compliance with the technical requirements of FCC 47 CFR section 20.19.

Test Location:	Kyocera Wireless Corp.		
	10300 Campus Point Drive, San Diego, CA 92121 USA		
Test performed by:	Thuy To Regulatory Engineer	Date of Test:	5/8/06 -5/12/06
Report Prepared by:	Thuy To Regulatory Engineer	Date of Report:	5/12/06
Report Reviewed by:	C. K. Li Hardware Engineer, Senior Staff/Manager	Date of Review:	5/16/06





TABLE OF CONTENTS

1	Intro	oduction	3
2	Equ	uipment Under Test (EUT)	3
3	Sun	nmary of Test Results	3
	Test 4.1 4.2 4.3 4.4	Ambient Conditions RF characteristics of the test site Test Signal, Frequencies and Output Power EUT Operating Conditions	4 4 4
	Des 5.1 5.2 5.3 5.4	Scription of the test equipment Test Equipment Used Near Field Measurement System Isotropic E-Field Probe Isotropic H-Field Probe	5 6 6
6	Sys	tem Validation	8
	7.1 7.2 7.3 7.4 7.4. 7.4.	PMF Test Results PMF Peak Power Measurement Plots	9 10 11 11 12
8	Emi	ission Data Extraction and Post processing	14
9	Mea	asurement Uncertainty	15
	10.1 10.2 10.3	Emissions Tests Emission Limits CDMA 1900 Test Results Worst-Case Configuration Evaluation 3.1 Peak Reading 360° Probe Rotation at Azimuth axis	16 17 18
11	Tes	t setup photos	19
Αp	pendi	x A: Probe Calibration Certification	20
Αp	pendi	x B: System Validation Data	22
Αp	pendi	x C: Test Results/Plots	23



1 Introduction

This test report describes the Hearing Aid Compatibility (HAC) measurement of a wireless portable device manufactured by Kyocera Wireless Corp. (KWC). These measurements were performed for compliance with the rules and regulations of the U.S. Federal Communications Commission (FCC). The testing was performed in accordance with ANSI PC63.19-2005.

This report covers test and data on:

Х	RF Emissions	ANSI PC63.19 Clause 4
	T-Coil	ANSI PC63.19 Clause 6

2 Equipment Under Test (EUT)

Product:	Single-Band Single-mode CDMA Cellular Phone
FCC ID:	OVFKWC-KX9D
Model Number:	KX9D
EUT Serial Number:	F0000006207458
Type:	[] Prototype, [X] Pre-Production, [] Production
Device Category:	Portable
RF Exposure Environment:	General Population / Uncontrolled
Antenna:	Stubby
Detachable Antenna:	No
External Input:	Audio/Digital Data
Quantity:	Quantity production is planned
Modes:	1900 CDMA
Multiple Access Scheme:	CDMA
TX Frequency (MHz):	1850 - 1910
Rated RF Conducted Output Power	23.0 Phone Open
(dBm)	

3 Summary of Test Results

ANSI PC63.19 (2005)			
Section 4 RF Emissions			
Test	Test Test Results Overall Category		
E-Field Emissions	M4	M4	
H-Field Emissions	M4		



4 Test conditions

4.1 Ambient Conditions

All tests were performed under the following environmental conditions:

Ambient Temperature:	23 ± 2 Degrees C
Tissue simulating liquid temperature:	22 ± 1 Degrees C
Relative Humidity (RH):	0% <rh 80%<="" <="" th=""></rh>
Atmospheric Pressure:	101.3kPa + 10 to -5kPa

4.2 RF characteristics of the test site

All HAC measurements were performed inside a shielded room that provide isolation from external EM fields, with the RF ambient at least 20 dB below the intended measurement limits.

4.3 Test Signal, Frequencies and Output Power

Peak and Average conducted power were measured for each mode for comparison. RC3 SO55 was chosen for worst case power configuration.

CONDUCTED POWER			
	CDMA 19	00 (ch 600)	
Mode	Peak (dBm)	Average (dBm)	
RC1, SO2, Full Rate	27.76	22.52	
RC1, SO55, Full Rate	27.83	22.59	
RC2, SO9, Full Rate	27.97	22.62	
RC2, SO55, Full Rate	27.70	22.57	
RC3, SO2, Full Rate	27.45	22.52	
RC3, SO55, Full Rate	27.79	22.60	
RC43, SO2, Full Rate	27.25	22.57	
RC43, SO55, Full	27.36	22.57	
Rate			
RC54, SO9, Full Rate	27.36	22.55	
RC54, SO55, Full	27.27	22.58	
Rate			

During tests, the EUT was put in in-call mode and controlled by a CDMA simulator to generate the required signal and power using the configuration below.

Protocol:	6 (IS-2000)
Radio Configuration:	3
Power Control:	All Up Bits
Service Option:	55
Data Rate:	Full





In all operating modes, the phone was set to rated maximum RF power level and the measurements were performed on low, mid and high channels.

The measurement system measures power drift during HAC testing by comparing E/H-field in the same location at the beginning and at the end of measurement. These records were used to monitor stability of power output during tests. Conducted RF power measurements were also performed before and after each HAC measurements to confirm the output power.

4.4 EUT Operating Conditions

The EUT was tested with the following configurations and conditions, if applicable:

Χ	Fully charged standard and extended battery as supplied with the handset
Χ	Open configuration, at ear use position.
	Both retracted and extended antenna positions
Х	Back-light tested ON and OFF

5 Description of the test equipment

5.1 Test Equipment Used

Below is a list of the calibrated equipment used for the measurements:

Description	Manufacturer	Model Number	Serial Number	Cal Due Date
Power Meter	Giga-tronics	8541C	1830971	05/27/06
Signal Generator	Hewlett Packard	E4421B	US38440337	06/20/07
Radio Communication Tester	Agilent	8960	US41070147	05/16/06
Data Acq	Speag	DAE4	530	01/16/07
E-field Probe	Speag	ER3DV6	2282	10/21/06
H-field Probe	Speag	H3DV5	6029	06/16/06
Dipole Antenna (1880MHz)	Speag	CD1880V3	1015	04/05/07
Spectrum Analyzer	Hewlett Packard	8594E	3543H02438	04/13/07

The calibration certificates of E-field and H-field probes are attached in Appendix A.



5.2 Near Field Measurement System

The measurements were performed with Dasy4 automated near-field scanning system comprised of high precision robot, robot controller, computer, near-field probe, probe alignment sensor, non-conductive phone positioner, Test Arch and software extension. The overall expanded uncertainty (K=2) of the measurement system is $\pm 10.9\%$ and $\pm 14.7\%$ for H-field and E-field resp. The measurement uncertainty budget is given in section 6.

5.3 Isotropic E-Field Probe

Model	■ ER3DV6
Construction	 One dipole parallel, two dipoles normal to probe axis Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., glycolether)
Calibration	■ In air from 100 MHz to 3.0 GHz (absolute accuracy ± 6%; k=2)
Frequency	100MHz to 6 GHzLinearity: ± 0.2dB (100MHz to 3GHz)
Directivity	■ ± 0.2 dB in air (rotation around probe axis)
	 ± 0.4 dB in air (rotation normal to probe axis)
Dynamic Range	2 V/m to > 1000 V/m
	■ Linearity: ± 0.2 dB
Dimensions	Overall length: 330 mm (Tip: 16 mm)
	■ Tip diameter: 8 mm (Body: 12 mm)
	 Distance from probe tip to dipole centers: 2.5 mm
Application	 General near-field measurements up to 6 GHz
	 Field component measurements
	 Fast automatic scanning in phantoms



5.4 Isotropic H-Field Probe

Model	■ H3DV5
Construction	Three concentric loop sensors with 3.8 mm loop diameters
	Resistively loaded detector diodes for linear response
	Built-in shielding against static charges
	■ PEEK enclosure material (resistant to organic solvents, e.g.,
	glycolether)
Frequency	 200 MHz to 3 GHz (± 6.0%, k=2); Output linearized
Directivity	± 0.25 dB (spherical isotropy error)
Dynamic Range	■ 10 mA/m to 2 A/m at 1 GHz
E-Field Interference	< 10% at 3 GHz (for plane wave)
Dimensions	Overall length: 330 mm (Tip: 40 mm)
	Tip diameter: 6 mm (Body: 12 mm)
	 Distance from probe tip to dipole centers: 3 mm
Application	General magnetic near-field measurements up to 3 GHz
	Field component measurements
	Surface current measurements
	Measurements in air or liquids
	 Low interaction with the measured field



6 System Validation

The manufacturer calibrates the probes annually. The HAC measurements of the device were done within 24 hours of system accuracy verification, which was done using calibration dipoles. Unmodulated continuous wave of power level of 20dBm was supplied to a dipole antenna placed under Test Arch. The measurement probes are positioned over the illuminated dipole at 10mm distance from the top surface of the dipole element to the calibration reference point of the sensor, defined by the probe manufacturer.

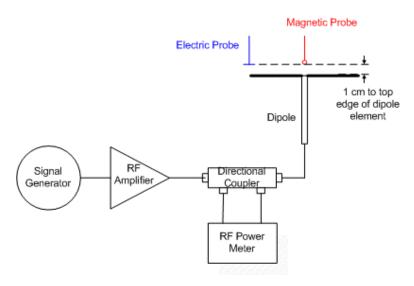


Figure 6 - System Check Setup

The length of the dipole was scanned with both E and H-field probes and the maximum values for each were recorded. The validation results are in the table below and printouts of the validation test are attached in Appendix B. All the measured parameters were within the specification.

Freq. (MHz)	Parameter	Target	Measured	Delta (%)	Limit (%)	Test date
1880	E dB(V/m)	140	140.6	0.43	± 25	05-10-06
	H dB(A/m)	0.458	0.479	4.54	± 25	05-10-06



7 Description Of The Test Procedure

The device was positioned and setup according to ANSI PC63.19-2005.

7.1 Test Positions

The device was placed on a non-conductive phone positioner under the Test Arch.

7.2 RF Emission Measurements Reference and Plane

Figure 7.2 illustrates the references and reference plane that shall be used in the EUT emissions measurement:

- The grid is 5 cm by 5 cm area that is divided into 9 evenly sized blocks or sub-grids.
- The grid is centered on the audio frequency output transducer (speaker) of the EUT.
- The grid is in a reference plane, which is defined as the planar area that contains the highest point in the area of the phone that normally rests against the user's ear. It is parallel to the centerline of the receiver of the EUT and is defined by the points of the receiver-end of the EUT, which, in normal handset use, rest against the ear.
- The measurement plane is parallel to, and 1.0 cm in front of, the reference plane.

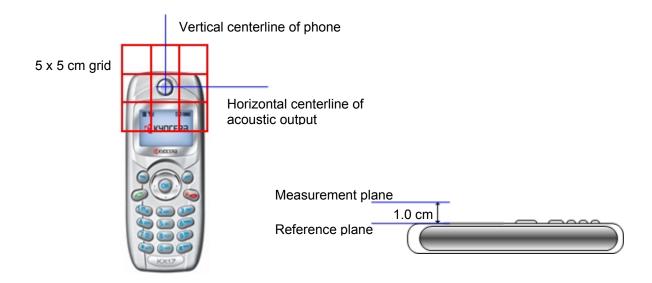


Figure 7.2 – Measurement Reference and Plane



7.3 RF Emissions Measurement Procedures

Figure 7.6 shows the near field emission measurement flowchart:

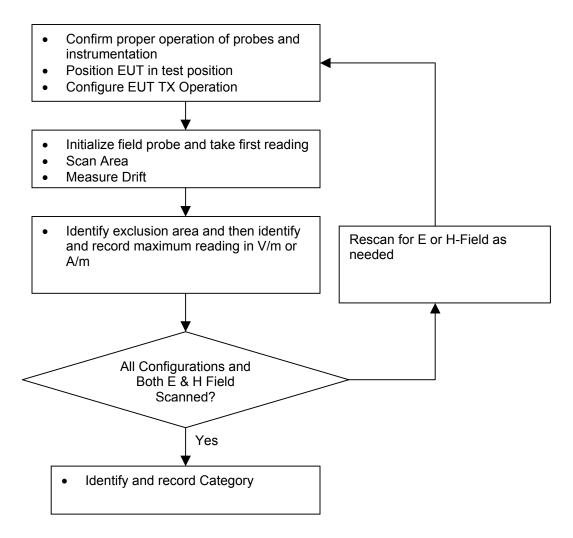


Figure 7.3 - Near field emission measurement flowchart

- 1. The center of the probe was scanning to the edges of the grid. Accordingly the total area covered by the outside edge of the probe was the 5 cm by 5 cm area, increased by half (½) the probe diameter on all sides.
- 2. The nearest point on the probe measurement element(s) was held 1.0 cm from the EUT reference plane.
- 3. The probe element is that portion of the probe that is designed to receive and sense the field being measured.
- 4. The physical body of the probe housing was not used when setting this 1.0 cm distance as this would place the sensing elements at an indeterminate distance from the reference plane.
- 5. The step size of the scan is set to 5 mm or less.
- 6. Up to three blocks were excluded for each field measurement.
 - The center block containing the EUT output was not excluded.
 - A maximum of five blocks were excluded for both E- and H-field measurements for the EUT
 output being measured. Stated differently, the center sub-grid or block and 3 other blocks were
 common to both the E- and H-field measurements for a given grid.



7.4 Probe Modulation Factor (PMF)

7.4.1 Measurement Procedures

A calibration was made of the modulation response of the probe and its instrumentation chain. This calibration was performed with the field probe, attached to its instrumentation. The response of the probe system to a CW field at the frequency of interest is compared to its response to a modulated signal with equal peak amplitude to that of a CW signal. The field level of the test signals shall be more than 10 dB above the ambient level and the noise floor of the instrumentation being used. The ratio of the CW reading to that taken with a modulated reading was applied to the DUT measurements. The measurement procedures are as following:

- 1. Fix the field probe in a set location relative to the dipole antenna, as illustrated in Figure 7.4.
- 2. Setup the wireless device (EUT) with intended signal at the intended measurement frequency.
- 3. Record the reading of the probe measurement system.
- 4. Replace the wireless device with a RF signal generator producing an unmodulated CW signal and set to the wireless device operating frequency.
- 5. Set the peak power of the unmodulated signal to equal that recorded from the wireless device
- 6. Record the reading of the probe measurement system of the unmodulated CW signal.
- 7. The ratio of probe reading (CW) in step 6 to the probe reading (EUT) in step 3 is the modulation factor.

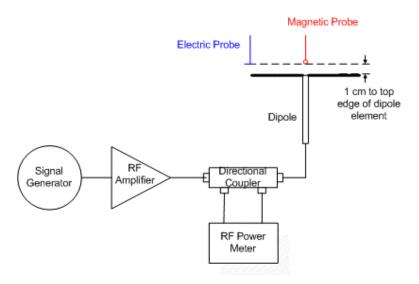


Figure 7.4 - Probe Modulation Setup

The modulation factors obtained by above method shall be applied to readings taken of the actual WD, in order to obtain an accurate peak field reading.






7.4.2 PMF Test Results


		E-Fi	ield		
Frequency (MHz)	Peak Power (dBm)	Protocol	Protocol Reading (V/m)	PMF Ratio	PMF (dB)
	22.87	CW	92.67		
1880	22.83	CDMA	93.84	0.99	-0.109
	22.84	AM	59.79	1.55	3.806
		H-F	ield		
Frequency (MHz)	Peak Power (dBm)	Protocol	Protocol Reading (A/m)	PMF Ratio	PMF (dB)
	22.91	CW	0.3549		
1880	22.89	CDMA	0.3624	0.98	-0.2
	22.89	AM	0.2355	1.51	3.6

7.4.3 PMF Peak Power Measurement Plots




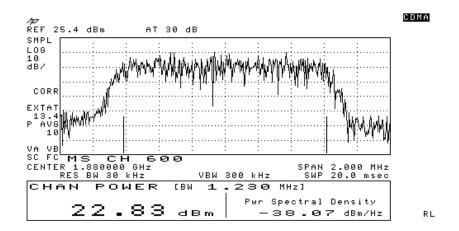

CDMA-1900

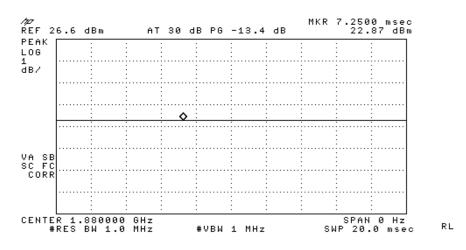

CW

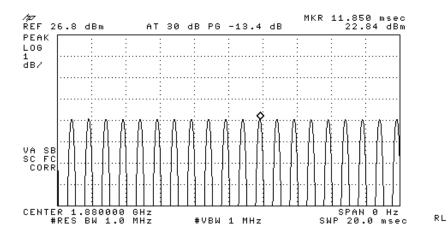

80% AM



8 Emission Data Extraction and Post processing

At the end of the measurements, the DASY4 system automatically evaluates the slot-averaged results, exclusion of the three highest sub-grid, application of the AWF factor per ANSI-C63.19 requirements.

The following AWF factors were used for the standard transmission protocols:

Standard	Technology	AWF
TIA/EIA/IS-2000	CDMA	0
TIA/EIA-136	TDMA (50 Hz)	0
J-STD-007	GSM (217)	-5
T1/T1P1/3GPP	UMTS (WCDMA)	0
iDEN [™]	TDMA(22 and 11 Hz)	0

Table 7.5a - Articulation Weighting Factor (AWF)

All DASY4 measurements are in RMS values. The Dasy4 system incorporates the crest factor of the signal in the computation of the RMS values. Although the software also has the capability to estimate the peak field by applying a square root of the crest factor value to the readings, the probe modulation factor was applied manually instead per ANSI PC63.19 in the measurement tables in this report using equation:

Peak Field = (DASY4 reading) x PMF

where DASY4 reading = measurement from DASY4 in V/m or A/m PMF = Probe Modulation Factor in linear unit



9 Measurement Uncertainty

Table 7.5b shows the uncertainty budget for HAC free field assessment according to ANSI PC63.19-2005. The budget is valid for the frequency range 800 MHz - 3 GHz and represents a worst-case analysis. For specific tests and configurations, the uncertainty could be smaller.

Uncertainty Description	Uncert. Value (± %)	Prob. Dist.	Div.	C _i (E)	C _i (H)	Stand. Uncert (E) (±%)	Stand. Uncert (H) (±%)
Measurement system							
Probe calibration	5.1	N	1	1	1	5.1	5.1
Axial isotropy of the probe	4.7	R	√3	1	1	2.7	2.7
Sensor displacement	16.5	R	√3	1	0.145	9.5	1.4
Boundary effects	2.4	R	√3	1	1	1.4	1.4
Probe linearity	4.7	R	√3	1	1	2.7	2.7
Scaling to Peak Envelope Power	2.0	R	√3	1	1	1.2	1.2
System Detection limit	1.0	R	√3	1	1	0.6	0.6
Readout electronics	0.3	N	1	1	1	0.3	0.3
Response time	0.8	R	√3	1	1	0.5	0.5
Integration time	2.6	R	√3	1	1	1.5	1.5
RF ambient conditions	3.0	R	√3	1	1	1.7	1.7
RF Reflections	12	R	√3	1	1	6.9	6.9
Probe Positioner	1.2	R	√3	1	0.67	0.7	0.5
Probe positioning	4.7	R	√3	1	0.67	2.7	1.8
Extrap. and integration	1.0	R	√3	1	1	0.6	0.6
Test Sample Related							
Device positioning vertical	4.7	R	√3	1	0.67	2.7	1.8
Device Positioning Lateral	1.0	R	√3	1	1	0.6	0.6
Device Holder and Phantom	2.4	R	√3	1	1	1.4	1.4
Power drift	5.0	R	√3	1	1	2.9	2.9
Phantom and Setup Related							
Phantom thickness	2.4	R	√3	1	0.67	1.4	0.9
	С	ombined	l Standa	ard Unce	rtainty:	14.7	10.9
Exten	ded Standa	ard Unce	rtainty	on Powe	r (k=2):	29.4	21.8
Exte	nded Stan	dard Und	ertainty	on Fiel	d (k=2):	14.7	10.9

N: Normal R: Rectangular

Table 7.5b - Worst-Case uncertainty budget for HAC free field assessment



10 RF Emissions Tests

10.1 Emission Limits

Table 8.1 shows the M-rating criteria from ANSCI C63.19. All digital transmission modes in all frequency bands contained in a HAC phone must meet M3 or M4 levels.

Category		Wireless Device RF Pa	arameters
Near	AWF	E-Field Emissions	H-Field Emissions
Field		dB(V/m) Peak	dB(A/m) Peak
M1	AWF = 0	46.0 to 51.0	-4.4 to 0.6
M2	AWF = 0	41.0 to 46.0	-9.4 to -4.4
M3	AWF = 0	36.0 to 41.0	-14.4 to -9.4
M4	AWF = 0	< 36.0	< -14.4

Table 10.1 - RF Emission Limits



10.2 CDMA 1900 Test Results

			CDN	IA 1900	E-Fiel	d			
Config	uration:	Open		Ant	enna	Stubb	у		
Ch.	Backlight	Battery	Power before Test	Power after Test	Da: Rea	•	PMF	Peak Field	Category
#			dBm	dBm	V/	m		V/m	M
25	ON	Standard	22.97	23.03	52.	.10	1.00	52.10	4
600	ON	Standard	23.22	23.24	53.	.40	1.00	53.40	4
1175	ON	Standard	22.84	22.76	44.	.40	1.00	44.40	4
600	ON	Extended	23.22	23.24	46	.10	1.00	46.10	4
600	OFF	Standard	23.22	23.24	52	.00	1.00	52.00	4
600	OFF	Extended	23.22	23.24	49	.70	1.00	49.70	4

Data plots are shown in Appendix C

			CDM	A 1900	H-Fiel	d			
Config	uration:	Open		Ant	enna	Stubb	y		
Ch.	Backlight	Battery	Power before Test	Power after Test	Da: Rea	sy4 ding	PMF	Peak Field	Category
#			dBm	dBm	A	m		A/m	M
25	ON	Standard	22.97	23.03	0.	13	1.00	0.13	4
600	ON	Standard	23.22	23.24	0.	14	1.00	0.14	4
1175	ON	Standard	22.84	22.76	0.	12	1.00	0.12	4
600	ON	Extended	23.22	23.24	0.	13	1.00	0.13	4
600	OFF	Standard	23.22	23.24	0.	14	1.00	0.14	4
600	OFF	Extended	23.22	23.24	0.	13	1.00	0.13	4

Data plots are shown in Appendix C





10.3 Worst-Case Configuration Evaluation

10.3.1 Peak Reading 360° Probe Rotation at Azimuth axis

The probe was rotated 360° in the worst case configuration. The rotation was performed at the location of maximum field strength in the included blocks.

Data plots are shown in Appendix C



11 Test setup photos



Figure 11a - Open



Figure 11b - Open (close-up)





Appendix A: Probe Calibration Certification

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schwelzerischer Kallbriardienst
C Service suisse d'étalonnage
Sorvizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Multilateral Agreement for the recognition of calibration certificates

Client Kyocera USA.

Gentificate:No: ER3-2282_Oct05

Accreditation No.: SCS 108

			R CO BECOMBADA E INVENTANTA PARTE SANCO S
bject	ER3DV6 - SN:2	282	
- (Share 1)	QA CAL-02.v4		
alibration procedure(s)		edure for E-field probes optimized for	riose near fiéid
	evaluations in a		
	and the second of the second		
alibration date:	October 21, 200	 5	
	mindelin unter two bisk mindeline (1987) kvaliti kvali	handari (jag 1997) ta puning anna ga na Agustu. Na tuning a tuning anna an an agus i se gegenere genere en en	AND CONTROL OF CONTROL
ondition of the calibrated Item	Įn Tolerance ∵		
	nanta the transchilit - t	tional standards which malins the obvious units of	f maggiromonte (SI)
		itional standards, which realize the physical units of probability are given on the following pages and are	
ie measurements and the und	erianthes with confidence	probability are given on the following pages and are	e part of the continoate.
II11545	eted in the aloned takensh		d burnidity > 700/
i calibrations have been condu	icted in the glosed laborat	ory facility: environment temperature (22 ± 3)°C and	a numicity < 70%.
althration Continuous transf /MR	TE oritical for a dibration t		
alibration Equipment used (M8	TE critical for calibration)		
	TE critical for calibration)	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
alibration Equipment used (M8 rimary Standards ower meter E4419B			Scheduled Calibration May-06
rmary Standards ower meter E4419B	ID #	Cal Date (Calibrated by, Certificate No.)	
imary Standards ower meter E4419B ower sensor E4412A	ID# GB41293874	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466)	May-06
nmary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A	ID # GB41293874 MY41495277	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466)	May-06 May-06
imary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A eference 3 dB Attenuator	ID # GB41293874 MY41495277 MY41498087	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466)	May-06 May-06 May-06
imary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (206)	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467)	May-06 May-06 May-06 Aug-06
imary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: \$5054 (3c) SN: \$5086 (206) SN: \$5129 (306)	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00469) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500)	May-06 May-06 May-06 Aug-06 May-06
imary Standards over meter E4419B over sensor E4412A over sensor E4412A oference 3 dB Attenuator oference 20 dB Attenuator oference 30 dB Attenuator oference Probe ER3DV6	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (206)	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467)	May-06 May-06 May-06 Aug-06 May-06 Aug-06
hmery Standards ower meter E4419B ower sensor E4412A ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator eference B dB Attenuator eference Probe ER3DV6 AE4	ID # GB41293874 MY41495277 MY41496087 SN: \$5054 (3c) SN: \$5086 (20b) SN: \$5129 (30b) SN: 2328	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 3-Oct-05 (SPEAG, No. ER3-2328_Oct05)	May-06 May-06 May-06 Aug-06 May-06 Aug-06 Oct-06
nimary Standards ower meter E44198 ower sensor E4412A ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator eference 30 dB Attenuator eference Probe ER3DV6 AE4 econdary Standards	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: G328 SN: 654	Cal Date (Calibrated by, Cartificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 3-Oct-05 (SPEAG, No. ER3-2328_Oct05) 29-Nov-04 (SPEAG, No. DAE4-654_Nov04)	May-06 May-06 May-06 Aug-06 May-06 Aug-06 Oct-06 Nov-05
rimary Standards	ID # GB41293874 MY41495277 MY41498087 SN: \$5054 (3c) SN: \$5086 (20b) SN: \$5129 (30b) SN: 2328 SN: 654	Cal Date (Calibrated by, Cartificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 3-Oct-05 (SPEAG, No. ER3-2228_Oct05) 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Check Date (in house)	May-06 May-06 May-06 Aug-06 May-06 Aug-06 Oct-06 Nov-05 Scheduled Check
nimary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator eference 30 dB Attenuator eference Probe ER3DV6 AE4 econdary Standards F generator HP 8648C	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 2328 SN: 654 ID # US3642U01700	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 3-Oct-05 (SPEAG, No. ER3-2328_Oct05) 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Check Date (in house)	May-06 May-06 May-06 Aug-06 May-05 Aug-06 Oct-06 Nov-05 Schoduled Check In house check: Dec-05
nimary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator eference 30 dB Attenuator eference Probe ER3DV6 AE4 econdary Standards F generator HP 8648C	ID # GB41293874 MY41495277 MY41498087 SN: \$5054 (3c) SN: \$5086 (20b) SN: \$5129 (30b) SN: 2328 SN: 654 ID # US3642U01700 US37390585	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 3-Oct-05 (SPEAG, No. ER3-2328_Oct05) 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Check Date (in house) 4-Aug-89 (SPEAG, in house check Doc-03) 18-Oct-01 (SPEAG, in house check Nov-04)	May-06 May-06 May-06 Aug-06 Aug-06 Aug-06 Oct-06 Nov-05 Schoduled Check In house check: Nov-05
ower meter E4419B ower sensor E4412A ower sensor E4412A ower sensor E4412A ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator eference Probe ER3DV6 AE4 econdary Standards F generator HP 8648C etwork Analyzer HP 8753E	ID# GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 2328 SN: 654 ID# US3642U01700 US37390585 Name	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 3-Oct-05 (SPEAG, No. ER3-2328_Oct05) 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Check Date (in house) 4-Aug-89 (SPEAG, in house check Doc-03) 18-Oct-01 (SPEAG, in house check Nov-04)	May-06 May-06 May-06 Aug-06 Aug-06 Aug-06 Oct-06 Nov-05 Schoduled Check In house check: Nov-05
nimary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator eference 30 dB Attenuator eference Probe ER3DV6 AE4 econdary Standards F generator HP 8648C etwork Analyzer HP 8753E	ID# GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 2328 SN: 654 ID# US3642U01700 US37390585 Name	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 3-Oct-05 (SPEAG, No. ER3-2328_Oct05) 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Check Date (in house) 4-Aug-89 (SPEAG, in house check Doc-03) 18-Oct-01 (SPEAG, in house check Nov-04)	May-06 May-06 May-06 Aug-06 Aug-06 Aug-06 Oct-06 Nov-05 Schoduled Check In house check: Nov-05
hmary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator eference Probe ER3DV6 AE4 econdary Standards F generator HP 8648C etwork Analyzer HP 8753E	ID # GB41293874 MY41495277 MY41498087 SN: \$5054 (3c) SN: \$5086 (206) SN: \$5129 (30b) SN: 2328 SN: 654 ID # US3642U01700 US37390585 Name Nico Vetterii	Cal Date (Calibrated by, Cartificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 3-Oct-05 (SPEAG, No. ER3-2328_Oct05) 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Check Date (in house) 4-Aug-89 (SPEAG, in house check Doc-03) 18-Oct-01 (SPEAG, in house check Nov-04) Function	May-06 May-06 May-06 Aug-06 Aug-06 Aug-06 Oct-06 Nov-05 Schoduled Check In house check: Nov-05

Certificate No: ER3-2282_Oct05



039988

Calibration Laboratory of Schmid & Partner Engineering AG' Zeughaussträsse 43, 8004 Zurich, Switzerland

SNISS OF BRATE Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 108

Client

Kyocera USA

Certificate No: H3-6029_Jun05

CALIBRATION O	CERTIFICAT	E	
Object	H3DV5 - SN:60	29	
Calibration procedure(s).	QA CAL-03.v4 Calibration proc evaluations in a	edure for H-field probes optimized for ir	close near field
Celibration date:	June 13, 2005		
Condition of the calibrated item	In Tolerance		
The measurements and the unce	ertainties with confidence	ational standards, which realize the physical units of probability are given on the following pages and are	e part of the certificate.
		ory facility: environment temperature (22 ± 3)°C and	a numidity < 70%.
Calibration Equipment used (M&	TE critical for calibration)		
Calibration Equipment used (M&	TE critical for calibration)	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Calibration Equipment used (M& Primary Standards Power meter E4419B	TE critical for calibration) ID # GB41293874	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466)	Scheduled Callibration May-06
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A	TE critical for calibration) ID # GB41293874 MY41495277	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-90466) 3-May-05 (METAS, No. 251-90466)	Scheduled Calibration May-06 May-06
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A	ID # GB41293874 MY41495277 MY41498087	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-90466) 3-May-05 (METAS, No. 251-90466) 3-May-05 (METAS, No. 251-90466)	Scheduled Calibration May-06 May-06 May-06
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c)	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 10-Aug-04 (METAS, No. 251-00403)	Scheduled Calibration May-06 May-06 May-06 Aug-05
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b)	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 10-Aug-04 (METAS, No. 251-00403) 3-May-05 (METAS, No. 251-00467)	Scheduled Calibration May-06 May-06 May-06 Aug-05 May-06
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator	TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b)	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00403) 3-May-05 (METAS, No. 251-00407) 10-Aug-04 (METAS, No. 251-00404)	Scheduled Calibration May-06 May-06 May-06 Aug-05 May-06 Aug-05
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe H3DV6	TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b)	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 10-Aug-04 (METAS, No. 251-00403) 3-May-05 (METAS, No. 251-00467)	Scheduled Calibration May-06 May-06 May-06 Aug-05 May-06
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe H3DV6 DAE4	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 6182 SN: 617	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 10-Aug-04 (METAS, No. 251-00403) 3-May-05 (METAS, No. 251-00407) 10-Aug-04 (METAS, No. 251-00404) 6-Oct-04 (SPEAG, No. H3-6182_Oct04) 19-Jan-05 (SPEAG, No. DAE4-617_Jan05) Check Date (in house)	Scheduled Calibration May-06 May-06 May-06 Aug-05 Aug-05 Cot-05 Jan-06 Scheduled Check
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe H3DV6 DAE4	TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 6182 SN: 617	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 10-Aug-04 (METAS, No. 251-00403) 3-May-05 (METAS, No. 251-00407) 10-Aug-04 (METAS, No. 251-00404) 6-Oct-04 (SPEAG, No. H3-6182_Oct04) 19-Jan-05 (SPEAG, No. DAE4-617_Jan05) Check Date (in house) 4-Aug-99 (SPEAG, in house check Dec-03)	Scheduled Calibration May-06 May-06 May-06 Aug-05 May-06 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Dec-05
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 70 dB Attenuator Reference Probe H3DV6 DAE4 Secondary Standards RF generator HP 8848C	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 6182 SN: 617	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 10-Aug-04 (METAS, No. 251-00403) 3-May-05 (METAS, No. 251-00407) 10-Aug-04 (METAS, No. 251-00404) 6-Oct-04 (SPEAG, No. H3-6182_Oct04) 19-Jan-05 (SPEAG, No. DAE4-617_Jan05) Check Date (in house)	Scheduled Calibration May-06 May-06 May-06 Aug-05 Aug-05 Cot-05 Jan-06 Scheduled Check
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe H3DV6 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 6182 SN: 617 ID # U\$3642U01700 U\$37390585 Name	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 10-Aug-04 (METAS, No. 251-00403) 3-May-05 (METAS, No. 251-00467) 10-Aug-04 (METAS, No. 251-00404) 6-Oct-04 (SPEAG, No. H3-6182_Oct04) 19-Jan-05 (SPEAG, No. DAE4-617_Jan05) Check Date (in house) 4-Aug-99 (SPEAG, in house check Dec-03) 18-Oct-01 (SPEAG, in house check Nov-04) Function	Scheduled Calibration May-06 May-06 May-06 Aug-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Dec-05 In house check: Nov 05
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 70 dB Attenuator Reference Probe H3DV6 DAE4 Secondary Standards RF generator HP 8648C	TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 65122 SN: 617 ID # US3642U01700 US37390585	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 10-Aug-04 (METAS, No. 251-00403) 3-May-05 (METAS, No. 251-00467) 10-Aug-04 (METAS, No. 251-00404) 6-Oct-04 (SPEAG, No. H3-6182_Oct04) 19-Jan-05 (SPEAG, No. DAE4-617_Jan05) Check Date (in house) 4-Aug-99 (SPEAG, in house check Dec-03) 18-Oct-01 (SPEAG, in house check Nov-04)	Scheduled Callibration May-06 May-06 May-06 Aug-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Dec-05 In house check: Nov 05
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe H3DV6 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 6182 SN: 617 ID # U\$3642U01700 U\$37390585 Name	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 10-Aug-04 (METAS, No. 251-00403) 3-May-05 (METAS, No. 251-00467) 10-Aug-04 (METAS, No. 251-00404) 6-Oct-04 (SPEAG, No. H3-6182_Oct04) 19-Jan-05 (SPEAG, No. DAE4-617_Jan05) Check Date (in house) 4-Aug-99 (SPEAG, in house check Dec-03) 18-Oct-01 (SPEAG, in house check Nov-04) Function	Scheduled Calibration May-06 May-06 May-06 Aug-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Dec-05 In house check: Nov 05

Certificate No: H3-6029_Jun05

Page 1 of 8





Appendix B: System Validation Data

(See attachment)





Appendix C: Test Results/Plots

(See attachment)