	Date of Evaluation:	July 30, 2007	Document Serial No.:	SV450B-073007-R1.0
	Evaluation Type:	System Validation	Validation Dipole:	450 MHz
			Fluid Type:	Brain

450 MHz SYSTEM VALIDATION

Type:

450 MHz Validation Dipole

Asset Number:

00024

Serial Number:

136

Place of Validation:

Celltech Labs Inc.

Date of Validation:

July 30, 2007

Celltech Labs Inc. certifies that the 450 MHz System Validation was performed on the date indicated above.



Validated by:


Cheri Frangiadakis

Approved by:

Sean Johnston

2. Validation Dipole VSWR Data

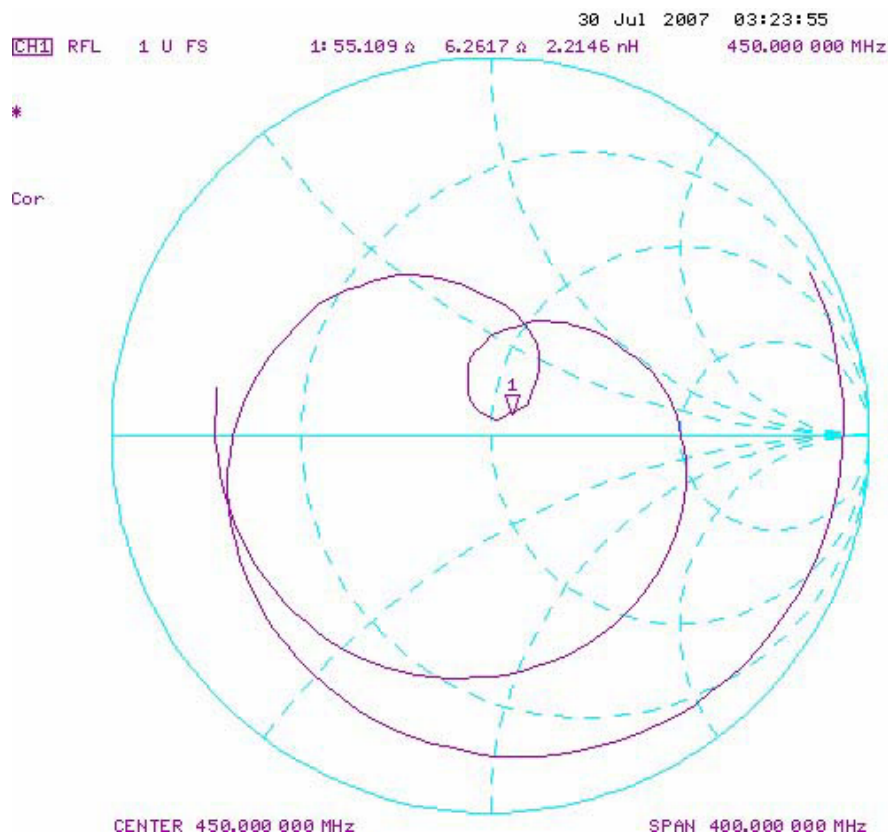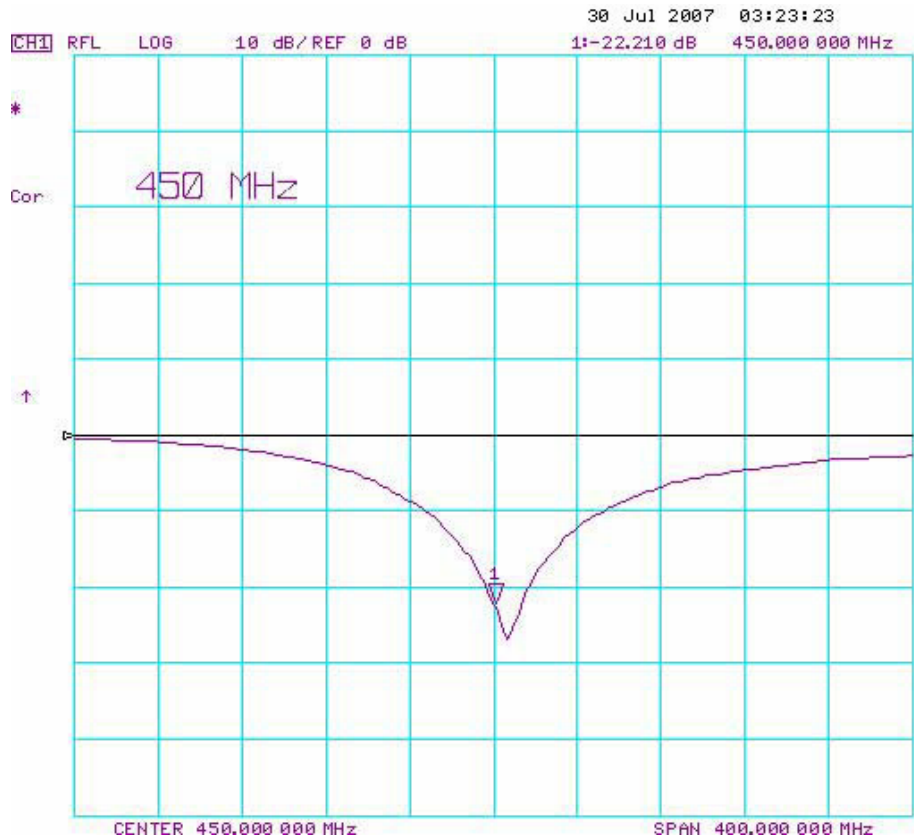

	Date of Evaluation:	July 30, 2007	Document Serial No.:	SV450B-073007-R1.0
	Evaluation Type:	System Validation	Validation Dipole:	450 MHz
			Fluid Type:	Brain

3. Validation Dipole Dimensions

Frequency (MHz)	L (mm)	h (mm)	d (mm)
300	396.0	250.0	6.0
450	270.0	167.0	6.0
835	161.0	89.8	3.6
900	149.0	83.3	3.6
1450	89.1	51.7	3.6
1800	72.0	41.7	3.6
1900	68.0	39.5	3.6
2000	64.5	37.5	3.6
2450	51.5	30.4	3.6
3000	41.5	25.0	3.6

4. Validation Phantom

The validation phantom (planar) was constructed using relatively low-loss tangent Plexiglas material.

The inner dimensions of the validation phantom are as follows:


Length: 83.5 cm
Width: 36.9 cm
Height: 21.8 cm


The bottom section of the validation phantom is constructed of 6.2 ± 0.1 mm Plexiglas.

5. Test Equipment List

TEST EQUIPMENT	ASSET NO.	SERIAL NO.	DATE OF CAL.	CAL. DUE DATE
SPEAG DASY4 Measurement Server	00158	1078	N/A	N/A
SPEAG Robot	00046	599396-01	N/A	N/A
SPEAG DAE4	00019	353	10Jul07	10Jul08
SPEAG ET3DV6 E-Field Probe	00016	1387	16Mar07	16Mar08
450 MHz Validation Dipole	00024	136	30Jul07	30Jul08
Plexiglas Validation Planar Phantom	00157	137	N/A	N/A
HP 85070C Dielectric Probe Kit	00033	US39240170	N/A	N/A
Gigatronics 8652A Power Meter	00007	1835272	26Mar07	26Mar08
Gigatronics 80701A Power Sensor	00014	1833699	22Jan07	22Jan08
Gigatronics 80701A Power Sensor	00109	1834366	26Mar07	26Mar08
HP 8753ET Network Analyzer	00134	US39170292	20Apr07	20Apr08
HP 8648D Signal Generator	00005	3847A00611	NCR	NCR
Amplifier Research 5S1G4 Power Amplifier	00106	26235	NCR	NCR


6. Dimensions of Plexiglas Planar Phantom

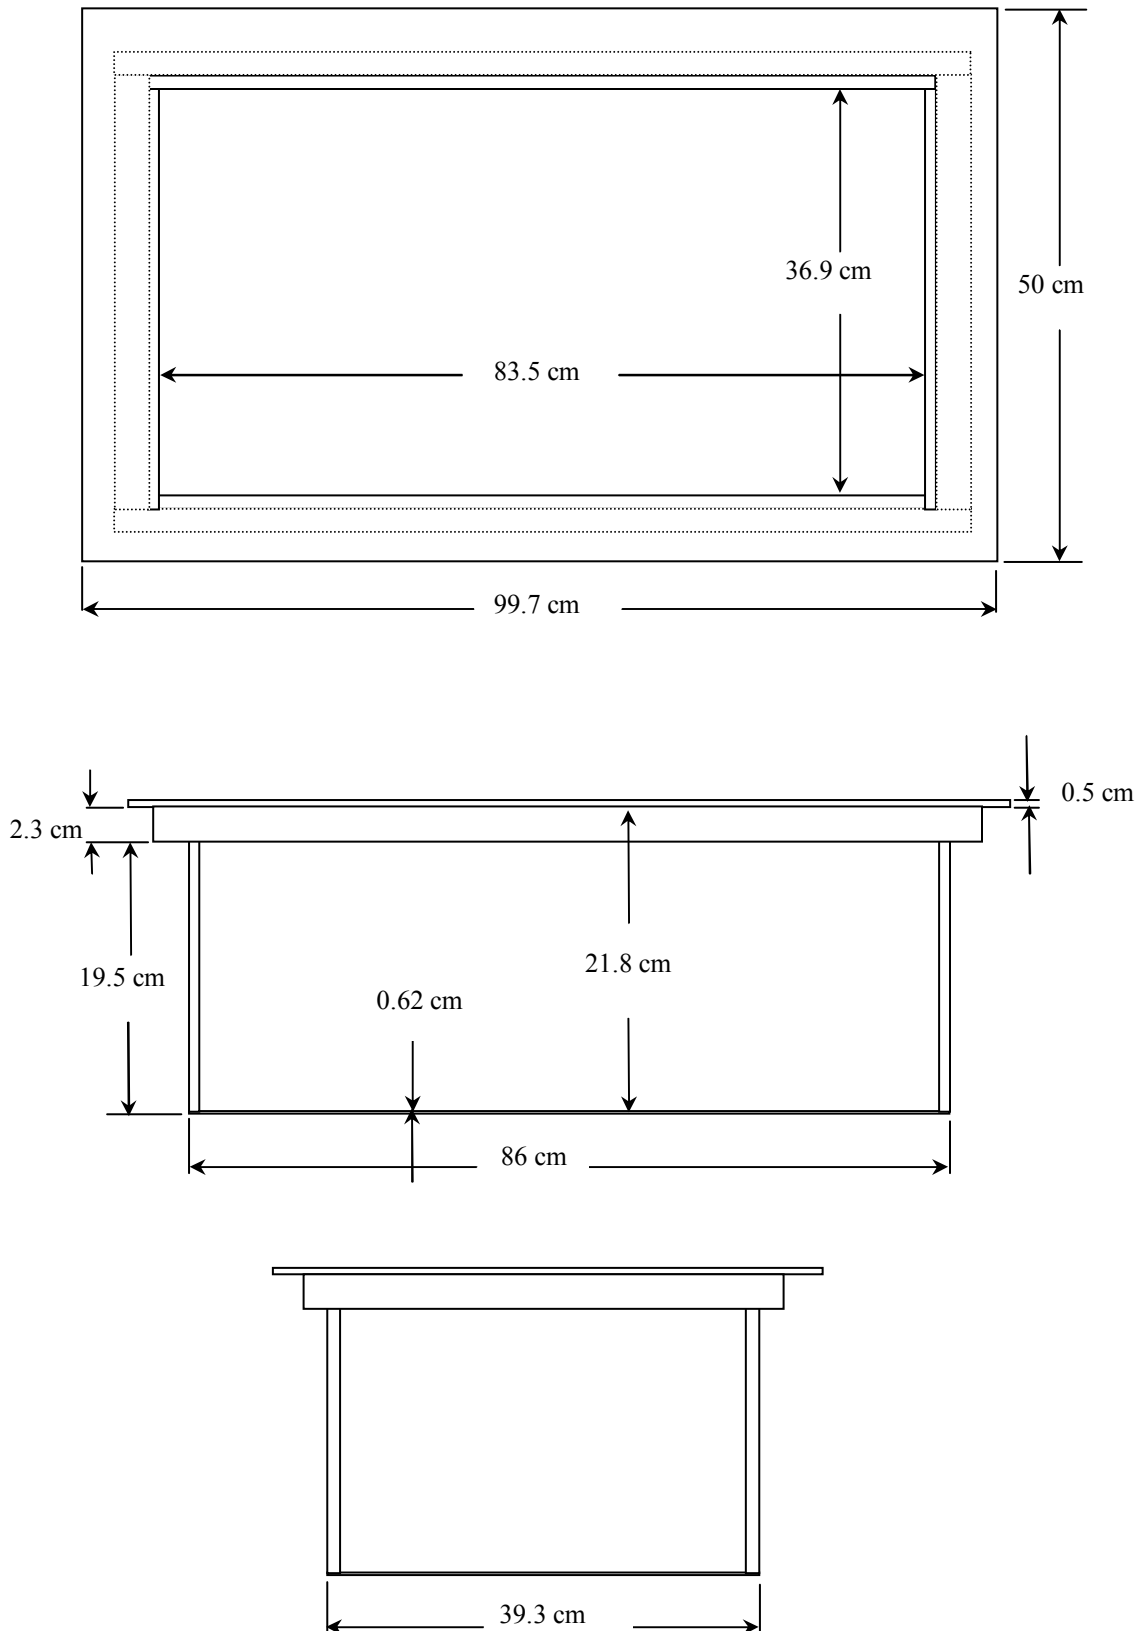

	Date of Evaluation:	July 30, 2007	Document Serial No.:	SV450B-073007-R1.0
	Evaluation Type:	System Validation	Validation Dipole:	450 MHz
			Fluid Type:	Brain


7. 450 MHz System Validation Setup



	Date of Evaluation:		July 30, 2007	Document Serial No.:		SV450B-073007-R1.0	
	Evaluation Type:	System Validation	Validation Dipole:	450 MHz	Fluid Type:	Brain	

8. 450 MHz Validation Dipole Setup





	Date of Evaluation:	July 30, 2007	Document Serial No.:	SV450B-073007-R1.0
	Evaluation Type:	System Validation	Validation Dipole:	450 MHz
			Fluid Type:	Brain

9. SAR Measurement

Measurements were made using a dosimetric E-field probe ET3DV6 (S/N: 1387, Conversion Factor 7.0). The SAR measurement was performed with the E-field probe in mechanical detection mode only. The setup and determination of the forward power into the dipole was performed using the procedures described below.

First the power meter PM1 (including attenuator Att1) is connected to the cable to measure the forward power at the location of the dipole connector (X). The signal generator is adjusted for the desired forward power at the dipole connector (taking into account the attenuation of Att1) as read by power meter PM2. After connecting the cable to the dipole, the signal generator is readjusted for the same reading at power meter PM2. If the signal generator does not allow adjustment in 0.01dB steps, the remaining difference at PM2 must be taken into consideration. PM3 records the reflected power from the dipole to ensure that the value is not changed from the previous value. The reflected power should be 20dB below the forward power.

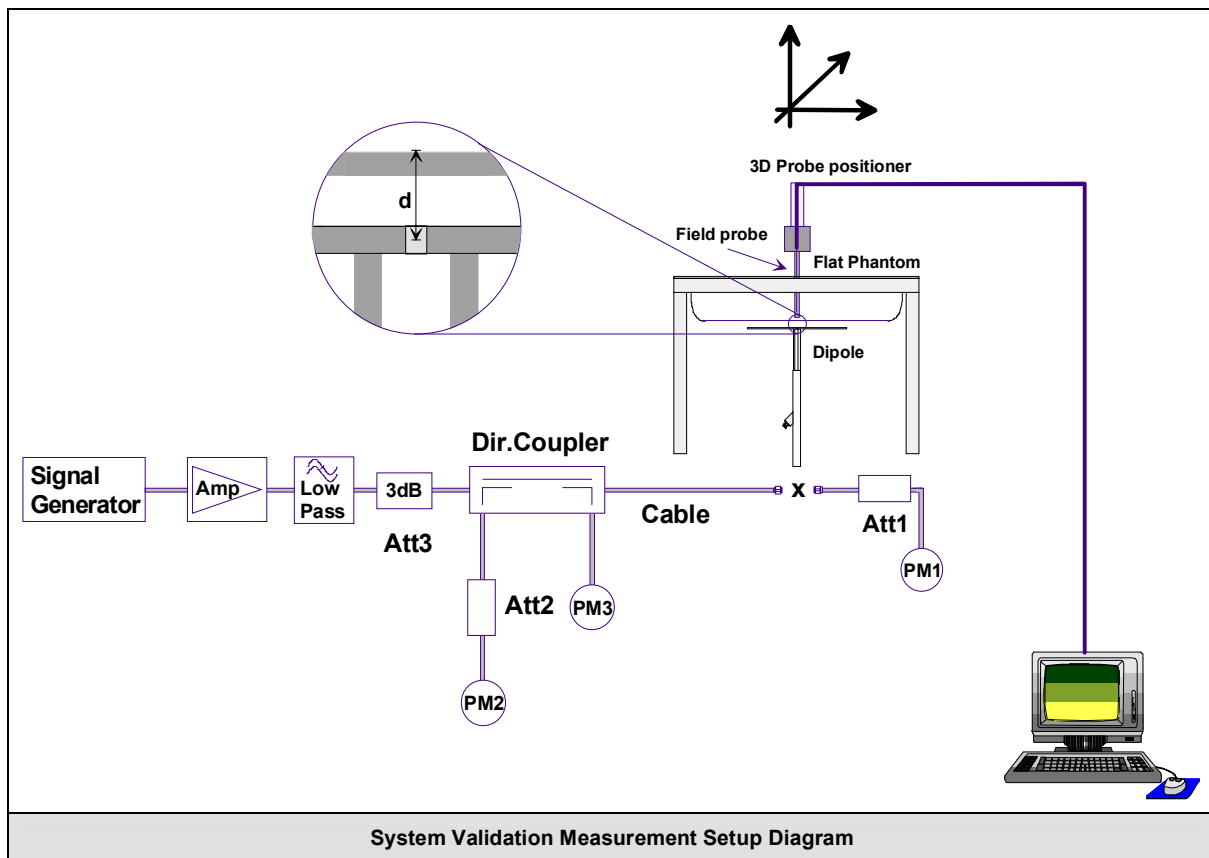

	Date of Evaluation:	July 30, 2007	Document Serial No.:	SV450B-073007-R1.0
	Evaluation Type:	System Validation	Validation Dipole:	450 MHz
			Fluid Type:	Brain

10. Measurement Conditions

The validation phantom was filled with 450 MHz Brain tissue simulant.

Relative Permittivity: 43.1 (-0.9% deviation from target)
 Conductivity: 0.85 mho/m (-2.3% deviation from target)
 Fluid Temperature: 23.1°C (Start of Test) / 23.3°C (End of Test)
 Fluid Depth: ≥ 15.0 cm

Environmental Conditions:


Ambient Temperature: 24.5°C
 Barometric Pressure: 101.1 kPa
 Humidity: 31%

The 450 MHz Brain tissue simulant consisted of the following ingredients:

Ingredient	Percentage by weight
Water	38.56%
Sugar	56.32%
Salt	3.95%
HEC	0.98%
Dowicil 75	0.19%
IEEE Target Dielectric Parameters:	$\epsilon_r = 43.5 (+/- 5\%)$ $\sigma = 0.87 \text{ S/m } (+/- 5\%)$

11. System Validation SAR Results

SAR @ 0.25W Input averaged over 1g (W/kg)				SAR @ 1W Input averaged over 1g (W/kg)																																																										
IEEE/IEC Target		Measured	Deviation	IEEE/IEC Target		Measured	Deviation																																																							
1.23	+/- 10%	1.29	+4.9%	4.9	+/- 10%	5.16	+5.3%																																																							
SAR @ 0.25W Input averaged over 10g (W/kg)				SAR @ 1W Input averaged over 10g (W/kg)																																																										
IEEE/IEC Target		Measured	Deviation	IEEE/IEC Target		Measured	Deviation																																																							
0.825	+/- 10%	0.832	+0.8%	3.3	+/- 10%	3.33	+1.0%																																																							
<table><tr><th>Frequency (MHz)</th><th>1 g SAR</th><th>10 g SAR</th><th>Local SAR at surface (above feed-point)</th><th>Local SAR at surface (y = 2 cm offset from feed-point)^a</th></tr><tr><td>300</td><td>3.0</td><td>2.0</td><td>4.4</td><td>2.1</td></tr><tr><td>450</td><td>4.9</td><td>3.3</td><td>7.2</td><td>3.2</td></tr><tr><td>835</td><td>9.5</td><td>6.2</td><td>4.1</td><td>4.9</td></tr><tr><td>900</td><td>10.8</td><td>6.9</td><td>16.4</td><td>5.4</td></tr><tr><td>1450</td><td>29.0</td><td>16.0</td><td>50.2</td><td>6.5</td></tr><tr><td>1800</td><td>38.1</td><td>19.8</td><td>69.5</td><td>6.8</td></tr><tr><td>1900</td><td>39.7</td><td>20.5</td><td>72.1</td><td>6.6</td></tr><tr><td>2000</td><td>41.1</td><td>21.1</td><td>74.6</td><td>6.5</td></tr><tr><td>2450</td><td>52.4</td><td>24.0</td><td>104.2</td><td>7.7</td></tr><tr><td>3000</td><td>63.8</td><td>25.7</td><td>140.2</td><td>9.5</td></tr></table>								Frequency (MHz)	1 g SAR	10 g SAR	Local SAR at surface (above feed-point)	Local SAR at surface (y = 2 cm offset from feed-point) ^a	300	3.0	2.0	4.4	2.1	450	4.9	3.3	7.2	3.2	835	9.5	6.2	4.1	4.9	900	10.8	6.9	16.4	5.4	1450	29.0	16.0	50.2	6.5	1800	38.1	19.8	69.5	6.8	1900	39.7	20.5	72.1	6.6	2000	41.1	21.1	74.6	6.5	2450	52.4	24.0	104.2	7.7	3000	63.8	25.7	140.2	9.5
Frequency (MHz)	1 g SAR	10 g SAR	Local SAR at surface (above feed-point)	Local SAR at surface (y = 2 cm offset from feed-point) ^a																																																										
300	3.0	2.0	4.4	2.1																																																										
450	4.9	3.3	7.2	3.2																																																										
835	9.5	6.2	4.1	4.9																																																										
900	10.8	6.9	16.4	5.4																																																										
1450	29.0	16.0	50.2	6.5																																																										
1800	38.1	19.8	69.5	6.8																																																										
1900	39.7	20.5	72.1	6.6																																																										
2000	41.1	21.1	74.6	6.5																																																										
2450	52.4	24.0	104.2	7.7																																																										
3000	63.8	25.7	140.2	9.5																																																										
Numerical reference SAR values for reference dipole and flat phantom normalized to 1 W (IEEE 1528-2003; IEC 62209-1:2005)																																																														

	Date of Evaluation:	July 30, 2007	Document Serial No.:	SV450B-073007-R1.0
	Evaluation Type:	System Validation	Validation Dipole:	450 MHz
			Fluid Type:	Brain

System Validation - 450 MHz Dipole - July 30, 2007 - HSL

DUT: Dipole 450 MHz; Asset: 00024; Serial: 136; Validation: 07/30/2007

Ambient Temp: 24.5°C; Fluid Temp: 23.1°C; Barometric Pressure: 101.1 kPa; Humidity: 31%

Communication System: CW

Forward Conducted Power: 250 mW

Frequency: 450 MHz; Duty Cycle: 1:1

Medium: HSL450 Medium parameters used: $f = 450 \text{ MHz}$; $\sigma = 0.85 \text{ mho/m}$; $\epsilon_r = 43.1$; $\rho = 1000 \text{ kg/m}^3$

- Probe: ET3DV6 - SN1387; ConvF(7, 7, 7); Calibrated: 16/03/2007
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn353; Calibrated: 10/07/2007
- Phantom: Validation Planar; Type: Plexiglas; Serial: 137
- Measurement SW: DASY4, V4.7 Build 44; Postprocessing SW: SEMCAD, V1.8 Build 171

450 MHz Dipole - System Validation/Area Scan (6x11x1):

Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (measured) = 1.35 mW/g

450 MHz Dipole - System Validation/Zoom Scan (5x5x7)/Cube 0:


Measurement grid: $dx=7.5\text{mm}$, $dy=7.5\text{mm}$, $dz=5\text{mm}$


Reference Value = 39.3 V/m; Power Drift = 0.042 dB

Peak SAR (extrapolated) = 2.24 W/kg

SAR(1 g) = 1.29 mW/g; SAR(10 g) = 0.832 mW/g

Maximum value of SAR (measured) = 1.37 mW/g

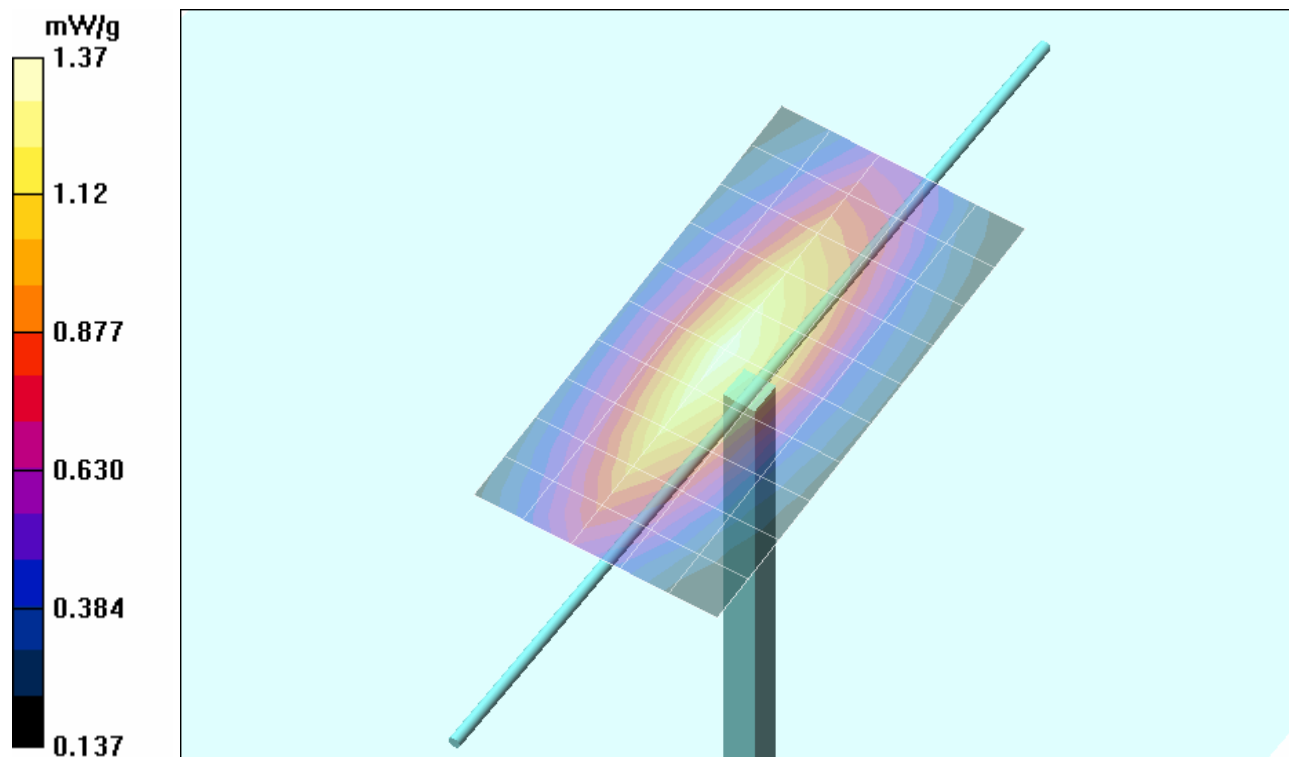

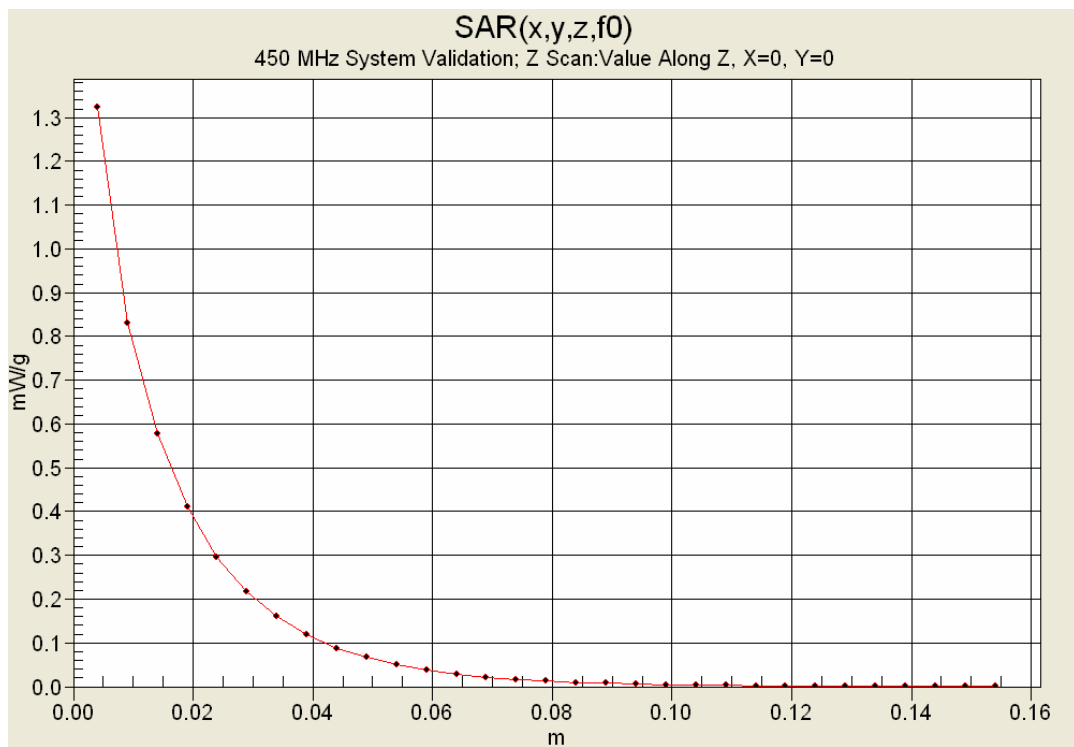

12. Measured Fluid Dielectric Parameters

System Validation - 450 MHz (Brain)

Celltech Labs Inc.

Test Result for UIM Dielectric Parameter

Mon 30/Jul/2007

Frequency (GHz)


FCC_eH FCC OET 65 Supplement C (June 2001) Limits for Head Epsilon

FCC_sH FCC OET 65 Supplement C (June 2001) Limits for Head Sigma

Test_e Epsilon of UIM

Test_s Sigma of UIM

Freq	FCC_eH	FCC_sH	Test_e	Test_s
0.3500	44.70	0.87	45.67	0.76
0.3600	44.58	0.87	45.22	0.77
0.3700	44.46	0.87	45.13	0.78
0.3800	44.34	0.87	44.88	0.79
0.3900	44.22	0.87	44.58	0.80
0.4000	44.10	0.87	44.42	0.81
0.4100	43.98	0.87	44.21	0.82
0.4200	43.86	0.87	43.93	0.82
0.4300	43.74	0.87	43.66	0.83
0.4400	43.62	0.87	43.15	0.84
0.4500	43.50	0.87	43.09	0.85
0.4600	43.45	0.87	42.96	0.86
0.4700	43.40	0.87	42.63	0.87
0.4800	43.34	0.87	42.72	0.87
0.4900	43.29	0.87	42.45	0.89
0.5000	43.24	0.87	42.18	0.90
0.5100	43.19	0.87	42.03	0.90
0.5200	43.14	0.88	41.77	0.91
0.5300	43.08	0.88	41.78	0.92
0.5400	43.03	0.88	41.42	0.93
0.5500	42.98	0.88	41.19	0.93

	Date of Evaluation:		July 30, 2007		Document Serial No.:		SV450B-073007-R1.0	
	Evaluation Type:	System Validation		Validation Dipole:	450 MHz	Fluid Type:	Brain	

13. Measurement Uncertainties

UNCERTAINTY BUDGET FOR SYSTEM VALIDATION						
Error Description	Uncertainty Value ±%	Probability Distribution	Divisor	ci 1g	Uncertainty Value ±% (1g)	V _i or V _{eff}
Measurement System						
Probe calibration (450 MHz)	8.0	Normal	1	1	8.0	∞
Axial isotropy of the probe	4.7	Rectangular	1.732050808	1	2.7	∞
Spherical isotropy of the probe	0	Rectangular	1.732050808	1	0.0	∞
Spatial resolution	0	Rectangular	1.732050808	1	0.0	∞
Boundary effects	1	Rectangular	1.732050808	1	0.6	∞
Probe linearity	4.7	Rectangular	1.732050808	1	2.7	∞
Detection limit	1	Rectangular	1.732050808	1	0.6	∞
Readout electronics	0.3	Normal	1	1	0.3	∞
Response time	0	Rectangular	1.732050808	1	0.0	∞
Integration time	0	Rectangular	1.732050808	1	0.0	∞
RF ambient conditions	3	Rectangular	1.732050808	1	1.7	∞
Mech. constraints of robot	0.4	Rectangular	1.732050808	1	0.2	∞
Probe positioning	2.9	Rectangular	1.732050808	1	1.7	∞
Extrapolation & integration	1	Rectangular	1.732050808	1	0.6	∞
Test Sample Related						
Dipole Positioning	2	Normal	1.732050808	1	1.2	∞
Power & Power Drift	4.7	Normal	1.732050808	1	2.7	∞
Phantom and Setup						
Phantom uncertainty	4	Rectangular	1.732050808	1	2.3	∞
Liquid conductivity (target)	5	Rectangular	1.732050808	0.64	1.8	∞
Liquid conductivity (measured)	5	Normal	1	0.64	3.2	∞
Liquid permittivity (target)	5	Rectangular	1.732050808	0.6	1.7	∞
Liquid permittivity (measured)	5	Normal	1	0.6	3.0	∞
Combined Standard Uncertainty					11.20	
Expanded Uncertainty (k=2)					22.39	
Measurement Uncertainty Table in accordance with IEEE Standard 1528-2003						