

Validation Dipole D835V2 SN:406, $d = 15\text{mm}$

Frequency: 835 MHz; Antenna Input Power: 250 [mW]


Generic Twin Phantom; Flat Section; Grid Spacing: $D_x = 20.0$, $D_y = 20.0$, $D_z = 10.0$

Probe: ET3DV5 - SN1342/DAE3; ConvF(5.75,5.75,5.75); Brain 835 MHz: $\sigma = 0.79$ mho/m $\epsilon_r = 41.9$ $\rho = 1.00$ g/cm³

Cubes (2): Peak: 3.17 mW/g ± 0.03 dB, SAR (1g): 2.11 mW/g ± 0.03 dB, SAR (10g): 1.41 mW/g ± 0.04 dB, (Worst-case extrapolation)

Penetration depth: 13.4 (12.3, 14.9) [mm]

Powerdrift: -0.01 dB

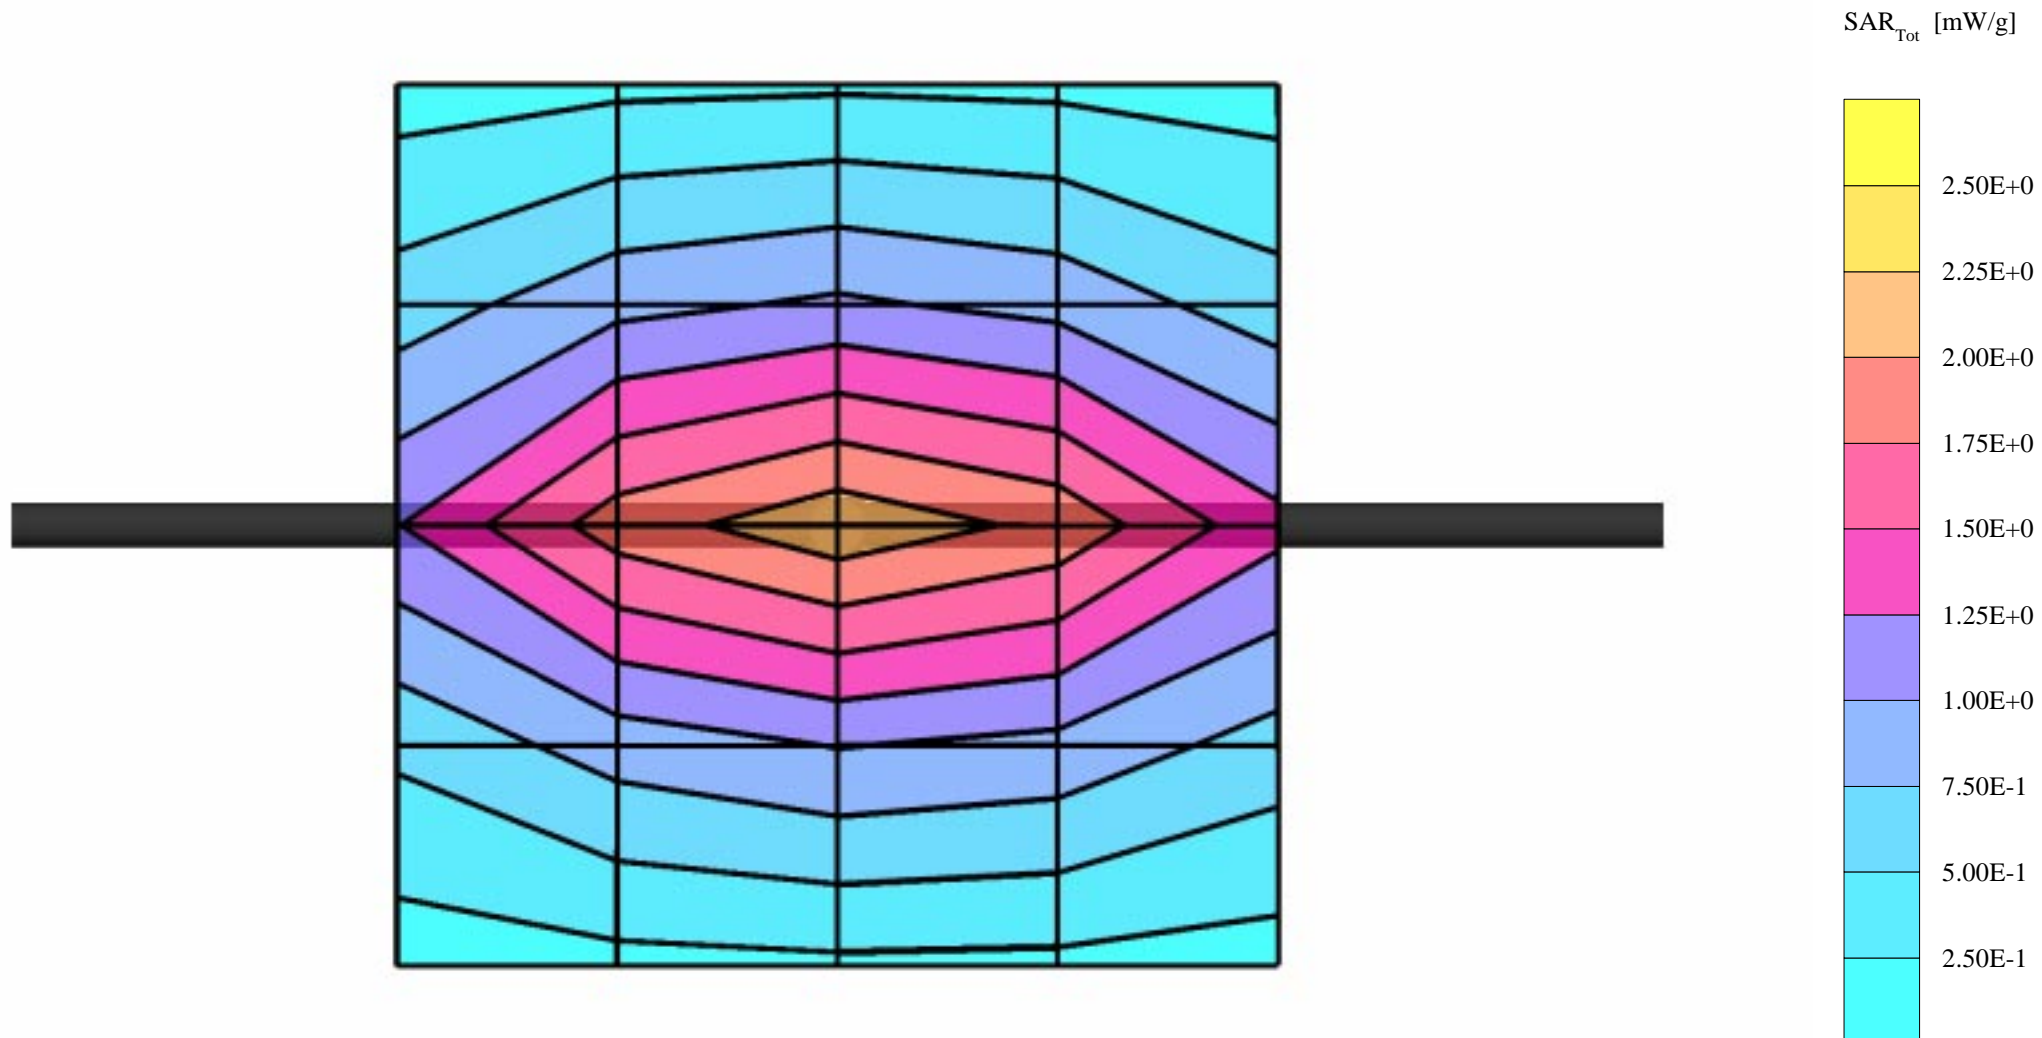

835MHz Muscle Dipole Validation

Generic Twin Phantom; Flat Section; Probe: ET3DV5 - SN1368 -- Probe Cal Date 2/99

Medium Parameters 835 Muscle: $\sigma = 0.95$ mho/m $\epsilon_r = 56.2$ $\rho = 1.00$ g/cm³; Antenna Position -- Out; Crest Factor 1.0

SAR (1g): 2.20 mW/g, SAR (10g): 1.36 mW/g

835MHz Muscle Dipole Validation (D835V2 S/N: 406)

Frequency: 835 MHz; Antenna Input Power: 250 [mW]

PCTEST Muscle Tissue Simulating Liquid

