

## Appendix C for KSCR240300047301


### Calibration Certificate

Object	Apply	No	Model	SN	Calibration Date	Due date of calibration
Dipole	<input type="checkbox"/>	1	D750V3	1188	2022/03/29	2025/03/28
	<input checked="" type="checkbox"/>	2	D835V2	4d114	2022/03/31	2025/03/30
	<input type="checkbox"/>	3	D900V2	1d079	2022/06/07	2025/06/06
	<input checked="" type="checkbox"/>	4	D1800V2	2d170	2022/03/31	2025/03/30
	<input checked="" type="checkbox"/>	5	D1900V2	5d136	2022/06/07	2025/06/06
	<input type="checkbox"/>	6	D2000V2	1041	2022/06/06	2025/06/05
	<input type="checkbox"/>	7	D2300V2	1096	2022/03/31	2025/03/30
	<input checked="" type="checkbox"/>	8	D2450V2	817	2022/04/01	2025/03/31
	<input checked="" type="checkbox"/>	9	D2600V2	1158	2022/03/31	2025/03/30
	<input type="checkbox"/>	10	D5GHzV2	1095	2022/06/01	2025/05/31
DAE	<input checked="" type="checkbox"/>	11	DAE4ip	1826	2023/12/27	2024/12/26
Probe	<input checked="" type="checkbox"/>	12	EX3DV4	7833	2023/08/24	2024/08/23

# 1 Dipole

## 1.1 D750V3 - SN 1188

<p><b>TTL</b> <i>s p e a g</i> CALIBRATION LABORATORY</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com</p> <p>Client: <b>SGS-CN</b> Certificate No: <b>Z22-60103</b></p> <p><b>CALIBRATION CERTIFICATE</b></p> <p>Object: <b>D750V3 - SN: 1188</b></p> <p>Calibration Procedure(s): <b>FF-Z11-003-01</b> Calibration Procedures for dipole validation kits</p> <p>Calibration date: <b>March 29, 2022</b></p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity&lt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL, No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CTTL, No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21 (SPEAG, No EX3-7307, May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22 (CTTL-SPEAG, No Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4438C</td> <td>MY49071430</td> <td>13-Jan-22 (CTTL, No.J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY46110673</td> <td>14-Jan-22 (CTTL, No.J22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table> <p>Calibrated by: <b>Zhao Jing</b> SAR Test Engineer Reviewed by: <b>Lin Hao</b> SAR Test Engineer Approved by: <b>Qi Dianyuan</b> SAR Project Leader</p> <p>Issued: April 3, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No: Z22-60103 Page 1 of 6</p>	Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CTTL, No.J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG, No EX3-7307, May21)	May-22	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG, No Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No.J22X00409)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No.J22X00406)	Jan-23	<p><b>TTL</b> <i>s p e a g</i> CALIBRATION LABORATORY</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com</p> <p><b>CAICT</b> CALIBRATION ONE-LEVEL</p> <p><b>Glossary:</b> TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORM<sub>x,y,z</sub> N/A: not applicable or not measured</p> <p><b>Calibration is Performed According to the Following Standards:</b> a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865684, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p><b>Additional Documentation:</b> c) DASy4.5 System Handbook</p> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li><b>Measurement Conditions:</b> Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.</li> <li><b>Antenna Parameters with TSL:</b> The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.</li> <li><b>Feed Point Impedance and Return Loss:</b> These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.</li> <li><b>Electrical Delay:</b> One-way delay between the SMA connector and the antenna feed point. No uncertainty required.</li> <li><b>SAR measured:</b> SAR measured at the stated antenna input power.</li> <li><b>SAR normalized:</b> SAR as measured, normalized to an input power of 1 W at the antenna connector.</li> <li><b>SAR for nominal TSL parameters:</b> The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: Z22-60103 Page 2 of 6</p>																												
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																										
Power Meter NRP2	106277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22																																																										
Power sensor NRP8S	104291	24-Sep-21 (CTTL, No.J21X08326)	Sep-22																																																										
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG, No EX3-7307, May21)	May-22																																																										
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG, No Z22-60007)	Jan-23																																																										
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																										
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No.J22X00409)	Jan-23																																																										
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No.J22X00406)	Jan-23																																																										
<p><b>TTL</b> <i>s p e a g</i> CALIBRATION LABORATORY</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com</p> <p><b>CAICT</b></p> <p><b>Measurement Conditions</b> DASy system configuration, as far as not given on page 1.</p> <table border="1"> <thead> <tr> <th>DASy Version</th> <th>DASyS2</th> <th>V52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>750 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p><b>Head TSL parameters</b> The following parameters and calculations were applied.</p> <table border="1"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>42.0</td> <td>0.80 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>41.4 ± 6 %</td> <td>0.89 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>&lt;1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p><b>SAR result with Head TSL</b></p> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</th> <th>Condition</th> <th>2.07 W/kg</th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td></td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>8.27 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</td> <th>Condition</th> <th>1.37 W/kg</th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td></td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>5.48 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> <p>Certificate No: Z22-60103 Page 3 of 6</p>	DASy Version	DASyS2	V52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	750 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	42.0	0.80 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	2.07 W/kg	SAR measured	250 mW input power		SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	1.37 W/kg	SAR measured	250 mW input power		SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)	<p><b>TTL</b> <i>s p e a g</i> CALIBRATION LABORATORY</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com</p> <p><b>CAICT</b></p> <p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1"> <thead> <tr> <th>Impedance, transformed to feed point</th> <th>53.60- 1.13jΩ</th> </tr> </thead> <tbody> <tr> <td>Return Loss</td> <td>-28.7dB</td> </tr> </tbody> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1"> <thead> <tr> <th>Electrical Delay (one direction)</th> <th>0.947 ns</th> </tr> </thead> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1"> <thead> <tr> <th>Manufactured by</th> <th>SPEAG</th> </tr> </thead> </table> <p>Certificate No: Z22-60103 Page 4 of 6</p>	Impedance, transformed to feed point	53.60- 1.13jΩ	Return Loss	-28.7dB	Electrical Delay (one direction)	0.947 ns	Manufactured by	SPEAG
DASy Version	DASyS2	V52.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	Triple Flat Phantom 5.1C																																																												
Distance Dipole Center - TSL	15 mm	with Spacer																																																											
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																												
Frequency	750 MHz ± 1 MHz																																																												
	Temperature	Permittivity	Conductivity																																																										
Nominal Head TSL parameters	22.0 °C	42.0	0.80 mho/m																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %																																																										
Head TSL temperature change during test	<1.0 °C	---	---																																																										
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	2.07 W/kg																																																											
SAR measured	250 mW input power																																																												
SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)																																																											
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	1.37 W/kg																																																											
SAR measured	250 mW input power																																																												
SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)																																																											
Impedance, transformed to feed point	53.60- 1.13jΩ																																																												
Return Loss	-28.7dB																																																												
Electrical Delay (one direction)	0.947 ns																																																												
Manufactured by	SPEAG																																																												

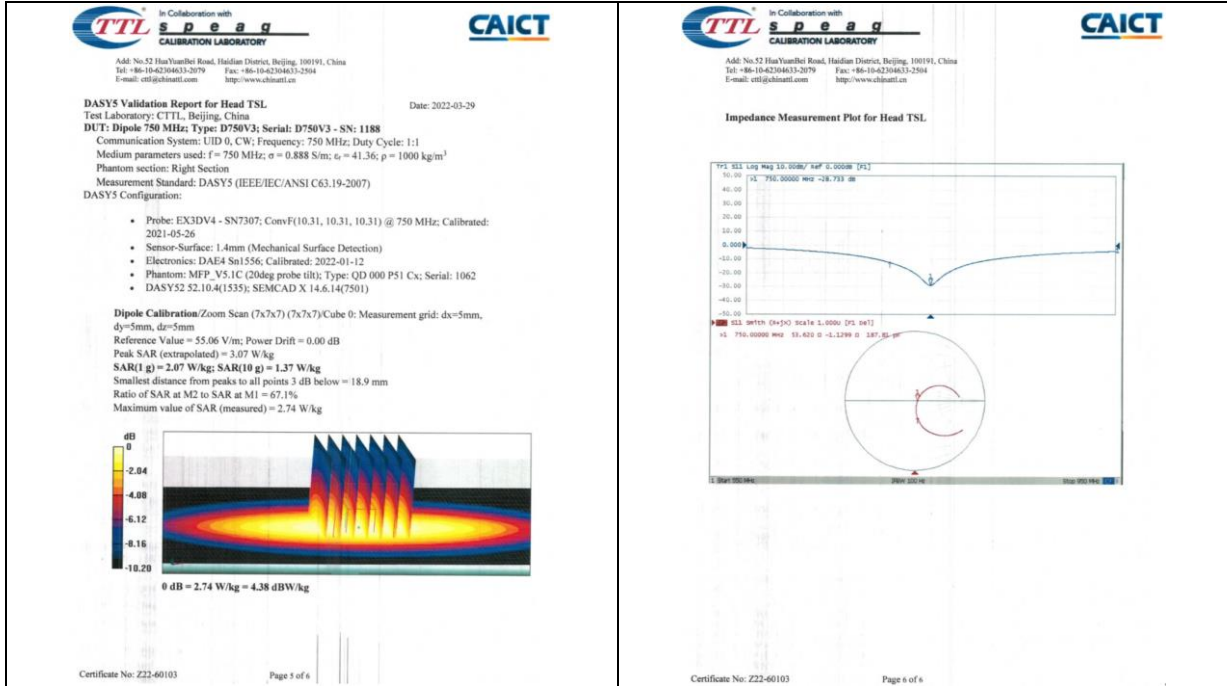

## 1.2 D835V2 - SN 4d114

<p>In Collaboration with <b>TTT S p e a g</b> CALIBRATION LABORATORY and <b>CAICT</b></p> <p>Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttt.com.cn http://www.china.ttt.com.cn</p> <p><b>Client:</b> SGS-CN <b>Certificate No.:</b> Z22-60104</p> <p><b>CALIBRATION CERTIFICATE</b></p> <p><b>Object:</b> D835V2 - SN: 4d114</p> <p><b>Calibration Procedure(s):</b> FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p><b>Calibration date:</b> March 31, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity &lt;70%.</p> <p><b>Calibration Equipment used (M&amp;TE critical for calibration)</b></p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL, No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRPBS</td> <td>104281</td> <td>24-Sep-21 (CTTL, No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21(SPEAG No EX3-7307_May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22(CTTL-SPEAG No Z22-60007)</td> <td>Jan-23</td> </tr> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Signal Generator E4439C</td> <td>MY46071430</td> <td>13-Jan-22 (CTTL, No.J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY46110673</td> <td>14-Jan-22 (CTTL, No.J22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table> <p><b>Calibrated by:</b> Zhao Jing, SAR Test Engineer (Signature)</p> <p><b>Reviewed by:</b> Lin Hao, SAR Test Engineer (Signature)</p> <p><b>Approved by:</b> Qi Dianyuan, SAR Project Leader (Signature)</p> <p>Issued: April 6, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No: Z22-60104 Page 1 of 6</p>	Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22	Power sensor NRPBS	104281	24-Sep-21 (CTTL, No.J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7307	26-May-21(SPEAG No EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E4439C	MY46071430	13-Jan-22 (CTTL, No.J22X00409)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No.J22X00406)	Jan-23	<p>In Collaboration with <b>TTT S p e a g</b> CALIBRATION LABORATORY and <b>CAICT</b></p> <p>Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttt.com.cn http://www.china.ttt.com.cn</p> <p><b>Glossary:</b> TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORMx.y.z N/A: not applicable or not measured</p> <p><b>Calibration is Performed According to the Following Standards:</b></p> <ol style="list-style-type: none"> <li>IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020</li> <li>KDB 685664, "SAR Measurement Requirements for 100 MHz to 6 GHz"</li> </ol> <p><b>Additional Documentation:</b></p> <ol style="list-style-type: none"> <li>DASY4/5 System Handbook</li> </ol> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li><b>Measurement Conditions:</b> Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.</li> <li><b>Antenna Parameters with TSL:</b> The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.</li> <li><b>Feed Point Impedance and Return Loss:</b> These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.</li> <li><b>Electrical Delay:</b> One-way delay between the SMA connector and the antenna feed point. No uncertainty required.</li> <li><b>SAR measured:</b> SAR measured at the stated antenna input power.</li> <li><b>SAR normalized:</b> SAR as measured, normalized to an input power of 1 W at the antenna connector.</li> <li><b>SAR for nominal TSL parameters:</b> The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: Z22-60104 Page 2 of 6</p>
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																														
Power Meter NRP2	106277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22																														
Power sensor NRPBS	104281	24-Sep-21 (CTTL, No.J21X08326)	Sep-22																														
Reference Probe EX3DV4	SN 7307	26-May-21(SPEAG No EX3-7307_May21)	May-22																														
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No Z22-60007)	Jan-23																														
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																														
Signal Generator E4439C	MY46071430	13-Jan-22 (CTTL, No.J22X00409)	Jan-23																														
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No.J22X00406)	Jan-23																														

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504  
 E-mail: cti@china.ttl.com http://www.china.ttl.com

**Measurement Conditions**  
 DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	VS2 10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

**Head TSL parameters**  
 The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.0 ± 8 %	0.91 mho/m ± 8 %
Head TSL temperature change during test	<1.0 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.37 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>9.40 W/kg ± 18.6 % (k=2)</b>
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.54 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>6.12 W/kg ± 18.7 % (k=2)</b>

Certificate No: Z22-60104 Page 3 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504  
 E-mail: cti@china.ttl.com http://www.china.ttl.com

**Appendix (Additional assessments outside the scope of CNAS L0570)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	48.7Ω - j22Ω
Return Loss	-25.3dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.307 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z22-60104 Page 4 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504  
 E-mail: cti@china.ttl.com http://www.china.ttl.com

**DASY5 Validation Report for Head TSL** Date: 2022-03-21  
 Test Laboratory: CTTL, Beijing, China  
 DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d114  
 Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1  
 Medium parameters used: f = 835 MHz; σ = 0.907 S/m; ε<sub>r</sub> = 40.98; ρ = 1000 kg/m<sup>3</sup>  
 Phantom section: Right Section  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)  
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(10.13, 10.13, 10.13) @ 835 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA E4 Sn 1556; Calibrated: 2022-01-12
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm**  
 Reference Value = 57.88 V/m; Power Drift = 0.04 dB  
 Peak SAR (extrapolated) = 3.56 W/kg  
**SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.54 W/kg**  
 Smallest distance from peaks to all points 3 dB below = 15.8 mm  
 Ratio of SAR at M2 to SAR at M1 = 66.2%  
 Maximum value of SAR (measured) = 3.17 W/kg

Certificate No: Z22-60104 Page 5 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504  
 E-mail: cti@china.ttl.com http://www.china.ttl.com

**Impedance Measurement Plot for Head TSL**

Certificate No: Z22-60104 Page 6 of 6

## 1.3 D900V2 - SN 1d079

<div style="display: flex; justify-content: space-between; align-items: center;"> </div> <p style="font-size: 8px; margin-top: 5px;">             Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China              Tel: +86-10-42396633-2117              E-mail: cti@china.com.cn http://www.caict.ac.cn         </p> <p style="margin-top: 5px;"> <b>Client:</b> SGS-CN      <b>Certificate No.:</b> Z22-60184         </p> <h3 style="text-align: center; margin-top: 10px;">CALIBRATION CERTIFICATE</h3> <p><b>Object:</b> D900V2 - SN: 1d079</p> <p><b>Calibration Procedure(s):</b> FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p><b>Calibration date:</b> June 7, 2022</p> <p style="font-size: 8px; margin-top: 5px;">             This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.         </p> <p style="font-size: 8px; margin-top: 5px;">             All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity &lt;70%.         </p> <p style="font-size: 8px; margin-top: 5px;">             Calibration Equipment used (M&amp;TE critical for calibration)         </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7464</td> <td>26-Jan-22 (SPEAG No. EX3-7464_Jan22)</td> <td>Jan-23</td> </tr> <tr> <td>DAE4</td> <td>SN 1566</td> <td>12-Jan-22 (CTTL-SPEAG No. Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4438C</td> <td>M146071430</td> <td>13-Jan-22 (CTTL No. J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>M146110673</td> <td>14-Jan-22 (CTTL No. J22X00409)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px; margin-top: 5px;"> <thead> <tr> <th>Calibrated by:</th> <th>Name</th> <th>Function</th> <th>Signature</th> </tr> </thead> <tbody> <tr> <td></td> <td>Zhao Jing</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <td>Reviewed by:</td> <td>Lin Hao</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <td>Approved by:</td> <td>Qi Diqiyuan</td> <td>SAR Project Leader</td> <td></td> </tr> </tbody> </table> <p style="font-size: 8px; margin-top: 5px; text-align: center;">             Issued: June 13, 2022              The calibration certificate shall not be reproduced except in full without written approval of the laboratory.         </p> <p style="font-size: 8px; margin-top: 10px;">             Certificate No: Z22-60184      Page 1 of 6         </p>	Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21X08326)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CTTL No. J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7464	26-Jan-22 (SPEAG No. EX3-7464_Jan22)	Jan-23	DAE4	SN 1566	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	M146071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23	Network Analyzer E5071C	M146110673	14-Jan-22 (CTTL No. J22X00409)	Jan-23	Calibrated by:	Name	Function	Signature		Zhao Jing	SAR Test Engineer		Reviewed by:	Lin Hao	SAR Test Engineer		Approved by:	Qi Diqiyuan	SAR Project Leader		<div style="display: flex; justify-content: space-between; align-items: center;"> </div> <p style="font-size: 8px; margin-top: 5px;">             Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China              Tel: +86-10-42396633-2117              E-mail: cti@china.com.cn http://www.caict.ac.cn         </p> <p style="margin-top: 10px;"> <b>Glossary:</b>              TSL      tissue simulating liquid              ConvF      sensitivity in TSL / NORM<sub>x,y,z</sub>              N/A      not applicable or not measured         </p> <p style="font-size: 8px; margin-top: 10px;"> <b>Calibration is Performed According to the Following Standards:</b>              a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020              b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"              c) DASY4/S System Handbook         </p> <p style="font-size: 8px; margin-top: 5px;"> <b>Additional Documentation:</b>              c) DASY4/S System Handbook         </p> <p style="font-size: 8px; margin-top: 5px;"> <b>Methods Applied and Interpretation of Parameters:</b> </p> <ul style="list-style-type: none"> <li>• <b>Measurement Conditions:</b> Further details are available from the Validation Report at the end of the certificate. All figures stated in this certificate are valid at the frequency indicated.</li> <li>• <b>Antenna Parameters with TSL:</b> The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.</li> <li>• <b>Feed Point Impedance and Return Loss:</b> These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.</li> <li>• <b>Electrical Delay:</b> One-way delay between the SMA connector and the antenna feed point. No uncertainty required.</li> <li>• <b>SAR measured:</b> SAR measured at the stated antenna input power.</li> <li>• <b>SAR normalized:</b> SAR as measured, normalized to an input power of 1 W at the antenna connector.</li> <li>• <b>SAR for nominal TSL parameters:</b> The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <div style="border: 1px solid black; padding: 5px; font-size: 8px; margin-top: 10px;">             The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.         </div> <p style="font-size: 8px; margin-top: 10px;">             Certificate No: Z22-60184      Page 2 of 6         </p>												
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																										
Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21X08326)	Sep-22																																																										
Power sensor NRP8S	104291	24-Sep-21 (CTTL No. J21X08326)	Sep-22																																																										
Reference Probe EX3DV4	SN 7464	26-Jan-22 (SPEAG No. EX3-7464_Jan22)	Jan-23																																																										
DAE4	SN 1566	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23																																																										
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																										
Signal Generator E4438C	M146071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23																																																										
Network Analyzer E5071C	M146110673	14-Jan-22 (CTTL No. J22X00409)	Jan-23																																																										
Calibrated by:	Name	Function	Signature																																																										
	Zhao Jing	SAR Test Engineer																																																											
Reviewed by:	Lin Hao	SAR Test Engineer																																																											
Approved by:	Qi Diqiyuan	SAR Project Leader																																																											
<div style="display: flex; justify-content: space-between; align-items: center;"> </div> <p style="font-size: 8px; margin-top: 5px;">             Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China              Tel: +86-10-42396633-2117              E-mail: cti@china.com.cn http://www.caict.ac.cn         </p> <p style="margin-top: 10px;"> <b>Measurement Conditions</b>              DASY system configuration, as far as not given on page 1.         </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>DASY Version</th> <th>DASY52</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dk, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>900 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p style="font-size: 8px; margin-top: 5px;"> <b>Head TSL parameters</b>              The following parameters and calculations were applied.         </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>41.5</td> <td>0.07 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>42.1 ± 6 %</td> <td>0.08 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>&lt;1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p style="font-size: 8px; margin-top: 5px;"> <b>SAR result with Head TSL</b> </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>2.70 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>11.0 W/kg ± 18.8 % (k=2)</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px; margin-top: 5px;"> <thead> <tr> <th>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>1.73 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>7.09 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> <p style="font-size: 8px; margin-top: 10px;">             Certificate No: Z22-60184      Page 3 of 6         </p>	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dk, dy, dz = 5 mm		Frequency	900 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	41.5	0.07 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.08 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition		SAR measured	250 mW input power	2.70 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	11.0 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition		SAR measured	250 mW input power	1.73 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	7.09 W/kg ± 18.7 % (k=2)	<div style="display: flex; justify-content: space-between; align-items: center;"> </div> <p style="font-size: 8px; margin-top: 5px;">             Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China              Tel: +86-10-42396633-2117              E-mail: cti@china.com.cn http://www.caict.ac.cn         </p> <p style="margin-top: 10px;"> <b>Appendix (Additional assessments outside the scope of CNAS L0570)</b> </p> <p style="margin-top: 5px;"> <b>Antenna Parameters with Head TSL</b> </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <tbody> <tr> <td>Impedance, transformed to feed point</td> <td>48.10 - 8.48jΩ</td> </tr> <tr> <td>Return Loss</td> <td>-23.3 dB</td> </tr> </tbody> </table> <p style="margin-top: 5px;"> <b>General Antenna Parameters and Design</b> </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <tbody> <tr> <td>Electrical Delay (one direction)</td> <td>1.312 ns</td> </tr> </tbody> </table> <p style="font-size: 8px; margin-top: 5px;">             After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.         </p> <p style="font-size: 8px; margin-top: 5px;">             The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.         </p> <p style="margin-top: 10px;"> <b>Additional EUT Data</b> </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table> <p style="font-size: 8px; margin-top: 10px;">             Certificate No: Z22-60184      Page 4 of 6         </p>	Impedance, transformed to feed point	48.10 - 8.48jΩ	Return Loss	-23.3 dB	Electrical Delay (one direction)	1.312 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	Triple Flat Phantom 5.1C																																																												
Distance Dipole Center - TSL	15 mm	with Spacer																																																											
Zoom Scan Resolution	dk, dy, dz = 5 mm																																																												
Frequency	900 MHz ± 1 MHz																																																												
	Temperature	Permittivity	Conductivity																																																										
Nominal Head TSL parameters	22.0 °C	41.5	0.07 mho/m																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.08 mho/m ± 6 %																																																										
Head TSL temperature change during test	<1.0 °C	---	---																																																										
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	2.70 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	11.0 W/kg ± 18.8 % (k=2)																																																											
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	1.73 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	7.09 W/kg ± 18.7 % (k=2)																																																											
Impedance, transformed to feed point	48.10 - 8.48jΩ																																																												
Return Loss	-23.3 dB																																																												
Electrical Delay (one direction)	1.312 ns																																																												
Manufactured by	SPEAG																																																												

In Collaboration with  
**TTL**  
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-4230603-2117  
E-mail: cti@china.ttl.com

中国合格评定国家认可委员会  
CALIBRATION  
CNAS LIST

In Collaboration with  
**TTL**  
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-4230603-2117  
E-mail: cti@china.ttl.com

Date: 2022-06-07

**DASY5 Validation Report for Head TSL**

Test Laboratory: CTTL, Beijing, China  
DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN: 14079  
Communication System: UTD 0, CW; Frequency: 900 MHz; Duty Cycle: 1:1  
Medium parameters used: f = 900 MHz;  $\sigma = 0.98$  S/m;  $\epsilon_r = 42.05$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Right Section  
Measurement Standard: DASY5 (IEE/IEC/ANSI C63.19-2007)  
DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(9.72, 9.72) @ 900 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronic: DA44 SN1556; Calibrated: 2022-01-12
- Phantom: MFP\_V5.1C (2ddeg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52.52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7) (7x7) Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 59.81 V/m; Power Drift = -0.01 dB  
Peak SAR (extrapolated) = 4.20 W/kg  
SAR(1g) = 2.78 W/kg; SAR(10g) = 1.78 W/kg  
Smallest distance from peaks to all points 3 dB below = 16 mm  
Ratio of SAR at M2 to SAR at M1 = 65.8%  
Maximum value of SAR (measured) = 3.71 W/kg

0 dB = 3.71 W/kg = 5.69 dBW/kg

Certificate No: Z22-60184
Page 3 of 6

In Collaboration with  
**TTL**  
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-4230603-2117  
E-mail: cti@china.ttl.com

中国合格评定国家认可委员会  
CALIBRATION  
CNAS LIST

In Collaboration with  
**TTL**  
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-4230603-2117  
E-mail: cti@china.ttl.com

Date: 2022-06-07

**Impedance Measurement Plot for Head TSL**

0 dB = 3.71 W/kg = 5.69 dBW/kg

Certificate No: Z22-60184
Page 6 of 6

## 1.4 D1800V2 - SN 2d170

In Collaboration with  
**TTL**  
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-4230603-2117  
E-mail: cti@china.ttl.com

中国合格评定国家认可委员会  
CALIBRATION  
CNAS LIST

In Collaboration with  
**TTL**  
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-4230603-2079  
E-mail: cti@china.ttl.com

Certificate No: Z22-60105

Client: **SGS-CN**

**CALIBRATION CERTIFICATE**

Object: D1800V2 - SN: 2d170

Calibration Procedure(s): FF-Z11-003-01  
Calibration Procedures for dipole validation kits

Calibration date: March 31, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP5	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY46110973	14-Jan-22 (CTTL No.J22X00406)	Jan-23

Calibrated by: Zhao Jing, SAR Test Engineer, Signature: [Signature]

Reviewed by: Lin Hao, SAR Test Engineer, Signature: [Signature]

Approved by: Qi Diqian, SAR Project Leader, Signature: [Signature]

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60105
Page 1 of 6

In Collaboration with  
**TTL**  
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-4230603-2079  
E-mail: cti@china.ttl.com

中国合格评定国家认可委员会  
CALIBRATION  
CNAS LIST

In Collaboration with  
**TTL**  
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-4230603-2117  
E-mail: cti@china.ttl.com

Certificate No: Z22-60105

Glossary:

TSL: tissue simulating liquid  
ConvF: sensitivity in TSL / NORMx,y,z  
N/A: not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 855684, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60105
Page 2 of 6

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504  
 E-mail: cti@chinaeui.com http://www.chinaeui.com

**Measurement Conditions**  
 DASYS system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1800 MHz ± 1 MHz	

**Head TSL parameters**  
 The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mholm
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.8 ± 8 %	1.41 mholm ± 8 %
Head TSL temperature change during test	<1.0 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.73 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	38.9 W/kg ± 18.8 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.11 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	20.4 W/kg ± 18.7 % (k=2)

Certificate No: Z22-60105 Page 3 of 6

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504  
 E-mail: cti@chinaeui.com http://www.chinaeui.com

**Appendix (Additional assessments outside the scope of CNAS L0570)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	47.90-2.54jΩ
Return Loss	-29.4dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.116 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z22-60105 Page 4 of 6

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504  
 E-mail: cti@chinaeui.com http://www.chinaeui.com

**DASY5 Validation Report for Head TSL** Date: 2022-03-31  
 Test Laboratory: CTTL, Beijing, China  
 DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d170  
 Communication System: UID 0, CW; Frequency: 1800 MHz; Duty Cycle: 1:1  
 Medium parameters used: f = 1800 MHz; σ = 1.411 S/m; ε = 40.62; ρ = 1000 kg/m<sup>3</sup>  
 Phantom section: Right Section  
 Measurement Standard: DASY5 (IEEE/ANSI C63.19-2007)  
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(8.34, 8.34) @ 1800 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration/Zoom Scan (7x7x7) (Cube 0):** Measurement grid: dx=5mm, dy=5mm, dz=5mm  
 Reference Value = 98.14 V/m; Power Drift = 0.03 dB  
 Peak SAR (extrapolated) = 18.2 W/kg  
 SAR(1 g) = 9.73 W/kg; SAR(10 g) = 5.11 W/kg  
 Smallest distance from peaks to all points 3 dB below = 10 mm  
 Ratio of SAR at M2 to SAR at M1 = 54%  
 Maximum value of SAR (measured) = 15.2 W/kg

Certificate No: Z22-60105 Page 5 of 6

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504  
 E-mail: cti@chinaeui.com http://www.chinaeui.com

**Impedance Measurement Plot for Head TSL**

Certificate No: Z22-60105 Page 6 of 6

## 1.5 D1900V2 - SN 5d136

<div style="display: flex; justify-content: space-between; align-items: center;"> </div> <p style="font-size: small;">In Collaboration with <b>TTL Calibration Laboratory</b> S P E A G Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: vt@ttslab.com http://www.caict.ac.cn</p> <p style="text-align: center;">Client: <b>SGS-CN</b> Certificate No: <b>Z22-60185</b></p> <div style="border: 1px solid black; padding: 5px;"> <p><b>CALIBRATION CERTIFICATE</b></p> <p>Object: D1900V2 - SN: 5d136</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: June 7, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility; environment temperature (23±)°C and humidity&lt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1" style="width: 100%; font-size: x-small;"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP6S</td> <td>104291</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EXSDV4</td> <td>SN 7464</td> <td>28-Jan-22 (SPEAG No. EX3-7464_Jan22)</td> <td>Jan-23</td> </tr> <tr> <td>DAE4</td> <td>SN 1656</td> <td>12-Jan-22 (CTTL-SPEAG No. Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1" style="width: 100%; font-size: x-small;"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4438C</td> <td>MY48071430</td> <td>13-Jan-22 (CTTL No. J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyser ES071C</td> <td>MY48110673</td> <td>14-Jan-22 (CTTL No. J22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table> <div style="display: flex; justify-content: space-between; font-size: x-small;"> <div> <p>Calibrated by: Zhao Jing SAR Test Engineer</p> <p>Reviewed by: Lin Hao SAR Test Engineer</p> <p>Approved by: Qi Dianyuan SAR Project Leader</p> </div> <div style="text-align: right;"> <p>Signature</p> <p>Issued: June 13, 2022</p> </div> </div> <p style="font-size: x-small;">This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> </div>	Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21X08326)	Sep-22	Power sensor NRP6S	104291	24-Sep-21 (CTTL No. J21X08326)	Sep-22	Reference Probe EXSDV4	SN 7464	28-Jan-22 (SPEAG No. EX3-7464_Jan22)	Jan-23	DAE4	SN 1656	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23	Network Analyser ES071C	MY48110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23	<div style="display: flex; justify-content: space-between; align-items: center;"> </div> <p style="font-size: small;">In Collaboration with <b>TTL Calibration Laboratory</b> S P E A G Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: vt@ttslab.com http://www.caict.ac.cn</p> <p><b>Glossary:</b></p> <p>TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORMx.y.z NA: not applicable or not measured</p> <p><b>Calibration is Performed According to the Following Standards:</b></p> <p>a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1526: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865984, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p><b>Additional Documentation:</b> c) DASY4/S System Handbook</p> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li>• <b>Measurement Conditions:</b> Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.</li> <li>• <b>Antenna Parameters with TSL:</b> The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.</li> <li>• <b>Feed Point Impedance and Return Loss:</b> These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.</li> <li>• <b>Electrical Delay:</b> One-way delay between the SMA connector and the antenna feed point. No uncertainty required.</li> <li>• <b>SAR measured:</b> SAR measured at the stated antenna input power.</li> <li>• <b>SAR normalized:</b> SAR as measured, normalized to an input power of 1 W at the antenna connector.</li> <li>• <b>SAR for nominal TSL parameters:</b> The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <div style="border: 1px solid black; padding: 5px; font-size: x-small;"> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> </div>																												
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																										
Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21X08326)	Sep-22																																																										
Power sensor NRP6S	104291	24-Sep-21 (CTTL No. J21X08326)	Sep-22																																																										
Reference Probe EXSDV4	SN 7464	28-Jan-22 (SPEAG No. EX3-7464_Jan22)	Jan-23																																																										
DAE4	SN 1656	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23																																																										
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																										
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23																																																										
Network Analyser ES071C	MY48110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23																																																										
<div style="display: flex; justify-content: space-between; align-items: center;"> </div> <p style="font-size: small;">In Collaboration with <b>TTL Calibration Laboratory</b> S P E A G Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: vt@ttslab.com http://www.caict.ac.cn</p> <p><b>Measurement Conditions</b> DASY system configuration, as far as not given on page 1.</p> <table border="1" style="width: 100%; font-size: x-small;"> <thead> <tr> <th>DASY Version</th> <th>DASY52</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 6 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>1900 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p><b>Head TSL parameters</b> The following parameters and calculations were applied:</p> <table border="1" style="width: 100%; font-size: x-small;"> <thead> <tr> <th>Nominal Head TSL parameters</th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td></td> <td>22.0 °C</td> <td>40.0</td> <td>1.40 mS/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.9 ± 6 %</td> <td>1.39 mS/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>&lt;1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p><b>SAR result with Head TSL</b></p> <table border="1" style="width: 100%; font-size: x-small;"> <thead> <tr> <th>SAR averaged over 1 cm² (1 g) of Head TSL</th> <th>Condition</th> <th>9.55 W/kg</th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td></td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>40.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <th>SAR averaged over 10 cm² (10 g) of Head TSL</th> <th>Condition</th> <th>5.18 W/kg</th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td></td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>20.8 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table>	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 6 mm		Frequency	1900 MHz ± 1 MHz		Nominal Head TSL parameters	Temperature	Permittivity	Conductivity		22.0 °C	40.0	1.40 mS/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	39.9 ± 6 %	1.39 mS/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---	SAR averaged over 1 cm² (1 g) of Head TSL	Condition	9.55 W/kg	SAR measured	250 mW input power		SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm² (10 g) of Head TSL	Condition	5.18 W/kg	SAR measured	250 mW input power		SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 18.7 % (k=2)	<div style="display: flex; justify-content: space-between; align-items: center;"> </div> <p style="font-size: small;">In Collaboration with <b>TTL Calibration Laboratory</b> S P E A G Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: vt@ttslab.com http://www.caict.ac.cn</p> <p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1" style="width: 100%; font-size: x-small;"> <tbody> <tr> <td>Impedance, transformed to feed point</td> <td>51.2Ω ± 7.5Ω(j)</td> </tr> <tr> <td>Return Loss</td> <td>-22.4dB</td> </tr> </tbody> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1" style="width: 100%; font-size: x-small;"> <tbody> <tr> <td>Electrical Delay (one direction)</td> <td>1.109 ns</td> </tr> </tbody> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1" style="width: 100%; font-size: x-small;"> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table>	Impedance, transformed to feed point	51.2Ω ± 7.5Ω(j)	Return Loss	-22.4dB	Electrical Delay (one direction)	1.109 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	Triple Flat Phantom 5.1C																																																												
Distance Dipole Center - TSL	10 mm	with Spacer																																																											
Zoom Scan Resolution	dx, dy, dz = 6 mm																																																												
Frequency	1900 MHz ± 1 MHz																																																												
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity																																																										
	22.0 °C	40.0	1.40 mS/m																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.9 ± 6 %	1.39 mS/m ± 6 %																																																										
Head TSL temperature change during test	<1.0 °C	---	---																																																										
SAR averaged over 1 cm² (1 g) of Head TSL	Condition	9.55 W/kg																																																											
SAR measured	250 mW input power																																																												
SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 18.8 % (k=2)																																																											
SAR averaged over 10 cm² (10 g) of Head TSL	Condition	5.18 W/kg																																																											
SAR measured	250 mW input power																																																												
SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 18.7 % (k=2)																																																											
Impedance, transformed to feed point	51.2Ω ± 7.5Ω(j)																																																												
Return Loss	-22.4dB																																																												
Electrical Delay (one direction)	1.109 ns																																																												
Manufactured by	SPEAG																																																												



In Collaboration with **TTL Speag** Calibration Laboratory and **CAICT**

Address: No.52 HuaYuanBei Road, HaiDian District, Beijing, 100191, China  
Tel: +86-10-62066317 E-mail: cti@tstmail.com http://www.caict.ac.cn

Date: 2022-06-07

**DASY5 Validation Report for Head TSL**  
Test Laboratory: CTTL, Beijing, China  
DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 54136  
Communication System: UTD 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1  
Medium parameters used:  $f = 1900 \text{ MHz}$ ;  $\sigma = 1.385 \text{ S/m}$ ;  $\epsilon_r = 39.85$ ;  $\rho = 1000 \text{ kg/m}^3$   
Phantom section: Right Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)  
DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(8, 8, 18, 8, 18) @ 1900 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP\_V5\_IC (20kg probe kit); Type: QD 000 P51 Cx; Serial: 1062
- DASY52.52.10.4(1555); SEMCAD X.14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube D: Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 99.99 V/m; Power Drift = 0.04 dB  
Peak SAR (extrapolated) = 18.6 W/kg  
SAR(1g) = 9.95 W/kg; SAR(10g) = 5.18 W/kg  
Smallest distance from peaks to all points 3 dB below = 9.2 mm  
Ratio of SAR at M2 to SAR at M1 = 54.1%

Maximum value of SAR (measured) = 15.6 W/kg

0 dB = 15.6 W/kg = 11.93 dBW/kg

Certificate No: Z22-60185 Page 5 of 6

In Collaboration with **TTL Speag** Calibration Laboratory and **CAICT**

Address: No.52 HuaYuanBei Road, HaiDian District, Beijing, 100191, China  
Tel: +86-10-62066317 E-mail: cti@tstmail.com http://www.caict.ac.cn

**Impedance Measurement Plot for Head TSL**

Certificate No: Z22-60185 Page 6 of 6

### 1.6 D2000V2 - SN 1041

In Collaboration with **TTL Speag** Calibration Laboratory, **CNAN** (China National Accreditation Administration), and **CAICT**

Address: No.52 HuaYuanBei Road, HaiDian District, Beijing, 100191, China  
Tel: +86-10-62066317 E-mail: cti@tstmail.com http://www.caict.ac.cn

Client: **SGS-CN** Certificate No: **Z22-60188**

**CALIBRATION CERTIFICATE**

Object: D2000V2 - SN: 1041

Calibration Procedure(s): FF-Z11-003-01  
Calibration Procedures for dipole validation kits

Calibration date: June 8, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (8). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22±3)°C and humidity < 70%.

Calibration Equipment used (M&E critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP	106277	24-Sep-21 (CTTL No.J21X06326)	Sep-22
Power sensor KRPS	104291	24-Sep-21 (CTTL No.J21X06326)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG.No EX3-7464-Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Dianyuan SAR Project Leader

Issued: June 13, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60188 Page 1 of 6

In Collaboration with **TTL Speag** Calibration Laboratory and **CAICT**

Address: No.52 HuaYuanBei Road, HaiDian District, Beijing, 100191, China  
Tel: +86-10-62066317 E-mail: cti@tstmail.com http://www.caict.ac.cn

**Glossary:**

TSL: Issue simulating liquid  
ConvF: sensitivity in TSL, INORMx,y,z  
N/A: not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 865964, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60188 Page 2 of 6

In Collaboration with **TTL S p e a g** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-42396633-2117  
 E-mail: ott@china.ttl.com http://www.caict.ac.cn

**Measurement Conditions**  
 DASYS system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2000 MHz ± 1 MHz	

**Head TSL parameters**  
 The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	1.39 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.4 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>41.8 W/kg ± 18.8 % (k=2)</b>
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>21.3 W/kg ± 18.7 % (k=2)</b>

Certificate No: Z22-60186 Page 3 of 6

In Collaboration with **TTL S p e a g** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-42396633-2117  
 E-mail: ott@china.ttl.com http://www.caict.ac.cn

**Appendix (Additional assessments outside the scope of CNAS L0570)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	48.4Ω ± 0.74jΩ
Return Loss	-34.9dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.088 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z22-60186 Page 4 of 6

In Collaboration with **TTL S p e a g** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-42396633-2117  
 E-mail: ott@china.ttl.com http://www.caict.ac.cn

**DASY5 Validation Report for Head TSL** Date: 2022-06-06

Test Laboratory: CTTL, Beijing, China  
 DUT: Dipole 2000 MHz; Type: D2000V2; Serial: D2000V2 - SN: 1041  
 Communication System: LIID 0; CW; Frequency: 2000 MHz; Duty Cycle: 1:1  
 Medium parameters used:  $f = 2000$  MHz;  $\sigma = 1.392$  S/m;  $\epsilon_r = 40.21$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Phantom section: Right Section  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)  
 DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(R,2, 8.2, 8.2) @ 2000 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA64 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52: S2.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm**  
 Reference Value = 103.4 V/m; Power Drift = 0.03 dB  
 Peak SAR (extrapolated) = 19.6 W/kg  
 SAR(1 g) = 10.4 W/kg; SAR(10 g) = 5.3 W/kg  
 Smallest distance from peaks to all points 3 dB below = 9.1 mm  
 Ratio of SAR at M2 to SAR at M1 = 53.6%  
 Maximum value of SAR (measured) = 16.3 W/kg

Certificate No: Z22-60186 Page 5 of 6

In Collaboration with **TTL S p e a g** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-42396633-2117  
 E-mail: ott@china.ttl.com http://www.caict.ac.cn

**Impedance Measurement Plot for Head TSL**

Certificate No: Z22-60186 Page 6 of 6

## 1.7 D2300V2 - SN 1096

<p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p>		<p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p>																			
<p>Client: <b>SGS-CN</b> Certificate No: <b>Z22-60106</b></p>																					
<p><b>CALIBRATION CERTIFICATE</b></p>																					
Object	D2300V2 - SN 1096																				
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits																				
Calibration date:	March 31, 2022																				
<p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity &lt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p>																					
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																		
Power Meter NRP2	108277	24-Sep-21 (CTTL No.J21X08326)	Sep-22																		
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																		
Reference Probe EX3DV4 DAE4	SN 7307 SN 1556	26-May-21 (SPEAG No.EK3-7307_May21) 12-Jan-22 (CTTL-SPEAG No.Z22-60007)	May-22 Jan-23																		
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																		
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23																		
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23																		
Calibrated by:	Name	Function	Signature																		
	Zhao Jing	SAR Test Engineer																			
Reviewed by:	Lin Hao	SAR Test Engineer																			
Approved by:	Qi Diaryuan	SAR Project Leader																			
<p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p>																					
Certificate No: Z22-60106		Page 1 of 6																			
<p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p>		<p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p>																			
<p><b>Measurement Conditions</b> DASY system configuration, as far as not given on page 1</p> <table border="1"> <tr> <td>DASY Version</td> <td>DASY2</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2300 MHz ± 1 MHz</td> <td></td> </tr> </table>				DASY Version	DASY2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2300 MHz ± 1 MHz	
DASY Version	DASY2	52.10.4																			
Extrapolation	Advanced Extrapolation																				
Phantom	Triple Flat Phantom 5.1C																				
Distance Dipole Center - TSL	10 mm	with Spacer																			
Zoom Scan Resolution	dx, dy, dz = 5 mm																				
Frequency	2300 MHz ± 1 MHz																				
<p><b>Head TSL parameters</b> The following parameters and calculations were applied:</p> <table border="1"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.5</td> <td>1.67 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.8 ± 6 %</td> <td>1.70 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>&lt;1.0 °C</td> <td>—</td> <td>—</td> </tr> </tbody> </table>					Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.70 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—		
	Temperature	Permittivity	Conductivity																		
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m																		
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.70 mho/m ± 6 %																		
Head TSL temperature change during test	<1.0 °C	—	—																		
<p><b>SAR result with Head TSL</b></p> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm<sup>3</sup> (1g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>12.4 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>49.2 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <th>SAR averaged over 10 cm<sup>3</sup> (10g) of Head TSL</th> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>5.88 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>23.4 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table>				SAR averaged over 1 cm <sup>3</sup> (1g) of Head TSL	Condition		SAR measured	250 mW input power	12.4 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	49.2 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm <sup>3</sup> (10g) of Head TSL	Condition		SAR measured	250 mW input power	5.88 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)
SAR averaged over 1 cm <sup>3</sup> (1g) of Head TSL	Condition																				
SAR measured	250 mW input power	12.4 W/kg																			
SAR for nominal Head TSL parameters	normalized to 1W	49.2 W/kg ± 18.8 % (k=2)																			
SAR averaged over 10 cm <sup>3</sup> (10g) of Head TSL	Condition																				
SAR measured	250 mW input power	5.88 W/kg																			
SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)																			
<p><b>Glossary:</b></p> <p>TSL: Issue simulating liquid ConvF: sensitivity in TSL / NORMx,y,z N/A: not applicable or not measured</p> <p><b>Calibration is Performed According to the Following Standards:</b></p> <p>a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p><b>Additional Documentation:</b> c) DASY4/5 System Handbook</p> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li>Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.</li> <li>Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.</li> <li>Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.</li> <li>Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.</li> <li>SAR measured: SAR measured at the stated antenna input power.</li> <li>SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.</li> <li>SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.</p>																					
Certificate No: Z22-60106		Page 2 of 6																			
<p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p>		<p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p>																			
<p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>49.2Ω - 4.56jΩ</td> </tr> <tr> <td>Return Loss</td> <td>-26.6dB</td> </tr> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>1.083 ns</td> </tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table>				Impedance, transformed to feed point	49.2Ω - 4.56jΩ	Return Loss	-26.6dB	Electrical Delay (one direction)	1.083 ns	Manufactured by	SPEAG										
Impedance, transformed to feed point	49.2Ω - 4.56jΩ																				
Return Loss	-26.6dB																				
Electrical Delay (one direction)	1.083 ns																				
Manufactured by	SPEAG																				
Certificate No: Z22-60106		Page 4 of 6																			

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
 E-mail: cti@china.ttl.com http://www.china.ttl.com

**DASY5 Validation Report for Head TSL** Date: 2022-03-31

Test Laboratory: CTTL, Beijing, China  
 DUT: Dipole 2300 MHz; Type: D2300V2; Serial: D2300V2 - SN: 1096  
 Communication System: UTD 0, CW; Frequency: 2300 MHz; Duty Cycle: 1:1  
 Medium parameters used:  $f = 2300$  MHz;  $\sigma = 1.702$  S/m;  $\epsilon = 39.77$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Phantom section: Right Section  
 Measurement Standard: DASY5 (IEEE/EC/ANSI C63.19-2007)  
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(8.01, 8.01, 8.01) @ 2300 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sst1556; Calibrated: 2022-01-12
- Phantom: MFP V5.1C (2ldag probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 S2.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm**  
 Reference Value = 102.7 V/m; Power Drift = 0.00 dB  
 Peak SAR (extrapolated) = 24.8 W/kg  
 SAR(1 g) = 12.4 W/kg; SAR(10 g) = 5.88 W/kg  
 Smallest distance from peaks to all points 3 dB below = 9 mm  
 Ratio of SAR at M2 to SAR at M1 = 50.4%  
 Maximum value of SAR (measured) = 20.3 W/kg

Certificate No: Z22-60106 Page 1 of 6

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
 E-mail: cti@china.ttl.com http://www.china.ttl.com

**Impedance Measurement Plot for Head TSL**

Certificate No: Z22-60106 Page 4 of 6

1.8 D2450V2 - SN 817

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY, **CNAS** 中国认可 国家互认 校准 CALIBRATION CNAS 10578, and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
 E-mail: cti@china.ttl.com http://www.china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60107**

**CALIBRATION CERTIFICATE**

Object: D2450V2 - SN: 817  
 Calibration Procedure(s): FF-Z11-003-01  
 Calibration Procedures for dipole validation kits  
 Calibration date: April 1, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter	NRP2	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Power sensor	NRP8S	104291 24-Sep-21 (CTTL No.J21X08320)	Sep-22
Reference Probe	EX3DV4	SN 7307 26-May-21(SPEAG.No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator	E4438C	MY49071430 13-Jan-22 (CTTL No. J22X00406)	Jan-23
Network Analyzer	E5071C	MY46110873 14-Jan-22 (CTTL No. J22X00406)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer  
 Reviewed by: Lin Hao SAR Test Engineer  
 Approved by: Qi Dianyuan SAR Project Leader

Signature: [Signatures]  
 Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60107 Page 1 of 6

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
 E-mail: cti@china.ttl.com http://www.china.ttl.com

**Glossary:**

TSL tissue simulating liquid  
 ConvF sensitivity in TSL / NORMx.yz  
 N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 855664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**







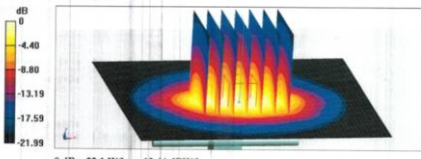



- DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60107 Page 2 of 6
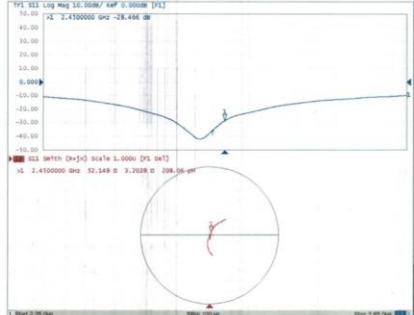
<div style="display: flex; justify-content: space-between;">   </div> <p style="font-size: small;">             In Collaboration with              TTT Speag CALIBRATION LABORATORY              Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China              Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504              E-mail: cti@china.ttl.com http://www.china.ttl.com         </p> <p><b>Measurement Conditions</b>          DASYS system configuration, as far as not given on page 1</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>DASY Version</td> <td>DASY52</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2450 MHz ± 1 MHz</td> <td></td> </tr> </table> <p><b>Head TSL parameters</b>          The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.2</td> <td>1.80 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.5 ± 6 %</td> <td>1.79 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>&lt;+1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p><b>SAR result with Head TSL</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>13.2 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>53.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>6.15 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>24.7 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> <p style="font-size: x-small;">Certificate No: Z22-60107 Page 3 of 6</p>	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2450 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.79 mho/m ± 6 %	Head TSL temperature change during test	<+1.0 °C	---	---	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition		SAR measured	250 mW input power	13.2 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	53.0 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition		SAR measured	250 mW input power	6.15 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 18.7 % (k=2)	<div style="display: flex; justify-content: space-between;">   </div> <p style="font-size: small;">             In Collaboration with              TTT Speag CALIBRATION LABORATORY              Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China              Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504              E-mail: cti@china.ttl.com http://www.china.ttl.com         </p> <p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Impedance, transformed to feed point</td> <td>52.10 ± 3.20Ω</td> </tr> <tr> <td>Return Loss</td> <td>-28.5dB</td> </tr> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Electrical Delay (one direction)</td> <td>1.066 ns</td> </tr> </table> <p style="font-size: x-small;">             After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.              The dipole is made of standard serringrid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.         </p> <p><b>Additional EUT Data</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table> <p style="font-size: x-small;">Certificate No: Z22-60107 Page 4 of 6</p>	Impedance, transformed to feed point	52.10 ± 3.20Ω	Return Loss	-28.5dB	Electrical Delay (one direction)	1.066 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	Triple Flat Phantom 5.1C																																																												
Distance Dipole Center - TSL	10 mm	with Spacer																																																											
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																												
Frequency	2450 MHz ± 1 MHz																																																												
	Temperature	Permittivity	Conductivity																																																										
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.79 mho/m ± 6 %																																																										
Head TSL temperature change during test	<+1.0 °C	---	---																																																										
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	13.2 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	53.0 W/kg ± 18.8 % (k=2)																																																											
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	6.15 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 18.7 % (k=2)																																																											
Impedance, transformed to feed point	52.10 ± 3.20Ω																																																												
Return Loss	-28.5dB																																																												
Electrical Delay (one direction)	1.066 ns																																																												
Manufactured by	SPEAG																																																												
<div style="display: flex; justify-content: space-between;">   </div> <p style="font-size: small;">             In Collaboration with              TTT Speag CALIBRATION LABORATORY              Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China              Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504              E-mail: cti@china.ttl.com http://www.china.ttl.com         </p> <p><b>DASY5 Validation Report for Head TSL</b> <span style="float: right;">Date: 2022-04-01</span></p> <p>Test Laboratory: CTTL, Beijing, China          DUT: Dipole 2450 MHz; Type: D2450V2 - SN: 817          Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1          Medium parameters used: f = 2450 MHz; σ = 1.79 S/m; ε = 39.52; ρ = 1000 kg/m<sup>3</sup>          Phantom section: Right Section          Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)          DASY5 Configuration:</p> <ul style="list-style-type: none"> <li>Probe: EX3DV4 - SN7307; ConvF(7.75, 7.75, 7.75) @ 2450 MHz; Calibrated: 2021-05-26</li> <li>Sensor-Surface: 1.4mm (Mechanical Surface Detection)</li> <li>Electronics: DA14 Sn1556; Calibrated: 2022-01-12</li> <li>Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062</li> <li>DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)</li> </ul> <p><b>Dipole Calibration</b> Zoom Scan (7x7x7) (7x7x7)/Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm          Reference Value = 104.6 V/m; Power Drift = -0.03 dB          Peak SAR (extrapolated) = 27.0 W/kg  <b>SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.15 W/kg</b>          Smallest distance from peaks to all points 3 dB below = 8.9 mm          Ratio of SAR at M2 to SAR at M1 = -49.2%          Maximum value of SAR (measured) = 22.1 W/kg</p>  <p style="font-size: x-small;">Certificate No: Z22-60107 Page 1 of 6</p>	<div style="display: flex; justify-content: space-between;">   </div> <p style="font-size: small;">             In Collaboration with              TTT Speag CALIBRATION LABORATORY              Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China              Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504              E-mail: cti@china.ttl.com http://www.china.ttl.com         </p> <p><b>Impedance Measurement Plot for Head TSL</b></p>  <p style="font-size: x-small;">Certificate No: Z22-60107 Page 6 of 6</p>																																																												

## 1.9 D2600V2 - SN 1158

<div style="text-align: center;"> </div> <p style="font-size: small;">             Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China              Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504              E-mail: cti@china.ttl.com.cn http://www.chinatitl.cn         </p> <p>             Client: <b>SGS-CN</b> Certificate No: <b>Z22-60108</b> </p> <h3 style="text-align: center;">CALIBRATION CERTIFICATE</h3> <p>             Object: <b>D2600V2 - SN: 1158</b> </p> <p>             Calibration Procedure(s): <b>FF-Z11-003-01</b>              Calibration Procedures for dipole validation kits         </p> <p>             Calibration date: <b>March 31, 2022</b> </p> <p>             This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.         </p> <p>             All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity&lt;70%.         </p> <p>             Calibration Equipment used (M&amp;TE critical for calibration)         </p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>102577</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21(SPEAG.No.EX3-7307_May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22(CTTL-SPEAG.No.Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4438C</td> <td>MY49071430</td> <td>13-Jan-22 (CTTL No.J22X00406)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY49110673</td> <td>14-Jan-22 (CTTL No.J22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table> <p>             Calibrated by: <b>Zhao Jing</b> SAR Test Engineer  </p> <p>             Reviewed by: <b>Lin Hao</b> SAR Test Engineer  </p> <p>             Approved by: <b>Qi Diaryuan</b> SAR Project Leader  </p> <p style="text-align: right;">             Issued: April 6, 2022         </p> <p style="font-size: x-small;">             This calibration certificate shall not be reproduced except in full without written approval of the laboratory.         </p> <p style="font-size: x-small;">             Certificate No: Z22-60108 Page 1 of 6         </p>	Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	102577	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23	Network Analyzer E5071C	MY49110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23	<div style="text-align: center;"> </div> <p style="font-size: small;">             Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China              Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504              E-mail: cti@china.ttl.com.cn http://www.chinatitl.cn         </p> <p>             Glossary:              TSL: tissue simulating liquid              ConvF: sensitivity in TSL / NORMx.y.z              N/A: not applicable or not measured         </p> <p> <b>Calibration is Performed According to the Following Standards:</b>              a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020              b) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"         </p> <p> <b>Additional Documentation:</b>              c) DASY4/5 System Handbook         </p> <p> <b>Methods Applied and Interpretation of Parameters:</b> </p> <ul style="list-style-type: none"> <li>Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.</li> <li>Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.</li> <li>Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.</li> <li>Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.</li> <li>SAR measured: SAR measured at the stated antenna input power.</li> <li>SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.</li> <li>SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <div style="border: 1px solid black; padding: 5px; margin-top: 10px;"> <p style="font-size: x-small;">                     The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.                 </p> </div> <p style="font-size: x-small;">             Certificate No: Z22-60108 Page 2 of 6         </p>																												
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																										
Power Meter NRP2	102577	24-Sep-21 (CTTL No.J21X08326)	Sep-22																																																										
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																																																										
Reference Probe EX3DV4	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22																																																										
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23																																																										
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																																										
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23																																																										
Network Analyzer E5071C	MY49110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23																																																										
<div style="text-align: center;"> </div> <p style="font-size: small;">             Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China              Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504              E-mail: cti@china.ttl.com.cn http://www.chinatitl.cn         </p> <p> <b>Measurement Conditions</b>              DASY system configuration, as far as not given on page 1.         </p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tbody> <tr> <td>DASY Version</td> <td>DASY52</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2600 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p> <b>Head TSL parameters</b>              The following parameters and calculations were applied.         </p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.0</td> <td>1.96 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>38.7 ± 6 %</td> <td>1.96 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>&lt;1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p> <b>SAR result with Head TSL</b> </p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>SAR averaged over 1 cm<sup>2</sup> (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>13.7 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>54.8 W/kg ± 18.8 % (k=2)</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>SAR averaged over 10 cm<sup>2</sup> (10 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>6.12 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>24.6 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> <p style="font-size: x-small;">             Certificate No: Z22-60108 Page 3 of 6         </p>	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2600 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 6 %	1.96 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---	SAR averaged over 1 cm <sup>2</sup> (1 g) of Head TSL	Condition		SAR measured	250 mW input power	13.7 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm <sup>2</sup> (10 g) of Head TSL	Condition		SAR measured	250 mW input power	6.12 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	24.6 W/kg ± 18.7 % (k=2)	<div style="text-align: center;"> </div> <p style="font-size: small;">             Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China              Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504              E-mail: cti@china.ttl.com.cn http://www.chinatitl.cn         </p> <p> <b>Appendix (Additional assessments outside the scope of CNAS L0570)</b>  <b>Antenna Parameters with Head TSL</b> </p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tbody> <tr> <td>Impedance, transformed to feed point</td> <td>49.90- 6.49jΩ</td> </tr> <tr> <td>Return Loss</td> <td>- 23.8dB</td> </tr> </tbody> </table> <p> <b>General Antenna Parameters and Design</b> </p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tbody> <tr> <td>Electrical Delay (one direction)</td> <td>1.053 ns</td> </tr> </tbody> </table> <p>             After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.         </p> <p>             The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.         </p> <p> <b>Additional EUT Data</b> </p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table> <p style="font-size: x-small;">             Certificate No: Z22-60108 Page 4 of 6         </p>	Impedance, transformed to feed point	49.90- 6.49jΩ	Return Loss	- 23.8dB	Electrical Delay (one direction)	1.053 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	Triple Flat Phantom 5.1C																																																												
Distance Dipole Center - TSL	10 mm	with Spacer																																																											
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																												
Frequency	2600 MHz ± 1 MHz																																																												
	Temperature	Permittivity	Conductivity																																																										
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 6 %	1.96 mho/m ± 6 %																																																										
Head TSL temperature change during test	<1.0 °C	---	---																																																										
SAR averaged over 1 cm <sup>2</sup> (1 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	13.7 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)																																																											
SAR averaged over 10 cm <sup>2</sup> (10 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	6.12 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	24.6 W/kg ± 18.7 % (k=2)																																																											
Impedance, transformed to feed point	49.90- 6.49jΩ																																																												
Return Loss	- 23.8dB																																																												
Electrical Delay (one direction)	1.053 ns																																																												
Manufactured by	SPEAG																																																												

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
 E-mail: cti@china.ttl.com http://www.china.ttl.com

Date: 2022-03-31

**DASY5 Validation Report for Head TSL**  
 Test Laboratory: CTTL, Beijing, China  
 DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1158  
 Communication System: UID 0, CW; Frequency: 2600 MHz; Duty Cycle: 1:1  
 Medium parameters used:  $f = 2600 \text{ MHz}$ ;  $\sigma = 1.955 \text{ S/m}$ ;  $\epsilon_r = 38.68$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Right Section  
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)  
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(7.5, 7.5, 7.5) @ 2600 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP\_V5.1C (2dkg probe fill); Type: QD 000 P51 Cx; Serial: 1062
- DASY5 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm**  
 Reference Value = 103.3 V/m; Power Drift = 0.04 dB  
 Peak SAR (extrapolated) = 29.0 W/kg  
 SAR(1 g) = 13.7 W/kg; SAR(10 g) = 6.12 W/kg  
 Smallest distance from peaks to all points 3 dB below = 8.9 mm  
 Ratio of SAR at M2 to SAR at M1 = 47.5%  
 Maximum value of SAR (measured) = 23.4 W/kg

0 dB = 23.4 W/kg = 13.69 dBW/kg

Certificate No: Z22-60108 Page 5 of 6

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
 E-mail: cti@china.ttl.com http://www.china.ttl.com

**Impedance Measurement Plot for Head TSL**

Certificate No: Z22-60108 Page 6 of 6

## 1.10 D5GHZV2 - SN 1095

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
 E-mail: cti@china.ttl.com http://www.china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60187**

**CALIBRATION CERTIFICATE**

Object: D5GHZV2 - SN: 1095

Calibration Procedure(s): FF-Z11-003-01  
 Calibration Procedures for dipole validation kits

Calibration date: June 1, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (23±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21008326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21008326)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG No EX3-7464_Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY46071430	13-Jan-22 (CTTL No. J22X00406)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23

Calibrated by: Zhao Jing, SAR Test Engineer

Reviewed by: Lin Hao, SAR Test Engineer

Approved by: Qi Dianyan, SAR Project Leader

Issued: June 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60187 Page 1 of 10

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
 E-mail: cti@china.ttl.com http://www.china.ttl.com

**Glossary:**

TSL: Issue simulating liquid  
 ConvF: sensitivity in TSL / NORMx,y,z  
 N/A: not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

c) DASY4/G System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60187 Page 2 of 10

In Collaboration with  
**TTL**  
CALIBRATION LABORATORY

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62382117  
E-mail: cti@ttsintl.com http://www.ttsintl.com

**Measurement Conditions**  
DAZY system configuration, as far as not given on page 1.

DASY Version	DAZY52	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5000 MHz ± 1 MHz 5200 MHz ± 1 MHz 5500 MHz ± 1 MHz 5800 MHz ± 1 MHz	

**Head TSL parameters at 5200MHz**  
The following parameters and calculations were applied.

Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.0	4.66 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.4 ± 6 %	4.82 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

**SAR result with Head TSL at 5200MHz**

SAR averaged over 1 cm <sup>2</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	7.79 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	17.6 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm <sup>2</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.22 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg ± 24.2 % (k=2)

Certificate No: Z22-60187 Page 3 of 10

In Collaboration with  
**TTL**  
CALIBRATION LABORATORY

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62382117  
E-mail: cti@ttsintl.com http://www.ttsintl.com

**Head TSL parameters at 5300MHz**  
The following parameters and calculations were applied.

Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

**SAR result with Head TSL at 5300MHz**

SAR averaged over 1 cm <sup>2</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.94 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	79.1 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm <sup>2</sup> (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.27 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.6 W/kg ± 24.2 % (k=2)

**Head TSL parameters at 5500MHz**  
The following parameters and calculations were applied.

Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.6	4.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	4.94 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

**SAR result with Head TSL at 5500MHz**

SAR averaged over 1 cm <sup>2</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.29 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	82.6 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm <sup>2</sup> (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.34 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.3 W/kg ± 24.2 % (k=2)

Certificate No: Z22-60187 Page 4 of 10

In Collaboration with  
**TTL**  
CALIBRATION LABORATORY

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62382117  
E-mail: cti@ttsintl.com http://www.ttsintl.com

**Head TSL parameters at 5600MHz**  
The following parameters and calculations were applied.

Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.05 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

**SAR result with Head TSL at 5600MHz**

SAR averaged over 1 cm <sup>2</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.12 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	80.8 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm <sup>2</sup> (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.9 W/kg ± 24.2 % (k=2)

**Head TSL parameters at 5800MHz**  
The following parameters and calculations were applied.

Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	5.25 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

**SAR result with Head TSL at 5800MHz**

SAR averaged over 1 cm <sup>2</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.71 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	76.7 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm <sup>2</sup> (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.16 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.8 W/kg ± 24.2 % (k=2)

Certificate No: Z22-60187 Page 5 of 10

In Collaboration with  
**TTL**  
CALIBRATION LABORATORY

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62382117  
E-mail: cti@ttsintl.com http://www.ttsintl.com

**Appendix (Additional assessments outside the scope of CNAS L0570)**

**Antenna Parameters with Head TSL at 5200MHz**

Impedance, transformed to feed point	46.1D-5.03jΩ
Return Loss	-23.6dB

**Antenna Parameters with Head TSL at 5300MHz**

Impedance, transformed to feed point	47.8D-2.42jΩ
Return Loss	-28.5dB

**Antenna Parameters with Head TSL at 5500MHz**

Impedance, transformed to feed point	50.3D-4.26jΩ
Return Loss	-27.4dB

**Antenna Parameters with Head TSL at 5600MHz**

Impedance, transformed to feed point	54.5D-4.80jΩ
Return Loss	-24.0dB

**Antenna Parameters with Head TSL at 5800MHz**

Impedance, transformed to feed point	51.5D-5.61jΩ
Return Loss	-24.9dB

Certificate No: Z22-60187 Page 6 of 10



In Collaboration with  
**T T L**  
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62920117  
E-mail: [ott@ttsnet.com](mailto:ott@ttsnet.com) <http://www.ttsnet.com>

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.101 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z22-60187 Page 7 of 10

In Collaboration with  
**T T L**  
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62920117  
E-mail: [ott@ttsnet.com](mailto:ott@ttsnet.com) <http://www.ttsnet.com>

**DASY5 Validation Report for Head TSL** Date: 2022-06-01

Test Laboratory: CTTL, Beijing, China  
DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1095

Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Frequency: 5900 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 5200$  MHz;  $\sigma = 4.62$  S/m;  $\epsilon_r = 35.38$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Medium parameters used:  $f = 5300$  MHz;  $\sigma = 4.73$  S/m;  $\epsilon_r = 35.19$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Medium parameters used:  $f = 5500$  MHz;  $\sigma = 4.939$  S/m;  $\epsilon_r = 34.83$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Medium parameters used:  $f = 5600$  MHz;  $\sigma = 5.051$  S/m;  $\epsilon_r = 34.68$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Medium parameters used:  $f = 5800$  MHz;  $\sigma = 5.247$  S/m;  $\epsilon_r = 34.42$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Right Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN7484; ConvF(5.6, 5.6, 5.6) @ 5200 MHz; ConvF(5.32, 5.32, 5.32) @ 5300 MHz; ConvF(5.11, 5.11, 5.11) @ 5500 MHz; ConvF(4.91, 4.91, 4.91) @ 5600 MHz; ConvF(5, 5, 5) @ 5800 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm**  
Reference Value = 60.80 V/m; Power Drift = -0.06 dB  
Peak SAR (extrapolated) = 29.8 W/kg  
SAR(1 g) = 7.79 W/kg; SAR(10 g) = 2.22 W/kg  
Smallest distance from peaks to all points 3 dB below = 7.2 mm  
Ratio of SAR at M2 to SAR at M1 = 66.8%  
Maximum value of SAR (measured) = 18.3 W/kg

**Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm**  
Reference Value = 61.08 V/m; Power Drift = -0.07 dB  
Peak SAR (extrapolated) = 31.5 W/kg  
SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.27 W/kg  
Smallest distance from peaks to all points 3 dB below = 7.2 mm  
Ratio of SAR at M2 to SAR at M1 = 65.5%  
Maximum value of SAR (measured) = 19.0 W/kg

Certificate No: Z22-60187 Page 8 of 10

In Collaboration with  
**T T L**  
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62920117  
E-mail: [ott@ttsnet.com](mailto:ott@ttsnet.com) <http://www.ttsnet.com>

**Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm**  
Reference Value = 61.92 V/m; Power Drift = -0.08 dB  
Peak SAR (extrapolated) = 34.7 W/kg  
SAR(1 g) = 8.28 W/kg; SAR(10 g) = 2.34 W/kg  
Smallest distance from peaks to all points 3 dB below = 7.2 mm  
Ratio of SAR at M2 to SAR at M1 = 63.9%  
Maximum value of SAR (measured) = 20.2 W/kg

**Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm**  
Reference Value = 65.08 V/m; Power Drift = -0.07 dB  
Peak SAR (extrapolated) = 35.2 W/kg  
SAR(1 g) = 8.12 W/kg; SAR(10 g) = 2.3 W/kg  
Smallest distance from peaks to all points 3 dB below = 7.2 mm  
Ratio of SAR at M2 to SAR at M1 = 62.5%  
Maximum value of SAR (measured) = 19.1 W/kg

**Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm**  
Reference Value = 62.13 V/m; Power Drift = -0.06 dB  
Peak SAR (extrapolated) = 34.8 W/kg  
SAR(1 g) = 7.71 W/kg; SAR(10 g) = 2.16 W/kg  
Smallest distance from peaks to all points 3 dB below = 7.2 mm  
Ratio of SAR at M2 to SAR at M1 = 61.6%  
Maximum value of SAR (measured) = 18.7 W/kg

0 dB = 18.7 W/kg = 12.72 dBW/kg

Certificate No: Z22-60187 Page 9 of 10

In Collaboration with  
**T T L**  
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62920117  
E-mail: [ott@ttsnet.com](mailto:ott@ttsnet.com) <http://www.ttsnet.com>

**Impedance Measurement Plot for Head TSL**

Certificate No: Z22-60187 Page 10 of 10

## 2 DAE4IP - SN 1826

<div style="display: flex; justify-content: space-between; align-items: center;"> <div style="font-size: 8px;"> <p>Schmid &amp; Partner Engineering AG                  Ziefgassestrasse 43, 8004 Zurich, Switzerland                  Phone +41 44 245 9700, Fax +41 44 245 9779                  www.speag.ch, info@speag.ch</p> </div> <div style="text-align: center; font-weight: bold; font-size: 12px;"> <span style="border-bottom: 1px solid black; padding: 0 5px;">s p e a g</span> </div> </div> <p style="text-align: center; color: red; font-weight: bold; margin-top: 10px;">IMPORTANT NOTICE</p> <p><b>USAGE OF THE DAE4ip</b></p> <p>The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points:</p> <p><b>Shipping of the DAE:</b> Before shipping the DAE to SPEAG for calibration, pack the DAE in an antistatic bag. This antistatic bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside.</p> <p><b>E-Stop Failure:</b> Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements.</p> <p><b>Repair:</b> Minor repairs are performed at no extra cost during the calibration. However, SPEAG reserves the right to charge for any repair especially if rough/unprofessional handling caused the defect.</p> <p><b>DASY Configuration Files:</b> Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MΩ is given in the corresponding configuration file.</p> <div style="border: 1px solid red; padding: 2px; margin-top: 5px;"> <p><b>Important Note:</b>  <span style="color: red;">Warranty and calibration is void if the DAE unit is disassembled partly or fully by the customer.</span></p> </div> <div style="border: 1px solid red; padding: 2px; margin-top: 5px;"> <p><b>Important Note:</b>  <span style="color: red;">Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the calibration procedure.</span></p> </div> <div style="border: 1px solid red; padding: 2px; margin-top: 5px;"> <p><b>Important Note:</b>  <span style="color: red;">To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE.</span></p> </div> <p style="font-size: 8px; margin-top: 10px;">TN_EH231006AA DAE4ip.docx <span style="float: right;">08.10.2023</span></p>	<div style="display: flex; justify-content: space-between; align-items: center;"> <div style="font-size: 8px;"> <p>Calibration Laboratory of                  Schmid &amp; Partner                  Engineering AG                  Zeughausstrasse 43, 8004 Zurich, Switzerland</p> </div> <div style="text-align: center;"> </div> <div style="font-size: 8px;"> <p>S Schweizerischer Kalibrierdienst                  C Service suisse d'étalonnage                  S Service svizzero di taratura                  S Swiss Calibration Service</p> </div> </div> <p style="font-size: 8px; margin-top: 5px;">         Accredited by the Swiss Accreditation Service (SAS)          The Swiss Accreditation Service is one of the signatories to the EA          Multilateral Agreement for the recognition of calibration certificates          Accreditation No.: SCS 0108     </p> <p style="font-size: 8px; margin-top: 5px;">         Client: <b>SGS</b> <span style="float: right;">Certificate No: DAE4ip-1826_Dec23</span>          Kunshan     </p> <div style="border: 1px solid black; padding: 2px; margin-top: 5px;"> <p style="text-align: center; font-weight: bold; font-size: 8px;">CALIBRATION CERTIFICATE</p> <p style="font-size: 8px;">Client: DAE4ip - SD 000 D14 AG - SN: 1826</p> <p style="font-size: 8px;">Calibration procedure(s): QA CAL-06-v30                  Calibration procedure for the data acquisition electronics (DAE)</p> <p style="font-size: 8px;">Calibration date: December 27, 2023</p> <p style="font-size: 8px; margin-top: 5px;">This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p style="font-size: 8px; margin-top: 5px;">All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p style="font-size: 8px; margin-top: 5px;">Calibration: Equipment used (MATE critical for calibration)</p> <table style="font-size: 8px; width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="text-align: left;">Primary Standards</th> <th style="text-align: left;">ID #</th> <th style="text-align: left;">Cal Date (Certificate No.)</th> <th style="text-align: left;">Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Kettley Multimeter Type 2001</td> <td>SN: 0810278</td> <td>29-Aug-23 (No:21421)</td> <td>Aug-24</td> </tr> </tbody> </table> <table style="font-size: 8px; width: 100%; border-collapse: collapse; margin-top: 5px;"> <thead> <tr> <th style="text-align: left;">Secondary Standards</th> <th style="text-align: left;">ID #</th> <th style="text-align: left;">Check Date (in house)</th> <th style="text-align: left;">Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Auto DAE Definition Unit</td> <td>SE LWS 003 AA 1001</td> <td>27-Jan-23 (in house check)</td> <td>In house check: Jan-24</td> </tr> <tr> <td>Calibree Res V3.1</td> <td>SE LWS 006 AA 1002</td> <td>27-Jan-23 (in house check)</td> <td>In house check: Jan-24</td> </tr> </tbody> </table> <div style="display: flex; justify-content: space-between; margin-top: 10px;"> <div style="font-size: 8px;"> <p>Calibrated by: Dominique Steffen                  Function: Laboratory Technician</p> </div> <div style="font-size: 8px;"> <p>Approved by: Sven Kuhn                  Function: Technical Manager</p> </div> </div> <p style="font-size: 8px; margin-top: 5px;">This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued: December 27, 2023</p> </div> <p style="font-size: 8px; margin-top: 5px;">Certificate No: DAE4ip-1826_Dec23 <span style="float: right;">Page 1 of 5</span></p>	Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Kettley Multimeter Type 2001	SN: 0810278	29-Aug-23 (No:21421)	Aug-24	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Auto DAE Definition Unit	SE LWS 003 AA 1001	27-Jan-23 (in house check)	In house check: Jan-24	Calibree Res V3.1	SE LWS 006 AA 1002	27-Jan-23 (in house check)	In house check: Jan-24
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																		
Kettley Multimeter Type 2001	SN: 0810278	29-Aug-23 (No:21421)	Aug-24																		
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																		
Auto DAE Definition Unit	SE LWS 003 AA 1001	27-Jan-23 (in house check)	In house check: Jan-24																		
Calibree Res V3.1	SE LWS 006 AA 1002	27-Jan-23 (in house check)	In house check: Jan-24																		
<div style="display: flex; justify-content: space-between; align-items: center;"> <div style="font-size: 8px;"> <p>Calibration Laboratory of                  Schmid &amp; Partner                  Engineering AG                  Zeughausstrasse 43, 8004 Zurich, Switzerland</p> </div> <div style="text-align: center;"> </div> <div style="font-size: 8px;"> <p>S Schweizerischer Kalibrierdienst                  C Service suisse d'étalonnage                  S Service svizzero di taratura                  S Swiss Calibration Service</p> </div> </div> <p style="font-size: 8px; margin-top: 5px;">         Accredited by the Swiss Accreditation Service (SAS)          The Swiss Accreditation Service is one of the signatories to the EA          Multilateral Agreement for the recognition of calibration certificates          Accreditation No.: SCS 0108     </p> <p style="font-size: 8px; margin-top: 5px;">         Glossary          DAE: data acquisition electronics          Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system.     </p> <p style="font-size: 8px; margin-top: 5px;"> <b>Methods Applied and Interpretation of Parameters</b> <ul style="list-style-type: none"> <li><b>DC Voltage Measurement:</b> Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.</li> <li><b>Connector angle:</b> The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.</li> <li>The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.                     <ul style="list-style-type: none"> <li><b>DC Voltage Measurement Linearity:</b> Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.</li> <li><b>Common mode sensitivity:</b> Influence of a positive or negative common mode voltage on the differential measurement.</li> <li><b>Channel separation:</b> Influence of a voltage on the neighbor channels not subject to an input voltage.</li> <li><b>AD Converter Values with inputs shorted:</b> Values on the internal AD converter corresponding to zero input voltage</li> <li><b>Input Offset Measurement:</b> Output voltage and statistical results over a large number of zero voltage measurements.</li> <li><b>Input Offset Current:</b> Typical value for information; Maximum channel input offset current, not considering the input resistance.</li> <li><b>Input resistance:</b> Typical value for information; DAE input resistance at the connector, during internal auto-zeroing and during measurement.</li> <li><b>Low Battery Alarm Voltage:</b> Typical value for information. Below this voltage, a battery alarm signal is generated.</li> <li><b>Power consumption:</b> Typical value for information. Supply currents in various operating modes.</li> </ul> </li> </ul> </p> <p style="font-size: 8px; margin-top: 10px;">Certificate No: DAE4ip-1826_Dec23 <span style="float: right;">Page 2 of 5</span></p>	<p style="font-size: 8px; margin-top: 5px;"> <b>DC Voltage Measurement</b>          AD - Converter Resolution nominal: 6 bit V, full range = -100...+300 mV          High Range: 1LSB = 6 bit V, full range = -100...+300 mV          Low Range: 1LSB = 6 bit V, full range = -1...+30 mV          DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec     </p> <table style="font-size: 8px; width: 100%; border-collapse: collapse; margin-top: 5px;"> <thead> <tr> <th style="text-align: left;">Calibration Factors</th> <th style="text-align: left;">X</th> <th style="text-align: left;">Y</th> <th style="text-align: left;">Z</th> </tr> </thead> <tbody> <tr> <td>High Range</td> <td>404.998 ± 0.02% (k=2)</td> <td>404.997 ± 0.02% (k=2)</td> <td>404.991 ± 0.02% (k=2)</td> </tr> <tr> <td>Low Range</td> <td>3.98544 ± 1.50% (k=2)</td> <td>3.98262 ± 1.50% (k=2)</td> <td>3.98874 ± 1.50% (k=2)</td> </tr> </tbody> </table> <p style="font-size: 8px; margin-top: 5px;"> <b>Connector Angle</b>          Connector Angle to be used in DASY system: 44.5° ± 1°     </p> <p style="font-size: 8px; margin-top: 10px;">Certificate No: DAE4ip-1826_Dec23 <span style="float: right;">Page 3 of 6</span></p>	Calibration Factors	X	Y	Z	High Range	404.998 ± 0.02% (k=2)	404.997 ± 0.02% (k=2)	404.991 ± 0.02% (k=2)	Low Range	3.98544 ± 1.50% (k=2)	3.98262 ± 1.50% (k=2)	3.98874 ± 1.50% (k=2)								
Calibration Factors	X	Y	Z																		
High Range	404.998 ± 0.02% (k=2)	404.997 ± 0.02% (k=2)	404.991 ± 0.02% (k=2)																		
Low Range	3.98544 ± 1.50% (k=2)	3.98262 ± 1.50% (k=2)	3.98874 ± 1.50% (k=2)																		

Appendix (Additional assessments outside the scope of SCS0108)				
<b>1. DC Voltage Linearity</b>				
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec				
<b>High Range</b>	Reading (µV)	Difference (µV)	Error (%)	
Channel X + Input	200026.55	5.13	0.00	
Channel X - Input	19991.55	0.01	0.00	
Channel X + Input	-20021.43	-0.49	0.00	
Channel Y + Input	200021.86	0.45	0.00	
Channel Y + Input	19999.29	-2.85	-0.01	
Channel Y - Input	-20022.88	-0.07	0.01	
Channel Z + Input	200022.09	0.87	0.00	
Channel Z + Input	19991.17	-0.50	-0.00	
Channel Z - Input	-20021.18	-0.49	0.00	
<b>Low Range</b>	Reading (µV)	Difference (µV)	Error (%)	
Channel X + Input	185.36	-0.23	-0.01	
Channel X + Input	185.86	-0.54	-0.29	
Channel X - Input	-214.25	-1.12	0.53	
Channel Y + Input	1988.41	-0.30	-0.02	
Channel Y + Input	185.56	-1.10	-0.59	
Channel Y - Input	-213.87	-0.60	0.28	
Channel Z + Input	1986.27	-0.58	-0.03	
Channel Z + Input	185.83	-0.85	-0.45	
Channel Z - Input	-213.36	-0.20	0.10	
<b>2. Common mode sensitivity</b>				
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec				
	Common mode Input Voltage (mV)	High Range Average Reading (µV)	Low Range Average Reading (µV)	
Channel X	200	-12.32	-13.70	
	-200	14.81	13.33	
Channel Y	200	8.62	6.45	
	-200	-9.97	-8.85	
Channel Z	200	-9.23	-9.23	
	-200	7.29	9.07	
<b>3. Channel separation</b>				
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec				
	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200	-	0.64	-2.58
Channel Y	200	5.74	-	9.70
Channel Z	200	9.03	4.08	-

Certificate No: DAE4p-1826\_Dec23

Page 4 of 5

**4. AD-Converter Values with inputs shorted**

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15882	17594
Channel Y	16588	16408
Channel Z	15926	14197

**5. Input Offset Measurement**

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input (100µV)	Average (µV)	min. Offset (µV)	max. Offset (µV)	Std. Deviation (µV)
Channel X	0.58	-0.12	1.52	0.34
Channel Y	-2.67	-2.89	0.59	0.46
Channel Z	-0.31	-0.05	0.60	0.46

**6. Input Offset Current**

Normal Input circuitry offset current on all channels: <25µA

**7. Input Resistance** (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

**8. Low Battery Alarm Voltage** (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.5
Supply (- Vcc)	-7.6

**9. Power Consumption** (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-6	-9

Certificate No: DAE4p-1826\_Dec23

Page 5 of 6

## 3 EX3DV4 - SN 7833

Calibration Laboratory of Schmid & Partner Engineering AG			
<p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p>		<p>Accreditation No.: SCS 0108</p>	
Client:	SGS Kunshan	Certificate No.:	EX-7833_Aug23
<b>CALIBRATION CERTIFICATE</b>			
Object:	EX3DV4 - SN7833		
Calibration procedure(s):	QA CAL-01.v10, QA CAL-12.v10, QA CAL-14.v7, QA CAL-23.v6, QA CAL-25.v6 Calibration procedure for dosimetric E-field probes		
Calibration date:	August 24, 2023		
<p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the certified laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (MATE: serial for calibration):</p>			
Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 132778	30-Mar-23 (No. 217-03824-03805)	Mar-24
Power sensor NRP 231	SN: 103944	30-Mar-23 (No. 217-0381)	Mar-24
DCP DAK-3.5 (repaired)	SN: 7349	30-Oct-22 (DCP-DAK3.5-1944_Oct22)	Oct-23
DCP DAK-12	SN: 7316	30-Oct-22 (DCP-DAK12-1076_Oct22)	Oct-23
Reference 20 dB Attenuator	SN: C22563 (20s)	30-Mar-23 (No. 217-03809)	Mar-24
DAK4	SN: 586	18-Mar-23 (No. DA4-489_Mar23)	Mar-24
Reference Probe ES3DV2	SN: 3913	06-Jun-23 (No. ES3-3023_Jun23)	Jun-24
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E41195	SN: G841292874	06-Apr-18 (in house check Jun-23)	in house check Jun-24
Power sensor E4111A	SN: 1014438897	06-Apr-18 (in house check Jun-23)	in house check Jun-24
Power sensor E4111A	SN: 000110216	06-Apr-18 (in house check Jun-23)	in house check Jun-24
RF generator HP 8463A	SN: U8564507190	04-Aug-19 (in house check Jun-23)	in house check Jun-24
Network Analyser E8363A	SN: U841069477	31-Mar-14 (in house check Oct-22)	in house check Oct-24
Calibrated by:	Name: Sven Kastner	Function: Laboratory Technician	Signature:
Approved by:	Name: Sven Klein	Function: Technical Manager	Signature:
This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued: August 28, 2023			
Certificate No: EX-7833_Aug23	Page 1 of 22		

**Calibration Laboratory of Schmid & Partner Engineering AG**

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

**Glossary**

TSL: Tissue stimulating liquid  
 NORM<sub>M,z,z'</sub>: sensitivity in free space  
 ConvF: diode compression point  
 DCP: crest factor (1:50); cycle of the RF signal  
 A, B, C, D: modulation dependent inactivation parameters  
 Polarization φ: φ rotation around probe axis  
 φ rotation around axis that is in the plane normal to probe axis (at measurement center), i.e., φ = 0 is normal to probe axis  
 Connector Angle: information used in DASY system to align probe sensor X to the robot coordinate system

**Calibration is Performed According to the Following Standards:**

- a) IEC/IEEE 62209-1528: "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Ranges of 4 MHz to 10 GHz)", October 2020.
- b) IEC 605684: "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Methods Applied and Interpretation of Parameters:**

- NORM<sub>M,z,z'</sub>: Assessed for E-field polarization (θ = 0) (f < 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORM<sub>M,z,z'</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>M,z,z'</sub> does not affect the E-field uncertainty inside TSL (see below ConvF).
- NORM<sub>M,z,z'</sub> - NORM<sub>M,z,z'</sub> - frequency\_response (see Frequency Response Chart). This inactivation is implemented in DASY4 software version later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP: DCP are numerical inactivation parameters assessed based on the data of power sweep with CW signal. DCP does not depend on frequency nor media.
- PMS: PMS is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A<sub>M,z,z'</sub>, B<sub>M,z,z'</sub>, C<sub>M,z,z'</sub>, D<sub>M,z,z'</sub>, V<sub>M,z,z'</sub>: A, B, C, D are numerical inactivation parameters assessed based on the data of calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameter: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f < 300 MHz) and made equivalent using analytical field distributions based on power measurements for f > 300 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>M,z,z'</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from 150 MHz to 1100 MHz.
- Spherical Isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe lip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORM<sub>M</sub> (no uncertainty required).

Certificate No: EX-7833\_Aug23

Page 2 of 22

EX3DV4 - SN:7833 August 24, 2023

**Parameters of Probe: EX3DV4 - SN:7833**

**Basic Calibration Parameters**

Norm. $\mu\text{V}/(\text{V/m})^A$	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
	0.65	0.68	0.59	$\pm 10.1\%$
DCP (mV) <sup>B</sup>	111.0	108.3	108.3	$\pm 4.7\%$

**Calibration Results for Modulation Response**

UID	Communication System Name	A	B	C	D	VR	Mix dev.	Max Unc <sup>C</sup> (k=2)
		dB	dB $\mu\text{V}$		dB	mV		
0	CW	X 0.00	0.00	1.00	0.00	138.2	$\pm 2.2\%$	$\pm 4.7\%$
		Y 1.93	0.00	1.00		137.5		
		Z 0.00	0.00	1.00		138.7		
10352	Pulse Wavform (200Hz, 10%)	X 1.43	62.39	6.12	10.00	60.0	$\pm 3.2\%$	$\pm 9.6\%$
		Y -1.27	51.29	6.51		60.0		
		Z 1.81	60.88	6.30		60.0		
10353	Pulse Wavform (200Hz, 20%)	X 10.00	72.50	9.00	8.60	90.0	$\pm 2.9\%$	$\pm 8.8\%$
		Y 0.84	60.00	4.70		80.0		
		Z 44.00	70.30	11.00		80.0		
10354	Pulse Wavform (200Hz, 40%)	X 0.57	66.00	3.54	3.98	96.0	$\pm 2.8\%$	$\pm 8.6\%$
		Y 0.06	73.00	0.00		95.0		
		Z 0.00	68.00	0.00		95.0		
10355	Pulse Wavform (200Hz, 60%)	X 7.50	77.02	2.05	2.22	100.0	$\pm 1.7\%$	$\pm 9.6\%$
		Y -4.84	73.60	12.83		100.0		
		Z 0.00	68.00	0.00		95.0		
10357	QPSK Wavform, 1MHz	X 0.97	66.00	14.25	1.00	100.0	$\pm 3.0\%$	$\pm 9.2\%$
		Y 0.49	83.39	12.04		100.0		
		Z 0.68	74.04	12.82		100.0		
10388	QPSK Wavform, 10MHz	X 1.43	67.97	14.98	0.00	100.0	$\pm 0.9\%$	$\pm 9.6\%$
		Y 1.79	65.58	13.88		100.0		
		Z 1.25	68.73	13.78		100.0		
10399	64-QAM Wavform, 100MHz	X 1.77	68.60	18.47	0.01	100.0	$\pm 1.0\%$	$\pm 9.6\%$
		Y 1.79	66.50	16.95		100.0		
		Z 1.76	68.45	18.14		100.0		
10399	64-QAM Wavform, 40MHz	X 1.51	68.91	18.44	0.00	100.0	$\pm 2.1\%$	$\pm 9.6\%$
		Y 2.58	68.63	18.33		100.0		
		Z 2.74	68.79	18.24		100.0		
10414	WLAN CDDF, 64-QAM, 40MHz	X 3.87	68.03	18.69	0.00	100.0	$\pm 3.5\%$	$\pm 9.6\%$
		Y -3.87	68.40	18.44		100.0		
		Z -3.80	68.37	18.51		100.0		

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is based on the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X, Y, Z do not affect the E1 field uncertainty inside T30. See Page 5 and 6.  
<sup>B</sup> Precision parameter uncertainty for maximum specified field strength.  
<sup>C</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: EX-7833\_Aug23 Page 3 of 22

EX3DV4 - SN:7833 August 24, 2023

**Parameters of Probe: EX3DV4 - SN:7833**

**Sensor Model Parameters**

	C1	C2	V1	V2	T3	T4	T5	T6
	dB	dB	V/m	mm/s	mm	mm	mm	mm
x	8.8	60.54	31.91	4.38	0.30	4.90	0.61	0.00
y	8.8	60.77	32.80	4.78	0.00	4.90	0.61	0.00
z	7.3	51.94	32.49	3.79	0.30	4.90	0.61	0.00

**Other Probe Parameters**

Parameter	Value
Sensor Arrangement	Triangular
Connector Angle	$\pm 4^\circ$
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	237 mm
Probe Body Diameter	19 mm
Tip Diameter	9 mm
Probe Tip to Sensor X Calibration Point	2.5 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Note: Measurement distance from surface can be increased to 3.4 mm for an App30 pin jack.

Certificate No: EX-7833\_Aug23 Page 4 of 22

EX3DV4 - SN:7833 August 24, 2023

**Parameters of Probe: EX3DV4 - SN:7833**

**Calibration Parameter Determined in Head Tissue Simulating Media**

f (MHz)	Relative Permittivity <sup>A</sup>	Conductivity <sup>B</sup> (S/m)	CompF X	CompV Y	CompZ Z	Alpha <sup>C</sup>	Depth <sup>D</sup> (mm)	Unc (k=2)
750	41.9	0.89	7.85	8.96	8.55	0.43	1.27	$\pm 12.0\%$
835	41.5	0.90	7.57	8.62	8.54	0.42	1.27	$\pm 12.0\%$
1750	40.1	1.07	7.08	8.09	7.85	0.31	1.27	$\pm 12.0\%$
1900	40.0	1.40	6.39	7.26	5.93	0.31	1.27	$\pm 12.0\%$
2150	39.8	1.49	6.25	7.10	6.78	0.32	1.27	$\pm 12.0\%$
2300	39.5	1.57	6.07	6.82	6.58	0.33	1.27	$\pm 12.0\%$
2450	39.2	1.80	5.98	6.77	6.44	0.31	1.27	$\pm 12.0\%$
2500	39.0	1.95	6.11	6.91	6.68	0.30	1.27	$\pm 12.0\%$
3300	38.2	2.71	6.16	7.02	6.07	0.36	1.27	$\pm 14.0\%$
3500	37.9	2.91	5.61	6.40	6.07	0.36	1.27	$\pm 14.0\%$
3700	37.7	3.12	5.65	6.46	6.15	0.32	1.30	$\pm 14.0\%$
3900	37.5	3.32	6.07	6.91	6.66	0.38	1.27	$\pm 14.0\%$
4100	37.2	3.53	5.78	6.58	6.21	0.37	1.27	$\pm 14.0\%$
4200	37.1	3.63	5.41	6.17	5.88	0.36	1.27	$\pm 14.0\%$
4400	36.9	3.84	5.25	5.96	5.69	0.37	1.27	$\pm 14.0\%$
4600	36.7	4.04	5.85	6.44	6.12	0.36	1.30	$\pm 14.0\%$
4800	36.4	4.25	5.77	6.55	6.25	0.38	1.27	$\pm 14.0\%$
4950	36.3	4.40	5.26	5.93	5.69	0.41	1.38	$\pm 14.0\%$
5000	36.0	4.68	5.16	5.87	5.61	0.34	1.51	$\pm 14.0\%$
5300	35.9	4.78	5.02	5.70	5.39	0.32	1.83	$\pm 14.0\%$
5500	35.6	4.96	4.50	5.15	4.85	0.36	1.61	$\pm 14.0\%$
5600	35.5	5.07	4.33	4.92	4.68	0.41	1.54	$\pm 14.0\%$
5900	35.3	5.27	4.20	5.13	4.87	0.31	1.66	$\pm 14.0\%$

<sup>A</sup> Frequency validity above 803.0MHz is only applicable for DNFV-A4 level higher than Page 20, when it is specified to  $\pm 0.5\%$ . The uncertainty is the RSS of the CompF uncertainty of calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 803.0MHz is  $\pm 1\%$ ,  $\pm 2\%$ ,  $\pm 3\%$ ,  $\pm 4\%$ ,  $\pm 5\%$ ,  $\pm 6\%$ ,  $\pm 7\%$ ,  $\pm 8\%$ ,  $\pm 9\%$ ,  $\pm 10\%$ ,  $\pm 12\%$ ,  $\pm 15\%$ ,  $\pm 20\%$ ,  $\pm 25\%$ ,  $\pm 30\%$ ,  $\pm 35\%$ ,  $\pm 40\%$ ,  $\pm 45\%$ ,  $\pm 50\%$ ,  $\pm 55\%$ ,  $\pm 60\%$ ,  $\pm 65\%$ ,  $\pm 70\%$ ,  $\pm 75\%$ ,  $\pm 80\%$ ,  $\pm 85\%$ ,  $\pm 90\%$ ,  $\pm 95\%$ ,  $\pm 100\%$ .  
<sup>B</sup> The probe is not calibrated using tissue simulating media (TSM) that deviates from a dielectric loss tangent of  $\pm 0.10$ .  
<sup>C</sup> AlphaDepth are determined using calibration. AlphaDepth is the distance from the boundary effect due to the boundary effect after compensation is always less than  $\pm 1\%$  for frequencies below 3GHz and below  $\pm 2\%$  for frequencies between 3-6GHz and below  $\pm 4\%$  for frequencies between 6-10GHz at any distance larger than half the probe to distance from the boundary.  
<sup>D</sup> AlphaDepth are determined using calibration. AlphaDepth is the distance from the boundary effect due to the boundary effect after compensation is always less than  $\pm 1\%$  for frequencies below 3GHz and below  $\pm 2\%$  for frequencies between 3-6GHz and below  $\pm 4\%$  for frequencies between 6-10GHz at any distance larger than half the probe to distance from the boundary.

Certificate No: EX-7833\_Aug23 Page 5 of 22

EX3DV4 - SN:7833 August 24, 2023





**Parameters of Probe: EX3DV4 - SN:7833**

**Calibration Parameter Determined in Head Tissue Simulating Media**

f (MHz)	Relative Permittivity <sup>A</sup>	Conductivity <sup>B</sup> (S/m)	CompF X	CompV Y	CompZ Z	Alpha <sup>C</sup>	Depth <sup>D</sup> (mm)	Unc (k=2)
6500	24.5	6.07	6.74	5.36	4.91	0.20	2.00	$\pm 18.6\%$

<sup>A</sup> Frequency validity at 6.5GHz is  $\pm 0.5\%$ ,  $\pm 1\%$ ,  $\pm 2\%$ ,  $\pm 3\%$ ,  $\pm 4\%$ ,  $\pm 5\%$ ,  $\pm 6\%$ ,  $\pm 7\%$ ,  $\pm 8\%$ ,  $\pm 9\%$ ,  $\pm 10\%$ ,  $\pm 12\%$ ,  $\pm 15\%$ ,  $\pm 20\%$ ,  $\pm 25\%$ ,  $\pm 30\%$ ,  $\pm 35\%$ ,  $\pm 40\%$ ,  $\pm 45\%$ ,  $\pm 50\%$ ,  $\pm 55\%$ ,  $\pm 60\%$ ,  $\pm 65\%$ ,  $\pm 70\%$ ,  $\pm 75\%$ ,  $\pm 80\%$ ,  $\pm 85\%$ ,  $\pm 90\%$ ,  $\pm 95\%$ ,  $\pm 100\%$ . The uncertainty is the RSS of the CompF uncertainty of calibration frequency and the uncertainty for the indicated frequency band.  
<sup>B</sup> The probe is not calibrated using tissue simulating media (TSM) that deviates from a dielectric loss tangent of  $\pm 0.10$ .  
<sup>C</sup> AlphaDepth are determined using calibration. AlphaDepth is the distance from the boundary effect due to the boundary effect after compensation is always less than  $\pm 1\%$  for frequencies below 3GHz and below  $\pm 2\%$  for frequencies between 3-6GHz and below  $\pm 4\%$  for frequencies between 6-10GHz at any distance larger than half the probe to distance from the boundary.  
<sup>D</sup> AlphaDepth are determined using calibration. AlphaDepth is the distance from the boundary effect due to the boundary effect after compensation is always less than  $\pm 1\%$  for frequencies below 3GHz and below  $\pm 2\%$  for frequencies between 3-6GHz and below  $\pm 4\%$  for frequencies between 6-10GHz at any distance larger than half the probe to distance from the boundary.

Certificate No: EX-7833\_Aug23 Page 6 of 22

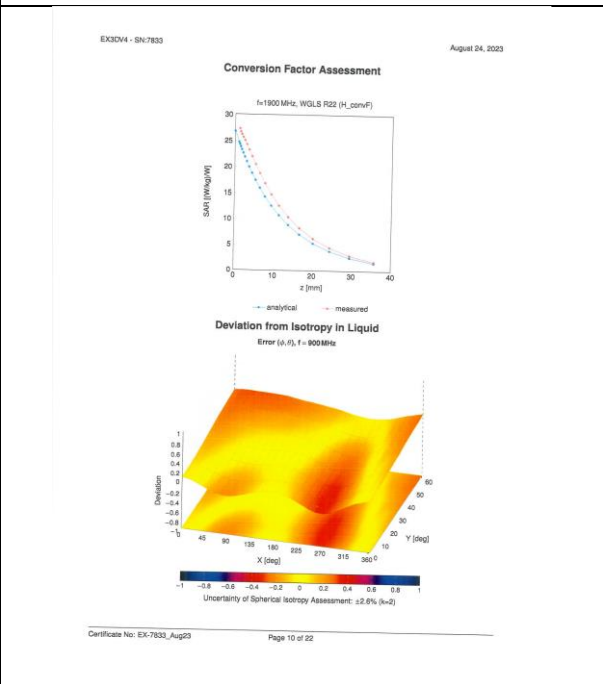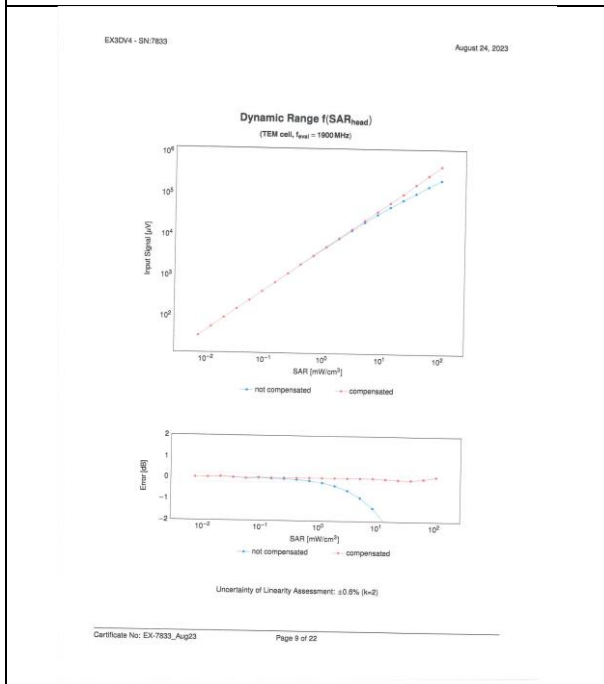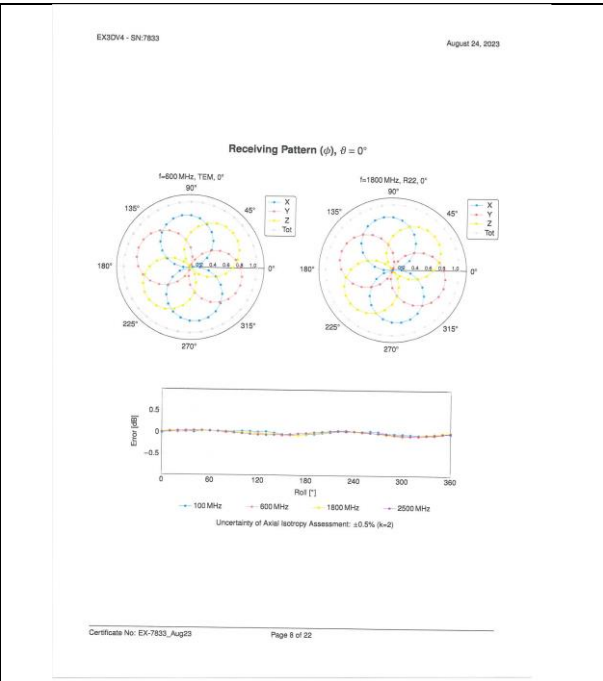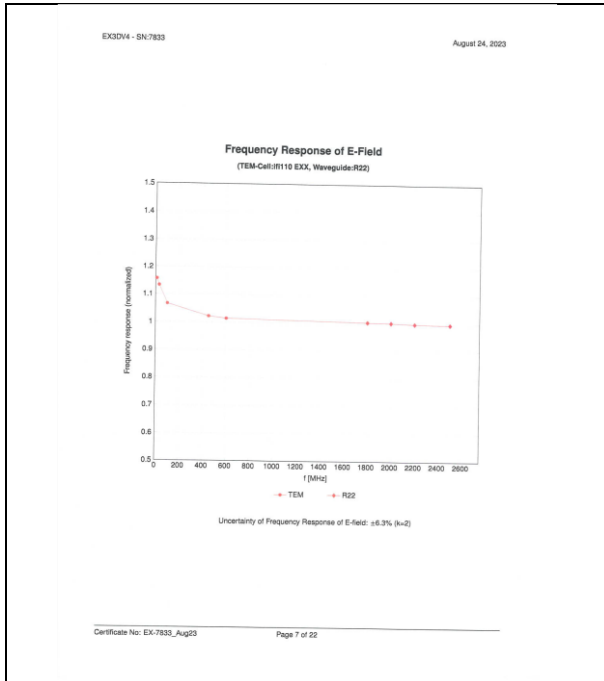



EX3004 - 5N7833

August 24, 2023

Appendix: Modulation Calibration Parameters

Table with columns: LNB, Rev, Communication System Name, Group, HNR(dB), UHF # x 2. Lists various modulation calibration parameters for different systems.

Certificate No: EX-7833\_Aug23 Page 11 of 22

EX3004 - 5N7833

August 24, 2023

Table with columns: LNB, Rev, Communication System Name, Group, HNR(dB), UHF # x 2. Continuation of modulation calibration parameters.

Certificate No: EX-7833\_Aug23 Page 12 of 22

EX3004 - 5N7833

August 24, 2023

Table with columns: LNB, Rev, Communication System Name, Group, HNR(dB), UHF # x 2. Continuation of modulation calibration parameters.

Certificate No: EX-7833\_Aug23 Page 13 of 22

EX3004 - 5N7833

August 24, 2023

Table with columns: LNB, Rev, Communication System Name, Group, HNR(dB), UHF # x 2. Continuation of modulation calibration parameters.

Certificate No: EX-7833\_Aug23 Page 14 of 22