

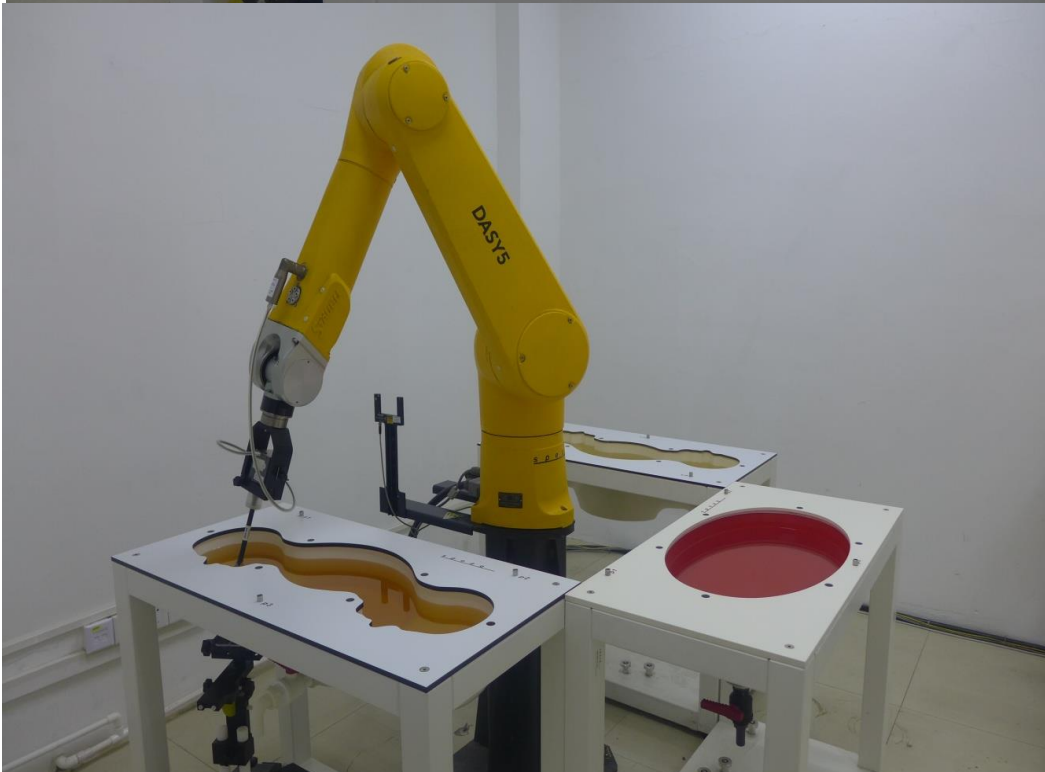
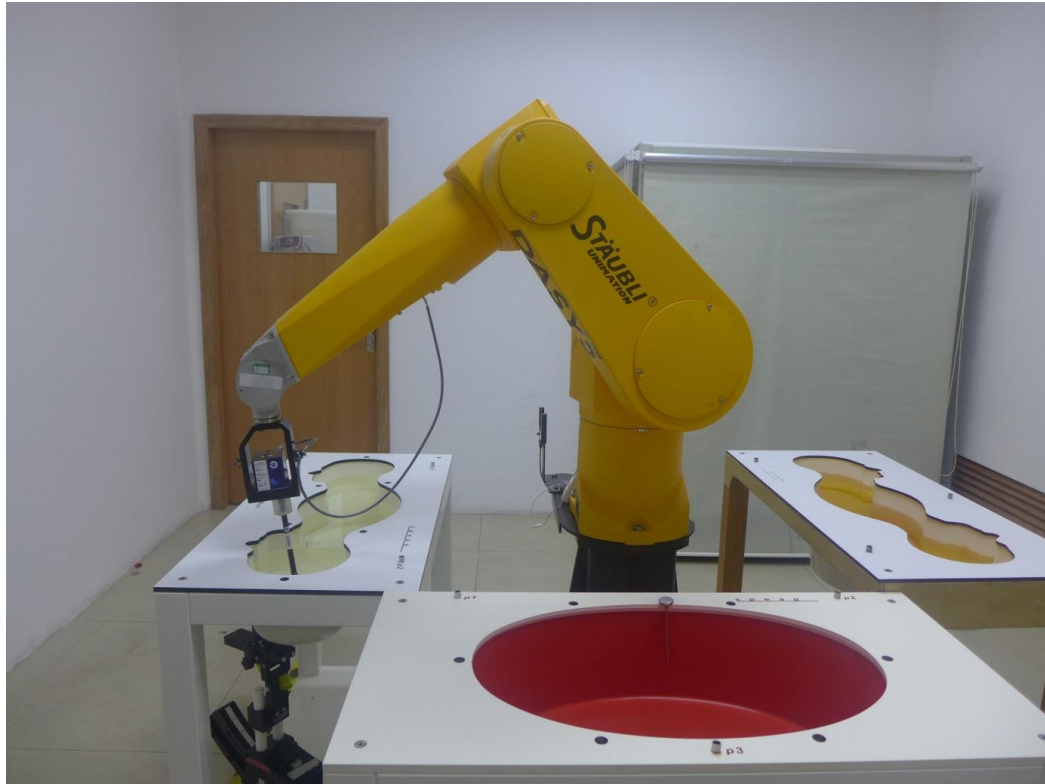


Appendix D

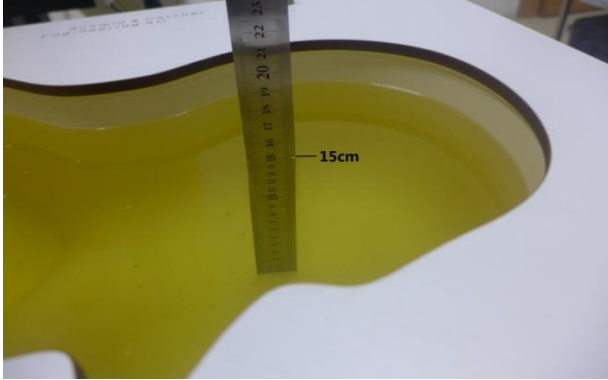
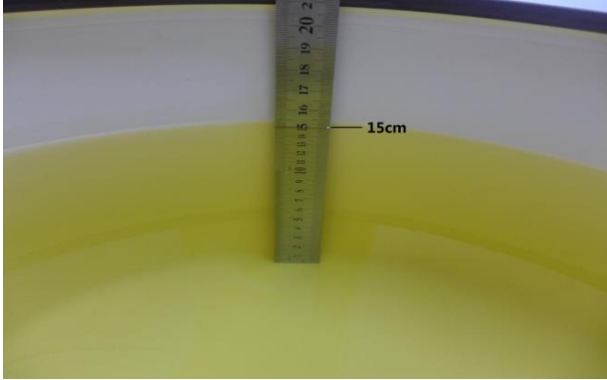
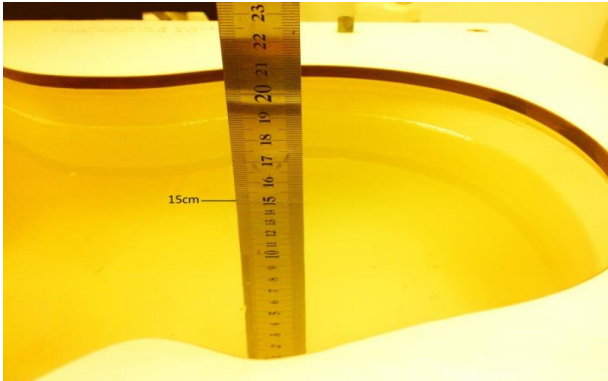
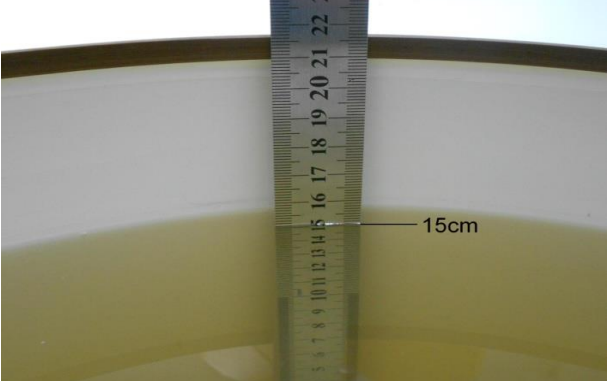
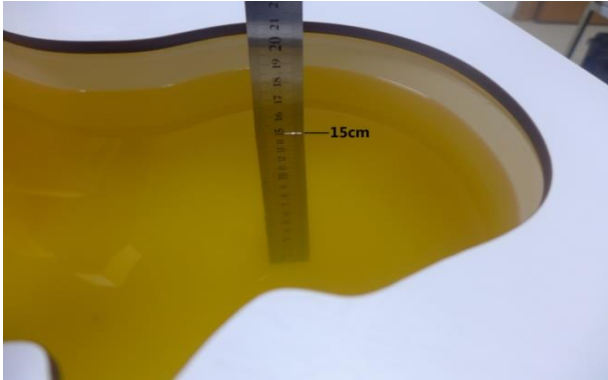
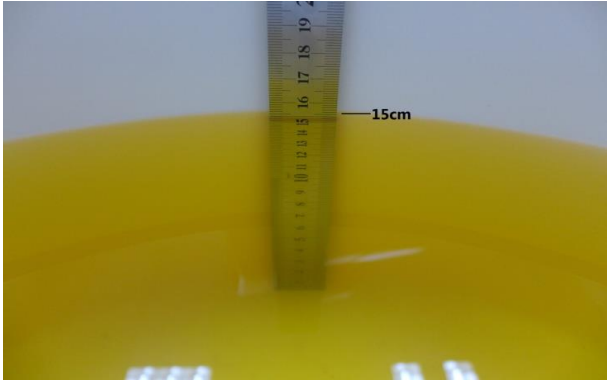
Photographs

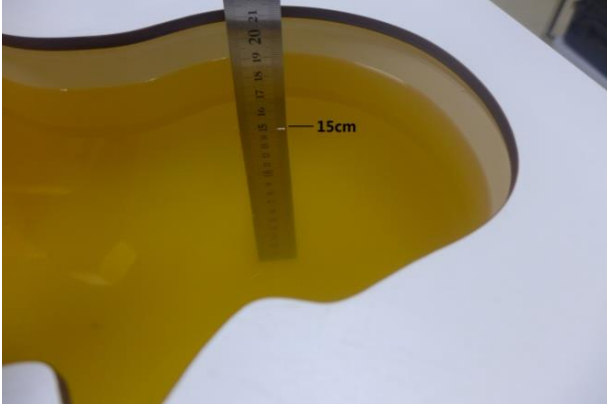
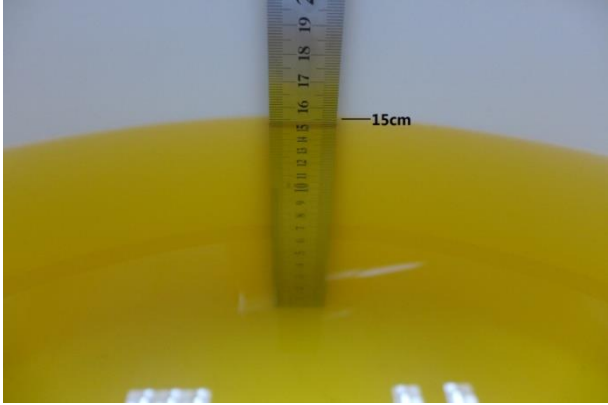
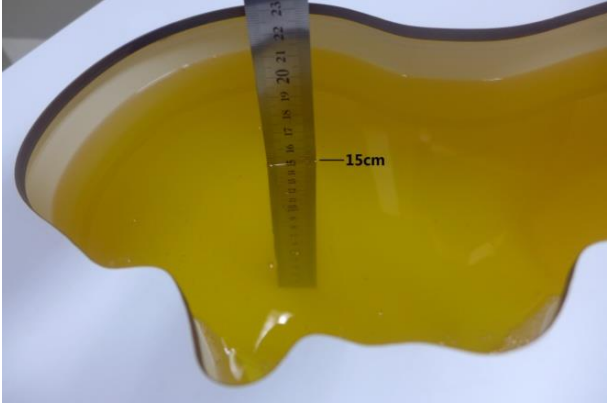
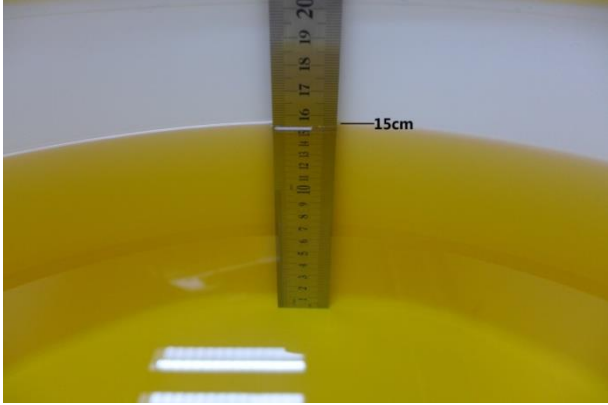
1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details
5. Serial Number of EUT

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 750</p>	<p>Photo 2: Tissue Simulant Liquid for Body 750</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 835</p>	<p>Photo 4: Tissue Simulant Liquid for Body 835</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 1750</p>	<p>Photo 6: Tissue Simulant Liquid for Body 1750</p>
	

<p>Photo 7: Tissue Simulant Liquid for Head 1900</p>	<p>Photo 8: Tissue Simulant Liquid for Body 1900</p>
	
<p>Photo 9: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 10: Tissue Simulant Liquid for Body 2450</p>
	

3. Photographs of EUT test position

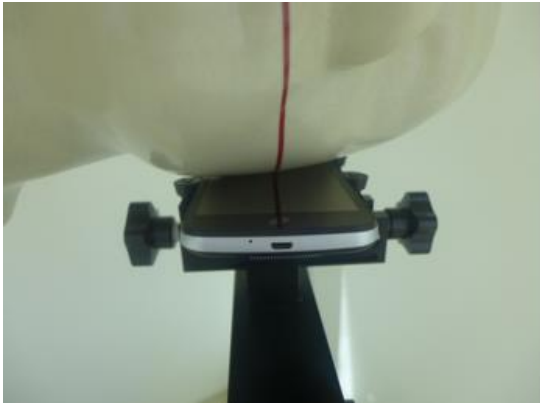
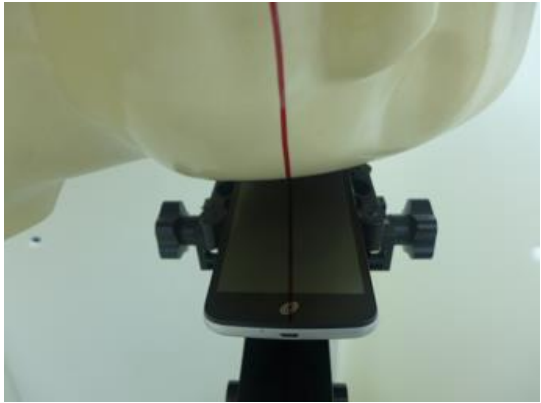
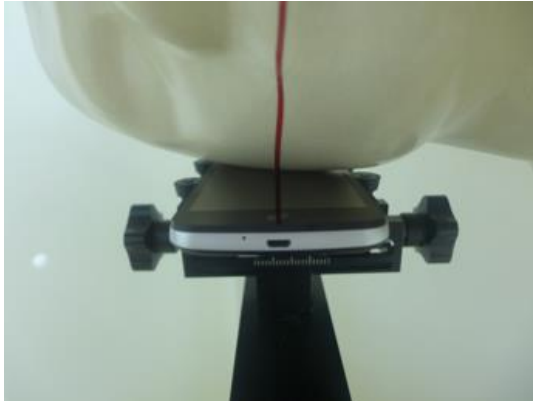
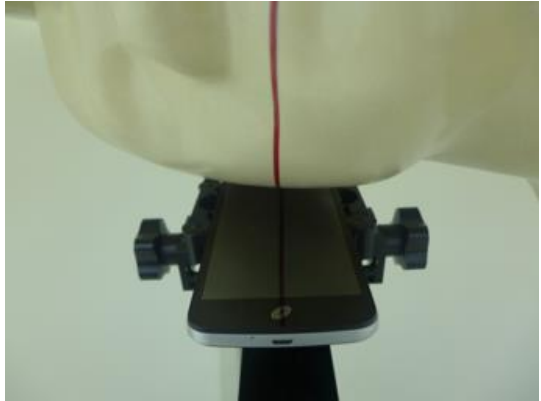








<p align="center">Photo 11: Left cheek</p>	<p align="center">Photo 12: Left tilted</p>
	
<p align="center">Photo 13: Right cheek</p>	<p align="center">Photo 14: Right tilted</p>
	
<p align="center">Photo 15: Front side 15mm</p>	<p align="center">Photo 16: Back side 15mm</p>
	

Photo 17: Front side 10mm	Photo 18: Back side 10mm
	
Photo 19: Left side 10mm	Photo 20: Right side 10mm
	
Photo 21: Top side 10mm	Photo 22: Bottom side 10mm
	

4. EUT Constructional Details

