

Report No.: HR/2019/1000505

Appendix D

Photographs

- 1. SAR measurement System
- 2. Photographs of Tissue Simulate Liquid
- 3. Photographs of EUT test position
- 4. EUT Constructional Details




Report No.: HR/2019/1000505

1. SAR measurement System



Report No.: HR/2019/1000505

2. Photographs of Tissue Simulate Liquid

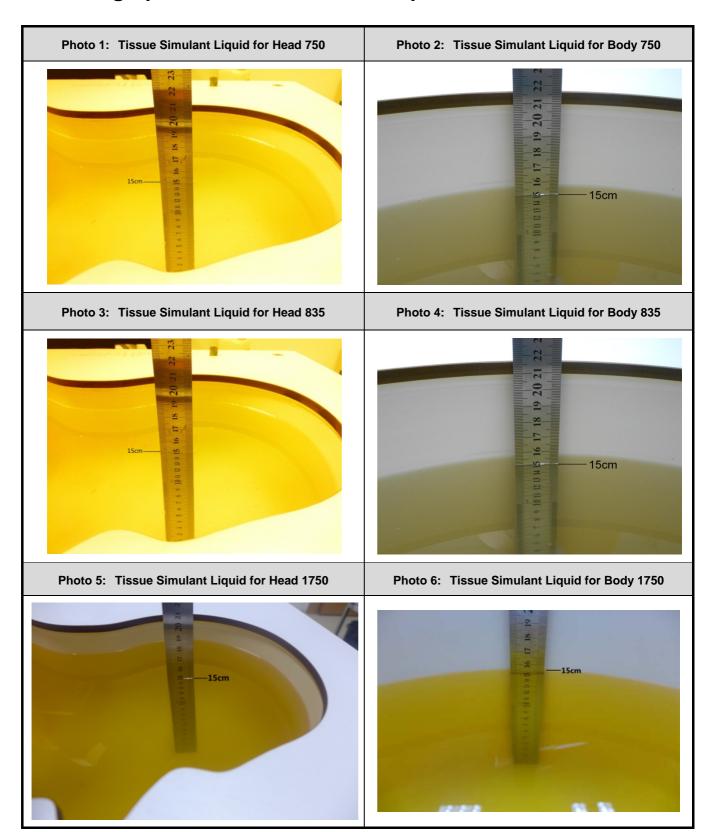



Report No.: HR/2019/1000505

Photo 7: Tissue Simulant Liquid for Head 1900 Photo 8: Tissue Simulant Liquid for Body 1900 Photo 9: Tissue Simulant Liquid for Head 2450 Photo 10: Tissue Simulant Liquid for Body 2450 Photo 12: Tissue Simulant Liquid for Body 2600 Photo 11: Tissue Simulant Liquid for Head 2600



Report No.: HR/2019/1000505

3. Photographs of EUT test position

Photo 13: Left touch cheek

Photo 15: Right touch cheek



Photo 17: Front side 15mm



Photo 14: Left tilted 15 degree

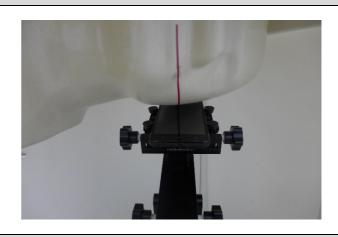


Photo 16: Right tilted 15 degree

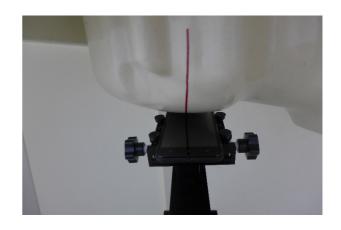


Photo 18: Back side 15mm





Report No.: HR/2019/1000505

Photo 19: Front side 10mm

Photo 20: Back side 10mm



Photo 21: Left side 10mm

Photo 22: Right side 10mm



Photo 23: Top side 10mm

Photo 24: Bottom side 10mm







Report No.: HR/2019/1000505

4. EUT Constructional Details

