

Date of Issue:

2011-10-05

Page:

1/56

SAR TEST REPORT

Equipment Under Test

: Tablet PC

Model No.

AMD120

Applicant

AnyDATA Corporation

Address of Applicant

5 Oldfield, Irvine, CA, 92602

FCC ID

P4M-AMD120

Device Category

Portable Device

Exposure Category

General Population/Uncontrolled Exposure

Date of Receipt

2011-08-11

Date of Test(s)

2011-10-04

Date of Issue

2011-10-05

Max. SAR

1.13 W/kg (11b)

Standards:

FCC OET Bulletin 65 supplement C IEEE 1528, 2003 ANSI/IEEE C95.1, C95.3

In the configuration tested, the EUT complied with the standards specified above.

Remarks:

This report details the results of the testing carried out on one sample, the results contained in this test report do not relate to other samples of the same product. The manufacturer should ensure that all products in series production are in conformity with the product sample detailed in this report.

This report may only be reproduced and distributed in full. If the product in this report is used in any configuration other than that detailed in the report, the manufacturer must ensure the new system complies with all relevant standards. Any mention of SGS Korea Co., Ltd. (Gunpo Laboratory) or testing done by SGS Korea Co., Ltd. (Gunpo Laboratory) in connection with distribution or use of the product described in this report must be approved by SGS Korea Co., Ltd. (Gunpo Laboratory) in writing.

Tested by

: Fred Jeong

2011-10-05

Approved by

: Charles Kim

2011-10-05



19

Date of Issue : 2011-10-05
Page : 2 / 56

Contents

1. (Genera	l Information	
	1.1	Testing Laboratory	3
	1.2	Details of Applicant.	3
	1.3	Version of Report	3
	1.4	Description of EUT(s).	3
	1.5	Test Environment.	4
	1.6	Operation description.	4
	1.7	Evaluation procedures.	5
	1.8	The SAR Measurement System.	6
	1.9	System Components	8
	1.10	SAR System Verification.	9
	1.11	Tissue Simulant Fluid for the Frequency Band	11
	1.12	Test Standards and Limits	12
	1.13	Justification for Extended SAR Dipole Calibrations	13
2. 1	[nstrun	nents List	14
3. 8	Summa	ary of Results	15
	3.1	FCC Power Measurement Procedures.	15
	3.2	RF Conducted Power.	15
	3.3	SAR Test Configuration.	17

SAR Data Summary....

APPENDIX

3.4

- A. DASY4 SAR Report
- B. Uncertainty Analysis
- C. Calibration certificate



Date of Issue : 2011-10-05 Page : 3 / 56

1. General Information

1.1 Testing Laboratory

SGS Korea Co., Ltd. (Gunpo Laboratory)

18-34, Sanbon-dong, Gunpo-si, Gyeonggi-do, 435-040, Korea

Telephone : +82 +31 428 5700 FAX : +82 +31 427 2371 Homepage : www.kr.sgs.com/ee

1.2 Details of Applicant

Applicant : AnyDATA Corporation.
Address : 5 Oldfield, Irvine, CA, 92602
Email : Kevinkim@anydata.com

Phone No. : 949-900-6040

1.3 Version of Report

Version Number	Date	Revision
00	2011-08-25	Initial issue
01	2011-10-05	Revision 01

1.4 Description of EUT(s)

EUT Type	: Tablet PC
Model	: AMD120
FCC ID	: P4M-AMD120
Serial Number	: 0228433
Mode of Operation	: WLAN
Duty Cycle	: 1(WLAN)
Body worn Accessory	: None
Tx Frequency Range	: 2412 MHz ~ 2462 MHz (WLAN) 2402 MHz ~ 2480 MHz (Bluetooth)
Conducted Max Power	: 15.01 dBm (WLAN), -3.40 dBm(Bluetooth)



Date of Issue : 2011-10-05 Page : 4 / 56

1.5 Test Environment

Ambient temperature	: (22 ± 2) ° C
Tissue Simulating Liquid	: (22 ± 2) ° C
Relative Humidity	$: (55 \pm 5) \% \text{ R.H.}$

1.6 Operation Configuration

The client provided a special driver and test program which can control the frequency and power of the WLAN. Measurements were performed at the lowest, middle and highest channels of the operating band. The EUT was set to maximum power level during all tests and at the beginning of each test the battery was fully charged. The DASY4 system measures power drift during SAR testing by comparing e-field in the same location at the beginning and at the end of measurement.



Date of Issue : 2011-10-05 Page : 5 / 56

1.7 EVALUATION PROCEDURES

- Power Reference Measurement Procedures

The Power Reference Measurement and Power Drift Measurements are for monitoring the power drift of the device under test in the batch process. The Minimum distance of probe sensors to surface determines the closest measurement point to phantom surface. The minimum distance of probe sensors to surface is 4 mm. This distance cannot be smaller than the Distance of sensor calibration points to probe tip as defined in the probe properties (for example, 2.7 mm for an ET3DV6 probe type).

- The entire evaluation of the spatial peak values is performed within the Post-processing engine (SEMCAD). The system always gives the maximum values for the 1 g and 10 g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:
- 1. The extraction of the measured data (grid and values) from the Zoom Scan.
- 2. The calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- 3. The generation of a high-resolution mesh within the measured volume
- 4. The interpolation of all measured values from the measurement grid to the high-resolution grid
- 5. The extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- 6. The calculation of the averaged SAR within masses of 1 g and 10 g.

The probe is calibrated at the center of the dipole sensors that is located 1 mm to 2.7 mm away from the probe tip. During measurements, the probe stops shortly above the phantom surface, depending on the probe and the surface detecting system. Both distances are included as parameters in the probe configuration file. The software always knows exactly how far away the measured point is from the surface. As the probe cannot directly measure at the surface, the values between the deepest measured point and the surface must be extrapolated. The angle between the probe axis and the surface normal line is less than 30 degree.

In the Area Scan, the gradient of the interpolation function is evaluated to find all the extreme of the SAR distribution. The uncertainty on the locations of the extreme is less than 1/20 of the grid size. Only local maximum within –2 dB of the global maximum are searched and passed for the Cube Scan measurement. In the Cube Scan, the interpolation function is used to extrapolate the Peak SAR from the lowest measurement points to the inner phantom surface (the extrapolation distance). The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1 % for the 1 g and 10 g cubes, the extrapolation distance should not be larger than 5 mm.

The maximum search is automatically performed after each area scan measurement. It is based on splines in two or three dimensions. The procedure can find the maximum for most SAR distributions even with



Date of Issue : 2011-10-05 Page : 6 / 56

relatively large grid spacing. After the area scanning measurement, the probe is automatically moved to a position at the interpolated maximum. The following scan can directly use this position for reference, e.g., for a finer resolution grid or the cube evaluations. The 1 g and 10 g peak evaluations are only available for the predefined cube 7x7x7 scans. The routines are verified and optimized for the grid dimensions used in these cube measurements. The measured volume of 30x30x30mm contains about 30 g of tissue. The first procedure is an extrapolation (incl. Boundary correction) to get the points between the lowest measured plane and the surface. The next step uses 3D interpolation to get all points within the measured volume. In the last step, a 1 g cube is placed numerically into the volume and its averaged SAR is calculated. This cube is the moved around until the highest averaged SAR is found. If the highest SAR is found at the edge of the measured volume, the system will issue a warning: higher SAR values might be found outside of the measured volume. In that case the cube measurement can be repeated, using the new interpolated maximum as the center.

1.8 The SAR Measurement System

A photograph of the SAR measurement System is given in Fig. a. This SAR Measurement System uses a Computer-controlled 3-D stepper motor system (Speag Dasy 4 professional system). A Model ET3DV6 1782 E-field probe is used to determine the internal electric fields. The SAR can be obtained from the equation SAR= σ (|Ei|2)/ ρ where σ and ρ are the conductivity and mass density of the tissue-simulant. The DASY4 system for performing compliance tests consists of the following items:

- •A standard high precision 6-axis robot (Staubli RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- •A dosimeter probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- •A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.



Date of Issue : 2011-10-05 Page : 7/56

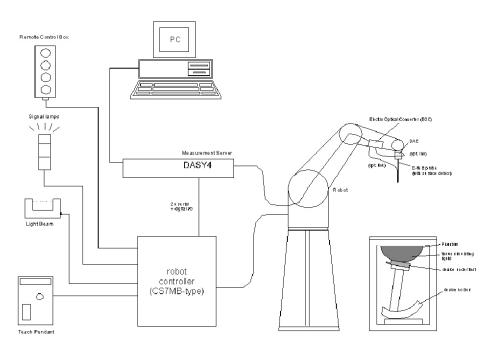


Fig a. The microwave circuit arrangement used for SAR system verification

- The Electro-optical converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection. The EOC is connected to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- A computer operating Windows 2000 or Windows XP.
- DASY4 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM twin phantom enabling testing body usage.
- The device holder for flat phantom.
- Tissue simulating liquid mixed according to the given recipes.
- Validation dipole kits allowing to validate the proper functioning of the system.



Date of Issue : 2011-10-05 Page : 8 / 56

1.9 System Components

ET3DV6 E-Field Probe

Construction: Symmetrical design with triangular core Built-in shielding

against static charges PEEK enclosure material (resistant to

organic solvents, e.g. glycol).

Calibration : In air from 10 MHz to 2.5 GHz In brain simulating tissue

 $(accuracy \pm 8 \%)$

Frequency: 10 MHz to > 6 GHz; Linearity: $\pm 0.2 \text{ dB}$ (30 MHz to 3 GHz)

Directivity : ± 0.2 dB in brain tissue (rotation around probe axis)

 ± 0.4 dB in brain tissue (rotation normal to probe axis)

Dynamic Range : $5 \mu W/g$ to >100 mW/g; Linearity: $\pm 0.2 dB$

tange

Srfce. Detect : ± 0.2 mm repeatability in air and clear liquids over diffuse

reflecting surfaces


Dimensions: Overall length: 330 mm

Tip length: 16 mm Body diameter: 12 mm Tip diameter: 6.8 mm

Distance from probe tip to dipole centers: 2.7 mm

Application: General dosimetry up to 3 GHz Compliance tests of mobile

phone



ET3DV6 E-Field Probe

NOTE:

1. The Probe parameters have been calibrated by the SPEAG. Please reference "APPENDIX D" for the Calibration Certification Report.



Date of Issue : 2011-10-05 Page : 9/56

SAM Phantom

Construction: The SAM Phantom is constructed of a fiberglass

shell integrated in a wooden table. The shape of the shell is based on data from an anatomical study designed to determine the maximum exposure in at least 90 % of all users. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents the evaporation of the liquid. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually

teaching three points in the robot

Shell Thickness: $2.0 \text{ mm} \pm 0.1 \text{ mm}$ Filling Volume: Approx. 25 liters



SAM Phantom

DEVICE HOLDER

Construction

In combination with the Twin SAM PhantomV4.0/V4.0C or Twin SAM, the Mounting Device (made from POM) enables the rotation of the mounted transmitter in spherical coordinates, whereby the rotation point is the ear opening. The devices can be easily and accurately positioned according to IEC, IEEE, CENELEC, FCC or other specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).



Device Holder

1.10 SAR System Verification

The microwave circuit arrangement for system verification is sketched in Fig. b. The daily system accuracy verification occurs within the flat section of the SAM phantom. A SAR measurement was performed to see if the measured SAR was within \pm 10 % from the target SAR values. These tests were done at 2450 MHz. The tests for EUT were conducted within 24 hours after each validation. The obtained results from the system accuracy verification are displayed in the table 1. During the tests, the ambient temperature of the laboratory was in the range (22 \pm 2) ° C, the relative humidity was in the range (55 \pm 5) % R.H. and the liquid depth above the ear reference points was above 15 cm in all the cases. It is seen that the system is operating within its specification, as the results are within acceptable tolerance of the reference values.



Date of Issue : 2011-10-05 Page : 10 / 56




Fig b. The microwave circuit arrangement used for SAR system verification

- A. Agilent Model E4421B Signal Generator
- B. EMPOWER Model 2057-BBS3Q5KCK Amplifier
- C. Agilent Model E4419B Power Meter
- D. Agilent Model 9300H Power Sensor
- E. Agilent Model 777D/778D Dual directional coupling
- F. Reference dipole Antenna



Photo of the dipole Antenna

System Validation Results

Validation Kit	Tissue	Target SAR 1 g from Calibration Certificate (1 W)	Measured SAR 1 g (1 W)	Deviation (%)	Date	Liquid Temp. (°C)
D2450V2 S/N: 734	2450 MHz Body	53.5 W/kg	53.6 W/kg	0.19	2011-10-04	21.9

Table 1. Results system validation



Date of Issue : 2011-10-05 Page : 11 / 56

1.11 Tissue Simulant Fluid for the Frequency Band

The dielectric properties for this simulant fluid were measured by using the Agilent Model 85070D Dielectric Probe (rates frequence band 200 MHz to 20 GHz) in conjunction with Agilent E5070B Network Analyzer(300 KHz - 3 GHz) by using a procedure detailed in Section V.

	Tissue		Dielectric Parameters			
f (MHz)	type	Limits / Measured	Permittivity	Conductivity	Simulated Tissue Temp()	
	Body	Measured, 2011-10-04	50.7	2.01	21.9	
2450		Recommended Limits	52.7	1.95	21.0 ~ 23.0	
		Deviation(%)	-3.80	3.08	-	



Date of Issue : 2011-10-05 Page : 12 / 56

The composition of the tissue simulating liquid

The following tissue formulations are provided for reference only as some of the parameters have not been thoroughly verified. The composition of ingredients may be modified accordingly to achieve the desired target tissue parameters required for routine SAR evaluation.

Ingredients	Freque	Frequency (MHz)								
(% by weight)	450		835		915		1900		2450	
Tissue Type	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body
Water	38.56	51.16	41.45	52.4	41.05	56.0	54.9	40.4	62.7	73.2
Salt (NaCl)	3.95	1.49	1.45	1.4	1.35	0.76	0.18	0.5	0.5	0.04
Sugar	56.32	46.78	56.0	45.0	56.5	41.76	0.0	58.0	0.0	0.0
HEC	0.98	0.52	1.0	1.0	1.0	1.21	0.0	1.0	0.0	0.0
Bactericide	0.19	0.05	0.1	0.1	0.1	0.27	0.0	0.1	0.0	0.0
Triton X-100	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	36.8	0.0
DGBE	0.0	0.0	0.0	0.0	0.0	0.0	44.92	0.0	0.0	26.7
Dielectric Constant	43.42	58.0	42.54	56.1	42.0	56.8	39.9	54.0	39.8	52.5
Conductivity (S/m)	0.85	0.83	0.91	0.95	1.0	1.07	1.42	1.45	1.88	1.78

Salt: 99 $^{+}$ % Pure Sodium Chloride Sugar: 98 $^{+}$ % Pure Sucrose Water: De-ionized, 16 M Ω^{+} resistivity HEC: Hydroxyethyl Cellulose

DGBE: 99 ⁺% Di(ethylene glycol) butyl ether, [2-(2-butoxyethoxy)ethanol]

Triton X-100 (ultra pure): Polyethylene glycol mono [4-(1,1, 3, 3-tetramethylbutyl)phenyl]ether

1.12 Test Standards and Limits

According to FCC 47CFR §2.1093(d) The limits to be used for evaluation are based generally on criteria published by the American National Standards Institute (ANSI) for localized specific absorption rate ("SAR") in Section 4.2 of "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz," ANSI/IEEE C95.3–2003, Copyright 2003 by the Institute of Electrical and Electronics Engineers, Inc., New York, New York 10017. These criteria for SAR evaluation are similar to those recommended by the National Council on Radiation Protection and Measurements (NCRP) in "Biological Effects and Exposure Criteria for Radio frequency Electromagnetic Fields," NCRP Report No. 86, Section 17.4.5. Copyright NCRP, 1986, Bethesda, Maryland 20814. SAR is a measure of the rate of energy absorption due to exposure to an RF transmitting source. SAR values have been related to threshold levels for potential biological hazards. The criteria to be used are specified in paragraphs (d)(1) and (d)(2) of this section and shall apply for portable devices transmitting in the frequency range from 100 kHz to 6 GHz. Portable devices that transmit at frequencies above 6 GHz are to be evaluated in terms of the MPE limits specified in § 1.1310 of this chapter. Measurements and calculations to demonstrate compliance with MPE field strength or power density limits for devices operating above 6 GHz should be made at a minimum distance of 5 cm from the radiating source.

(1) Limits for Occupational/Controlled exposure: 0.4 W/kg as averaged over the whole-body and spatial



Date of Issue : 2011-10-05 Page : 13 / 56

peak SAR not exceeding 8 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 20 W/kg, as averaged over an 10 grams of tissue (defined as a tissue volume in the shape of a cube). Occupational/Controlled limits apply when persons are exposed as a consequence of their employment provided these persons are fully aware of and exercise control over their exposure. Awareness of exposure can be accomplished by use of warning labels or by specific training or education through appropriate means, such as an RF safety program in a work environment.

(2) Limits for General Population/Uncontrolled exposure: 0.08 W/kg as averaged over the whole-body and spatial peak SAR not exceeding 1.6 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 4 W/kg, as averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube). General Population/Uncontrolled limits apply when the general public may be exposed, or when persons that are exposed as a consequence of their employment may not be fully aware of the potential for exposure or do not exercise control over their exposure. Warning labels placed on consumer devices such as cellular telephones will not be sufficient reason to allow these devices to be evaluated subject to limits for occupational/controlled exposure in paragraph (d)(1) of this section. (Table .4)

Human Exposure	Uncontrolled Environment General Population	Controlled Environment Occupational
Partial Peak SAR (Partial)	1.60 m W/g	8.00 m W/g
Partial Average SAR (Whole Body)	0.08 m W/g	0.40 m W/g
Partial Peak SAR (Hands/Feet/Ankle/Wrist)	4.00 m W/g	20.00 m W/g

Table .4 RF exposure limits

1.13 Justification for Extended SAR Dipole Calibrations

Usage of SAR dipoles calibrated less than 2 years ago but more than 1 year ago were confirmed in maintaining return loss (< -20 dB, within 20 % of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB publication 450824:

D2450V2_Body (SN: 734)					
Measurement Date	Return Loss (dB)	$\Delta\%$	Impedence (Ω)	$\Delta\Omega$	
2010-05-27	-27.1	-	49.8	-	
2011-06-07	-26.2	-3.32	48.3	-3.01	



Date of Issue : 2011-10-05
Page : 14 / 56

2. Instruments List

Maunfacturer	Device	Туре	Serial Number	Due date of Calibration
Stäubli	Robot	RX90BL	F03/5W05A1/A/01	N/A
Schmid& Partner Engineering AG	Dosimetric E-Field Probe	ET3DV6	1782	April 13, 2012
Schmid& Partner Engineering AG	2450 MHz System Validation Dipole	D2450V2	734	May 27, 2012
Schmid& Partner Engineering AG	Data acquisition Electronics	DAE3	567	January 27, 2012
Schmid& Partner Engineering AG	Software	DASY 4 V4.7	-	N/A
Schmid& Partner Engineering AG	Phantom	SAM Phantom V4.0	TP-1645 TP-1300	N/A
Agilent	Network Analyzer	E5070B	MY42100282	March 31, 2012
Agilent	Dielectric Probe Kit	85070D	2184	N/A
Agilent	Power Meter	E4419B	GB43311126	July 04, 2012
Agilent	Power Sensor	Е9300Н	MY41495307 MY41495308	September 29, 2012 September 29, 2012
Agilent	Signal Generator	E4421B	MY43350132	July 05, 2012
Empower RF Systems	Power Amplifier	2001- BBS3Q7ECK	1032 D/C 0336	April 01, 2012
Agilent	Dual Directional	777D	50128	July 10, 2012
	Coupler	778D	50454	July 06, 2012
Microlab	LP Filter	LA-15N LA-30N	N/A	September 29, 2012



Date of Issue : 2011-10-05 Page : 15 / 56

3.Summary of Results

3.1 FCC Power Measurement Procedures

Power measurements were performed using a power meter under digital average mode.

In order to verify that the device was tested and maintained at full power, this was configured with the base station simulator. The SAR measurement Software calculates a reference point at the start and end of the test to check for power drifts. If conducted power deviations of more than 5 % occurred, the tests were repeated.

3.2 RF Conducted Average Power

Bluetooth

Channel	Frequency (MHz)	Average Power (dBm)		
Chamiei		GFSK	8DPSK	
Low	2402	-3.90	-5.20	
Middle	2441	-3.84	-4.90	
High	2480	-3.40	-4.70	

WLAN

802.118) Mode	Rated	Measured Average Power																			
Frequency (MHz)	Frequency (MHz) Channel No.		(dBm)																			
		1	14.88																			
2412	1	2	14.91																			
2412	1	5.5	15.01																			
		11	14.89																			
	6	6	6	1	14.70																	
2437				6	(6	6	6	((6	6	6	6	6	6	6	6	2	14.76
2437					5.5	14.62																
		11	14.68																			
		1	14.07																			
2462	11	2	13.96																			
2402	11	5.5	13.91																			
		11	13.99																			



Date of Issue : 2011-10-05 Page : 16 / 56

802.11g	g Mode	Rated	Measured Power
Frequency (MHz)	Channel No.	(Mbps)	(dBm)
		6	12.21
		9	12.17
		12	12.21
2412	1	18	12.17
2412	1	24	12.20
		36	12.23
		48	12.13
		54	12.40
		6	11.71
	6	9	11.73
		12	11.67
2437		18	11.65
2437		24	11.68
		36	11.73
		48	11.67
		54	11.73
		6	11.95
		9	12.04
		12	11.96
2462	11	18	11.95
2702	11	24	11.96
		36	11.98
		48	12.04
		54	12.05

802.11r	Mode	Rated	Measured Power
Frequency (MHz)	Channel No.	(Mbps)	(dBm)
		MCS0	12.12
		MCS1	12.13
		MCS2	12.14
2412	1	MCS3	12.07
2412	1	MCS4	12.11
		MCS5	12.07
		MCS6	12.14
		MCS7	12.15
	6	MCS0	11.71
		MCS1	11.72
		MCS2	11.69
2437		MCS3	11.69
2437		MCS4	11.70
		MCS5	11.73
		MCS6	11.73
		MCS7	11.73
		MCS0	12.06
		MCS1	12.05
		MCS2	12.04
2462	11	MCS3	12.05
2702	11	MCS4	12.03
		MCS5	12.06
		MCS6	12.09
		MCS7	12.10



Date of Issue : 2011-10-05 Page : 17 / 56

3.3 SAR Test Configuration

Tablet Testing for SAR

Devices are to be setup according to KDB 447498 requirements and are configured with maximum output power during SAR assessment for a worst-case SAR evaluation.

(The overall diagonal dimension is over 20 cm. Please see the distance on 18 page of this report)

SAR Testing for Tablet per KDB 447498 & KDB 616217

Per KDB 447498 4) b) i), the bottom face is required to be tested touching the flat phantom.

Per KDB 447498 4) b) ii) (1), SAR is required for each antenna located within 5 cm of the tablet edge closet to the user for the applicable display orientation. For antenna(s) located ≥ 5 cm from this edge, the test reduction and exclusion procedures for laptop computers in KDB 616217 are applied.

** The RF output power of Bluetooth was 0.46 mW, which is less than the threshold power (60/f). Therefore, SAR is not required for the Bluetooth transmitter per KDB 447498 and also simultaneous transmission SAR evaluation is not required because two transmitters can't transmit simultaneously.




Date of Issue : 2011-10-05 Page : 18 / 56

According to KDB 616217, the WLAN antenna is required to be tested for SAR at the back, top and right edges of the device.

Mode	Front	Back	Left	Right	Тор	Bottom
WLAN	X	О	X	О	О	X

<The Distance information of Antenna to Edges of EUT>

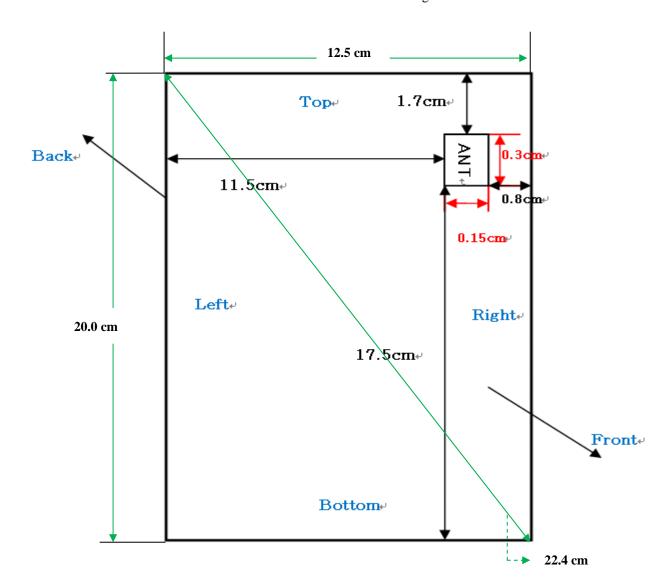



Date of Issue : 2011-10-05 Page : 19 / 56

3.4 SAR Data Summary

WLAN Body SAR

Ambient Temperature (°C)	21.9
Liquid Temperature (°C)	21.9
Date	2011-10-04

T-4M-1-	EUT	Traffic (Channel	Power	1 g SAR	1 g SAR
Test Mode	Position	Frequency (MHz)	Channel Drift(dB)		(W/kg)	Limits (W/kg)
11b	Back	2412	1	0.019	0.965	
11b	Back	2437	6	0.088	1.11	
11b	Back	2462	11	-0.036	1.13	1.6
11b	Right	2462	11	-0.135	0.533	
11b	Тор	2462	11	-0.096	0.249	

<Note>

- 1. The test data reported are the worst-case SAR value with the position set in a typical configuration.
- 2. According to KDB 447498, the back side is required to be tested touching the flat phantom.
- 3. According to KDB 616217, SAR testing applies for the tablet edges with antenna located within 5 cm of each tablet edge closest to the user.
- 2. All modes of operation were investigated, and worst-case results are reported.
- 3. Battery is fully charged for all readings and the standard batteries are the only options.
- 4. Liquid tissue depth was at least 15 cm.
- 5. The distance from EUT to flat phantom for testing Body SAR is 0 mm.
- 6. SAR is not required for 802.11g channels when the maximum average output power is less than 1/4 dB higher than that measured on the corresponding 802.11b channels. <KDB 248227>
- 7. Left and Bottom position was not tested since the antenna distance to edge was greater than 5 cm per KDB616217.



Date of Issue : 2011-10-05 Page : 20 / 56

Appendix

List

Appendix A	DASY4 Report (Plots of the SAR Measurements)	- WLAN Test
Appendix B	Uncertainty Analysis	
Appendix C	Calibration Certificate	- PROBE - DAE3 - DIPOLE



Date of Issue : 2011-10-05
Page : 21/56

Appendix A

Test Plot - DASY4 Report



Date of Issue : 2011-10-05 Page : 22 / 56

2450 MHz Validation Test Body

Date: 2011-10-04

Test Laboratory: SGS Korea (Gunpo Laboratory) File Name: <u>Validation 2450 MHz Body.da4</u>

Input Power: 250 mW

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:734

Program Name: Validation 2450 MHz_Body

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2450 MHz; $\sigma = 2.01 \text{ mho/m}$; $\varepsilon_r = 50.7$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(3.94, 3.94, 3.94); Calibrated: 2011-04-14

- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2011-01-27
- Phantom: SAM with CRP 2011(left); Type: SAM; Serial: TP-1645
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186


Validation 2450 MHz/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 16.6 mW/g

Validation 2450 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 79.2 V/m; Power Drift = -0.005 dB

Peak SAR (extrapolated) = 33.2 W/kg


SAR(1 g) = 13.4 mW/g; SAR(10 g) = 6.01 mW/g Maximum value of SAR (measured) = 14.5 mW/g

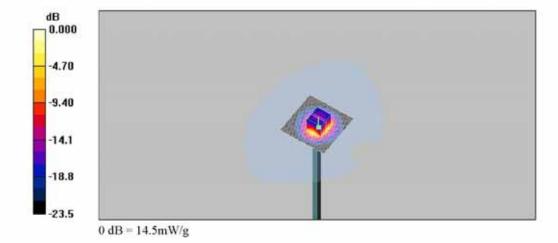



Date of Issue : 2011-10-05 Page : 23 / 56

Z Scan

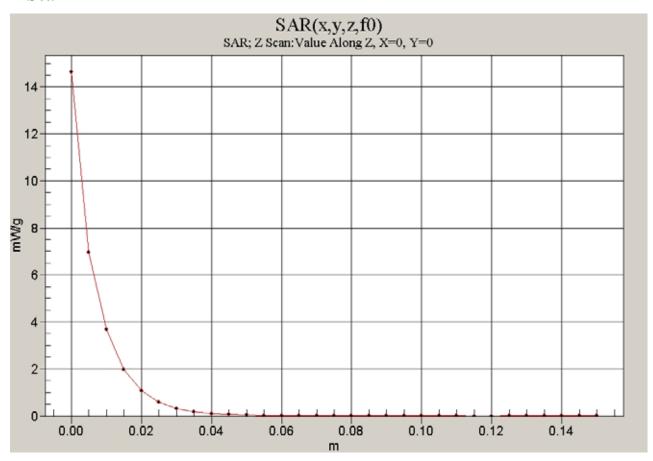



Date of Issue: 2011-10-05 Page: 24 / 56

WLAN Body SAR Test

Date: 2011-10-04

Test Laboratory: SGS Korea (Gunpo Laboratory)

File Name: WLAN Body.da4

DUT: AMD120; Type: Tablet Base; Serial: 0228433

Program Name: WLAN_Body

Communication System: WLAN; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2412 MHz; $\sigma = 1.96$ mho/m; $\varepsilon_r = 50.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(3.94, 3.94, 3.94); Calibrated: 2011-04-14

- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2011-01-27
- Phantom: SAM with CRP 2011(left); Type: SAM; Serial: TP-1645
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

WLAN 11b Back Low 0mm/Area Scan (81x101x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.693 mW/g

WLAN 11b_Back_Low_0mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 4.94 V/m; Power Drift = 0.019 dB

Peak SAR (extrapolated) = 3.42 W/kg

SAR(1 g) = 0.965 mW/g; SAR(10 g) = 0.353 mW/gMaximum value of SAR (measured) = 1.08 mW/g


WLAN_11b_Back_Low_0mm/Zoom Scan (7x7x7)/Cube 1: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 4.94 V/m; Power Drift = 0.019 dB

Peak SAR (extrapolated) = 3.47 W/kg

SAR(1 g) = 0.871 mW/g; SAR(10 g) = 0.334 mW/g

Maximum value of SAR (measured) = 1.02 mW/g

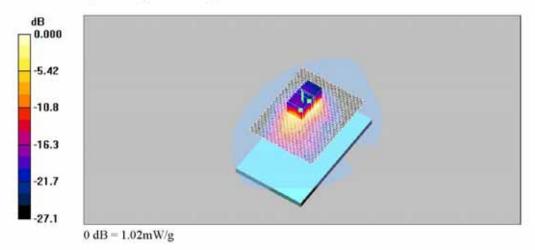



Date of Issue : 2011-10-05 Page : 25 / 56

Date: 2011-10-04

Test Laboratory: SGS Korea (Gunpo Laboratory)

File Name: WLAN Body.da4

DUT: AMD120; Type: Tablet_Base; Serial: 0228433

Program Name: WLAN_Body

Communication System: WLAN; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2437 MHz; $\sigma = 1.99$ mho/m; $\varepsilon_r = 50.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(3.94, 3.94, 3.94); Calibrated: 2011-04-14

- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2011-01-27
- Phantom: SAM with CRP 2011(left); Type: SAM; Serial: TP-1645
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

WLAN_11b_Back_Mid_0mm/Area Scan (81x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.726 mW/g


WLAN_11b_Back_Mid_0mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 4.95 V/m; Power Drift = 0.088 dB

Peak SAR (extrapolated) = 4.24 W/kg

SAR(1 g) = 1.11 mW/g; SAR(10 g) = 0.419 mW/g

Maximum value of SAR (measured) = 1.24 mW/g

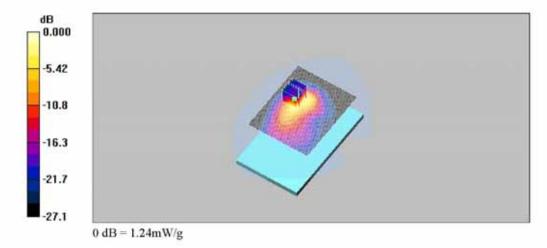



Date of Issue : 2011-10-05 Page : 26 / 56

Date: 2011-10-04

Test Laboratory: SGS Korea (Gunpo Laboratory)

File Name: WLAN Body.da4

DUT: AMD120; Type: Tablet_Base; Serial: 0228433

Program Name: WLAN_Body

Communication System: WLAN; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2462 MHz; $\sigma = 2.03$ mho/m; $\varepsilon_r = 50.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(3.94, 3.94, 3.94); Calibrated: 2011-04-14

- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2011-01-27
- Phantom: SAM with CRP 2011(left); Type: SAM; Serial: TP-1645
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186


WLAN_11b_Back_High_0mm/Area Scan (71x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 1.14 mW/g

WLAN_11b_Back_High_0mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 4.42 V/m; Power Drift = -0.036 dB

Peak SAR (extrapolated) = 4.30 W/kg

SAR(1 g) = 1.13 mW/g; SAR(10 g) = 0.428 mW/g


Maximum value of SAR (measured) = 1.22 mW/g

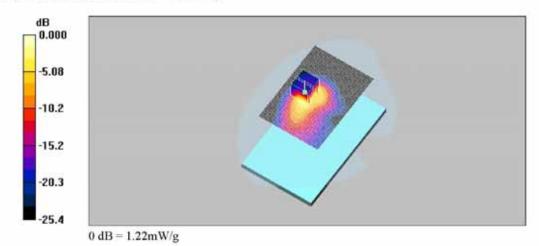



Date of Issue : 2011-10-05 Page : 27/56

Z Scan

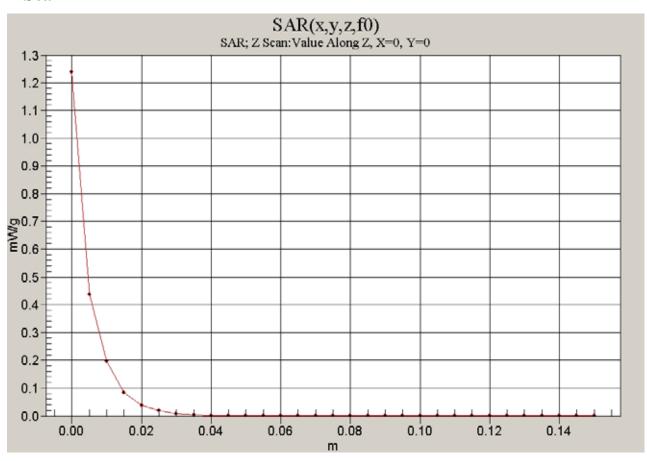



Date of Issue : 2011-10-05 Page : 28 / 56

Date: 2011-10-04

Test Laboratory: SGS Korea (Gunpo Laboratory) File Name: WLAN Body Side Edge.da4

DUT: AMD120; Type: Tablet_Side; Serial: 0228433

Program Name: WLAN_Body

Communication System: WLAN; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2462 MHz; $\sigma = 2.03$ mho/m; $\varepsilon_r = 50.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1782; ConvF(3.94, 3.94, 3.94); Calibrated: 2011-04-14

- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2011-01-27
- Phantom: SAM with CRP 2011(left); Type: SAM; Serial: TP-1645
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

WLAN_11b_Right_Side_High_0mm/Area Scan (71x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.583 mW/g


WLAN_11b_Right_Side_High_0mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm,

Reference Value = 14.8 V/m; Power Drift = -0.135 dB

Peak SAR (extrapolated) = 1.48 W/kg

SAR(1 g) = 0.533 mW/g; SAR(10 g) = 0.230 mW/g

Maximum value of SAR (measured) = 0.596 mW/g

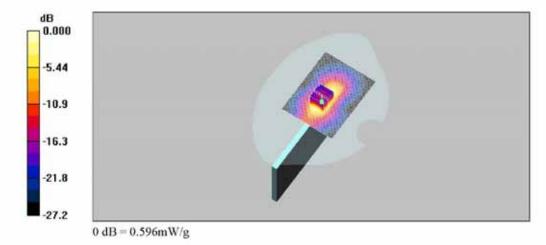



Date of Issue : 2011-10-05 Page : 29 / 56

Date: 2011-10-04

Test Laboratory: SGS Korea (Gunpo Laboratory)

File Name: WLAN Body Top.da4

DUT: AMD120; Type: Tablet_Top; Serial: 0228433

Program Name: WLAN_Body

Communication System: WLAN; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2462 MHz; $\sigma = 2.03$ mho/m; $\varepsilon_r = 50.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY4 Configuration:


- Probe: ET3DV6 SN1782; ConvF(3.94, 3.94, 3.94); Calibrated: 2011-04-14
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2011-01-27
- Phantom: SAM with CRP_2011(left); Type: SAM; Serial: TP-1645
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

WLAN_11b_Top_High_0mm/Area Scan (71x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.245 mW/g

WLAN_11b_Top_High_0mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 10.2 V/m; Power Drift = -0.096 dB

Peak SAR (extrapolated) = 0.709 W/kg

SAR(1 g) = 0.249 mW/g; SAR(10 g) = 0.101 mW/gMaximum value of SAR (measured) = 0.268 mW/g

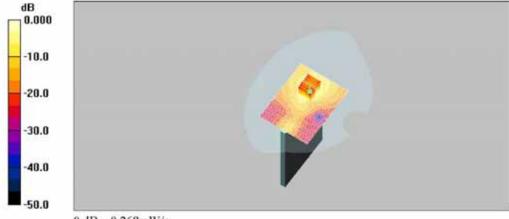

0~dB=0.268mW/g



Date of Issue : 2011-10-05 Page : 30 / 56

Appendix B

Uncertainty Analysis

а	b	С	d	e = f(d,k)	g	i = cxg/e	k
Uncertainty Component	Sectio n in P1528	Tol (%)	Prob . Dist.	Div.	Ci (1g)	1g ui (%)	Vi (Veff)
Probe calibration	E.2.1	6.3	N	1	1	6.30	
Axial isotropy	E.2.2	0.5	R	1.73	0.71	0.20	
hemispherical isotropy	E.2.2	2.6	R	1.73	0.71	1.06	
Boundary effect	E.2.3	0.8	R	1.73	1	0.46	
Linearity	E.2.4	0.6	R	1.73	1	0.35	
System detection limit	E.2.5	0.25	R	1.73	1	0.14	
Readout electronics	E.2.6	0.3	N	1	1	0.30	
Response time	E.2.7	0	R	1.73	1	0.00	
Integration time	E.2.8	2.6	R	1.73	1	1.50	
RF ambient Condition -Noise	E.6.1	3	R	1.73	1	1.73	
RF ambient Condition - reflections	E.6.1	3	R	1.73	1	1.73	
Probe positioning - mechanical tolerance	E.6.2	1.5	R	1.73	1	0.87	
Probe positioning - with respect to phantom	E.6.3	2.9	R	1.73	1	1.67	
Max. SAR evaluation	E.5.2	1	R	1.73	1	0.58	
Test sample positioning	E.4.2	2.3	N	1	1	2.30	9
Device holder uncertainty	E.4.1	3.6	N	1	1	3.60	
Output power variation - SAR drift measurement	6.62	5	R	1.73	1	2.89	
Phantom uncertainty (shape and thickness tolerances)	E.3.1	4	R	1.73	1	2.31	
Liquid conductivity - deviation from target values	E.3.2	5	R	1.73	0.64	1.85	
Liquid conductivity - measurement uncertainty	E.3.2	1.2	N	1	0.64	0.77	5
Liquid permittivity - deviation from target values	E.3.3	5	R	1.73	0.6	1.73	
Liquid permittivity - measurement uncertainty	E.3.3	1.1	N	1	0.6	0.66	5
Combined standard uncertainty				RSS		9.63	2754
Expanded uncertainty (95% CONFIDENCE INTERVAL)				K=2		19.27	



Appendix C

Calibration Certificate

- PROBE
- **DAE 3**
- 2450 MHz DIPOLE

Report File No.: F690501/RF-SAR001955-A1

Date of Issue : 2011-10-05
Page : 31 / 56



2011-10-05 Date of Issue: 32 / 56 Page:

- PROBE Calibration Certificate

Calibration Laboratory of Schmid & Partner Engineering AG eughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client SGS (Dymstec)

Certificate No: ET3-1782_Apr11

Accreditation No.: SCS 108

S

CALIBRATION CERTIFICATE

ET3DV6 - SN:1782 Object

Calibration procedure(s) QA CAL-01.v7, QA CAL-12.v6, QA CAL-23.v4, QA CAL-25.v3

Calibration procedure for dosimetric E-field probes

Calibration date: April 14, 2011

This calibration certificate documents the traceability to national standards, which realize the physical units of mea-The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID.	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	GB41293874 31-Mar-11 (No. 217-01372)	
Power sensor E4412A	MY41495277	31-Mar-11 (No. 217-01372)	Apr-12
Power sensor E4412A	MY41498087	31-Mar-11 (No. 217-01372)	Apr-12
Reference 3 dB Attenuator	SN: S5054 (3c)	29-Mar-11 (No. 217-01369)	Apr-12
Reference 20 dB Attenuator	SN: S5086 (20b)	29-Mar-11 (No. 217-01367)	Apr-12
Reference 30 dB Attenuator	SN: S5129 (30b)	29-Mar-11 (No. 217-01370)	Apr-12
Reference Probe ES3DV2	SN: 3013	29-Dec-10 (No. ES3-3013_Dec10)	Dec-11
DAE4	SN: 654	23-Apr-10 (No. DAE4-054_Apr10)	Apr-11
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-10)	In house check: Oct-11

Calibrated by: Jeton Kastrati Laboratory Technician Katja Pokovic Technical Manager Approved by: Issued: April 14, 2011 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: ET3-1782_Apr11

Page 1 of 11



Date of Issue : 2011-10-05 Page : 33 / 56

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kallbrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid NORMx,y,z sensitivity in free space ConvF sensitivity in TSL / NORMx,y,z diode compression point

CF crest factor (1/duty_cycle) of the RF signal A, B, C modulation dependent linearization parameters

Polarization φ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

- iEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- Techniques", December 2003
 b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization ⊕ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z are numerical linearization parameters in dB assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media.
- . VR: VR is the validity range of the calibration related to the average diode voltage or DAE voltage in mV.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom
 exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ET3-1782 Apr11

Page 2 of 11



Date of Issue : 2011-10-05 Page : 34 / 56

ET3DV6 - SN:1782 April 14, 2011

Probe ET3DV6

SN:1782

Manufactured: April 15, 2003 Calibrated: April 14, 2011

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: ET3-1782_Apr11

Page 3 of 11



Date of Issue: 2011-10-05 Page: 35 / 56

ET3DV6-SN:1782 April 14, 2011

DASY/EASY - Parameters of Probe: ET3DV6 - SN:1782

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (µV/(V/m) ²) ^A	2.07	1.66	1.92	± 10.1 %
DCP (mV) ⁸	96.4	96.6	97.6	

Modulation Calibration Parameters

UID	Communication System Name	PAR		A dB	B dB	C dB	VR mV	Unc ^E (k=2)
10000	CW 0.00	CW 0.00 X	X	0.00	0.00	1.00	111.1	±1.9 %
		1	Y	0.00	0.00	1.00	141.0	
			Z	0.00	0.00	1.00	145.1	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).
^B Numerical linearization parameter: uncertainty not required.
^B Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



Date of Issue: 2011-10-05 Page: 36 / 56

ET3DV6- SN:1782 April 14, 2011

DASY/EASY - Parameters of Probe: ET3DV6 - SN:1782

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
450	43.5	0.87	6.89	6.89	6.89	0.21	2.29	± 13.4 %
835	41.5	0.90	6.22	6:22	6.22	0.88	1.63	± 12.0 %
1750	40,1	1.37	5.14	5.14	5.14	0.57	2.53	± 12.0 %
1900	40.0	1.40	4.95	4.95	4.95	0.58	2.54	± 12.0 %
2450	39.2	1.80	4.37	4.37	4.37	0.80	1.93	± 12.0 %

Certificate No: ET3-1782_Apr11

Page 5 of 11

⁶ Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), etse it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.
⁷ At frequencies below 3 GHz, the validity of tissue parameters (e and e) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. Aft requencies above 3 GHz, the validity of tissue parameters (e and e) is restricted to ± 5%. The uncertainty is the RSS of the CowF uncertainty for indicated target tissue parameters.



Date of Issue: 2011-10-05 Page: 37 / 56

ET3DV6- SN:1782 April 14, 2011

DASY/EASY - Parameters of Probe: ET3DV6- SN:1782

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity	Conductivity (S/m)	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
450	56.7	0.94	7.49	7.49	7.49	0.16	2.34	± 13.4 %
835	55.2	0.97	6.03	6.03	6.03	0.85	1.72	± 12.0 %
1750	53.4	1.49	4.54	4.54	4.54	0.64	2.70	± 12.0 %
1900	53.3	1,52	4.34	4.34	4.34	0.63	2.57	± 12.0 %
2450	52.7	1.95	3.94	3.94	3.94	0.99	1.21	± 12.0 %

Certificate No: ET3-1782_Apr11

Page 6 of 11

Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


At Inquencies below 3 GHz, the validity of tissue parameters (s and a) can be relaxed to ± 10% if fliquid compensation formula is applied to measured SAF values. Aft requencies above 3 GHz, the validity of tissue parameters (s and a) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.



Date of Issue: 2011-10-05 Page: 38 / 56

ET3DV6-SN:1782 April 14, 2011

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

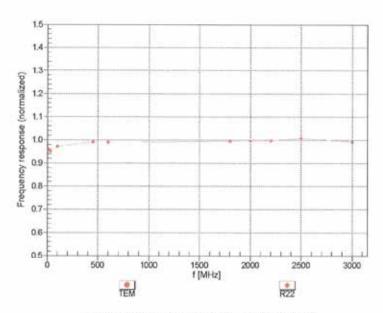

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)





Date of Issue: 2011-10-05 Page: 39 / 56

ET3DV6-- SN:1782 April 14, 2011

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$



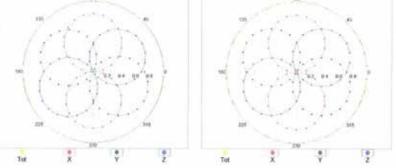

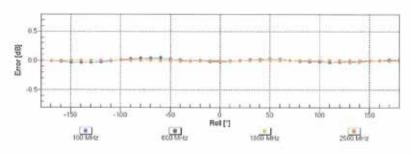


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)




Date of Issue : 2011-10-05 Page : 40 / 56

ET3DV6- SN:1782 April 14, 2011

Dynamic Range f(SAR_{head}) (TEM cell , f = 900 MHz)

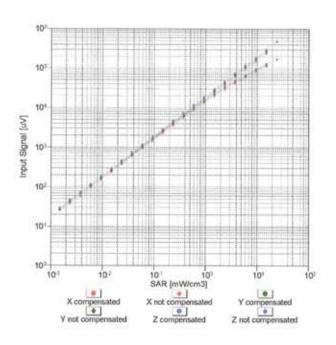

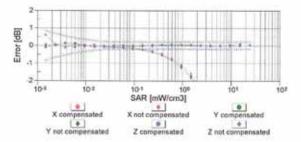


Uncertainty of Linearity Assessment: ± 0.6% (k≈2)




Date of Issue : 2011-10-05 Page : 41/56


ET3DV6-SN:1782 April 14, 2011

Conversion Factor Assessment

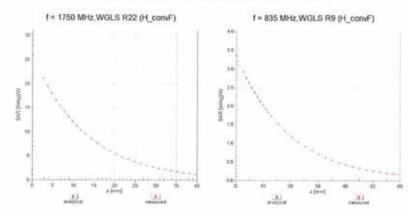

Deviation from Isotropy in Liquid Error (o, 9), f = 900 MHz





Certificate No: ET3-1782_Apr11

Page 10 of 11



Date of Issue : 2011-10-05 Page : 42 / 56

ET3DV6- SN:1782 April 14, 2011

DASY/EASY - Parameters of Probe: ET3DV6 - SN:1782

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (*)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	6.8 mm
Probe Tip to Sensor X Calibration Point	2.7 mm
Probe Tip to Sensor Y Calibration Point	2.7 mm
Probe Tip to Sensor Z Calibration Point	2.7 mm
Recommended Measurement Distance from Surface	4 mm



2011-10-05 Date of Issue: 43 / 56 Page:

-DAE 3 Calibration Certificate

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

S

C

CALIBRATION (CERTIFICATE		
Object	DAE3 - SD 000 D03 AA - SN: 567		
Calibration procedure(s)	QA CAL-06.v22 Calibration procedure for the data acquisition electronics (DAE)		
Calibration date:	January 27, 2011		
Calibration Equipment used (M&		facility: environment temperature (22 ± Call Date (Certificate No.)	
Calibration Equipment used (M& Primary Standards	FE critical for calibration)	facility: environment temperature (22 ± Cal Date (Certificate No.) 28-Sep-10 (No:10376)	3)°C and humidity < 70%. Scheduled Calibration Sep-11
alitization Equipment used (M&T imary Standards etituley Multimeter Type 2001	FE critical for calibration)	Cal Date (Certificate No.)	Scheduled Calibration Sep-11
Calibration Equipment used (M&) Primary Standards Keithley Multimeter Type 2001 Secondary Standards	ID # SN: 0810278	Cal Date (Certificate No.) 28-Sep-10 (No:10376)	Scheduled Calibration
All calibrations have been conducted (M&) Calibration Equipment used (M&) Primary Standards Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	ID # SN: 0810278	Cal Date (Certificate No.) 28-Sep-10 (No:10376) Check Date (in house)	Scheduled Calibration Sep-11 Scheduled Check In house check: Jun-1
Calibration Equipment used (M&T Primary Standards Ceithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	ID # SN: 0810278 ID # SE UMS 006 AB 1004	Cal Date (Certificate No.) 28-Sep-10 (No:10376) Check Date (in house) 07-Jun-10 (in house check)	Scheduled Calibration Sep-11 Scheduled Check



Date of Issue: 2011-10-05 Page: 44/56

Calibration Laboratory of Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE data acquisition electronics

Connector angle information used in DASY system to align probe sensor X to the robot

coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
 - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
 - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
 - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - Power consumption: Typical value for information. Supply currents in various operating modes.



Date of Issue: 2011-10-05 45 / 56 Page:

DC Voltage Measurement A/D - Converter Resolution nominal

High Range: 1LSB = 6.1μ V, full range = -100...+300 mV Low Range: 1LSB = 61nV, full range = -1....+3mV DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	x	Y	Z
High Range	404.644 ± 0.1% (k=2)	404.400 ± 0.1% (k=2)	404.475 ± 0.1% (k=2)
Low Range	3.94940 ± 0.7% (k=2)	3.96974 ± 0.7% (k=2)	3.94828 ± 0.7% (k=2)

Connector Angle

Connector Angle to be used in DASY system	5.5°±1°



Date of Issue: 2011-10-05 Page: 46 / 56

Appendix

1. DC Voltage Linearity

Reading (µV)	Difference (µV)	Error (%)
200011.1	0.86	0.00
20005.53	5.63	0.03
-19994.55	6.05	-0.03
200012.0	3.19	0.00
19998.16	-0.94	-0.00
-19999.31	0.89	-0.00
200007.6	-0.57	-0.00
20000.62	1.02	0.01
-19997.10	3.20	-0.02
	200011.1 20005.53 -19994.55 200012.0 19998.16 -19999.31 200007.6 20000.62	200011.1 0.86 20005.53 5.63 -19994.55 6.05 200012.0 3.19 19998.16 -0.94 -19999.31 0.89 200007.6 -0.57 20000.62 1.02

Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	1999.6	-0.43	-0.02
Channel X + Input	200.86	0.86	0.43
Channel X - Input	-198.93	1,07	-0.54
Channel Y + Input	2000.2	0.40	0.02
Channel Y + Input	200.07	0.07	0.03
Channel Y - Input	-199.81	0.09	-0.05
Channel Z + Input	1999.8	-0.29	-0.01
Channel Z + Input	199.45	-0.75	-0.38
Channel Z - Input	-200.35	-0.25	0.12

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring tir

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	3.83	1,88
	- 200	0.20	+2.32
Channel Y	200	0.69	-0.01
	- 200	-1.13	-1.19
Channel Z	200	4.39	4.66
	- 200	-6.15	-6.31

3. Channel separation DASY measurement parar

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200		2.13	-0.21
Channel Y	200	3.01	12	3.24
Channel Z	200	1.69	-1.11	



2011-10-05 Date of Issue:

47 / 56 Page:

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16333	16454
Channel Y	16169	16436
Channel Z	15951	16115

Input Offset Measurement
 DASY measurement parameters; Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	-0.23	-1.40	0.68	0.42
Channel Y	-0.84	-2.05	0.49	0.41
Channel Z	-0.76	-1.62	0.54	0.38

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9



Date of Issue: 2011-10-05 Page: 48 / 56

- 2450 MHz Dipole Calibration Certificate

Calibration Laboratory of Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

SGS (Dymstec)

Accreditation No.: SCS 108

C

Certificate No: D2450V2-734 May10

Object	D2450V2 - SN: 7	34	
Calibration procedure(s)	QA CAL-05.v7 Calibration proce	dure for dipole validation kits	
Calibration date:	May 27, 2010		
All calibrations have been condu	cted in the closed laborator	robability are given on the following pages a ry facility: environment temperature (22 \pm 3) $^{\prime}$	C and humidity < 70%.
All calibrations have been condu Calibration Equipment used (M&	cted in the closed laborator	ry facility: environment temperature (22 ± 3)	
All calibrations have been condu Calibration Equipment used (M& Primary Standards	cted in the closed laborator TE critical for calibration)		C and humidity < 70%. Scheduled Calibration Oct-10
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A	cted in the closed laborator TE critical for calibration)	ry facility; environment temperature (22 ± 3) ⁴ Cal Date (Certificate No.)	Scheduled Calibration
All calibrations have been conductalibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	TE critical for calibration) ID # GB37480704	ry facility: environment temperature (22 ± 3) ⁴ Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086)	Scheduled Calibration Oct-10
All calibrations have been condu- Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 9481A Reference 20 dB Attenuator Type-N mismatch combination	TE critical for calibration) ID # GB37480704 US37292783	ry facility: environment temperature (22 ± 3) ⁴ Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086)	Scheduled Calibration Oct-10 Oct-10
All calibrations have been conducted (M& Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3	Cited in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3205	Cal Date (Certificate No.) 08-Oct-09 (No. 217-01086) 08-Oct-09 (No. 217-01086) 30-Mar-10 (No. 217-01158) 30-Mar-10 (No. 217-01162) 30-Apr-10 (No. ES3-3205_Apr10)	Scheduled Calibration Oct-10 Oct-10 Mar-11
All calibrations have been conducted (M& Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3	TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327	cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 30-Mar-10 (No. 217-01158) 30-Mar-10 (No. 217-01152)	Scheduled Calibration Oct-10 Oct-10 Mar-11 Mar-11
All calibrations have been conducted (M& Calibration Equipment used (M& Primary Standards - Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4	Cited in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3205	Cal Date (Certificate No.) 08-Oct-09 (No. 217-01086) 08-Oct-09 (No. 217-01086) 30-Mar-10 (No. 217-01158) 30-Mar-10 (No. 217-01162) 30-Apr-10 (No. 253-3205_Apr10) 02-Mar-10 (No. DAE4-601_Mar10)	Scheduled Calibration Oct-10 Oct-10 Mar-11 Mar-11 Apr-11 Mar-11
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 9481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards	TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3205 SN: 601	Cal Date (Certificate No.) 08-Oct-09 (No. 217-01086) 08-Oct-09 (No. 217-01086) 30-Mar-10 (No. 217-01158) 30-Mar-10 (No. 217-01162) 30-Apr-10 (No. ES3-3205_Apr10)	Scheduled Calibration Oct-10 Oct-10 Mar-11 Mar-11 Apr-11
All calibrations have been conducted (M& Calibration Equipment used (M& Primary Standards) Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A	TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3205 SN: 601	Cal Date (Certificate No.) 08-Oct-09 (No. 217-01086) 08-Oct-09 (No. 217-01086) 30-Mar-10 (No. 217-01168) 30-Mar-10 (No. 217-01162) 30-Apr-10 (No. ES3-3205_Apr10) 02-Mar-10 (No. DAE4-601_Mar10) Check Date (in house)	Scheduled Calibration Oct-10 Oct-10 Mar-11 Mar-11 Apr-11 Mar-11 Scheduled Check
All calibrations have been condu- Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 9481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3205 SN: 601 ID # MY41092317	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 30-Mar-10 (No. 217-01158) 30-Mar-10 (No. 217-01162) 30-Apr-10 (No. ES3-3205_Apr10) 02-Mar-10 (No. DAE4-601_Mar10) Check Date (in house)	Scheduled Calibration Oct-10 Oct-10 Mar-11 Mar-11 Apr-11 Mar-11 Scheduled Check In house check: Oct-11
All calibrations have been condu- Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 9481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 9481A RF generator R&S SMT-06	Cited in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3205 SN: 601 ID # MY41082317 100005	Cal Date (Certificate No.) 08-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 30-Mar-10 (No. 217-01168) 30-Mar-10 (No. 217-01162) 30-Apr-10 (No. ES3-3205_Apr10) 02-Mar-10 (No. DAE4-601_Mar10) Check Date (In house) 18-Oct-02 (in house check Oct-09) 4-Aug-99 (in house check Oct-09)	Scheduled Calibration Oct-10 Oct-10 Mar-11 Mar-11 Apr-11 Mar-11 Scheduled Check In house check: Oct-11 In house check: Oct-11
	Cited in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005 US37390585 S4206	Cal Date (Certificate No.) 08-Oct-09 (No. 217-01086) 08-Oct-09 (No. 217-01086) 30-Mar-10 (No. 217-01158) 30-Mar-10 (No. 217-01162) 30-Apr-10 (No. ES3-3205_Apr10) 02-Mar-10 (No. DAE4-601_Mar10) Check Date (in house) 18-Oct-02 (in house check Oct-09) 4-Aug-99 (in house check Oct-09)	Scheduled Calibration Oct-10 Oct-10 Mar-11 Mar-11 Apr-11 Mar-11 Scheduled Check In house check: Oct-11 In house check: Oct-10



Date of Issue:

2011-10-05

Page:

49 / 56

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage

C Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL

tissue simulating liquid

ConvF N/A

sensitivity in TSL / NORM x,y,z

not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- . Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.



Date of Issue:

2011-10-05

Page:

50 / 56

Measurement Conditions

Extrapolation Advanced Extrapolation	
Phantom Modular Flat Phantom V4.9	
Distance Dipole Center - TSL 10 mm	with Spacer
Zoom Scan Resolution dx, dy, dz = 5 mm	
Frequency 2450 MHz ± 1 MHz	

Head TSL parameters
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.0 ± 6 %	1.76 mho/m ± 6 %
Head TSL temperature during test	(21.5 ± 0.2) °C		****

SAR result with Head TSL

SAR averaged over 1 cm3 (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	12.8 mW / g
SAR normalized	normalized to 1W	51.2 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	51.7 mW /g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.03 mW / g
SAR normalized	normalized to 1W	24.1 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	24.2 mW /g ± 16.5 % (k=2)



Date of Issue:

2011-10-05

Page:

51/56

Body TSL parameters
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.6 ± 6 %	1.97 mho/m ± 6 %
Body TSL temperature during test	(21.8 ± 0.2) °C	****	****

SAR result with Body TSL

SAR averaged over 1 cm3 (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.4 mW / g
SAR normalized	normalized to 1W	53.6 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	53.5 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.31 mW / g
SAR normalized	normalized to 1W	25.2 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	25.2 mW / g ± 16.5 % (k=2)

Certificate No: D2450V2-734_May10



Date of Issue : 2011-10-05 Page : 52 / 56

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.8 Ω + 3.2 jΩ	
Return Loss	- 26.4 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$49.8 \Omega + 4.4 j\Omega$	
Return Loss	- 27.1 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.153 ns
and all the state of the state	1.100110

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG	
Manufactured on	May 07, 2003	

Certificate No: D2450V2-734_May10

Page 5 of 9



Date of Issue : 2011-10-05 Page : 53 / 56

DASY5 Validation Report for Head TSL

Date/Time: 25.05.2010 14:48:31

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:734

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U11 BB

Medium parameters used: f = 2450 MHz; $\sigma = 1.76 \text{ mho/m}$; $\varepsilon_r = 39$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 30.04.2010

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 02.03.2010

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

Measurement SW: DASY5, V5.2 Build 162; SEMCAD X Version 14.0 Build 61

Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement


grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 101.2 V/m; Power Drift = 0.030 dB

Peak SAR (extrapolated) = 26.1 W/kg

SAR(1 g) = 12.8 mW/g; SAR(10 g) = 6.03 mW/g

Maximum value of SAR (measured) = 16.7 mW/g




0 dB = 16.7 mW/g

Certificate No: D2450V2-734_May10



Date of Issue : 2011-10-05 Page : 54 / 56

Impedance Measurement Plot for Head TSL

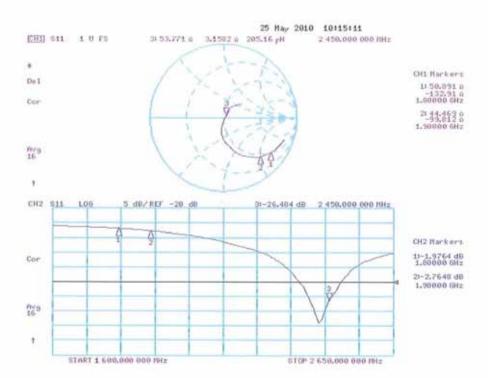



Date of Issue : 2011-10-05 Page : 55 / 56

DASY5 Validation Report for Body

Date/Time: 27.05.2010 10:14:45

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:734

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL U11 BB

Medium parameters used: f = 2450 MHz; $\sigma = 1.97 \text{ mho/m}$; $\varepsilon_r = 53.6$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.31, 4.31, 4.31); Calibrated: 30.04.2010

Sensor-Surface: 3mm (Mechanical Surface Detection)

· Electronics: DAE4 Sn601; Calibrated: 02.03.2010

Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002

Measurement SW: DASY5, V5.2 Build 162; SEMCAD X Version 14.0 Build 61

Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement


grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 96.7 V/m; Power Drift = -0.030 dB

Peak SAR (extrapolated) = 27.3 W/kg

SAR(1 g) = 13.4 mW/g; SAR(10 g) = 6.31 mW/g

Maximum value of SAR (measured) = 17.4 mW/g



0 dB = 17.4 mW/g

Certificate No: D2450V2-734_May10



Date of Issue : 2011-10-05 Page : 56 / 56

Impedance Measurement Plot for Body TSL

