



# Specific Absorption Rate (SAR) Test Report for MiTAC International Corp. on the PDA phone

# Report No.: FA742004-2-2-01Trade Name: MiTACModel Name: A702FCC ID: P4Q-MIOA702Date of Testing: May 28, 2007Date of Report: Jun. 04, 2007Date of Review: Jun. 04, 2007

- The test results refer exclusively to the presented test model / sample only.
- Without written approval of SPORTON International Inc., the test report shall not be reproduced except in full.
- Report Version: Rev. 01

# SPORTON International Inc.

6F, No.106, Sec. 1, Hsin Tai Wu Rd., Hsi Chih, Taipei Hsien, Taiwan, R.O.C.



# **Table of Contents**

		nent of Compliance	
2. A	dmini	istration Data	
	2.1	Testing Laboratory	2
	2.2	Detail of Applicant	2
	2.3	Detail of Manufacturer	2
	2.4	Application Detail	2
3. Se	cope.		
	3.1	Description of Device Under Test (DUT)	
	3.2	Product Photo	4
	3.3	Applied Standards:	5
	3.4	Device Category and SAR Limits	6
	3.5	Test Conditions	6
		3.5.1 Ambient Condition:	
		3.5.2 Test Configuration:	6
4. S	pecifi	ic Absorption Rate (ŠAR)	
	4.1	Introduction	
	4.2	SAR Definition	
5. S/	AR M	leasurement Setup	
	5.1	DASY4 E-Field Probe System	
		5.1.1 ET3DV6 E-Field Probe Specification	
		5.1.2 ET3DV6 E-Field Probe Calibration	10
	5.2	DATA Acquisition Electronics (DAE)	
	5.3	Robot	
	5.4	Measurement Server	
	5.5	SAM Twin Phantom	
	5.6	Data Storage and Evaluation	
		5.6.1 Data Storage	
		5.6.2 Data Evaluation	
	5.7	Test Equipment List	
6. Ti		Simulating Liquids	
		tainty Assessment	
		leasurement Evaluation	
	8.1	Purpose of System Performance check	
	8.2	System Setup	
	8.3	Validation Results	
9. D		ption for DUT Testing Position	
		surement Procedures	
	10.1		
	10.2	Scan Procedures	
		SAR Averaged Methods	
11.		Test Results	
	11.1		
	11.2		
	11.3		
	11.4		
	11.5		
	11.6		
12.		reypad Bown with Hoom Cup	

Appendix A – System Performance Check Data Appendix B – SAR Measurement Data Appendix C – Calibration Data



# 1. <u>Statement of Compliance</u>

The Specific Absorption Rate (SAR) maximum result found during testing for the **MiTAC International Corp. PDA phone MiTAC A702 are 0.03 W/Kg on the WLAN 2.4GHz head SAR and 0.025 W/Kg on the WLAN 2.4GHz body SAR** with expanded uncertainty 20.6%. The co-location of GSM/GPRS/EDGE, WLAN and Bluetooth were also checked. It is in compliance with Specific Absorption Rate (SAR) for general population/uncontrolled exposure limits specified in FCC 47 CFR part 2 (2.1093) and ANSI/IEEE C95.1-1999 and had been tested in accordance with the measurement methods and procedures specified in OET Bulletin 65 Supplement C (Edition 01-01).

Approved by

y Wu

Roy Wu O Deputy Manager

©2007 SPORTON International Inc. SAR Testing Lab This report shall not be reproduced except in full, without the written approval of Sporton. Page 1 of 34 Rev. 01 FORTON LAR. FCC SAR Test Report

Test Report No 🔅 FA742004-2-2-01

# 2. Administration Data

2.1	Testing	Laboratory	
		20000.000.0	

Company Name :	Sporton International Inc.
<b>Department :</b>	Antenna Design/SAR
Address :	No.52, Hwa-Ya 1 <sup>st</sup> RD., Hwa Ya Technology Park, Kwei-Shan Hsiang, TaoYuan
	Hsien, Taiwan, R.O.C.
<b>Telephone Number :</b>	886-3-327-3456
Fax Number :	886-3-328-4978

# 2.2 Detail of Applicant

<b>Company Name :</b>	MiTAC International Corp.
Address :	No. 1, Yen-Fa 2nd Rd., Hsin-Chu Science Based Industrial Park, Hsin-Chu Hsien,
	Taiwan, R.O.C.
<b>Telephone Number :</b>	886-2-26271188 ext 5506
Fax Number :	886-2-26579355
<b>Contact Person :</b>	colin.cheng@mic.com.tw

### 2.3 Detail of Manufacturer

<b>Company Name :</b>	Mitac computer (Kunshan) CO., Ltd.
Address :	No. 269, 2nd Road, Export Processing Zone, Changjiang South Road,
	KunShan,JiangSu prov.China

### 2.4 Application Detail

Date of reception of application:	Apr. 20, 2007
Start of test :	May 28, 2007
End of test :	May 28, 2007



# 3. <u>Scope</u>

# 3.1 <u>Description of Device Under Test (DUT)</u>

PDA phone
MiTAC
A702
P4Q-MIOA702
GSM850 : 824 ~ 849 MHz PCS1900 : 1850 ~ 1910 MHz Bluetooth : 2400 ~ 2483.5 MHz WLAN : 2400 ~ 2483.5 MHz
GSM850 : 869 ~ 894 MHz PCS1900 : 1930 ~ 1990 MHz Bluetooth : 2400 ~ 2483.5 MHz WLAN : 2400 ~ 2483.5 MHz
Bluetooth : 79 WLAN : 11
Bluetooth : 2402+n*1 MHz; n=0~78 WLAN : 2412+(n-1)*5 MHz; n=1~11
Fixed Internal
N/A
Bluetooth : -3.5 dBi WLAN : -3.5 dBi
GSM850: 32.80 dBm ; GSM850(GPRS10): 32.71 dBm ; GSM850(EDGE10): 26.11 dBm DCS1900: 30.81 dBm ; PCS1900(GPRS10): 30.66 dBm ; PCS1900(EDGE10): 23.72 dBm Bluetooth : -0.47 dBm 802.11b : 13.92 dBm / 802.11g: 18.42 dBm
GSM/GPRS : GMSK EDGE : 8PSK Bluetooth : GFSK WLAN : DSSS / OFDM
R02
R30
Production Unit
Battery : Welldone, E4MT211303B12 Earphone : BIMOS, 70425-02
Certification



### Test Report No 🔅 FA742004-2-2-01

### 3.2 Product Photo



Page 4 of 34 Rev. 01



Test Report No 👘 FA742004-2-2-01

### 3.3 <u>Applied Standards:</u>

The Specific Absorption Rate (SAR) testing specification, method and procedure for this PDA phone is in accordance with the following standards:

47 CFR Part 2 (2.1093), IEEE C95.1-1999, IEEE C95.3-2002, IEEE P1528 -2003, and OET Bulletin 65 Supplement C (Edition 01-01)



### 3.4 Device Category and SAR Limits

This device belongs to portable device category because its radiating structure is allowed to be used within 20 centimeters of the body of the user.

Limit for General Population/Uncontrolled exposure should be applied for this device, it is 1.6 W/kg as averaged over any 1 gram of tissue.

### 3.5 <u>Test Conditions</u>

### 3.5.1 Ambient Condition:

Item	HSL_2450	MSL_2450
Ambient Temperature ( )	20-24	
Tissue simulating liquid temperature ( )	21.5	21.3
Humidity (%)	<60	

### 3.5.2 <u>Test Configuration:</u>

The data rates for SAR testing are 11Mbps for 802.11b and 6Mbps for 802.11g. Engineering testing software installed on the EUT can provide continuous transmitting RF signal. This RF signal utilized in SAR measurement has almost 100% duty cycle and its crest factor is 1. The measurements were performed on the lowest, middle, and highest channel, i.e. channel 1, channel 6, and channel 11 for each testing position. However, measurements were performed only on the middle channel if the SAR is below 3 dB of limit.



# 4. <u>Specific Absorption Rate (SAR)</u> 4.1 <u>Introduction</u>

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The FCC recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

# 4.2 SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density.

). The equation description is as below:

$$\mathbf{SAR} = \frac{d}{dt} \left( \frac{dW}{dm} \right) = \frac{d}{dt} \left( \frac{dW}{\rho dv} \right)$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$\mathbf{SAR} = C \, \frac{\delta T}{\delta t}$$

, where C is the specific head capacity,  $\delta T$  is the temperature rise and  $\delta t$  the exposure duration,

or related to the electrical field in the tissue by

$$\mathbf{SAR} = \frac{\sigma |E|^2}{\rho}$$

, where is the conductivity of the tissue, is the mass density of the tissue and E is the rms electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.

©2007 SPORTON International Inc. SAR Testing Lab

Page 7 of 34 Rev. 01

This report shall not be reproduced except in full, without the written approval of Sporton.



Test Report No FA742004-2-2-01

# 5. SAR Measurement Setup

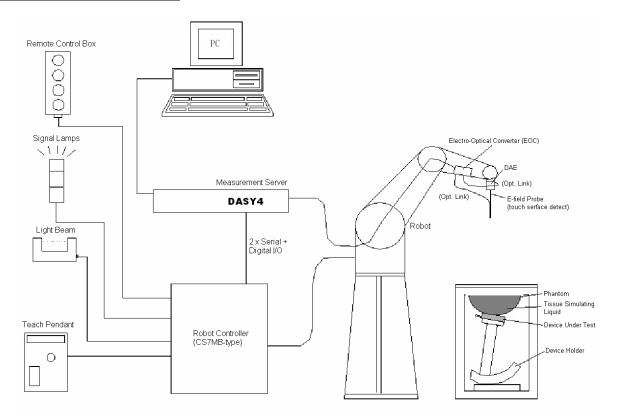


Fig. 5.1 DASY4 system



The DASY4 system for performance compliance tests is illustrated above graphically. This system consists of the following items:

- A standard high precision 6-axis robot with controller, a teach pendant and software
- A data acquisition electronic (DAE) attached to the robot arm extension
- A dosimetric probe equipped with an optical surface detector system
- > The electro-optical converter (ECO) performs the conversion between optical and electrical signals
- A measurement server performs the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the accuracy of the probe positioning
- A computer operating Windows XP
- DASY4 software
- Remove control with teach pendant and additional circuitry for robot safety such as warming lamps, etc.
- The SAM twin phantom
- ➢ A device holder
- Tissue simulating liquid
- > Dipole for evaluating the proper functioning of the system

Some of the components are described in details in the following sub-sections.

# 5.1 DASY4 E-Field Probe System

The SAR measurement is conducted with the dosimetric probe ET3DV6 (manufactured by SPEAG). The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency. This probe has a built in optical surface detection system to prevent from collision with phantom.




### Test Report No 🔅 FA742004-2-2-01

### 5.1.1 ET3DV6 E-Field Probe Specification

Construction	Symmetrical design with triangular core Built-in optical fiber for surface detection system Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents)				
Calibration	Simulating tissue at frequencies of 900MHz, 1.8GHz and 2.45GHz for brain and muscle (accuracy $\pm 8\%$ )				
Frequency	10 MHz to $>$ 3 GHz				
Directivity	$\pm$ 0.2 dB in brain tissue (rotation around probe axis) $\pm$ 0.4 dB in brain tissue (rotation perpendicular to probe axis)				
Dynamic Range	$5 \mu W/g \text{ to } > 100 \text{mW/g}; \text{ Linearity: } \pm 0.2 \text{dB}$				
Surface Detection	$\pm$ 0.2 mm repeatability in air and clear liquids on reflecting surface				
Dimensions	Overall length: 330mm				
	Tip length: 16mm				
	Body diameter: 12mm				
	Tip diameter: 6.8mm Distance from probe tip to dipole centers:				
	2.7mm				
Application	General dosimetry up to 3GHz Compliance tests for mobile phones and				
	Wireless LAN				
	Fast automatic scanning in arbitrary phantoms				





### 5.1.2 ET3DV6 E-Field Probe Calibration

Each probe needs to be calibrated according to a dosimetric assessment procedure with accuracy better than  $\pm$  10%. The spherical isotropy shall be evaluated and within  $\pm$  0.25dB. The sensitivity parameters (NormX, NormY, and NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested. The calibration data are as below:

Page 10 of 34 Rev. 01



### Test Report No 👘 FA742004-2-2-01

ET3DV6 SN1787					
Sensitivity	X axis : 1.5	X axis : 1.57 μV		is : 1.71 μV	Z axis : 2.09 μV
Diode compression point	X axis : 94	4 mV	Y av	xis : 94 mV	Z axis : 94 mV
Conversion factor	Frequency (MHz)	X axis		Y axis	Z axis
(Body)	2350~2550	4.13		4.13	4.13
Boundary effect	Frequency (MHz)	Alı	oha	Depth	
(Body)	2350~2550	0.	62	2.13	

### ET3DV6 SN1788

Sensitivity	X axis : 1.7	73 μV	Y ax	is : 1.67 μV	Z axis : 1.70 μV
Diode compression point	X axis : 95	5 mV	Y ax	is : 101 mV	Z axis : 93 mV
Conversion factor	Frequency (MHz)	X axis		Y axis	Z axis
(Head / Body)	2350~2550	4.66 / 4.11		4.66 / 4.11	4.66 / 4.11
Boundary effect	Frequency (MHz)	Alpha		Depth	
(Head / Body)	2350~2550	0.68 /	0.60	1.96 / 1.70	

NOTE:

1. The probe parameters have been calibrated by the SPEAG.

### 5.2 DATA Acquisition Electronics (DAE)

The data acquisition electronics (DAE4) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE4 is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is above 80dB.



# 5.3 <u>Robot</u>

The DASY4 system uses the high precision robots RX90BL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASYS system, the CS7MB robot controller version from Stäubli is used. The RX robot series have many features that are important for our application:

- → High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- > Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- ➢ 6-axis controller

# 5.4 <u>Measurement Server</u>

The DASY4 measurement server is based on a PC/104 CPU board with 166 MHz CPU 32 MB chipset and 64 MB RAM.

Communication with the DAE4 electronic box the 16-bit AD-converter system for optical detection and digital I/O interface.

The measurement server performs all the real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operations.

### 5.5 <u>SAM Twin Phantom</u>

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- ➢ Left head
- Right head
- ➢ Flat phantom

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections.



Test Report No 🔅 FA742004-2-2-01

A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters.

On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

The phantom can be used with the following tissue simulating liquids: \*Water-sugar based liquid \*Glycol based liquids

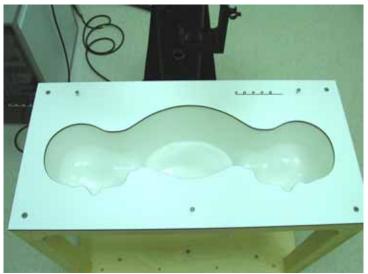


Fig. 5.3 Top view of twin phantom



Fig. 5.4 Bottom view of twin phantom



### 5.6 Data Storage and Evaluation

### 5.6.1 Data Storage

The DASY4 software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension .DA4. The postprocessing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type (e.g., [V/m], [A/m], [mW/g]). Some of these units are not available in certain situations or give meaningless results, e.g., a SAR-output in a loseless media, will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

# 5.6.2 Data Evaluation

The DASY4 postprocessing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software :

Probe parameters :	- Sensitivity	Norm <sub><i>i</i></sub> , $a_{i0}$ , $a_{i1}$ , $a_{i2}$
	- Conversion factor	ConvF <sub>i</sub>
	- Diode compression point	dcp <sub>i</sub>
Device parameters :	- Frequency	f
	- Crest factor	cf
Media parameters :	- Conductivity	
	- Density	

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel



Test Report No : FA742004-2-2-01

can be given as :

$$Vi = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with

 $V_i$  = compensated signal of channel i (i = x, y, z)  $U_i$  = input signal of channel i (i = x, y, z) cf = crest factor of exciting field (DASY parameter)  $dcp_i$  = diode compression point (DASY parameter)

From the compensated input signals, the primary field data for each channel can be evaluated :

E-field probes : 
$$E_i = \sqrt{\frac{V_i}{Norm_iConvF}}$$
  
H-field probes :  $H_i = \sqrt{V_i \frac{a_{i0+}a_{i1}f + a_{i2}f^2}{f}}$ 

with  $V_i$  = compensated signal of channel i (i = x, y, z)  $Norm_i$  = sensor sensitivity of channel i (i = x, y, z)  $\mu V/(V/m)2$  for E-field Probes ConvF = sensitivity enhancement in solution  $a_{ij}$  = sensor sensitivity factors for H-field probes f = carrier frequency [GHz]  $E_i$  = electric field strength of channel i in V/m  $H_i$  = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude) :

$$E_{tot} = \sqrt{E_X^2 + E_Y^2 + E_Z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with

SAR = local specific absorption rate in mW/g
Etot = total field strength in V/m
= conductivity in [mho/m] or [Siemens/m]
= equivalent tissue density in g/ cm<sup>3</sup>



\* Note that the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$
 or  $P_{pwe} = H_{tot}^2 \cdot 37.7$ 

with  $P_{pwe}$  = equivalent power density of a plane wave in mW/cm<sup>2</sup>  $E_{tot}$  = total electric field strength in V/m  $H_{tot}$  = total magnetic field strength in A/m



# 5.7 <u>Test Equipment List</u>

Manufacture	Norma of Farrian and	T-me (Medal	Serial Number	Calib	ration
Manufacture	Name of Equipment	Type/Model	Serial Number	Last Cal.	Due Date
SPEAG	Dosimetric E-Filed Probe	ET3DV6	1787	May 31, 2006	May 31, 2007
SPEAG	Dosimetric E-Filed Probe	ET3DV6	1788	Sep. 19, 2006	Sep. 19, 2007
SPEAG	835MHz System Validation Kit	D835V2	499	Mar. 15, 2006	Mar. 15, 2008
SPEAG	900MHz System Validation Kit	D900V2	190	Jul. 19, 2005	Jul. 19, 2007
SPEAG	1800MHz System Validation Kit	D1800V2	2d076	Jul. 20, 2005	Jul. 20, 2007
SPEAG	1900MHz System Validation Kit	D1900V2	5d041	Mar. 21, 2006	Mar. 21, 2008
SPEAG	2450MHz System Validation Kit	D2450V2	736	Jul. 12, 2005	Jul. 12, 2007
SPEAG	Data Acquisition Electronics	DAE3	577	Nov. 21, 2006	Nov. 21, 2007
SPEAG	Device Holder	N/A	N/A	NCR	NCR
SPEAG	Phantom	QD 000 P40 C	TP-1150	NCR	NCR
SPEAG	Robot	Staubli RX90BL	F03/5W15A1/A/01	NCR	NCR
SPEAG	Software	DASY4 V4.7 Build 53	N/A	NCR	NCR
SPEAG	Software	SEMCAD V1.8 Build 172	N/A	NCR	NCR
SPEAG	Measurement Server	SE UMS 001 BA	1021	NCR	NCR
Agilent	ENA Series Network Analyzer	E5071C	MY46100746	Feb. 21, 2007	Feb. 21, 2008
Agilent	Dielectric Probe Kit	85070D	US01440205	NCR	NCR
Agilent	Dual Directional Coupler	778D	50422	NCR	NCR
Agilent	Power Amplifier	8449B	3008A01917	NCR	NCR
R&S	Radio Communication Tester	CMU200	105513	Jul. 25, 2006	Jul. 24, 2007
Agilent	Power Meter	E4416A	GB41292344	Feb. 08, 2007	Feb. 08, 2008
Agilent	Power Sensor	E9327A	US40441548	Feb. 08, 2007	Feb. 08, 2008
Agilent	Signal Generator	E8247C	MY43320596	Mar. 01, 2006	Mar. 01, 2008

Table 5.1 Test Equipment List



# 6. <u>Tissue Simulating Liquids</u>

For the measurement of the field distribution inside the SAM phantom with DASY4, the phantom must be filled with around 25 liters of homogeneous body tissue simulating liquid. The liquid height from the bottom of the phantom body is 15.2 centimeters, which is shown in Fig. 6.1.

The following ingredients for tissue simulating liquid are used:

- **Water**: deionized water (pure  $H_20$ ), resistivity 16M as basis for the liquid
- Sugar: refined sugar in crystals, as available in food shops to reduce relative permittyvity
- Salt: pure NaCl to increase conductivity
- Cellulose: Hydroxyethyl-cellulose, medium viscosity (75-125 mPa.s, 2% in water, 20°C), CAS#54290-to increase viscosity and to keep sugar in solution.
- Preservative: Preventol D-7 Bayer AG, D-51368 Leverkusen, CAS#55965-84-9- to prevent the spread of bacteria and molds.
- DGMBE: Deithlenglycol-monobuthyl ether (DGMBE), Fluka Chemie GmbH, CAS#112-34-5 to reduce relative permittivity.

Table 6.1 gives the recipes for one liter of tissue simulating liquid for frequency band 2450 MHz.

Ingredient	HSL-2450	MSL-2450
Water	450.0 ml	698.3 ml
DGMBE	550.0 ml	301.7 ml
Total amount	1 liter (1.0 kg)	1 liter (1.0 kg)
Dielectric Parameters at 22°	f = 2450MHz	f = 2450MHz
	$_{\rm I}$ = 39.2±5%, = 1.8±5% S/m	$r = 52.7 \pm 5\%, = 1.95 \pm 5\%$ S/m

### Table 6.1

The dielectric parameters of the liquids were verified prior to the SAR evaluation using an Agilent 85070D Dielectric Probe Kit and an Agilent Network Analyzer.

	Bands	Frequency(MHz)	Permittivity ( r)	Conductivity ( )	Measurement Date
		2412	38.6	1.73	
Head	Head 2450 MHz	2437	38.2	1.74	May 28, 2007
		2462	38	1.78	
		2412	52.5	1.9	
Body	Body 2450 MHz	2437	52.4	1.96	May 28, 2007
		2462	52.4	1.96	
-					

Table 6.2 shows the measuring results for head and muscle simulating liquid.

# Table 6.2

The measuring data are consistent with  $r = 39.2 \pm 5\%$  and  $r = 1.80 \pm 5\%$  for head 2450 band and  $r = 52.7 \pm 5\%$  and  $r = 1.95 \pm 5\%$  for body 2450 band.

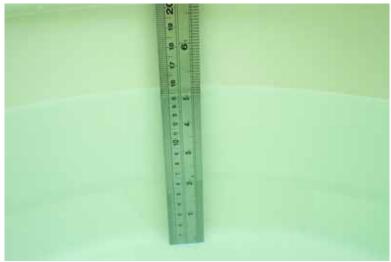


Fig. 6.1



# 7. <u>Uncertainty Assessment</u>

The component of uncertainly may generally be categorized according to the methods used to evaluate them. The evaluation of uncertainly by the statistical analysis of a series of observations is termed a Type A evaluation of uncertainty. The evaluation of uncertainty by means other than the statistical analysis of a series of observation is termed a Type B evaluation of uncertainty. Each component of uncertainty, however evaluated, is represented by an estimated standard deviation, termed standard uncertainty, which is determined by the positive square root of the estimated variance.

A Type A evaluation of standard uncertainty may be based on any valid statistical method for treating data. This includes calculating the standard deviation of the mean of a series of independent observations; using the method of least squares to fit a curve to the data in order to estimate the parameter of the curve and their standard deviations; or carrying out an analysis of variance in order to identify and quantify random effects in certain kinds of measurement.

A type B evaluation of standard uncertainty is typically based on scientific judgment using all of the relevant information available. These may include previous measurement data, experience and knowledge of the behavior and properties of relevant materials and instruments, manufacture's specification, data provided in calibration reports and uncertainties assigned to reference data taken from handbooks. Broadly speaking, the uncertainty is either obtained from an outdoor source or obtained from an assumed distribution, such as the normal distribution, rectangular or triangular distributions indicated in Table 7.1

Uncertainty Distributions	Normal	Rectangular	Triangular	U-shape
Multiplying factor <sup>(a)</sup>	$_{1/k}$ (b)	1/ 3	1/ 6	1/ 2

(a) standard uncertainty is determined as the product of the multiplying factor and the estimated range of variations in the measured quantity
 (b) is the coverage factor

### Table 7.1

The combined standard uncertainty of the measurement result represents the estimated standard deviation of the result. It is obtained by combining the individual standard uncertainties of both Type A and Type B evaluation using the usual "root-sum-squares" (RSS) methods of combining standard deviations by taking the positive square root of the estimated variances.

Expanded uncertainty is a measure of uncertainty that defines an interval about the measurement result within which the measured value is confidently believed to lie. It is obtained by multiplying the combined standard uncertainty by a coverage factor. Typically, the coverage factor ranges from 2 to 3. Using a coverage factor allows the true value of a measured quantity to be specified with a defined probability within the specified uncertainty range. For purpose of this document, a coverage factor two is used, which corresponds to confidence interval of about 95 %. The DASY4 uncertainty Budget is showed in Table 7.2.



### Test Report No FA742004-2-2-01

Error Description	Uncertainty Value ± %	Probability Distribution	Divisor	Ci 1g	Standard Unc. (1-g)	Vi or Veff
Measurement System			11		1	
Probe Calibration	$\pm 4.8$	Normal	1	1	±4.8	
Axial Isotropy	± 4.7	Rectangular	$\sqrt{3}$	0.7	±1.9	
Hemispherical Isotropy	± 9.6	Rectangular	$\sqrt{3}$	0.7	±3.9	
Boundary Effect	± 1.0	Rectangular	$\sqrt{3}$	1	±0.6	
Linearity	± 4.7	Rectangular	$\sqrt{3}$	1	±2.7	
System Detection Limit	± 1.0	Rectangular	$\sqrt{3}$	1	±0.6	
Readout Electronics	± 1.0	Normal	1	1	±1.0	
Response Time	$\pm 0.8$	Rectangular	$\sqrt{3}$	1	± 0.5	
Integration time	± 2.6	Rectangular	$\sqrt{3}$	1	± 1.5	
RF Ambient Conditions	± 3.0	Rectangular	$\sqrt{3}$	1	±1.7	
Probe Positioner Mech. Tolerance	$\pm 0.4$	Rectangular	$\sqrt{3}$	1	±0.2	
Probe Positioning with respect to Phantom Shell	± 2.9	Rectangular	$\sqrt{3}$	1	±1.7	
Extrapolation and Interpolation Algorithms for Max. SAR Evaluation	± 1.0	Rectangular	√3	1	±0.6	
Test sample Related						
Test sample Positioning	±2.9	Normal	1	1	±2.9	145
Device Holder Uncertainty	±3.6	Normal	1	1	±3.6	5
Output Power Variation-SAR drift measurement	±5.0	Rectangular	√3	1	±2.9	
Phantom and Setup						
Phantom uncertainty(Including shap and thickness tolerances)	±4.0	Rectangular	$\sqrt{3}$	1	±2.3	
Liquid Conductivity Target tolerance	±5.0	Rectangular	√3	0.64	±1.8	
Liquid Conductivity measurement uncertainty	±2.5	Normal	1	0.64	±1.6	
Liquid Permittivity Target tolerance	±5.0	Rectangular	√3	0.6	±1.7	
Liquid Permittivity measurement uncertainty	±2.5	Normal	1	0.6	±1.5	
Combined standard uncertainty					±10.3	330
Coverage Factor for 95 %		<u>K=2</u>				
Expanded uncertainty (Coverage factor = 2)			Normal (k=2) 27		±20.6	

 Table 7.2 Uncertainty Budget of DASY



# 8. <u>SAR Measurement Evaluation</u>


Each DASY system is equipped with one or more system validation kits. These units, together with the predefined measurement procedures within the DASY software, enable the user to conduct the system performance check and system validation. System validation kit includes a dipole, tripod holder to fix it underneath the flat phantom and a corresponding distance holder.

# 8.1 <u>Purpose of System Performance check</u>

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal SAR measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

# 8.2 <u>System Setup</u>

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave which comes from a signal generator at frequency 2450 MHz. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

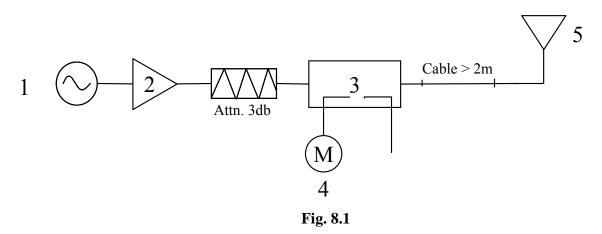



- 1. Signal Generator
- 2. Amplifier
- 3. Directional Coupler
- 4. Power Meter
- 5. 2450 MHz Dipole

The output power on dipole port must be calibrated to 100 mW (20 dBm) before dipole is connected.



Fig 8.2 Dipole Setup



# 8.3 Validation Results

Comparing to the original SAR value provided by Speag, the validation data should within its specification of 10 %. Table 8.1 shows the target SAR and measured SAR after normalized to 1W input power.

			Target (W/kg)	Measurement data (W/kg)	Variation	Measurement date
Hood	ISM band	SAR (1g)	52.8	54	2.3 %	May 28, 2007
Head (2450 MHz)	SAR (10g)	24.7	25.5	3.2 %	wiay 28, 2007	
Dadu	ISM band	SAR (1g)	52.8	57.7	9.3 %	May 28, 2007
Body (2450 MHz	(2450 MHz)	SAR (10g)	24.5	26.7	9.0 %	May 28, 2007

Table 8.1

The table above indicates the system performance check can meet the variation criterion.




# 9. <u>Description for DUT Testing Position</u>

This DUT was tested in 6 different positions. They are left cheek, left tilted, right cheek, right tilted, body worn with keypad up and body worn with keypad down as illustrated below:

- 1) "Cheek Position"
  - i) To position the device with the vertical center line of the body of the device and the horizontal line crossing the center piece in a plane parallel to the sagittal plane of the phantom. While maintaining the device in this plane, align the vertical center line with the reference plane containing the three ear and mouth reference point (M, RE and LE) and align the center of the ear piece with the line RE-LE.
  - ii) To move the device towards the phantom with the ear piece aligned with the line LE-RE until the phone touched the ear. While maintaining the device in the reference plane and maintaining the phone contact with the ear, move the bottom of the phone until any point on the front side is in contact with the cheek of the phantom or until contact with the ear is lost (see Fig. 9.1).
- 2) "Tilted Position"
  - i) To position the device in the "cheek" position described above.
  - ii) While maintaining the device the reference plane described above and pivoting against the ear, move it outward away from the mouth by an angle of 15 degrees or until contact with the ear is lost (see Fig. 9.2).
- 3) "Body Worn"
  - i) To position the device parallel to the phantom surface.
  - ii) To adjust the phone parallel to the flat phantom.
  - iii) To adjust the distance between the EUT surface and the flat phantom to 1.5 cm.



Test Report No 👘 FA742004-2-2-01

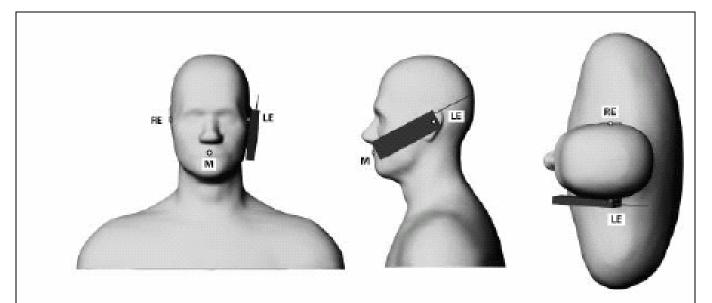

**Fig. 9.1** Phone Position 1, "Cheek" or "Touch" Position. The reference points for the right ear (RE), left ear (LE) and mouth (M), which define the plane for phone positioning, are indicated.

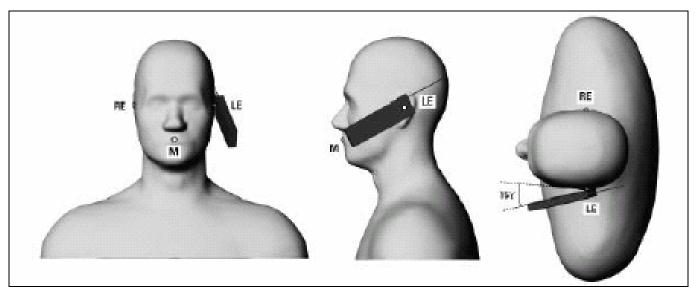


Fig. 9.2 Phone Position 2, "Tilted Position". The reference point for the right ear (RE), left ear (LE) and mouth (M), which define the plane for phone positioning, are indicated.



Test Report No FA742004-2-2-01

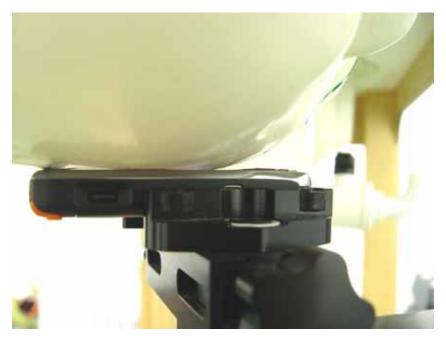


Fig. 9.3 Right Cheek

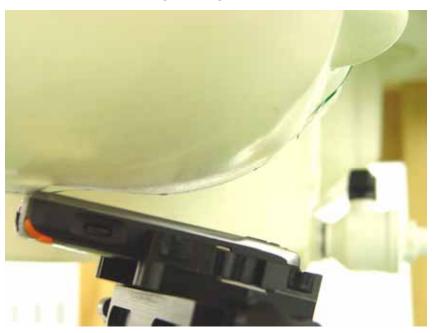


Fig. 9.4 Right Tilted



### Test Report No FA742004-2-2-01

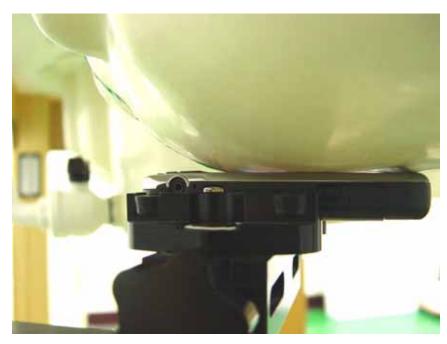


Fig. 9.5 Left Cheek

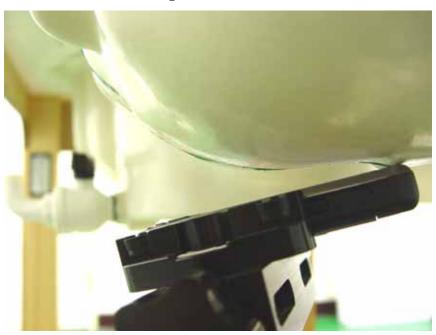


Fig. 9.6 Left Tilted



Test Report No 🔅 FA742004-2-2-01



Fig. 9.7 Keypad Up with 1.5cm Gap



Fig. 9.8 Keypad Down with 1.5cm Gap



# 10. Measurement Procedures

The measurement procedures are as follows:

- ▶ Using engineering software to transmit RF power continuously (continuous Tx) in the middle channel
- Placing the DUT in the positions described in the last section
- Setting scan area, grid size and other setting on the DASY4 software
- Taking data for the low channel
- Repeat the previous steps for the low and high channels.

According to the IEEE P1528 draft standard, the recommended procedure for assessing the peak spatial-average SAR value consists of the following steps:

Power reference measurement

- Area scan
- Zoom scan
- Power reference measurement

# 10.1 Spatial Peak SAR Evaluation

The procedure for spatial peak SAR evaluation has been implemented according to the IEEE1528-2003 standard. It can be conducted for 1g and 10g, as well as for user-specific masses. The DASY4 software includes all numerical procedures necessary to evaluate the spatial peak SAR value.

Base on the Draft: SCC-34, SC-2, WG-2-Computational Dosimetry, P1528/D1.2 (Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques), a new algorithm has been implemented. The spatial-peak SAR can be computed over any required mass.

The base for the evaluation is a "cube" measurement. The measured volume must include the 1g and 10g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan.



The entire evaluation of the spatial peak values is performed within the postprocessing engine (SEMCAD). The system always gives the maximum values for the 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- extraction of the measured data (grid and values) from the Zoom Scan
- calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- generation of a high-resolution mesh within the measured volume
- interpolation of all measured values form the measurement grid to the high-resolution grid
- extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- calculation of the averaged SAR within masses of 1g and 10g

# 10.2 <u>Scan Procedures</u>

First **Area Scan** is used to locate the approximate location(s) of the local peak SAR value(s). The measurement grid within an **Area Scan** is defined by the grid extent, grid step size and grid offset. Next, in order to determine the EM field distribution in a three-dimensional spatial extension, **Zoom Scan** is required. The **Zoom Scan** measures 5x5x7 points with step size 8, 8 and 5 mm. The **Zoom Scan** is performed around the highest E-field value to determine the averaged SAR-distribution over 1 g.

### 10.3 <u>SAR Averaged Methods</u>

In DASY4, the interpolation and extrapolation are both based on the modified Quadratic Shepard's method. The interpolation scheme combines a least-square fitted function method and a weighted average method which are the two basic types of computational interpolation and approximation.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1 g and 10 g cubes, the extrapolation distance should not be larger than 5 mm.



# 11. SAR Test Results

### 11.1 <u>Right Cheek</u>

Bands	Chan.	Freq. (MHz)	Modulation type	Conducted Power (dBm)	Power Drift (dB)	Measured 1g SAR (W/kg)	Limits (W/Kg)	Results
	1	2412(Low)	ССК	13.92	-0.166	0.03	1.6	Pass
802.11b	6	2437(Mid)	CCK	13.83	-0.129	0.027	1.6	Pass
	11	2462(High)	CCK	13.73	-0.141	0.026	1.6	Pass
802.11b with BT On	1	2412(Low)	ССК	13.92	-0.124	0.03	1.6	Pass
	1	2412(Low)	OFDM	18.25	-	-	-	-
802.11g	6	2437(Mid)	OFDM	18.02	0.137	0.025	1.6	Pass
	11	2462(High)	OFDM	18.42	-	-	-	-

# 11.2 Right Tilted

Bands	Chan.	Freq. (MHz)	Modulation type	Conducted Power (dBm)	Power Drift (dB)	Measured 1g SAR (W/kg)	Limits (W/Kg)	Results
	1	2412(Low)	CCK	13.92	-	-	-	-
802.11b	6	2437(Mid)	CCK	13.83	-0.152	0.00447	1.6	Pass
	11	2462(High)	CCK	13.73	-	-	-	-
	1	2412(Low)	OFDM	18.25	-	-	-	-
802.11g	6	2437(Mid)	OFDM	18.02	-	-	-	-
	11	2462(High)	OFDM	18.42	-	-	-	-

# 11.3 Left Cheek

Bands	Chan.	Freq. (MHz)	Modulation type	Conducted Power (dBm)	Power Drift (dB)	Measured 1g SAR (W/kg)	Limits (W/Kg)	Results
802.11b	1	2412(Low)	CCK	13.92	-	-	-	-
	6	2437(Mid)	CCK	13.83	-0.125	0.018	1.6	Pass
	11	2462(High)	CCK	13.73	-	-	-	-
	1	2412(Low)	OFDM	18.25	-	-	-	-
802.11g	6	2437(Mid)	OFDM	18.02	-	-	-	-
	11	2462(High)	OFDM	18.42	-	-	-	-



### Test Report No 👘 FA742004-2-2-01

# 11.4 Left Tilted

Bands	Chan.	Freq. (MHz)	Modulation type	Conducted Power (dBm)	Power Drift (dB)	Measured 1g SAR (W/kg)	Limits (W/Kg)	Results
	1	2412(Low)	CCK	13.92	-	-	-	-
802.11b	6	2437(Mid)	CCK	13.83	-0.19	0.00432	1.6	Pass
	11	2462(High)	CCK	13.73	-	-	-	-
	1	2412(Low)	OFDM	18.25	-	-	-	-
802.11g	6	2437(Mid)	OFDM	18.02	-	-	-	-
	11	2462(High)	OFDM	18.42	-	-	-	-

### 11.5 Keypad Up with 1.5cm Gap

Bands	Chan.	Freq. (MHz)	Modulation type	Conducted Power (dBm)	Power Drift (dB)	Measured 1g SAR (W/kg)	Limits (W/Kg)	Results
	1	2412(Low)	CCK	13.92	-	-	-	-
802.11b	6	2437(Mid)	CCK	13.83	0.119	0.00422	1.6	Pass
	11	2462(High)	CCK	13.73	-	-	-	-
	1	2412(Low)	OFDM	18.25	-	-	-	-
802.11g	6	2437(Mid)	OFDM	18.02	-	-	-	-
	11	2462(High)	OFDM	18.42	-	-	-	-

# 11.6 Keypad Down with 1.5cm Gap

Bands	Chan.	Freq. (MHz)	Modulation type	Conducted Power (dBm)	Power Drift (dB)	Measured 1g SAR (W/kg)	Limits (W/Kg)	Results
802.11b	1	2412(Low)	CCK	13.92	-	-	-	-
	6	2437(Mid)	CCK	13.83	-0.124	0.019	1.6	Pass
	11	2462(High)	CCK	13.73	-	-	-	-
	1	2412(Low)	OFDM	18.25	-0.143	0.025	1.6	Pass
802.11g	6	2437(Mid)	OFDM	18.02	0.103	0.022	1.6	Pass
-	11	2462(High)	OFDM	18.42	0.173	0.019	1.6	Pass
802.11g with BT On	01	2412(Low)	OFDM	18.25	-0.134	0.018	1.6	Pass

Remark:

1.

The largest summation of GSM and WLAN for head SAR is 0.857 W/Kg, and its position is right cheek. The largest summation of GSM/GPRS/EDGE and WLAN for body SAR is 1.205 W/Kg and its position is 2. keypad down with 1.5cm Gap.

Test Engineer : Eric Huang and John Tsai



# 12. References

- [1] FCC 47 CFR Part 2 "Frequency Allocations and Radio Treaty Matters; General Rules and Regulations"
- [2] IEEE Std. P1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", April 21,2003.
- [3] Supplement C (Edition 01-01) to OET Bulletin 65 (Edition 97-01), "Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to RF Emissions", June 2001
- [4] IEEE Std. C95.3-2002, "IEEE Recommended Practice for the Meaurement of Potentially Hazardous Electromagnetic Fields-RF and Microwave", 2002
- [5] IEEE Std. C95.1-1999, "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz", 1999
- [6] Robert J. Renka, "Multivariate Interpolation Of Large Sets Of Scattered Data", University of Noth Texas ACM Transactions on Mathematical Software, vol. 14, no. 2, June 1988, pp. 139-148
- [7] DAYS4 System Handbook



## Appendix A - System Performance Check Data

Test Laboratory: Sporton International Inc. SAR Testing Lab

Date: 2007/5/28

#### System Check Head 2450MHz

#### DUT: Dipole 2450 MHz

Communication System: CW; Frequency: 2450 MHz;Duty Cycle: 1:1 Medium: HSL\_2450 Medium parameters used: f = 2450 MHz;  $\sigma = 1.76$  mho/m;  $\epsilon_c = 38.1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature : 22.5 'C; Liquid Temperature : 21.5 'C


DASY4 Configuration:

- Probe: ET3DV6 - SN1788; ConvF(4.66, 4.66, 4.66); Calibrated: 2006/9/19

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
   Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

2450MHz/Area Scan (41x41x1): Measurement grid: dx=20mm, dy=20mm Maximum value of SAR (interpolated) = 5.83 mW/g

2450MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 57.8 V/m; Power Drift = -0.036 dB Peak SAR (extrapolated) = 11.4 W/kg SAR(1 g) = 5.4 mW/g; SAR(10 g) = 2.55 mW/g Maximum value of SAR (measured) = 6.11 mW/g

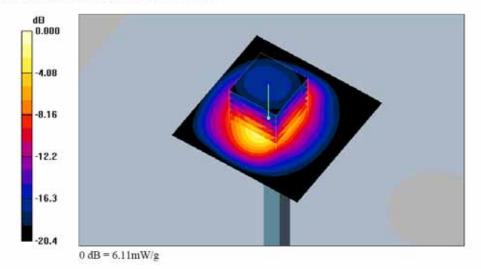



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date: 2007/5/28

#### System Check Body 2450MHz

#### DUT: Dipole 2450 MHz

Communication System: CW; Frequency: 2450 MHz;Duty Cycle: 1:1 Medium: MSL\_2450 Medium parameters used: f = 2450 MHz;  $\sigma = 1.95$  mho/m;  $\epsilon_r = 52.4$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature : 22.6 'C; Liquid Temperature : 21.3 'C


DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(4.13, 4.13, 4.13); Calibrated: 2006/5/31 - Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)Sensor-Surface: 4mm (Mechanical Surface Detection) - Electronics: DAE3 Sn577; Calibrated: 2006/11/21

- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
   Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 6.81 mW/g

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 60.9 V/m; Power Drift = -0.005 dB Peak SAR (extrapolated) = 12.8 W/kg SAR(1 g) = 5.77 mW/g; SAR(10 g) = 2.67 mW/g Maximum value of SAR (measured) = 6.49 mW/g

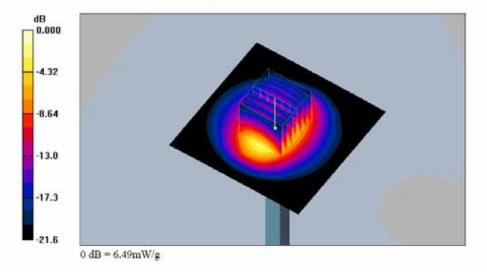



## Appendix B - SAR Measurement Data

Test Laboratory: Sporton International Inc. SAR Testing Lab

Date: 2007/5/28

#### Right Cheek 802.11b Ch1

DUT: 742004

Communication System: 802.11b ; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: HSL\_2450 Medium parameters used: f = 2412 MHz;  $\sigma$  = 1.73 mho/m;  $\epsilon_r$  = 38.6;  $\rho$  = 1000 kg/m<sup>3</sup> Ambient Temperature : 22.5 °C; Liquid Temperature : 21.5 °C


DASY4 Configuration:

- Probe: ET3DV6 - SN1788; ConvF(4.66, 4.66, 4.66); Calibrated; 2006/9/19

- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch1/Area Scan (61x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.034 mW/g

Ch1/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8nnn, dy=8nnn, dz=5nnn Reference Value = 0.831 V/m; Power Drift = -0.166 dB Peak SAR (extrapolated) = 0.055 W/kg SAR(1 g) = 0.030 mW/g; SAR(10 g) = 0.014 mW/g Maximum value of SAR (measured) = 0.036 mW/g

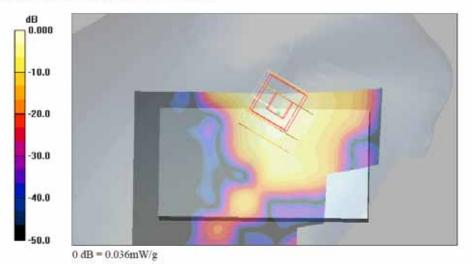



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date: 2007/5/28

#### Right Cheek 802.11b Ch1 Bluetooth On

DUT: 742004

Communication System: 802.11b ; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: HSL\_2450 Medium parameters used: f = 2412 MHz;  $\sigma$  = 1.73 mho/m;  $\varepsilon_r$  = 38.6;  $\rho$  = 1000 kg/m<sup>3</sup> Ambient Temperature : 22.6 °C; Liquid Temperature : 21.5 °C


DASY4 Configuration:

Probe: ET3DV6 - SN1788; ConvF(4.66, 4.66, 4.66); Calibrated; 2006/9/19
 Sensor-Surface: 4mm (Mechanical Surface Detection)
 Electronics: DAE3 Sn577; Calibrated; 2006/11/21

Phantom: SAM-B: Type: QD 000 P40 C; Serial: TP-1383
 Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch1/Area Scan (61x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.031 mW/g

Ch1/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 0.460 V/m; Power Drift = -0.124 dB Peak SAR (extrapolated) = 0.057 W/kg SAR(1 g) = 0.030 mW/g; SAR(10 g) = 0.014 mW/g Maximum value of SAR (measured) = 0.033 mW/g

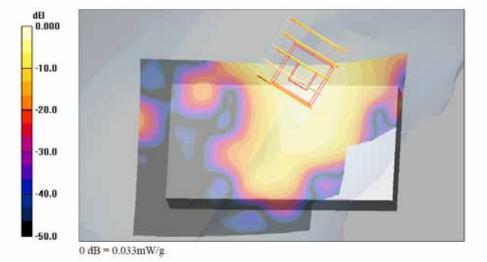



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date: 2007/5/28

#### Right Cheek 802.11g Ch6

DUT: 742004

Communication System: 802.11g; Frequency: 2437 MHz;Duty Cycle: 1:1 Medium: HSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.74$  mho/m;  $\epsilon_r = 38.2$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature : 22.6 'C; Liquid Temperature : 21.5 'C


DASY4 Configuration:

- Probe: ET3DV6 - SN1788; ConvF(4.66, 4.66, 4.66); Calibrated; 2006/9/19 - Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B: Type: QD 000 P40 C; Serial: TP-1383
   Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch6/Area Scan (61x91x1): Measurement grid: dx=15mm. dy=15mm Maximum value of SAR (interpolated) = 0.030 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 0.607 V/m; Power Drift = -0.137 dB Peak SAR (extrapolated) = 0.038 W/kg SAR(1 g) = 0.025 mW/g; SAR(10 g) = 0.012 mW/g Maximum value of SAR (measured) = 0.029 mW/g

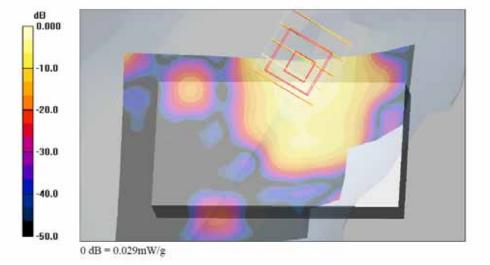



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date: 2007/5/28

#### Right Tilted\_802.11b Ch6

DUT: 742004

Communication System: 802.11b ; Frequency: 2437 MHz;Duty Cycle: 1:1 Medium: HSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.74$  mho/m;  $\epsilon_r = 38.2$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature : 22.6 °C; Liquid Temperature : 21.5 °C

DASY4 Configuration:


Probe: ET3DV6 - SN1788; ConvF(4.66, 4.66, 4.66); Calibrated; 2006/9/19
Sensor-Surface: 4mm (Mechanical Surface Detection)
Electronics: DAE3 Sn577; Calibrated: 2006/11/21
Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch6/Area Scan (61x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.007 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.33 V/m; Power Drift = -0.152 dB Peak SAR (extrapolated) = 0.005 W/kg SAR(1 g) = 3.45e-005 mW/g; SAR(10 g) = 5.36e-006 mW/g

Maximum value of SAR (measured) = 0.005 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.33 V/m; Power Drift = -0.152 dB Peak SAR (extrapolated) = 0.021 W/kg SAR(1 g) = 0.00447 mW/g; SAR(10 g) = 0.00121 mW/g Maximum value of SAR (measured) = 0.004 mW/g

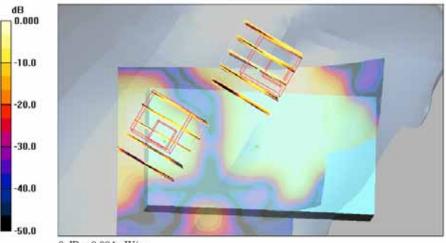

0 dB = 0.004 mW/g



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date: 2007/5/28

#### Left Cheek 802.11b Ch6

DUT: 742004

Communication System: 802.11b ; Frequency: 2437 MHz;Duty Cycle: 1:1 Medium: HSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.74$  mho/m;  $\epsilon_r = 38.2$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature : 22.6 'C; Liquid Temperature : 21.5 'C

DASY4 Configuration:


- Probe: ET3DV6 - SN1788; ConvF(4.66, 4.66, 4.66); Calibrated: 2006/9/19 - Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE3 Sn577; Calibrated: 2006/11/21

Phantom: SAM-B: Type: QD 000 P40 C; Serial: TP-1383
Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch6/Area Scan (61x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.024 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 0.941 V/m; Power Drift = -0.125 dB Peak SAR (extrapolated) = 0.035 W/kg SAR(1 g) = 0.018 mW/g; SAR(10 g) = 0.00824 mW/g Maximum value of SAR (measured) = 0.022 mW/g

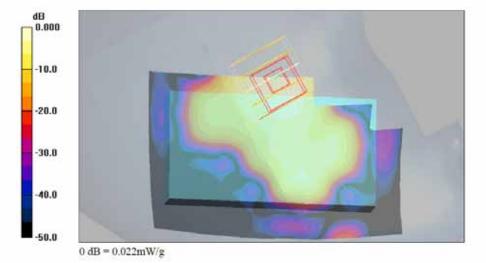



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date: 2007/5/28

#### Left Tilted\_802.11b Ch6

DUT: 742004

Communication System: 802.11b ; Frequency: 2437 MHz;Duty Cycle: 1:1 Medium: HSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.74$  mho/m;  $\varepsilon_r = 38.2$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature : 22.5 °C; Liquid Temperature : 21.5 °C

DASY4 Configuration:


Probe: ET3DV6 - SN1788; ConvF(4.66, 4.66, 4.66); Calibrated; 2006/9/19
Sensor-Surface: 4mm (Mechanical Surface Detection)
Electronics: DAE3 Sn577; Calibrated: 2006/11/21
Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch6/Area Scan (61x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.010 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.34 V/m; Power Drift = -0.1904dB Peak SAR (extrapolated) = 0.019 W/kg SAR(1 g) = 0.00389 mW/g; SAR(10 g) = 0.000935 mW/g

Maximum value of SAR (measured) = 0.003 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.34 V/m; Power Drift = -0.190 dB Peak SAR (extrapolated) = 0.020 W/kg SAR(1 g) = 0.00432 mW/g; SAR(10 g) = 0.00173 mW/g Maximum value of SAR (measured) = 0.004 mW/g

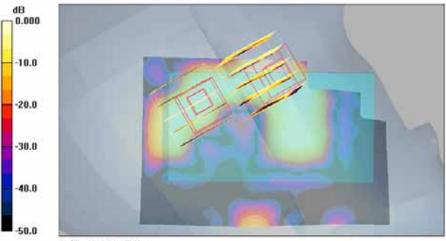

0 dB = 0.004 mW/g



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date: 2007/5/28

#### Body\_802.11b Ch6\_Keypad Up with 1.5cm Gap

DUT: 742004

Communication System: 802.11b ; Frequency: 2437 MHz;Duty Cycle: 1:1 Medium: MSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma$  = 1.94 mho/m;  $\varepsilon_r$  = 52.4;  $\rho$  = 1000 kg/m<sup>3</sup> Ambient Temperature : 22.6 °C; Liquid Temperature : 21.3 °C


DASY4 Configuration:

Probe: ET3DV6 - SN1787; ConvF(4.13, 4.13, 4.13); Calibrated; 2006/5/31
Sensor-Surface: 4mm (Mechanical Surface Detection)
Electronics: DAE3 Sn577; Calibrated: 2006/11/21
Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch6/Area Scan (61x91x1): Measurement grid: dx=15mm Maximum value of SAR (interpolated) = 0.006 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 0.764 V/m; Power Drift = 0.119 dB Peak SAR (extrapolated) = 0.018 W/kg SAR(1 g) = 0.00422 mW/g; SAR(10 g) = 0.00168 mW/g Maximum value of SAR (measured) = 0.004 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 0.764 V/m; Power Drift = 0.119 dB Peak SAR (extrapolated) = 0.018 W/kg SAR(1 g) = 0.00325 mW/g; SAR(10 g) = 0.000707 mW/g

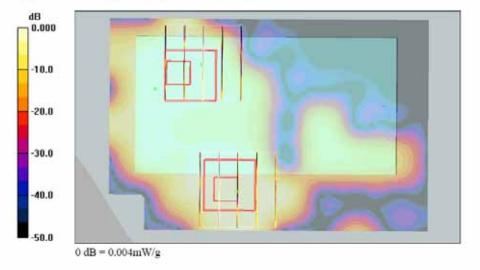



Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/5/28

#### Body 802.11b Ch6 Keypad Down with 1.5cm Gap

DUT: 742004

Communication System: 802.11b ; Frequency: 2437 MHz;Duty Cycle: 1:1 Medium: MSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma$  = 1.94 mho/m;  $\varepsilon_r$  = 52.4;  $\rho$  = 1000 kg/m<sup>3</sup> Ambient Temperature : 22.6 °C; Liquid Temperature : 21.3 °C


DASY4 Configuration:

Probe: ET3DV6 - SN1787; ConvF(4.13, 4.13, 4.13); Calibrated; 2006/5/31
Sensor-Surface: 4mm (Mechanical Surface Detection)
Electronics: DAE3 Sn577; Calibrated: 2006/11/21
Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch6/Area Scan (61x91x1): Measurement grid: dx=15mm Maximum value of SAR (interpolated) = 0.021 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 0.977 V/m; Power Drift = -0.124 dB Peak SAR (extrapolated) = 0.035 W/kg SAR(1 g) = 0.019 mW/g; SAR(10 g) = 0.00984 mW/g Maximum value of SAR (measured) = 0.022 mW/g

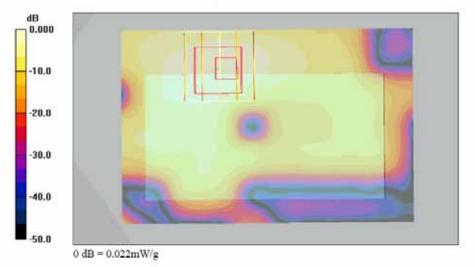



Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/5/28

#### Body 802.11g Ch1 Keypad Down with 1.5cm Gap

DUT: 742004


Communication System: 802.11g; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: MSL\_2450 Medium parameters used: f = 2412 MHz;  $\sigma = 1.9$  mho/m;  $\epsilon_r = 52.5$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature : 22.6 °C; Liquid Temperature : 21.3 °C

DASY4 Configuration:

Probe: ET3DV6 - SN1787; ConvF(4.13, 4.13, 4.13); Calibrated; 2006/5/31
Sensor-Surface: 4mm (Mechanical Surface Detection)
Electronics: DAE3 Sn577; Calibrated: 2006/11/21
Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch1/Area Scan (61x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.026 mW/g

Ch1/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.15 V/m; Power Drift = -0.143 dB Peak SAR (extrapolated) = 0.045 W/kg SAR(1 g) = 0.025 mW/g; SAR(10 g) = 0.013 mW/g Maximum value of SAR (measured) = 0.028 mW/g

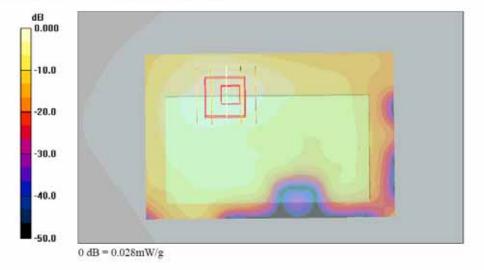



Test Laboratory: Sporton International Inc. SAR Testing Lab Date

Date: 2007/5/28

#### Body\_802.11g Ch1\_Keypad Down with 1.5cm Gap\_Bluetooth On

DUT: 742004

Communication System: 802.11g; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: MSL\_2450 Medium parameters used: f = 2412 MHz;  $\sigma = 1.9$  mho/m;  $\epsilon_r = 52.5$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature : 22.6 °C; Liquid Temperature : 21.3 °C


DASY4 Configuration:

Probe: ET3DV6 - SN1787; ConvF(4.13, 4.13, 4.13); Calibrated: 2006/5/31
Sensor-Surface: 4mm (Mechanical Surface Detection)
Electronics: DAE3 Sn577; Calibrated: 2006/11/21
Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch1/Area Scan (61x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.024 mW/g

Ch1/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.13 V/m; Power Drift = -0.134 dB Peak SAR (extrapolated) = 0.035 W/kg SAR(1 g) = 0.018 mW/g; SAR(10 g) = 0.00995 mW/g Maximum value of SAR (measured) = 0.021 mW/g

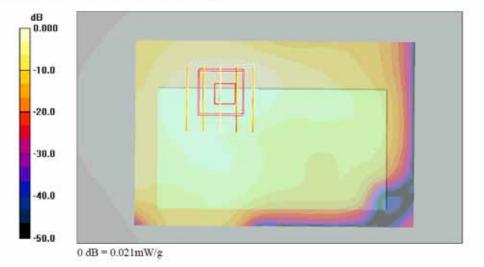



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date: 2007/5/28

#### Right Cheek 802.11b Ch1 2D

DUT: 742004

Communication System: 802.11b ; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: HSL\_2450 Medium parameters used: f = 2412 MHz;  $\sigma = 1.73$  mho/m;  $\epsilon_r = 38.6$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature : 22.5 'C; Liquid Temperature : 21.5 'C

DASY4 Configuration:


- Probe: ET3DV6 - SN1788; ConvF(4.66, 4.66, 4.66); Calibrated; 2006/9/19

- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21

Phantom: SAM-B: Type: QD 000 P40 C; Serial: TP-1383
Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch1/Area Scan (61x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.034 mW/g

Ch1/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 0.831 V/m; Power Drift = -6.67 dB Peak SAR (extrapolated) = 0.055 W/kg SAR(1 g) = 0.030 mW/g; SAR(10 g) = 0.014 mW/g Maximum value of SAR (measured) = 0.036 mW/g

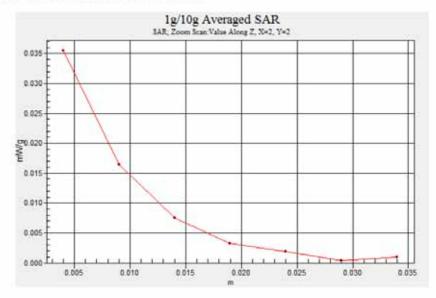



Test Laboratory: Sporton International Inc. SAR Testing Lab Date:

Date: 2007/5/28

#### Body\_802.11g Ch1\_Keypad Down with 1.5cm Gap\_2D

DUT: 742004

Communication System: 802.11g; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: MSL\_2450 Medium parameters used: f = 2412 MHz;  $\sigma = 1.9$  mho/m;  $\epsilon_r = 52.5$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature : 22.6 °C; Liquid Temperature : 21.3 °C

DASY4 Configuration:


- Probe: ET3DV6 - SN1787; ConvF(4.13, 4.13, 4.13); Calibrated: 2006/5/31

- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch1/Area Scan (61x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.026 mW/g

Ch1/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.15 V/m; Power Drift = -0.435 dB Peak SAR (extrapolated) = 0.045 W/kg SAR(1 g) = 0.025 mW/g; SAR(10 g) = 0.013 mW/g Maximum value of SAR (measured) = 0.028 mW/g

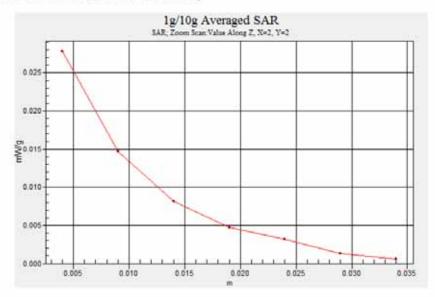



## Appendix C – Calibration Data

Client

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Sporton (Auden)

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates CREATE S

SAINSS

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 108

s

Certificate No: D2450V2-736\_Jul05

bject	D2450V2 - SN: 7	36	
Calibration procedure(s)	QA CAL-05.v6 Calibration proce	dure for dipole validation kits	
aibration date	July 12, 2005		
ondition of the calibrated item	In Tolerance		
Il calibrations have been conduc	cted in the closed laborator	robability are given on the following pages and an ny facility: environment temperature (22 ± 3)°C and	
alloration Equipment used (M&)	re chical for calibration)		
	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
rimary Standards ower meter EPM E442	1.517	Cal Date (Calibrated by, Certificate No.) 12-Oct-04 (METAS, No. 251-00412)	Scheduled Calibration Oct-05
rimary Standards ower meter EPM E442 ower sensor HP 8481A	ID # GB37480704 US37292783	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412)	Oct-05 Oct-05
rimary Standards ower meter EPM E442 ower sensor HP 8481A eference 20 dB Attenuator	ID # GB37480704 US37292783 SN: 5085 (20g)	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No 251-00402)	Oct-05 Oct-05 Aug-05
rimary Standards ower meter EPM E442 ower sensor HP 8481A eference 20 dB Attenuator eference 10 dB Attenuator	ID # GB37480704 US37292763 SN: 5085 (20g) SN: 5085 (20g) SN: 5047.2 (10r)	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No 251-00402) 10-Aug-04 (METAS, No 251-00402)	Oct-05 Oct-05 Aug-05 Aug-05
rimary Standards ower meter EPM E442 ower sensor HP 8481A eference 20 dB Attenuator eference 10 dB Attenuator eference Probe ES3DV2	ID # GB37480704 US37292763 SN: 5085 (20g) SN: 5087 (2 (10r) SN 3025	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No 251-00402) 10-Aug-04 (METAS, No 251-00402) 28-Oct-04 (SPEAG, No. ES3-3025_Oct04)	Oct-05 Oct-05 Aug-05 Aug-05 Oct-05
rimary Standards ower meter EPM E442 ower sensor HP 8481A telerence 20 dB Attenuator telerence 10 dB Attenuator telerence Probe ES3DV2	ID # GB37480704 US37292763 SN: 5085 (20g) SN: 5087.2 (10r)	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No 251-00402) 10-Aug-04 (METAS, No 251-00402)	Oct-05 Oct-05 Aug-05 Aug-05
rrimary Standards lower meter EPM E442 lower sensor HP 8461A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 0AE4	ID # GB37480704 US37292763 SN: 5085 (20g) SN: 5087 (2 (10r) SN 3025	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No 251-00402) 10-Aug-04 (METAS, No 251-00402) 28-Oct-04 (SPEAG, No. ES3-3025_Oct04)	Oct-05 Oct-05 Aug-05 Aug-05 Oct-05
Primary Standards Power meter EPM E442 Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	ID # GB37480704 US37292783 SN: 5085 (20g) SN: 5047.2 (10r) SN 3025 SN 601	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No 251-00402) 10-Aug-04 (METAS, No 251-00402) 28-Oct-04 (SPEAG, No. ES3-3025_Oct04) 07-Jan-05 (SPEAG, No. DAE4-601_Jan05)	Oct-05 Oct-05 Aug-05 Aug-05 Oct-05 Jan-06
rimary Standards lower meter EPM E442 lower sensor HP 8461A leference 20 dB Attenuator telerence 10 dB Attenuator telerence Probe ES3DV2 ME4 lecondary Standards lower sensor HP 8461A	ID # GB37480704 US37292783 SN: 5085 (20g) SN: 5047.2 (10r) SN 3025 SN 601 ID #	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No 251-00402) 10-Aug-04 (METAS, No 251-00402) 29-Oct-04 (SPEAG, No. ES3-3025_Oct04) 07-Jan-05 (SPEAG, No. DAE4-601_Jan05) Check Date (in house)	Oct-05 Oct-05 Aug-05 Aug-05 Oct-05 Oct-05 Jan-06 Scheduled Check
Primary Standards Power meter EPM E442 Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Recondary Standards Power sensor HP 8461A RE generator R&S SML-03	ID # GB37480704 US37292783 SN: 5085 (20g) SN: 5047.2 (10r) SN 3025 SN 601 ID # MY41092317	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No. 251-00402) 10-Aug-04 (METAS, No. 251-00402) 29-Oct-04 (SPEAG, No. ES3-3025_Oct04) 07-Jan-05 (SPEAG, No. DAE4-601_Jan05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-03)	Oct-05 Oct-05 Aug-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Oct-05
Primary Standards Power meter EPM E442 Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SML-03	ID # GB37480704 US37292763 SN: 5085 (20g) SN: 5047.2 (10r) SN 3025 SN 601 ID # MY41092317 100698 US37390585 54206	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No. 251-00402) 10-Aug-04 (METAS, No. 251-00402) 29-Oct-04 (SPEAG, No. ES3-3025_Oct04) 07-Jan-05 (SPEAG, No. DAE4-601_Jan05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-03) 27-Mar-02 (SPEAG, in house check Dec-03) 18-Oct-01 (SPEAG, in house check Nov-04)	Oct-05 Oct-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Oct-05 In house check: Dec-05 In house check: Nav-05
rrimary Standards lower meter EPM E442 lower sensor HP 8461A Reference 20 dB Attenuator telerence 10 dB Attenuator telerence Probe ES30V2 AE4 Becondary Standards lower sensor HP 8461A FF generator R&S SML-03 letwork Analyzer HP 8753E	ID # GB37480704 US37292783 SN: 5085 (20g) SN: 5047.2 (10r) SN 3025 SN 601 ID # MY41092317 100598	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No 251-00402) 10-Aug-04 (METAS, No 251-00402) 29-Oct-04 (SPEAG, No. ES3-3025_Oct04) 07-Jan-05 (SPEAG, No. DAE4-601_Jan05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-03) 27-Mar-02 (SPEAG, in house check Dec-03)	Oct-05 Oct-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check Oct-05 In house check Dec-05 In house check Nav-05 Signature
rimary Standards lower meter EPM E442 ower sensor HP 8461A leterence 20 dB Attenuator leterence 10 dB Attenuator leterence 10 dB Attenuator leterence Probe ES30V2 WE4 econdary Standards lower sensor HP 8451A /F generator R&S SML-03 letwork Analyzer HP 8753E	ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN 3025 SN 601 ID # MY41092317 100698 US37390585 S4206 Name	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No 251-00402) 10-Aug-04 (METAS, No 251-00402) 29-Oct-04 (SPEAG, No. ES3-3025_Oct04) 07-Jan-05 (SPEAG, No. DAE4-601_Jan05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-03) 27-Mar-02 (SPEAG, in house check Dec-03) 18-Oct-01 (SPEAG, in house check Nov-04) Function	Oct-05 Oct-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Oct-05 In house check: Dec-05 In house check: Nav-05
Primary Standards Power meter EPM E442 Power sensor HP 8461A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 AAE4 Secondary Standards Power sensor HP 8461A RF generator R&S SML-03 Network Analyzer HP 8753E Calibrated by	ID # GB37480704 US37292783 SN: 5085 (20g) SN: 5047.2 (10r) SN 3025 SN 601 ID # MY41092317 100698 US37390585 S4206 Name Mike Meili	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No. 251-00402) 10-Aug-04 (METAS, No. 251-00402) 29-Oct-04 (SPEAG, No. 251-00402) 29-Oct-04 (SPEAG, No. DAE4-601_Jan05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-03) 27-Mar-02 (SPEAG, in house check Oct-03) 18-Oct-01 (SPEAG, in house check Nov-04) Function Laboratory Technician	Oct-05 Oct-05 Aug-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Oct-05 In house check: Dec-05 In house check: Dec-05 Signature H. H. C. N.
rrimary Standards Power meter EPM E442 Power sensor HP 8461A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 AAE4 Secondary Standards Power sensor HP 8461A RF generator R&S SML-03 Reference R&S SML-03 Reference PR 8753E Calibrated by:	ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN 3025 SN 601 ID # MY41092317 100698 US37390585 S4206 Name	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No 251-00402) 10-Aug-04 (METAS, No 251-00402) 29-Oct-04 (SPEAG, No. ES3-3025_Oct04) 07-Jan-05 (SPEAG, No. DAE4-601_Jan05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-03) 27-Mar-02 (SPEAG, in house check Dec-03) 18-Oct-01 (SPEAG, in house check Nov-04) Function	Oct-05 Oct-05 Aug-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Oct-05 In house check: Dec-05 In house check: Dec-05 Signature H. H. C. N.
Calibration Equipment used (M&T Primary Standards Power sensor HP 8481A Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 3AE4 Secondary Standards Tower sensor HP 8451A RF generator R&S SML-03 Network Analyzer HP 8753E Calibrated by:	ID # GB37480704 US37292783 SN: 5085 (20g) SN: 5047.2 (10r) SN 3025 SN 601 ID # MY41092317 100698 US37390585 S4206 Name Mike Meili	12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No. 251-00402) 10-Aug-04 (METAS, No. 251-00402) 29-Oct-04 (SPEAG, No. 251-00402) 29-Oct-04 (SPEAG, No. DAE4-601_Jan05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-03) 27-Mar-02 (SPEAG, in house check Oct-03) 18-Oct-01 (SPEAG, in house check Nov-04) Function Laboratory Technician	Oct-05 Oct-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Oct-05 In house check: Dec-05 In house check: Nav-05 Signature

Certificate No: D2450V2-736\_Jul05

Page 1 of 9

## ©2007 SPORTON International Inc. SAR Testing Lab



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



S

С

s

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

d) DASY4 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D2450V2-736 Jul05

Page 2 of 9



#### Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.6
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Area Scan resolution	dx, dy = 15 mm	
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

#### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.5 ± 6 %	1.73 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) *C		

#### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	condition	
SAR measured	250 mW input power	13.1 mW / g
SAR normalized	normalized to 1W	52.4 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	52.8 mW / g ± 17.0 % (k=2)
SAR averaged over 10 cm <sup>2</sup> (10 g) of Head TSL	condition	
SAR averaged over 10 cm <sup>2</sup> (10 g) of Head TSL SAR measured	condition 250 mWV input power	6.13 mW / g
		6.13 mW / g 24.5 mW / g

<sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D2450V2-736\_Jul05

Page 3 of 9



## Body TSL parameters

The following parameters and calculations were applied.

4

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.2 ± 0.2) °C	52.5 ± 6 %	2.02 mho/m ± 8 %
Body TSL temperature during test	(22.2 ± 0.2) *C		

## SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	condition	
SAR measured	250 mW input power	13.5 mW / g
SAR normalized	normalized to 1W	54.0 mW / g
SAR for nominal Body TSL parameters 2	normalized to 1W	52.8 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.26 mW / g
SAR normalized	normalized to 1W	25.0 mW / g
SAR for nominal Body TSL parameters 2	normalized to 1W	24.5 mW / g ± 16.5 % (k=2)

<sup>2</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D2450V2-736\_Jul05

Page 4 of 9



#### Appendix

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.6 Ω + 3.7 jΩ	
Return Loss	-26.0 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.9 Ω + 5.3 jΩ	
Return Loss	- 25.5 dB	

#### General Antenna Parameters and Design

4

Electrical Delay (one direction)	1.157 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

Manufactured by	SPEAG	
Manufactured on	August 26, 2003	

Certificate No: D2450V2-736\_Jul05

Page 5 of 9



#### **DASY4 Validation Report for Head TSL**

Date/Time: 12.07.2005 12:53:00

Test Laboratory: SPEAG, Zurich, Switzerland

#### DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN736

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: HSL U10 BB Medium parameters used: f = 2450 MHz;  $\sigma$  = 1.73 mho/m;  $\epsilon_e$  = 38.5;  $\rho$  = 1000 kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:


- Probe: ES3DV2 SN3025; ConvF(4.4, 4.4, 4.4); Calibrated: 29.10.2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 22.07.2004
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA
- Measurement SW: DASY4, V4.5 Build 30; Postprocessing SW: SEMCAD, V1.8 Build 149

Pin = 250 mW; d = 10 mm 2/Area Scan (41x61x1):

Measurement grid: dx=15mm, dy=15mm


Maximum value of SAR (interpolated) = 16.6 mW/g

Pin = 250 mW; d = 10 mm 2/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 91.6 V/m; Power Drift = 0.077 dB Peak SAR (extrapolated) = 27.0 W/kg SAR(1 g) = 13.1 mW/g; SAR(10 g) = 6.13 mW/g Maximum value of SAR (measured) = 15.0 mW/g

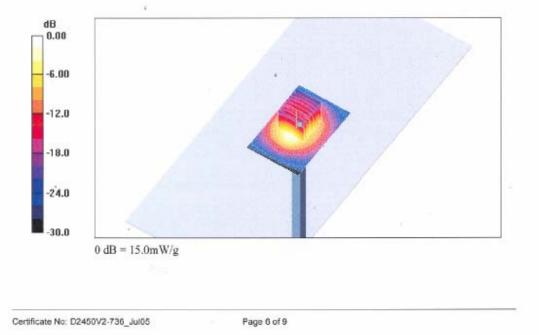



## Impedance Measurement Plot for Head TSL

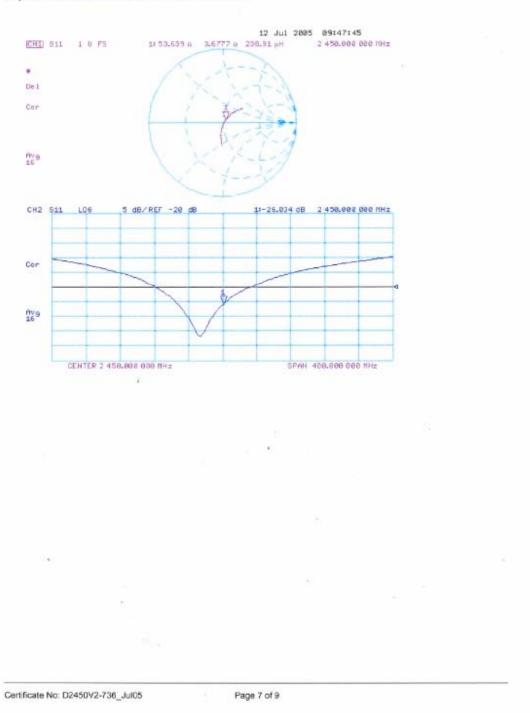



#### DASY4 Validation Report for Body TSL

Date/Time: 11.07.2005 17:33:35

Test Laboratory: SPEAG, Zurich, Switzerland

#### DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN736

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: MSL 2450 Medium parameters used: f = 2450 MHz;  $\sigma$  = 2.02 mho/m;  $\epsilon_r$  = 52.5;  $\rho$  = 1000 kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)


DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.13, 4.13, 4.13); Calibrated: 29.10.2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601: Calibrated: 22.07.2004
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA
- Measurement SW: DASY4, V4.6 Build 4; Postprocessing SW: SEMCAD, V1.8 Build 149

Pin = 250 mW; d = 10 mm/Area Scan (81x81x1): Measurement grid: dx=15mm, dy=15mm


Maximum value of SAR (interpolated) = 15.8 mW/g

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx-5mm, dy-5mm, dz-5mm Reference Value = 85.9 V/m; Power Drift = 0.160 dB Peak SAR (extrapolated) = 27.6 W/kg SAR(1 g) = 13.5 mW/g; SAR(10 g) = 6.26 mW/g Maximum value of SAR (measured) = 15.5 mW/g

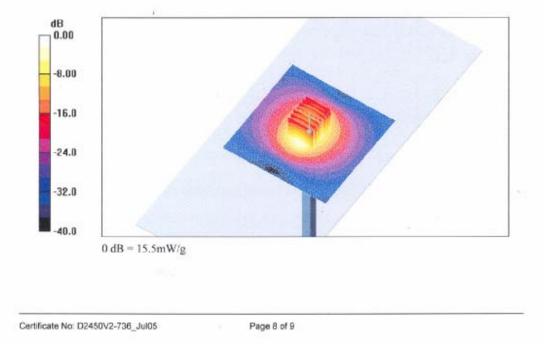



## Impedance Measurement Plot for Body TSL

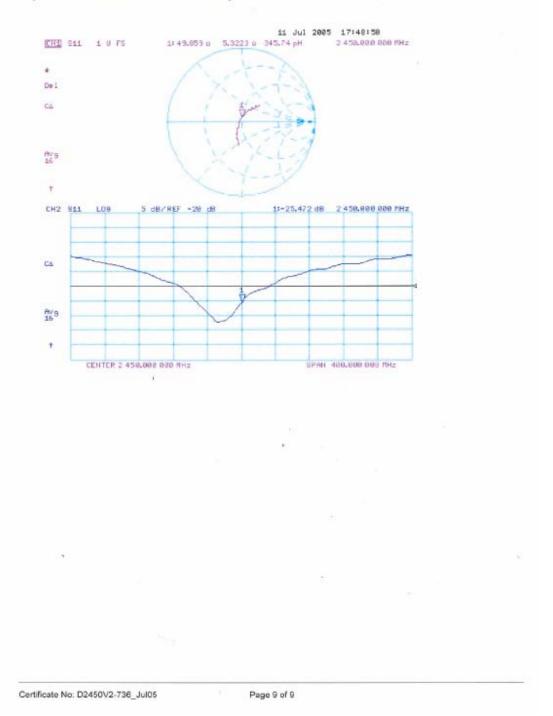



consultant has then Student Enclosed.			
he Swiss Accreditation Service	Office of Metrology and A		.: SCS 108
luitilateral Agreement for the	승규는 방법이 집에 가지 않는 것 같아. 가지 않는 것 같아. 가지 않는 것이 같아. 나는 것이 않 것이 같아. 나는 것이 같아. 아. 나는 것이 같아. 나는 않 않아. 아. 나는 것이 같아. 나는 것이 않아. 나는 것이 않아. 나는 것이 않아. 나는 것이 않아		
and the second se	2		TO 4707 May 66
lient Sporton (Aude	en)	Certificate No: E	T3-1787_May06
CALIBRATION	CERTIFICAT	F	
ALIDITATION	OLIVIII IOAI		
Dbject	ET3DV6 - SN: 1	(707	100 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0
and an a	E10040-014.	1101	AND PERSON AND ADDRESS OF THE PARTY OF
Calibration procedure(s)	QA CAL-01.v5	IN SOUTH AND	
	Calibration proc	edure for dosimetric E-field probes	
	The second second second		CONTRACTOR OF STREET, ST.
Calibration data:	May 31, 2006		and the second fit
Condition of the calibrated item	In Tolerance	entered birth the second second second second second	Contraction of the
	in i unuturiou		A REAL PROPERTY OF A REAL PROPER
The measurements and the unc	nents the traceability to re entainties with confidence	ational standards, which realize the physical units o probability are given on the following pages and ar tory facility: environment temperature (22 ± 3)°C an	e part of the certificate.
The measurements and the uno All calibrations have been condu	nents the traceability to ru estainties with confidence ucted in the closed laborat	probability are given on the following pages and ar lory facility: environment temperature (22 $\pm$ 3)°C an	e part of the certificate.
The measurements and the uno Of calibrations have been condu- Calibration Equipment used (M8	nents the traceability to ru estainties with confidence ucted in the closed laborat .TE-catical for calibration)	probability are given on the following pages and ar long facility: environment temperature (22 $\pm$ 3)°C an	e part of the certificate. d humidity < 70%.
The measurements and the uno All calibrations have been condu Calibration Equipment used (M8 Primary Standards	nents the traceability to ru estainties with confidence ucted in the closed laborat	probability are given on the following pages and ar lory facility: environment temperature (22 ± 3)°C an Cal Data (Calibrated by, Certificate No.)	e part of the certificate.
The measurements and the uno All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter E44198	nents the traceability to n estainties with confidence acted in the closed laborat CTE-critical for calibration)	probability are given on the following pages and ar long facility: environment temperature (22 $\pm$ 3)°C an	e part of the certificate. d humidity < 70%. Scheduled Calibration
The measurements and the uno All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A	nents the traceability to ru entainties with confidence inded in the closed laborat TE-critical for calibration) ID # GB41293874	probability are given on the following pages and an lory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 5-Apr-05 (METAS, No. 251-00557)	e part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07
The measurements and the uno All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power sensor E4412A Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator	nents the traceability to re estainties with confidence octed in the closed laboral TE-unitical for calibration) ID # GB41293874 MY41498067 SN: S5054 (3c)	probability are given on the following pages and an lory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 5-Apr-08 (METAS, No. 251-00557) 5-Apr-08 (METAS, No. 251-00557) 5-Apr-08 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00499)	s part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07 Apr-07 Apr-07 Apr-06
The measurements and the uno All calibrations have been condu Calibration Equipment used (M& Primary Standards Prover sensor E4412A Prover sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator	nents the traceability to re estainties with confidence octed in the closed laboral TE-critical for calibration) ID # GB41293874 MY41498087 SN: S5054 (3c) SN: S5058 (20b)	probability are given on the following pages and ar lory facility: environment temperature (22 ± 3)°C an Call Date (Calibrated by, Certificate No.) 5-Apr-08 (METAS, No. 251-00557) 5-Apr-08 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00499) 4-Apr-08 (METAS, No. 251-00558)	e part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07 Apg-06 Apr-07
The measurements and the uno All calibrations have been condu Calibration Equipment used (M& Primary Standards Prover sensor E44198 Power sensor E4412A Reference 3 dE Attenuator Reference 3 dE Attenuator Reference 3 dE Attenuator	Annual state traceability to rule attainties with confidence incled in the closed laborat TE-critical for calibration) ID # GB41293874 MY41495087 MY41495087 SN: S5054 (3c) SN: S5054 (3c) SN: S5058 (20b) SN: S5129 (30b)	probability are given on the following pages and ar lory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) S-Apr-08 (METAS, No. 251-00557) S-Apr-08 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00499) 4-Apr-08 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00500)	s part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07 Apr-06 Apr-06 Apr-06
The measurements and the uno All calibrations have been condu- Calibration Equipment used (M8 Primary Standards Power meter E44198 Power sonsor E4412A Reference 3 dE Attenuator Reference 9 dB Attenuator Reference Probe ES3DV2	nents the traceability to re estainties with confidence octed in the closed laboral TE-critical for calibration) ID # GB41293874 MY41498087 SN: S5054 (3c) SN: S5058 (20b)	probability are given on the following pages and ar lory facility: environment temperature (22 ± 3)°C an <u>Cal Date (Calibrated by, Certificate No.)</u> 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00569) 2-Jan-06 (SPEAG, No. ES3-3013' Jan06)	e part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07 Apg-06 Apr-07
The measurements and the uno All calibrations have been condu- Calibration Equipment used (M8 Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dE Attenuator Reference 3 dE Attenuator Reference 3 dE Attenuator Reference 3 dE Attenuator Reference 9 dB Attenuator	nents the traceability to re estainties with confidence acted in the closed laboral TE-critical for calibration) ID # G841293874 MY41405277 MY41405277 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5055 (3c) SN: S5029 (30b) SN: S013	probability are given on the following pages and ar lory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) S-Apr-08 (METAS, No. 251-00557) S-Apr-08 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00499) 4-Apr-08 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00500)	s part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07 Apr-06 Apr-06 Apr-06 Apr-06 Apr-07 Aug-06 Jan-07
The measurements and the uno All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meters: E44198 Power sensor: E4412A Power sensor: E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	nents the traceability to ru estainties with confidence octed in the closed laboral TE-critical for calibration) ID # GB41293874 MY41495277 MY41495087 SN: S50854 (3c) SN: S50854 (3c) SN: S50855 (30c) SN: S5129 (30c) SN: S5129 (30c) SN: S513 SN: S54 ID #	probability are given on the following pages and an lory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 5-Apr-08 (METAS, No. 251-00557) 5-Apr-08 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-06 (SPEAG, No. 253-3013, Jan06) 2-Jan-06 (SPEAG, No. DAE4-654, Feb06) Check Date (in house)	e part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07 Apr-07 Apr-06 Apr-17 Aug-06 Jan-07 Feb-07 Scheduled Check
The measurements and the uno All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	nents the traceability to ru ettainties with confidence incled in the closed laboral ID # GB41293874 MY414950874 MY41495087 MY41495087 SN: S5054 (3c) SN: S5054 (3c) SN: S5055 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: S013 SN: 654 ID # US3642U01700	probability are given on the following pages and ar tory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 5-Apr-05 (METAS, No. 251-00557) 5-Apr-05 (METAS, No. 251-00557) 5-Apr-05 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-06 (SPEAG, No. DAE4-654_Feb00) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-05)	e part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-06 Apr-07 Aug-06 Jan-07 Feb-07 Scheduled Check In house check: Nov-07
The measurements and the uno All calibrations have been condu- Calibration Equipment used (M8 Primary Standards Power series E44136 Power series E4413A Power series E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Recondary Standards RF generator HP 8648C	nents the traceability to ru estainties with confidence octed in the closed laboral TE-critical for calibration) ID # GB41293874 MY41495277 MY41495087 SN: S50854 (3c) SN: S50854 (3c) SN: S50855 (30c) SN: S5129 (30c) SN: S5129 (30c) SN: S513 SN: S54 ID #	probability are given on the following pages and an lory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 5-Apr-08 (METAS, No. 251-00557) 5-Apr-08 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-06 (SPEAG, No. 253-3013, Jan06) 2-Jan-06 (SPEAG, No. DAE4-654, Feb06) Check Date (in house)	e part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07 Apr-07 Apr-06 Apr-17 Aug-06 Jan-07 Feb-07 Scheduled Check
The measurements and the uno All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	nents the traceability to ru ettainties with confidence incled in the closed laboral ID # GB41293874 MY414950874 MY41495087 MY41495087 SN: S5054 (3c) SN: S5054 (3c) SN: S5055 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: S013 SN: 654 ID # US3642U01700	probability are given on the following pages and ar tory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 5-Apr-05 (METAS, No. 251-00557) 5-Apr-05 (METAS, No. 251-00557) 5-Apr-05 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-06 (SPEAG, No. DAE4-654_Feb00) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-05)	e part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-06 Apr-07 Aug-06 Jan-07 Feb-07 Scheduled Check In house check: Nov-07
The measurements and the uno All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor E44198 Power sensor E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C setwork Analyzer HP 8753E	nents the traceability to n estainties with confidence acted in the closed laboral TE-critical for calibration) ID # GB41293874 MY41405277 MY41405277 MY41405277 MY41405277 SN: S5054 (3c) SN: S5054 (3c) SN: S5054 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37300565 Name	probability are given on the following pages and ar tory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00558) 12-Be-06 (SPEAG, No. DAE4-654 [Feb06] Check Date (in house) 4-Aug-59 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05) Function	e part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-06 Apr-07 Aug-06 Jan-07 Feb-07 Scheduled Check In house check: Nov-07 In house check: Nov-06
The measurements and the uno All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 9 Tobe ES30V2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	nents the traceability to n estainties with confidence acted in the closed laboral (TE-critical for calibration) ID # GB41293874 MY41498087 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5058 (20b) SN: S5058 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: S013 SN: 654 ID # US3642U01700 US37390585	probability are given on the following pages and ar tory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00558) 12-Be-06 (SPEAG, No. DAE4-654, Feb06) Check Date (in house) 4-Aug-99 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	e part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-06 Apr-07 Aug-06 Jan-07 Feb-07 Scheduled Check In house check: Nov-07 In house check: Nov-06
The measurements and the uno All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dE Attenuator Reference 30 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES30V2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	nents the traceability to ru entainties with confidence acted in the closed laboral TE-critical for calibration) ID # GB41293874 MY41495277 MY41495067 SN: S5054 (3c) SN: S5085 (20b) SN: S5085 (20b) SN: S5085 (20b) SN: 3013 SN: 654 ID # US3642U01700 US37390565 Name Katja Potovic	probability are given on the following pages and an lory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 5-Apr-08 (METAS, No. 251-00557) 5-Apr-08 (METAS, No. 251-00557) 5-Apr-08 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00508) 2-Jan-06 (SPEAG, No. DAE4-054, Feb06) 2-Feb-06 (SPEAG, No. DAE4-054, Feb06) Check Date (in house) 4-Aug-59 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05) Function Technicol Manager	e part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-06 Apr-07 Aug-06 Jan-07 Feb-07 Scheduled Check In house check: Nov-07 In house check: Nov-06
The measurements and the uno All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 9 Tobe ES30V2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	nents the traceability to n estainties with confidence acted in the closed laboral TE-critical for calibration) ID # GB41293874 MY41405277 MY41405277 MY41405277 MY41405277 SN: S5054 (3c) SN: S5054 (3c) SN: S5054 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37300565 Name	probability are given on the following pages and ar tory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00558) 12-Be-06 (SPEAG, No. DAE4-654 [Feb06] Check Date (in house) 4-Aug-59 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05) Function	e part of the certificate. Id humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-06 Apr-07 Aug-06 Jan-07 Feb-07 Scheduled Check In house check: Nov-07 In house check: Nov-06



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



CR D Z

S Schweizerischer Kalibrierdienst

C Service suisse d'étalonnage

Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
Polarization $\phi$	o rotation around probe axis
Polarization 9	S rotation around an axis that is in the plane normal to probe axis (at
	measurement center), i.e., 8 = 0 is normal to probe axis

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This
  linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of
  the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of
  power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a
  flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ET3-1787\_May06

Page 2 of 9



ET3DV6 SN:1787

May 31, 2006

# Probe ET3DV6

## SN:1787

Manufactured: Last calibrated: Recalibrated: May 28, 2003 August 29, 2003 May 31, 2006

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

20 V

Certificate No: ET3-1787\_May06

Page 3 of 9





### ET3DV6 SN:1787

May 31, 2006

## DASY - Parameters of Probe: ET3DV6 SN:1787

Sensitivity in Free Space<sup>A</sup> Diode Compression<sup>B</sup> NormX  $1.57 \pm 10.1\%$  $\mu V/(V/m)^2$ DCP X 94 mV  $\mu V/(V/m)^2$ NormY 1.71 ± 10.1% DCP Y 94 mV  $\mu V/(V/m)^2$ NormZ  $2.09 \pm 10.1\%$ DCP Z 94 mV Sensitivity in Tissue Simulating Liquid (Conversion Factors) Please see Page 8. Boundary Effect TSL Typical SAR gradient: 5 % per mm 900 MHz 3.7 mm 4.7 mm Sensor Center to Phantom Surface Distance SAR ... [%] Without Correction Algorithm 7.2 3.8 SAR<sub>bs</sub> [%] 0.0 0.2 With Correction Algorithm 1810 MHz Typical SAR gradient: 10 % per mm TSL Sensor Center to Phantom Surface Distance 3.7 mm 4.7 mm SAR<sub>6+</sub> [%] Without Correction Algorithm 6.3 3.6 SAR<sub>bo</sub> [%] 0.3 With Correction Algorithm 0.1 Sensor Offset Probe Tip to Sensor Center 2.7 mm The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. \* The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 8). \* Numerical linearization parameter: uncertainty not required.

Certificate No: ET3-1787\_May08

Page 4 of 9





ET3DV6 SN:1787

May 31, 2006

## (TEM-Cell:ifi110 EXX, Waveguide: R22) 1.5 1.4 1.3 Frequency response (normalized) 1.2 1.1 1.0 0.9 0.8 0.7 0.6 0.5 3000 0 1000 1500 2500 500 2000 f [MHz] --- TEM

## Frequency Response of E-Field

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Certificate No: ET3-1787\_May06

Page 5 of 9




ET3DV6 SN:1787

May 31, 2006

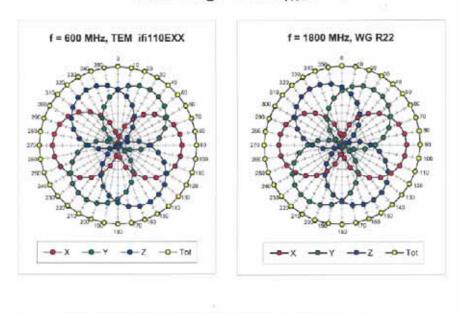

## Receiving Pattern (\$), 9 = 0°

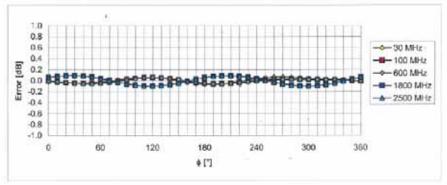


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: ET3-1787\_May06

Page 6 cf 9



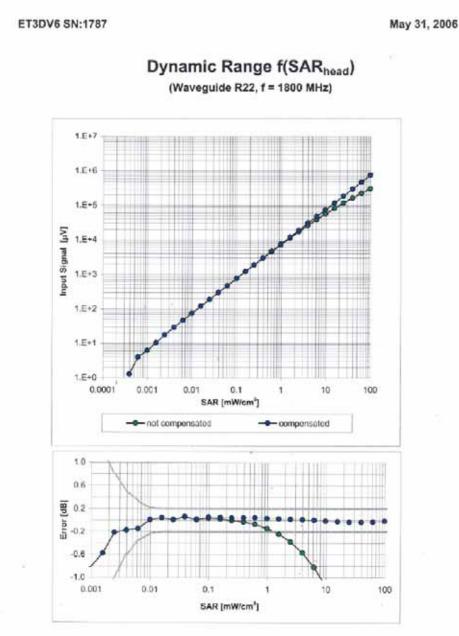

Uncertainty of Linearity Assessment: ± 0.6% (k=2)


Certificate No: ET3-1787\_May06

Page 7 of 9



#### ET3DV6 SN:1787

```
May 31, 2006
```

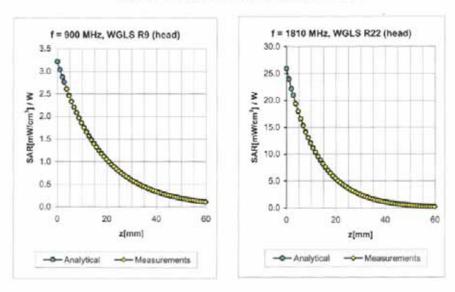

## **Conversion Factor Assessment**

Validity [MHz] <sup>C</sup>	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
± 50 / ± 100	Head	41.5±5%	0.97 ± 5%	0.50	1.85	6.38 ± 11.0% (k=2)
± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.59	2.46	5.26 ± 11.0% (k=2)
± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.44	2.10	6.18 ± 11.0% (k=2)
± 50 / ± 100	Body	53.3 ± 5%	$1.52 \pm 5\%$	0.62	2.44	4.66 ± 11.0% (k=2)
± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.62	2.13	4.13 ± 11.8% (k=2)
	± 50 / ± 100 ± 50 / ± 100 ± 50 / ± 100 ± 50 / ± 100	± 50 / ± 100 Head ± 50 / ± 100 Head ± 50 / ± 100 Body ± 50 / ± 100 Body	± 50 / ± 100 Head 41.5 ± 5% ± 50 / ± 100 Head 40.0 ± 5% ± 50 / ± 100 Body 55.0 ± 5% ± 50 / ± 100 Body 53.3 ± 5%	± 50 / ± 100 Head 41.5 ± 5% 0.97 ± 5% ± 50 / ± 100 Head 40.0 ± 5% 1.40 ± 5% ± 50 / ± 100 Body 55.0 ± 5% 1.05 ± 5% ± 50 / ± 100 Body 53.3 ± 5% 1.52 ± 5%	± 50 / ± 100 Head 41.5 ± 5% 0.97 ± 5% 0.50 ± 50 / ± 100 Head 40.0 ± 5% 1.40 ± 5% 0.59 ± 50 / ± 100 Body 55.0 ± 5% 1.05 ± 5% 0.44 ± 50 / ± 100 Body 53.3 ± 5% 1.52 ± 5% 0.62	± 50 / ± 100 Head 41.5 ± 5% 0.97 ± 5% 0.50 1.85 ± 50 / ± 100 Head 40.0 ± 5% 1.40 ± 5% 0.59 2.46 ± 50 / ± 100 Body 55.0 ± 5% 1.05 ± 5% 0.44 2.10 ± 50 / ± 100 Body 53.3 ± 5% 1.52 ± 5% 0.62 2.44

<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Certificate No: ET3-1787\_May06


Page 8 of 9



ET3DV6 SN:1787

May 31, 2006

## Deviation from Isotropy in HSL Error (¢, 3), f = 900 MHz

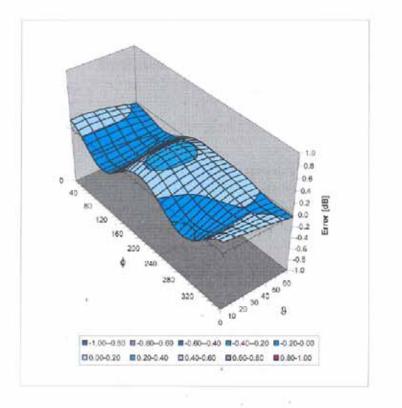

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)



Page 9 of 9

©2007 SPORTON International Inc. SAR Testing Lab



chmid & Partner Engineering AG ughausstrasse 43, 8004 Zuric	y of		hweizerischer Kalibrierdienst nvice suisse d'étalonnage ervizio svizzero di taratura wiss Calibration Service
coredited by the Swiss Federal ( he Swiss Accreditation Servic) ultilateral Agreement for the n	e is one of the signator	ies to the EA	: SCS 108
lient Sporton (Aude	1999. <del>3</del> . 1999 1997 1998		T3-1788_Sep06
CALIBRATION C	ERTIFICAT	E	
Object	ET3DV6 - SN:1	788	
Calibration procedure(s)	QA CAL-01.v5 Calibration proc	edure for dosimetric E-field probes	
Calibration date:	September 19, 2	2006	· · · · · · · · · · · · · · · · · · ·
Condition of the calibrated item	In Tolerance		
The measurements and the unce	rtainties with confidence	ational standards, which realize the physical units of probability are given on the following pages and arr ory facility: environment temperature (22 ± 3)°C arr	e part of the certificate.
The measurements and the unce	rtainties with confidence	probability are given on the following pages and are ony facility: environment temperature $(22 \pm 3)$ *C and	e part of the certificate.
The measurements and the unce All celibrations have been conclu- Calibration Equipment used (M& Primary Standards	rtainties with confidence cted in the closed laborat TE:critical for calibration)	probability are given on the following pages and arr ory facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.)	a part of the certificate. d humidity < 70%. Scheduled Calibration
The measurements and the unce All celibrations have been conduc Celibration Equipment used (M& Primary Standards Power meter E44198	rtainties with confidence ated in the closed laborat TE-critical for calibration)	probability are given on the following pages and are ory facility: environment temperature (22 ± 3)*C and Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A	rtainties with confidence cted in the closed laborat TE-critical for calibration) ID # GB41293874 MY41495277	probability are given on the following pages and are ony facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07
The measurements and the unce All celibrations have been conduc Celibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A	rtainties with confidence cted in the closed laborat TE-critical for calibration) ID # GB41293874 MY41495277 MY41498087	probability are given on the following pages and arr ory facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07
The measurements and the unce All calibrations have been condu- Calibration Equipment used (M& Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator	rtainties with confidence cted in the closed laborat TE-critical for calibration) ID # GB41293874 MY41495277	probability are given on the following pages and are ony facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07
The measurements and the unce All celibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator	rtainties with confidence ted in the closed laborat TErcritical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c)	probability are given on the following pages and are ony facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 217-00592) 10-Aug-06 (METAS, No. 217-00593)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-07 Aug-07 Aug-07 Aug-07
The measurements and the unce All celibrations have been conduct Celibration Equipment used (M& Primary Standards Power sensor E44198 Power sensor E4412A Power sensor E4412A Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator	rtainties with confidence cted in the closed laborat TE-critical for calibration) ID # GB41293874 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: 3013	probability are given on the following pages and arr ory facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 217-00593) 10-Aug-06 (METAS, No. 217-00593) 10-Aug-06 (METAS, No. 217-00593) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07 Aug-07 Aug-07 Jan-07
The measurements and the unce All celibrations have been conduct Celibration Equipment used (M& Primary Standards Power sensor E44198 Power sensor E4412A Power sensor E4412A Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator	rtainties with confidence ated in the closed laborat TE-critical for calibration) ID # GB41293874 MY41495277 MY4149807 SN: S5086 (20b) SN: S5086 (20b) SN: S5129 (30b)	probability are given on the following pages and are ony facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 217-00592) 10-Aug-06 (METAS, No. 217-00593)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-07 Aug-07 Aug-07 Aug-07
The measurements and the unce	rtainties with confidence cted in the closed laborat TE-critical for calibration) ID # GB41293874 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: 3013	probability are given on the following pages and arr ory facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 217-00593) 10-Aug-06 (METAS, No. 217-00593) 10-Aug-06 (METAS, No. 217-00593) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07 Aug-07 Aug-07 Jan-07
The measurements and the unce All celibrations have been conduct Celibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 90 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	rtainties with confidence ted in the closed laborat TE-critical for calibration) ID # GB41293874 MY41495077 MY41495077 MY41495077 SN: S5054 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: 3013 SN: 654	probability are given on the following pages and arr ony facility: environment temperature (22 ± 3)°C and 5-Apr-06 (METAS, No. 251-00557)           5-Apr-06 (METAS, No. 251-00557)           5-Apr-06 (METAS, No. 251-00557)           5-Apr-06 (METAS, No. 251-00557)           10-Aug-06 (METAS, No. 251-00558)           10-Aug-06 (METAS, No. 217-00592)           4-Apr-06 (METAS, No. 217-00558)           10-Aug-06 (METAS, No. 217-00593)           2-Jan-06 (SPEAG, No. ES3-3013_Jan06)           21-Jun-06 (SPEAG, No. DAE4-654_Jun06)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07 Aug-07 Aug-07 Aug-07 Jun-07 Jun-07
The measurements and the unce All celibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	rtainties with confidence cted in the closed laborat TE-critical for calibration) ID # GB41253874 MY41495277 MY41498087 SN: \$5054 (3c) SN: \$5058 (20b) SN: \$5129 (30b) SN: \$5129 (30b) SN: \$614 ID #	probability are given on the following pages and are ony facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 251-00552) 4-Apr-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 217-00593) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06) 21-Jun-06 (SPEAG, No. DAE4-654_Jun06) Chack Date (in house)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-07 Aug-07 Aug-07 Jun-07 Jun-07 Scheduled Check
The measurements and the unce All celibrations have been conduct Celibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	rtainties with confidence cted in the closed laborat TE-critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5029 (30b) SN: S5129 (30b) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3842U01700	probability are given on the following pages and arr ory facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 217-00593) 10-Aug-06 (METAS, No. 217-00593) 2-Jan-06 (SPEAG, No. 283-3013_Jan06) 21-Jun-06 (SPEAG, No. DAE4-654_Jun06) Check Date (in house) 4-Aug-98 (SPEAG, in house check Nov-05)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-07 Aug-07 Jan-07 Jun-07 Scheduled Check In house check: Nov-07
The measurements and the under All calibration Equipment used (M& Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 9 robs ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	rtainties with confidence cted in the closed laborat TErcritical for calibration) ID # GB41293874 MY41495277 MY41495087 SN: S5054 (3c) SN: S5054 (3c) SN: S5054 (3c) SN: S5054 (3c) SN: S5054 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3842U01700 US3842U01700 US37390585	probability are given on the following pages and arr ory facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 251-00559) 10-Aug-06 (METAS, No. 251-00559) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 217-00593) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06) 21-Jun-06 (SPEAG, No. DAE4-654_Jun06) Check Date (in house) 4-Aug-99 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-07 Aug-07 Aug-07 Jan-07 Jun-07 Scheduled Check In house check: Nov-07 In house check: Nov-06
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	rtainties with confidence cted in the closed laborat TE-critical for calibration) ID # GB41293874 MY41495087 SN: 55054 (3c) SN: 55056 (20b) SN: 55129 (30b) SN: 55129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37390585 Name	probability are given on the following pages and are ony facility: environment temperature (22 ± 3)°C and S-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 251-00558) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 217-00593) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06) 21-Jun-06 (SPEAG, No. DAE4-654_Jun06) Check Date (in house) 4-Aug-98 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05) Function	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-07 Aug-07 Aug-07 Jan-07 Jun-07 Scheduled Check In house check: Nov-07 In house check: Nov-06
The measurements and the unce All celibrations have been conduct Celibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	rtainties with confidence cted in the closed laborat TE-critical for calibration) ID # GB41293874 MY41495087 SN: 55054 (3c) SN: 55056 (20b) SN: 55129 (30b) SN: 55129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37390585 Name	probability are given on the following pages and are ony facility: environment temperature (22 ± 3)°C and S-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 251-00558) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 217-00593) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06) 21-Jun-06 (SPEAG, No. DAE4-654_Jun06) Check Date (in house) 4-Aug-98 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05) Function	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-07 Aug-07 Aug-07 Jan-07 Jun-07 Scheduled Check In house check: Nov-07 In house check: Nov-06
The measurements and the unce All celibrations have been conduct Celibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 30 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Natwork Analyzer HP 8753E	rtainties with confidence ted in the closed laborat TE-critical for calibration) ID # GB41293874 MY41495277 MY41495077 SN: S5054 (3c) SN: S5054 (3c) SN: S5054 (3c) SN: S5054 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: S5129 (30b) SN: S5129 (30b) SN: 654 ID # US3842U01700 US3842U01700 US37390585 Name Katja Pokovic	probability are given on the following pages and arr ory facility: environment temperature (22 ± 3)°C and 5 Apr-06 (METAS, No. 251-00557) 5 Apr-06 (METAS, No. 251-00557) 5 Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 217-00592) 4 Apr-06 (METAS, No. 217-00593) 2 Jan-06 (SPEAG, No. ES3-3013, Jan06) 21 Jun-06 (SPEAG, No. Jan04, Jan06) 21 Jun-06 (SPEAG, No. Jan04, Jan06) 21 Jun-06 (SPEAG, In house check Nov-05) 18 Out-06 (SPEAG, In house check Nov-05) 31 Section Technical Manager	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-07 Aug-07 Aug-07 Jun-07 Jun-07 Scheduled Check In house check: Nov-07 In house check: Nov-06



Schmid & Partn Engineering A	G Servizio svizzero di taratura
Zeughausstrasse 43, 8	004 Zurich, Switzerland
The Swiss Accreditation	Federal Office of Metrology and Accreditation Accreditation No.: SCS 108 on Service is one of the signatories to the EA t for the recognition of calibration certificates
Glossary:	
TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConF	sensitivity in TSL / NORMx,y,z
DCP Relatization	diode compression point
Polarization φ Polarization θ	φ rotation around probe axis 9 rotation around an axis that is in the plane normal to probe axis (at
ruianzation a	measurement center), i.e., $9 = 0$ is normal to probe axis
Averaged Commun b) CENELE related to GHz), Jul Methods Applie • NORMx,J R22 wave NORMx,J • NORM(f) linearizat the freque	ed and Interpretation of Parameters: <i>x</i> , <i>z</i> : Assessed for E-field polarization $\vartheta = 0$ (f $\le 900$ MHz in TEM-cell; f > 1800 MHz: eguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of <i>x</i> ,z does not effect the E <sup>2</sup> -field uncertainty inside TSL (see below <i>ConvF</i> ). <i>x</i> , <i>y</i> , <i>z</i> = <i>NORMx</i> , <i>y</i> , <i>z</i> * <i>frequency_response</i> (see Frequency Response Chart). This ion is implemented in DASY4 software versions later than 4.2. The uncertainty of ency response is included in the stated uncertainty of <i>ConvF</i> . <i>c</i> : DCP are numerical linearization parameters assessed based on the data of reep (no uncertainty required). DCP does not depend on frequency nor media. <i>nd Boundary Effect Parameters</i> : Assessed in flat phantom using E-field (or ture Transfer Standard for f $\le 800$ MHz) and inside waveguide using analytical field
power sw ConvF all Tempera distribution assessm typical ur improve p NORMx,	ons based on power measurements for f > 800 MHz. The same setups are used for ent of the parameters applied for boundary compensation (alpha, depth) of which icertainty values are given. These parameters are used in DASY4 software to probe accuracy close to the boundary. The sensitivity in TSL corresponds to <i>r</i> , <i>z</i> * <i>ConvF</i> whereby the uncertainty corresponds to that given for <i>ConvF</i> . A y dependent <i>ConvF</i> is used in DASY version 4.4 and higher which allows
<ul> <li>power sw</li> <li>ConvF at Tempera distributio assessm typical ur improve p NORMx, frequency extending</li> <li>Spherical</li> </ul>	ent of the parameters applied for boundary compensation (alpha, depth) of which acertainty values are given. These parameters are used in DASY4 software to probe accuracy close to the boundary. The sensitivity in TSL corresponds to <i>r</i> , <i>z</i> * <i>ConvF</i> whereby the uncertainty corresponds to that given for <i>ConvF</i> . A y dependent <i>ConvF</i> is used in DASY version 4.4 and higher which allows the validity from ± 50 MHz to ± 100 MHz.
power sw ConvF all Tempera distribution assessmutypical ur improve p NORMx.) frequency extending Spherical flat phant Sensor C	ent of the parameters applied for boundary compensation (alpha, depth) of which incertainty values are given. These parameters are used in DASY4 software to probe accuracy close to the boundary. The sensitivity in TSL corresponds to $7, z * ConvF$ whereby the uncertainty corresponds to that given for $ConvF$ . A y dependent $ConvF$ is used in DASY version 4.4 and higher which allows to the validity from $\pm$ 50 MHz to $\pm$ 100 MHz.



ET3DV6 SN:1788

September 19, 2006

# Probe ET3DV6

## SN:1788

Manufactured: Last calibrated: Recalibrated: May 28, 2003 September 30, 2004 September 19, 2006

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: ET3-1788\_Sep06

Page 3 of 9



### ET3DV6 SN:1788

September 19, 2006

## DASY - Parameters of Probe: ET3DV6 SN:1788

Sensitivity in Free	ensitivity in Free Space <sup>A</sup>			Compression <sup>B</sup>	
NormX	1.73 ± 10.1%	μV/(V/m) <sup>2</sup>	DCP X	95 mV	
NormY	1.67 ± 10.1%	μV/(V/m) <sup>2</sup>	DCP Y	101 mV	
NormZ	1.70 ± 10.1%	$\mu V/(V/m)^2$	DCP Z	93 mV	

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

Boundary Effect

TSL 900 MHz Typical SAR gradient: 5 % per mm

Sensor Cente	r to Phantom Surface Distance	3.7 mm	4.7 mm
SAR <sub>te</sub> [%]	Without Correction Algorithm	7.9	4.3
SAR <sub>be</sub> [%]	With Correction Algorithm	0.1	0.3

TSL 1810 MHz Typical SAR gradient: 10 % per mm

Sensor Cente	r to Phantom Surface Distance	3.7 mm	4.7 mm
SARbe [%]	Without Correction Algorithm	11.8	7.0
SAR <sub>be</sub> [%]	With Correction Algorithm	0.2	0.4

Sensor Offset

Probe Tip to Sensor Center 2.7 mm

-----

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^ The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 8). <sup>9</sup> Numerical linearization parameter; uncertainty not required.

Certificate No: ET3-1788\_Sep06


Page 4 of 9



ET3DV6 SN:1788

Test Report No 🔅 FA742004-2-2-01

September 19, 2006

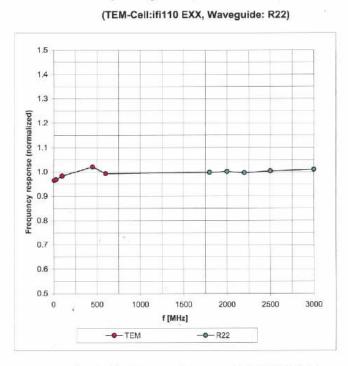

## Frequency Response of E-Field

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)




Page 5 of 9

©2007 SPORTON International Inc. SAR Testing Lab






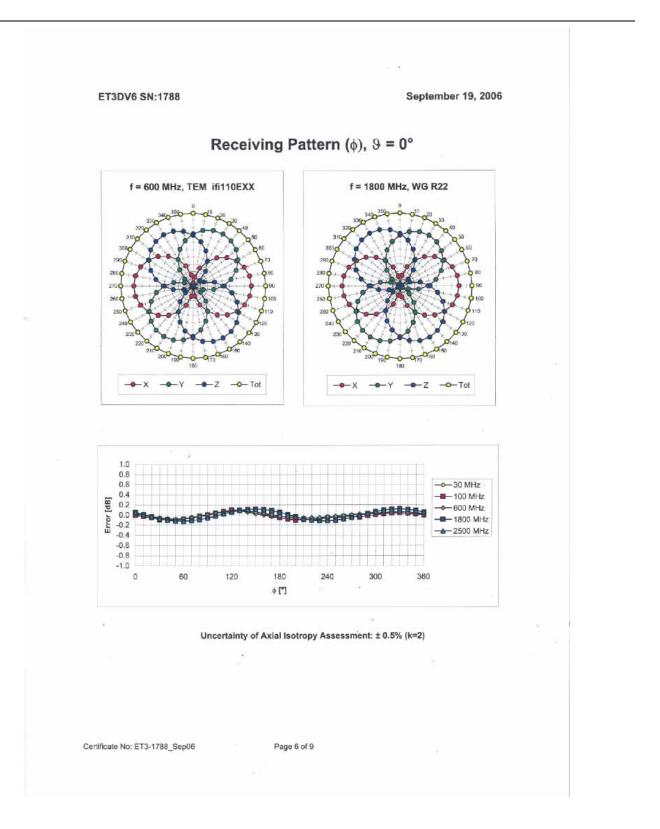

#### ©2007 SPORTON International Inc. SAR Testing Lab



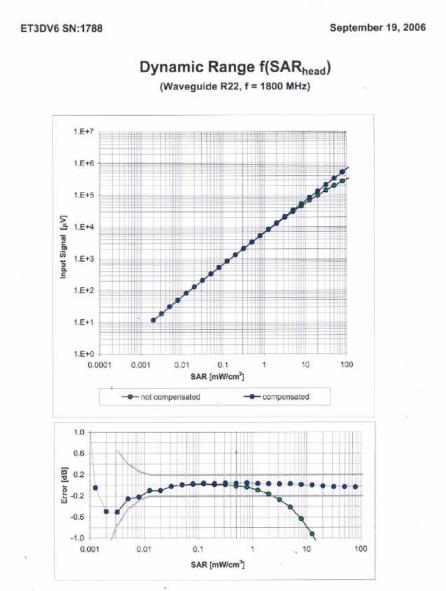

Uncertainty of Linearity Assessment: ± 0.6% (k=2)


Certificate No: ET3-1788\_Sep06

Page 7 of 9

September 19, 2006



ET3DV6 SN:1788

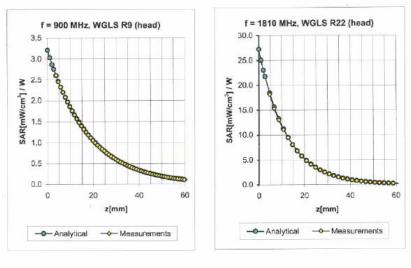

## **Conversion Factor Assessment**

f [MHz]	Validity [MHz] <sup>C</sup>	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF	Uncertainty
900	±50/±100	Head	41.5 ± 5%	0.97 ± 5%	0.49	1.94	6.60	± 11.0% (k=2)
1810	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.48	2.74	5.30	± 11.0% (k=2)
2000	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.53	2.75	5.00	± 11.0% (k=2)
2450	± 50 / ± 100	Head	$39.2\pm5\%$	1.80 ± 5%	0.68	1.96	4.66	± 11.8% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.45	2.12	6.33	± 11.0% (k=2)
1810	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.59	2.89	4.67	± 11.0% (k=2)
2000	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.56	2.79	4.50	± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.60	1.70	4.11	± 11.8% (k=2)


<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Certificate No: ET3-1788\_Sep06

Page 8 of 9

©2007 SPORTON International Inc. SAR Testing Lab



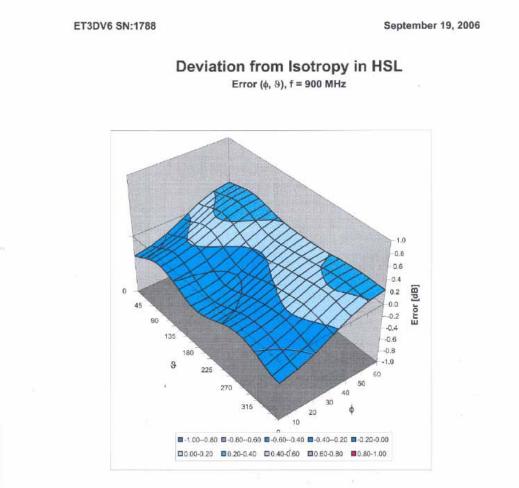

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Page 9 of 9




Certificate No: ET3-1788\_Sep06



ccredited by the Swiss Federal Off	Switzerland	reditation Accreditation N	Swiss Calibration Service
he Swiss Accreditation Service is	s one of the signatories	s to the EA	
lultilateral Agreement for the rec-			DAE3-577_Nov06
CALIBRATION CI	ERTIFICATE		
Object	DAE3 - SD 000 D	003 AA - SN: 577	
Calibration procedure(s)	QA CAL-06.v12		
	Calibration proce	dure for the data acquisition electr	onics (DAE)
Calibration date:	November 21, 20	06	
Condition of the calibrated item	In Tolerance		
The measurements and the uncerta	ainties with confidence pr	onal standards, which realize the physical units robability are given on the following pages and v facility: environment temperature (22 ± 3)°C.	are part of the certificate.
The measurements and the uncerta	ainties with confidence pr		are part of the certificate.
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards	ainties with confidence pr id in the closed laborator critical for calibration)	robability are given on the following pages and y facility: environment temperature (22 ± 3)°C i Cal Date (Calibrated by, Certificate No.)	are part of the certificate. and humidity < 70%. Scheduled Calibration
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702	ainties with confidence pr id in the closed laborator critical for calibration)	robability are given on the following pages and y facility: environment temperature (22 ± 3)°C i	are part of the certificate. and humidity < 70%.
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001	ainties with confidence pr ed in the closed laborator critical for calibration) ID # SN: 6295803	Cal Date (Calibrated by, Certificate No.) 13-Oct-06 (Elcal AG, No: 5492)	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-07
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	ainties with confidence pr d in the closed laboratory crítical for calibration) ID # SN: 6295803 SN: 0810278 ID #	Cal Date (Calibrated by, Certificate No.) 13-Oct-06 (Elcal AG, No: 5492) 03-Oct-06 (Elcal AG, No: 5478)	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-07 Oct-07
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	ainties with confidence pr d in the closed laboratory crítical for calibration) ID # SN: 6295803 SN: 0810278 ID #	robability are given on the following pages and y facility: environment temperature (22 ± 3)°C i Cal Date (Calibrated by, Certificate No.) 13-Oct-06 (Elcal AG, No: 5492) 03-Oct-06 (Elcal AG, No: 5478) Check Date (in house)	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-07 Oct-07 Scheduled Check
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	Inties with confidence pr d in the closed laborator chtical for calibration) ID # SN: 6295803 SN: 0810278 ID # SE UMS 006 AB 1002	robability are given on the following pages and y facility: environment temperature (22 ± 3)°C i Cal Date (Calibrated by, Certificate No.) 13-Oct-06 (Elcal AG, No: 5492) 03-Oct-06 (Elcal AG, No: 5478) Check Date (in house) 15-Jun-06 (SPEAG, in house check)	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-07 Oct-07 Scheduled Check In house check Jun-07
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	ainties with confidence pr d in the closed laboratory crítical for calibration) ID # SN: 6295803 SN: 0810278 ID #	robability are given on the following pages and y facility: environment temperature (22 ± 3)°C i Cal Date (Calibrated by, Certificate No.) 13-Oct-06 (Elcal AG, No: 5492) 03-Oct-06 (Elcal AG, No: 5478) Check Date (in house)	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-07 Oct-07 Scheduled Check
The measurements and the uncerta	A in the closed laborator childen the closed laborator childen for calibration) ID # SN: 6295803 SN: 0810278 ID # SE UMS 006 AB 1002	robability are given on the following pages and y facility: environment temperature (22 ± 3)°C i Cal Date (Calibrated by, Certificate No.) 13-Oct-06 (Elcal AG, No: 5492) 03-Oct-06 (Elcal AG, No: 5478) Check Date (in house) 15-Jun-06 (SPEAG, in house check) Function Technician	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-07 Oct-07 Scheduled Check In house check Jun-07



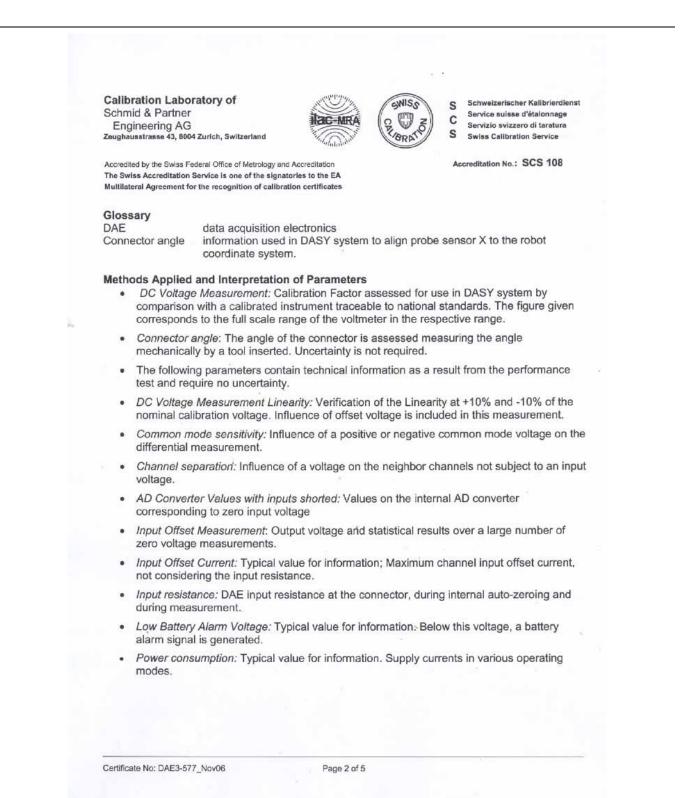



## DC Voltage Measurement

High Range:	1LSB =	6.1µV,	full range =	-100+300 mV
Low Range:	1LSB =	61nV ,	full range =	-1+3mV
DASY measurement	parameters: Au	to Zero Time: 3	sec; Measuring	time: 3 sec

Calibration Factors	X	Y	z
High Range	404.355 ± 0.1% (k=2)	403.806 ± 0.1% (k=2)	404.276 ± 0.1% (k=2)
Low Range	3.92854 ± 0.7% (k=2)	3.93862 ± 0.7% (k=2)	3.93591 ± 0.7% (k=2)

#### **Connector Angle**

The state of the second st	1 Alexandra (187) (197) (197) (197)
Connector Angle to be used in DASY system	268 ° ± 1 °

Certificate No: DAE3-577\_Nov06

Page 3 of 5



1.0

#### Appendix

1.	DC	Voltage	Linearity

High Range	Input (µV)	Reading (µV)	Error (%)
Channel X + Input	200000	199999.5	0.00
Channel X + Input	20000	20005.87	0.03
Channel X - Input	20000	-19998.71	-0.01
Channel Y + Input	200000	200000	0.00
Channel Y + Input	20000	20004.22	0.02
Channel Y - Input	20000	-20003.23	0.02
Channel Z + Input	200000	200000.6	0.00
Channel Z + Input	20000	20005.24	0.03
Channel Z - Input	20000	-20001.80	0.01
Low Range	Input (μV)	Reading (µV)	Error (%)
Laborative statistics and the statistics with	souther a real		

Low Range		Input (µV)	Reading (µV)	Error (%)
Channel X	+ Input	2000	1999.9	0.00
Channel X	+ Input	200	200.27	0.13
Channel X	- Input	200	-200.73	0.36
Channel Y	+ Input	2000	2000.1	0.00
Channel Y	+ Input	200	199.22	-0.39
Channel Y	- Input	- 200	-200.86	0.43
Channel Z	+ Input	2000	1999.9	0.00
Channel Z	+ Input	200	199.28	-0.36
Channel Z	- Input	200	-200.94	0.47

2. Common mode sensitivity DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (µV)
Channel X	200	14.24	12.49
	- 200	-12.13	-12.92
Channel Y	200	-6.51	-7.06
	- 200	6.05	5.81
Channel Z	200	1.09	0.86
	- 200	-2.86	-2.63

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200	3	2.51	0.09
Channel Y	200	0.43		3.37
Channel Z	200	-0.55	0.96	1. <b>-</b> 5

Certificate No: DAE3-577\_Nov06

Page 4 of 5

#### ©2007 SPORTON International Inc. SAR Testing Lab

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15970	16306
Channel Y	15851	16305
Channel Z	16208	17068

5. Input Offset Measurement DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input 10MΩ

	Average (µV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	-0.51	-1.55	0.47	0.50
Channel Y	-2.06	-4.32	-0.65	0.60
Channel Z	-1.63	-2.56	-0.15	0.35

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance

	Zeroing (MOhm)	Measuring (MOhm)
Channel X	0.2000	199.8
Channel Y	0.2000	200.7
Channel Z	0.2000	199.8

#### 8. Low Battery Alarm Voltage (verified during pre test)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

#### 9. Power Consumption (verified during pre test)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.0	+6 .	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE3-577\_Nov06

Page 5 of 5

#### ©2007 SPORTON International Inc. SAR Testing Lab