

SAR Analysis of Cylos DR-T (PG6CYLOS) By Similarity to Philos DR-T (PG6BAOT)

Certification of medical-implant transmitters under FCC Part 95 Medical Implant Communication Service (MICS) requires a measurement or Finite Difference Time Domain (FDTD) analysis of the Specific Absorption Rate (SAR) associated with the presence of a non-ionizing, radio frequency (RF) transmitters in a human body.

Biotronik, a manufacturer of Pacemaker and Defibrillator implant devices employing ultra low-power RF transmitters, has performed FDTD SAR analysis on numerous products that have been approved by the FCC and are currently in production. These implants comply with the FCC Part 95 MICS specified SAR limits with a margin of 25.5 dB. That is, Biotronik's currently approved medical implants generate SAR levels of 4.54 mW/kg, only 0.28% of the maximum acceptable level permitted by the FCC (1.6 W/kg). By their very nature, battery-powered implants, must operate at very low power levels to achieve a battery service life of 5 to 7 years in a patient, and hence the resulting SAR levels are inherently very low. This is very different than typical cellular telephone electronics which transmit signals at SAR levels more than 350 times higher than the 4.54 mW/kg level of currently approved Biotronik medical implants.

Since the ultra low-power RF transmitters employed in Biotronik's implants produce SAR levels significantly lower than the maximum acceptable level, Biotronik submits this SAR analysis for the Cylos DR-T pacemaker (FCC ID: PG6CYLOS) based upon its similarity to a currently approved product, Philos DR-T (FCC ID: PG6BAOT). The PG6CYLOS RF transmitter is similar to the PG6BAOT RF transmitter that was granted FCC approval, and complies with the SAR limits with a margin of 25.5 dB.

Biotronik submits the following exhibits to demonstrate compliance with the Specific Absorption Rate (SAR) limits as part of the FCC Part 95 submission for the Cylos DR-T Pacemaker (FCC ID: PG6CYLOS).

- Exhibit (S1) - Similarity of RF Transmitter Circuits
- Exhibit (S2) - Similarity of RF Transmitter Antenna and Housing Design
- Exhibit (S3) - Similarity of Production Acceptance Test Specification
- Exhibit (S4) - Similarity of Measured Radiated Emissions
- Exhibit (S5) – SAR Analysis of Philos (FCC ID# PG6BAOT)

Exhibit (S1) - Similarity of RF Transmitter Circuits

Figure (S1) in **Exhibit K – Schematics**, shows the RF transmitter circuitry of the Cylos (PG6CYLOS) and Philos (PG6BAOT) pacemakers. Both pacemakers utilize a single transistor SAW-stabilized Colpitts oscillator (Q801 in PG6CYLOS, and Q101 in PG6BAOT). Both pacemakers also use a single transistor buffer amplifier stage (Q802 in PG6CYLOS, and Q102 in PG6BAOT) to couple the oscillator signal to the antenna. The transistors used in PG6CYLOS are equivalent replacements for the transistors used in PG6BAOT, which are now obsolete. The transistors in PG6CYLOS are biased with slightly more collector current than those in PG6BAOT. This results in a slight increase in output power in PG6CYLOS, but as shown in Exhibit (S3) and Exhibit (S4), the power is significantly below the acceptable 47 CFR 95.639 (f) (1)-(2) limits. PG6CYLOS also incorporates a low pass filter (L803 and C812) at the output of the buffer amplifier thereby ensuring emissions at the harmonics of the fundamental are further attenuated.

Exhibit (S2) - Similarity of RF Transmitter Antenna and Housing Design

As shown in Figure 2. Photograph of Philos (PG6BAOT) and Cylos (PG6CYLOS) pacemakers, the PG6CYLOS pacemaker's housing and antenna design are similar to the PG6BAOT pacemaker. Both pacemakers utilize the same construction materials: a welded titanium case, and an epoxy header for the transmit antenna and pacemaker lead sockets. The housing of the Cylos pacemaker is approximately 0.5 cm wider to accommodate a larger circuit board assembly. Note that the Philos (PG6BAOT) pacemaker passed FCC SAR limits with 25.5 dB of margin. Increasing the housing dimension will not impact the SAR margin.

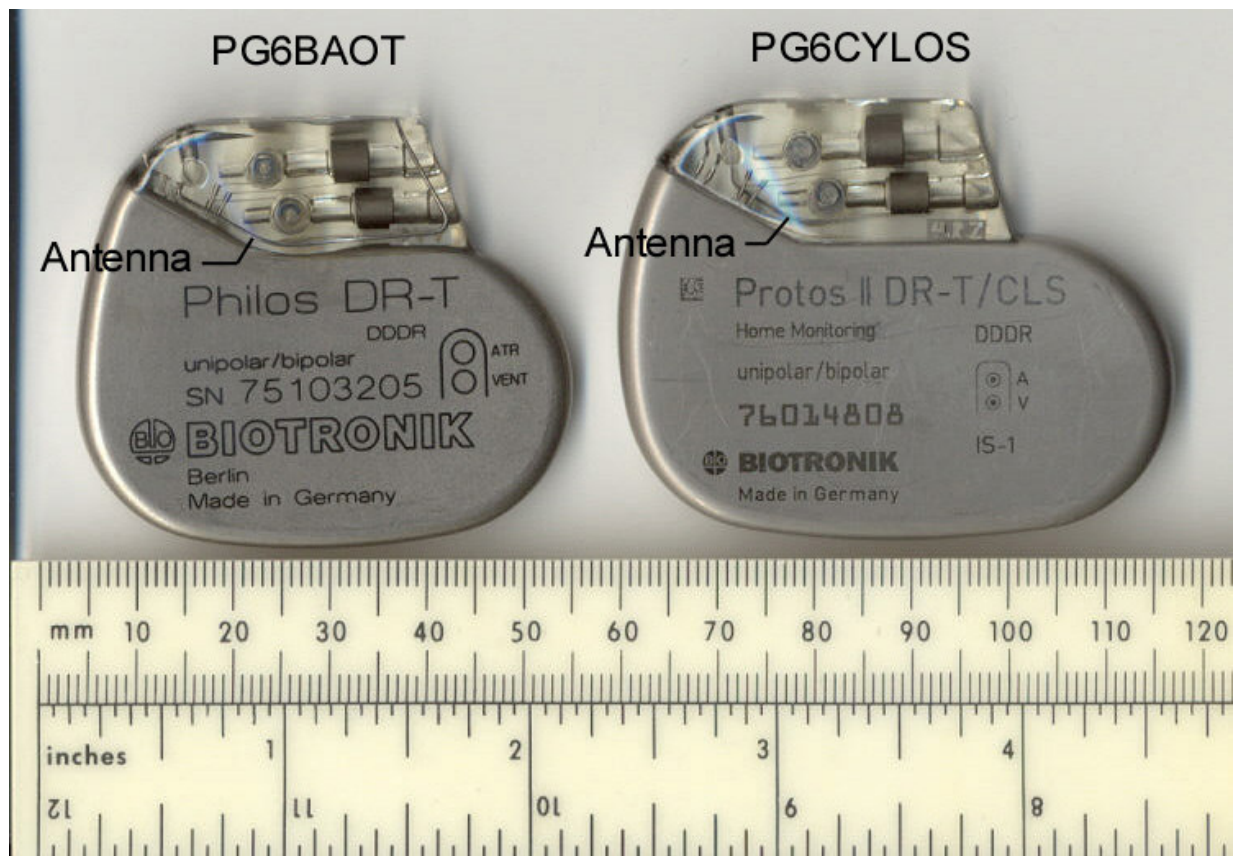


Figure 2. Photograph of Philos (PG6BAOT) and Cylos (PG6CYLOS) Pacemakers

Exhibit (S3) - Similarity of Production Acceptance Test Specification

As shown in Table (S3) in **Exhibit N - Acceptance Test Specification**, the Cylos (PG6CYLOS) and Philos (PG6BAOT) implants have similar RF output power level limits. The RF output power level is measured on every production unit to ensure compliance with this specification. Although the High Limit for PG6CLYOS is 6 dB above the limit for PG6BAOT, PG6BOAT's 25.5 dB of SAR margin ensures that PG6CYLOS will never exceed the SAR limit stipulated by the FCC. PG6CYLOS will comply with FCC SAR limits with a worst-case margin of 19.5 dB.

Exhibit (S4) - Similarity of Measured Radiated Emissions

As further evidence that the ultra low-power RF transmitter in Cylos (PG6CYLOS) complies with FCC SAR limits with ample margin, note the measured level of the Radiated Emissions shown in Table (S4) below. PG6CYLOS exhibits radiated emission levels substantially less (-36.7 dB) than the Field Strength of the Fundamental limits stipulated in 47 CFR 95.639 (f) (1)-(2). This data supports Exhibit (S3) - Similarity of Production Acceptance Test Specification, in that the RF transmit power limit of PG6CYLOS, which is 6 dB above PG6BAOT, can result in approximately 6 dB of additional radiated power. Although the 6 dB increase in radiated power will increase the power absorbed by the body, the net absorption is 19.5 dB less than the FCC SAR limits. This, combined with the 36.7 dB of margin in the radiated emissions level provides assurance that PG6CYLOS complies with the FCC SAR limits.

Table (S4) Comparison of PG6BAOT and PG6CYLOS Radiated Emissions

	Frequency (MHz)	Measured Field Strength (dBuV/m)	47 CFR 95.639 (f) (1) – (2) Spec. Limit (dBuV/m)	Measured Level Compared to Spec. (dB)
PG6CYLOS <i>Note (1)</i>	403.617	48.5	85.2	-36.7
PG6BAOT <i>Note (2)</i>	403.572	42.1	85.2	-43.1

Note (1):

Measured by NW EMC, Inc., 22975 NW Evergreen Pkwy., #400, Hillsboro, Oregon 97124 on June 10, 2005, Work Order BIOT0009. Note that the transmit frequency specification for the SAW-stabilized oscillator is 403.63 MHz +/- 95 KHz.

Note (2):

Measured by NW EMC, Inc., 22975 NW Evergreen Pkwy., #400, Hillsboro, Oregon 97124 on Oct. 19, 2000, Job Number MICR0001. Note that the transmit frequency specification for the SAW-stabilized oscillator is 403.63 MHz +/- 95 KHz.

EXHIBIT (S5) – SAR Analysis of Philos (FCC ID# PG6BAOT)

**Specific Absorption Rate (SAR) Analysis
Using Finite Difference Time Domain Computation
for RF Transmitter Circuit Employed in Biotronik
Pacemakers Actros TO+ and Philos DR-T**



**Ed Wardzala
Mark Johnson**

February 3, 2001

Introduction

Biotronik has developed an RF communications system for use in implantable pacemakers allowing for patient data regarding cardiac condition to be transmitted wirelessly to the physician for evaluation. The amount of irradiated power transmitted through the human body using this technology can be defined by a measure termed the Specific Absorption Rate (SAR). Values of SAR that can be safely used in these applications have been defined by ANSI/IEEE and are part of the FCC guidelines for medical implant communications.

Certification of medical-implant transmitters under the FCC Part 95 Medical Implant Communication Service (MICS) requires a measurement or Finite Difference Time Domain (FDTD) analysis of the SAR associated with the presence of a non-ionizing, radio frequency (RF) transmitter. This report details the SAR analysis of the unidirectional RF transmitter found in Biotronik's Philos DR-T and Actros TO+ pacemakers.

Summary

Using a commercially available FDTD program (XFDTD, Remcom Inc.), the computed SAR values determined by this analysis are:

Maximum SAR	4.54 mW/kg
Maximum 1g average SAR	1.11 mW/kg
Average SAR	427 nW/kg

The ANSI C95-1-1992 limit is 1.6 W/kg. The computed value in this study of the maximum SAR is 4.54 mW/kg. The margin between the maximum attained SAR and the ANSI/IEEE specification limit is 25.5 dB (only 0.28% of the specification limit).

These FDTD results prove that the Biotronik RF transmitter circuitry can safely be used in its intended application with respect to the energy emitted during communication.

Method of Analysis:

Equipment and tools used for the analysis:

Hardware

Dell dual processor Windows 2000 Workstation, 1 Gb RAM 3 drive SCSI RAID
Hewlett-Packard 8591 Spectrum Analyzer
Hewlett Packard 8753E Vector Network Analyzer

Software

XFDTD 5.1.0.5 Bio-Pro, Calc FDTD 5.1, Remesher 5.1, HIFI Body model
Eagleware SuperStar Pro. 6.5b
MicroSim PSPICE ver 8.0

The computational tool used for this FDTD analysis was XFDTD with the hi-fidelity Visible Man model (also from Remcom). The first proposed method for analysis was to use the subgrid tool where the implant at 1 mm^3 resolution would be placed in the biomodel, which is meshed at 5 mm^3 . It was found that the subgrid technique, when used with high-dielectric constant materials, does not yield a stable solution. This was verified with Remcom¹. Because it was desirable to show the fine structure of the implant, and yet restrict the computational effort of the equipment, a mesh size of 2 mm^3 was chosen for the analysis.

Note: This 2mm mesh provides for resolution 15 times greater than the 5mm grid pattern that has been used by Biotronik competitors in similar applications for their analysis to prove compliance with the SAR limit safety standards.

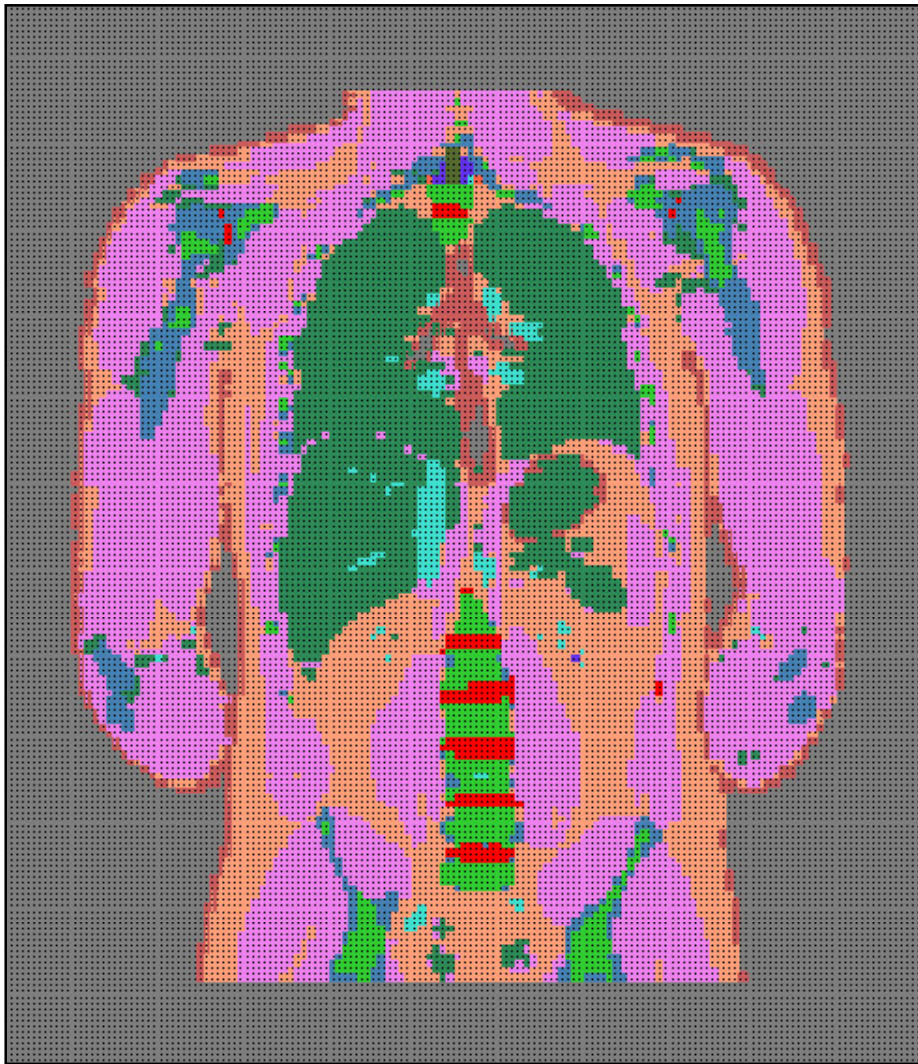


Figure 1.

Truncated Biomesh
Resampled at 2 mm^3

The biomesh was resampled to a 2 mm^3 grid, and the body was truncated to include only the torso (Figure 1). Limiting analysis to the torso was deemed rational as the RF power

emanates from the pacemaker located in the chest and remains concentrated within this region as proven in this analysis. While feasible, utilizing the entire human body model complicates the analysis, without providing additional insight into the irradiation properties of the pacemaker signal propagating through the tissue of concern.

1.1.1. Pacemaker Model

Remcom, to date, does not have a 3-D import tool and the model of the implant was restricted to the primitive geometry tools that are currently available. Figure 2 below shows the pacemaker model utilized for this analysis, which is a rectangle-box tool.

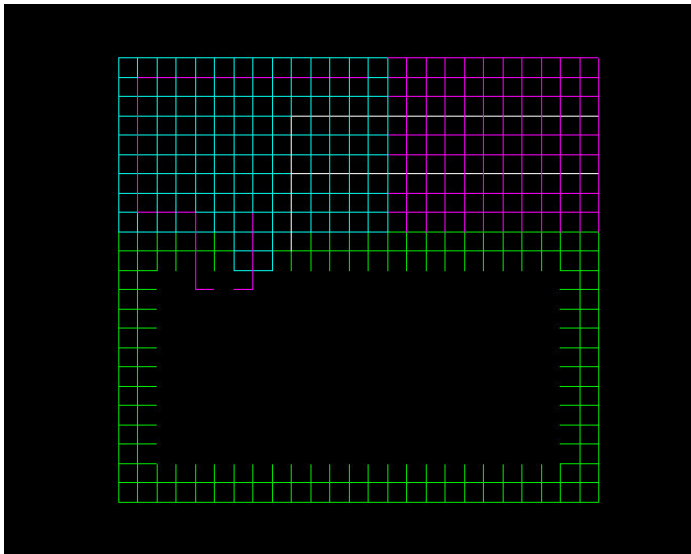


Figure 2.
Implant Mesh 2 mm³

The loop antenna and pacing lead wires were realized with a combination of PEC wire and thin-wire models. Thin wire models allow any FDTD algorithm to include the effects of wire diameter. The epoxy-header material, shown in light blue, used to enclose the loop antenna, was characterized for values of dielectric constant and conductivity. Using a HP8753E network analyzer and a TEM transmission line test cell, it was found the epoxy has a dielectric constant 0 ~3 and a conductivity ~.001 S/m. The green area is the titanium case. The actual thickness of the titanium case is not 4 mm as shown below; it is on the order of 1/3 mm, but FDTD modeling requires at least 1 full cell width on the wall of a hollow object to correctly model the object. The skin depth of titanium at this frequency is such that the attenuation of an EM wave is not changed with this modeled wall thickness compared to the actual case. The violet and white lines show the loop antenna and the pacing wires, respectively. The upper right corner (violet) shows an area of muscle tissue. This addition of biological tissue was included with the pacemaker to ensure that the pacemaker could be correctly merged with the biological model of Figure 1. As the mesh is 2 mm³, Figure 2 shows that the pacemaker is 4.6 cm x 5.0 cm x 1.6 cm. Shown inside the case is a pair of violet, “L” shaped antenna wires for the source. The source cell is thus shielded by the case, as it is in the actual pacemaker, and does not effect the field distribution in the SAR calculation.

A photo of the actual pacemaker is shown on the cover of this report. In this photo, the loop antenna is easily identifiable embedded in the header of the device (around the perimeter).

1.1.2. Integration of Pacemaker and Torso Model

The geometry for the implant was merged with the torso and pacing leads in a typical configuration were added. The composite model (anterior view) is shown in Figure 3a; Figure 3b shows a top view. The RF transmission source can be seen inside the composite anterior view as the green “speck” inside the titanium case.



Figure 3a.
Composite Mesh
Showing Torso
and Implant,
Anterior View

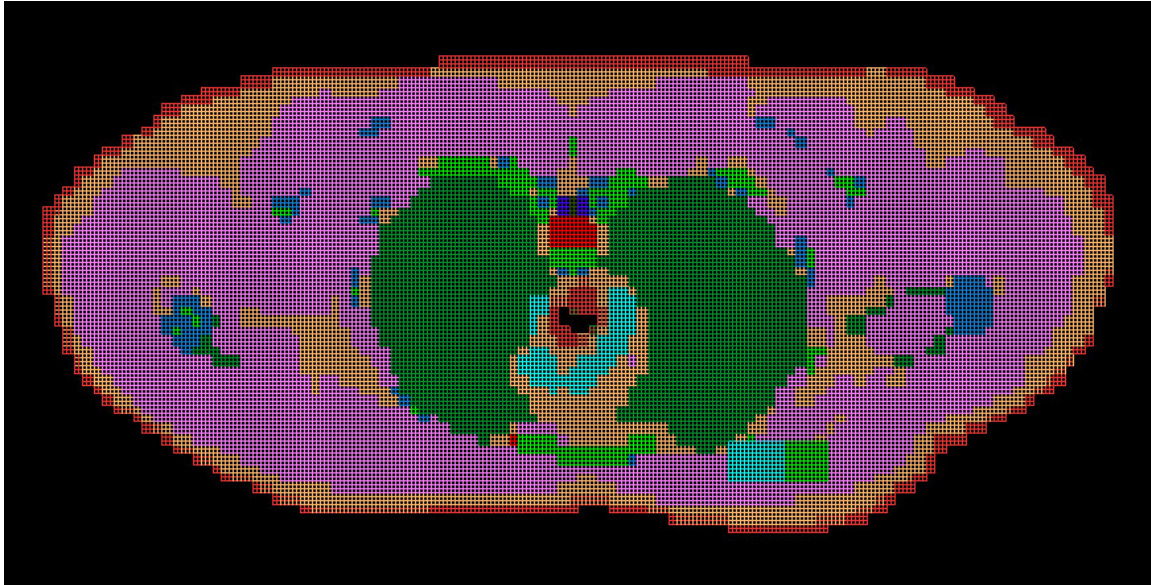


Figure 3b Composite Mesh Showing Torso and Implant, Top View

Elements Developed for SAR Analysis

The computation for SAR requires a source value and a source resistance. These were obtained as follows. An FDTD model of the antenna and FCC torso² were used to determine the input reflection coefficient of the antenna. This data was input to a RF linear modeling tool (Eagleware), and a lumped element description, using the optimization tools in Eagleware, of the input reflection coefficient was obtained. Figure 4 shows that the lumped element model and the reflection coefficient data are in good agreement to the 4th harmonic.

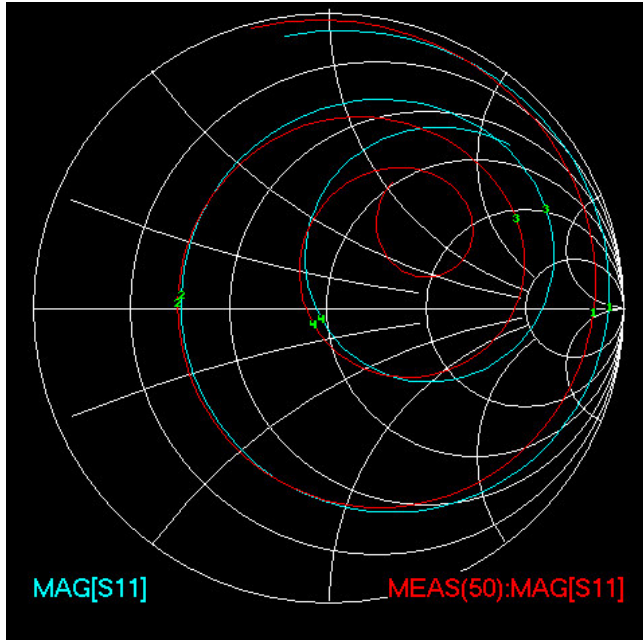


Figure 4.

Antenna Reflection Coefficient
(red) and Lumped Element
Antenna Model (blue)

The transmitter was modeled using PSpice, and this lumped element antenna model was used in the simulation. A range of resistive loads and this lumped element antenna were used to determine a Thevenin equivalent for the transmitter. These results were used as the source conditions in the XFDTD analysis. Source modeling in XFDTD is restricted to resistive loads only; the source impedance was found to be $\sim 67 \Omega$, and the open circuit voltage to be $157 \text{ mV}_{\text{RMS}}$. A conducted measurement of the implant transmitter power into a 50Ω load gives a value of -16 dBm at the fundamental. Using the information from the Pspice simulation to determine the available power from the transmitter,

$$P_{\text{AVAIL}} \equiv \frac{V_{\text{OC}}^2}{4 \cdot R_S}$$

The available power from the transmitter in the simulation is calculated to be -10.4 dBm . The calculated power delivered to a 50Ω load would be -10.5 dBm . This shows good correlation (6 dB error) between the modeled result and the actual measured result, and furthermore it is noted that the error is conservative in that the modeled power is higher than the measured value.

SAR Analysis at 403 MHz

XFDTD provides an application to compute the SAR at a single frequency. This analysis and the biomesh model material were computed at 403.6 MHz. In the MICS band, the

electrical properties of biological tissue are described by a dipolar mechanism. The dipolar region is characterized by slowly changing permittivity and conductivity, with many tissue types exhibiting a Cole-Cole behavior³. Thus, it is reasonable to expect similar SAR results over the entire MICS band. Figure 5 shows the distribution of the SAR in the y plane, where the maximum value was computed. This is the maximum value in this computation and not an averaged value.

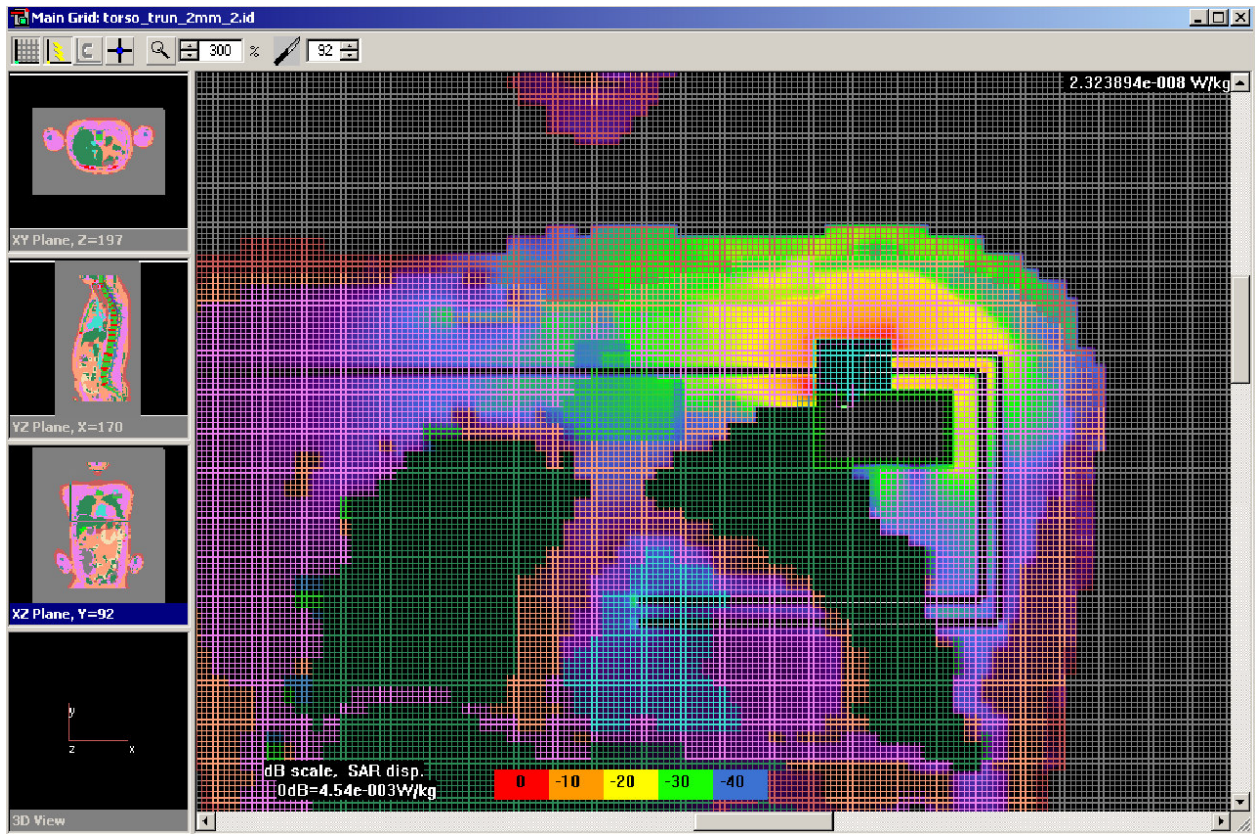


Figure 5. Plot of the maximum (unaveraged) Specific Absorption Rate (SAR)

Summary of Results

A summary table for the SAR statistics as generated by the XFDTD program is shown in Figure 6 on the following page. Since a typical implant device is located in the subcutaneous tissue, nominally a couple of cm below the surface, a 10 g average of SAR was not computed.

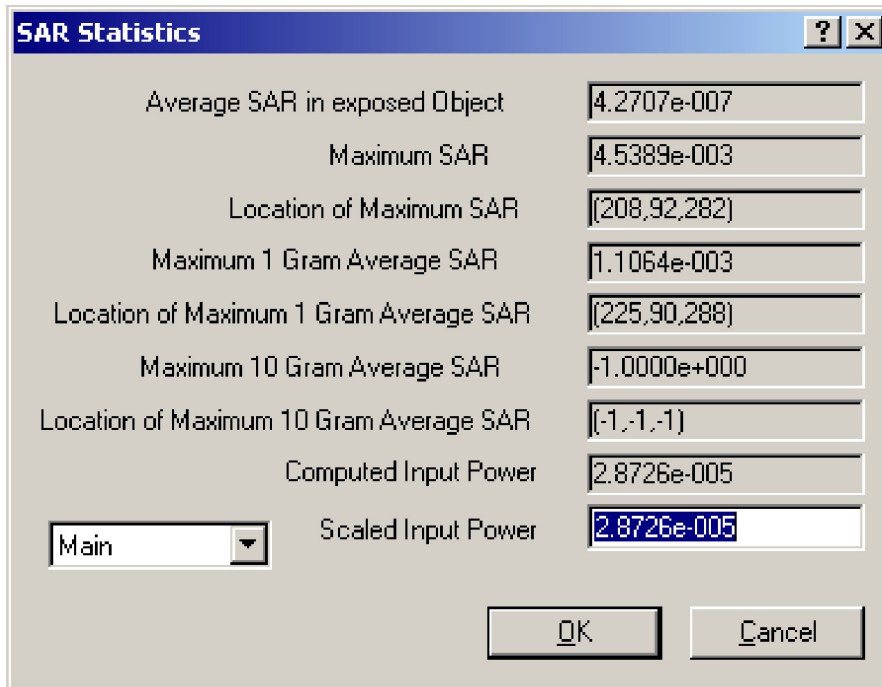


Figure 6.

Summary of SAR Statistics

The statistics summary in Figure 6 combined with the SAR plot of Figure 5 show that the location of maximum SAR is located in the area of the pacemaker antenna. The color map scale at the bottom center of Figure 5 is 10 dB per hue, so Figure 5 shows a color gradation of 40 dB. Using the pacemaker width of 5 cm as a scale notice that the SAR drops at ~20 dB in any 5 cm direction from the point of maximum SAR.

Conclusions:

As shown from this Finite Difference Time Domain analysis, the RF transmitter used by Biotronik in implantable pacemakers Philos DR-T and Actros TO+ meet the Specific Absorption Rate (SAR) standard set by ANSI/IEEE and incorporated into the FCC guidelines for medical implantable communications devices. The specific results reveal that the computed maximum SAR value for this RF circuit has a margin of 25.5 dB.

This analysis proves the safety of the implantable RF transmitter when used in its intended application, and can be compared very favorably with cellular telephone electronics, which propagate signals at SAR levels more than 350 times higher than the 4.54mWatt/kg Biotronik system. (cell phones SAR values are typically 500 to 1500mWatts/kg).

References:

- 1 Phone conversation with Ray Luebbbers, Remcom Inc.
2. FCC torso model for MICS FCC 99-363 page 23
3. Camelia Gabriel “Compilation of the Dielectric Properties of Body Tissues at RF and Microwave Frequencies”.

<http://www.brooks.af.mil/AFRL/HED/hedr/reports/dielectric/cover.html>