

Validation Data (1900MHz Brain)

Dipole 1900 MHz

SAM II Phantom; Flat Section; Position: (90°,90°); Frequency: 1900 MHz

Probe: ET3DV6 - SN1609; ConvF(5.40,5.40,5.40); Crest factor: 1.0; Brain 1900 MHz: $\sigma = 1.39$

mho/m $\epsilon_r = 40.0$ $\rho = 1.00$ g/cm³

Cubes (2): SAR (1g): 40.8 mW/g ± 0.01 dB, SAR (10g): 21.1 mW/g ± 0.01 dB

Coarse: Dx = 20.0, Dy = 20.0, Dz = 10.0

Powerdrift: -0.07 dB

Comment:


1900 MHz Brain Dipole Validation (D1900V2/ S.N: 5d032)

Antenna Input Power : 30 dBm (1W)

HCT Co., Ltd. Brain Tissue Simulating Liquid

Liquid Temperature : 21.4 °C

Date Tested : January 5, 2004

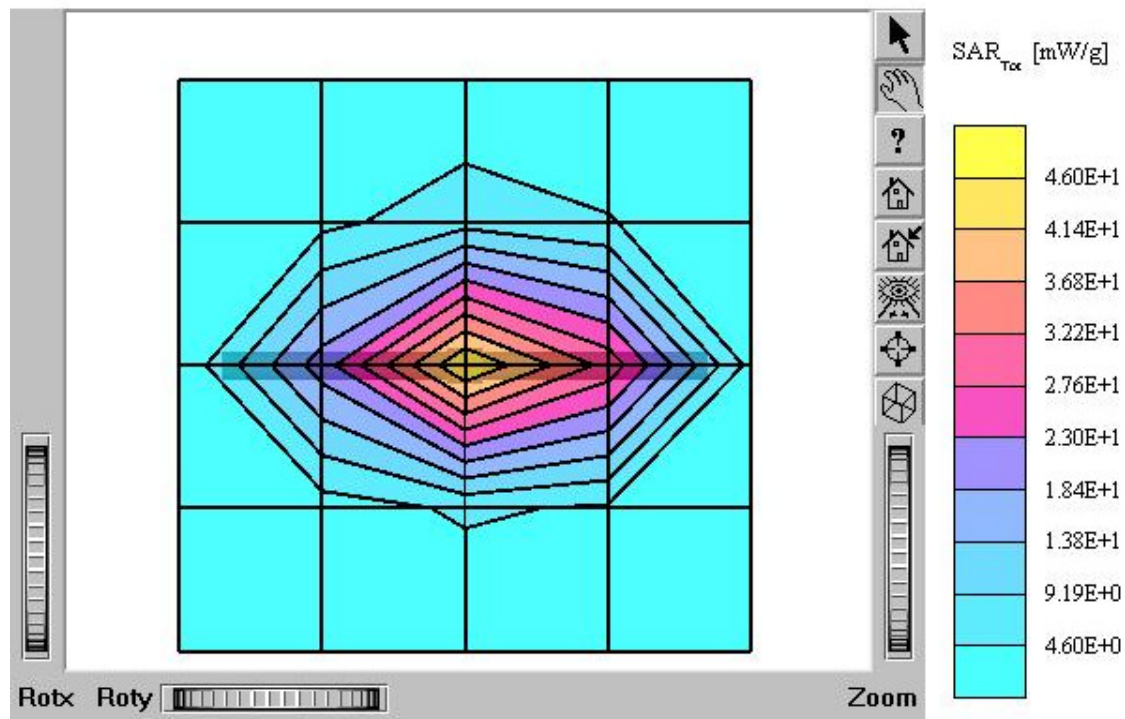

Dipole 1900 MHz

SAM II Phantom; Flat Section; Position: (90°,90°); Frequency: 1900 MHz

Probe: ET3DV6 - SN1609; ConvF(5.40,5.40,5.40); Crest factor: 1.0; Brain 1900 MHz: $\sigma = 1.39$

mho/m $\epsilon_r = 40.0$ $\rho = 1.00$ g/cm³

Cubes (2): SAR (1g): 40.8 mW/g ± 0.01 dB, SAR (10g): 21.1 mW/g ± 0.01 dB

Cube 5x5x7: Dx = 8.0, Dy = 8.0, Dz = 5.0

Comment:


1900 MHz Brain Dipole Validation (D1900V2/ S.N: 5d032)

Antenna Input Power : 30 dBm (1W)

HCT Co., Ltd. Brain Tissue Simulating Liquid

Liquid Temperature : 21.4 °C

Date Tested : January 5, 2004

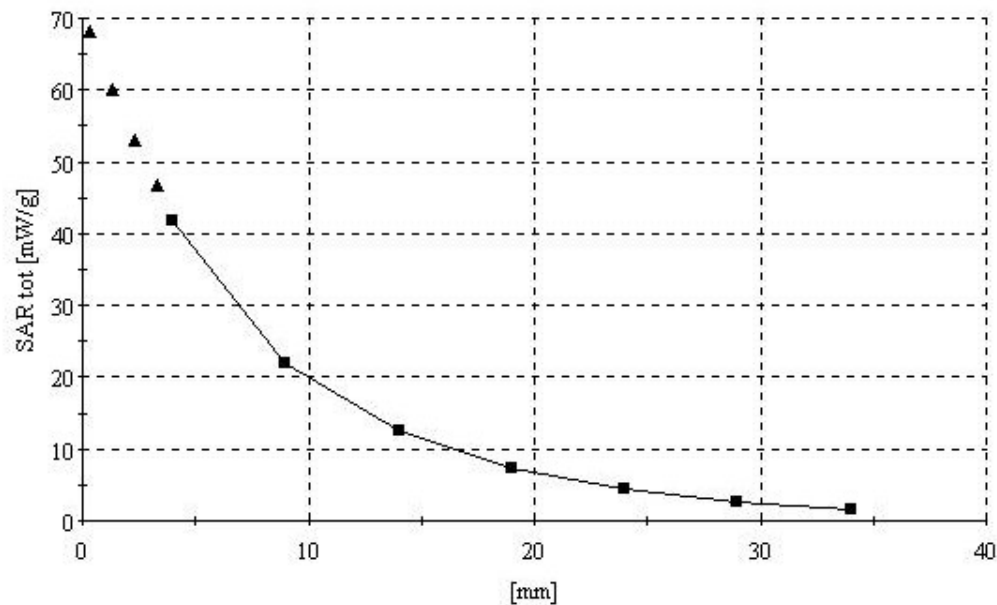

! Dielectric Parameter (1900MHz Brain)

Title : AXW-P1900B

SubTitle : 1900 MHz Brain

January 05, 2004 12:50 PM

Frequency	e'	e''
1.800000000 GHz	40.3901	12.8211
1.810000000 GHz	40.3164	12.8698
1.820000000 GHz	40.3184	12.9107
1.830000000 GHz	40.2520	12.9853
1.840000000 GHz	40.2416	13.0215
1.850000000 GHz	40.2300	13.0583
1.860000000 GHz	40.1996	13.0828
1.870000000 GHz	40.2028	13.1248
1.880000000 GHz	40.1258	13.1104
1.890000000 GHz	40.0960	13.1346
1.900000000 GHz	39.9993	13.1279
1.910000000 GHz	39.9357	13.1241
1.920000000 GHz	39.8376	13.1523
1.930000000 GHz	39.7559	13.1939
1.940000000 GHz	39.7089	13.2278
1.950000000 GHz	39.6335	13.2925
1.960000000 GHz	39.6260	13.3418
1.970000000 GHz	39.5969	13.3877
1.980000000 GHz	39.5958	13.4383
1.990000000 GHz	39.6073	13.4624
2.000000000 GHz	39.6095	13.4927

Dielectric Parameter (1900MHz Body)**Title : AXW-P1900B****SubTitle : 1900 MHz Body**

January 05, 2004 01:13 PM

Frequency	e'	e''
1.700000000 GHz	52.7887	14.2488
1.710000000 GHz	52.7326	14.3045
1.720000000 GHz	52.7336	14.3510
1.730000000 GHz	52.6998	14.3745
1.740000000 GHz	52.7002	14.3883
1.750000000 GHz	52.6654	14.3836
1.760000000 GHz	52.6346	14.3904
1.770000000 GHz	52.5923	14.3815
1.780000000 GHz	52.5684	14.3794
1.790000000 GHz	52.5448	14.3844
1.800000000 GHz	52.4787	14.4184
1.810000000 GHz	52.4469	14.4562
1.820000000 GHz	52.3655	14.5224
1.830000000 GHz	52.3531	14.5694
1.840000000 GHz	52.3149	14.6425
1.850000000 GHz	52.2783	14.6856
1.860000000 GHz	52.2254	14.7036
1.870000000 GHz	52.2020	14.7284
1.880000000 GHz	52.1904	14.7359
1.890000000 GHz	52.1696	14.7193
1.900000000 GHz	52.1163	14.7249
1.910000000 GHz	52.0323	14.7227
1.920000000 GHz	51.9873	14.7219
1.930000000 GHz	51.9544	14.7250
1.940000000 GHz	51.9389	14.7844
1.950000000 GHz	51.8440	14.8488
1.960000000 GHz	51.8352	14.8954
1.970000000 GHz	51.8184	14.9389
1.980000000 GHz	51.7303	14.9847
1.990000000 GHz	51.7277	15.0047
2.000000000 GHz	51.7188	15.0202

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland

Client **Hyundai CT (Dymstec)**

CALIBRATION CERTIFICATE

Object(s) **D1900V2 - SN:5d032**

Calibration procedure(s) **QA CAL-05.v2**
Calibration procedure for dipole validation kits

Calibration date: **May 12, 2003**

Condition of the calibrated item **In Tolerance (according to the specific calibration document)**

This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.

Calibration Equipment used (M&TE critical for calibration)

Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
RF generator R&S SML-03	100698	27-Mar-2002 (R&S, No. 20-92389)	In house check: Mar-05
Power sensor HP 8481A	MY41092317	18-Oct-02 (Agilent, No. 20021018)	Oct-04
Power sensor HP 8481A	US37292783	30-Oct-02 (METAS, No. 252-0236)	Oct-03
Power meter EPM E442	GB37480704	30-Oct-02 (METAS, No. 252-0236)	Oct-03
Network Analyzer HP 8753E	US38432426	3-May-00 (Agilent, No. 8702K064602)	In house check: May 03

	Name	Function	Signature
Calibrated by:	Judith Mueller	Technician	

Approved by:	Katja Polovik	Laboratory Director
---------------------	---------------	---------------------

Date issued: May 13, 2003

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 1 245 9700, Fax +41 1 245 9779
info@speag.com, <http://www.speag.com>

DASY

Dipole Validation Kit

Type: D1900V2

Serial: 5d032

Manufactured: March 17, 2003

Calibrated: May 12, 2003

1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with head simulating solution of the following electrical parameters at 1900 MHz:

Relative Dielectricity	38.8	$\pm 5\%$
Conductivity	1.44 mho/m	$\pm 5\%$

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 5.2 at 1900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was $250 \text{ mW} \pm 3\%$. The results are normalized to 1W input power.

2. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the advanced extrapolation are:

averaged over 1 cm^3 (1 g) of tissue: **$42.0 \text{ mW/g} \pm 16.8\% (k=2)^1$**

averaged over 10 cm^3 (10 g) of tissue: **$21.6 \text{ mW/g} \pm 16.2\% (k=2)^1$**

¹ validation uncertainty

3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay: **1.195 ns** (one direction)
Transmission factor: **0.980** (voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

Feedpoint impedance at 1900 MHz: $\text{Re}\{Z\} = 50.5 \, \Omega$

$\text{Im}\{Z\} = 3.2 \, \Omega$

Return Loss at 1900 MHz **-29.9 dB**

4. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

5. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Small end caps have been added to the dipole arms in order to improve matching when loaded according to the position as explained in Section 1. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

6. Power Test

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

Date/Time: 05/12/03 20:36:30

Test Laboratory: SPEAG, Zurich, Switzerland

File Name: SN5d032_SN1507_HSL1900_120503.da4**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN5d032****Program: Dipole Calibration**

Communication System: CW-1900; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL 1900 MHz ($\sigma = 1.44 \text{ mho/m}$, $\epsilon_r = 38.8$, $\rho = 1000 \text{ kg/m}^3$)

Phantom section: Flat Section

Measurement Standard: DAS4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1507; ConvF(5.2, 5.2, 5.2); Calibrated: 1/18/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 - SN411; Calibrated: 1/16/2003
- Phantom: SAM with CRP - TP1006; Type: SAM 4.0; Serial: TP:1006
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

Pin = 250 mW; d = 10 mm/Area Scan (81x81x1): Measurement grid: dx=15mm, dy=15mm

Reference Value = 94.9 V/m

Power Drift = 0.06 dB

Maximum value of SAR = 11.6 mW/g

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Peak SAR (extrapolated) = 18.4 W/kg

SAR(1 g) = 10.5 mW/g; SAR(10 g) = 5.39 mW/g

Reference Value = 94.9 V/m

Power Drift = 0.06 dB

Maximum value of SAR = 11.8 mW/g

