



■ Test Setup Photo

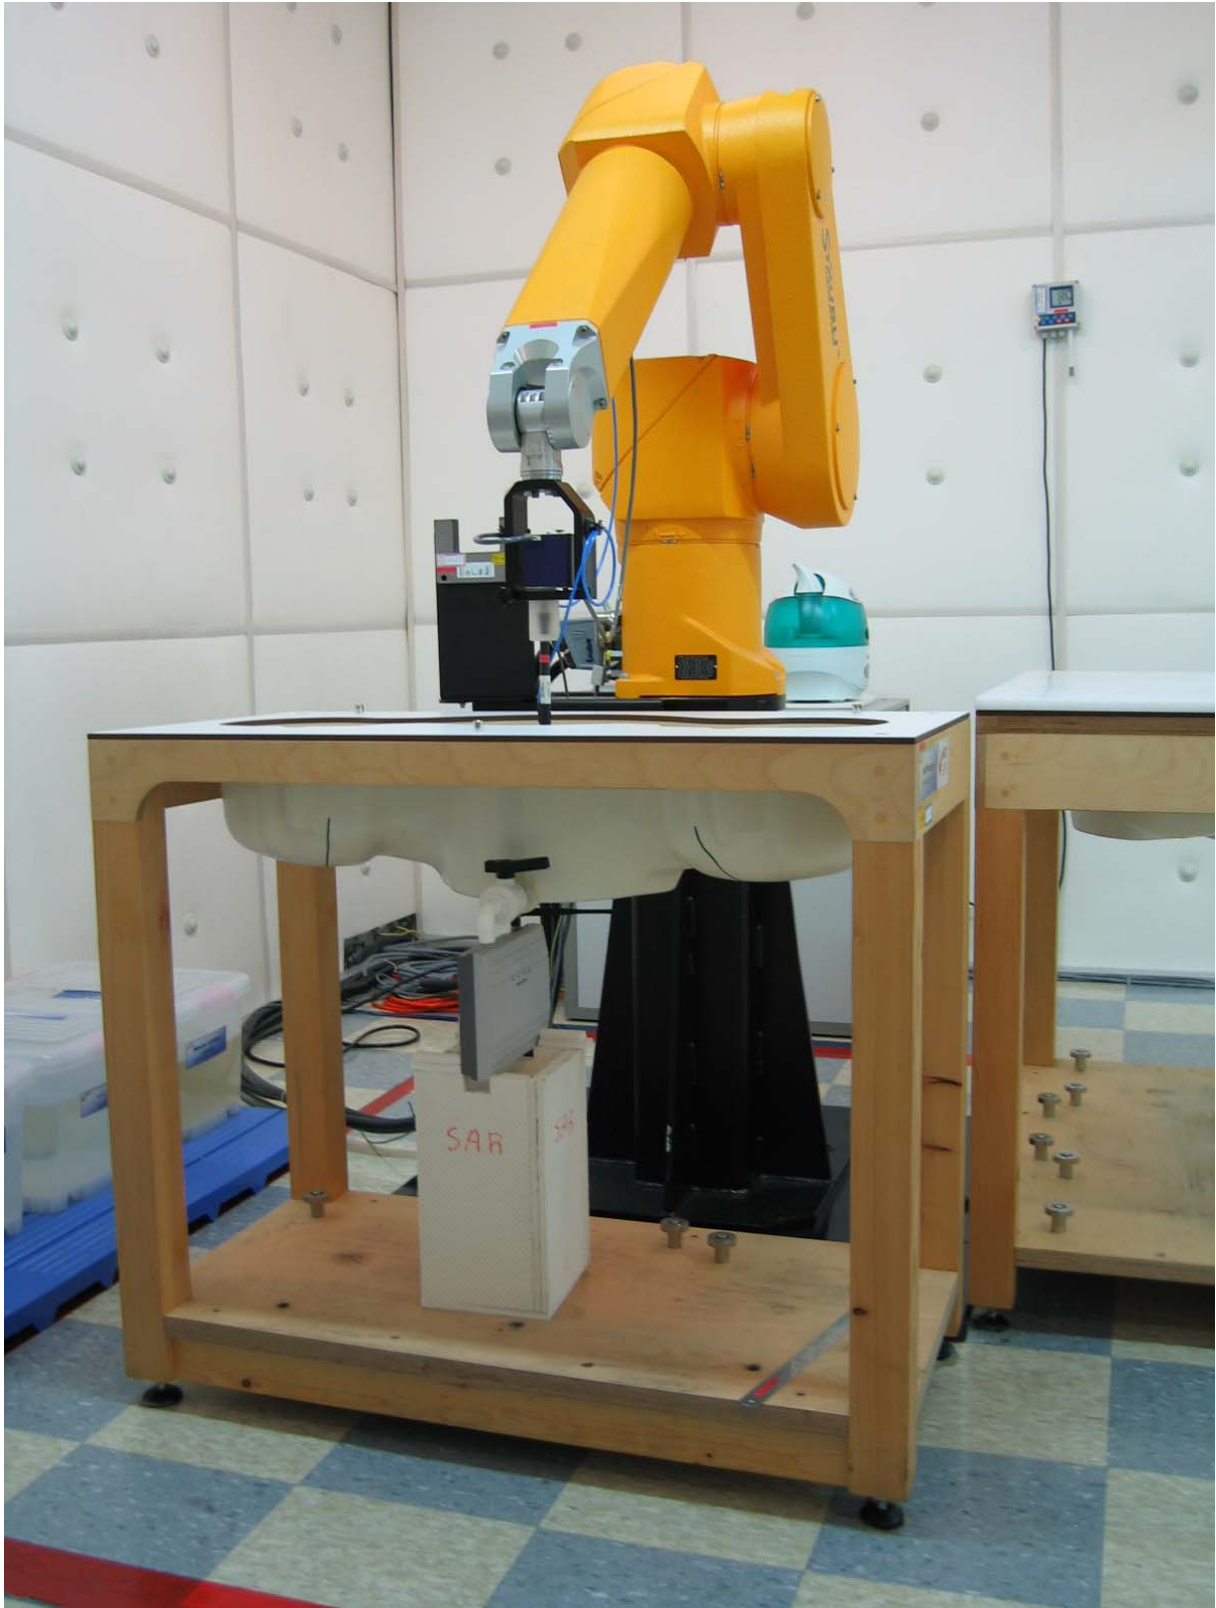


■ Test Setup Photo

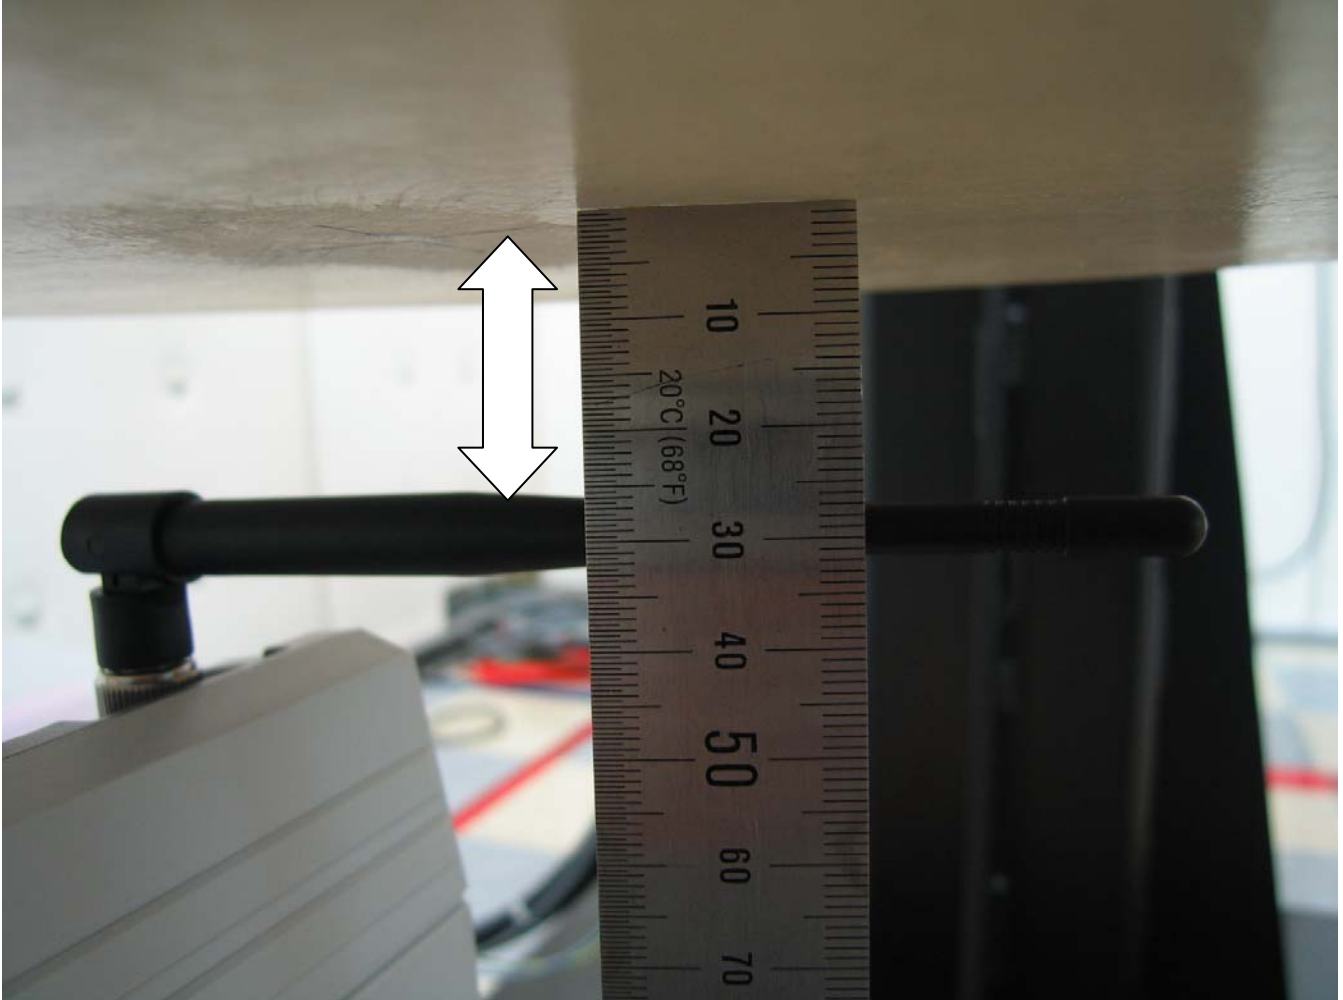

[Distance of 25 mm from the EUT]

■ Test Setup Photo

[1900 MHz Body Tissue Liquid Depth : 15cm]

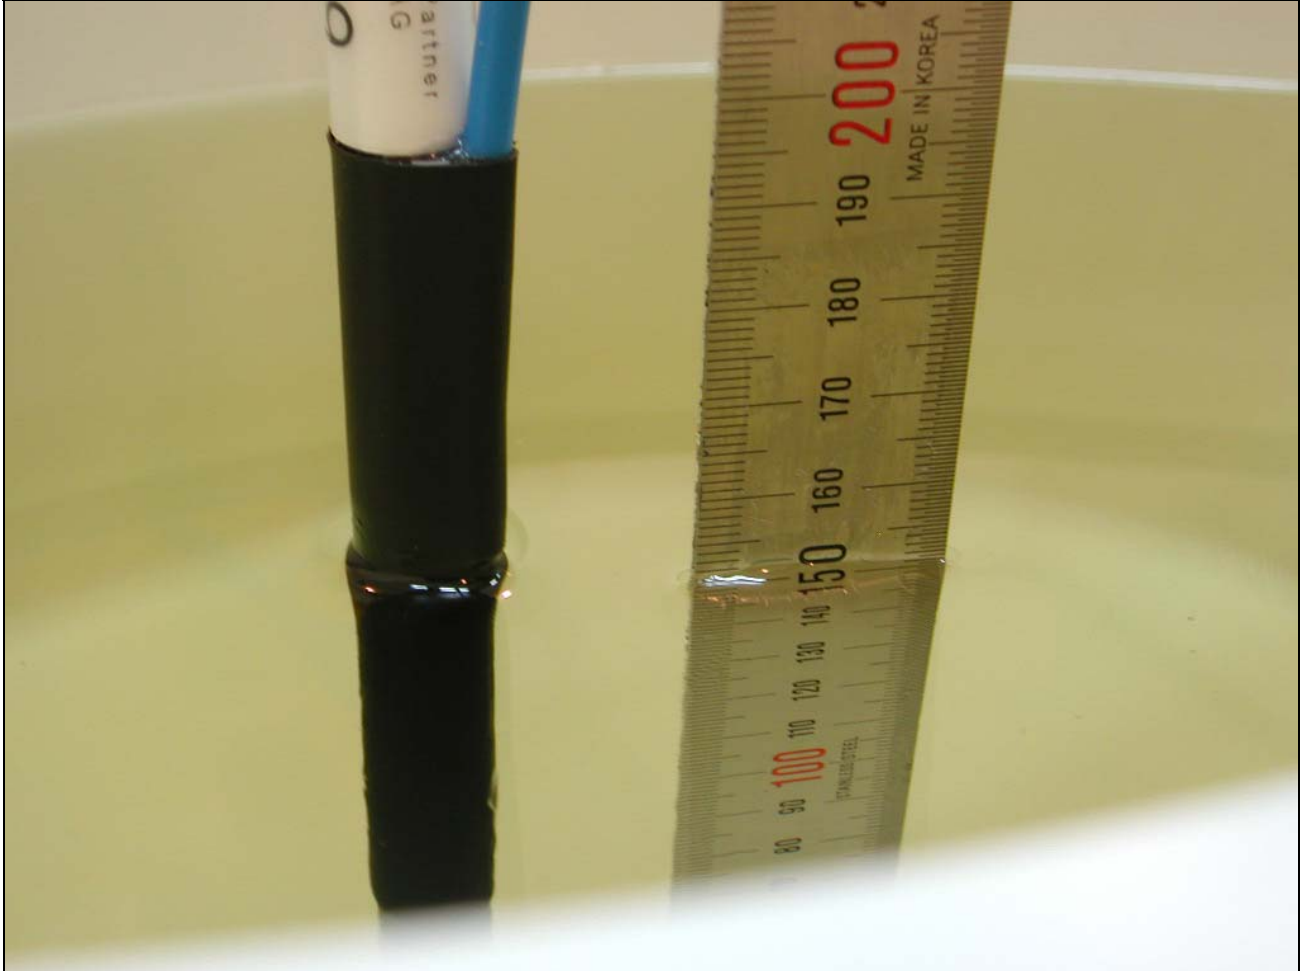

■ Test Setup Photo (Validation)

