

## SAR TEST REPORT

**Test report No:** EMC-FCC-A0013  
**Type of Equipment:** Mobile Photo Printer  
**Model Name:** M1  
**Applicant:** PRINICS Co., Ltd.  
**FCC ID:** PO5M1  
**FCC Rule Part:** CFR §2.1093  
**Test standards** FCC OET Bulletin 65 supplement C  
IEEE 1528,2003  
ANSI/IEEE C95.1  
**Max. SAR(1g)** 0.949 W/kg  
**Test result:** Complied

This report details the results of the testing carried out on one sample, the results contained in this testreport do not relate to other samples of the same product. The manufacturer should ensure that all products in series production are in conformity with the product sample detailed in this report.


This report may only be reproduced and distributed in full. If the product in this report is used in anyconfiguration other than that detailed in the report, the manufacturer must ensure the new system complies with all relevant standards. Any mention of EMC Compliance Ltd. or testing done by EMC compliance Ltd. in connection with distribution or use of the product described in this report must be approved by EMC Compliance Ltd. in writing.

Date of receipt: 2014. 07.11

Date of testing: 2014. 09.30

Issued date: 2014. 10.02

Tested by:

  
Min Kyong-hoo

Approved by:

  
Choi Cheon-sig

## Contents

|   |    |
|---|----|
| 1. Applicant information .....            | 3  |
| 2. Laboratory information .....           | 4  |
| 3. Identification of Sample.....          | 5  |
| 4. Test Result Summary .....              | 6  |
| 5. Report Overview .....                  | 6  |
| 6. Test Lab Declaration or Comments.....  | 6  |
| 7. Applicant Declaration or Comments..... | 6  |
| 8. Measurement Uncertainty .....          | 7  |
| 9. The SAR Measurement System .....       | 8  |
| 9.1 Isotropic E-field Probe EX3DV4 .....  | 9  |
| 9.2 Phantom.....                          | 10 |
| 9.3 Device Holder for Transmitters .....  | 11 |
| 10. System Verification.....              | 12 |
| 10.1 Tissue Verification .....            | 12 |
| 10.2 Test System Verification .....       | 14 |
| 11. Operation Configurations .....        | 15 |
| 12. SAR Measurement Procedures .....      | 16 |
| 13. Test Equipment Information.....       | 18 |
| 14. RF Power.....                         | 19 |
| 14.1 Average Conducted Output Power.....  | 19 |
| 14.2 Max. tune up power.....              | 19 |
| 15. SAR Test Results .....                | 19 |
| 16. Test System Verification Results..... | 20 |
| 17. Test Results.....                     | 21 |
| Annex A. Photographs.....                 | 29 |
| Annex B. Calibration certificate .....    | 37 |

## 1. Applicant information

**Applicant:** PRINICS Co., Ltd.  
**Address:** 3F, 108, Saneop-Ro, Gwonseon-Gu, Suwon-Si, Gyeonggi-Do, Korea  
**Telephone No.:** +82-31-293-5993  
**Facsimile No.:** +82-31-293-5994  
**Contact Person:** Jungbok-Kim/ jbkim@prinics.com

**Manufacturer:** PRINICS Co., Ltd.  
**Address:** 3F, 108, Saneop-Ro, Gwonseon-Gu, Suwon-Si, Gyeonggi-Do, Korea

## 2. Laboratory information

### Address

**EMC compliance Ltd.**

65, Sinwon-ro, Yeongtong-gu, Suwon- si, Gyeonggi-do, 443-390, Korea

Telephone No.: 82-31-336-9919      Facsimile No.: 82-505-299-8311

### Certificate


KOLAS No.: 231

FCCSite Registration No.: 687132

VCCI Site Registration No.: R-3327, G-198, C-3706, T-1849

IC Site Registration No.:8035A-2

### SITE MAP

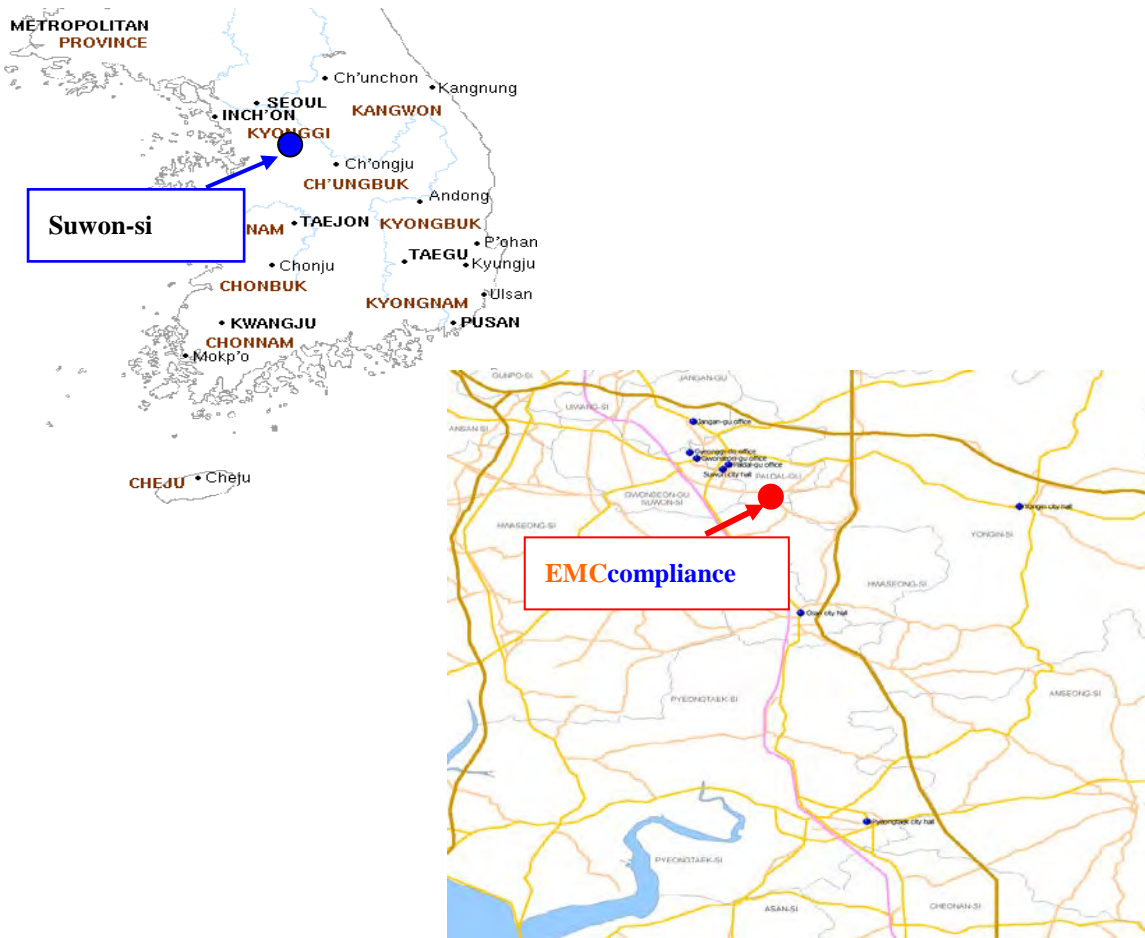

### 3. Identification of Sample

|                   |  |
|-------------------|--|
| Mode of Operation | WLAN 802.11b/g/n(HT-20)  |
| Model Number      | M1   |
| Serial Number     | N/A  |
| Sample Version    | N/A  |
| TxFreq.Range      | 2412 MHz ~ 2462 MHz  |
| Rx Freq.Range     | 2412 MHz ~ 2462 MHz  |
| RF Output Power   | 802.11b : 16.5 dBm<br>802.11g : 14 dBm<br>802.11n(HT-20) : 9 dBm |
| Antenna Type      | PCB Antenna  |
| Antenna Gain      | - 0.37 dBi   |
| Normal Voltae     | DC 7.4 V   |

## 4. Test Result Summary

| Frequency |     | RF Output Power (dBm) | Max. tune up power (dBm) | Scaling Factor | EUT Position | Distance (mm) | Measured 1 g SAR (W/kg) | Scaled 1 g SAR (W/kg) |
|-----------|-----|-----------------------|--------------------------|----------------|--------------|---------------|-------------------------|-----------------------|
| MHz       | Ch. |                       |                          |                |              |               |                         |                       |
| 2 412     | 1   | 14.53                 | 16.5                     | 1.574          | Left         | 0             | 0.603                   | <b>0.949</b>          |

## 5. Report Overview

This report details the results of testing carried out on the samples listed in section 3, the results contained in this test report do not relate to other samples of the same product. The manufacturer should ensure that all products in series production are in conformity with the product sample detailed in this report.

This report may only be reproduced and distributed in full. If the product in this test report is used in any configuration other than that detailed in the test report, the manufacturer must ensure the new configuration complies with all relevant standards and certification requirements. Any mention of EMC Compliance Ltd Wireless lab or testing done by EMC Compliance Ltd Wireless lab made in connection with the distribution or use of the tested product must be approved in writing by EMC Compliance Ltd Wireless lab.

## 6. Test Lab Declaration or Comments

None

## 7. Applicant Declaration or Comments

None

## 8. Measurement Uncertainty


All measurements and results are recorded and maintained at the laboratory performing the tests and measurement uncertainties are taken into account when comparing measurements to pass/ fail criteria.

### Uncertainty of SAR equipments for measurement Body300 MHz to 3GHz

#### 2013 FCC SAR Measurement Uncertainty

| <i>A</i>   | <i>b</i>                  | <i>c</i>                           | <i>D</i>                    | $\epsilon = f(d,k)$ | <i>g</i> | $i = c \times g / \epsilon$ | <i>k</i>         |
|--|---------------------------|------------------------------------|-----------------------------|---------------------|----------|-----------------------------|------------------|
| Source of Uncertainty  | Description<br>IEEE P1528 | Tolerance/<br>Uncertainty<br>value | Probability<br>Distribution | Div.                | Ci       | Standard<br>uncertainty     | Vi<br>or<br>Veff |
|  | (0.3 ~ 3 GHz)             | ± %                                |                             |                     | (1 g)    | ± %, (1 g)                  |                  |
| <b>Measurement System</b>  |                           |                                    |                             |                     |          |                             |                  |
| Probe calibration(k=1)   | E.2.1                     | 6.30                               | N                           | 1                   | 1        | 6.30                        | ∞                |
| Axial isotropy   | E.2.2                     | 0.50                               | R                           | 1.73                | 0.71     | 0.20                        | ∞                |
| Hemispherical isotropy   | E.2.2                     | 2.60                               | R                           | 1.73                | 0.71     | 1.06                        | ∞                |
| Linearity  | E.2.4                     | 0.60                               | R                           | 1.73                | 1        | 0.35                        | ∞                |
| Boundary effect  | E.2.3                     | 1.00                               | R                           | 1.73                | 1        | 0.58                        | ∞                |
| System detection limits  | E.2.5                     | 1.00                               | R                           | 1.73                | 1        | 0.58                        | ∞                |
| Readout electronics  | E.2.6                     | 0.30                               | N                           | 1                   | 1        | 0.30                        | ∞                |
| Response time  | E.2.7                     | 0.80                               | R                           | 1.73                | 1        | 0.46                        | ∞                |
| Integration time   | E.2.8                     | 2.60                               | R                           | 1.73                | 1        | 1.50                        | ∞                |
| RF ambient conditions—noise  | E.6.1                     | 3.00                               | R                           | 1.73                | 1        | 1.73                        | ∞                |
| RF ambient conditions—<br>reflections  | E.6.1                     | 3.00                               | R                           | 1.73                | 1        | 1.73                        | ∞                |
| Probe positioner mechanical<br>tolerance   | E.6.2                     | 0.40                               | R                           | 1.73                | 1        | 0.23                        | ∞                |
| Probe positioning with respect to<br>phantom shell                                     | E.6.3                     | 2.90                               | R                           | 1.73                | 1        | 1.67                        | ∞                |
| Extrapolation, interpolation, and<br>integration algorithms for max.<br>SAR evaluation | E.5                       | 2.00                               | R                           | 1.73                | 1        | 1.15                        | ∞                |
| <b>Test Sample Related</b>   |                           |                                    |                             |                     |          |                             |                  |
| Test sample positioning  | E.4.2                     | 4.71                               | N                           | 1                   | 1        | 4.71                        | 9                |
| Device holder uncertainty  | E.4.1                     | 3.60                               | N                           | 1                   | 1        | 3.60                        | 5                |
| Output power variation—SAR<br>drift measurement  | 6.6.2                     | 5.00                               | R                           | 1.73                | 1        | 2.89                        | ∞                |
| <b>Phantom and Tissue Parameters</b>   |                           |                                    |                             |                     |          |                             |                  |
| Phantom uncertainty<br>(shape and thickness tolerances)                                | E.3.1                     | 7.50                               | R                           | 1.73                | 1        | 4.33                        | ∞                |
| Liquid conductivity-measurement<br>uncertainty   | E.3.3                     | 1.53                               | N                           | 1                   | 0.64     | 0.98                        | 5                |
| Liquid permittivity-measurement<br>uncertainty   | E.3.3                     | 3.07                               | N                           | 1                   | 0.6      | 1.84                        | 5                |
| Liquid conductivity-deviation<br>from target values                                    | E.3.2                     | 5.00                               | R                           | 1.73                | 0.64     | 1.85                        | ∞                |
| Liquid permittivity-deviation<br>from target values                                    | E.3.2                     | 5.00                               | R                           | 1.73                | 0.6      | 1.73                        | ∞                |
| Combined standard uncertainty  |                           |                                    |                             | RSS                 |          | 11.29                       | 183              |
| Expanded uncertainty<br>(95% CONFIDENCE<br>INTERVAL)                                   |                           |                                    |                             | K=2                 |          | 22.57                       |                  |

## 9. The SAR Measurement System

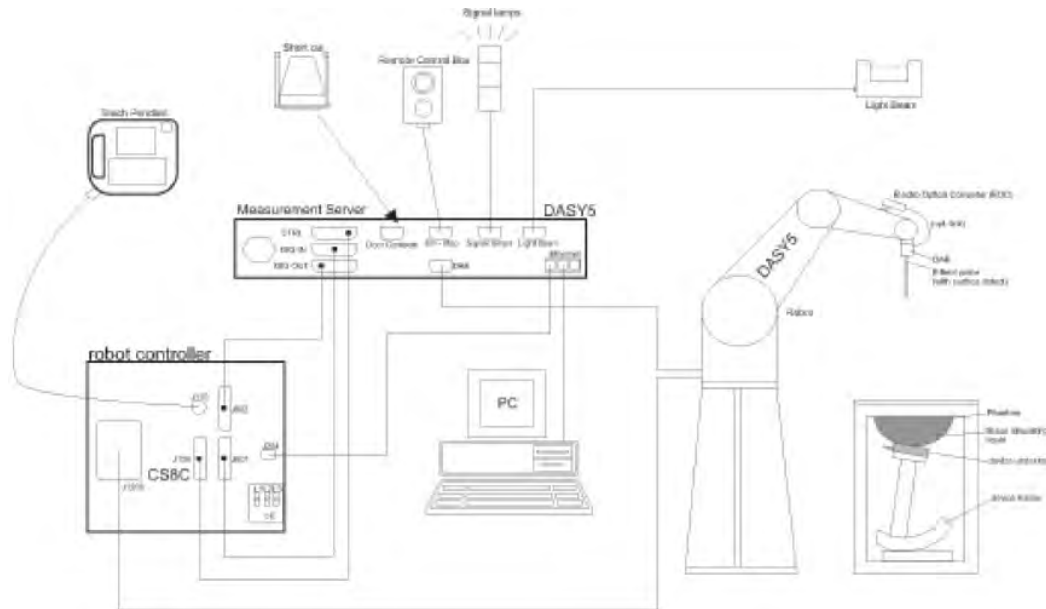


### <SAR System Configuration>

- A standard high precision 6-axis robot with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- An isotropic Field probe optimized and calibrated for the targeted measurement.
- Data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion from optical to electrical signals for the digital communication to the DAE. To use optical surface detection, a special version of the EOC is required. The EOC signal is transmitted to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- The Light Beam used is for probe alignment. This improves the (absolute) accuracy of the probe positioning.
- A computer running WinXP or Win7 and the DASY5 software.
- Remote control and teach pendant as well as additional circuitry for robot safety such as warning lamps, etc.
- The phantom, the device holder and other accessories according to the targeted measurement.



## 9.1 Isotropic E-field Probe EX3DV4

| <b>EX3DV4</b><br><b>Smallest Isotropic E-Field Probe for Dosimetric Measurements</b><br><b>(Preliminary Specifications)</b> |   |
|---|---|
|    | Symmetrical design with triangular core<br>Built-in shielding against static charges<br>PEEK enclosure material (resistant to organic solvents, e.g., DGBE)   |
| <b>Calibration</b>  | ISO/IEC 17025 <a href="#">calibration service</a> available.  |
| <b>Frequency</b>  | 10 MHz to > 6 GHz<br>Linearity: $\pm 0.2$ dB (30 MHz to 6 GHz)  |
| <b>Directivity</b>  | $\pm 0.3$ dB in TSL (rotation around probe axis)<br>$\pm 0.5$ dB in TSL (rotation normal to probe axis)   |
| <b>Dynamic Range</b>  | 10 $\mu$ W/g to > 100 mW/g<br>Linearity: $\pm 0.2$ dB (noise: typically < 1 $\mu$ W/g)  |
| <b>Dimensions</b>   | Overall length: 337 mm (Tip: 20 mm)<br>Tip diameter: 2.5 mm (Body: 12 mm)<br>Typical distance from probe tip to dipole centers: 1 mm  |
| <b>Application</b>  | High precision dosimetric measurements in any exposure scenario (e.g., very strong gradient fields); the only probe that enables compliance testing for frequencies up to 6 GHz with precision of better 30%. |
| <b>Compatibility</b>  | DASY3, DASY4, DASY52 SAR and higher, EASY4/MRI  |

## 9.2 Phantom

| Twin SAM  |  |
|---|--|
|  | <p>The shell corresponds to the specifications of the Specific Anthropomorphic Mannequin (SAM) phantom defined in IEEE 1528 and IEC 62209-1. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents evaporation of the liquid. Reference markings on the phantom allow the complete setup of all predefined phantom positions and measurement grids by teaching three points with the robot.</p> <p>Twin SAM V5.0 has the same shell geometry and is manufactured from the same material as Twin SAM V4.0, but has reinforced top structure.</p> |
| <b>Material</b>   | Vinylester, glass fiber reinforced (VE-GF)   |
| <b>Liquid Compatibility</b>   | Compatible with all SPEAG tissue simulating liquids (incl. DGBE type)  |
| <b>Shell Thickness</b>  | 2 ± 0.2 mm (6 ± 0.2 mm at ear point)   |
| <b>Dimensions</b><br>(incl. Wooden Support)                                       | Length: 1000 mm<br>Width: 500 mm<br>Height: adjustable feet  |
| <b>Filling Volume</b>   | approx. 25 liters  |
| <b>Wooden Support</b>   | SPEAG standard phantom table   |
| <b>Accessories</b>  | <a href="#">Mounting Device and Adaptors</a>   |

## 9.3 Device Holder for Transmitters

### Mounting Devices and Adaptors



Mounting Device for Hand-Held Transmitters

#### MD4HHTV5 - Mounting Device for Hand-Held Transmitters

In combination with the Twin SAM V5.0/V5.0c or ELI Phantoms, the Mounting Device for Hand-Held Transmitters enables rotation of the mounted transmitter device to specified spherical coordinates. At the heads, the rotation axis is at the ear opening. Transmitter devices can be easily and accurately positioned according to IEC 62209-1, IEEE 1528, FCC, or other specifications. The device holder can be locked for positioning at different phantom sections (left head, right head, flat).

**Material:** Polyoxymethylene (POM)

## 10. System Verification

### 10.1 Tissue Verification

The dielectric properties for this Tissue Simulant Liquids were measured by using the Speag DAK-3.5 in conjunction with Agilent E5071B Network Analyzer. The Conductivity ( $\sigma$ ) and Permittivity ( $\rho$ ) are listed in Table 1. For the SAR measurement given in this report. The temperature variation of the Tissue Simulant Liquids was  $(21 \pm 2) ^\circ\text{C}$ .

| Freq. (MHz) | Tissue Type | Limit/Measured       | Permittivity ( $\rho$ )                | Conductivity ( $\sigma$ )           | Temp ( $^\circ\text{C}$ ) |
|-------------|-------------|----------------------|--|-------------------------------------|---------------------------|
| 2 412       | Body        | Recommended Limit    | 52.75 $\pm$ 5 %<br>(50.1131 ~ 55.3882) | 1.91 $\pm$ 5 %<br>(1.8180 ~ 2.0094) | 21 $\pm$ 2                |
|             |             | Measured, 2014-09-30 | 51.18                                  | 1.93                                | 22.32                     |
| 2 437       | Body        | Recommended Limit    | 52.72 $\pm$ 5 %<br>(50.0815 ~ 55.3532) | 1.94 $\pm$ 5 %<br>(1.8407 ~ 2.0345) | 21 $\pm$ 2                |
|             |             | Measured, 2014-09-30 | 51.07                                  | 1.96                                | 22.32                     |
| 2 450       | Body        | Recommended Limit    | 52.70 $\pm$ 5 %<br>(50.0650 ~ 55.3350) | 1.95 $\pm$ 5 %<br>(1.8525 ~ 2.0475) | 21 $\pm$ 2                |
|             |             | Measured, 2014-09-30 | 51.01                                  | 1.97                                | 22.32                     |
| 2 462       | Body        | Recommended Limit    | 52.69 $\pm$ 5 %<br>(50.0530 ~ 55.3218) | 1.93 $\pm$ 5 %<br>(1.8380 ~ 2.0315) | 21 $\pm$ 2                |
|             |             | Measured, 2014-09-30 | 50.96                                  | 1.98                                | 22.32                     |

<Table 1.Measurement result of Tissue electric parameters>

The following tissue formulations are provided for reference only as some of the parameters have not been thoroughly verified. The composition of ingredients may be modified accordingly to achieve the desired target tissue parameters required for routine SAR evaluation.

| Ingredients<br>(% by weight) | Frequency (MHz) |       |       |      |       |       |       |      |      |      |
|------------------------------|-----------------|-------|-------|------|-------|-------|-------|------|------|------|
|                              | 450             |       | 835   |      | 915   |       | 1900  |      | 2450 |      |
| Tissue Type                  | Head            | Body  | Head  | Body | Head  | Body  | Head  | Body | Head | Body |
| Water                        | 38.56           | 51.16 | 41.45 | 52.4 | 41.05 | 56.0  | 54.9  | 40.4 | 62.7 | 73.2 |
| Salt (NaCl)                  | 3.95            | 1.49  | 1.45  | 1.4  | 1.35  | 0.76  | 0.18  | 0.5  | 0.5  | 0.04 |
| Sugar                        | 56.32           | 46.78 | 56.0  | 45.0 | 56.5  | 41.76 | 0.0   | 58.0 | 0.0  | 0.0  |
| HEC                          | 0.98            | 0.52  | 1.0   | 1.0  | 1.0   | 1.21  | 0.0   | 1.0  | 0.0  | 0.0  |
| Bactericide                  | 0.19            | 0.05  | 0.1   | 0.1  | 0.1   | 0.27  | 0.0   | 0.1  | 0.0  | 0.0  |
| Triton X-100                 | 0.0             | 0.0   | 0.0   | 0.0  | 0.0   | 0.0   | 0.0   | 0.0  | 36.8 | 0.0  |
| DGBE                         | 0.0             | 0.0   | 0.0   | 0.0  | 0.0   | 0.0   | 44.92 | 0.0  | 0.0  | 26.7 |
| Dielectric Constant          | 43.42           | 58.0  | 42.54 | 56.1 | 42.0  | 56.8  | 39.9  | 54.0 | 39.8 | 52.5 |
| Conductivity (S/m)           | 0.85            | 0.83  | 0.91  | 0.95 | 1.0   | 1.07  | 1.42  | 1.45 | 1.88 | 1.78 |

Salt: 99<sup>+</sup>% Pure Sodium Chloride

Sugar: 98<sup>+</sup>% Pure Sucrose

Water: De-ionized, 16 MΩ<sup>+</sup> resistivity


HEC: Hydroxyethyl Cellulose

DGBE: 99<sup>+</sup>% Di(ethylene glycol) butyl ether, [2-(2-butoxyethoxy)ethanol]

Triton X-100 (ultra pure): Polyethylene glycol mono [4-(1,1, 3, 3-tetramethylbutyl)phenyl]ether

## 10.2 Test System Verification

The microwave circuit arrangement for system verification is sketched below picture. The daily system accuracy verification occurs within the flat section of the SAM phantom. A SAR measurement was performed to see if the measured SAR was within  $\pm 10\%$  from the target SAR values. These tests were done at 2450MHz. The tests were conducted on the same days as the measurement of the EUT. The obtained results from the system accuracy verification are displayed in the table Table 2 (A power level of 250mW was input to the dipole antenna). During the tests, the ambient temperature of the laboratory was in the range  $(21 \pm 2)^\circ\text{C}$ , the relative humidity was in the range  $(50 \pm 20)\%$  and the liquid depth above the ear/grid reference points was above 15 cm in all the cases. It is seen that the system is operating within its specification, as the results are within acceptable tolerance of the reference values.

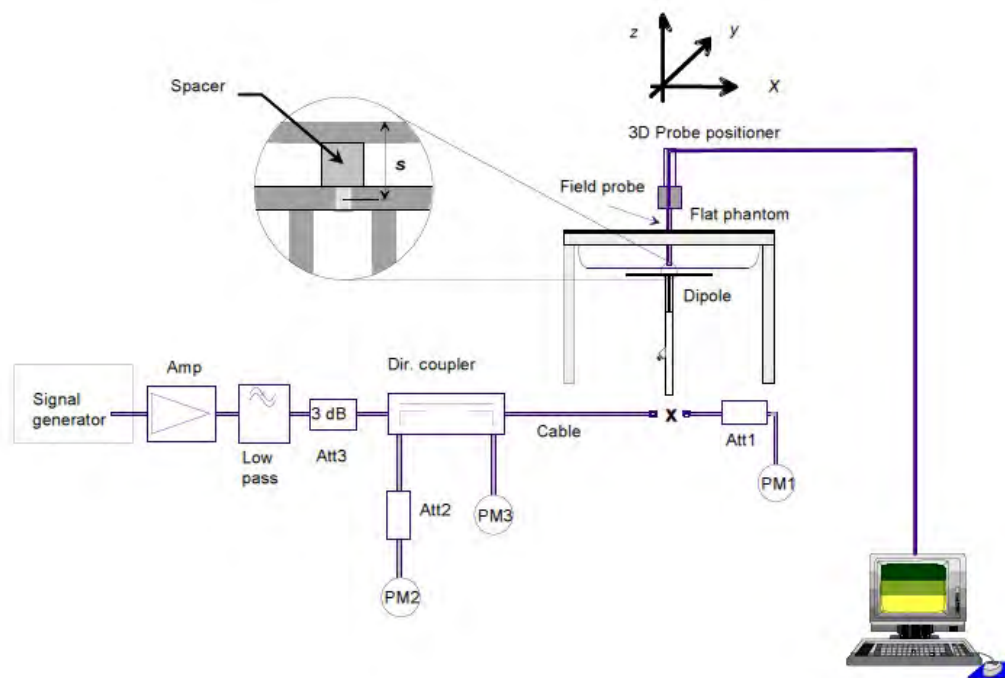

| Validation Kit | Dipole Ant. S/N | Frequency (MHz) | Tissue Type | Limit/Measurement (Normalized to 1 W) |                                    |                                    |
|----------------|-----------------|-----------------|-------------|---------------------------------------|------------------------------------|------------------------------------|
|                |                 |                 |             |                                       | 1 g                                | 10 g                               |
| D2450V2        | 895             | 2 450           | Body        | Recommended Limit (Normalized)        | 50.9 $\pm$ 10 %<br>(45.81 ~ 55.99) | 23.6 $\pm$ 10 %<br>(21.24 ~ 25.96) |
|                |                 |                 |             | Measured, 2014-09-30                  | 54.00                              | 25.08                              |

<Table 2. Test System Verification Result>

## 11. Operation Configurations

For the Wireless Transceiver SAR tests, a communication link is set up with the operating mode for can be controlled by EUT. The Absolute Radio Frequency Channel Number is allocated to 1,6and 11 respectively in the case of 2412 ~ 2462MHz.During the test,at the each test frequency channel, the EUT is operated at the RF continuous emission mode.

## 12. SAR Measurement Procedures

### Step 1: Power Reference Measurement

The Power Reference Measurement and Power Drift Measurements are for monitoring the power drift of the device under test in the batch process. The Minimum distance of probe sensors to surface determines the closest measurement point to phantom surface. The minimum distance of probe sensor to surface is 2 mm. This distance cannot be smaller than the Distance of sensor calibration points to probe tip as defined in the probe properties.

### Step 2: Area Scan

The Area Scan is used as a fast scan in two dimensions to find the area of high field values, before doing a fine measurement around the hot spot. The sophisticated interpolation routines implemented in DASY software can find the maximum locations even in relatively coarse grids. When an Area Scan has measured all reachable points, it computes the field maximal found in the scanned area, within a range of the global maximum. The range (in dB) is specified in the standards for compliance testing. For example, a 2 dB range is required in IEEE Standard 1528 and IEC 62209 standards, whereby 3 dB is a requirement when compliance is assessed in accordance with the ARIB standard (Japan). If only one Zoom Scan follows the Area Scan, then only the absolute maximum will be taken as reference. For cases where multiple maximums are detected, the number of Zoom Scans has to be increased accordingly.

Area Scan Parameters extracted from KDB 865664 D01 SAR Measurement 100 MHz to 6 GHz v01r03.

|  | ≤ 3 GHz   | > 3 GHz  |
|--|---|--|
| Maximum distance from closest measurement point (geometric center of probe sensors) to phantom surface | 5 ± 1 mm  | $\frac{1}{2} \cdot \delta \cdot \ln(2) \pm 0.5$ mm |
| Maximum probe angle from probe axis to phantom surface normal at the measurement location              | 30° ± 1°  | 20° ± 1°   |
| Maximum area scan spatial resolution: $\Delta x_{Area}$ , $\Delta y_{Area}$                            | ≤ 2 GHz: ≤ 15 mm<br>2 – 3 GHz: ≤ 12 mm  | 3 – 4 GHz: ≤ 12 mm<br>4 – 6 GHz: ≤ 10 mm           |
|  | When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the above, the measurement resolution must be ≤ the corresponding x or y dimension of the test device with at least one measurement point on the test device. |  |



### Step 3: Zoom Scan

Zoom Scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The Zoom Scan measures 5x5x7 points within a cube whose base faces are centered on the maxima found in a preceding area scan job within the same procedure. When the measurement is done, the Zoom Scan evaluates the averaged SAR for 1 g and 10 g and displays these values next to the job's label.

Zoom Scan Parameters extracted from KDB 865664 D01 SAR Measurement 100 MHz to 6 GHz v01r03.

|  |   |   | ≤ 3 GHz                               | > 3 GHz  |
|--|---|---|---------------------------------------|--|
| Maximum zoom scan spatial resolution, normal to phantom surface  | uniform grid: $\Delta z_{\text{Zoom}(n)}$ |   | ≤ 5 mm                                | 3 – 4 GHz: ≤ 4 mm<br>4 – 5 GHz: ≤ 3 mm<br>5 – 6 GHz: ≤ 2 mm    |
|  | graded grid                               | $\Delta z_{\text{Zoom}(1)}$ : between 1 <sup>st</sup> two points closest to phantom surface | ≤ 4 mm                                | 3 – 4 GHz: ≤ 3 mm<br>4 – 5 GHz: ≤ 2.5 mm<br>5 – 6 GHz: ≤ 2 mm  |
|  |   | $\Delta z_{\text{Zoom}(n>1)}$ : between subsequent points                                   | ≤ 1.5 · $\Delta z_{\text{Zoom}(n-1)}$ |  |
| Minimum zoom scan volume   | x, y, z                                   |   | ≥ 30 mm                               | 3 – 4 GHz: ≥ 28 mm<br>4 – 5 GHz: ≥ 25 mm<br>5 – 6 GHz: ≥ 22 mm |
| Note: $\delta$ is the penetration depth of a plane-wave at normal incidence to the tissue medium; see draft standard IEEE P1528-2011 for details.<br>* When zoom scan is required and the <i>reported</i> SAR from the <i>area scan based 1-g SAR estimation</i> procedures of KDB 447498 is ≤ 1.4 W/kg, ≤ 8 mm, ≤ 7 mm and ≤ 5 mm zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz. |   |   |                                       |  |

### Step 4: Power drift measurement

The Power Drift Measurement measures the field at the same location as the most recent power reference measurement within the same procedure, and with the same settings. The Power Drift Measurement gives the field difference in dB from the reading conducted within the last Power Reference Measurement. This allows a user to monitor the power drift of the device under test within a batch process. The measurement procedure is the same as Step 1.

### Step 5: Z-Scan

The Z Scan measures points along a vertical straight line. The line runs along the Z-axis of a one-dimensional grid. In order to get a reasonable extrapolation, the extrapolated distance should not be larger than the step size in Z-direction.

\* Z Scan Report on Liquid Measure the height Annex A.4 Liquid Depth photo to replace

### 13. Test Equipment Information

| Test Platform                | SPEAG DASY5 System                            |                 |                     |                              |
|------------------------------|---|-----------------|---------------------|------------------------------|
| Description                  | SAR Test System (Frequency range 300MHz-6GHz) |                 |                     |                              |
| Software Reference           | DASY5: V52.8.8.1222, SEMCAD: V14.6.10 (7331)  |                 |                     |                              |
| Hardware Reference           |   |                 |                     |                              |
| Equipment                    | Model   | Serial Number   | Date of Calibration | Due date of next Calibration |
| DASY5 Robot                  | TX90XL Speag                                  | F12/5L7FA1/A/01 | N/A                 | N/A                          |
| DASY5 Controller             | TX90XL Speag                                  | F12/5L7FA1/C/01 | N/A                 | N/A                          |
| Phantom                      | TwinSAM Phantom                               | 1728            | N/A                 | N/A                          |
| Mounting Device              | Mounting Device                               | None            | N/A                 | N/A                          |
| DAE                          | DAE4  | 1342            | 2014-07-24          | 2015-07-24                   |
| Probe                        | EX3DV4  | 3928            | 2014-01-15          | 2015-01-15                   |
| Dipole Validation Kits       | D2450V2                                       | 895             | 2014-07-24          | 2016-07-24                   |
| Network Analyzer             | E5071B  | MY42403524      | 2014-07-15          | 2015-07-15                   |
| Dielectric Assessment Kit    | DAK-3.5                                       | 1078            | 2014-08-19          | 2015-08-19                   |
| Dual Directional Coupler     | 772D  | 2839A00719      | 2014-08-29          | 2015-08-29                   |
| Signal Generator             | E4438C  | MY42080486      | 2014-02-11          | 2015-02-11                   |
| Power Amplifier              | 2055-BBS3Q7E9I                                | 1005D/C0521     | 2014-05-15          | 2015-05-15                   |
| Dual Power Meter             | E4419B  | GB43312301      | 2014-07-17          | 2015-07-17                   |
| Power Sensor                 | 8481H   | 3318A19377      | 2014-08-30          | 2015-08-30                   |
| Power Sensor                 | 8481H   | 331BA19379      | 2014-08-30          | 2015-08-30                   |
| LP Filter                    | LA-30N  | 40058           | 2014-08-28          | 2015-08-28                   |
| Humidity/Temp. Data Recorder | MHB-382SD                                     | 73871           | 2014-08-26          | 2015-08-26                   |

## 14. RF Power

### 14.1 Average Conducted Output Power

| WLAN                    | 2 412 MHz | 2 437 MHz | 2 462 MHz |
|-------------------------|-----------|-----------|-----------|
| 802.11b 1 Mbps          | 14.53dBm  | 15.47dBm  | 16.42dBm  |
| 802.11g 6 Mbps          | 12.65 dBm | 12.20 dBm | 12.24 dBm |
| 802.11n(HT-20) 6.5 Mbps | 8.09 dBm  | 7.06 dBm  | 7.56 dBm  |

### 14.2 Max. tune up power

| WLAN           | 2 412 MHz | 2 437 MHz | 2 462 MHz |
|----------------|-----------|-----------|-----------|
| 802.11b        | 16.5dBm   | 16.5 dBm  | 16.5 dBm  |
| 802.11g        | 14.0dBm   | 14.0dBm   | 14.0dBm   |
| 802.11n(HT-20) | 9.0dBm    | 9.0dBm    | 9.0dBm    |

## 15. SAR Test Results

| Frequency |         | Average Power (dBm) | Max. tune up power (dBm) | Scaling Factor | EUT Position | Distance (mm) | Measured 1 g SAR (W/kg) | Scaled 1 g SAR (W/kg) |
|-----------|---------|---------------------|--------------------------|----------------|--------------|---------------|-------------------------|-----------------------|
| MHz       | Channel |                     |                          |                |              |               |                         |                       |
| 2 437     | 6       | 15.47               | 16.5                     | 1.268          | Front        | 0             | 0.111                   | 0.141                 |
| 2 437     | 6       | 15.47               | 16.5                     | 1.268          | Back         | 0             | 0.558                   | 0.708                 |
| 2 437     | 6       | 15.47               | 16.5                     | 1.268          | Top          | 0             | 0.063                   | 0.080                 |
| 2 437     | 6       | 15.47               | 16.5                     | 1.268          | Left         | 0             | 0.603                   | 0.765                 |
| 2 437     | 6       | 15.47               | 16.5                     | 1.268          | Right        | 0             | 0.015                   | 0.019                 |
| 2 437     | 6       | 15.47               | 16.5                     | 1.268          | Bottom       | 0             | 0.029                   | 0.037                 |
| 2 412     | 1       | 14.53               | 16.5                     | 1.574          | Left         | 0             | 0.603                   | <b>0.949</b>          |
| 2 462     | 11      | 16.42               | 16.5                     | 1.019          | Left         | 0             | 0.658                   | 0.671                 |

<Note>

SAR values were scaled to the maximum allowed power to determine compliance per KDB Publication 447498 D01v05r02.

## 16. Test System Verification Results

### System check for 2 450MHz-Body(2014-09-30)

DUT: Dipole 2450 MHz D2450V2; Type: D2450V2; Serial: D2450V2 - SN:895  
Procedure Name: d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe)

Communication System: UID 0, cw1; Frequency: 2450 MHz; Duty Cycle: 1:1  
Medium parameters used:  $f = 2450$  MHz,  $\sigma = 1.972$  S/m,  $\epsilon_r = 51.011$ ,  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section


DASY5 Configuration:

- Probe: EX3DV4 - SN3928; ConvF(6.84, 6.84, 6.84); Calibrated: 2014-01-15;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1342; Calibrated: 2014-07-24
- Phantom: SAM twin 1728; Type: QD000P40CD; Serial: TP:1728
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

System Performance Check at Frequencies/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Area Scan (81x101x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm  
Maximum value of SAR (interpolated) = 20.7 W/kg

System Performance Check at Frequencies/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 102.2 V/m; Power Drift = 0.10 dB  
Peak SAR (extrapolated) = 27.4 W/kg  
SAR(1 g) = 13.5 W/kg; SAR(10 g) = 6.27 W/kg  
Maximum value of SAR (measured) = 20.4 W/kg

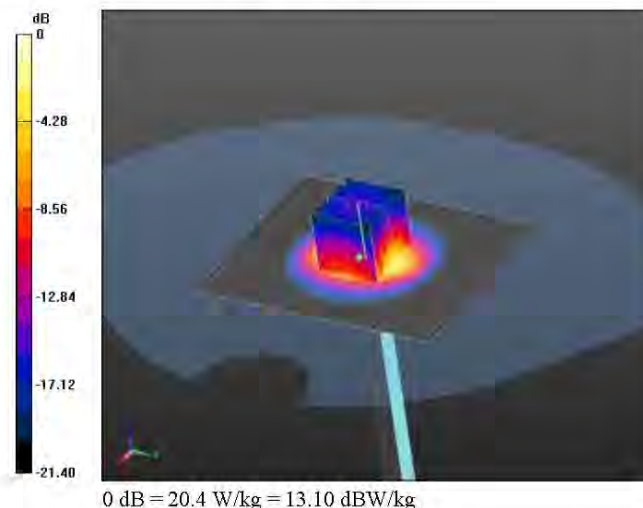

## 17. Test Results

### Body\_2 437MHz\_Front\_Gap0mm

DUT: M1; Type: Mobile Photo Printer; Serial: N/A  
Procedure Name: 802.11b\_ch6\_f2 437\_Body Front\_Gap 0 mm


Communication System: UID 0, 2.4G WLAN (0); Frequency: 2437 MHz; Duty Cycle: 1:1  
Medium parameters used:  $f = 2437$  MHz;  $\sigma = 1.959$  S/m;  $\epsilon_r = 51.071$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY5 Configuration:

- Probe: EX3DV4 - SN3928; ConvF(6.84, 6.84, 6.84); Calibrated: 2014-01-15;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1342; Calibrated: 2014-07-24
- Phantom: SAM twin 1728; Type: QD000P40CD; Serial: TP:1728
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

M1/802.11b\_ch6\_f2 437\_Body Front\_Gap 0 mm/Area Scan (101x171x1): Interpolated  
grid: dx=1.200 mm, dy=1.200 mm  
Maximum value of SAR (interpolated) = 0.154 W/kg

M1/802.11b\_ch6\_f2 437\_Body Front\_Gap 0 mm/Zoom Scan (7x7x7)/Cube 0:  
Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 5.700 V/m; Power Drift = 0.18 dB  
Peak SAR (extrapolated) = 0.235 W/kg  
SAR(1 g) = 0.111 W/kg; SAR(10 g) = 0.056 W/kg  
Maximum value of SAR (measured) = 0.177 W/kg

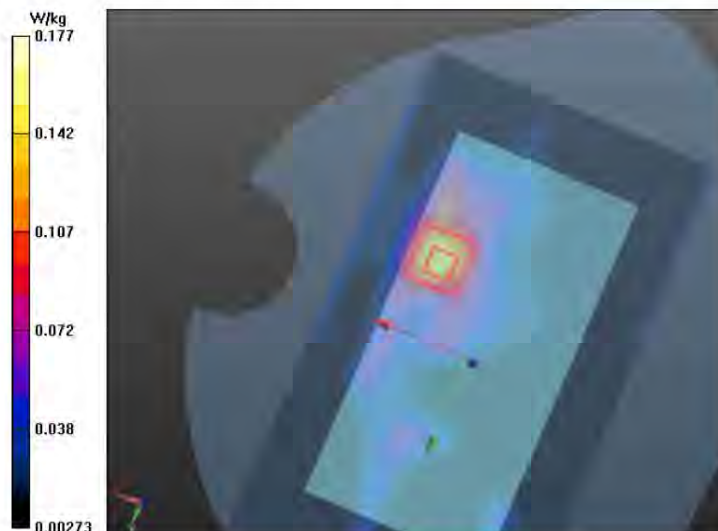

## Body\_2 437MHz\_Back\_Gap0mm

DUT: M1; Type: Mobile Photo Printer; Serial: N/A  
Procedure Name: 802.11b\_ch6\_f2 437\_Body Back\_Gap 0 mm


Communication System: UID 0, 2.4GWLAN (0); Frequency: 2437 MHz; Duty Cycle: 1:1  
Medium parameters used:  $f = 2437$  MHz;  $\sigma = 1.959$  S/m;  $\epsilon_r = 51.071$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY5 Configuration:

- Probe: EX3DV4 - SN3928; ConvF(6.84, 6.84, 6.84); Calibrated: 2014-01-15;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1342; Calibrated: 2014-07-24
- Phantom: SAM twin 1728; Type: QD000P40CD; Serial: TP:1728
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

M1/802.11b\_ch6\_f2 437\_Body Back\_Gap 0 mm/Area Scan (101x171x1): Interpolated  
grid: dx=1.200 mm, dy=1.200 mm  
Maximum value of SAR (interpolated) = 0.726 W/kg

M1/802.11b\_ch6\_f2 437\_Body Back\_Gap 0 mm/Zoom Scan (7x7x7)/Cube 0:  
Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 6.715 V/m; Power Drift = 0.13 dB  
Peak SAR (extrapolated) = 1.17 W/kg  
SAR(1 g) = 0.558 W/kg; SAR(10 g) = 0.281 W/kg  
Maximum value of SAR (measured) = 0.842 W/kg

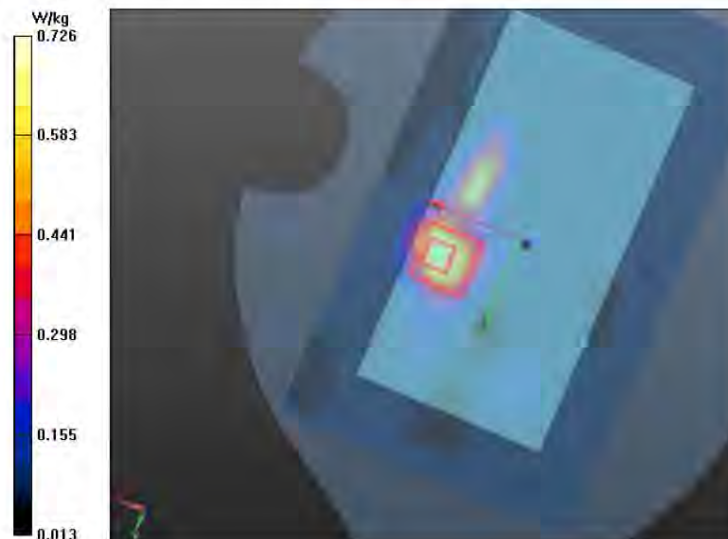

## Body\_2 437MHz\_Top\_Gap0mm

DUT: M1; Type: Mobile Photo Printer; Serial: N/A  
Procedure Name: 802.11b\_ch6\_f2 437\_Body Top\_Gap 0 mm


Communication System: UID 0, 2.4G WLAN (0); Frequency: 2437 MHz; Duty Cycle: 1:1  
Medium parameters used:  $f = 2437$  MHz;  $\sigma = 1.959$  S/m;  $\epsilon_r = 51.071$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY5 Configuration:

- Probe: EX3DV4 - SN3928; ConvF(6.84, 6.84, 6.84); Calibrated: 2014-01-15;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1342; Calibrated: 2014-07-24
- Phantom: SAM twin 1728; Type: QD000P40CD; Serial: TP:1728
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

M1/802.11b\_ch6\_f2 437\_Body Top\_Gap 0 mm/Area Scan (51x91x1): Interpolated grid:  
dx=1.200 mm, dy=1.200 mm  
Maximum value of SAR (interpolated) = 0.0949 W/kg

M1/802.11b\_ch6\_f2 437\_Body Top\_Gap 0 mm/Zoom Scan (7x7x7)/Cube 0:  
Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 4.900 V/m; Power Drift = 0.07 dB  
Peak SAR (extrapolated) = 0.125 W/kg  
SAR(1 g) = 0.063 W/kg; SAR(10 g) = 0.031 W/kg  
Maximum value of SAR (measured) = 0.0934 W/kg

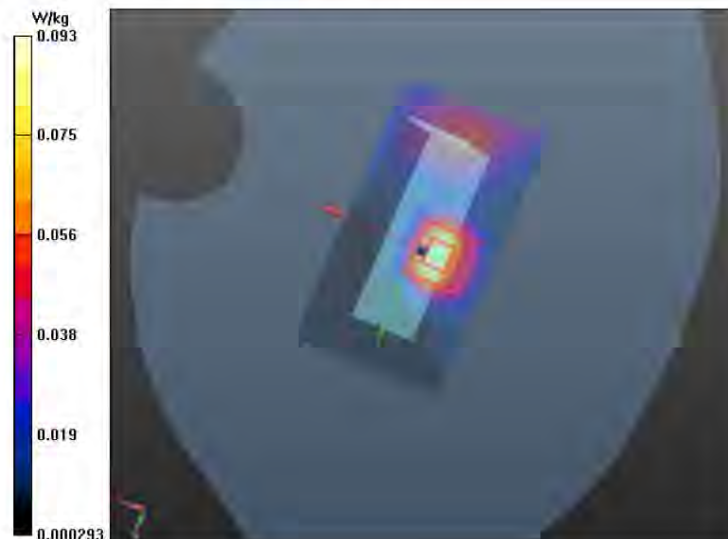

## Body\_2 437MHz\_Left\_Gap0mm

DUT: M1; Type: Mobile Photo Printer; Serial: N/A  
Procedure Name: 802.11b\_ch6\_f2 437\_Body Left\_Gap 0 mm


Communication System: UID 0, 2.4G WLAN (0); Frequency: 2437 MHz; Duty Cycle: 1:1  
Medium parameters used:  $f = 2437$  MHz;  $\sigma = 1.959$  S/m;  $\epsilon_r = 51.071$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY5 Configuration:

- Probe: EX3DV4 - SN3928; ConvF(6.84, 6.84, 6.84); Calibrated: 2014-01-15;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1342; Calibrated: 2014-07-24
- Phantom: SAM twin 1728; Type: QD000P40CD; Serial: TP:1728
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

M1/802.11b\_ch6\_f2 437\_Body Left\_Gap 0 mm/Area Scan (61x131x1): Interpolated grid:  
dx=1.200 mm, dy=1.200 mm  
Maximum value of SAR (interpolated) = 0.820 W/kg

M1/802.11b\_ch6\_f2 437\_Body Left\_Gap 0 mm/Zoom Scan (7x7x7)/Cube 0:  
Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 3.867 V/m; Power Drift = 0.08 dB  
Peak SAR (extrapolated) = 1.58 W/kg  
SAR(1 g) = 0.603 W/kg; SAR(10 g) = 0.281 W/kg  
Maximum value of SAR (measured) = 1.07 W/kg

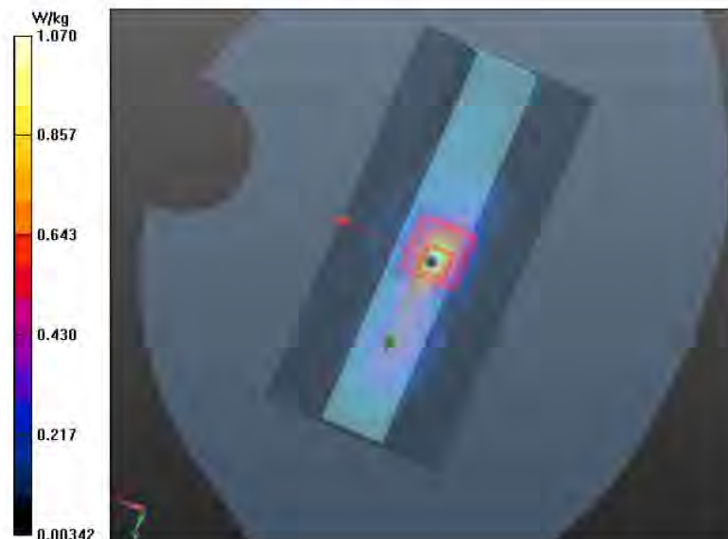



## Body\_2 437MHz\_Right\_Gap0mm

DUT: M1; Type: Mobile Photo Printer; Serial: N/A  
Procedure Name: 802.11b\_ch6\_f2 437\_Body Right\_Gap 0 mm


Communication System: UID 0, 2.4G WLAN (0); Frequency: 2437 MHz; Duty Cycle: 1:1  
Medium parameters used:  $f = 2437$  MHz;  $\sigma = 1.959$  S/m;  $\epsilon_r = 51.071$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY5 Configuration:

- Probe: EX3DV4 - SN3928; ConvF(6.84, 6.84, 6.84); Calibrated: 2014-01-15;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1342; Calibrated: 2014-07-24
- Phantom: SAM twin 1728; Type: QD000P40CD; Serial: TP:1728
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

M1/802.11b\_ch6\_f2 437\_Body Right\_Gap 0 mm/Area Scan (71x131x1): Interpolated grid:  
dx=1.200 mm, dy=1.200 mm  
Maximum value of SAR (interpolated) = 0.0436 W/kg

M1/802.11b\_ch6\_f2 437\_Body Right\_Gap 0 mm/Zoom Scan (7x7x7)/Cube 0:  
Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 3.602 V/m; Power Drift = -0.12 dB  
Peak SAR (extrapolated) = 0.0470 W/kg  
SAR(1 g) = 0.015 W/kg; SAR(10 g) = 0.00771 W/kg  
Maximum value of SAR (measured) = 0.0266 W/kg

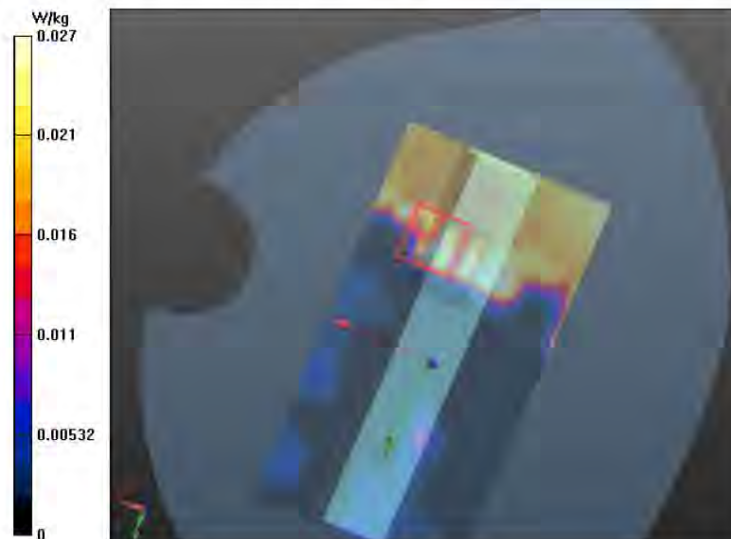

## Body\_2 437MHz\_Bottom\_Gap0mm

DUT: M1; Type: Mobile Photo Printer; Serial: N/A  
Procedure Name: 802.11b\_ch6\_f2 437\_Body Bottom\_Gap 0 mm

Communication System: UID 0, 2.4G WLAN (0); Frequency: 2437 MHz; Duty Cycle: 1:1  
Medium parameters used:  $f = 2437$  MHz;  $\sigma = 1.959$  S/m;  $\epsilon_r = 51.071$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY5 Configuration:

- Probe: EX3DV4 - SN3928; ConvF(6.84, 6.84, 6.84); Calibrated: 2014-01-15;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1342; Calibrated: 2014-07-24
- Phantom: SAM twin 1728; Type: QD000P40CD; Serial: TP:1728
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

M1/802.11b\_ch6\_f2 437\_Body Bottom\_Gap 0 mm/Area Scan (51x91x1): Interpolated  
grid: dx=1.200 mm, dy=1.200 mm  
Maximum value of SAR (interpolated) = 0.0573 W/kg

M1/802.11b\_ch6\_f2 437\_Body Bottom\_Gap 0 mm/Zoom Scan (7x7x7)/Cube 0:  
Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 4.146 V/m; Power Drift = 0.03 dB  
Peak SAR (extrapolated) = 0.0600 W/kg  
SAR(1 g) = 0.029 W/kg; SAR(10 g) = 0.015 W/kg  
Maximum value of SAR (measured) = 0.0429 W/kg



## Body\_2 412MHz\_Left\_Gap0mm

DUT: M1; Type: Mobile Photo Printer; Serial: N/A  
Procedure Name: 802.11b\_ch1\_f2 412\_Body Left\_Gap 0 mm


Communication System: UID 0, 2.4G WLAN (0); Frequency: 2412 MHz; Duty Cycle: 1:1  
Medium parameters used:  $f = 2412$  MHz;  $\sigma = 1.926$  S/m;  $\epsilon_r = 51.176$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY5 Configuration:

- Probe: EX3DV4 - SN3928; ConvF(6.84, 6.84, 6.84); Calibrated: 2014-01-15;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1342; Calibrated: 2014-07-24
- Phantom: SAM twin 1728; Type: QD000P40CD; Serial: TP:1728
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

M1/802.11b\_ch1\_f2 412\_Body Left\_Gap 0 mm/Area Scan (61x131x1): Interpolated grid:  
dx=1.200 mm, dy=1.200 mm  
Maximum value of SAR (interpolated) = 0.870 W/kg

M1/802.11b\_ch1\_f2 412\_Body Left\_Gap 0 mm/Zoom Scan (7x7x7)/Cube 0:  
Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 7.607 V/m; Power Drift = -0.02 dB  
Peak SAR (extrapolated) = 1.56 W/kg  
SAR(1 g) = 0.603 W/kg; SAR(10 g) = 0.276 W/kg  
Maximum value of SAR (measured) = 1.08 W/kg

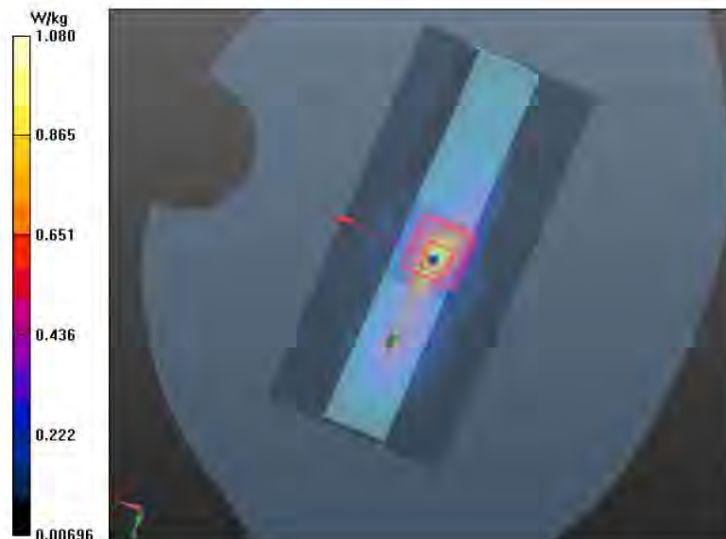

## Body\_2 462MHz\_Left\_Gap0mm

DUT: M1; Type: Mobile Photo Printer; Serial: N/A  
Procedure Name: 802.11b\_ch11\_f2 462\_Body Left\_Gap 0 mm


Communication System: UID 0, 2.4G WLAN (0); Frequency: 2462 MHz; Duty Cycle: 1:1  
Medium parameters used:  $f = 2462$  MHz;  $\sigma = 1.982$  S/m;  $\epsilon_r = 50.96$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY5 Configuration:

- Probe: EX3DV4 - SN3928; ConvF(6.84, 6.84, 6.84); Calibrated: 2014-01-15;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1342; Calibrated: 2014-07-24
- Phantom: SAM twin 1728; Type: QD000P40CD; Serial: TP:1728
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

M1/802.11b\_ch11\_f2 462\_Body Left\_Gap 0 mm/Area Scan (61x131x1): Interpolated grid:  
dx=1.200 mm, dy=1.200 mm  
Maximum value of SAR (interpolated) = 1.01 W/kg

M1/802.11b\_ch11\_f2 462\_Body Left\_Gap 0 mm/Zoom Scan (7x7x7)/Cube 0:  
Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 9.665 V/m; Power Drift = 0.04 dB  
Peak SAR (extrapolated) = 1.45 W/kg  
SAR(1 g) = 0.658 W/kg; SAR(10 g) = 0.318 W/kg  
Maximum value of SAR (measured) = 0.958 W/kg

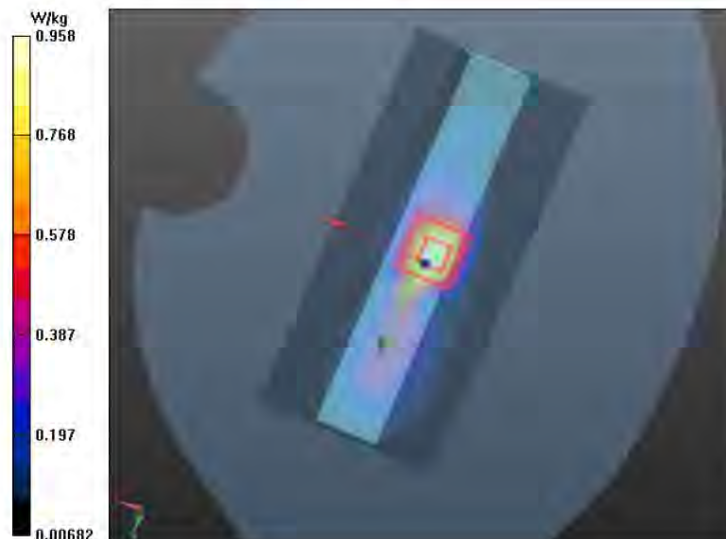

## Annex A. Photographs

### Annex A.1 EUT



**Front View**



**Back View**



**Right side View**



**Left side View**




**Top side View**



**Bottom side View**

## Annex A.2 Photographs of Test Setup

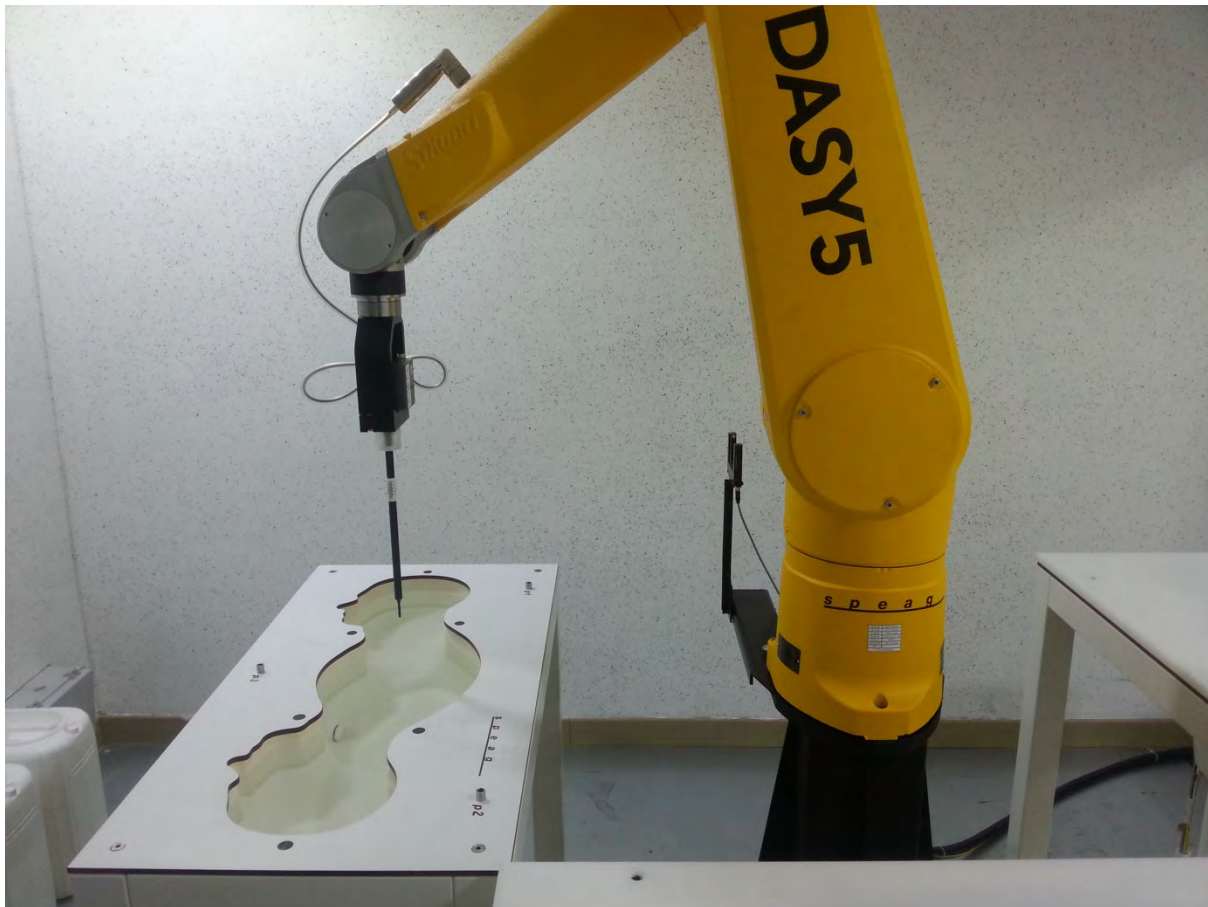

**Photograph of the SAR measurement System**




**Annex A.3 Test Position**



**(a) Body\_Front**



**(b) Body\_Back**

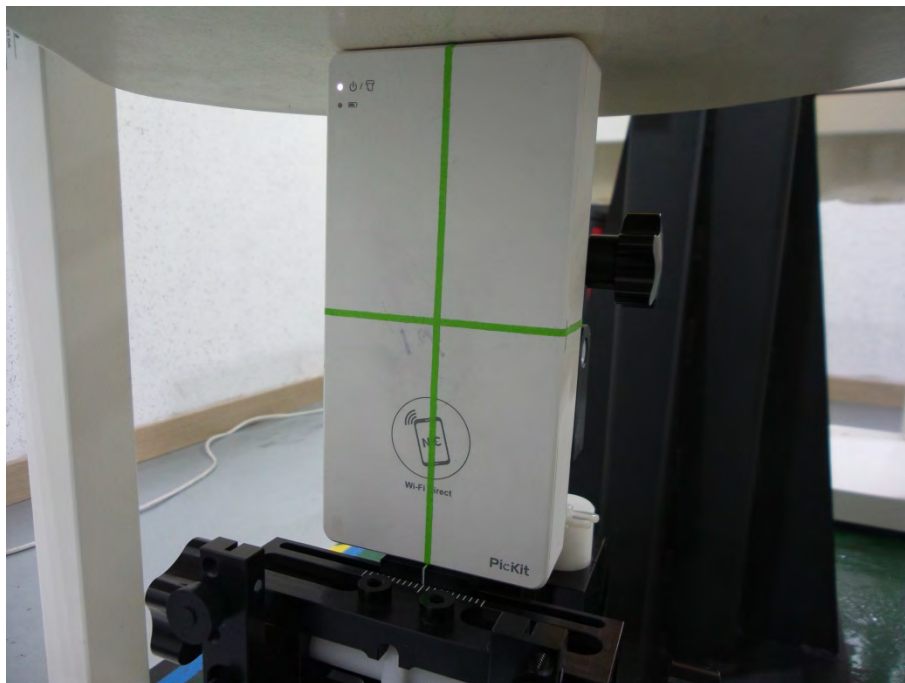

(c) Body\_Top




(d) Body\_Left



(e) Body\_Right




(f) Body\_Bottom

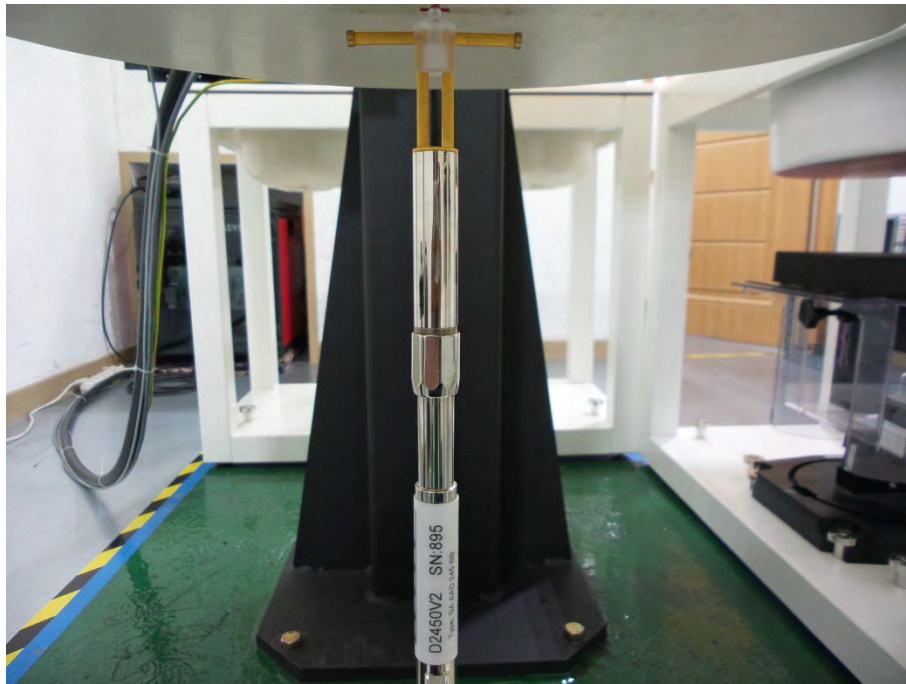

**(g) Body Validation 2 450 MHz**

#### **Annex A.4 Liquid Depth**

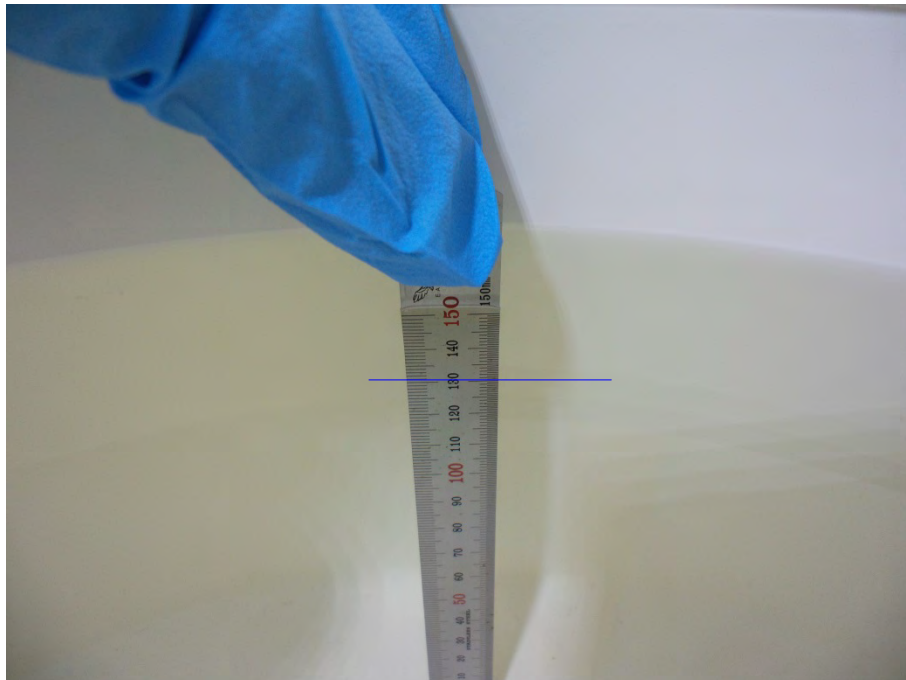

**Body 2 450 MHz**

## Annex B. Calibration certificate

### Annex B.1 Probe Calibration certificate

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **EMC Compliance (Dymstec)**

Certificate No: **EX3-3928\_Jan14**

#### CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3928**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,  
QA CAL-25.v6  
Calibration procedure for dosimetric E-field probes**

Calibration date: **January 15, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID              | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Power sensor E4412A        | MY41498087      | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 04-Apr-13 (No. 217-01737)         | Apr-14                 |
| Reference 20 dB Attenuator | SN: S5277 (20x) | 04-Apr-13 (No. 217-01735)         | Apr-14                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 04-Apr-13 (No. 217-01738)         | Apr-14                 |
| Reference Probe ES3DV2     | SN: 3013        | 30-Dec-13 (No. ES3-3013_Dec13)    | Dec-14                 |
| DAE4                       | SN: 660         | 13-Dec-13 (No. DAE4-660_Dec13)    | Dec-14                 |
| Secondary Standards        | ID              | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Apr-13)  | In house check: Apr-16 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-13) | In house check: Oct-14 |

|                | Name           | Function              | Signature |
|----------------|----------------|-----------------------|-----------|
| Calibrated by: | Jeton Kastrati | Laboratory Technician |           |
| Approved by:   | Katja Pokovic  | Technical Manager     |           |

Issued: January 15, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

| 결 | 작성 | 검토 | 승인 |
|---|----|----|----|
| 재 | X  |    |    |

**Calibration Laboratory of**  
**Schmid & Partner**  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

**Glossary:**

|                        |   |
|------------------------|---|
| TSL                    | tissue simulating liquid  |
| NORM <sub>x,y,z</sub>  | sensitivity in free space   |
| ConvF                  | sensitivity in TSL / NORM <sub>x,y,z</sub>  |
| DCP                    | diode compression point   |
| CF                     | crest factor (1/duty_cycle) of the RF signal  |
| A, B, C, D             | modulation dependent linearization parameters   |
| Polarization $\varphi$ | $\varphi$ rotation around probe axis  |
| Polarization $\theta$  | $\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\theta = 0$ is normal to probe axis |
| Connector Angle        | information used in DASY system to align probe sensor X to the robot coordinate system  |

**Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

**Methods Applied and Interpretation of Parameters:**

- NORM<sub>x,y,z</sub>:** Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>:** DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR:** PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>:** A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle:** The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

EX3DV4 – SN:3928

January 15, 2014

# Probe EX3DV4

## SN:3928

Manufactured: March 8, 2013  
Calibrated: January 15, 2014

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

EX3DV4- SN:3928

January 15, 2014

### DASY/EASY - Parameters of Probe: EX3DV4 - SN:3928

#### Basic Calibration Parameters

|  | Sensor X | Sensor Y | Sensor Z | Unc (k=2)     |
|--|----------|----------|----------|---------------|
| Norm ( $\mu\text{V}/(\text{V/m})^2$ ) <sup>A</sup> | 0.50     | 0.23     | 0.56     | $\pm 10.1 \%$ |
| DCP (mV) <sup>B</sup>                              | 97.4     | 89.0     | 98.9     |               |

#### Modulation Calibration Parameters

| UID | Communication System Name |   | A<br>dB | B<br>dB $\sqrt{\mu\text{V}}$ | C   | D<br>dB | VR<br>mV | Unc <sup>C</sup><br>(k=2) |
|-----|---------------------------|---|---------|------------------------------|-----|---------|----------|---------------------------|
| 0   | CW                        | X | 0.0     | 0.0                          | 1.0 | 0.00    | 167.7    | $\pm 2.5 \%$              |
|     |                           | Y | 0.0     | 0.0                          | 1.0 |         | 181.5    |                           |
|     |                           | Z | 0.0     | 0.0                          | 1.0 |         | 168.9    |                           |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter; uncertainty not required.

<sup>C</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



EX3DV4- SN:3928

January 15, 2014

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3928

### Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth (mm) <sup>G</sup> | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 450                  | 43.5                               | 0.87                            | 10.24   | 10.24   | 10.24   | 0.14               | 1.58                    | ± 13.4 %    |
| 850                  | 41.5                               | 0.92                            | 9.41    | 9.41    | 9.41    | 0.76               | 0.59                    | ± 12.0 %    |
| 900                  | 41.5                               | 0.97                            | 9.33    | 9.33    | 9.33    | 0.42               | 0.83                    | ± 12.0 %    |
| 1750                 | 40.1                               | 1.37                            | 7.88    | 7.88    | 7.88    | 0.62               | 0.66                    | ± 12.0 %    |
| 1900                 | 40.0                               | 1.40                            | 7.62    | 7.62    | 7.62    | 0.33               | 0.92                    | ± 12.0 %    |
| 2450                 | 39.2                               | 1.80                            | 6.91    | 6.91    | 6.91    | 0.35               | 0.87                    | ± 12.0 %    |
| 2600                 | 39.0                               | 1.96                            | 6.73    | 6.73    | 6.73    | 0.46               | 0.71                    | ± 12.0 %    |
| 5200                 | 36.0                               | 4.66                            | 5.09    | 5.09    | 5.09    | 0.30               | 1.80                    | ± 13.1 %    |
| 5300                 | 35.9                               | 4.76                            | 4.80    | 4.80    | 4.80    | 0.35               | 1.80                    | ± 13.1 %    |
| 5500                 | 35.6                               | 4.96                            | 4.83    | 4.83    | 4.83    | 0.35               | 1.80                    | ± 13.1 %    |
| 5600                 | 35.5                               | 5.07                            | 4.46    | 4.46    | 4.46    | 0.45               | 1.80                    | ± 13.1 %    |
| 5800                 | 35.3                               | 5.27                            | 4.76    | 4.76    | 4.76    | 0.35               | 1.80                    | ± 13.1 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3928

January 15, 2014

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3928

### Calibration Parameter Determined in Body Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>E</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth (mm) <sup>G</sup> | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 450                  | 56.7                               | 0.94                            | 10.53   | 10.53   | 10.53   | 0.06               | 1.20                    | ± 13.4 %    |
| 850                  | 55.2                               | 0.99                            | 9.33    | 9.33    | 9.33    | 0.80               | 0.64                    | ± 12.0 %    |
| 900                  | 55.0                               | 1.05                            | 9.21    | 9.21    | 9.21    | 0.52               | 0.77                    | ± 12.0 %    |
| 1750                 | 53.4                               | 1.49                            | 7.65    | 7.65    | 7.65    | 0.38               | 0.88                    | ± 12.0 %    |
| 1900                 | 53.3                               | 1.52                            | 7.31    | 7.31    | 7.31    | 0.31               | 0.98                    | ± 12.0 %    |
| 2450                 | 52.7                               | 1.95                            | 6.84    | 6.84    | 6.84    | 0.77               | 0.55                    | ± 12.0 %    |
| 2600                 | 52.5                               | 2.16                            | 6.61    | 6.61    | 6.61    | 0.80               | 0.50                    | ± 12.0 %    |
| 5200                 | 49.0                               | 5.30                            | 4.39    | 4.39    | 4.39    | 0.40               | 1.90                    | ± 13.1 %    |
| 5300                 | 48.9                               | 5.42                            | 4.21    | 4.21    | 4.21    | 0.40               | 1.90                    | ± 13.1 %    |
| 5500                 | 48.6                               | 5.65                            | 3.96    | 3.96    | 3.96    | 0.45               | 1.90                    | ± 13.1 %    |
| 5600                 | 48.5                               | 5.77                            | 4.07    | 4.07    | 4.07    | 0.30               | 1.90                    | ± 13.1 %    |
| 5800                 | 48.2                               | 6.00                            | 4.10    | 4.10    | 4.10    | 0.45               | 1.90                    | ± 13.1 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


<sup>E</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3928

January 15, 2014

### Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)


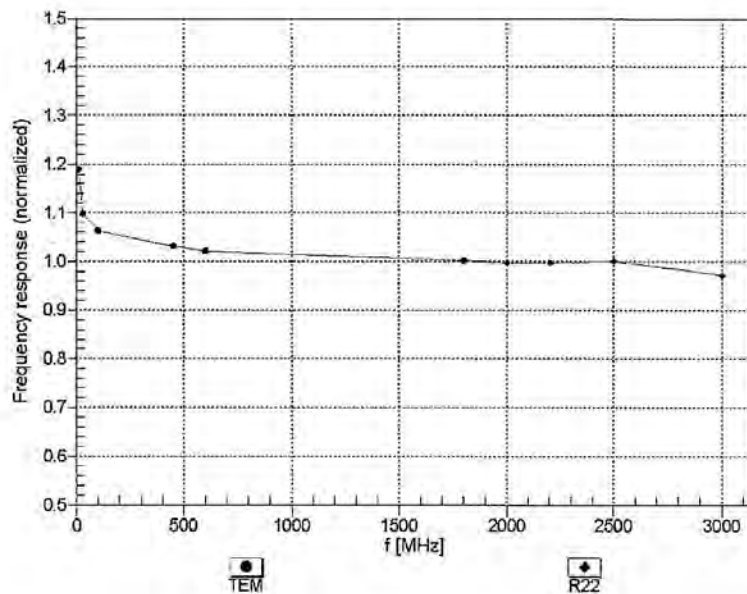


Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

EX3DV4- SN:3928

January 15, 2014

**Receiving Pattern ( $\phi$ ),  $\theta = 0^\circ$**

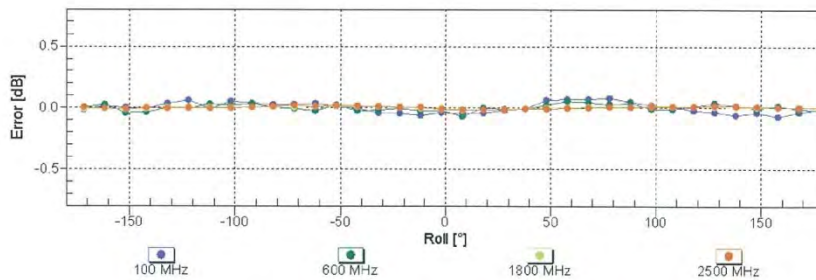
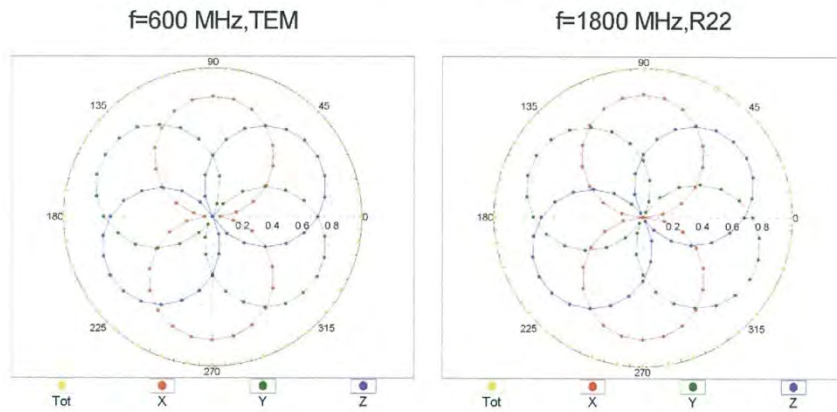


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

EX3DV4- SN:3928

January 15, 2014

**Dynamic Range f(SAR<sub>head</sub>)**  
 (TEM cell , f = 900 MHz)

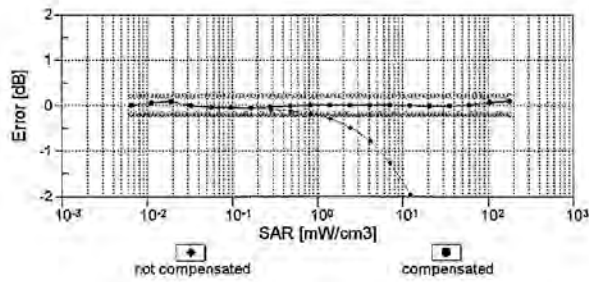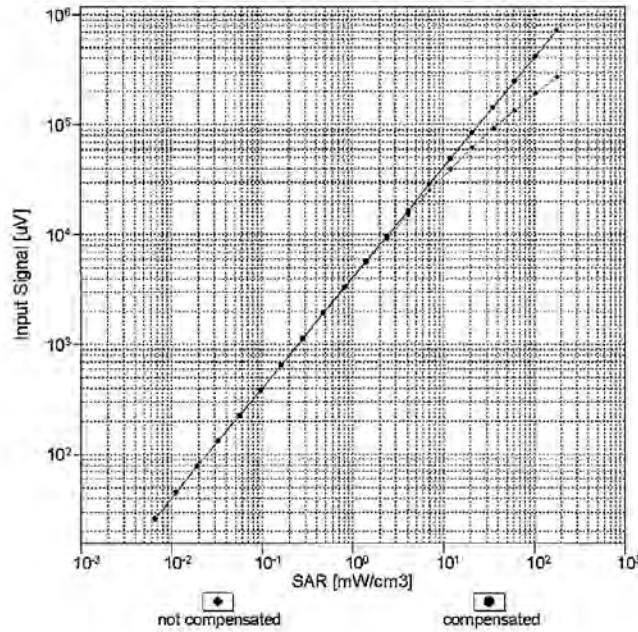


Uncertainty of Linearity Assessment:  $\pm 0.6\%$  (k=2)

EX3DV4- SN:3928


January 15, 2014

### Conversion Factor Assessment

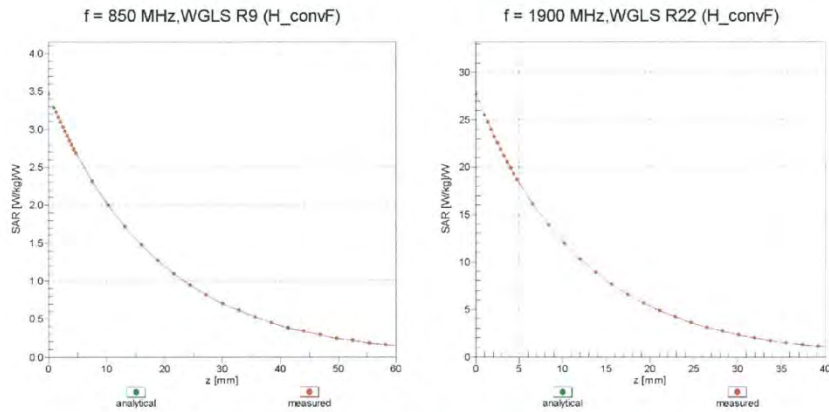

### Deviation from Isotropy in Liquid

Error ( $\phi, \theta$ ), f = 900 MHz

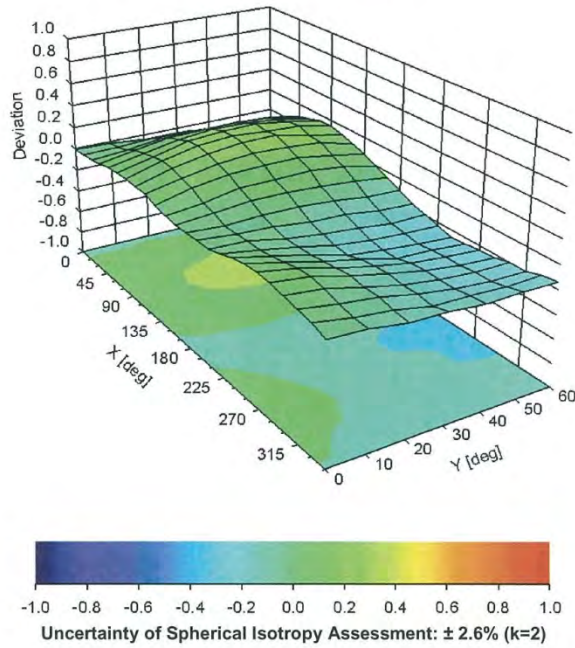

EX3DV4- SN:3928

January 15, 2014

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3928

### Other Probe Parameters

|   |            |
|---|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle (°)                           | -112       |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disabled   |
| Probe Overall Length                          | 337 mm     |
| Probe Body Diameter                           | 10 mm      |
| Tip Length                                    | 9 mm       |
| Tip Diameter                                  | 2.5 mm     |
| Probe Tip to Sensor X Calibration Point       | 1 mm       |
| Probe Tip to Sensor Y Calibration Point       | 1 mm       |
| Probe Tip to Sensor Z Calibration Point       | 1 mm       |
| Recommended Measurement Distance from Surface | 2 mm       |

**Annex B.2 DAE Calibration certification**

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client **EMC Compliance (Dymstec)**

Certificate No: DAE4-1342\_Jul14

| CALIBRATION CERTIFICATE  |   |                            |                        |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
|--|---|----------------------------|------------------------|----------------------------|-----------------------|-------------------------------|-------------|----------------------|--------------------------|---------------------|------|-----------------------|-----------------|---------------------------|--------------------|----------------------------|------------------------|---------------------|--------------------|----------------------------|------------------------|
| Object   | DAE4 - SD 000 D04 BM - SN: 1342   |                            |                        |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Calibration procedure(s)   | QA CAL-06.v26<br>Calibration procedure for the data acquisition electronics (DAE)   |                            |                        |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Calibration date:  | July 24, 2014   |                            |                        |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| <table border="1"> <tr> <td>결</td> <td>작</td> <td>성</td> <td>검</td> <td>토</td> <td>승</td> <td>인</td> </tr> <tr> <td>재</td> <td>X</td> <td></td> <td>NA</td> <td></td> <td></td> <td>4/16</td> </tr> </table>   |   | 결                          | 작                      | 성                          | 검                     | 토                             | 승           | 인                    | 재                        | X                   |      | NA                    |                 |                           | 4/16               |                            |                        |                     |                    |                            |                        |
| 결  | 작   | 성                          | 검                      | 토                          | 승                     | 인                             |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| 재  | X   |                            | NA                     |                            |                       | 4/16                          |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).<br/>The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Keithley Multimeter Type 2001</td> <td>SN: 0810278</td> <td>01-Oct-13 (No:13976)</td> <td>Oct-14</td> </tr> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> <tr> <td>Auto DAE Calibration Unit</td> <td>SE UWS 053 AA 1001</td> <td>07-Jan-14 (in house check)</td> <td>In house check: Jan-15</td> </tr> <tr> <td>Calibrator Box V2.1</td> <td>SE UMS 006 AA 1002</td> <td>07-Jan-14 (in house check)</td> <td>In house check: Jan-15</td> </tr> </tbody> </table> |   | Primary Standards          | ID #                   | Cal Date (Certificate No.) | Scheduled Calibration | Keithley Multimeter Type 2001 | SN: 0810278 | 01-Oct-13 (No:13976) | Oct-14                   | Secondary Standards | ID # | Check Date (in house) | Scheduled Check | Auto DAE Calibration Unit | SE UWS 053 AA 1001 | 07-Jan-14 (in house check) | In house check: Jan-15 | Calibrator Box V2.1 | SE UMS 006 AA 1002 | 07-Jan-14 (in house check) | In house check: Jan-15 |
| Primary Standards  | ID #  | Cal Date (Certificate No.) | Scheduled Calibration  |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Keithley Multimeter Type 2001  | SN: 0810278   | 01-Oct-13 (No:13976)       | Oct-14                 |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Secondary Standards  | ID #  | Check Date (in house)      | Scheduled Check        |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Auto DAE Calibration Unit  | SE UWS 053 AA 1001  | 07-Jan-14 (in house check) | In house check: Jan-15 |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Calibrator Box V2.1  | SE UMS 006 AA 1002  | 07-Jan-14 (in house check) | In house check: Jan-15 |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Calibrated by:   | <table border="1"> <tr> <th>Name</th> <th>Function</th> <th>Signature</th> </tr> <tr> <td>Eric Hainfeld</td> <td>Technician</td> <td></td> </tr> <tr> <td>Fin Bomholt</td> <td>Deputy Technical Manager</td> <td></td> </tr> </table> | Name                       | Function               | Signature                  | Eric Hainfeld         | Technician                    |             | Fin Bomholt          | Deputy Technical Manager |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Name   | Function  | Signature                  |                        |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Eric Hainfeld  | Technician  |                            |                        |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Fin Bomholt  | Deputy Technical Manager  |                            |                        |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Approved by:   |   |                            |                        |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| <p>Issued: July 24, 2014</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p>  |   |                            |                        |                            |                       |                               |             |                      |                          |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |



**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**S** Service suisse d'étalonnage  
**C** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

### Glossary

**DAE** data acquisition electronics  
**Connector angle** information used in DASY system to align probe sensor X to the robot coordinate system.

### Methods Applied and Interpretation of Parameters

- **DC Voltage Measurement:** Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- **Connector angle:** The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - **DC Voltage Measurement Linearity:** Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - **Common mode sensitivity:** Influence of a positive or negative common mode voltage on the differential measurement.
  - **Channel separation:** Influence of a voltage on the neighbor channels not subject to an input voltage.
  - **AD Converter Values with inputs shorted:** Values on the internal AD converter corresponding to zero input voltage
  - **Input Offset Measurement:** Output voltage and statistical results over a large number of zero voltage measurements.
  - **Input Offset Current:** Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - **Input resistance:** Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - **Low Battery Alarm Voltage:** Typical value for information. Below this voltage, a battery alarm signal is generated.
  - **Power consumption:** Typical value for information. Supply currents in various operating modes.

**DC Voltage Measurement**

A/D - Converter Resolution nominal  
 High Range: 1LSB = 6.1 $\mu$ V , full range = -100...+300 mV  
 Low Range: 1LSB = 61nV , full range = -1.....+3mV  
 DASYS measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | X                         | Y                         | Z                         |
|---------------------|---------------------------|---------------------------|---------------------------|
| High Range          | 404.079 $\pm$ 0.02% (k=2) | 404.229 $\pm$ 0.02% (k=2) | 404.193 $\pm$ 0.02% (k=2) |
| Low Range           | 3.97194 $\pm$ 1.50% (k=2) | 3.97818 $\pm$ 1.50% (k=2) | 3.97832 $\pm$ 1.50% (k=2) |

**Connector Angle**

|  |                                    |
|--|------------------------------------|
| Connector Angle to be used in DASYS system | 36.5 $^{\circ}$ $\pm$ 1 $^{\circ}$ |
|--|------------------------------------|

**Appendix (Additional assessments outside the scope of SCS108)**

**1. DC Voltage Linearity**

| High Range        | Reading ( $\mu$ V) | Difference ( $\mu$ V) | Error (%) |
|-------------------|--------------------|-----------------------|-----------|
| Channel X + Input | 199994.48          | -2.71                 | -0.00     |
| Channel X + Input | 20003.12           | 2.03                  | 0.01      |
| Channel X - Input | -19998.22          | 2.56                  | -0.01     |
| Channel Y + Input | 199994.97          | -2.37                 | -0.00     |
| Channel Y + Input | 20000.20           | -0.94                 | -0.00     |
| Channel Y - Input | -20001.55          | -0.79                 | 0.00      |
| Channel Z + Input | 199993.69          | -3.29                 | -0.00     |
| Channel Z + Input | 20000.13           | -0.86                 | -0.00     |
| Channel Z - Input | -20001.35          | -0.58                 | 0.00      |

| Low Range         | Reading ( $\mu$ V) | Difference ( $\mu$ V) | Error (%) |
|-------------------|--------------------|-----------------------|-----------|
| Channel X + Input | 2000.66            | -0.29                 | -0.01     |
| Channel X + Input | 201.58             | 0.18                  | 0.09      |
| Channel X - Input | -198.71            | -0.04                 | 0.02      |
| Channel Y + Input | 2001.16            | 0.25                  | 0.01      |
| Channel Y + Input | 201.20             | -0.03                 | -0.02     |
| Channel Y - Input | -199.87            | -1.04                 | 0.53      |
| Channel Z + Input | 2001.06            | 0.27                  | 0.01      |
| Channel Z + Input | 200.54             | -0.49                 | -0.24     |
| Channel Z - Input | -200.16            | -1.24                 | 0.62      |

**2. Common mode sensitivity**

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Common mode Input Voltage (mV) | High Range Average Reading ( $\mu$ V) | Low Range Average Reading ( $\mu$ V) |
|-----------|--------------------------------|---------------------------------------|--------------------------------------|
| Channel X | 200                            | 11.07                                 | 9.27                                 |
|           | -200                           | -8.95                                 | -10.56                               |
| Channel Y | 200                            | 0.81                                  | 0.58                                 |
|           | -200                           | -2.58                                 | -2.76                                |
| Channel Z | 200                            | 1.15                                  | 0.69                                 |
|           | -200                           | -2.73                                 | -3.02                                |

**3. Channel separation**

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Input Voltage (mV) | Channel X ( $\mu$ V) | Channel Y ( $\mu$ V) | Channel Z ( $\mu$ V) |
|-----------|--------------------|----------------------|----------------------|----------------------|
| Channel X | 200                | -                    | 4.50                 | -2.81                |
| Channel Y | 200                | 9.68                 | -                    | 6.17                 |
| Channel Z | 200                | 10.07                | 7.09                 | -                    |

**4. AD-Converter Values with inputs shorted**

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 15949            | 15477           |
| Channel Y | 16473            | 14871           |
| Channel Z | 15667            | 14031           |

**5. Input Offset Measurement**

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ

|           | Average (μV) | min. Offset (μV) | max. Offset (μV) | Std. Deviation (μV) |
|-----------|--------------|------------------|------------------|---------------------|
| Channel X | 0.59         | -0.36            | 1.97             | 0.56                |
| Channel Y | -0.70        | -1.87            | 0.51             | 0.54                |
| Channel Z | -0.60        | -1.90            | 0.78             | 0.60                |

**6. Input Offset Current**

Nominal Input circuitry offset current on all channels: <25fA

**7. Input Resistance** (Typical values for information)

|           | Zeroing (kOhm) | Measuring (MOhm) |
|-----------|----------------|------------------|
| Channel X | 200            | 200              |
| Channel Y | 200            | 200              |
| Channel Z | 200            | 200              |

**8. Low Battery Alarm Voltage** (Typical values for information)

| Typical values | Alarm Level (VDC) |
|----------------|-------------------|
| Supply (+ Vcc) | +7.9              |
| Supply (- Vcc) | -7.6              |

**9. Power Consumption** (Typical values for information)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.01             | +6            | +14               |
| Supply (- Vcc) | -0.01             | -8            | -9                |

**Annex B.3 Dipole Calibration certification**  
**D2450V2**

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **EMC Compliance (Dymstec)**

Certificate No: **D2450V2-895\_Jul14**

| CALIBRATION CERTIFICATE   |  |                                   |                        |   |   |   |   |   |   |   |   |
|---|--|-----------------------------------|------------------------|---|---|---|---|---|---|---|---|
| Object  | D2450V2 - SN: 895  |                                   |                        |   |   |   |   |   |   |   |   |
| Calibration procedure(s)  | QA CAL-05.v9<br>Calibration procedure for dipole validation kits above 700 MHz |                                   |                        |   |   |   |   |   |   |   |   |
| Calibration date:   | July 24, 2014  |                                   |                        |   |   |   |   |   |   |   |   |
| <table border="1"> <tr> <td>결</td> <td>작</td> <td>검</td> <td>승</td> </tr> <tr> <td>재</td> <td>X</td> <td>토</td> <td>인</td> </tr> </table>   |  |                                   |                        | 결 | 작 | 검 | 승 | 재 | X | 토 | 인 |
| 결   | 작  | 검                                 | 승                      |   |   |   |   |   |   |   |   |
| 재   | X  | 토                                 | 인                      |   |   |   |   |   |   |   |   |
| This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).<br>The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. |  |                                   |                        |   |   |   |   |   |   |   |   |
| All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.  |  |                                   |                        |   |   |   |   |   |   |   |   |
| Calibration Equipment used (M&TE critical for calibration)  |  |                                   |                        |   |   |   |   |   |   |   |   |
| Primary Standards   | ID #   | Cal Date (Certificate No.)        | Scheduled Calibration  |   |   |   |   |   |   |   |   |
| Power meter EPM-442A  | GB37480704   | 09-Oct-13 (No. 217-01827)         | Oct-14                 |   |   |   |   |   |   |   |   |
| Power sensor HP 8481A   | US37292783   | 09-Oct-13 (No. 217-01827)         | Oct-14                 |   |   |   |   |   |   |   |   |
| Power sensor HP 8481A   | MY41092317   | 09-Oct-13 (No. 217-01828)         | Oct-14                 |   |   |   |   |   |   |   |   |
| Reference 20 dB Attenuator  | SN: 5058 (20k)   | 03-Apr-14 (No. 217-01918)         | Apr-15                 |   |   |   |   |   |   |   |   |
| Type-N mismatch combination   | SN: 5047.2 / 06327   | 03-Apr-14 (No. 217-01921)         | Apr-15                 |   |   |   |   |   |   |   |   |
| Reference Probe ES3DV3  | SN: 3205   | 30-Dec-13 (No. ES3-3205_Dec13)    | Dec-14                 |   |   |   |   |   |   |   |   |
| DAE4  | SN: 601  | 30-Apr-14 (No. DAE4-601_Apr14)    | Apr-15                 |   |   |   |   |   |   |   |   |
| Secondary Standards   | ID #   | Check Date (in house)             | Scheduled Check        |   |   |   |   |   |   |   |   |
| RF generator R&S SMT-06   | 100005   | 04-Aug-99 (in house check Oct-13) | In house check: Oct-16 |   |   |   |   |   |   |   |   |
| Network Analyzer HP 8753E   | US37390585 S4206   | 18-Oct-01 (in house check Oct-13) | In house check: Oct-14 |   |   |   |   |   |   |   |   |
| Calibrated by:  | Name<br>Claudio Leubler  | Function<br>Laboratory Technician | Signature<br>          |   |   |   |   |   |   |   |   |
| Approved by:  | Name<br>Katja Pokovic  | Function<br>Technical Manager     | Signature<br>          |   |   |   |   |   |   |   |   |
|   |  |                                   | Issued: July 24, 2014  |   |   |   |   |   |   |   |   |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory.   |  |                                   |                        |   |   |   |   |   |   |   |   |

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- d) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY5                  | V52.8.8     |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 10 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 2450 MHz ± 1 MHz       |             |

**Head TSL parameters**

The following parameters and calculations were applied.

|   | Temperature     | Permittivity | Conductivity     |
|---|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 39.2         | 1.80 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 37.8 ± 6 %   | 1.85 mho/m ± 6 % |
| Head TSL temperature change during test | < 0.5 °C        | ---          | ---              |

**SAR result with Head TSL**

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
|---|--------------------|--------------------------|
| SAR measured  | 250 mW input power | 13.4 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 52.5 W/kg ± 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                          |
|---|--------------------|--------------------------|
| SAR measured  | 250 mW input power | 6.20 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 24.5 W/kg ± 16.5 % (k=2) |

**Body TSL parameters**

The following parameters and calculations were applied.

|   | Temperature     | Permittivity | Conductivity     |
|---|-----------------|--------------|------------------|
| Nominal Body TSL parameters             | 22.0 °C         | 52.7         | 1.95 mho/m       |
| Measured Body TSL parameters            | (22.0 ± 0.2) °C | 50.6 ± 6 %   | 2.03 mho/m ± 6 % |
| Body TSL temperature change during test | < 0.5 °C        | ---          | ---              |

**SAR result with Body TSL**

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                          |
|---|--------------------|--------------------------|
| SAR measured  | 250 mW input power | 13.1 W/kg                |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 50.9 W/kg ± 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                          |
|---|--------------------|--------------------------|
| SAR measured  | 250 mW input power | 6.01 W/kg                |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 23.6 W/kg ± 16.5 % (k=2) |

**Appendix (Additional assessments outside the scope of SCS108)**

**Antenna Parameters with Head TSL**

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 53.0 $\Omega$ + 1.6 j $\Omega$ |
| Return Loss                          | - 29.5 dB                      |

**Antenna Parameters with Body TSL**

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 50.6 $\Omega$ + 3.7 j $\Omega$ |
| Return Loss                          | - 28.7 dB                      |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.157 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |               |
|-----------------|---------------|
| Manufactured by | SPEAG         |
| Manufactured on | June 19, 2012 |



**DASY5 Validation Report for Head TSL**

Date: 24.07.2014

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 895**

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.85$  S/m;  $\epsilon_r = 37.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 102.2 V/m; Power Drift = 0.08 dB


Peak SAR (extrapolated) = 27.9 W/kg

**SAR(1 g) = 13.4 W/kg; SAR(10 g) = 6.2 W/kg**

Maximum value of SAR (measured) = 17.9 W/kg

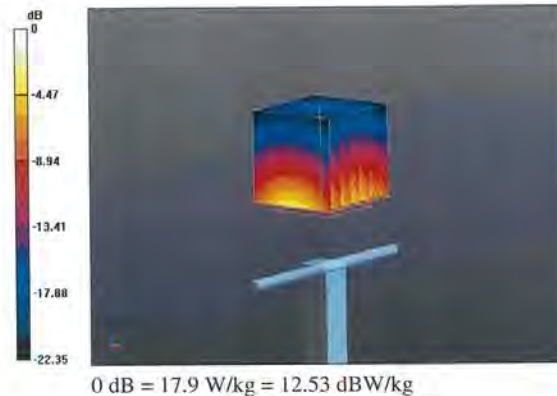

Impedance Measurement Plot for Head TSL

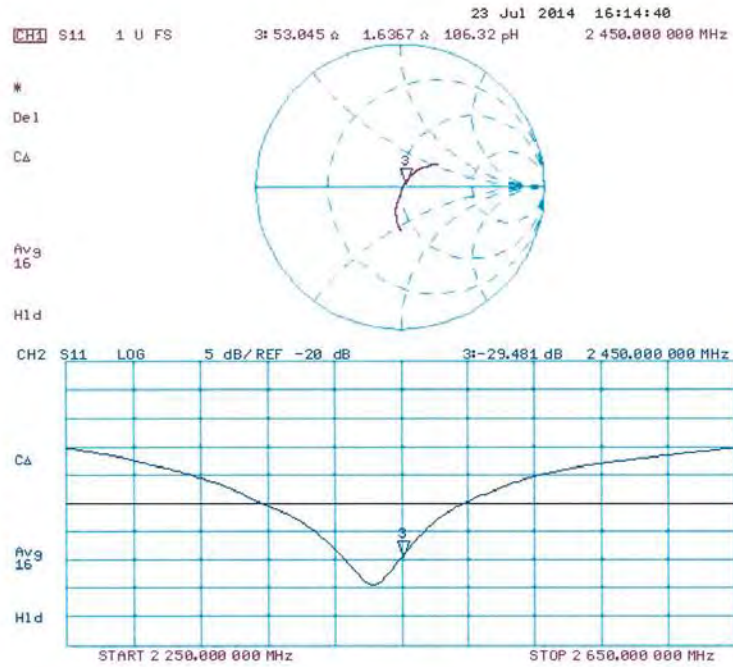

## DASY5 Validation Report for Body TSL

Date: 16.07.2014

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 895**

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 2.03$  S/m;  $\epsilon_r = 50.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.35, 4.35, 4.35); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.39 V/m; Power Drift = -0.00 dB


Peak SAR (extrapolated) = 27.6 W/kg

**SAR(1 g) = 13.1 W/kg; SAR(10 g) = 6.01 W/kg**

Maximum value of SAR (measured) = 17.3 W/kg

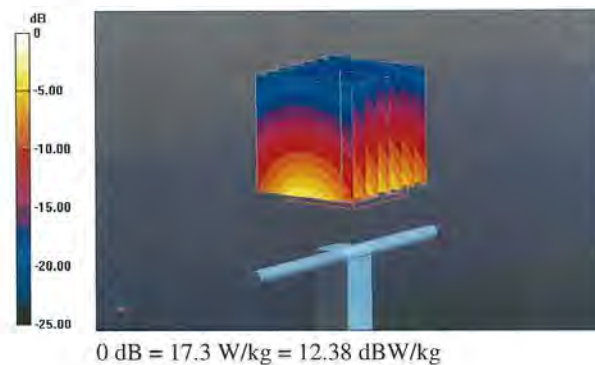

**Impedance Measurement Plot for Body TSL**

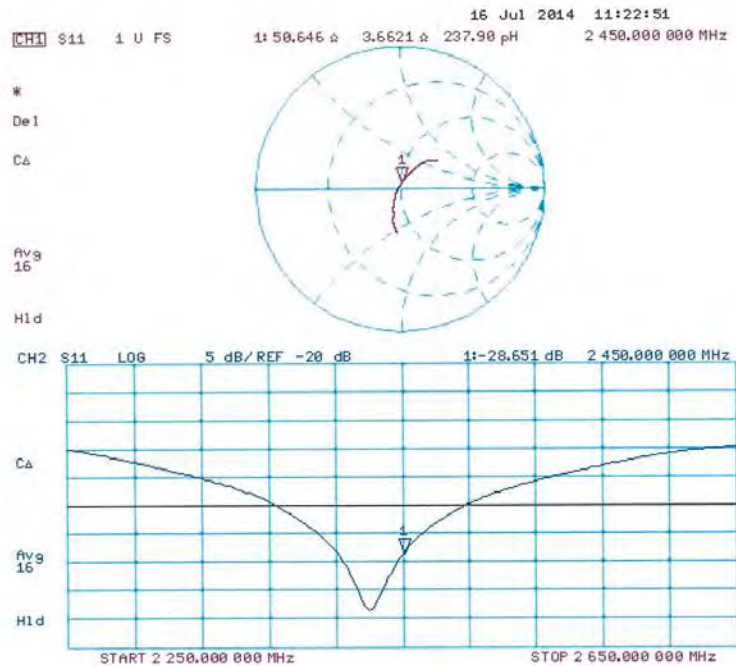

**-END OF REPORT -**