

Test Laboratory: UL CCS SAR Lab B

SystemPerformanceCheck-D2450V2 SN 706

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 2450$ MHz; $\sigma = 1.99$ mho/m; $\epsilon_r = 51.49$; $\rho = 1000$ kg/m³
 Phantom section: Flat Section


Room Ambient Temperature: 24.0 deg. C; Liquid Temperature: 23.0 deg. C

DASY5 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Probe: EX3DV4 - SN3773; ConvF(6.87, 6.87, 6.87); Calibrated: 5/3/2011
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1258; Calibrated: 5/2/2011
- Phantom: ELI v5.0 (B); Type: QDOVA001BB; Serial: 1118
- Measurement SW: DASY52, Version 52.6 (2);SEMCAD X Version 14.4.5 (3634)

Body/Pin=100 mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm
 Maximum value of SAR (measured) = 5.219 mW/g

Body/Pin=100 mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 64.584 V/m; Power Drift = 0.0065 dB
 Peak SAR (extrapolated) = 11.266 W/kg
SAR(1 g) = 5.43 mW/g; SAR(10 g) = 2.51 mW/g
 Maximum value of SAR (measured) = 7.729 mW/g

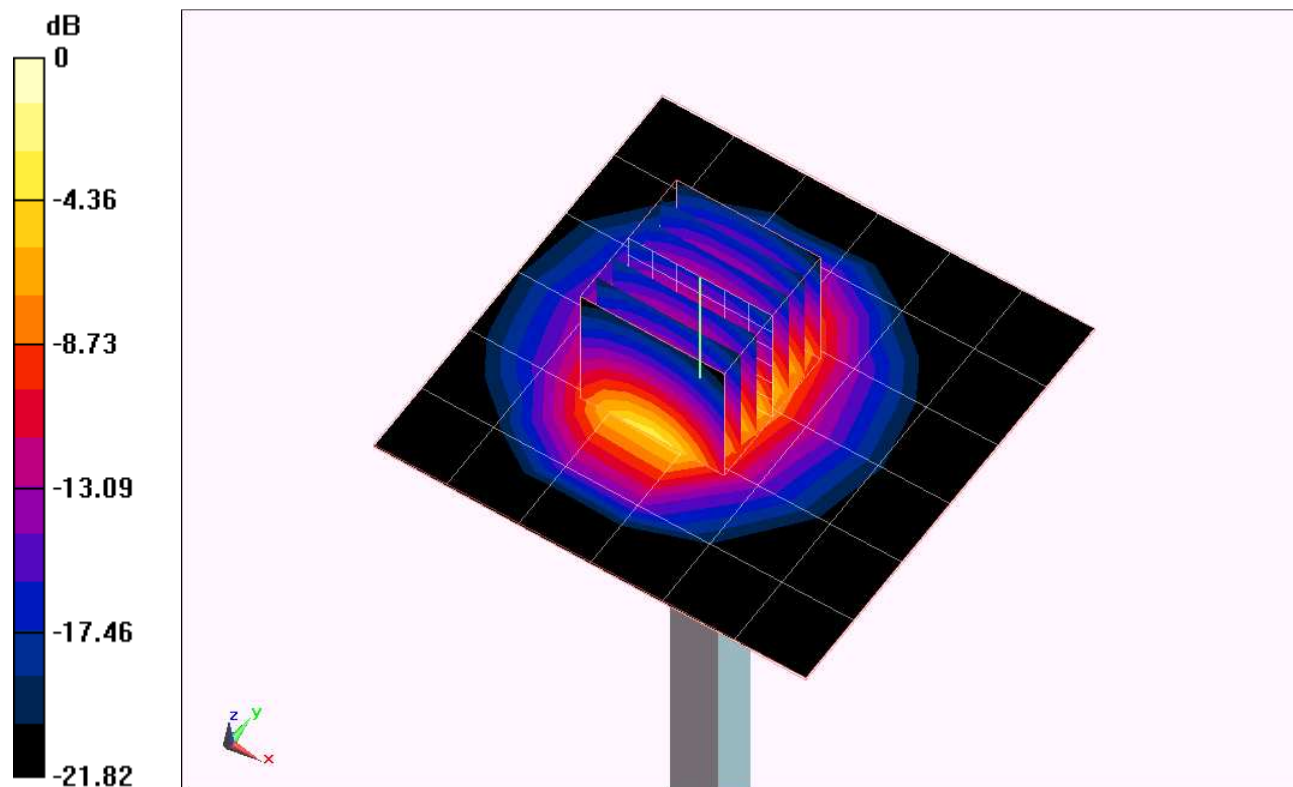

0 dB = 7.730mW/g

Test Laboratory: UL CCS SAR Lab B

SystemPerformanceCheck-D2450V2 SN 706

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Body/Pin=100 mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm
Maximum value of SAR (measured) = 4.162 mW/g

