

Date of Issue : 2013-08-06 Page : 1/52

SAR TEST REPORT

Equipment Under Test : QCMD335 (Tested inside of Samsung Notebook PC NP270E5G)

Model No. : QCMD335

Applicant : Qualcomm Atheros, Inc.

Manufacturer Samsung Electronics. Co., Ltd

Address of Manufacturer : 129, Samsung-Ro, Yeongtong-Gu, Suwon-Si, Gyeonggi-Do, KR

FCC ID : PPD-QCMD335 IC ID 4104A-OCMD335

Device Category : Portable Device

Exposure Category : General Population/Uncontrolled Exposure

Date of Receipt : 2013-06-13 Date of Test(s) : 2013-06-13 Date of Issue : 2013-08-06

Standards:

FCC OET Bulletin 65 supplement C IEEE 1528, 2003 ANSI/IEEE C95.1, C95.3

In the configuration tested, the EUT complied with the standards specified above.

Remarks:

This report details the results of the testing carried out on one sample, the results contained in this test report do not relate to other samples of the same product. The manufacturer should ensure that all products in series production are in conformity with the product sample detailed in this report.

This report may only be reproduced and distributed in full. If the product in this report is used in any configuration other than that detailed in the report, the manufacturer must ensure the new system complies with all relevant standards. Any mention of SGS Korea Co., Ltd. or testing done by SGS Korea Co., Ltd. in connection with distribution or use of the product described in this report must be approved by SGS Korea Co., Ltd. in writing.

Tested by : Minhyuk Han 2013-08-06

Approved by : Nicky You 2013-08-06



Date of Issue : 2013-08-06 Page : 2/52

Contents

1. General Information 1.1 Testing Laboratory.... 3 1.2 Details of Applicant..... 3 1.3 Version of Report. 3 1.4 Description of EUT(s)..... 1.5 Nominal and Maximum Output Power Specifications.... 1.6 Test Environment. 1.7 Operation description. Evaluation procedures. 1.8 4 5 1.9 SAR Measurement Procedures The SAR Measurement System. 1.10 6 1.11 System Components. 8 9 1.12 SAR System Verification. 1.13 Tissue Simulant Fluid for the Frequency Band. 11 Test System Validation..... 12 1.14 Test Standards and Limits.... 1.15 12 2. Instruments List..... 14 3. Summary of Results.... 15 FCC Power Measurement Procedures..... 3.1 15 3.2 Measured and Reported SAR.... 15 RF Conducted Power.... 3.3 15 SAR Test Configuration. 3.4 16 3.5 SAR Test Exclusions Applied.... 17 3.6 SAR Data Summary..... 18 3.7.1 Introduction.... 19 Simultaneous Transmission Procedures.... 19 3.7.2

The Simultaneous Transmission possibilities are listed as below.....

3.7.4 Body SAR Simultaneous Transmission Analysis.....

APPENDIX

3.7.3

- A. DASY4 SAR Report
- B. Uncertainty Analysis
- C. Calibration certificate

19

19



Date of Issue : 2013-08-06 Page : 3 / 52

1. General Information

1.1 Testing Laboratory

SGS Korea Co., Ltd. (Gunpo Laboratory)

18-34, Sanbon-dong, Gunpo-si, Gyeonggi-do, 435-040, Korea

Telephone : +82 +31 428 5700 FAX : +82 +31 427 2371

Homepage : All SGS services are rendered in accordance with the applicable SGS

conditions of service available on request and accessible at

http://www.sgs.com/en/Terms-and-Conditions.aspx

1.2 Details of Manufacturer

Manufacturer : Samsung Electronics Co., Ltd.

Address : 129, Samsung-Ro, Yeongtong-Gu, Suwon-Si, Gyeonggi-Do, KR

Email : johnlee@samsung.com
Phone No. : 82-31-277-4784

1.3 Version of Report

Date	Revision
2013-06-28	Initial issue
2013-07-04	Revision 01
2013-07-09	Revision 02
2013-07-11	Revision 03
2013-07-25	Revision 04
2013-08-06	Revision 05
	2013-06-28 2013-07-04 2013-07-09 2013-07-11 2013-07-25

1.4 Description of EUT(s)

. ,					
ype	: QCMD335 (Tested inside o	f Samsung Notebook PC NP270E5G)			
el	: QCMD335				
mber	: JGNR19ED600178N				
eration	: WLAN, Bluetooth				
ycle	: 1(WLAN)				
ccessory	: None				
D	: 2412 MHz ~ 2462 MHz (WLAN_11b/g/n)				
ey Kange	2402 MHz ~ 2480 MHz (Bluetooth)				
Гуре	: 11.1 V d.c. (Lithum-ion Bat	tery)			
	The highest reported SA	AR values			
	ъ .	Reported SAR			
	Band	1g Body-Worn (W/kg)			
2.45 GHz WLAN		0.360			
Bluetooth		N/A			
us SAR per KI	DB 690783 D01v01r02	0.402			
	mber peration yycle accessory ry Range	: QCMD335 : JGNR19ED600178N : JGNR19ED600178N : WLAN, Bluetooth : 1(WLAN) : None : 2412 MHz ~ 2462 MHz (WLAZ 2402 MHz ~ 2480 MHz (Bluez 11.1 V d.c. (Lithum-ion Bath			



Date of Issue : 2013-08-06 Page : 4 / 52

1.5 Maximum Output Power Specifications

This device operates using the following maximum output power specifications. SAR values were scaled to the maximum allowed power to determine compliance per KDB Publication 44798 D01v05.

	Average power for Production (dB m)									
Band	Frequency	Chain1(Main)								
(MHz)	(MHz)	11b	11g	HT20	HT40					
	2412	18.5	14.5	13.5						
	2437	18.5	18.5	17.5	16.5					
2450	2462	17.5	14.5	13.5						
	2422				12.5					
	2452				12.5					

Average power for Production (dBm)							
Mode	GFSK	PI/4DQPSK	8DPSK	LE			
Bluetooth	-4.0	-4.0	-4.0	1.0			

1.6 Test Environment

Ambient temperature	: (22 ± 2) ° C
Tissue Simulating Liquid	: (22 ± 2) ° C
Relative Humidity	$: (55 \pm 5) \% \text{ R.H.}$

1.7 Operation Configuration

The client provided a special driver and test program which can control the frequency and power of the WLAN module. The EUT was set to maximum power level during all tests and at the beginning of each test the battery was fully charged.

The DASY4 system measures power drift during SAR testing by comparing e-field in the same location at the beginning and at the end of measurement. Based on the RF Power and antenna separation distance, stand-alone BT SAR and simultaneous SAR evaluation are not required.

1.8 EVALUATION PROCEDURES

- Power Reference Measurement Procedures

The Power Reference Measurement and Power Drift Measurements are for monitoring the power drift of the device under test in the batch process. The Minimum distance of probe sensors to surface determines the closest measurement point to phantom surface. The minimum distance of probe sensors to surface is 2 mm. This distance cannot be smaller than the Distance of sensor calibration points to probe tip as defined in the probe properties (for example, 2.5 mm for an EX3DV4 probe type).



Date of Issue : 2013-08-06 Page : 5 / 52

1.9 SAR Measurement Procedures

Step 1: Power Reference Measurement

The Power Reference Measurement and Power Drift Measurements are for monitoring the power drift of the device under test in the batch process. The Minimum distance of probe sensors to surface determines the closest measurement point to phantom surface. The minimum distance of probe sensors to surface is 2 mm. This distance cannot be smaller than the Distance of sensor calibration points to probe tip as defined in the probe properties.

Step 2 and 3: Area Scan & Zoom Scan Procedures

The entire evaluation of the spatial peak values is performed within the Post-processing engine (SEMCAD). The system always gives the maximum values for the 1 g and 10 g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- 1. The extraction of the measured data (grid and values) from the Zoom Scan.
- 2. The calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- 3. The generation of a high-resolution mesh within the measured volume
- 4. The interpolation of all measured values from the measurement grid to the high-resolution grid
- 5. The extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- 6. The calculation of the averaged SAR within masses of 1 g and 10 g.



Date of Issue : 2013-08-06 Page : 6 / 52

< Area and Zoom Scan Resolutions per FCC KDB Publication 865664 D01v01 >

		≤3 GHz	> 3 GHz	
		5 ± 1 mm	½·δ·ln(2) ± 0.5 mm	
		30° ± 1° 20° ± 1°		
		\leq 2 GHz: \leq 15 mm 2 – 3 GHz: \leq 12 mm	3 – 4 GHz: ≤ 12 mm 4 – 6 GHz: ≤ 10 mm	
atial resol	ution: Δx_{Area} , Δy_{Area}	When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the above the measurement resolution must be ≤ the corresponding x or y dimension of the test device with at least one measurement point on the test device.		
patial reso	olution: Δx _{Zoom} , Δy _{Zoom}	≤2 GHz: ≤8 mm 2 – 3 GHz: ≤5 mm*	3 – 4 GHz: ≤ 5 mm* 4 – 6 GHz: ≤ 4 mm*	
uniform	grid: Δz _{Zeom} (n)	≤ 5 mm	3 – 4 GHz: ≤4 mm 4 – 5 GHz: ≤3 mm 5 – 6 GHz: ≤2 mm	
graded	Δz _{Zcom} (1): between 1 st two points closest to phantom surface	≤ 4 mm	3 – 4 GHz: ≤3 mm 4 – 5 GHz: ≤2.5 mm 5 – 6 GHz: ≤2 mm	
grid $\Delta z_{Z_{com}}(n>1)$: between subsequent points		≤ 1.5·∆z _{Zeem} (n-1)		
x, y, z		≥ 30 mm	3 – 4 GHz: ≥ 28 mm 4 – 5 GHz: ≥ 25 mm 5 – 6 GHz: ≥ 22 mm	
	spatial resolution uniform graded grid	graded grid Description Description	m closest measurement point obe sensors) to phantom surface from probe axis to phantom neasurement location $ \begin{array}{c} 5 \pm 1 \text{ mm} \\ 30^{\circ} \pm 1^{\circ} \\ & \leq 2 \text{ GHz:} \leq 15 \text{ mm} \\ 2 - 3 \text{ GHz:} \leq 12 \text{ mm} \end{array} $ when the x or y dimension of measurement plane orientative measurement plane orientative measurement point on the test of measurement point on the test	

Note: δ is the penetration depth of a plane-wave at normal incidence to the tissue medium; see draft standard IEEE P1528-2011 for details.

Step 4: Power drift measurement

The Power Drift Measurement measures the field at the same location as the most recent power reference measurement within the same procedure, and with the same settings. The Power Drift Measurement gives the field difference in dB from the reading conducted within the last Power Reference Measurement. This allows a user to monitor the power drift of the device under test within a batch process. The measurement procedure is the same as Step 1.

1.10 The SAR Measurement System

A photograph of the SAR measurement System is given in Fig. a. This SAR Measurement System uses a Computer-controlled 3-D stepper motor system (Speag DASY 4 professional system). A Model EX3DV4 3862 and 3791 E-field probe is used to determine the internal electric fields. The SAR can be obtained from the equation SAR= σ (|Ei|2)/ ρ where σ and ρ are the conductivity and mass density of the tissue-simulant. The DASY4 system for performing compliance tests consists of the following items:

- •A standard high precision 6-axis robot (Staubli RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- •A dosimeter probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating

^{*} When zoom scan is required and the <u>reported SAR</u> from the area scan based 1-g SAR estimation procedures of KDB 447498 is ≤ 1.4 W/kg, ≤ 8 mm, ≤ 7 mm and ≤ 5 mm zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.



Date of Issue : 2013-08-06 Page : 7/52

liquid. The probe is equipped with an optical surface detector system.

•A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.

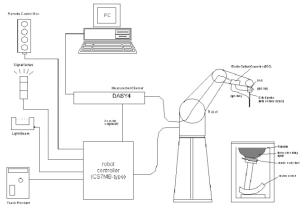


Fig a. The microwave circuit arrangement used for SAR system verification

- The Electro-optical converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection. The EOC is connected to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- A computer operating Windows XP.
- DASY4 software: V4.7 Build80.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM phantom enabling testing body usage.
- The device holder for flat phantom.
- Tissue simulating liquid mixed according to the given recipes.
- Validation dipole kits allowing to validate the proper functioning of the system.



Date of Issue : 2013-08-06 Page : 8 / 52

1.11 System Components

EX3DV4 E-Field Probe

Construction: Symmetrical design with triangular core.

Built-in shielding against static charges.

PEEK enclosure material (resistant to organic solvents, e.g.,

DGBE)

Calibration : Basic Broad Band Calibration in air Conversion Factors (CF)

for HSL 835 and HSL1900.

Additional CF-Calibration for other liquids and frequencies

upon request.

Frequency : 10 MHz to 6 GHz; Linearity: \pm 0.2 dB (30 MHz to 6 GHz)

Directivity : ± 0.3 dB in HSL (rotation around probe axis)

 ± 0.5 dB in tissue material (rotation normal to probe axis)

Dynamic : $10 \mu \text{W/g to} > 100 \text{ m W/g};$

Tip diameter: 2.5 mm (Body diameter: 12 mm)

Distance from probe tip to dipole centers: 1 mm

Application : High precision dosimetric measurements in any exposure

precision of better 30%

Construction Symmetrical design with triangular core.

Built-in shielding against static charges.

PEEK enclosure material (resistant to organic solvents, e.g.,

DGBE)



EX3DV4 E-Field Probe

NOTE:

1. The Probe parameters have been calibrated by the SPEAG. Please reference "APPENDIX C" for the Calibration Certification Report.



Date of Issue : 2013-08-06 Page : 9 / 52

ELI Phantom

Construction:

Phantom for compliance testing of handheld and body-mounted wireless devices in the frequency range of 30 Mbz to 6 Gbz. ELI is fully compatible with the IEC 62209-2 standard and all known tissue simulating liquids. ELI has been optimized regarding its performance and can be integrated into our standard phantom tables. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurement grids, by teaching three points. The phantom is compatible with all SPEAG dosimetric probes and dipoles.

ELI V5.0 has the same shell geometry and is manufactured from the same material as ELI4, but has reinforced top structure



ELI Phantom

Shell Thickness: $2.0 \text{ mm} \pm 0.2 \text{ mm}$

Dimensions Major axis: 600 mm

Minor axis: 400 mm

DEVICE HOLDER

Construction

Simple but effective and easy-to-use extension for Mounting Device that facilitates the testing of larger devices according to IEC 62209-2 (a.q.. laptops, Cameras, etc.). It is lightweight and fits easily on the upper part of the Mounting Device in place of the phone positioned.



Device Holder

1.12 SAR System verification

The microwave circuit arrangement for system verification is sketched in Fig. b. The daily system accuracy verification occurs within the flat section of the SAM phantom. A SAR measurement was performed to see if the measured SAR was within \pm 10 % from the target SAR values. These tests were done at 2450 Mb. The tests for EUT were conducted within 24 hours after each verification. The obtained results from the system accuracy verification are displayed in the table 1. During the tests, the ambient temperature of the laboratory was in the range (22 \pm 2) ° C, the relative humidity was in the range (55 \pm 5) % R.H. and the liquid depth above the ear reference points was above 15 cm in all the cases. It is seen that the system is operating within its specification, as the results are within acceptable tolerance of the reference values.



Date of Issue : 2013-08-06 Page : 10 / 52




Fig b. The microwave circuit arrangement used for SAR system verification

- A. Agilent Model E4438C Signal Generator
- B. EMPOWER Model 2001-BBS3Q7ECK Amplifier
- C. EMPOWER Model 2092-BBS5K9CAJ Amplifier
- D. Agilent Model E4419B Power Meter
- E. Agilent Model 9300H Power Sensor
- F. Agilent Model 86205A Directional RF Bridges
- G. Reference dipole Antenna



Photo of the dipole Antenna

System Verification Results

Verification Kit	Probe S/N	Tissue	Target SAR 1 g from Calibration Certificate (1 W)	Measured SAR 1 g (0.1 W)	Normalized SAR 1 g (1 W)	Deviation (%)	Date	Liquid Temp. (°C)
D2450V2 S/N: 892	3862	2450 MHz Body	52.1 W/kg	5.01 W/kg	50.1 W/kg	- 3.84	06-13-2013	22.0

Table 1. Results system verification



Date of Issue : 2013-08-06 Page : 11 / 52

1.13 Tissue Simulant Fluid for the Frequency Band

The dielectric properties for this simulant fluid were measured by using the Speag Model DAK-3.5 Dielectric Probe in conjunction with Agilent E5071C Network Analyzer(300 $\,\mathrm{kHz}$ - 6 $\,\mathrm{GHz}$) by using a procedure detailed in Section V.

	Tissue		Dielectric Parameters					
f (MHz)	type	Limits / Measured	Permittivity	Conductivity	Simulated Tissue Temp(°C)			
		Measured, 06-13-2013	52.0	2.01	22.0			
2450		Recommended Limits	52.7	1.95	21.0 ~ 23.0			
		Deviation(%)	-1.33	3.08	-			
2412	Body	Measured, 06-13-2013	52.2	1.96	22.0			
2412		Deviation(%)	-0.95	0.51	-			
2462		Measured, 06-13-2013	52.0	2.02	22.0			
2462	-	Deviation(%)	<u>-1.33</u>	3.59	-			

The composition of the brain & muscle tissue simulating liquid

The following tissue formulations are provided for reference only as some of the parameters have not been thoroughly verified. The composition of ingredients may be modified accordingly to achieve the desired target tissue parameters required for routine SAR evaluation.

Ingredients	Frequency (Mz)										
(% by weight)	45	50	83	35	91	15	1900		2450		
Tissue Type	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body	
Water	38.56	51.16	41.45	52.4	41.05	56.0	54.9	40.4	62.7	73.2	
Salt (NaCl)	3.95	1.49	1.45	1.4	1.35	0.76	0.18	0.5	0.5	0.04	
Sugar	56.32	46.78	56.0	45.0	56.5	41.76	0.0	58.0	0.0	0.0	
HEC	0.98	0.52	1.0	1.0	1.0	1.21	0.0	1.0	0.0	0.0	
Bactericide	0.19	0.05	0.1	0.1	0.1	0.27	0.0	0.1	0.0	0.0	
Triton X-100	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	36.8	0.0	
DGBE	0.0	0.0	0.0	0.0	0.0	0.0	44.92	0.0	0.0	26.7	
Dielectric Constant	43.42	58.0	42.54	56.1	42.0	56.8	39.9	54.0	39.8	52.5	
Conductivity (S/m)	0.85	0.83	0.91	0.95	1.0	1.07	1.42	1.45	1.88	1.78	

Salt: 99 ⁺% Pure Sodium Chloride Sugar: 98 ⁺% Pure Sucrose

Water: De-ionized, 16 M Ω^+ resistivity HEC: Hydroxyethyl Cellulose DGBE: 99 $^+$ % Di(ethylene glycol) butyl ether, [2-(2-butoxyethoxy)ethanol]

Triton X-100 (ultra pure): Polyethylene glycol mono [4-(1,1,3,3-tetramethylbutyl)phenyl]ether

Simulating Liquids for 5 GHz, Manufactured by SPEAG

Ingredients	(% by weight)
Water	78
Mineral Oil	11
Emulsifiers	9
Additives and Salt	2



Date of Issue : 2013-08-06 Page : 12 / 52

1.14 Test System Validation

Per FCC KDB 865664 D02v01, SAR system validation status should be documented to confirm measurement accuracy. The SAR systems (including SAR probes, system components and software versions) used for this device were validated against its performance specifications prior to the SAR measurements. Reference dipoles were used with the require tissue-equivalent media for system validation, according to the procedures outlined in IEEE 1528-2003 and FCC KDB 865664 D01v01. Since frequency within the valid frequency range of the probe calibration point, using the system that normally operates with the probe for routine SAR measurements and according to the required tissue-equivalent media.

A tabulated summary of the system validation status including the validation date(s), measurement frequencies, SAR probe and tissue dielectric parameters has been included.

f	Date	Probe	Probe	Tissue	Dielectric Parameters		CW Validation			Modulated Validation		
(MHz)	Date	S/N	Cal point	Type	Permitt ivity	Condu ctivity	Sensitivity	Probe Linearity	Probe Isotropy	Mod. Type	Duty Factor	PAR
2450	04/07/2013	3862	2450	Body	51.85	1.96	PASS	PASS	PASS	OFDM	N/A	PASS

< SAR System Validation Summary>

1.15 Test Standards and Limits

According to FCC 47CFR §2.1093(d) The limits to be used for evaluation are based generally on criteria published by the American National Standards Institute (ANSI) for localized specific absorption rate ("SAR") in Section 4.2 of "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kllz to 300 Gllz," ANSI/IEEE C95.3–2003, Copyright 2003 by the Institute of Electrical and Electronics Engineers, Inc., New York, New York 10017. These criteria for SAR evaluation are similar to those recommended by the National Council on Radiation Protection and Measurements (NCRP) in "Biological Effects and Exposure Criteria for Radio frequency Electromagnetic Fields," NCRP Report No. 86, Section 17.4.5. Copyright NCRP, 1986, Bethesda, Maryland 20814. SAR is a measure of the rate of energy absorption due to exposure to an RF transmitting source. SAR values have been related to threshold levels for potential biological hazards. The criteria to be used are specified in paragraphs (d)(1) and (d)(2) of this section and shall apply for portable devices transmitting in the frequency range from 100 kllz to 6 Gllz. Portable devices that transmit at frequencies above 6 Gllz are to be evaluated in terms of the MPE limits specified in § 1.1310 of this chapter. Measurements and calculations to demonstrate compliance with MPE field strength or power density limits for devices operating above 6 Gllz should be made at a minimum distance of 5 cm from the radiating source.

(1) Limits for Occupational/Controlled exposure: 0.4 W/kg as averaged over the whole-body and spatial peak SAR not exceeding 8 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 20 W/kg, as averaged over an 10 grams of tissue (defined as a tissue volume in the shape of a cube). Occupational/Controlled limits apply when persons are exposed as a consequence of their employment

SGS Korea Co., Ltd. #18-34, Sanbon-dong, Gunpo-si, Gyeonggi-do, 453-040 KOREA t+8231 428 5700 f+8231 427 2370 www.kr.sgs.com/ee



Date of Issue : 2013-08-06 Page : 13 / 52

provided these persons are fully aware of and exercise control over their exposure. Awareness of exposure can be accomplished by use of warning labels or by specific training or education through appropriate means, such as an RF safety program in a work environment.

(2) Limits for General Population/Uncontrolled exposure: 0.08 W/kg as averaged over the whole-body and spatial peak SAR not exceeding 1.6 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 4 W/kg, as averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube). General Population/Uncontrolled limits apply when the general public may be exposed, or when persons that are exposed as a consequence of their employment may not be fully aware of the potential for exposure or do not exercise control over their exposure. Warning labels placed on consumer devices such as cellular telephones will not be sufficient reason to allow these devices to be evaluated subject to limits for occupational/controlled exposure in paragraph (d)(1) of this section.(Table .4)

Human Exposure	Uncontrolled Environment General Population	Controlled Environment Occupational
Partial Peak SAR (Partial)	1.60 m W/g	8.00 m W/g
Partial Average SAR (Whole Body)	0.08 m W/g	0.40 m W/g
Partial Peak SAR (Hands/Feet/Ankle/Wrist)	4.00 m W/g	20.00 m W/g

Table .2 RF exposure limits



Date of Issue : 2013-08-06 Page : 14 / 52

2. Instruments List

Maunfacturer	Device	Туре	Serial Number	Cal Date	Cal Interval	Cal Due
Stäubli	Robot	RX90BL	F03/5W05A1/A/01	N/A	N/A	N/A
Schmid& Partner Engineering AG	Dosimetric E-Field Probe	EX3DV3	3862	02/04/2013	Annual	02/04/2014
Schmid& Partner Engineering AG	2450 Mb System Validation Dipole	D2450V2	892	07/09/ 2012	Biennial	07/09/2014
Schmid& Partner Engineering AG	Data acquisition Electronics	DAE3	567	01/25/2013	Annual	01/25/2014
Schmid& Partner Engineering AG	Software	DASY4 V4.7	-	N/A	N/A	N/A
Schmid& Partner Engineering AG	Phantom	ELI Phantom	TP-1169	N/A	N/A	N/A
Agilent	Network Analyzer	E5071C	MY46111535	07/03/2013	Annual	07/03/2014
Schmid& Partner Engineering AG	Dielectric Assessment Kit	DAK-3.5	1108	03/05/2013	Annual	03/05/2014
Agilent	Power Meter	E4419B	GB43311125	07/01/2012	Annual	07/01/2013
Agilent	Power Sensor	Е9300Н	MY41495314 MY41495307	09/18/2012 09/18/2012	Annual Annual	09/18/2013 09/18/2013
Agilent	Signal Generator	E4421B	MY42082477	03/28/2013	Annual	03/28/2014
Empower RF Systems	Power Amplifier	2001-BBS3Q7ECK	1032 D/C 0336	03/29/2013	Annual	03/29/2014
Agilent	Directional RF Bridges	86205A	MY31402302	07/03/2012	Annual	07/03/2013
Microlab	LP Filter	LA-15N LA-30N LA-60N	N/A	09/14/2012	Annual	09/14/2013
Agilent	Attenuator	8491B	50566	09/14/2012	Annual	09/14/2013



Date of Issue : 2013-08-06 Page : 15 / 52

3. Summary of Results

3.1 FCC Power Measurement Procedures

The SAR measurement Software calculates a reference point at the start and end of the test to check for power drifts. If conducted power deviations of more than 5 % occurred, the tests were repeated.

3.2 Measured and Reported SAR

Per FCC KDB Publication 447498 D01v05, When SAR is not measured at the maximum power level allowed for production units, the results must be scaled to the maximum tune-up tolerance limit according to the power applied to the individual channels tested to determine compliance. For simultaneous transmission, the measured aggregate SAR must be scaled according to the sum of the differences between the maximum tune-up tolerance and actual power used to test each transmitter. When SAR is measured at or scaled to the maximum tune-up tolerance limit, the results are referred to as reported SAR. Test highest reported SAR results are identified on the grant of equipment authorization according to procedures in KDB 690783 D01v01r02.

3.3 RF Conducted Power

WLAN 2.4 GHz

Mode	Freq. (MHz)	Ch. #	Rate	Measured Power [dB m]
	2412	1	1	17.68
802.11b	2437	6	1	17.69
	2462	11	1	16.80
	2412	1	6	13.37
802.11g	2437	6	6	17.60
	2462	11	6	13.29
000.44	2412	1	HT0	12.81
802.11n HT20	2437	6	HT0	16.98
11120	2462	11	HT0	13.11
000 11	2422	3	HT0	10.01
802.11n HT40	2437	6	HT0	15.70
11140	2452	9	HT0	11.25

Bluetooth

Channel	Frequency (Mb)	GFSK (dB m)	4DQPSK (dB m)	8DPSK (dB m)	LE (dB m)
Low	2402	-4.45	-4.12	-4.57	0.07
Middle	2441	-4.85	-4.44	-4.67	0.05
High	2480	-4.41	-4.37	-4.66	0.21



Date of Issue : 2013-08-06 Page : 16 / 52

3.4 SAR Test Configuration

IEEE 802.11 Transmitters

802.11 a/b/g and 4.9 \mbox{GHz} operating modes are tested independently according to the service requirements in each frequency band. 802.11 b/g modes are tested on channel 1, 6, and 11. 802.11a is tested for UNII operations on channels 36 and 48 in the 5.15 \sim 5.25 \mbox{GHz} band, channels 52 and 64 in the 5.25 \sim 5.35 \mbox{GHz} band, channels 104, 116, 124 and 136 in the 5.470 \sim 5.725 \mbox{GHz} band, and channels 149 and 161 in the 5.8 \mbox{GHz} band. When 5.8 \mbox{GHz} §15.247 is also available, channels 149, 157 and 165 should be tested instead of the UNII channels. 802.11g mode was evaluated only if the output power was 0.25 \mbox{dB} higher than the 802.11b mode.

3.7.1				Turbo	"De	fault Test	Channel	ls"
Mode		GHz	Channel	Channel		247	Uľ	JII
				Chainte	802.11b	802.11g	01	111
		2.412	1#		4	▽		
802.1	l b/g	2.437	6	6	4	⊽		
			11#		- √	7		
		5.18	36				4	
		5.20	40	42 (5.21 GHz)				•
		5.22	44	42 (J.21 G1E)				
		5.24	48	50 (5.25 GHz)			4	
		5.26	52	30 (3.23 G1E)			4	
	- 48	5.28	56	58 (5.29 GHz)		-		**
	88	5.30	60	J6 (J.25 G1E)				
		5.32	64				4	
		5.500	100					100
	UNII	5.520	104			100	4	
	100	5.540	108		7 7			•
802.11a	1	5.560	112			-		
802.11a	-	5.580	116		-		4	
	1	5.600	120	Unknown	and the same of the			
-		5.620	124		The same of		4	
		5.640	128					
430		5.660	132					189
1000		5.680	136		-		4	
The same of		5.700	140					•
700	TIMITE	5.745	149		4		4	
	UNII	5.765	153	152 (5.76 GHz)				•
	§15.247	5.785	157		4			
		5.805	161	160 (5.80 GHz)			4	
	§15.247	5.825	165		4			

- **√** = "default test channels"
- = possible 802.11 a channels with maximum average output > the "default test channels"
- ▼ = possible 802.11g channels with maximum average output ¼ dB ≥ the "default test channels"
- # = when output power is reduced for channel 1 and/or 11 to meet restricted band requirements the
 highest output channels closest to each of these channels should be tested



Date of Issue:

2013-08-06

Page:

17 / 52


3.5 SAR Test Exclusions Applied

Per FCC KDB 447498 D01v05, the SAR exclusion threshold for distances < 50 mm is defined by the following equation:

$$\frac{\text{Max Power of Channel (mW)}}{\text{Test Separation Distance (mm)}} * \sqrt{\text{Frequency(GHz)}} \le 3.0$$

Based on the maximum tune-up tolerance limit of Bluetooth the antenna to use separation distance, Bluetooth SAR was not required: $(1.26/5 * \sqrt{2.480} = 0.39 < 3.0)$

<The Distance information of Antenna to Edges of EUT>

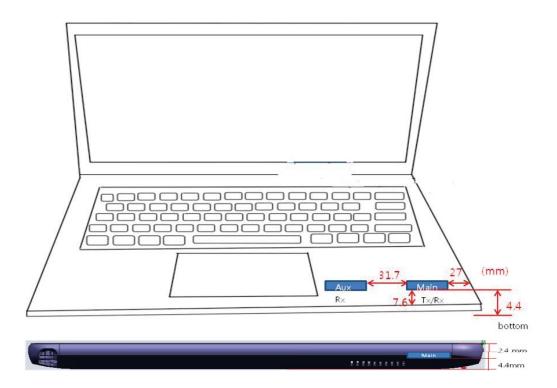



Date of Issue : 2013-08-06 Page : 18 / 52

3.6 SAR Data Summary

Ambient Temperature (°C) 23.8 Liquid Temperature (°C) 21.5 Date 06/13/2013

WLAN 2.45 GHz Body SAR

Test EUT		Traffic Channel		Distance	Power(dBm)		1-g SAR (W/kg)		1 g SAR
Mode	Eugenee	Frequency (Mt/z)	Channel	(MM)	Measured Power	Tune-Up Limit	Measured SAR	Scaled SAR	Limits (W/kg)
	2437	6	0	17.69	18.5	0.299	0.360		
	Base	2412	1	0	17.68	18.5	0.288	0.348	
802.11b		2462	11	0	16.80	17.5	0.230	0.270	1.6
Back Screen	2437	6	15	17.69	18.5	0.003	0.004		

SAR Test Notes

General Notes:

- 1. The test data reported are the worst-case SAR values according to test procedures specified in IEEE 1528-2003, FCC/OET Bulletin 65, Supplement C [June 2001] and FCC KDB Publication 447498 D01v05.
- 2. All modes of operation were investigated, and worst-case results are reported.
- 3. Battery is fully charged for all readings and the standard batteries are the only options.
- 4. The EUT is tested 2nd hot-spot peak, if it is less than 2 dB below the highest peak.
- 5. The manufacturer has confirmed that the device(s) tested have the same physical, mechanical and thermal characteristics and are within operational tolerances expected for production units.
- 6. SAR results were scaled to the maximum allowed power to demonstrate compliance per FCC KDB Publication 447498 D01v05.
- 7. Back screen Position tested according to RSS-102 (Issue 4) standard.

WLAN Notes:

- 1. For 2.4 GHz, justification for reduced test configuration for WIFI channels per KDB Publication 248227 and April 2010 FCC/TCB Meeting Notes: Highest average RF output power channel for the lowest data rate were selected for SAR evaluation. Other IEEE 802.11 modes (including 802.11g/n) were not investigated since the average output powers were not greater than 0.25 dB than that of the corresponding channel in the lowest data rate IEEE 802.11b modes
- 2. WLAN transmission was verified using a spectrum analyzer.



Date of Issue : 2013-08-06 Page : 19 / 52

3.7 FCC Multi-TX SAR considerations

3.7.1 Introduction

The following procedures adopted from FCC KDB Publication 447498 D01v05 are applicable to handsets with built-in unlicensed transmitters such as Bluetooth devices which may simultaneously transmit with the licensed transmitter.

3.7.2 Simultaneous Transmission Procedures

This device contains transmitters that may operate simultaneously. Therefore simultaneous transmission analysis is require. Per FCC KDB 447498 D01v05 IV.C.1,iii, simultaneous transmission SAR test exclusion may be applied when the sum of the 1-g SAR for all the simultaneous transmitting antennas in a specific a physical test configuration is ≤ 1.6 W/kg. When standalone SAR is not required to be measured per FCC KDB 447498 D01v05 4.3.2.2), the following equation must be used to estimate the standalone 1g SAR for simultaneous transmission involving that transmitter.

Estimated SAR =
$$\frac{\sqrt{f(GHz)}}{7.5} * \frac{\text{(Max Power of channel, mW)}}{\text{Min. Separation Distance, mm}}$$

Mode	Frequency	Maximum Allowed Power	Separation Distance	Estimated SAR
112000	[MHz]	[dBm]	[mm]	[W/kg]
Bluetooth	2480	0.21	5	0.042
Bluetooth	2460	0.21	15	0.014

<Tablet.3 Estimated SAR >

3.6.3 The Simultaneous Transmission possibilities are listed as below

No	Capable TX Configuration	Body SAR
1	Wi-Fi (Main Antenna) + Bluetooth(Aux Antenna)	Yes

3.6.5 Body SAR Simultaneous Transmission Analysis

Simultaneous Transmission Summation Scenario with Wi-Fi and Bluetooth

Simultaneous TX	configuration	Wi-Fi SAR(W/kg)	Bluetooth SAR (W/kg)	∑SAR (W/kg)
D - 4	Base	0.360	0.042	0.402
Body	Back Screen	0.004	0.014	0.018

Notes.

- The above numerical summed SAR was below the SAR limit. Therefore, the above analysis is sufficient to
 determine that simultaneous transmission cases will not exceed the SAR limit. Therefore, no volumetric SAR
 summation is required since the numerical sums are below the limit.
- 2. Bluetooth SAR was not required to be measured per KDB 447498D01v05.



Date of Issue : 2013-08-06 Page : 20 / 52

Appendix

List

Appendix A	DASY4 Report (Plots of the SAR Measurements)	- 2450 Mb, Verification Test - WLAN Test
Appendix B	Uncertainty Analysis	
Appendix C	Calibration Certificate	- PROBE - DAE - DIPOLE



Date of Issue : 2013-08-06 Page : 21 / 52

Appendix A

Test Plot – DASY4 Report



Date of Issue : 2013-08-06 Page : 22 / 52

2450 Mb Verification Test

Date: 2013-06-13

Test Laboratory: SGS Korea (Gunpo Laboratory)
File Name: Verification 2450 MHz Body.da4

Input Power: 100 mW

Ambient Temp: 23.9 °C Tissue Temp: 22.2 °C

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:892

Program Name: Verification 2450 MHz_Body

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2450 MHz; $\sigma = 2.01 \text{ mho/m}$; $\varepsilon_r = 52$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section


DASY4 Configuration:

- Probe: EX3DV4 SN3862; ConvF(7.25, 7.25, 7.25); Calibrated: 2013-02-04
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2013-01-25
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1169
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

Verification 2450 MHz_Body/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 7.98 mW/g

Verification 2450 MHz_Body/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm,

d2=3mm Reference Value = 58.7 V/m; Power Drift = -0.007 dB Peak SAR (extrapolated) = 10.9 W/kg SAR(1 g) = 5.01 mW/g; SAR(10 g) = 2.26 mW/g Maximum value of SAR (measured) = 7.82 mW/g

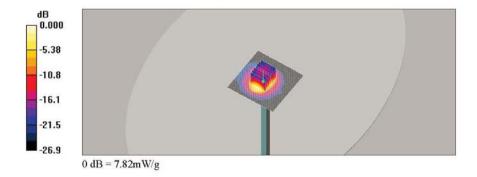



Date of Issue : 2013-08-06 Page : 23 / 52

WLAN 2450 MHz Body SAR Test

Date: 2013-06-13

Test Laboratory: SGS Korea (Gunpo Laboratory)
File Name: WLAN Base 802.11b 1Mbps CH6.da4

Ambient Temp: 23.9 °C Tissue Temp: 22.2 °C

DUT: NP270E5G; Type: Notebook; Serial: JGNR91ED600178N

Program Name: WLAN_Body

Communication System: WLAN; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2437 MHz; $\sigma = 1.99 \text{ mho/m}$; $\varepsilon_r = 52.1$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 SN3862; ConvF(7.25, 7.25, 7.25); Calibrated: 2013-02-04
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2013-01-25
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1169
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186


WLAN_Base_802.11b_1Mbps_CH6/Area Scan (201x201x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.437 mW/g

WLAN_Base_802.11b_1Mbps_CH6/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 6.31 V/m; Power Drift = -0.099 dB

Peak SAR (extrapolated) = 0.585 W/kg

SAR(1 g) = 0.299 mW/g; SAR(10 g) = 0.160 mW/g Maximum value of SAR (measured) = 0.427 mW/g

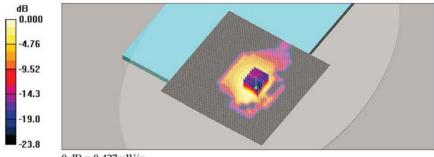

0 dB = 0.427 mW/g



Date of Issue : 2013-08-06 Page : 24 / 52

Date: 2013-06-13

Test Laboratory: SGS Korea (Gunpo Laboratory) File Name: <u>WLAN Base 802.11b 1Mbps CH1.da4</u>

Ambient Temp: 23.9 °C Tissue Temp: 22.2 °C

DUT: NP270E5G; Type: Notebook; Serial: JGNR91ED600178N

Program Name: WLAN_Body

Communication System: WLAN; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2412 MHz; $\sigma = 1.96$ mho/m; $\varepsilon_r = 52.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 SN3862; ConvF(7.25, 7.25, 7.25); Calibrated: 2013-02-04
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2013-01-25
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1169
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

WLAN_Base_802.11b_1Mbps_CH1/Area Scan (171x261x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.465 mW/g


WLAN_Base_802.11b_1Mbps_CH1/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 5.40 V/m; Power Drift = 0.053 dB

Peak SAR (extrapolated) = 0.548 W/kg

SAR(1 g) = 0.288 mW/g; SAR(10 g) = 0.135 mW/g

Maximum value of SAR (measured) = 0.412 mW/g

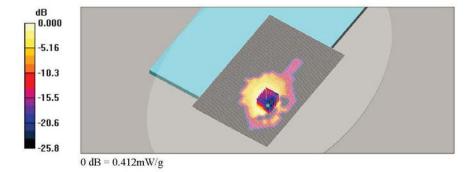



Date of Issue : 2013-08-06 Page : 25 / 52

Date: 2013-06-13

Test Laboratory: SGS Korea (Gunpo Laboratory) File Name: <u>WLAN Base 802.11b 1Mbps CH11.da4</u>

Ambient Temp: 23.9 °C Tissue Temp: 22.2 °C

DUT: NP270E5G; Type: Notebook; Serial: JGNR91ED600178N

Program Name: WLAN_Body

Communication System: WLAN; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2462 MHz; $\sigma = 2.02 \text{ mho/m}$; $\varepsilon_r = 52$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 SN3862; ConvF(7.25, 7.25, 7.25); Calibrated: 2013-02-04
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2013-01-25
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1169
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

WLAN_Base_802.11b_1Mbps_CH11/Area Scan (171x261x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.520 mW/g


WLAN_Base_802.11b_1Mbps_CH11/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 4.58 V/m; Power Drift = -0.156 dB

Peak SAR (extrapolated) = 0.474 W/kg

SAR(1 g) = 0.230 mW/g; SAR(10 g) = 0.108 mW/g

Maximum value of SAR (measured) = 0.329 mW/g

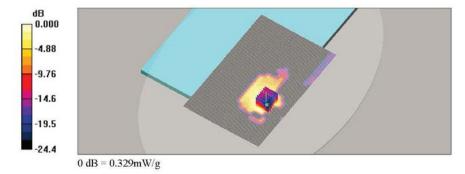



Date of Issue : 2013-08-06 Page : 26 / 52

Date: 2013-06-13

Test Laboratory: SGS Korea (Gunpo Laboratory)

File Name: WLAN Back Screen 802.11b 1Mbps CH6.da4

Ambient Temp: 23.9 °C Tissue Temp: 22.2 °C

DUT: NP270E5G; Type: Notebook; Serial: JGNR91ED600178N

Program Name: WLAN_Body

Communication System: WLAN; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2437 MHz; $\sigma = 1.99$ mho/m; $\varepsilon_r = 52.1$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 SN3862; ConvF(7.25, 7.25, 7.25); Calibrated: 2013-02-04
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn567; Calibrated: 2013-01-25
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1169
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

WLAN_Back Screen_802.11b_1Mbps_CH6/Area Scan (161x261x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.009 mW/g

WLAN_Back Screen_802.11b_1Mbps_CH6/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm,


dy=5mm, dz=5mm

Reference Value = 1.14 V/m; Power Drift = 0.041 dB

Peak SAR (extrapolated) = 0.011 W/kg

SAR(1 g) = 0.00304 mW/g; SAR(10 g) = 0.00225 mW/g

Maximum value of SAR (measured) = 0.006 mW/g

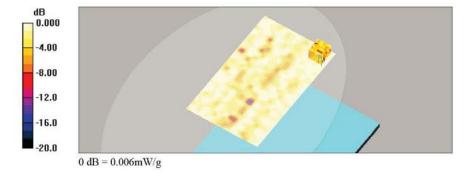



Date of Issue : 2013-08-06 Page : 27 / 52

Appendix B

Uncertainty Analysis

a	b	С	d	e = f(d,k)	g	i =
						cxg/e
Uncertainty Component	Section in	Tol	Prob .	Div.	Ci	1g
, .	P1528	(%)	Dist.		(1g)	ui (%)
Probe calibration	E.2.1	6.55	N	1	1	6.00
Axial isotropy	E.2.2	0.5	R	1.73	0.71	0.20
hemispherical isotropy	E.2.2	1.3	R	1.73	0.71	0.53
Boundary effect	E.2.3	0.8	R	1.73	1	0.46
Linearity	E.2.4	0.3	R	1.73	1	0.17
System detection limit	E.2.5	0.25	R	1.73	1	0.14
Readout electronics	E.2.6	0.3	N	1	1	0.30
Response time	E.2.7	0	R	1.73	1	0.00
Integration time	E.2.8	2.6	R	1.73	1	1.50
RF ambient Condition -Noise	E.6.1	3	R	1.73	1	1.73
RF ambient Condition - reflections	E.6.1	3	R	1.73	1	1.73
Probe positioning- mechanical tolerance	E.6.2	1.5	R	1.73	1	0.87
Probe positioning- with respect to phantom	E.6.3	2.9	R	1.73	1	1.67
Max. SAR evaluation	E.5.2	1	R	1.73	1	0.58
Test sample positioning	E.4.2	2.3	N	1	1	2.30
Device holder uncertainty	E.4.1	5.84	N	1	1	5.84
Output power variation -SAR drift measurement	6.62	5	R	1.73	1	2.89
Phantom uncertainty (shape and thickness tolerances)	E.3.1	6.6	R	1.73	1	3.81
Liquid conductivity - deviation from target values	E.3.2	5	R	1.73	0.64	1.85
Liquid conductivity	E.3.2	0.7	N	1	0.64	0.45
- measurement uncertainty	2.0.2	0.7	'`	· ·	0.01	0.40
Liquid permittivity	E.3.3	10	R	1.73	0.6	3.46
- deviation from target values			ļ '`	•	3.0	3.10
Liquid permittivity	E.3.3	0.56	N	1	0.6	0.34
- measurement uncertainty		3.00			3.0	
Combined standard uncertainty				RSS		11.56
Expanded uncertainty (95% CONFIDENCE INTERVAL)		-		k=2		23.13



Date of Issue : 2013-08-06 Page : 28 / 52

Appendix C

Calibration Certificate

- PROBE
- DAE
- 2450 Mb DIPOLE



Date of Issue:

2013-08-06

Page:

29 / 52

- PROBE Calibration Certificate

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

SGS (Dymstec)

Certificate No: EX3-3862 Feb13

Accreditation No.: SCS 108

CALIBRATION CERTIFICATE

Object

EX3DV4 - SN:3862

Calibration procedure(s)

QA CAL-01.v8, QA CAL-14.v3, QA CAL-23.v4, QA CAL-25.v4

Calibration procedure for dosimetric E-field probes

Calibration date:

February 4, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	29-Mar-12 (No. 217-01508)	Apr-13
Power sensor E4412A	MY41498087	29-Mar-12 (No. 217-01508)	Apr-13
Reference 3 dB Attenuator	SN: S5054 (3c)	27-Mar-12 (No. 217-01531)	Apr-13
Reference 20 dB Attenuator	SN: S5086 (20b)	27-Mar-12 (No. 217-01529)	Apr-13
Reference 30 dB Attenuator	SN: S5129 (30b)	27-Mar-12 (No. 217-01532)	Apr-13
Reference Probe ES3DV2	SN: 3013	28-Dec-12 (No. ES3-3013_Dec12)	Dec-13
DAE4	SN: 660	20-Jun-12 (No. DAE4-660_Jun12)	Jun-13
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-11)	In house check: Apr-13
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-12)	In house check: Oct-13

Name Function Calibrated by: Claudio Leubler Laboratory Technician Approved by: Katja Pokovic Technical Manager Issued: February 4, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: EX3-3862_Feb13

Page 1 of 11



Date of Issue : 2013-08-06

Page: 30 / 52

Calibration Laboratory of Schmid & Partner

Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S

C

S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid
NORMx,y,z sensitivity in free space
ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty_cycle) of the RF signal A, B, C, D modulation dependent linearization parameters

Polarization ϕ ϕ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques." December 2003
- Techniques", December 2003
 b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
 NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: EX3-3862_Feb13 Page 2 of 11



Date of Issue : 2013-08-06 Page : 31 / 52

EX3DV4 - SN:3862

February 4, 2013

Probe EX3DV4

SN:3862

Manufactured: February 2, 2012 Calibrated: February 4, 2013

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: EX3-3862_Feb13

Page 3 of 11



Date of Issue:

2013-08-06

Page:

32 / 52

EX3DV4-SN:3862

February 4, 2013

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3862

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (µV/(V/m) ²) ^A	0.42	0.43	0.37	± 10.1 %
DCP (mV) ^B	102.3	98.0	101.2	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	152.5	±3.3 %
		Y	0.0	0.0	1.0		150.7	
		Z	0.0	0.0	1.0		188.9	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: EX3-3862_Feb13

Page 4 of 11

A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

B Numerical linearization parameter: uncertainty not required.

E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



Date of Issue: 2013-08-06 Page: 33 / 52

EX3DV4-SN:3862 February 4, 2013

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3862

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
835	41.5	0.90	9.98	9.98	9.98	0.21	1.19	± 12.0 %
900	41.5 0.97 9.89 9.89 9		9.89 0.15	1.52	± 12.0 %			
1750	40.1	1.37	8.71	8.71	8.71	0.24	1.12	± 12.0 %
1900	40.0	1.40	8.36	8.36	8.36	0.37	0.80	± 12.0 %
2450	39.2	1.80	7.41	7.41	7.41	0.28	1.05	± 12.0 %
5200	36.0	4.66	4.92	4.92	4.92	0.40	1.80	± 13.1 %
5300	35.9	4.76	4.67	4.67	4.67	0.40	1.80	± 13.1 %
5500	35.6	4.96	4.49	4.49	4.49	0.50	1.80	± 13.1 %
5600	35.5	5.07	4.25	4.25	4.25	0.50 1.8	1.80	± 13.1 %
5800	35.3	5.27	4.09	4.09	4.09	0.50	1.80	± 13.1 %

Certificate No: EX3-3862_Feb13

Page 5 of 11

 $^{^{\}text{C}}$ Frequency validity of \pm 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to \pm 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. $^{\text{F}}$ At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to \pm 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to \pm 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.



Date of Issue: 2013-08-06 Page: 34 / 52

EX3DV4-SN:3862 February 4, 2013

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3862

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
835	55.2	0.97	9.76	9.76	9.76	0.27	1.11	± 12.0 %
900	55.0	1.05	9.66	9.66	9.66	0.30	1.00	± 12.0 %
1750	53.4	1.49	8.08	8.08	8.08	0.38	0.81	± 12.0 %
1900	53.3	1.52	7.72	7.72	7.72	0.30	0.96	± 12.0 %
2450	52.7	1.95	7.25	7.25	7.25	0.80	0.50	± 12.0 %
5200	49.0	5.30	4.26	4.26	4.26	0.50	1.90	± 13.1 %
5300	48.9	5.42	4.18	4.18	4.18	0.50	1.90	± 13.1 %
5500	48.6	5.65	3.89	3.89	3.89	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.73	3.73	3.73	0.50	1.90	± 13.1 %
5800	48.2	6.00	4.04	4.04	4.04	0.50	1.90	± 13.1 %

Certificate No: EX3-3862_Feb13

Page 6 of 11

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


⁷ At frequencies below 3 GHz, the validity of tissue parameters (a and d) can be reliaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (a and d) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.



Date of Issue: 2013-08-06 Page: 35 / 52

EX3DV4-SN:3862 February 4, 2013

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

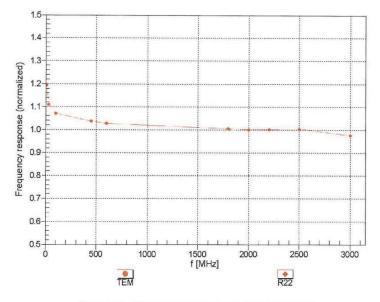

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: EX3-3862_Feb13


Page 7 of 11




Date of Issue : 2013-08-06 Page : 36 / 52

EX3DV4- SN:3862 February 4, 2013

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

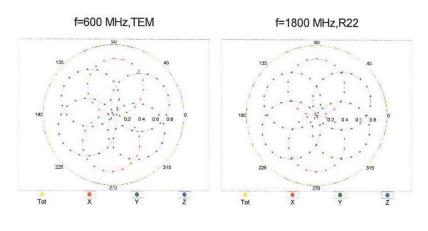

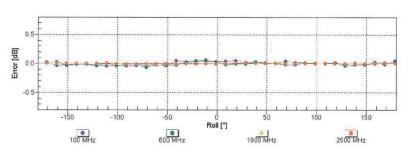

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: EX3-3862_Feb13

Page 8 of 11



Date of Issue:

2013-08-06


Page:


37 / 52

EX3DV4-SN:3862

February 4, 2013

Dynamic Range f(SAR_{head}) (TEM cell , f = 900 MHz)

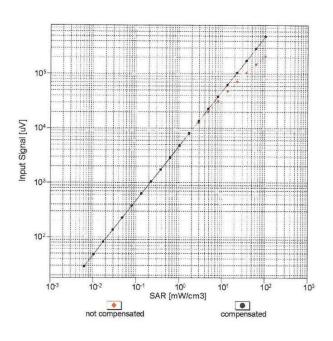



Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: EX3-3862_Feb13


Page 9 of 11




Date of Issue : 2013-08-06 Page : 38 / 52

EX3DV4- SN:3862 February 4, 2013

Conversion Factor Assessment

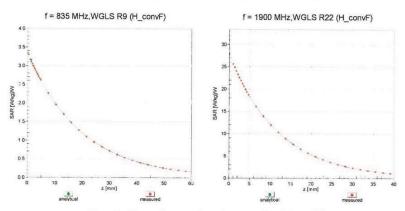

Deviation from Isotropy in Liquid Error (ϕ, ϑ) , f = 900 MHz

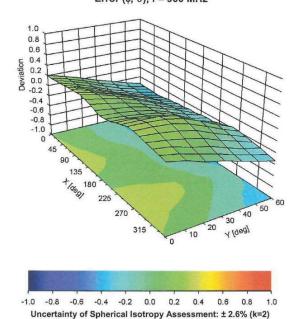

Certificate No: EX3-3862_Feb13

Page 10 of 11



Date of Issue : 2013-08-06 Page : 39 / 52

EX3DV4- SN:3862

February 4, 2013

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3862

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-71.3
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm

Certificate No: EX3-3862_Feb13

Page 11 of 11



Date of Issue:

2013-08-06

Page:

40 / 52

- DAE3 Calibration Certificate

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

SGS (Dymstec)

Certificate No: DAE3-567_Jan13

Accreditation No.: SCS 108

Object	DAE3 - SD 000 D	03 AA - SN: 567	
Calibration procedure(s)	QA CAL-06.v25 Calibration proced	lure for the data acquisition electr	ronics (DAE)
Calibration date:	January 25, 2013		
The measurements and the unce	ertainties with confidence pro	nal standards, which realize the physical units obability are given on the following pages and facility: environment temperature $(22 \pm 3)^{\circ}$ C a	are part of the certificate.
alibration Equipment used (Ma	TE critical for calibration)		
	ID #	Cal Date (Certificate No.)	Scheduled Calibration
rimary Standards		Cal Date (Certificate No.) 02-Oct-12 (No:12728)	Scheduled Calibration Oct-13
Primary Standards (eithley Multimeter Type 2001	ID#	02-Oct-12 (No:12728)	
rrimary Standards eithley Multimeter Type 2001 econdary Standards	ID # SN: 0810278		Oct-13
Primary Standards Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit Calibrator Box V2.1	ID# SN: 0810278 ID# SE UWS 053 AA 1001	02-Oct-12 (No:12728) Check Date (in house)	Oct-13 Scheduled Check
Primary Standards (eithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit	ID # SN: 0810278 ID # SE UWS 053 AA 1001 SE UMS 006 AA 1002	02-Oct-12 (No:12728) Check Date (in house) 07-Jan-13 (in house check) 07-Jan-13 (in house check)	Oct-13 Scheduled Check In house check: Jan-14 In house check: Jan-14
crimary Standards (eithley Multimeter Type 2001 Secondary Standards Suto DAE Calibration Unit Calibrator Box V2.1	ID# SN: 0810278 ID# SE UWS 053 AA 1001 SE UMS 006 AA 1002 Name	02-Oct-12 (No:12728) Check Date (in house) 07-Jan-13 (in house check) 07-Jan-13 (in house check)	Oct-13 Scheduled Check In house check: Jan-14 In house check: Jan-14
Primary Standards (eithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit Calibrator Box V2.1	ID # SN: 0810278 ID # SE UWS 053 AA 1001 SE UMS 006 AA 1002	02-Oct-12 (No:12728) Check Date (in house) 07-Jan-13 (in house check) 07-Jan-13 (in house check)	Oct-13 Scheduled Check In house check: Jan-14 In house check: Jan-14
Primary Standards Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit	ID# SN: 0810278 ID# SE UWS 053 AA 1001 SE UMS 006 AA 1002 Name	02-Oct-12 (No:12728) Check Date (in house) 07-Jan-13 (in house check) 07-Jan-13 (in house check)	Oct-13 Scheduled Check In house check: Jan-14 In house check: Jan-14

Certificate No: DAE3-567_Jan13

Page 1 of 5



Date of Issue: 2013-08-06 Page: 41 / 52

Calibration Laboratory of Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE data acquisition electronics

Connector angle information used in DASY system to align probe sensor X to the robot

coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
 - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
 - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
 - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - Power consumption: Typical value for information. Supply currents in various operating modes

Certificate No: DAE3-567_Jan13

Page 2 of 5



Date of Issue : 2013-08-06 Page : 42 / 52

DC Voltage Measurement

A/D - Converter Resolution nominal

 $\begin{array}{lll} \mbox{High Range:} & \mbox{1LSB} = & \mbox{6.1}\mu\mbox{V} \,, & \mbox{full range} = & \mbox{-100...+300 mV} \\ \mbox{Low Range:} & \mbox{1LSB} = & \mbox{61nV} \,, & \mbox{full range} = & \mbox{-1......+3mV} \\ \mbox{DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec} \end{array}$

Calibration Factors	X	Y	Z
High Range	404.652 ± 0.02% (k=2)	404.401 ± 0.02% (k=2)	404.491 ± 0.02% (k=2)
Low Range	3.95362 ± 1.55% (k=2)	3.97148 ± 1.55% (k=2)	3.96078 ± 1.55% (k=2)

Connector Angle

Connector Angle to be used in DASY system	7°±1°
---	-------

Certificate No: DAE3-567_Jan13

Page 3 of 5



2013-08-06 Date of Issue: Page: 43 / 52

Appendix

1. DC Voltage Linearity

High Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	199995.32	-0.62	-0.00
Channel X + Input	20002.46	1.32	0.01
Channel X - Input	-19998.40	1.69	-0.01
Channel Y + Input	199997.71	1.34	0.00
Channel Y + Input	19999.63	-1.28	-0.01
Channel Y - Input	-19997.89	2.47	-0.01
Channel Z + Input	199996.03	0.01	0.00
Channel Z + Input	19998.99	-1.92	-0.01
Channel Z - Input	-19998.51	1.81	-0.01

Low Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	2002.18	0.83	0.04
Channel X + Input	201.83	0.08	0.04
Channel X - Input	-198.32	-0.18	0.09
Channel Y + Input	2001.92	0.81	0.04
Channel Y + Input	201.24	-0.29	-0.15
Channel Y - Input	-199.03	-0.72	0.36
Channel Z + Input	2001.88	0.72	0.04
Channel Z + Input	200.70	-0.97	-0.48
Channel Z - Input	-199.17	-0.97	0.49

Common mode sensitivity
 DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	3.30	1.64
	- 200	0.20	-1.94
Channel Y	200	-0.21	-0.42
	- 200	0.96	0.59
Channel Z	200	4.66	3.87
	- 200	-5.94	-6.09

3. Channel separation
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	-0.86	-3.62
Channel Y	200	7.58	-	-0.08
Channel Z	200	5.96	5.73	-

Certificate No: DAE3-567_Jan13



Date of Issue : 2013-08-06 Page : 44 / 52

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16316	14587
Channel Y	16163	15684
Channel Z	15966	15490

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input $10M\Omega$

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	0.52	-0.92	1.43	0.45
Channel Y	-0.20	-2.46	1.17	0.46
Channel Z	-0.70	-1.79	0.17	0.39

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE3-567_Jan13



Date of Issue:

2013-08-06

Page:

45 / 52

- 2450 Mb Dipole Calibration Certificate

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

CALIBRATION (CERTIFICATE		
Object	D2450V2 - SN: 8	392	
Calibration procedure(s)	QA CAL-05.v8 Calibration proce	edure for dipole validation kits abo	ove 700 MHz
Calibration date:	July 09, 2012		
		ry facility: environment temperature (22 \pm 3)°	C and humidity < 70%.
Calibration Equipment used (M&			
Calibration Equipment used (M&	TE critical for calibration)	ry facility: environment temperature (22 ± 3)°(Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451)	C and humidity < 70%. Scheduled Calibration Oct-12
Calibration Equipment used (M& Primary Standards Power meter EPM-442A	TE critical for calibration)	Cal Date (Certificate No.)	Scheduled Calibration
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	TE critical for calibration) ID # GB37480704	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451)	Scheduled Calibration Oct-12
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	TE critical for calibration) ID # GB37480704 US37292783	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451)	Scheduled Calibration Oct-12 Oct-12
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3	TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k)	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 27-Mar-12 (No. 217-01530)	Scheduled Calibration Oct-12 Oct-12 Apr-13
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3	TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.2 / 06327	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 27-Mar-12 (No. 217-01530) 27-Mar-12 (No. 217-01533)	Scheduled Calibration Oct-12 Oct-12 Apr-13 Apr-13
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3)AE4	TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3205	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 27-Mar-12 (No. 217-01530) 27-Mar-12 (No. 217-01533) 30-Dec-11 (No. ES3-3205_Dec11) 05-Jun-12 (No. DAE4-901_Jun12)	Scheduled Calibration Oct-12 Oct-12 Apr-13 Apr-13 Dec-12 Jun-13
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4	TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3205 SN: 901	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 27-Mar-12 (No. 217-01530) 27-Mar-12 (No. 217-01533) 30-Dec-11 (No. ES3-3205_Dec11)	Scheduled Calibration Oct-12 Oct-12 Apr-13 Apr-13 Dec-12
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Recondary Standards Power sensor HP 8481A	ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3205 SN: 901	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 27-Mar-12 (No. 217-01530) 27-Mar-12 (No. 217-01533) 30-Dec-11 (No. ES3-3205_Dec11) 05-Jun-12 (No. DAE4-901_Jun12) Check Date (in house)	Scheduled Calibration Oct-12 Oct-12 Apr-13 Apr-13 Dec-12 Jun-13 Scheduled Check
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3205 SN: 901 ID # MY41092317	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 27-Mar-12 (No. 217-01530) 27-Mar-12 (No. 217-01533) 30-Dec-11 (No. ES3-3205_Dec11) 05-Jun-12 (No. DAE4-901_Jun12) Check Date (in house)	Scheduled Calibration Oct-12 Oct-12 Apr-13 Apr-13 Dec-12 Jun-13 Scheduled Check In house check: Oct-13
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3205 SN: 901 ID # MY41092317 100005 US37390585 S4206	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 27-Mar-12 (No. 217-01530) 27-Mar-12 (No. 217-01533) 30-Dec-11 (No. ES3-3205_Dec11) 05-Jun-12 (No. DAE4-901_Jun12) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11) 18-Oct-01 (in house check Oct-11)	Scheduled Calibration Oct-12 Oct-12 Apr-13 Apr-13 Dec-12 Jun-13 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-12
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3205 SN: 901 ID # MY41092317 100005 US37390585 S4206 Name	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 27-Mar-12 (No. 217-01530) 27-Mar-12 (No. 217-01533) 30-Dec-11 (No. ES3-3205_Dec11) 05-Jun-12 (No. DAE4-901_Jun12) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11)	Scheduled Calibration Oct-12 Oct-12 Apr-13 Apr-13 Dec-12 Jun-13 Scheduled Check In house check: Oct-13 In house check: Oct-13
All calibrations have been conducted Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Calibrated by:	TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3205 SN: 901 ID # MY41092317 100005 US37390585 S4206	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 27-Mar-12 (No. 217-01530) 27-Mar-12 (No. 217-01533) 30-Dec-11 (No. ES3-3205_Dec11) 05-Jun-12 (No. DAE4-901_Jun12) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11) 18-Oct-01 (in house check Oct-11)	Scheduled Calibration Oct-12 Oct-12 Apr-13 Apr-13 Dec-12 Jun-13 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-12

Certificate No: D2450V2-892_Jul12

Page 1 of 8

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Issued: July 9, 2012



Date of Issue : 2013-08-06

Page: 46 / 52

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage

C Service suisse d'étalonnage Servizio svizzero di taratura S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
 No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-892_Jul12 Page 2 of 8



Date of Issue : 2013-08-06 Page : 47 / 52

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.1
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.9 ± 6 %	1.85 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.5 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	53.2 mW /g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.24 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	24.8 mW /g ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.4 ± 6 %	2.01 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	V.C
SAR measured	250 mW input power	13.3 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	52.1 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.18 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	24.4 mW / g ± 16.5 % (k=2)

Certificate No: D2450V2-892_Jul12

Page 3 of 8



Date of Issue:

2013-08-06

Page:

48 / 52

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$53.4 \Omega + 1.2 j\Omega$	
Return Loss	- 29.0 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.1 Ω + 3.7 jΩ	
Return Loss	- 28.7 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.163 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	October 06, 2011

Certificate No: D2450V2-892_Jul12

Page 4 of 8



Date of Issue : 2013-08-06 Page : 49 / 52

DASY5 Validation Report for Head TSL

Date: 09.07.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 892

Communication System: CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz; $\sigma = 1.85$ mho/m; $\epsilon_r = 38.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section


Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.45, 4.45, 4.45); Calibrated: 30.12.2011;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn901; Calibrated: 05.06.2012
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.1(838); SEMCAD X 14.6.5(6469)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 100.7 V/m; Power Drift = 0.04 dB Peak SAR (extrapolated) = 27.968 mW/g SAR(1 g) = 13.5 mW/g; SAR(10 g) = 6.24 mW/g Maximum value of SAR (measured) = 17.4 mW/g



0 dB = 17.4 mW/g = 24.81 dB mW/g

Certificate No: D2450V2-892_Jul12

Page 5 of 8




Date of Issue:

2013-08-06

Page:

50 / 52

Impedance Measurement Plot for Head TSL

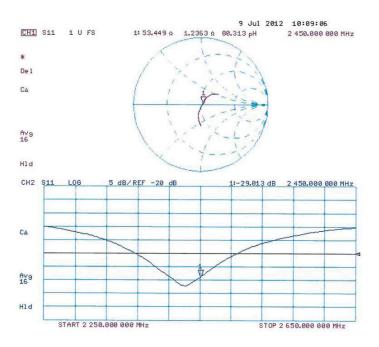

Certificate No: D2450V2-892_Jul12

Page 6 of 8



Date of Issue:

2013-08-06

Page:

51 / 52

DASY5 Validation Report for Body TSL

Date: 09.07.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 892

Communication System: CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz; $\sigma = 2.01$ mho/m; $\epsilon_r = 51.4$; $\rho = 1000$ kg/m 3

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

• Probe: ES3DV3 - SN3205; ConvF(4.26, 4.26, 4.26); Calibrated: 30.12.2011;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn901; Calibrated: 05.06.2012

• Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002


DASY52 52.8.1(838); SEMCAD X 14.6.5(6469)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 96.580 V/m; Power Drift = -0.00 dB Peak SAR (extrapolated) = 27.389 mW/g

SAR(1 g) = 13.3 mW/g; SAR(10 g) = 6.18 mW/g

Maximum value of SAR (measured) = 17.5 mW/g

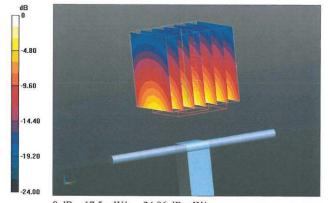

0 dB = 17.5 mW/g = 24.86 dB mW/g


Certificate No: D2450V2-892_Jul12

Page 7 of 8



Date of Issue : 2013-08-06 Page : 52 / 52

Impedance Measurement Plot for Body TSL

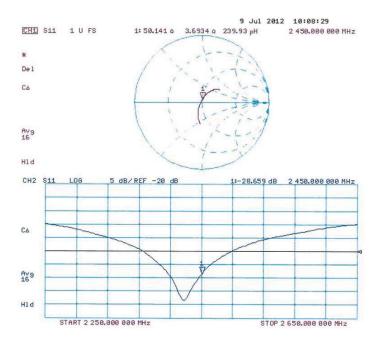

-THE END-