



Accredited by the Swiss Federal Office of Metrology and Accreditation  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client **Nokia Salo TCC**

Certificate No: **ER3-2333\_Jan06**

**CALIBRATION CERTIFICATE**

|                                  |                                                                                                            |
|----------------------------------|------------------------------------------------------------------------------------------------------------|
| Object                           | ER3DV6 - SN:2333                                                                                           |
| Calibration procedure(s)         | QA CAL-02.v4<br>Calibration procedure for E-field probes optimized for close near field evaluations in air |
| Calibration date:                | January 24, 2006                                                                                           |
| Condition of the calibrated item | In Tolerance                                                                                               |

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID #            | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration  |
|----------------------------|-----------------|-------------------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 3-May-05 (METAS, No. 251-00466)           | May-06                 |
| Power sensor E4412A        | MY41495277      | 3-May-05 (METAS, No. 251-00466)           | May-06                 |
| Power sensor E4412A        | MY41498087      | 3-May-05 (METAS, No. 251-00466)           | May-06                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 11-Aug-05 (METAS, No. 251-00499)          | Aug-06                 |
| Reference 20 dB Attenuator | SN: S5086 (20b) | 3-May-05 (METAS, No. 251-00467)           | May-06                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 11-Aug-05 (METAS, No. 251-00500)          | Aug-06                 |
| Reference Probe ER3DV6     | SN: 2328        | 3-Oct-05 (SPEAG, No. ER3-2328_Oct05)      | Oct-06                 |
| DAE4                       | SN: 654         | 27-Oct-05 (SPEAG, No. DAE4-654_Oct05)     | Oct-06                 |
| Secondary Standards        | ID #            | Check Date (in house)                     | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (SPEAG, in house check Nov-05)   | In house check: Nov-07 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (SPEAG, in house check Nov-05)  | In house check: Nov 06 |

|                |               |                   |           |
|----------------|---------------|-------------------|-----------|
|                | Name          | Function          | Signature |
| Calibrated by: | Katja Pokovic | Technical Manager |           |
| Approved by:   | Niels Kuster  | Quality Manager   |           |

Issued: January 24, 2006

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**DASY - Parameters of Probe: ER3DV6 SN:2333**Sensitivity in Free Space [ $\mu\text{V}/(\text{V}/\text{m})^2$ ]Diode Compression<sup>A</sup>NormX      **1.45 ± 10.1 % (k=2)**DCP X      **94 mV**NormY      **1.50 ± 10.1 % (k=2)**DCP Y      **94 mV**NormZ      **1.45 ± 10.1 % (k=2)**DCP Z      **99 mV**

Frequency Correction

X      **0.0**Y      **0.0**Z      **0.0**

Sensor Offset

(Probe Tip to Sensor Center)

X      **2.5 mm**Y      **2.5 mm**Z      **2.5 mm**


Connector Angle

**319 °**

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.



<sup>A</sup> numerical linearization parameter: uncertainty not required

Frequency Response of E-Field  
(TEM-Cell:ifi110 EXX, Waveguide R22)


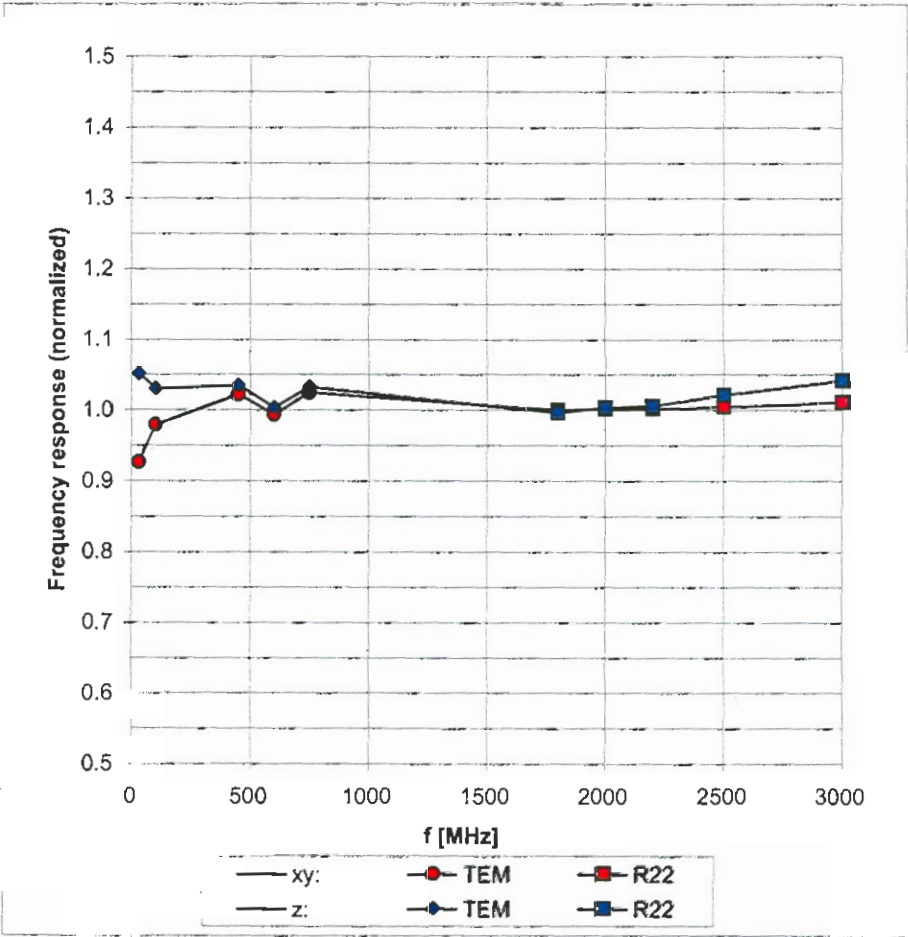


Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  (k=2)


Receiving Pattern ( $\phi$ ),  $\vartheta = 0^\circ$

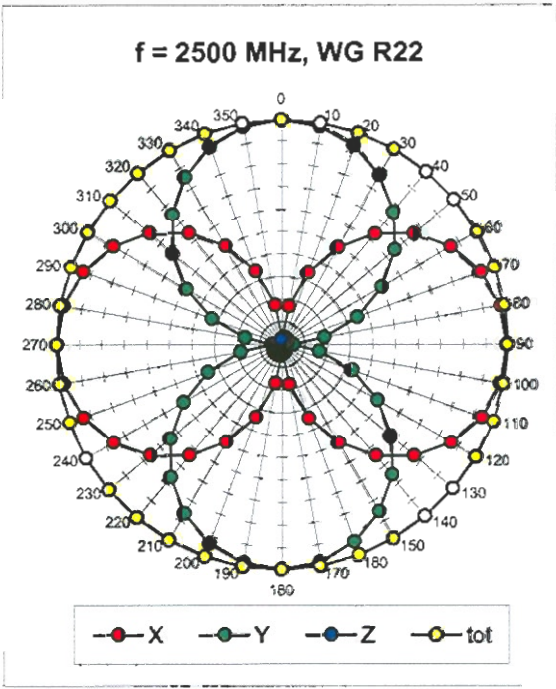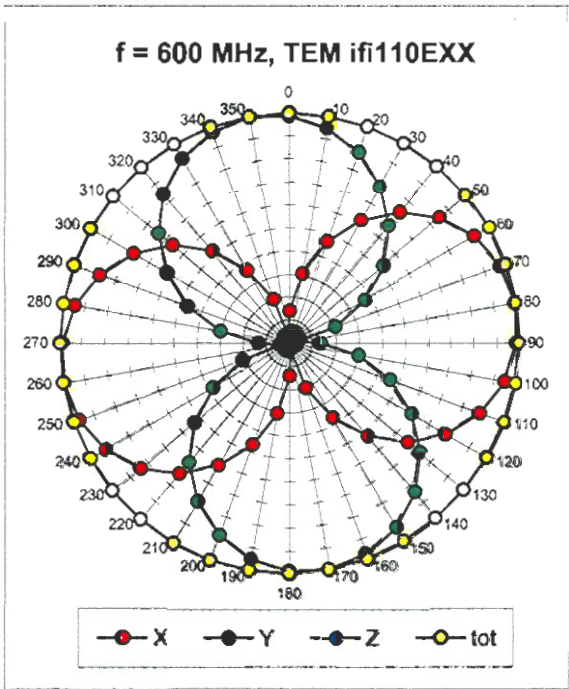

Receiving Pattern ( $\phi$ ),  $\vartheta = 90^\circ$

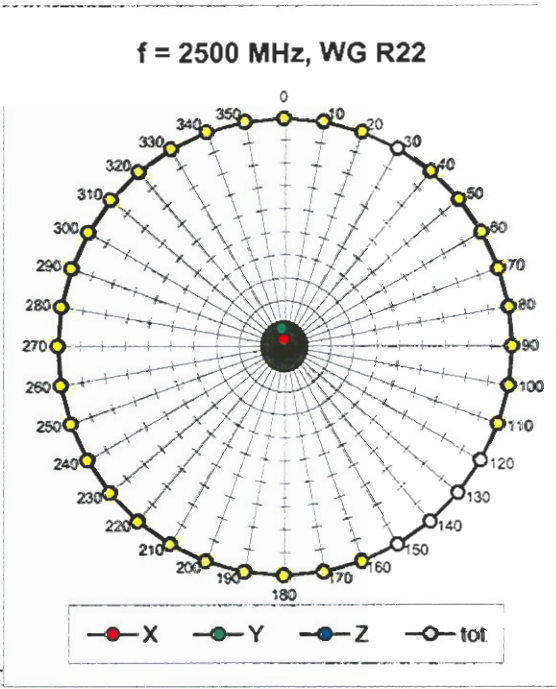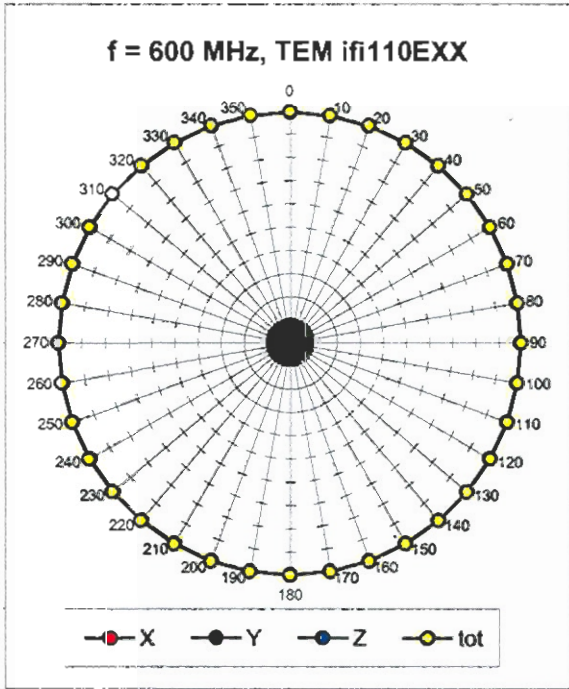


Receiving Pattern ( $\phi$ ),  $\vartheta = 0^\circ$

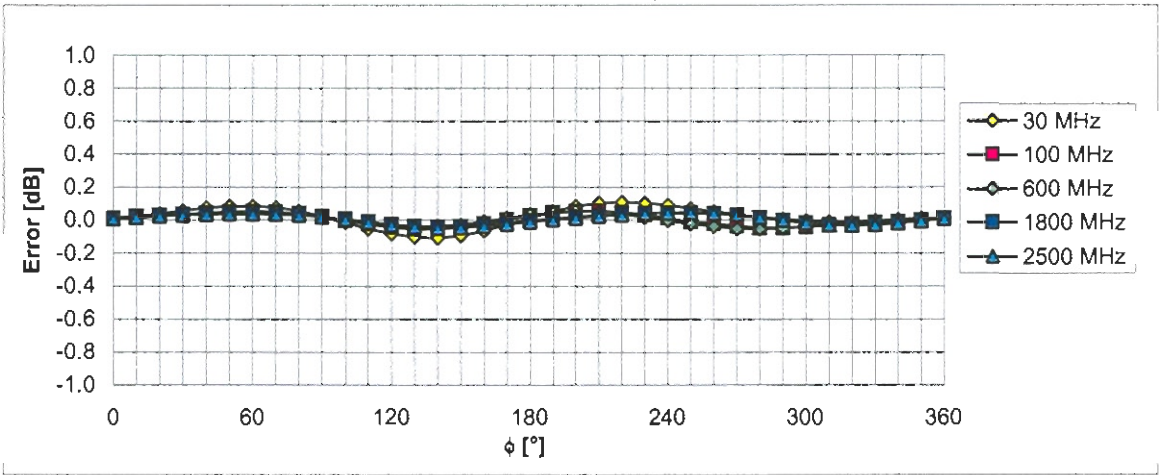


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

Receiving Pattern ( $\phi$ ),  $\vartheta = 90^\circ$

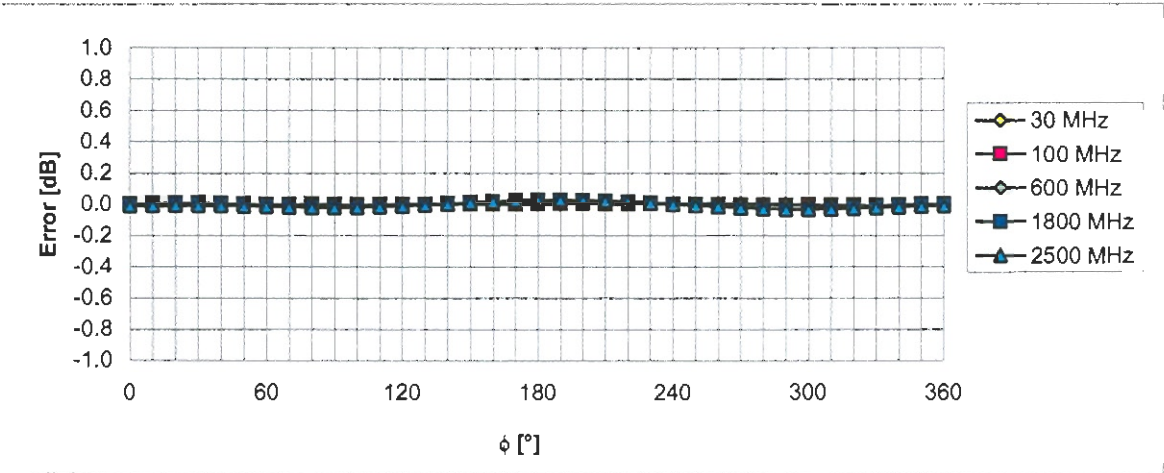


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

Dynamic Range f(E-field)  
(Waveguide R22, f = 1800 MHz)

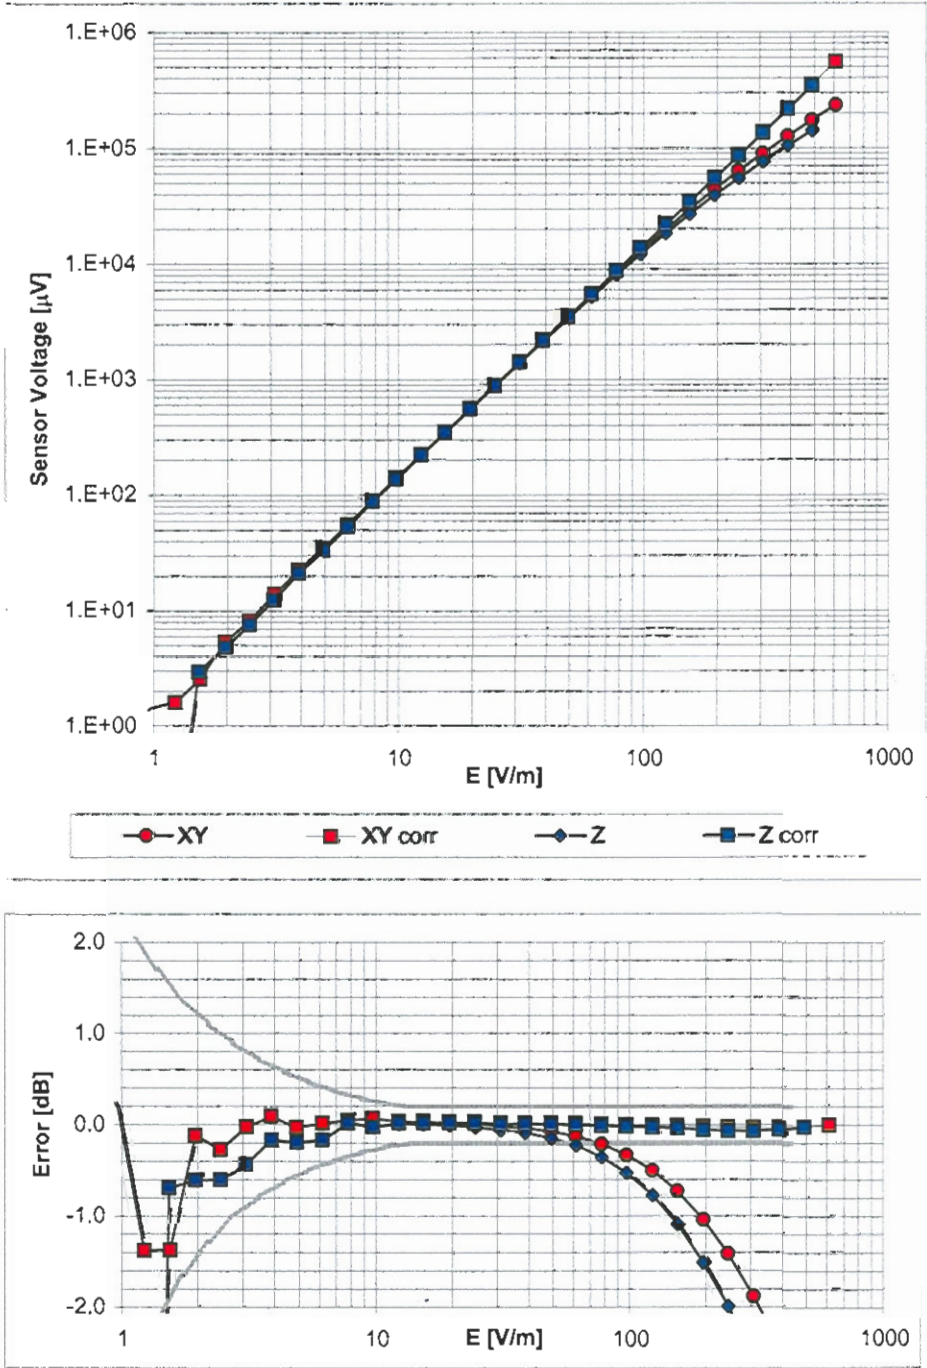

Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )

Deviation from Isotropy in Air  
Error ( $\phi, \vartheta$ ) ,  $f = 900 \text{ MHz}$

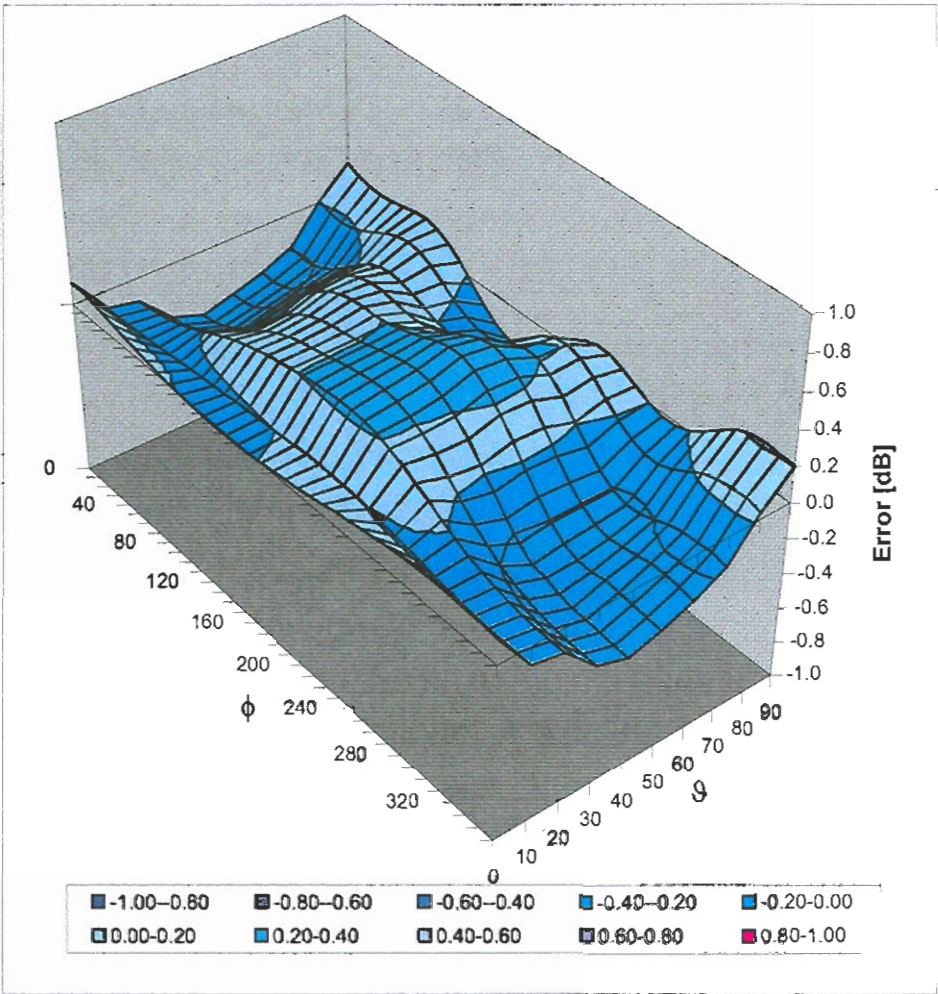

Uncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  ( $k=2$ )



Accredited by the Swiss Federal Office of Metrology and Accreditation  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Nokia Salo TCC**

Certificate No: **H3-6053\_Jan06**

## CALIBRATION CERTIFICATE

Object **H3DV6 - SN:6053**

Calibration procedure(s) **QA CAL-03.v4  
Calibration procedure for H-field probes optimized for close near field  
evaluations in air**

Calibration date: **January 24, 2006**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID #            | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|----------------------------|-----------------|-------------------------------------------|-----------------------|
| Power meter E4419B         | GB41293874      | 3-May-05 (METAS, No. 251-00466)           | May-06                |
| Power sensor E4412A        | MY41495277      | 3-May-05 (METAS, No. 251-00466)           | May-06                |
| Power sensor E4412A        | MY41498087      | 3-May-05 (METAS, No. 251-00466)           | May-06                |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 11-Aug-05 (METAS, No. 251-00499)          | Aug-06                |
| Reference 20 dB Attenuator | SN: S5086 (20b) | 3-May-05 (METAS, No. 251-00467)           | May-06                |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 11-Aug-05 (METAS, No. 251-00500)          | Aug-06                |
| Reference Probe H3DV6      | SN: 6182        | 3-Oct-05 (SPEAG, No. H3-6182_Oct05)       | Oct-06                |
| DAE4                       | SN: 654         | 27-Oct-05 (SPEAG, No. DAE4-654_Oct05)     | Oct-06                |

| Secondary Standards       | ID #         | Check Date (in house)                    | Scheduled Check        |
|---------------------------|--------------|------------------------------------------|------------------------|
| RF generator HP 8648C     | US3642U01700 | 4-Aug-99 (SPEAG, in house check Nov-05)  | In house check: Nov-07 |
| Network Analyzer HP 8753E | US37390585   | 18-Oct-01 (SPEAG, in house check Nov-05) | In house check: Nov 06 |

|                |                      |                          |           |
|----------------|----------------------|--------------------------|-----------|
|                | Name                 | Function                 | Signature |
| Calibrated by: | <b>Katja Pokovic</b> | <b>Technical Manager</b> |           |
| Approved by:   | <b>Niels Kuster</b>  | <b>Quality Manager</b>   |           |

Issued: January 24, 2006

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

DASY - Parameters of Probe: H3DV6 SN:6053

Sensitivity in Free Space [A/m /  $\sqrt{(\mu V)}$ ]

|   | a0        | a1        | a2                      |
|---|-----------|-----------|-------------------------|
| X | 2.712E-03 | -7.584E-5 | -4.156E-5 ± 5.1 % (k=2) |
| Y | 2.563E-03 | -1.967E-4 | 7.116E-5 ± 5.1 % (k=2)  |
| Z | 2.915E-03 | -3.764E-4 | 5.853E-5 ± 5.1 % (k=2)  |

Diode Compression<sup>1</sup>

|       |       |
|-------|-------|
| DCP X | 85 mV |
| DCP Y | 85 mV |
| DCP Z | 85 mV |

Sensor Offset (Probe Tip to Sensor Center)

|   |        |
|---|--------|
| X | 3.0 mm |
| Y | 3.0 mm |
| Z | 3.0 mm |


Connector Angle 33 °

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>1</sup> numerical linearization parameter: uncertainty not required



# Frequency Response of H-Field

(TEM-Cell:ifi110, Waveguide R22)


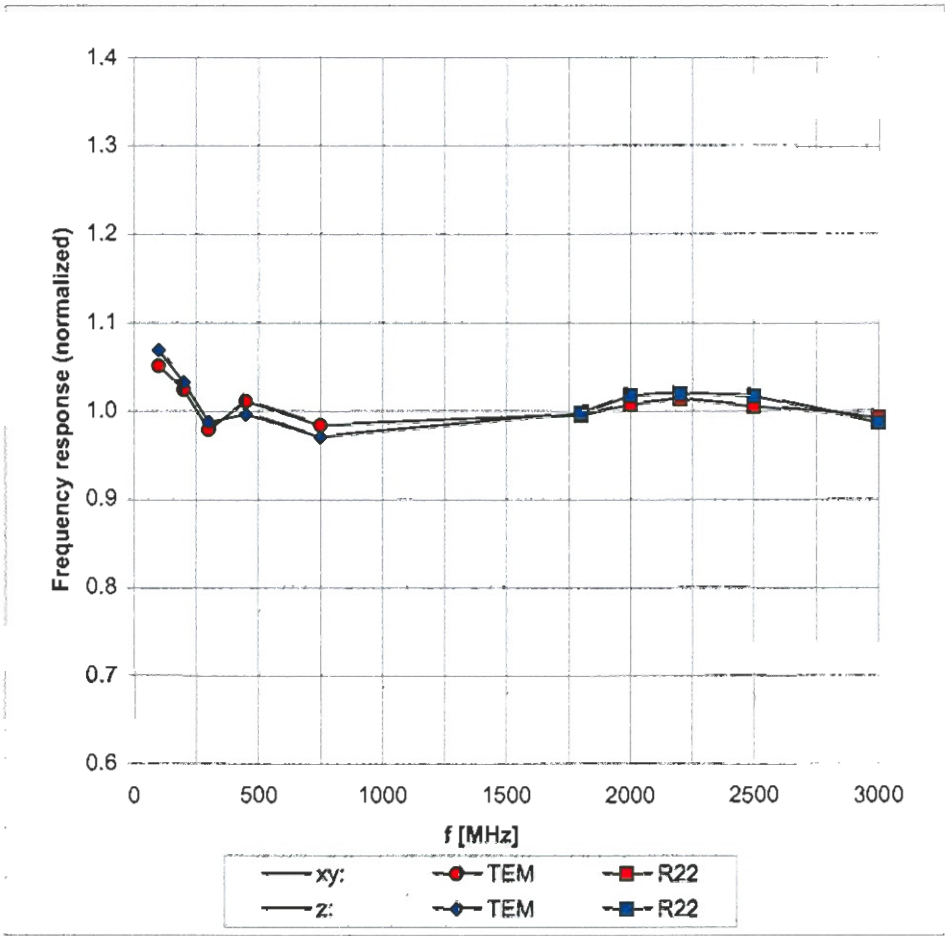


Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  (k=2)


Receiving Pattern ( $\phi$ ),  $\vartheta = 90^\circ$

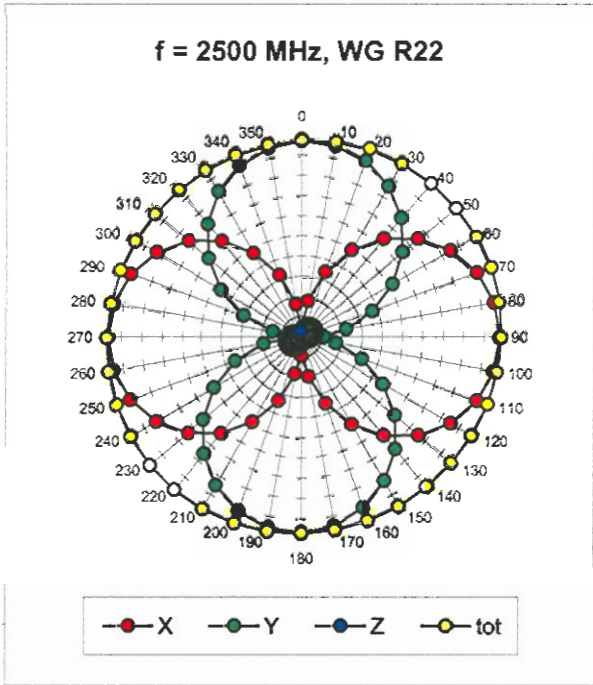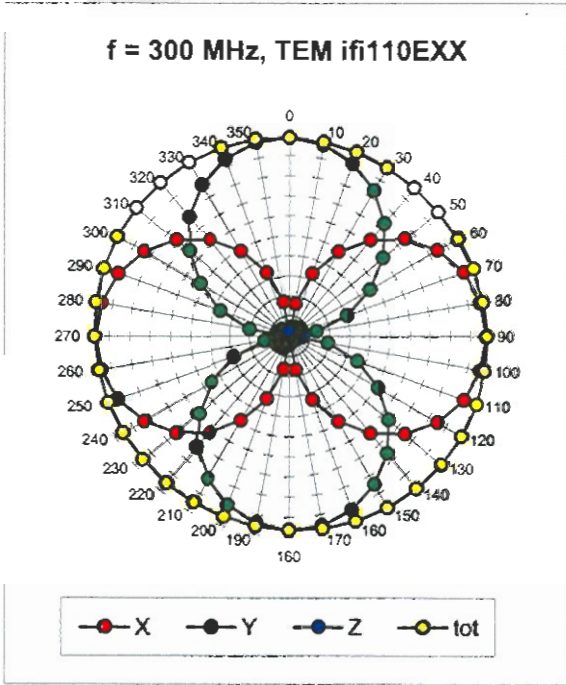

Receiving Pattern ( $\phi$ ),  $\vartheta = 0^\circ$

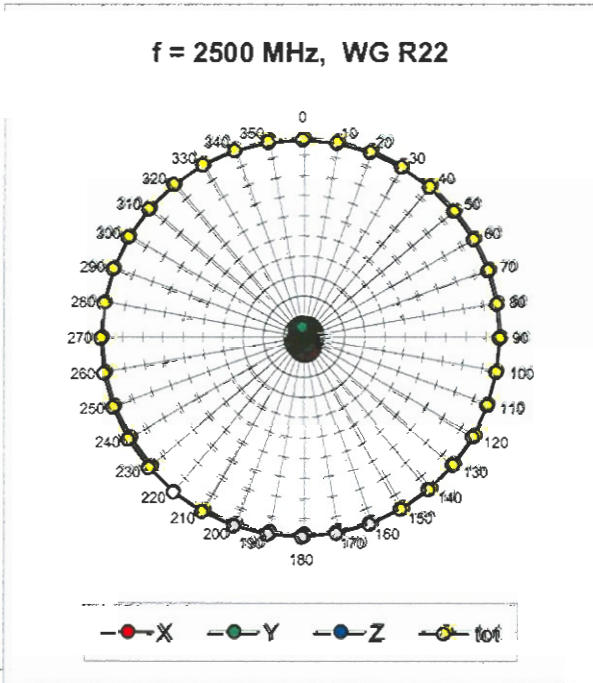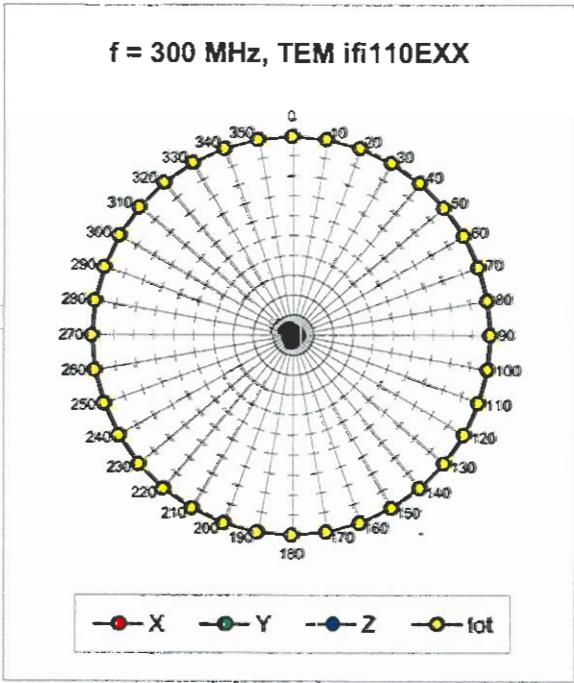


Receiving Pattern ( $\phi$ ),  $\vartheta = 90^\circ$

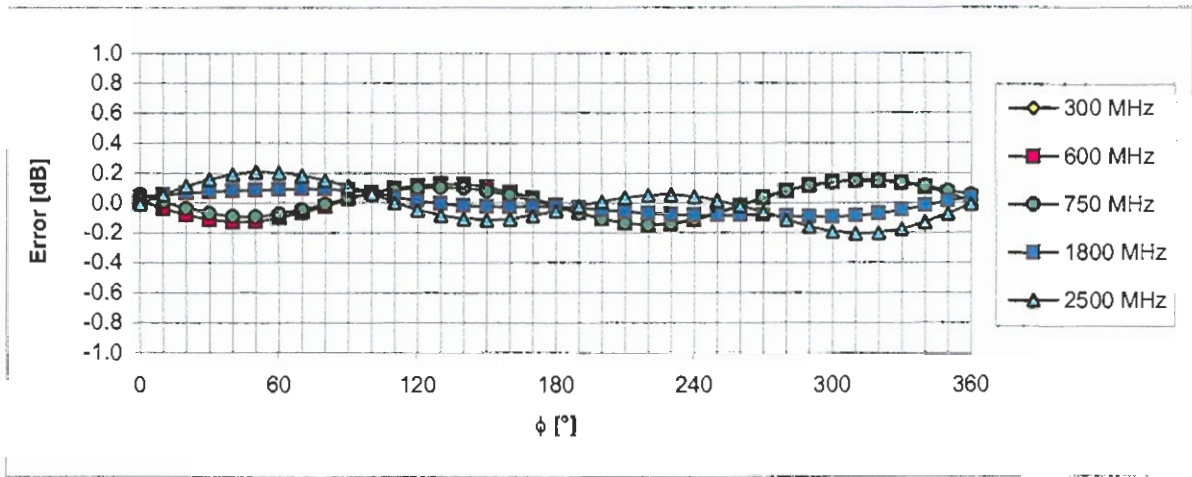


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

Receiving Pattern ( $\phi$ ),  $\vartheta = 0^\circ$

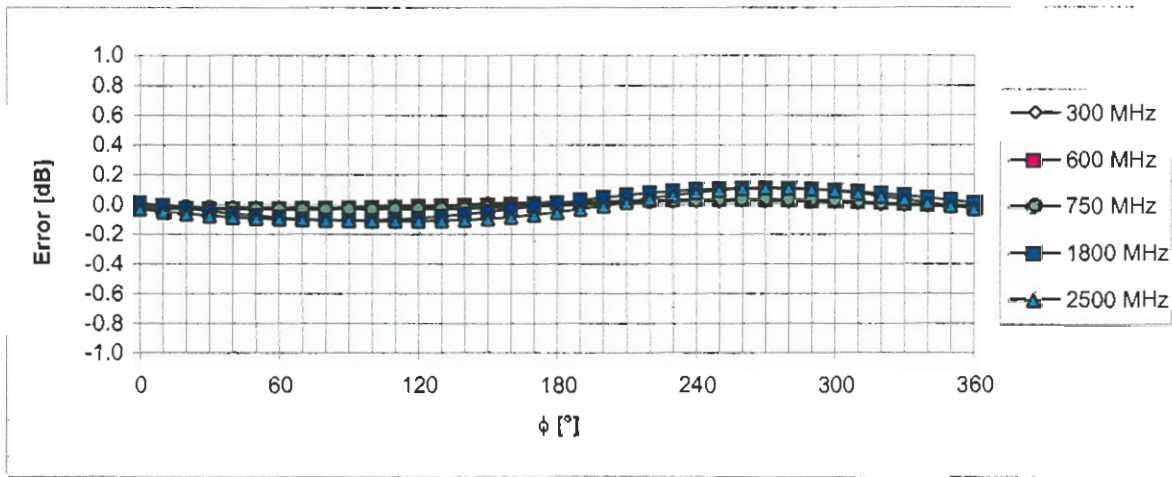

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

Dynamic Range f(H-field)  
(Waveguide R22, f = 1800 MHz)

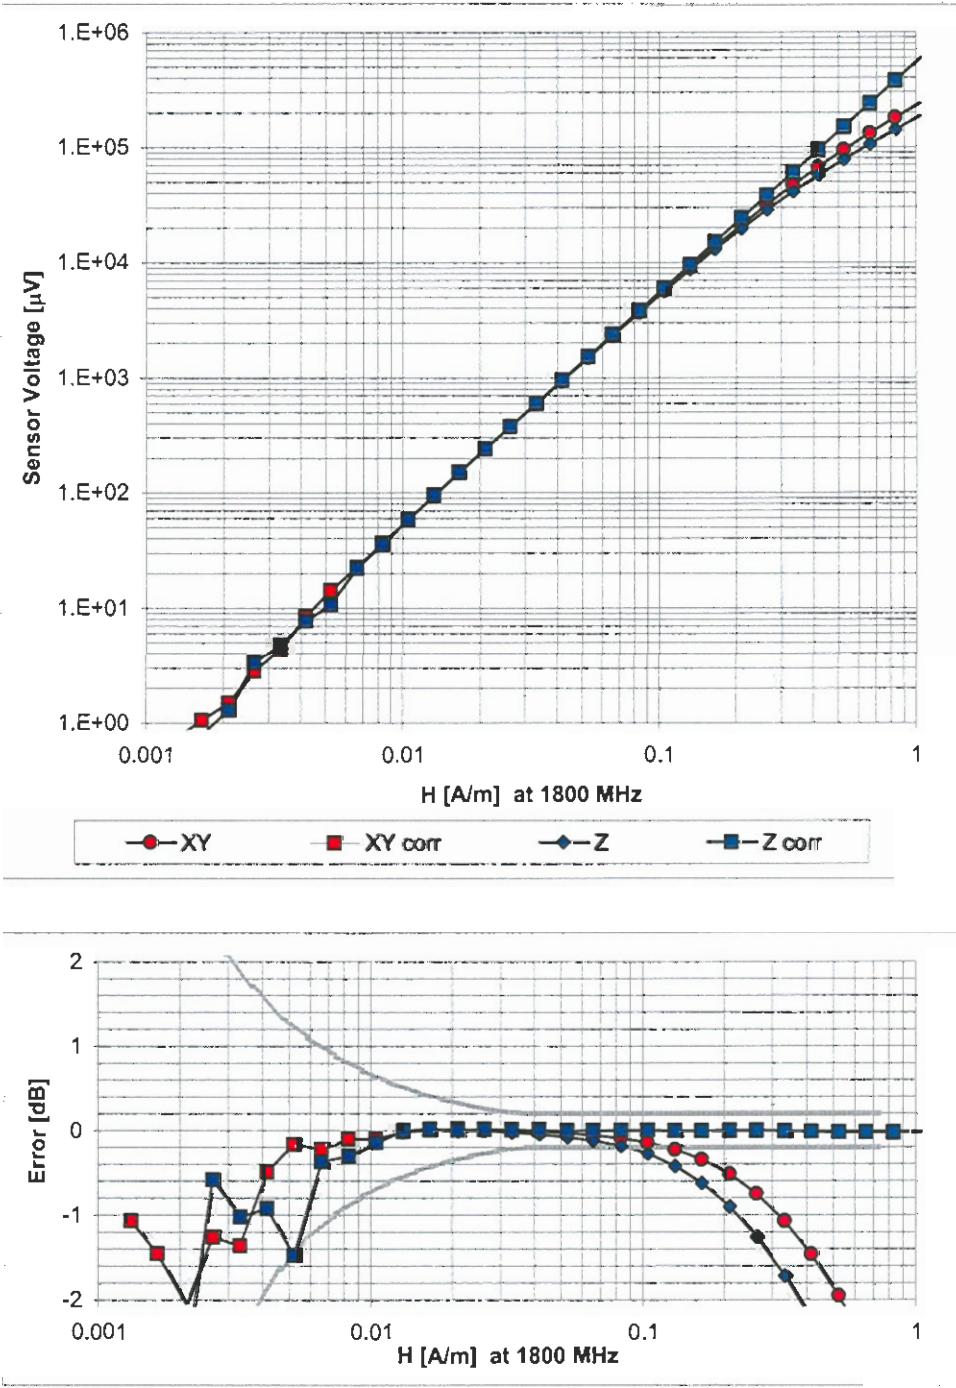

Uncertainty of Linearity Assessment:  $\pm 0.6\%$  (k=2)