

---

## APPENDIX B EUT TEST POSITION PHOTOS

---

### Liquid depth $\geq 15\text{cm}$

Phantom: SAM (30deg probe tilt) with CRP v5.0\_20150321; Type: QD000P40CD; Serial: TP:1874




**Head Left Cheek Setup Photo**




**Head Left Tilt Setup Photo**



**Head Right Cheek Setup Photo**

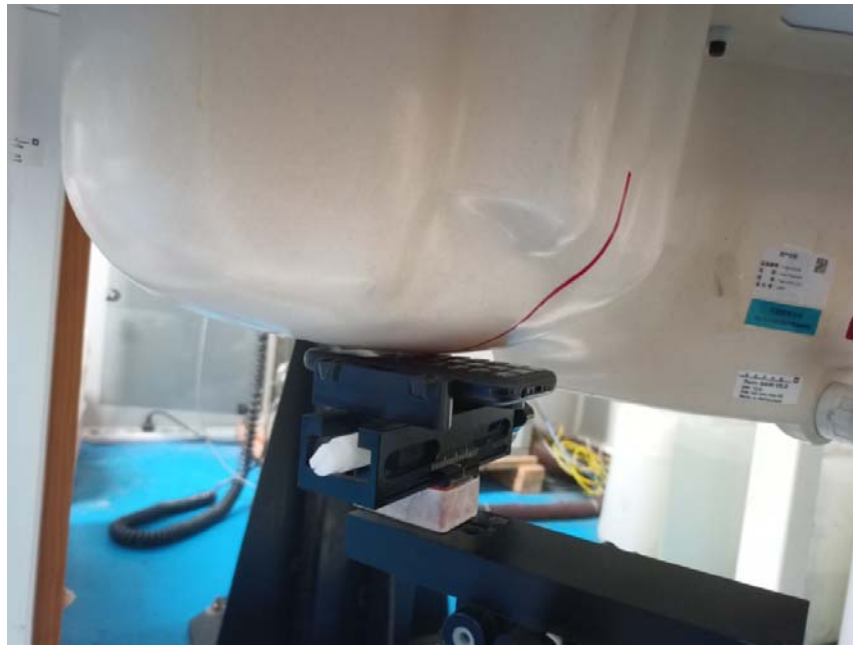

**Head Right Tilt Setup Photo**

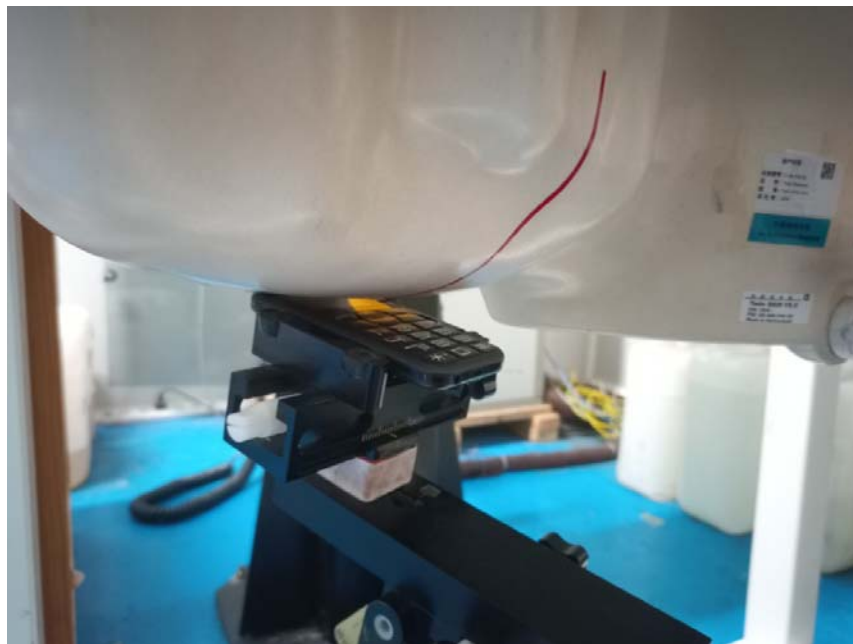

**Body (Worn) Back Setup Photo (5mm)**



**Body (Worn) Front Setup Photo (5mm)**



**Body Bottom Setup Photo (5mm)**

