

## TEST REPORT

Test Report No.: 1-1775-01-14/09



### Testing Laboratory

**CETECOM ICT Services GmbH**  
Untertürkheimer Straße 6 – 10  
66117 Saarbrücken/Germany  
Phone: + 49 681 5 98 - 0  
Fax: + 49 681 5 98 - 9075  
Internet: <http://www.cetecom-ict.de>  
e-mail: [info@ict.cetecom.de](mailto:info@ict.cetecom.de)

**Accredited Test Laboratory:**  
The test laboratory (area of testing) is accredited according to DIN EN ISO/IEC 17025

DAR registration number: DGA-PL-176/94-D1

### Applicant

**Philips Medizin Systeme Böblingen GmbH**  
Hewlett-Packard-Strasse 2  
71034 Böblingen/GERMANY

Phone:

Contact: Markus Stacha  
e-mail: [markus.stacha@philips.com](mailto:markus.stacha@philips.com)  
Phone: +49-7031-463-2840  
Fax: +49-7031-463 2442

### Manufacturer

**Philips Medizin Systeme Böblingen GmbH**  
Hewlett-Packard-Strasse 2  
71034 Böblingen/GERMANY

### Test Standard/s

|                              |   |
|------------------------------|---|
| IEEE 1528-2003               | Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques |
| OET Bulletin 65 Supplement C | Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields   |
| RSS-102 Issue 4              | Radio Frequency Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands)   |

For further applied test standards please refer to section 3 of this test report.

### Test Item

|                      |   |
|----------------------|---|
| Kind of test item:   | Components of IntelliVue Cableless Measurement System |
| Device type:         | portable device                                       |
| <b>Model name:</b>   | <b>IntelliVue CL with 3002-66480 WLAN module</b>      |
| S/N serial number:   | PN: 865221 / DE932Y0107                               |
| FCC-ID:              | PQC-WLANBV1   |
| IC:                  | 3549C-WLANBV1   |
| Hardware status:     | 0839 (for details see chapter 2.4)                    |
| Software status:     | ART6000 v1.0.9 (for details see chapter 2.4)          |
| Frequency:           | see technical details                                 |
| Antenna:             | integrated PCB antenna (for details see chapter 2.4)  |
| Battery option:      | ---   |
| Auxiliary equipment: | Laptop computer with Atheros control software         |
| Test sample status:  | identical prototype                                   |
| Exposure category:   | general population / uncontrolled environment         |

**Test performed:**

2010-09-09 Oleksandr Hnatovskiy

**Test Report authorised:**

2010-09-09 Thomas Vogler

|                 |  |           |
|-----------------|--|-----------|
| <b>1</b>        | <b>Table of contents</b>   |           |
| <b>1</b>        | <b>Table of contents</b>   | <b>2</b>  |
| <b>2</b>        | <b>General information</b>                                       | <b>3</b>  |
| 2.1             | Notes  | 3         |
| 2.2             | Application details  | 3         |
| 2.3             | Statement of compliance  | 3         |
| 2.4             | Technical details  | 4         |
| <b>3</b>        | <b>Test standard/s:</b>  | <b>5</b>  |
| 3.1             | RF exposure limits   | 5         |
| <b>4</b>        | <b>Summary of Measurement Results</b>                            | <b>6</b>  |
| <b>5</b>        | <b>Test Environment</b>  | <b>6</b>  |
| <b>6</b>        | <b>Test Set-up</b>   | <b>7</b>  |
| 6.1             | <b>Measurement system</b>  | <b>7</b>  |
| 6.1.1           | System Description   | 7         |
| 6.1.2           | Test environment   | 8         |
| 6.1.3           | Probe description  | 8         |
| 6.1.4           | Phantom description  | 9         |
| 6.1.5           | Device holder description  | 9         |
| 6.1.6           | Scanning procedure   | 10        |
| 6.1.7           | Spatial Peak SAR Evaluation                                      | 11        |
| 6.1.8           | Data Storage and Evaluation                                      | 12        |
| 6.1.9           | Tissue simulating liquids: dielectric properties                 | 14        |
| 6.1.10          | Tissue simulating liquids: parameters                            | 14        |
| 6.1.11          | Measurement uncertainty evaluation for SAR test                  | 15        |
| 6.1.12          | Measurement uncertainty evaluation for SAR test > 3 GHz          | 16        |
| 6.1.13          | Measurement uncertainty evaluation for system validation         | 17        |
| 6.1.14          | Measurement uncertainty evaluation for system validation > 3 Ghz | 18        |
| 6.1.15          | System validation  | 19        |
| 6.1.16          | Validation procedure   | 20        |
| <b>7</b>        | <b>Detailed Test Results</b>                                     | <b>21</b> |
| 7.1             | <b>Conducted power measurements WLAN</b>                         | <b>21</b> |
| 7.2             | <b>SAR test results</b>  | <b>22</b> |
| 7.2.1           | Results overview   | 22        |
| 7.2.2           | General description of test procedures                           | 23        |
| <b>8</b>        | <b>Test equipment and ancillaries used for tests</b>             | <b>24</b> |
| <b>9</b>        | <b>Observations</b>  | <b>24</b> |
| <b>Annex A:</b> | <b>System performance verification</b>                           | <b>25</b> |
| <b>Annex B:</b> | <b>DASY4 measurement results</b>                                 | <b>29</b> |
| Annex B.1:      | WLAN 2450MHz   | 29        |
| Annex B.2:      | WLAN 5GHz  | 36        |
| Annex B.3:      | Z-axis scan  | 44        |
| <b>Annex C:</b> | <b>Photo documentation</b>                                       | <b>45</b> |
| Annex C.4:      | Liquid depth   | 48        |
| <b>Annex D:</b> | <b>RF Technical Brief Cover Sheet acc. to RSS-102 Annex A</b>    | <b>49</b> |

Annex D.5: Declaration of RF Exposure Compliance.....49  
 Annex E: Calibration parameters.....50  
 Annex F: Document History.....50  
 Annex G: Further Information .....50

**2 General information**

**2.1 Notes**

The test results of this test report relate exclusively to the test item specified in this test report. CETECOM ICT Services GmbH does not assume responsibility for any conclusions and generalisations drawn from the test results with regard to other specimens or samples of the type of the equipment represented by the test item. The test report may only be reproduced or published in full. Reproduction or publication of extracts from the report requires the prior written approval of CETECOM ICT Services GmbH.

**2.2 Application details**

Date of receipt of order: 2009-11-18  
 Date of receipt of test item: 2010-04-26  
 Start of test: 2010-04-28  
 End of test: 2010-04-30  
 Person(s) present during the test:

**2.3 Statement of compliance**

The SAR values found for the IntelliVue CL with 3002-66480 WLAN module are below the maximum recommended levels of 1.6 W/Kg as averaged over any 1 g tissue according to the FCC rule §2.1093, the ANSI/IEEE C 95.1:1999, the NCRP Report Number 86 for uncontrolled environment, according to the Health Canada's Safety Code 6 and the Industry Canada Radio Standards Specification RSS-102 for General Population/Uncontrolled exposure.

For body worn operation, this device has been tested and meets FCC RF exposure guidelines when used in standard configuration with rear side towards the body without any distance or used with any accessory that contains no metal and that positions the front side of the device a minimum of 10 mm from the body. Use of other accessories may not ensure compliance with FCC RF exposure guidelines.

## 2.4 Technical details

| Band tested for this SAR test report | Technology | Frequency band | Lowest transmit frequency/MHz | Highest transmit frequency/MHz | Lowest receive Frequency/MHz | Highest receive Frequency/MHz | Kind of modulation | Power Class | Tested power control level | Test channel low | Test channel middle | Test channel high | Maximum output power/dBm )* |
|--------------------------------------|------------|----------------|-------------------------------|--------------------------------|------------------------------|-------------------------------|--------------------|-------------|----------------------------|------------------|---------------------|-------------------|-----------------------------|
| <input type="checkbox"/>             | WLAN       | ISM            | 2412                          | 2472                           | 2412                         | 2472                          | CCK OFDM           | --          | max                        | 1                | 7                   | 13                | --                          |
| <input checked="" type="checkbox"/>  | WLAN US    | ISM            | 2412                          | 2462                           | 2412                         | 2462                          | CCK OFDM           | --          | max                        | 1                | 6                   | 11                | 19.3                        |
| <input checked="" type="checkbox"/>  | WLAN       | ISM            | 5180                          | 5240                           | 5180                         | 5240                          | OFDM               | --          | max                        | 36               | --                  | 48                | 12.8                        |
| <input checked="" type="checkbox"/>  | WLAN       | ISM            | 5260                          | 5320                           | 5260                         | 5320                          | OFDM               | --          | max                        | 52               | --                  | 64                | 16.9                        |
| <input checked="" type="checkbox"/>  | WLAN       | ISM            | 5745                          | 5825                           | 5745                         | 5825                          | OFDM               | --          | max                        | 149              | 157                 | 165               | 20.6                        |
| <input type="checkbox"/>             | SRR        | ISM            | 2412                          | 2462                           | 2412                         | 2462                          | DSSS               | --          | max                        | --               | --                  | --                | -2.8                        |

)\*: averaged max. RMS power for UMTS, WLAN and BT.

Note : SRR (Short Range Radio) was not tested for SAR (output power < 60/f mW)

Hard- and Software Status from all components:

| Description  | Partnumber   | HW-Status              | SW-Status      |
|--------------|--------------|------------------------|----------------|
| Mainboard    | 453564118401 | 0939                   | A.00.30        |
| WLAN Module  | M3002-66480  | 0839                   | ART6000 v1.0.9 |
| WLAN Antenna | 453564175981 | 0933, modified to 1011 | -              |

### 3 Test standard/s:

| Test Standard                   | Version            | Test Standard Description   |
|---------------------------------|--------------------|---|
| IEEE 1528-2003                  | 2003-04            | Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques |
| OET Bulletin 65<br>Supplement C | 1997-01<br>2001-01 | Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields   |
| RSS-102 Issue 4                 | 2010-03            | Radio Frequency Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands)   |
| Canada's Safety Code No. 6      | 99-EHD-237         | Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3 kHz to 300 GHz  |
| IEEE Std. C95-3                 | 1991               | Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields – RF and Microwave   |
| IEEE Std. C95-1                 | 1999               | Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields   |

#### 3.1 RF exposure limits

| Human Exposure                                  | Uncontrolled Environment<br>General Population | Controlled Environment<br>Occupational |
|---|--|--|
| Spatial Peak SAR*<br>(Brain)                    | <b>1.60 mW/g</b>                               | 8.00 mW/g                              |
| Spatial Average SAR**<br>(Whole Body)           | 0.08 mW/g                                      | 0.40 mW/g                              |
| Spatial Peak SAR***<br>(Hands/Feet/Ankle/Wrist) | 4.00 mW/g                                      | 20.00 mW/g                             |

Table 1: RF exposure limits

The limit applied in this test report is shown in bold letters

Notes:

\* The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time

\*\* The Spatial Average value of the SAR averaged over the whole body.

\*\*\* The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure.

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation).

#### 4 Summary of Measurement Results

|                                     |  |
|-------------------------------------|--|
| <input checked="" type="checkbox"/> | <b>No deviations from the technical specifications ascertained</b> |
| <input type="checkbox"/>            | Deviations from the technical specifications ascertained           |

#### 5 Test Environment


|                            |                                       |
|----------------------------|---------------------------------------|
| Ambient temperature:       | 20 – 24 °C                            |
| Tissue Simulating liquid:  | 20 – 24 °C                            |
| Relative humidity content: | 40 – 50 %                             |
| Air pressure:              | not relevant for this kind of testing |
| Power supply:              | 230 V / 50 Hz                         |

Exact temperature values for each test are shown in the table(s) under 2.5. and/or on the measurement plots.

## 6 Test Set-up

### 6.1 Measurement system

#### 6.1.1 System Description

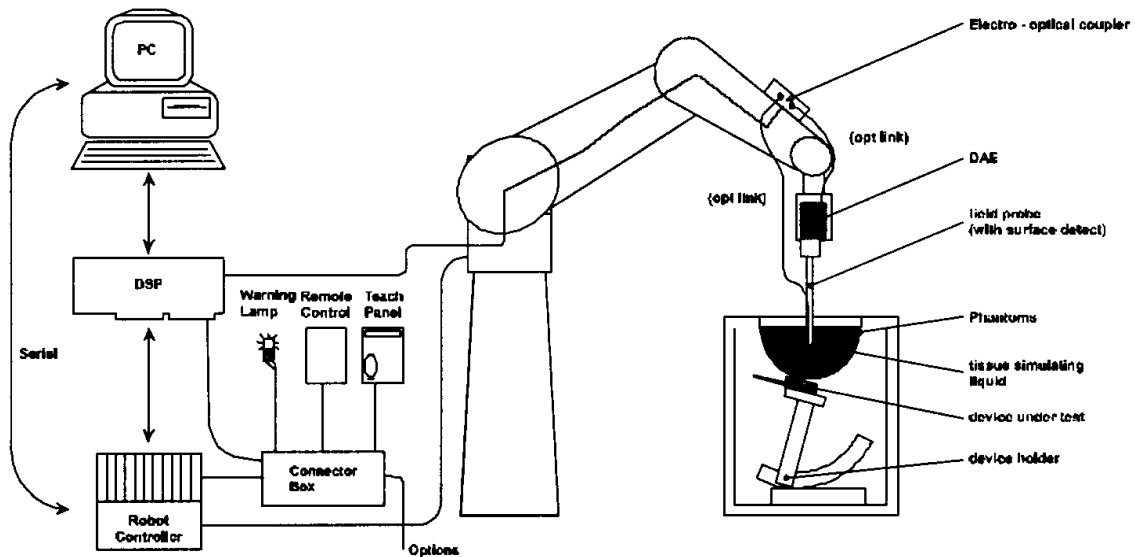

- The DAS4 system for performing compliance tests consists of the following items:
- A standard high precision 6-axis robot (Stäubli RX family) with controller and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e. an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronic (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- A unit to operate the optical surface detector which is connected to the EOC.
- The Electro-Optical Coupler (EOC) performs the conversion from the optical into a digital electric signal of the DAE. The EOC is connected to the DAS4 measurement server.
- The DAS4 measurement server, which performs all real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operation. A computer operating Windows 2000
- DAS4 software and SEMCAD data evaluation software.
- Remote control with teach panel and additional circuitry for robot safety such as warning lamps, etc.
- The generic twin phantom enabling the testing of left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- System validation dipoles allowing to validate the proper functioning of the system.

### 6.1.2 Test environment

The DASY4 measurement system is placed at the head end of a room with dimensions: 5 x 2.5 x 3 m<sup>3</sup>, the SAM phantom is placed in a distance of 75 cm from the side walls and 1.1m from the rear wall. Above the test system a 1.5 x 1.5 m<sup>2</sup> array of pyramid absorbers is installed to reduce reflections from the ceiling.

Picture 1 of the photo documentation shows a complete view of the test environment.

The system allows the measurement of SAR values larger than 0.005 mW/g.

### 6.1.3 Probe description

Isotropic E-Field Probe ET3DV6 for Dosimetric Measurements


| Technical data according to manufacturer information |  |
|--|--|
| Construction   | Symmetrical design with triangular core<br>Built-in optical fiber for surface detection system<br>Built-in shielding against static charges<br>PEEK enclosure material (resistant to organic solvents, e.g., glycoether) |
| Calibration  | In air from 10 MHz to 2.5 GHz<br>In head tissue simulating liquid (HSL) at 900 (800-1000) MHz and 1.8 GHz (1700-1910 MHz) (accuracy $\pm 9.5\%$ ; $k=2$ ) Calibration for other liquids and frequencies upon request     |
| Frequency  | 10 MHz to 3 GHz (dosimetry); Linearity: $\pm 0.2$ dB (30 MHz to 3 GHz)   |
| Directivity  | $\pm 0.2$ dB in HSL (rotation around probe axis)<br>$\pm 0.4$ dB in HSL (rotation normal to probe axis)  |
| Dynamic range  | 5 $\mu$ W/g to > 100 mW/g; Linearity: $\pm 0.2$ dB   |
| Optical Surface Detection                            | $\pm 0.2$ mm repeatability in air and clear liquids over diffuse reflecting surfaces (ET3DV6 only)   |
| Dimensions   | Overall length: 330 mm<br>Tip length: 16 mm<br>Body diameter: 12 mm<br>Tip diameter: 6.8 mm<br>Distance from probe tip to dipole centers: 2.7 mm   |
| Application  | General dosimetry up to 3 GHz<br>Compliance tests of mobile phones<br>Fast automatic scanning in arbitrary phantoms (ET3DV6)   |



#### 6.1.4 Phantom description

The used SAM Phantom meets the requirements specified in Edition 01-01 of Supplement C to OET Bulletin 65 for Specific Absorption Rate (SAR) measurements.

The phantom consists of a fibreglass shell integrated in a wooden table. It allows left-hand and right-hand head as well as body-worn measurements with a maximum liquid depth of 18 cm in head position and 22 cm in planar position (body measurements). The thickness of the Phantom shell is 2 mm +/- 0.1 mm.

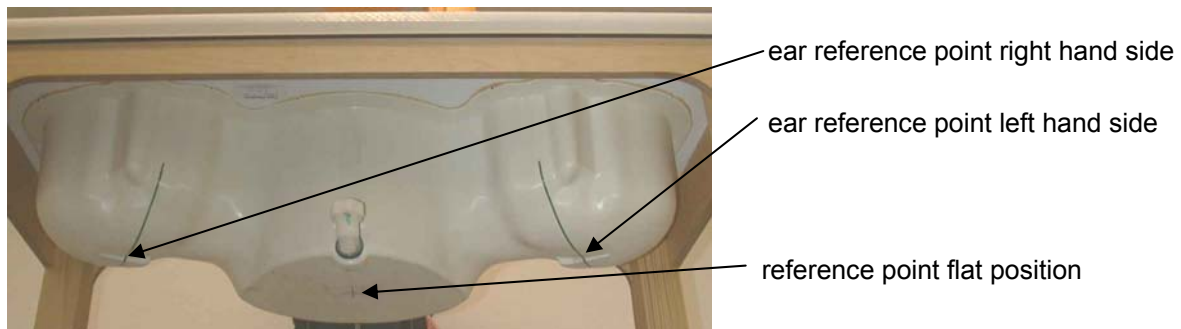

#### 6.1.5 Device holder description

The DASY4 device holder has two scales for device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear openings). The plane between the ear openings and the mouth tip has a rotation angle of 65°. The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. This device holder is used for standard mobile phones or PDA's only. If necessary an additional support of polystyrene material is used.



Larger DUT's (e.g. notebooks) cannot be tested using this device holder. Instead a support of bigger polystyrene cubes and thin polystyrene plates is used to position the DUT in all relevant positions to find and measure spots with maximum SAR values.

Therefore those devices are normally only tested at the flat part of the SAM.

### 6.1.6 Scanning procedure

- The DASY4 installation includes predefined files with recommended procedures for measurements and validation. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.
- The „reference“ and „drift“ measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT's output power and should vary max. +/- 5 %.
- The „surface check“ measurement tests the optical surface detection system of the DASY4 system by repeatedly detecting the surface with the optical and mechanical surface detector and comparing the results. The output gives the detecting heights of both systems, the difference between the two systems and the standard deviation of the detection repeatability. Air bubbles or refraction in the liquid due to separation of the sugar-water mixture gives poor repeatability (above  $\pm 0.1\text{mm}$ ). To prevent wrong results tests are only executed when the liquid is free of air bubbles. The difference between the optical surface detection and the actual surface depends on the probe and is specified with each probe. (It does not depend on the surface reflectivity or the probe angle to the surface within  $\pm 30^\circ$ .)
- The „area scan“ measures the SAR above the DUT or verification dipole on a parallel plane to the surface. It is used to locate the approximate location of the peak SAR with 2D spline interpolation. The robot performs a stepped movement along one grid axis while the local electrical field strength is measured by the probe. The probe is touching the surface of the SAM during acquisition of measurement values. The standard scan uses large grid spacing for faster measurement. Standard grid spacing for head measurements is 15 mm in x- and y- dimension. If a finer resolution is needed, the grid spacing can be reduced. Grid spacing and orientation have no influence on the SAR result. For special applications where the standard scan method does not find the peak SAR within the grid, e.g. mobile phones with flip cover, the grid can be adapted in orientation. Results of this coarse scan are shown in annex 2.
- A „7x7x7 zoom scan“ measures the field in a volume around the 2D peak SAR value acquired in the previous „coarse“ scan. This is a fine 7x7 grid where the robot additionally moves the probe in 7 steps along the z-axis away from the bottom of the Phantom. Grid spacing for the cube measurement is 5 mm in x and y-direction and 5 mm in z-direction. DASY4 is also able to perform repeated zoom scans if more than 1 peak is found during area scan. In this document, the evaluated peak 1g and 10g averaged SAR values are shown in the 2D-graphics in annex 2. Test results relevant for the specified standard (see section 3) are shown in table form in section 7.
- A Z-axis scan measures the total SAR value at the x-and y-position of the maximum SAR value found during the cube 7x7x7 scan. The probe is moved away in z-direction from the bottom of the SAM phantom in 2mm steps. This measurement shows the continuity of the liquid and can - depending in the field strength – also show the liquid depth. A z-axis scan of the measurement with maximum SAR value is shown in annex 2.

### 6.1.7 Spatial Peak SAR Evaluation

The spatial peak SAR - value for 1 and 10 g is evaluated after the Cube measurements have been done. The basis of the evaluation are the SAR values measured at the points of the fine cube grid consisting of 7 x 7 x 7 points. The algorithm that finds the maximal averaged volume is separated into three different stages.

- The data between the dipole center of the probe and the surface of the phantom are extrapolated. This data cannot be measured since the center of the dipole is 2.7 mm away from the tip of the probe and the distance between the surface and the lowest measuring point is about 1 mm (see probe calibration sheet). The extrapolated data from a cube measurement can be visualized by selecting 'Graph Evaluated'.
- The maximum interpolated value is searched with a straight-forward algorithm. Around this maximum the SAR - values averaged over the spatial volumes (1g or 10 g) are computed using the 3d-spline interpolation algorithm. If the volume cannot be evaluated (i.e., if a part of the grid was cut off by the boundary of the measurement area) the evaluation will be started on the corners of the bottom plane of the cube.
- All neighboring volumes are evaluated until no neighboring volume with a higher average value is found.

#### Extrapolation

The extrapolation is based on a least square algorithm [W. Gander, Computermathematik, p.168-180]. Through the points in the first 3 cm along the z-axis, polynomials of order four are calculated. These polynomials are then used to evaluate the points between the surface and the probe tip. The points, calculated from the surface, have a distance of 1 mm from each other.

#### Interpolation

The interpolation of the points is done with a 3d-Spline. The 3d-Spline is composed of three one-dimensional splines with the "Not a knot"-condition [W. Gander, Computermathematik, p.141-150] (x, y and z -direction) [Numerical Recipes in C, Second Edition, p.123ff ].

#### Volume Averaging

At First the size of the cube is calculated. Then the volume is integrated with the trapezoidal algorithm. 8000 points (20x20x20) are interpolated to calculate the average.

#### Advanced Extrapolation

DASY4 uses the advanced extrapolation option which is able to compensate boundary effects on E-field probes.

## 6.1.8 Data Storage and Evaluation

### Data Storage

The DASY4 software stores the acquired data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension ".DA4". The software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of incorrect parameter settings. For example, if a measurement has been performed with a wrong crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be re-evaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type ([V/m], [A/m], [°C], [mW/g], [mW/cm<sup>2</sup>], [dBrel], etc.). Some of these units are not available in certain situations or show meaningless results, e.g., a SAR output in a lossless media will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

### Data Evaluation by SEMCAD

The SEMCAD software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

|                    |                           |   |
|--------------------|---------------------------|---|
| Probe parameters:  | - Sensitivity             | Norm <sub>i</sub> , a <sub>i0</sub> , a <sub>i1</sub> , a <sub>i2</sub> |
|                    | - Conversion factor       | ConvF <sub>i</sub>  |
|                    | - Diode compression point | Dcpi  |
| Device parameters: | - Frequency               | f   |
|                    | - Crest factor            | cf  |
| Media parameters:  | - Conductivity            | $\sigma$  |
|                    | - Density                 | $\rho$  |

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY4 components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics.

If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot cf/dcp_i$$

with  $V_i$  = compensated signal of channel i (i = x, y, z)  
 $U_i$  = input signal of channel i (i = x, y, z)  
 cf = crest factor of exciting field (DASY parameter)  
 $dcp_i$  = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes:  $E_i = (V_i / Norm_i \cdot ConvF)^{1/2}$

H-field probes:  $H_i = (V_i)^{1/2} \cdot (a_{i0} + a_{i1}f + a_{i2}f^2)/f$

with  $V_i$  = compensated signal of channel i (i = x, y, z)  
 $Norm_i$  = sensor sensitivity of channel i (i = x, y, z)  
 [mV/(V/m)<sup>2</sup>] for E-field Probes  
 $ConvF$  = sensitivity enhancement in solution  
 $a_{ij}$  = sensor sensitivity factors for H-field probes  
 $f$  = carrier frequency [GHz]  
 $E_i$  = electric field strength of channel i in V/m  
 $H_i$  = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = (E_x^2 + E_y^2 + E_z^2)^{1/2}$$

The primary field data are used to calculate the derived field units.

$$SAR = (E_{tot}^2 \cdot \sigma) / (\rho \cdot 1000)$$

with SAR = local specific absorption rate in mW/g  
 $E_{tot}$  = total field strength in V/m  
 $\sigma$  = conductivity in [mho/m] or [Siemens/m]  
 $\rho$  = equivalent tissue density in g/cm<sup>3</sup>

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid. The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = E_{tot}^2 / 3770 \quad \text{or} \quad P_{pwe} = H_{tot}^2 \cdot 37.7$$

with  $P_{pwe}$  = equivalent power density of a plane wave in mW/cm<sup>2</sup>  
 $E_{tot}$  = total electric field strength in V/m  
 $H_{tot}$  = total magnetic field strength in A/m

### 6.1.9 Tissue simulating liquids: dielectric properties

The following materials are used for producing the tissue-equivalent materials.

(Liquids used for tests described in section 7. are marked with ☒) :

| Ingredients<br>(% of weight) | Frequency (MHz) |         |
|------------------------------|-----------------|---------|
|                              | ☒ 2450          | ☒ 5000  |
| frequency band               | ☒ 2450          | ☒ 5000  |
| Tissue Type                  | Body            | Body    |
| Water                        | 73.2            | 64 - 78 |
| Salt (NaCl)                  | 0.04            | 2 - 3   |
| Sugar                        | 0.0             | 0.0     |
| HEC                          | 0.0             | 0.0     |
| Bactericide                  | 0.0             | 0.0     |
| Triton X-100                 | 0.0             | 0.0     |
| DGBE                         | 26.7            | 0.0     |
| Emulsifiers                  | 0.0             | 9 - 15  |
| Mineral Oil                  | 0.0             | 11 - 18 |

Table 2: Body tissue dielectric properties

Salt: 99+% Pure Sodium Chloride

Sugar: 98+% Pure Sucrose

Water: De-ionized, 16MΩ+ resistivity

HEC: Hydroxyethyl Cellulose

DGBE: 99+% Di(ethylene glycol) butyl ether, [2-(2-butoxyethoxy)ethanol]

Triton X-100(ultra pure): Polyethylene glycol mono [4-(1,1,3,3-tetramethylbutyl)phenyl]ether

Note: Due to their availability body tissue simulating liquids as defined by FCC OET Bulletin 65 Supplement C are generally used for body worn SAR testing according to European standards.

### 6.1.10 Tissue simulating liquids: parameters

| Used Target<br>Frequency<br>[MHz] | Target<br>Body Tissue |                       | Measured<br>Body Tissue |                       | Measured Date |
|-----------------------------------|-----------------------|-----------------------|-------------------------|-----------------------|---------------|
|                                   | Permittivity          | Conductivity<br>[S/m] | Permittivity            | Conductivity<br>[S/m] |               |
| 2450                              | 52.7                  | 1.95                  | 51.9                    | 1.99                  | 2010-04-28    |
| 5200                              | 49.0                  | 5.30                  | 48.0                    | 5.34                  | 2010-04-29    |
| 5320                              | 49.0                  | 5.30                  | 47.8                    | 5.46                  | 2010-04-29    |
| 5500                              | 48.2                  | 6.00                  | 47.3                    | 5.71                  | 2010-04-29    |
| 5745                              | 48.2                  | 6.00                  | 46.8                    | 5.99                  | 2010-04-29    |
| 5800                              | 48.2                  | 6.00                  | 46.7                    | 6.10                  | 2010-04-29    |

Table 3: Parameter of the body tissue simulating liquid

Note: The dielectric properties have been measured using the contact probe method at 22°C.

### 6.1.11 Measurement uncertainty evaluation for SAR test

The overall combined measurement uncertainty of the measurement system is  $\pm 10.3\%$  ( $K=1$ ).

The expanded uncertainty ( $k=2$ ) is assessed to be  $\pm 20.6\%$

This measurement uncertainty budget is suggested by IEEE 1528-2003 and determined by Schmid & Partner Engineering AG. The breakdown of the individual uncertainties is as follows:

| Error Sources                    | Uncertainty Value | Probability Distribution | Divisor    | $c_i$ 1g | $c_i$ 10g | Standard Uncertainty 1g | Standard Uncertainty 10g | $v_i^2$ or $v_{\text{eff}}$ |
|----------------------------------|-------------------|--------------------------|------------|----------|-----------|-------------------------|--------------------------|-----------------------------|
| <b>Measurement System</b>        |                   |                          |            |          |           |                         |                          |                             |
| Probe calibration                | $\pm 4.8\%$       | Normal                   | 1          | 1        | 1         | $\pm 4.8\%$             | $\pm 4.8\%$              | $\infty$                    |
| Axial isotropy                   | $\pm 4.7\%$       | Rectangular              | $\sqrt{3}$ | 0.7      | 0.7       | $\pm 1.9\%$             | $\pm 1.9\%$              | $\infty$                    |
| Hemispherical isotropy           | $\pm 9.6\%$       | Rectangular              | $\sqrt{3}$ | 0.7      | 0.7       | $\pm 3.9\%$             | $\pm 3.9\%$              | $\infty$                    |
| Spatial resolution               | $\pm 0.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.0\%$             | $\pm 0.0\%$              | $\infty$                    |
| Boundary effects                 | $\pm 1.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.6\%$             | $\pm 0.6\%$              | $\infty$                    |
| Probe linearity                  | $\pm 4.7\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 2.7\%$             | $\pm 2.7\%$              | $\infty$                    |
| System detection limits          | $\pm 1.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.6\%$             | $\pm 0.6\%$              | $\infty$                    |
| Readout electronics              | $\pm 1.0\%$       | Normal                   | 1          | 1        | 1         | $\pm 1.0\%$             | $\pm 1.0\%$              | $\infty$                    |
| Response time                    | $\pm 0.8\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.5\%$             | $\pm 0.5\%$              | $\infty$                    |
| Integration time                 | $\pm 2.6\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 1.5\%$             | $\pm 1.5\%$              | $\infty$                    |
| RF ambient conditions            | $\pm 3.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 1.7\%$             | $\pm 1.7\%$              | $\infty$                    |
| Probe positioner                 | $\pm 0.4\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.2\%$             | $\pm 0.2\%$              | $\infty$                    |
| Probe positioning                | $\pm 2.9\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 1.7\%$             | $\pm 1.7\%$              | $\infty$                    |
| Max. SAR evaluation              | $\pm 1.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.6\%$             | $\pm 0.6\%$              | $\infty$                    |
| <b>Test Sample Related</b>       |                   |                          |            |          |           |                         |                          |                             |
| Device positioning               | $\pm 2.9\%$       | Normal                   | 1          | 1        | 1         | $\pm 2.9\%$             | $\pm 2.9\%$              | 145                         |
| Device holder uncertainty        | $\pm 3.6\%$       | Normal                   | 1          | 1        | 1         | $\pm 3.6\%$             | $\pm 3.6\%$              | 5                           |
| Power drift                      | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 2.9\%$             | $\pm 2.9\%$              | $\infty$                    |
| <b>Phantom and Set-up</b>        |                   |                          |            |          |           |                         |                          |                             |
| Phantom uncertainty              | $\pm 4.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 2.3\%$             | $\pm 2.3\%$              | $\infty$                    |
| Liquid conductivity (target)     | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 0.64     | 0.43      | $\pm 1.8\%$             | $\pm 1.2\%$              | $\infty$                    |
| Liquid conductivity (meas.)      | $\pm 2.5\%$       | Normal                   | 1          | 0.64     | 0.43      | $\pm 1.6\%$             | $\pm 1.1\%$              | $\infty$                    |
| Liquid permittivity (target)     | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 0.6      | 0.49      | $\pm 1.7\%$             | $\pm 1.4\%$              | $\infty$                    |
| Liquid permittivity (meas.)      | $\pm 2.5\%$       | Normal                   | 1          | 0.6      | 0.49      | $\pm 1.5\%$             | $\pm 1.2\%$              | $\infty$                    |
| <b>Combined Uncertainty</b>      |                   |                          |            |          |           | $\pm 10.3\%$            | $\pm 10.0\%$             | 330                         |
| <b>Expanded Std. Uncertainty</b> |                   |                          |            |          |           | $\pm 20.6\%$            | $\pm 20.1\%$             |                             |

Table 4: Measurement uncertainties

### 6.1.12 Measurement uncertainty evaluation for SAR test > 3 GHz

The overall combined measurement uncertainty of the measurement system is  $\pm 11.5\%$  ( $K=1$ ).  
 The expanded uncertainty ( $k=2$ ) is assessed to be  $\pm 23.0\%$   
 This measurement uncertainty budget is suggested by IEEE 1528-2003 and determined by Schmid & Partner Engineering AG. The breakdown of the individual uncertainties is as follows:

| Error Sources                    | Uncertainty Value | Probability Distribution | Divisor    | $c_i$ 1g | $c_i$ 10g | Standard Uncertainty 1g | Standard Uncertainty 10g | $v_i^2$ or $v_{eff}$ |
|----------------------------------|-------------------|--------------------------|------------|----------|-----------|-------------------------|--------------------------|----------------------|
| <b>Measurement System</b>        |                   |                          |            |          |           |                         |                          |                      |
| Probe calibration                | $\pm 6.3\%$       | Normal                   | 1          | 1        | 1         | $\pm 6.3\%$             | $\pm 6.3\%$              | $\infty$             |
| Axial isotropy                   | $\pm 4.7\%$       | Rectangular              | $\sqrt{3}$ | 0.7      | 0.7       | $\pm 1.9\%$             | $\pm 1.9\%$              | $\infty$             |
| Hemispherical isotropy           | $\pm 9.6\%$       | Rectangular              | $\sqrt{3}$ | 0.7      | 0.7       | $\pm 3.9\%$             | $\pm 3.9\%$              | $\infty$             |
| Spatial resolution               | $\pm 0.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.0\%$             | $\pm 0.0\%$              | $\infty$             |
| Boundary effects                 | $\pm 2.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 1.2\%$             | $\pm 1.2\%$              | $\infty$             |
| Probe linearity                  | $\pm 4.7\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 2.7\%$             | $\pm 2.7\%$              | $\infty$             |
| System detection limits          | $\pm 1.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.6\%$             | $\pm 0.6\%$              | $\infty$             |
| Readout electronics              | $\pm 1.0\%$       | Normal                   | 1          | 1        | 1         | $\pm 1.0\%$             | $\pm 1.0\%$              | $\infty$             |
| Response time                    | $\pm 0.8\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.5\%$             | $\pm 0.5\%$              | $\infty$             |
| Integration time                 | $\pm 2.6\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 1.5\%$             | $\pm 1.5\%$              | $\infty$             |
| RF ambient conditions            | $\pm 3.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 1.7\%$             | $\pm 1.7\%$              | $\infty$             |
| Probe positioner                 | $\pm 0.8\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.4\%$             | $\pm 0.4\%$              | $\infty$             |
| Probe positioning                | $\pm 5.8\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 3.4\%$             | $\pm 3.4\%$              | $\infty$             |
| Max. SAR evaluation              | $\pm 1.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.6\%$             | $\pm 0.6\%$              | $\infty$             |
| <b>Test Sample Related</b>       |                   |                          |            |          |           |                         |                          |                      |
| Device positioning               | $\pm 2.9\%$       | Normal                   | 1          | 1        | 1         | $\pm 2.9\%$             | $\pm 2.9\%$              | 145                  |
| Device holder uncertainty        | $\pm 3.6\%$       | Normal                   | 1          | 1        | 1         | $\pm 3.6\%$             | $\pm 3.6\%$              | 5                    |
| Power drift                      | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 2.9\%$             | $\pm 2.9\%$              | $\infty$             |
| <b>Phantom and Set-up</b>        |                   |                          |            |          |           |                         |                          |                      |
| Phantom uncertainty              | $\pm 4.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 2.3\%$             | $\pm 2.3\%$              | $\infty$             |
| Liquid conductivity (target)     | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 0.64     | 0.43      | $\pm 1.8\%$             | $\pm 1.2\%$              | $\infty$             |
| Liquid conductivity (meas.)      | $\pm 2.5\%$       | Normal                   | 1          | 0.64     | 0.43      | $\pm 1.6\%$             | $\pm 1.1\%$              | $\infty$             |
| Liquid permittivity (target)     | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 0.6      | 0.49      | $\pm 1.7\%$             | $\pm 1.4\%$              | $\infty$             |
| Liquid permittivity (meas.)      | $\pm 2.5\%$       | Normal                   | 1          | 0.6      | 0.49      | $\pm 1.5\%$             | $\pm 1.2\%$              | $\infty$             |
| <b>Combined Uncertainty</b>      |                   |                          |            |          |           | $\pm 11.5\%$            | $\pm 11.2\%$             | 330                  |
| <b>Expanded Std. Uncertainty</b> |                   |                          |            |          |           | $\pm 23.0\%$            | $\pm 22.5\%$             |                      |

Table 5: Measurement uncertainties



### 6.1.13 Measurement uncertainty evaluation for system validation

The overall combined measurement uncertainty of the measurement system is  $\pm 8.4\%$  ( $K=1$ ).  
 The expanded uncertainty ( $k=2$ ) is assessed to be  $\pm 16.8\%$   
 This measurement uncertainty budget is suggested by IEEE 1528-2003 and determined by Schmid & Partner Engineering AG. The breakdown of the individual uncertainties is as follows:

| Error Sources                    | Uncertainty Value | Probability Distribution | Divisor    | $c_i$ 1g | $c_i$ 10g | Standard Uncertainty 1g        | Standard Uncertainty 10g       | $v_i^2$ or $v_{eff}$ |
|----------------------------------|-------------------|--------------------------|------------|----------|-----------|--------------------------------|--------------------------------|----------------------|
| <b>Measurement System</b>        |                   |                          |            |          |           |                                |                                |                      |
| Probe calibration                | $\pm 4.8\%$       | Normal                   | 1          | 1        | 1         | $\pm 4.8\%$                    | $\pm 4.8\%$                    | $\infty$             |
| Axial isotropy                   | $\pm 4.7\%$       | Rectangular              | $\sqrt{3}$ | 0.7      | 0.7       | $\pm 1.9\%$                    | $\pm 1.9\%$                    | $\infty$             |
| Hemispherical isotropy           | $\pm 0.0\%$       | Rectangular              | $\sqrt{3}$ | 0.7      | 0.7       | $\pm 0.0\%$                    | $\pm 3.9\%$                    | $\infty$             |
| Boundary effects                 | $\pm 1.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.6\%$                    | $\pm 0.6\%$                    | $\infty$             |
| Probe linearity                  | $\pm 4.7\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 2.7\%$                    | $\pm 2.7\%$                    | $\infty$             |
| System detection limits          | $\pm 1.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.6\%$                    | $\pm 0.6\%$                    | $\infty$             |
| Readout electronics              | $\pm 1.0\%$       | Normal                   | 1          | 1        | 1         | $\pm 1.0\%$                    | $\pm 1.0\%$                    | $\infty$             |
| Response time                    | $\pm 0.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.0\%$                    | $\pm 0.0\%$                    | $\infty$             |
| Integration time                 | $\pm 0.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.0\%$                    | $\pm 0.0\%$                    | $\infty$             |
| RF ambient conditions            | $\pm 3.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 1.7\%$                    | $\pm 1.7\%$                    | $\infty$             |
| Probe positioner                 | $\pm 0.4\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.2\%$                    | $\pm 0.2\%$                    | $\infty$             |
| Probe positioning                | $\pm 2.9\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 1.7\%$                    | $\pm 1.7\%$                    | $\infty$             |
| Max. SAR evaluation              | $\pm 1.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.6\%$                    | $\pm 0.6\%$                    | $\infty$             |
| <b>Test Sample Related</b>       |                   |                          |            |          |           |                                |                                |                      |
| Dipole axis to liquid distance   | $\pm 2.0\%$       | Normal                   | 1          | 1        | 1         | $\pm 1.2\%$                    | $\pm 1.2\%$                    | $\infty$             |
| Power drift                      | $\pm 4.7\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 2.7\%$                    | $\pm 2.7\%$                    | $\infty$             |
| <b>Phantom and Set-up</b>        |                   |                          |            |          |           |                                |                                |                      |
| Phantom uncertainty              | $\pm 4.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 2.3\%$                    | $\pm 2.3\%$                    | $\infty$             |
| Liquid conductivity (target)     | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 0.64     | 0.43      | $\pm 1.8\%$                    | $\pm 1.2\%$                    | $\infty$             |
| Liquid conductivity (meas.)      | $\pm 2.5\%$       | Normal                   | 1          | 0.64     | 0.43      | $\pm 1.6\%$                    | $\pm 1.1\%$                    | $\infty$             |
| Liquid permittivity (target)     | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 0.6      | 0.49      | $\pm 1.7\%$                    | $\pm 1.4\%$                    | $\infty$             |
| Liquid permittivity (meas.)      | $\pm 2.5\%$       | Normal                   | 1          | 0.6      | 0.49      | $\pm 1.5\%$                    | $\pm 1.2\%$                    | $\infty$             |
| <b>Combined Uncertainty</b>      |                   |                          |            |          |           | <b><math>\pm 8.4\%</math></b>  | <b><math>\pm 8.1\%</math></b>  |                      |
| <b>Expanded Std. Uncertainty</b> |                   |                          |            |          |           | <b><math>\pm 16.8\%</math></b> | <b><math>\pm 16.2\%</math></b> |                      |

Table 6: Measurement uncertainties

### 6.1.14 Measurement uncertainty evaluation for system validation > 3 Ghz

The overall combined measurement uncertainty of the measurement system is  $\pm 9.9\%$  ( $K=1$ ).

The expanded uncertainty ( $k=2$ ) is assessed to be  $\pm 19.7\%$

This measurement uncertainty budget is suggested by IEEE 1528-2003 and determined by Schmid & Partner Engineering AG. The breakdown of the individual uncertainties is as follows:

| Error Sources                    | Uncertainty Value | Probability Distribution | Divisor    | $c_i$ 1g | $c_i$ 10g | Standard Uncertainty 1g        | Standard Uncertainty 10g       | $v_i^2$ or $v_{eff}$ |
|----------------------------------|-------------------|--------------------------|------------|----------|-----------|--------------------------------|--------------------------------|----------------------|
| <b>Measurement System</b>        |                   |                          |            |          |           |                                |                                |                      |
| Probe calibration                | $\pm 6.3\%$       | Normal                   | 1          | 1        | 1         | $\pm 6.3\%$                    | $\pm 6.3\%$                    | $\infty$             |
| Axial isotropy                   | $\pm 4.7\%$       | Rectangular              | $\sqrt{3}$ | 0.7      | 0.7       | $\pm 1.9\%$                    | $\pm 1.9\%$                    | $\infty$             |
| Hemispherical isotropy           | $\pm 0.0\%$       | Rectangular              | $\sqrt{3}$ | 0.7      | 0.7       | $\pm 0.0\%$                    | $\pm 3.9\%$                    | $\infty$             |
| Boundary effects                 | $\pm 2.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 1.2\%$                    | $\pm 1.2\%$                    | $\infty$             |
| Probe linearity                  | $\pm 4.7\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 2.7\%$                    | $\pm 2.7\%$                    | $\infty$             |
| System detection limits          | $\pm 1.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.6\%$                    | $\pm 0.6\%$                    | $\infty$             |
| Readout electronics              | $\pm 1.0\%$       | Normal                   | 1          | 1        | 1         | $\pm 1.0\%$                    | $\pm 1.0\%$                    | $\infty$             |
| Response time                    | $\pm 0.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.0\%$                    | $\pm 0.0\%$                    | $\infty$             |
| Integration time                 | $\pm 0.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.0\%$                    | $\pm 0.0\%$                    | $\infty$             |
| RF ambient conditions            | $\pm 3.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 1.7\%$                    | $\pm 1.7\%$                    | $\infty$             |
| Probe positioner                 | $\pm 0.8\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.4\%$                    | $\pm 0.4\%$                    | $\infty$             |
| Probe positioning                | $\pm 5.8\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 3.4\%$                    | $\pm 3.4\%$                    | $\infty$             |
| Max. SAR evaluation              | $\pm 1.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 0.6\%$                    | $\pm 0.6\%$                    | $\infty$             |
| <b>Test Sample Related</b>       |                   |                          |            |          |           |                                |                                |                      |
| Dipole axis to liquid distance   | $\pm 2.0\%$       | Normal                   | 1          | 1        | 1         | $\pm 1.2\%$                    | $\pm 1.2\%$                    | $\infty$             |
| Power drift                      | $\pm 4.7\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 2.7\%$                    | $\pm 2.7\%$                    | $\infty$             |
| <b>Phantom and Set-up</b>        |                   |                          |            |          |           |                                |                                |                      |
| Phantom uncertainty              | $\pm 4.0\%$       | Rectangular              | $\sqrt{3}$ | 1        | 1         | $\pm 2.3\%$                    | $\pm 2.3\%$                    | $\infty$             |
| Liquid conductivity (target)     | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 0.64     | 0.43      | $\pm 1.8\%$                    | $\pm 1.2\%$                    | $\infty$             |
| Liquid conductivity (meas.)      | $\pm 2.5\%$       | Normal                   | 1          | 0.64     | 0.43      | $\pm 1.6\%$                    | $\pm 1.1\%$                    | $\infty$             |
| Liquid permittivity (target)     | $\pm 5.0\%$       | Rectangular              | $\sqrt{3}$ | 0.6      | 0.49      | $\pm 1.7\%$                    | $\pm 1.4\%$                    | $\infty$             |
| Liquid permittivity (meas.)      | $\pm 2.5\%$       | Normal                   | 1          | 0.6      | 0.49      | $\pm 1.5\%$                    | $\pm 1.2\%$                    | $\infty$             |
| <b>Combined Uncertainty</b>      |                   |                          |            |          |           | <b><math>\pm 9.9\%</math></b>  | <b><math>\pm 9.6\%</math></b>  |                      |
| <b>Expanded Std. Uncertainty</b> |                   |                          |            |          |           | <b><math>\pm 19.7\%</math></b> | <b><math>\pm 19.2\%</math></b> |                      |

Table 7: Measurement uncertainties

### 6.1.15 System validation

The system validation is performed for verifying the accuracy of the complete measurement system and performance of the software. The system validation is performed with tissue equivalent material according to IEEE 1528. The following table shows validation results for all frequency bands and tissue liquids used during the tests (plot(s) see annex A).


| Validation Kit       | Frequency        | Target Peak SAR (1000 mW) (+/- 10%) | Target SAR <sub>1g</sub> (1000 mW) (+/- 10%) | Measured Peak SAR (1000 mW) | Measured SAR <sub>1g</sub> (1000 mW) | Measured date |
|----------------------|------------------|-------------------------------------|--|-----------------------------|--------------------------------------|---------------|
| D2450V2<br>S/N: 710  | 2450 MHz<br>body | 99.6 mW/g                           | 49.4 mW/g                                    | 111.5 mW/g                  | 52.8 mW/g                            | 2010-04-28    |
| D5GHzV2<br>S/N: 1055 | 5200 MHz<br>body | 302 mW/g                            | 78.7 mW/g                                    | 293 mW/g                    | 81.0 mW/g                            | 2010-04-29    |
| D5GHzV2<br>S/N: 1055 | 5500 MHz<br>body | 336 mW/g                            | 81.2 mW/g                                    | 317 mW/g                    | 83.4 mW/g                            | 2010-04-29    |
| D5GHzV2<br>S/N: 1055 | 5800 MHz<br>body | 312 mW/g                            | 71.8 mW/g                                    | 29.6 mW/g                   | 72.9 mW/g                            | 2010-04-29    |

Table 8: Results system validation

### 6.1.16 Validation procedure

The validation is performed by using a validation dipole which is positioned parallel to the planar part of the SAM phantom at the reference point. The distance of the dipole to the SAM phantom is determined by a plexiglass spacer. The dipole is connected to the signal source consisting of signal generator and amplifier via a directional coupler, N-connector cable and adaption to SMA. It is fed with a power of 1000 mW. To adjust this power a power meter is used. The power sensor is connected to the cable before the validation to measure the power at this point and do adjustments at the signal generator. At the outputs of the directional coupler both return loss as well as forward power are controlled during the validation to make sure that emitted power at the dipole is kept constant. This can also be checked by the power drift measurement after the test (result on plot).

Validation results have to be equal or near the values determined during dipole calibration (target SAR in table above) with the relevant liquids and test system.

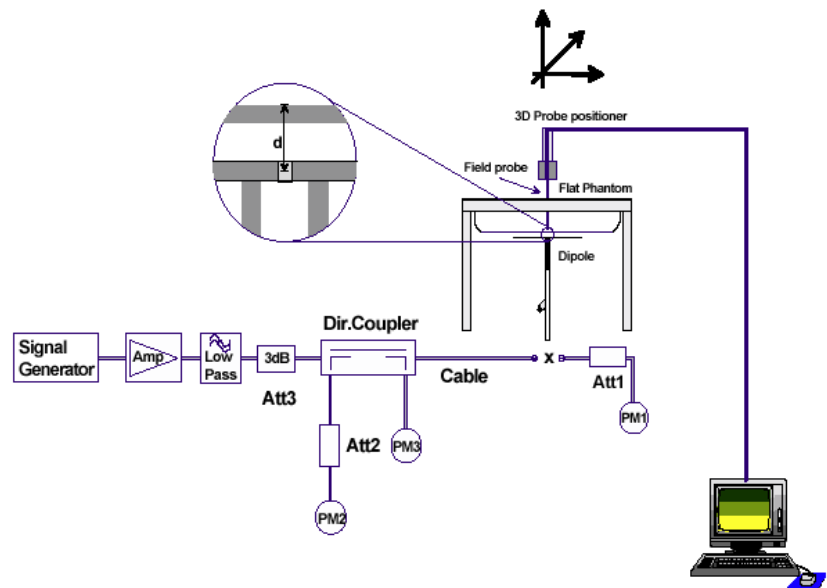

## 7 Detailed Test Results

### 7.1 Conducted power measurements WLAN

For the measurements Rhode & Schwarz NRP was used.  
The output power was measured using an integrated RF connector and attached power sensor.  
With 100% duty cycle average output power is equal to peak power.

| WLAN 2.4 GHz        |              | WLAN 5.2 GHz        |              |
|---------------------|--------------|---------------------|--------------|
| Channel / frequency | output power | Channel / frequency | output power |
| 1 / 2412 MHz CCK    | 18.1 dBm     | 36 / 5180 MHz       | 12.8 dBm     |
| 6 / 2437 MHz CCK    | 19.3 dBm     | 40 / 5200 MHz       | 12.5 dBm     |
| 11 / 2462 MHz CCK   | 17.7 dBm     | 48 / 5240 MHz       | 12.6 dBm     |
| 6 / 2437 MHz OFDM   | 22.8 dBm     |                     |              |
| WLAN 5.3 GHz        |              | WLAN 5.8 GHz        |              |
| Channel / frequency | output power | Channel / frequency | output power |
| 52 / 5260 MHz       | 16.2 dBm     | 149 / 5745 MHz      | 20.6 dBm     |
| 56 / 5280 MHz       | 16.7 dBm     | 157 / 5775 MHz      | 20.6 dBm     |
| 64 / 5320 MHz       | 16.9 dBm     | 165 / 5825 MHz      | 20.6 dBm     |

Table 9: Test results conducted power measurement WLAN 2.4 GHz

## 7.2 SAR test results

### 7.2.1 Results overview

| Body SAR WLAN 2450 MHz (averaged over 1g tissue volume) |          |          |                |                       |          |                    |
|---|----------|----------|----------------|-----------------------|----------|--------------------|
| Channel / frequency                                     | Position | distance | test condition | Body worn test result | Limit    | Liquid temperature |
| 1 / 2412 MHz  | front    | 0 mm     | CCK 1 Mbit/s   | 1.170 W/kg            | 1.6 W/kg | 22.5 °C            |
| 6 / 2437 MHz  | front    | 0 mm     | CCK 1 Mbit/s   | 0.950 W/kg            | 1.6 W/kg | 22.5 °C            |
| 11 / 2462 MHz   | front    | 0 mm     | CCK 1 Mbit/s   | 0.862 W/kg            | 1.6 W/kg | 22.5 °C            |
| 6 / 2437 MHz  | rear     | 0 mm     | CCK 1 Mbit/s   | 0.209 W/kg            | 1.6 W/kg | 22.5 °C            |
| 6 / 2437 MHz  | front    | 10 mm    | CCK 1 Mbit/s   | 0.201 W/kg            | 1.6 W/kg | 22.5 °C            |
| 6 / 2437 MHz  | front    | 10 mm    | OFDM 6 Mbit/s  | 0.284 W/kg            | 1.6 W/kg | 22.5 °C            |
| 6 / 2437 MHz  | front    | 0 mm     | OFDM 6 Mbit/s  | <b>1.340 W/kg</b>     | 1.6 W/kg | 22.5 °C            |

Table 10: Test results body SAR WLAN 2450 MHz

| Body SAR WLAN 5 GHz (averaged over 1g tissue volume) |          |          |                |                       |          |                    |
|--|----------|----------|----------------|-----------------------|----------|--------------------|
| Channel / frequency                                  | Position | distance | test condition | Body worn test result | Limit    | Liquid temperature |
| 36 / 5180 MHz  | rear     | 0 mm     | OFDM 6 MBit/s  | 0.014 W/kg            | 1.6 W/kg | 22.5 °C            |
| 36 / 5180 MHz  | front    | 10 mm    | OFDM 6 MBit/s  | 0.190 W/kg            | 1.6 W/kg | 22.8 °C            |
| 64 / 5320 MHz  | rear     | 0 mm     | OFDM 6 MBit/s  | 0.054 W/kg            | 1.6 W/kg | 22.9 °C            |
| 64 / 5320 MHz  | front    | 10 mm    | OFDM 6 MBit/s  | 0.270 W/kg            | 1.6 W/kg | 22.8 °C            |
| 149 / 5745 MHz                                       | rear     | 0 mm     | OFDM 6 MBit/s  | 0.079 W/kg            | 1.6 W/kg | 22.5 °C            |
| 149 / 5745 MHz                                       | front    | 10 mm    | OFDM 6 MBit/s  | <b>1.040 W/kg</b>     | 1.6 W/kg | 22.7 °C            |
| 157 / 5785 MHz                                       | front    | 10 mm    | OFDM 6 MBit/s  | 0.841 W/kg            | 1.6 W/kg | 22.7 °C            |
| 165 / 5825 MHz                                       | front    | 10 mm    | OFDM 6 MBit/s  | 0.694 W/kg            | 1.6 W/kg | 22.7 °C            |

Table 11: Test results body SAR WLAN 5 GHz

#### Note:

The SAR test shall be performed at the high, middle and low frequency channels of each operating mode. If the SAR measured at mid-band channel for each test configuration is at least 3.0 dB lower than the SAR limit (< 0.8 W/kg), testing at the high and low channels is optional.

## 7.2.2 General description of test procedures

The DUT is tested using a test software to control test channels and maximum output power of the DUT. Test positions as described in the tables above are in accordance with the specified test standard. Device positioning took the intended use position of the DUT into account (rear side to the body without any distance). To cover any other position of usage the DUT was additionally tested with front (antenna) side towards the body, which required a minimum distance of 10 mm. Tests in body position were performed in that configuration, which generates the highest time based averaged output power (see conducted power results). The WLAN module was supplied with external power. The same connector was also used to program test frequencies, power levels and 100% duty cycle via a control software installed on a notebook computer. The followings power settings declared by the manufacturer were used by the control software. All measurements were performed with the specified settings.

USA / Canada:

| Band              | Power setting |
|-------------------|---------------|
| 2.400 – 2.483 GHz | 15 dBm        |
| 5.15 – 5.25 GHz   | 11 dBm        |
| 5.25 – 5.35 GHz   | 15 dBm        |
| 5.725 – 5.825 GHz | 15 dBm        |

## 8 Test equipment and ancillaries used for tests

To simplify the identification of the test equipment and/or ancillaries which were used, the reporting of the relevant test cases only refer to the test item number as specified in the table below.

| No | used                                | Equipment                            | Type             | Manufacturer                    | Serial No. | Last Calibration | Frequency (months) |
|----|-------------------------------------|--------------------------------------|------------------|---------------------------------|------------|------------------|--------------------|
| 1  | <input checked="" type="checkbox"/> | Dosimetric E-Field Probe             | EX3DV4           | Schmid & Partner Engineering AG | 3566       | January 21, 2009 | 12                 |
| 2  | <input checked="" type="checkbox"/> | Dosimetric E-Field Probe             | ET3DV6           | Schmid & Partner Engineering AG | 1559       | January 20, 2010 | 12                 |
| 3  | <input type="checkbox"/>            | 900 MHz System Validation Dipole     | D900V2           | Schmid & Partner Engineering AG | 102        | August 17, 2009  | 12                 |
| 4  | <input type="checkbox"/>            | 1800 MHz System Validation Dipole    | D1800V2          | Schmid & Partner Engineering AG | 287        | August 18, 2009  | 12                 |
| 5  | <input checked="" type="checkbox"/> | 5 GHz System Validation Dipole       | D5GHzV2          | Schmid & Partner Engineering AG | 1055       | January 20, 2010 | 12                 |
| 6  | <input checked="" type="checkbox"/> | 2450 MHz System Validation Dipole    | D2450V2          | Schmid & Partner Engineering AG | 710        | August 17, 2009  | 12                 |
| 7  | <input checked="" type="checkbox"/> | Data acquisition electronics         | DAE3V1           | Schmid & Partner Engineering AG | 413        | January 4, 2010  | 12                 |
| 8  | <input checked="" type="checkbox"/> | Data acquisition electronics         | DAE3V1           | Schmid & Partner Engineering AG | 477        | May 14, 2009     | 12                 |
| 9  | <input checked="" type="checkbox"/> | Software                             | DASY 4 V4.5      | Schmid & Partner Engineering AG | ---        | N/A              | --                 |
| 10 | <input checked="" type="checkbox"/> | Phantom                              | SAM              | Schmid & Partner Engineering AG | ---        | N/A              | --                 |
| 11 | <input checked="" type="checkbox"/> | Universal Radio Communication Tester | CMU 200          | Rohde & Schwarz                 | 106826     | January 12, 2010 | 12                 |
| 12 | <input checked="" type="checkbox"/> | Network Analyser 300 kHz to 6 GHz    | 8753C            | Hewlett Packard)*               | 2937U00269 | January 8, 2010  | 12                 |
| 13 | <input checked="" type="checkbox"/> | Network Analyser 300 kHz to 6 GHz    | 85047A           | Hewlett Packard)*               | 2936A00872 | January 8, 2010  | 12                 |
| 14 | <input checked="" type="checkbox"/> | Dielectric Probe Kit                 | 85070C           | Hewlett Packard                 | US99360146 | N/A              | 12                 |
| 15 | <input checked="" type="checkbox"/> | Signal Generator                     | 8665A            | Hewlett Packard                 | 2833A00112 | January 8, 2010  | 12                 |
| 16 | <input checked="" type="checkbox"/> | Amplifier                            | 25S1G4 (25 Watt) | Amplifier Reasearch             | 20452      | N/A              | --                 |
| 17 | <input checked="" type="checkbox"/> | Power Meter                          | NRP              | Rohde & Schwarz                 | 101367     | January 8, 2010  | 12                 |
| 18 | <input checked="" type="checkbox"/> | Power Meter Sensor                   | NRP Z22          | Rohde & Schwarz                 | 100227     | January 8, 2010  | 12                 |
| 19 | <input checked="" type="checkbox"/> | Power Meter Sensor                   | NRP Z22          | Rohde & Schwarz                 | 100234     | January 8, 2010  | 12                 |

)\* : Network analyzer probe calibration against air, distilled water and a shorting block performed before measuring liquid parameters.

## 9 Observations

No observations exceeding those reported with the single test cases have been made.



**Annex A: System performance verification**

Date/Time: 2010-04-28 13:01:39 Date/Time: 2010-04-28 13:05:24

**System Performance Check-D2450 body 2010-04-28**

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 710**

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: M2450 Medium parameters used:  $f = 2450 \text{ MHz}$ ;  $\sigma = 1.99 \text{ mho/m}$ ;  $\epsilon_r = 51.9$ ;  $\rho = 1000 \text{ kg/m}^3$


Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1559; ConvF(4.04, 4.04, 4.04); Calibrated: 2010-01-20
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn477; Calibrated: 2009-05-14
- Phantom: SAM 12; Type: SAM; Serial: 1043
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

**d=10mm, Pin=1000mW/Area Scan (51x51x1):** Measurement grid: dx=15mm, dy=15mm  
 Maximum value of SAR (interpolated) = 80.1 mW/g

**d=10mm, Pin=1000mW/Zoom Scan (7x7x7) (7x7x7)/Cube 0:** Measurement grid:  
 dx=5mm, dy=5mm, dz=5mm  
 Reference Value = 184.1 V/m; Power Drift = 0.01 dB  
 Peak SAR (extrapolated) = 111.5 W/kg  
**SAR(1 g) = 52.8 mW/g; SAR(10 g) = 24.8 mW/g**  
 Maximum value of SAR (measured) = 59.6 mW/g

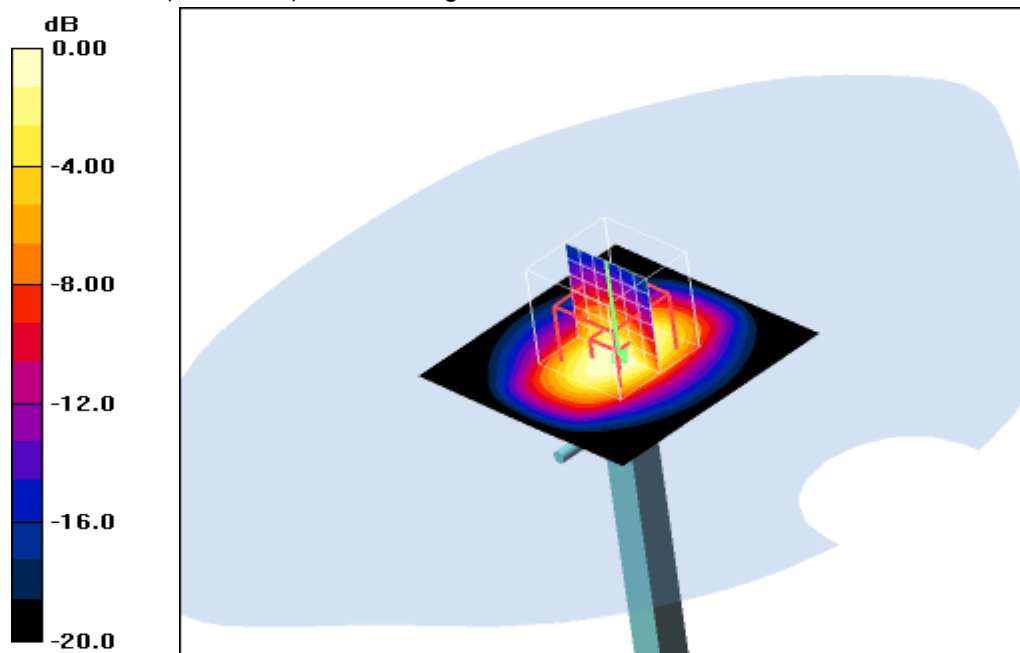

0 dB = 59.6mW/g

**Additional information:**

ambient temperature: 23.6°C; liquid temperature: 22.5°C

Date/Time: 29.04.2010 13:04:37 Date/Time: 29.04.2010 13:09:28

### System Performance Check-D5200 body 2010-04-29

DUT: Dipole 5 GHz; Type: D5GHzV2; Serial: 1055

Communication System: CW; Frequency: 5200 MHz; Duty Cycle: 1:1

Medium: M5200 Medium parameters used:  $f = 5200$  MHz;  $\sigma = 5.34$  mho/m;  $\epsilon_r = 48$ ;  $\rho = 1000$  kg/m<sup>3</sup>


Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 - SN3566; ConvF(3.53, 3.53, 3.53); Calibrated: 21.08.2009
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn413; Calibrated: 04.01.2010
- Phantom: SAM right; Type: SAM; Serial: 1042
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 146

**d=10mm, Pin=100mW/Area Scan (61x61x1):** Measurement grid: dx=10mm, dy=10mm  
 Maximum value of SAR (interpolated) = 17.3 mW/g

**d=10mm, Pin=100mW/Zoom Scan (8x8x8) (8x8x8)/Cube 0:** Measurement grid:  
 dx=4.3mm, dy=4.3mm, dz=3mm  
 Reference Value = 44.4 V/m; Power Drift = -0.057 dB  
 Peak SAR (extrapolated) = 29.3 W/kg  
**SAR(1 g) = 8.1 mW/g; SAR(10 g) = 2.29 mW/g**  
 Maximum value of SAR (measured) = 15.9 mW/g

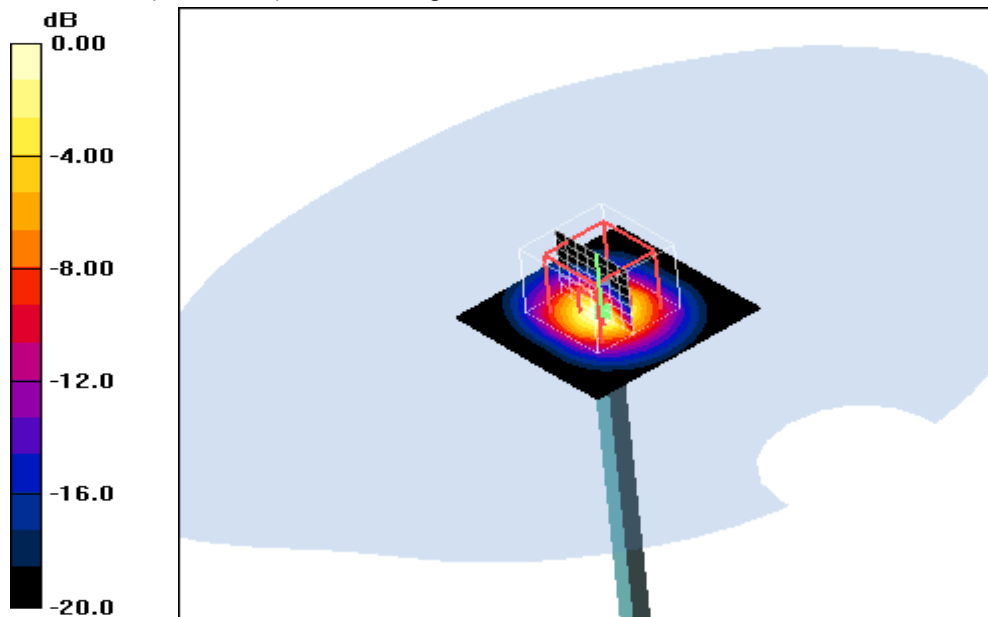

0 dB = 15.9mW/g

**Additional information:**

ambient temperature: 23.7°C; liquid temperature: 22.7°C

Date/Time: 29.04.2010 12:26:38 Date/Time: 29.04.2010 12:30:09

### System Performance Check-D5500 body 2010-04-29

DUT: Dipole 5 GHz; Type: D5GHzV2; Serial: 1055

Communication System: CW; Frequency: 5500 MHz; Duty Cycle: 1:1

Medium: M5500 Medium parameters used:  $f = 5500$  MHz;  $\sigma = 5.71$  mho/m;  $\epsilon_r = 47.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>


Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 - SN3566; ConvF(3.14, 3.14, 3.14); Calibrated: 21.08.2009
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn413; Calibrated: 04.01.2010
- Phantom: SAM right; Type: SAM; Serial: 1042
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 146

**d=10mm, Pin=100mW/Area Scan (51x51x1):** Measurement grid: dx=10mm, dy=10mm  
 Maximum value of SAR (interpolated) = 21.2 mW/g

**d=10mm, Pin=100mW/Zoom Scan (8x8x8) (8x8x8)/Cube 0:** Measurement grid:  
 dx=4.3mm, dy=4.3mm, dz=3mm  
 Reference Value = 62.9 V/m; Power Drift = -0.089 dB  
 Peak SAR (extrapolated) = 31.7 W/kg  
**SAR(1 g) = 8.34 mW/g; SAR(10 g) = 2.33 mW/g**  
 Maximum value of SAR (measured) = 16.1 mW/g

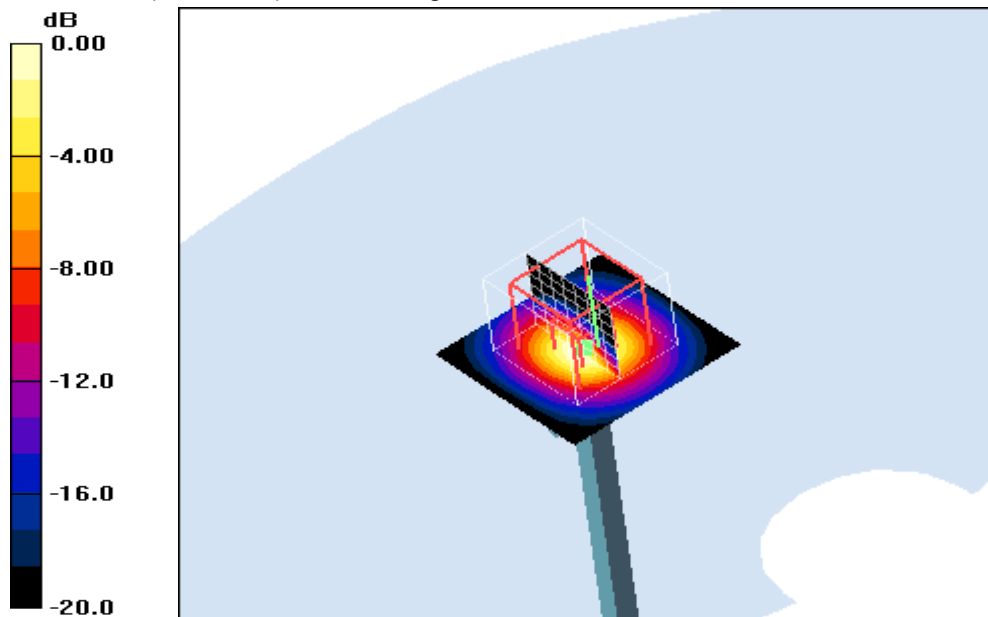

**Additional information:**  
 ambient temperature: 23.7°C; liquid temperature: 22.7°C

Date/Time: 29.04.2010 11:48:51 Date/Time: 29.04.2010 11:53:37

### System Performance Check-D5800 body 2010-04-29

**DUT: Dipole 5 GHz; Type: D5GHzV2; Serial: 1055**

Communication System: CW; Frequency: 5800 MHz; Duty Cycle: 1:1

Medium: M5800 Medium parameters used:  $f = 5800 \text{ MHz}$ ;  $\sigma = 6.1 \text{ mho/m}$ ;  $\epsilon_r = 46.7$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 - SN3566; ConvF(3.3, 3.3, 3.3); Calibrated: 21.08.2009
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn413; Calibrated: 04.01.2010
- Phantom: SAM right; Type: SAM; Serial: 1042
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 146

**d=10mm, Pin=100mW/Area Scan (61x61x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$

Maximum value of SAR (interpolated) = 16.0 mW/g

**d=10mm, Pin=100mW/Zoom Scan (8x8x8) (8x8x8)/Cube 0:** Measurement grid:


$dx=4.3\text{mm}$ ,  $dy=4.3\text{mm}$ ,  $dz=3\text{mm}$

Reference Value = 57.8 V/m; Power Drift = -0.106 dB

Peak SAR (extrapolated) = 29.6 W/kg

**SAR(1 g) = 7.29 mW/g; SAR(10 g) = 2.04 mW/g**

Maximum value of SAR (measured) = 14.5 mW/g

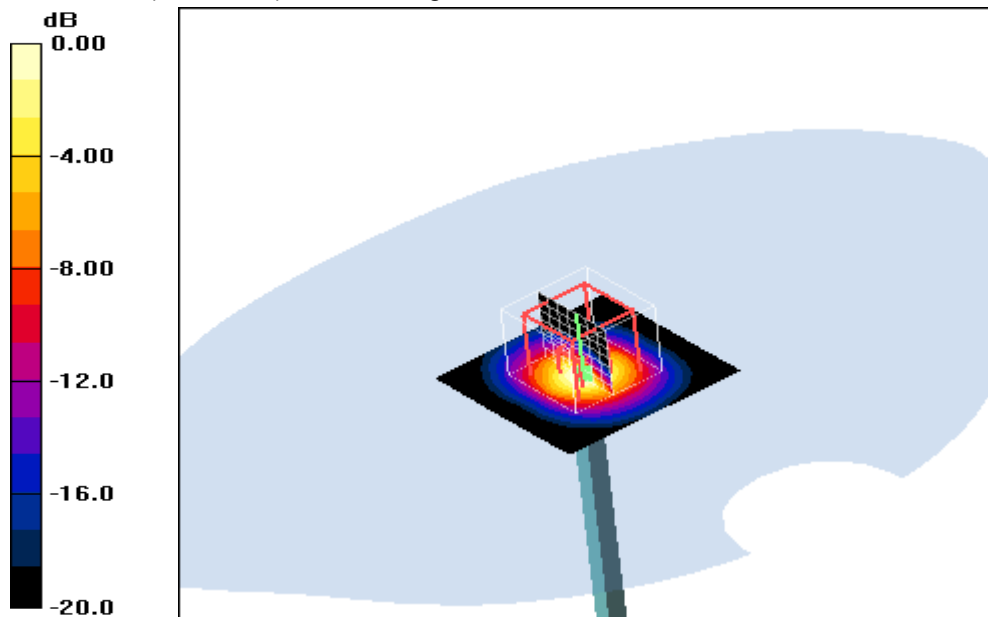

0 dB = 14.5mW/g

**Additional information:**

ambient temperature: 23.7°C; liquid temperature: 22.7°C

## Annex B: DASY4 measurement results

### Annex B.1: WLAN 2450MHz

Date/Time: 2010-04-28 19:17:09 Date/Time: 2010-04-28 19:27:35

#### IEEE1528\_OET65-Body-WLAN2450

DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107

Communication System: WLAN 2450 US; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium: M2450 Medium parameters used (interpolated):  $f = 2412$  MHz;  $\sigma = 1.99$  mho/m;  $\epsilon_r = 51.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1559; ConvF(4.04, 4.04, 4.04); Calibrated: 2010-01-20
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn477; Calibrated: 2009-05-14
- Phantom: SAM 12; Type: SAM; Serial: 1043
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

**Front position - Low/Area Scan (51x101x1):** Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 1.37 mW/g

**Front position - Low/Zoom Scan (7x7x7) (7x7x7)/Cube 0:** Measurement grid:


dx=5mm, dy=5mm, dz=5mm

Reference Value = 5.98 V/m; Power Drift = -0.122 dB

Peak SAR (extrapolated) = 3.37 W/kg

**SAR(1 g) = 1.17 mW/g; SAR(10 g) = 0.428 mW/g**

Maximum value of SAR (measured) = 1.43 mW/g

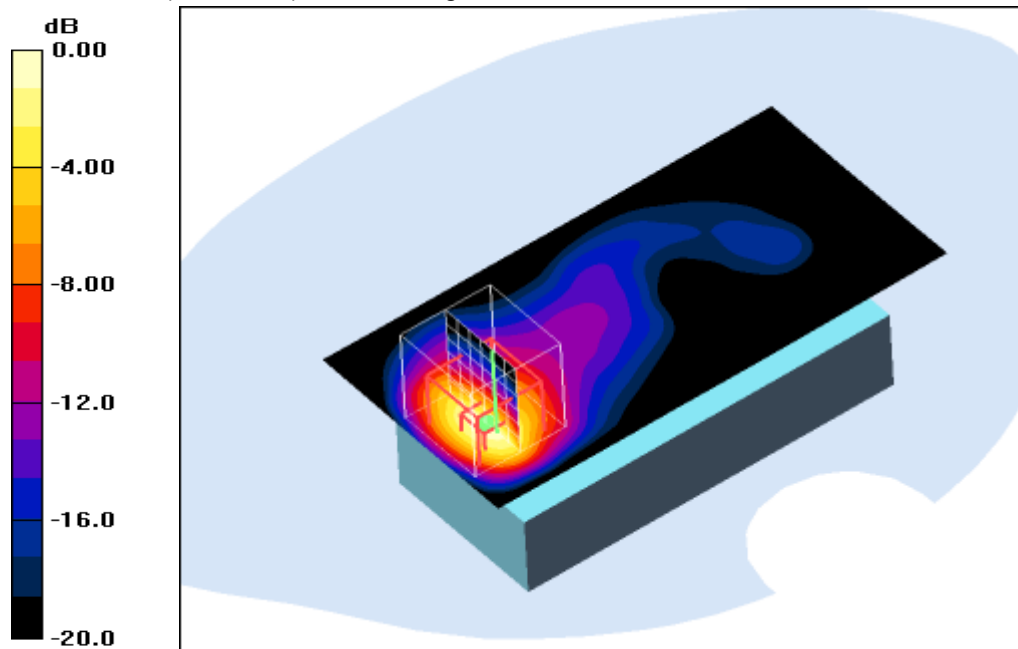

0 dB = 1.43mW/g

#### Additional information:

position or distance of DUT to SAM: DUT touching SAM

ambient temperature: 23.6°C; liquid temperature: 22.5°C

Date/Time: 2010-04-28 18:36:00 Date/Time: 2010-04-28 18:42:36

**IEEE1528\_OET65-Body-WLAN2450**

**DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107**

Communication System: WLAN 2450 US; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: M2450 Medium parameters used (interpolated):  $f = 2437$  MHz;  $\sigma = 1.99$  mho/m;  $\epsilon_r = 51.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1559; ConvF(4.04, 4.04, 4.04); Calibrated: 2010-01-20
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn477; Calibrated: 2009-05-14
- Phantom: SAM 12; Type: SAM; Serial: 1043
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

**Front position - Middle/Area Scan (51x101x1):** Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 1.16 mW/g

**Front position - Middle/Zoom Scan (7x7x7) (7x7x7)/Cube 0:** Measurement grid:


dx=5mm, dy=5mm, dz=5mm

Reference Value = 5.99 V/m; Power Drift = 0.174 dB

Peak SAR (extrapolated) = 2.78 W/kg

**SAR(1 g) = 0.950 mW/g; SAR(10 g) = 0.350 mW/g**

Maximum value of SAR (measured) = 1.13 mW/g

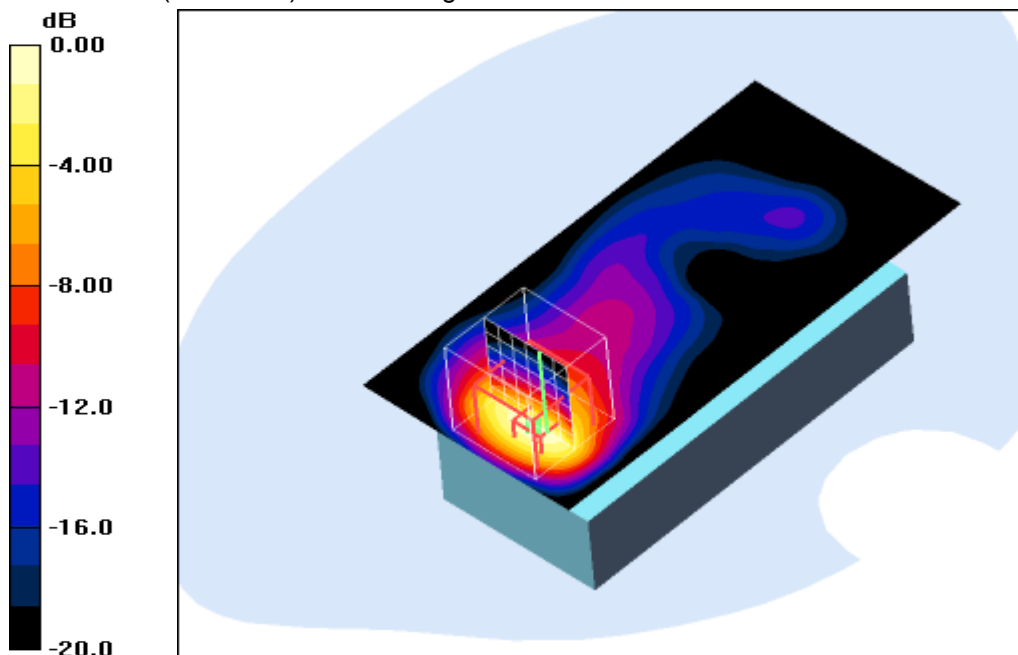

0 dB = 1.13mW/g

**Additional information:**

position or distance of DUT to SAM: DUT touching SAM

ambient temperature: 23.6°C; liquid temperature: 22.5°C

Date/Time: 2010-04-28 18:57:00 Date/Time: 2010-04-28 19:03:02

### IEEE1528\_OET65-Body-WLAN2450

DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107

Communication System: WLAN 2450 US; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium: M2450 Medium parameters used (interpolated):  $f = 2462$  MHz;  $\sigma = 1.99$  mho/m;  $\epsilon_r = 51.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>


Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1559; ConvF(4.04, 4.04, 4.04); Calibrated: 2010-01-20
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn477; Calibrated: 2009-05-14
- Phantom: SAM 12; Type: SAM; Serial: 1043
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

**Front position - High/Area Scan (51x81x1):** Measurement grid: dx=15mm, dy=15mm  
Maximum value of SAR (interpolated) = 0.844 mW/g

**Front position - High/Zoom Scan (7x7x7) (7x7x7)/Cube 0:** Measurement grid:  
dx=5mm, dy=5mm, dz=5mm  
Reference Value = 20.3 V/m; Power Drift = -0.106 dB  
Peak SAR (extrapolated) = 2.49 W/kg  
**SAR(1 g) = 0.862 mW/g; SAR(10 g) = 0.327 mW/g**  
Maximum value of SAR (measured) = 1.07 mW/g

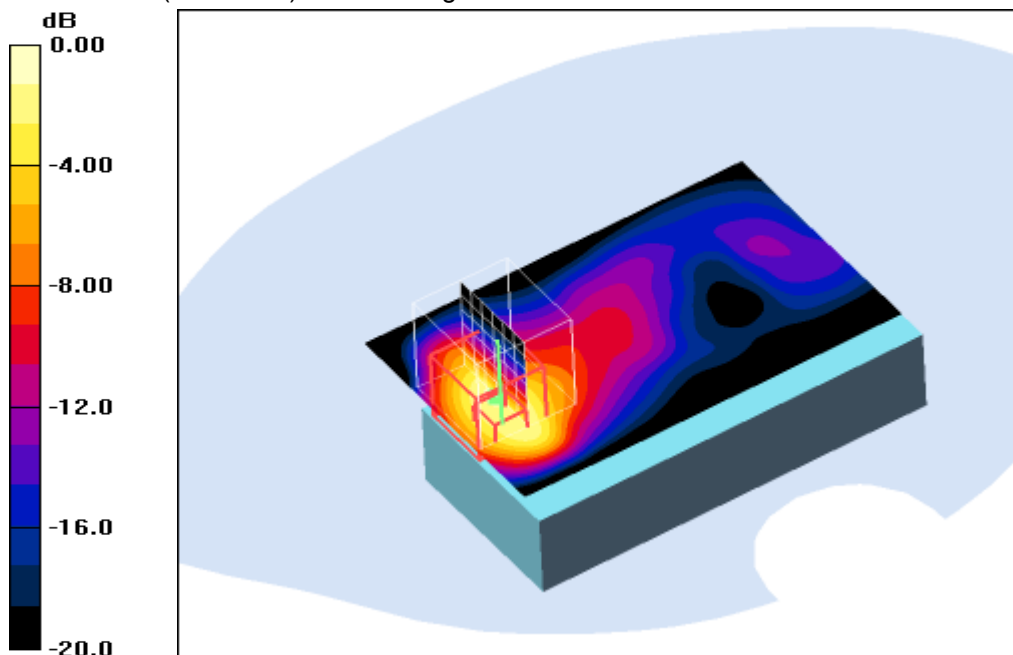

**Additional information:**  
position or distance of DUT to SAM: DUT touching SAM  
ambient temperature: 23.6°C; liquid temperature: 22.5°C

Date/Time: 2010-04-28 18:02:52 Date/Time: 2010-04-28 18:09:25 Date/Time: 2010-04-28 18:21:20

**IEEE1528\_OET65-Body-WLAN2450**

**DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107**

Communication System: WLAN 2450 US; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: M2450 Medium parameters used (interpolated):  $f = 2437$  MHz;  $\sigma = 1.99$  mho/m;  $\epsilon_r = 51.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1559; ConvF(4.04, 4.04, 4.04); Calibrated: 2010-01-20
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn477; Calibrated: 2009-05-14
- Phantom: SAM 12; Type: SAM; Serial: 1043
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

**Rear position - Middle/Area Scan (51x101x1):** Measurement grid: dx=15mm, dy=15mm  
 Maximum value of SAR (interpolated) = 0.248 mW/g

**Rear position - Middle/Zoom Scan (7x7x7) (7x7x7)/Cube 0:** Measurement grid:  
 dx=5mm, dy=5mm, dz=5mm

Reference Value = 6.16 V/m; Power Drift = -0.068 dB

Peak SAR (extrapolated) = 0.442 W/kg

**SAR(1 g) = 0.209 mW/g; SAR(10 g) = 0.104 mW/g**

Maximum value of SAR (measured) = 0.239 mW/g


**Rear position - Middle/Zoom Scan (7x7x7) (7x7x7)/Cube 1:** Measurement grid:  
 dx=5mm, dy=5mm, dz=5mm

Reference Value = 6.16 V/m; Power Drift = -0.068 dB

Peak SAR (extrapolated) = 0.338 W/kg

**SAR(1 g) = 0.191 mW/g; SAR(10 g) = 0.104 mW/g**

Maximum value of SAR (measured) = 0.210 mW/g

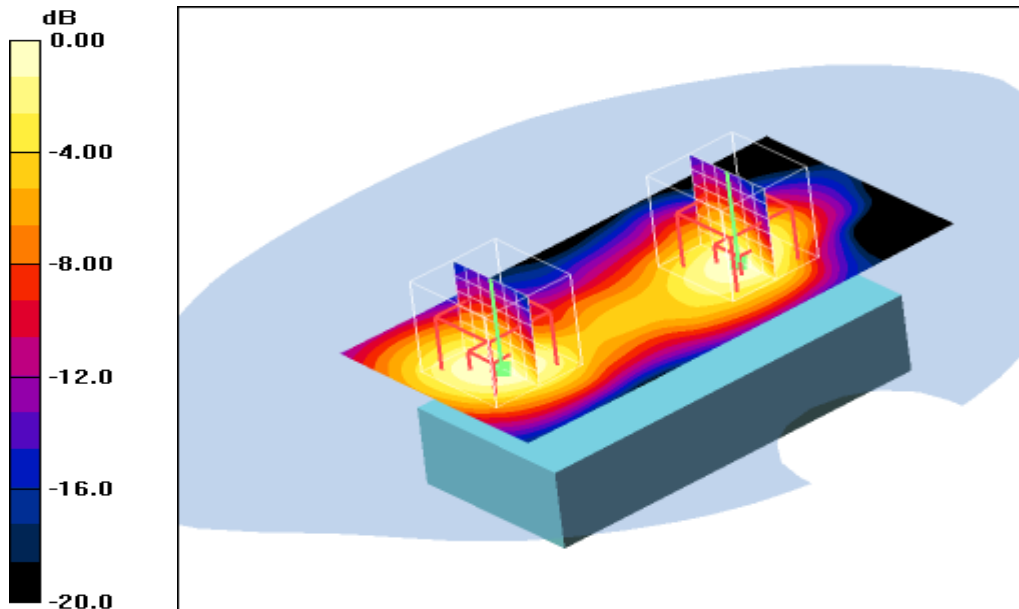

0 dB = 0.210mW/g

**Additional information:**

position or distance of DUT to SAM: DUT touching SAM

ambient temperature: 23.6°C; liquid temperature: 22.5°C



Date/Time: 2010-04-28 19:42:33 Date/Time: 2010-04-28 19:49:09

**IEEE1528\_OET65-Body-WLAN2450**

**DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107**

Communication System: WLAN 2450 US; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: M2450 Medium parameters used (interpolated):  $f = 2437$  MHz;  $\sigma = 1.99$  mho/m;  $\epsilon_r = 51.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1559; ConvF(4.04, 4.04, 4.04); Calibrated: 2010-01-20
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn477; Calibrated: 2009-05-14
- Phantom: SAM 12; Type: SAM; Serial: 1043
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

**Front position - Middle 10mm/Area Scan (51x101x1):** Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.223 mW/g

**Front position - Middle 10mm/Zoom Scan (7x7x7) (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 5.19 V/m; Power Drift = 0.038 dB

Peak SAR (extrapolated) = 0.466 W/kg

**SAR(1 g) = 0.201 mW/g; SAR(10 g) = 0.091 mW/g**

Maximum value of SAR (measured) = 0.227 mW/g

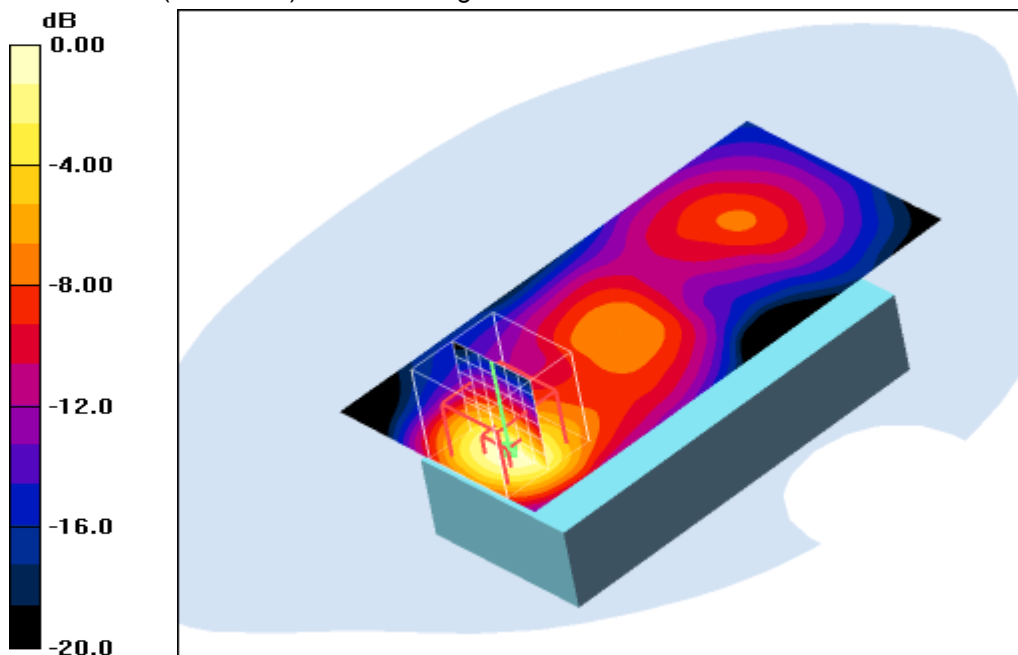

0 dB = 0.227mW/g

**Additional information:**

position or distance of DUT to SAM: 10 mm

ambient temperature: 23.6°C; liquid temperature: 22.5°C

Date/Time: 2010-04-28 21:05:17 Date/Time: 2010-04-28 21:12:01

**IEEE1528\_OET65-Body-WLAN2450**

**DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107**

Communication System: WLAN 2450 US; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: M2450 Medium parameters used (interpolated):  $f = 2437$  MHz;  $\sigma = 1.99$  mho/m;  $\epsilon_r = 51.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1559; ConvF(4.04, 4.04, 4.04); Calibrated: 2010-01-20
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn477; Calibrated: 2009-05-14
- Phantom: SAM 12; Type: SAM; Serial: 1043
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

**Front position - Middle 10mm 6 Mbps/Area Scan (51x101x1):** Measurement grid:

$dx=15$ mm,  $dy=15$ mm

Maximum value of SAR (interpolated) = 0.291 mW/g

**Front position - Middle 10mm 6 Mbps/Zoom Scan (7x7x7) (7x7x7)/Cube 0:**


Measurement grid:  $dx=5$ mm,  $dy=5$ mm,  $dz=5$ mm

Reference Value = 5.67 V/m; Power Drift = 0.166 dB

Peak SAR (extrapolated) = 0.673 W/kg

**SAR(1 g) = 0.284 mW/g; SAR(10 g) = 0.125 mW/g**

Maximum value of SAR (measured) = 0.324 mW/g

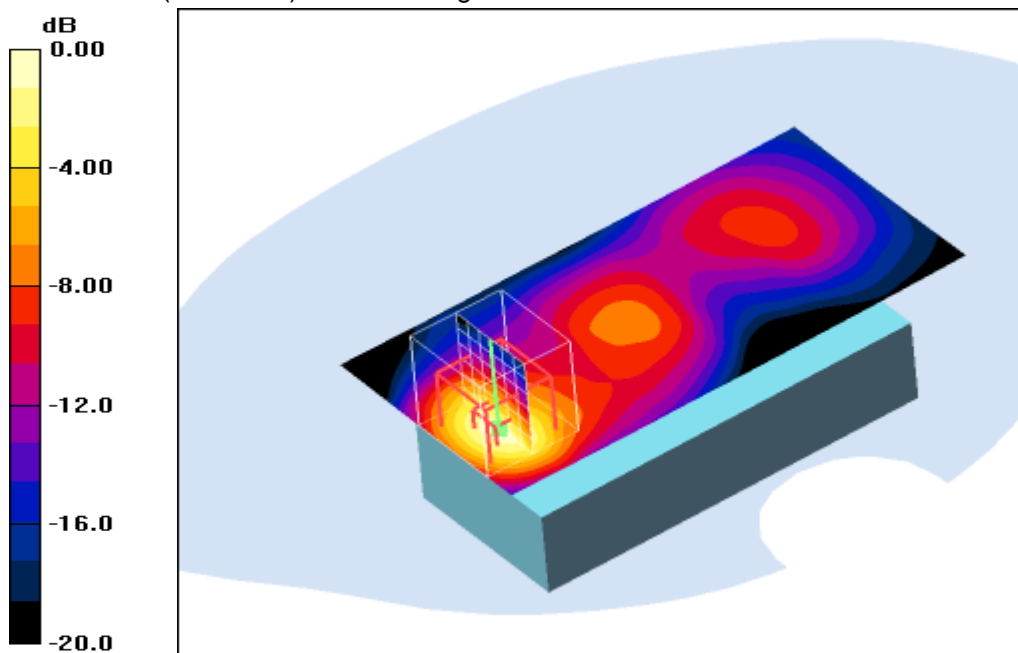

0 dB = 0.324mW/g

**Additional information:**

position or distance of DUT to SAM: 10 mm

ambient temperature: 23.6°C; liquid temperature: 22.5°C

Date/Time: 2010-04-28 20:38:09 Date/Time: 2010-04-28 20:44:49

**IEEE1528\_OET65-Body-WLAN2450**

**DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107**

Communication System: WLAN 2450 US; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium: M2450 Medium parameters used (interpolated):  $f = 2412 \text{ MHz}$ ;  $\sigma = 1.99 \text{ mho/m}$ ;  $\epsilon_r = 51.9$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1559; ConvF(4.04, 4.04, 4.04); Calibrated: 2010-01-20
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn477; Calibrated: 2009-05-14
- Phantom: SAM 12; Type: SAM; Serial: 1043
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

**Front position - Middle 6Mbps/Area Scan (51x101x1):** Measurement grid:  $dx=15\text{mm}$ ,  $dy=15\text{mm}$

Maximum value of SAR (interpolated) = 1.63 mW/g

**Front position - Middle 6Mbps/Zoom Scan (7x7x7) (7x7x7)/Cube 0:**


Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 6.58 V/m; Power Drift = -0.127 dB

Peak SAR (extrapolated) = 3.93 W/kg

**SAR(1 g) = 1.34 mW/g; SAR(10 g) = 0.489 mW/g**

Maximum value of SAR (measured) = 1.64 mW/g

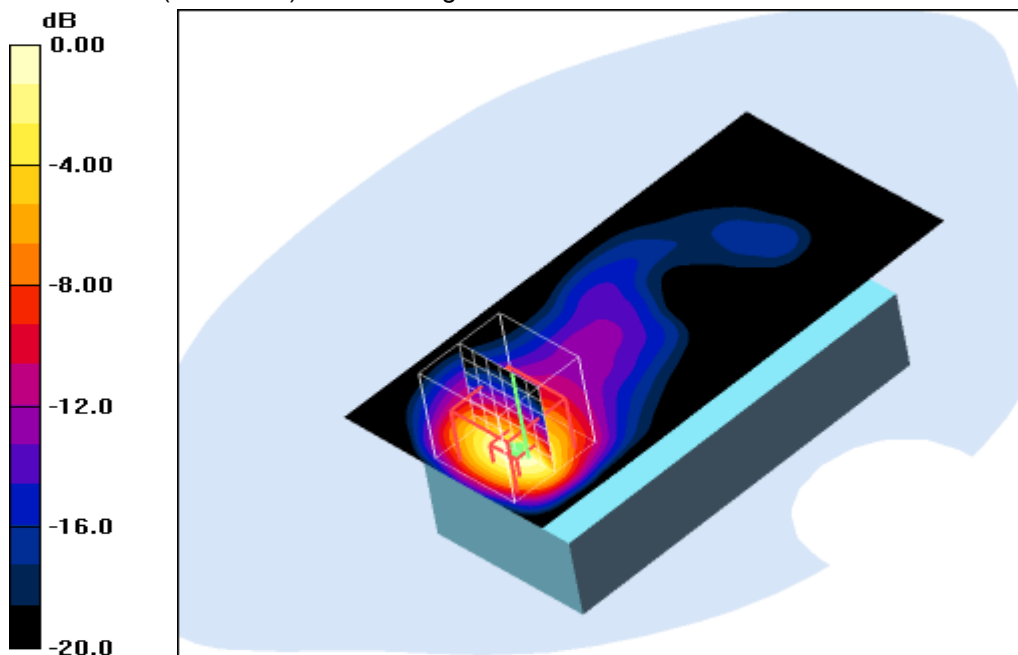

0 dB = 1.64mW/g

**Additional information:**

position or distance of DUT to SAM: DUT touching SAM  
 ambient temperature: 23.6°C; liquid temperature: 22.5°C

**Annex B.2: WLAN 5GHz**

Date/Time: 30.04.2010 10:45:26 Date/Time: 30.04.2010 10:59:54

**IEEE1528\_OET65\_EN62209-2-Body-WLAN 5GHz**

**DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107**

Communication System: WLAN 5200; Frequency: 5180 MHz; Duty Cycle: 1:1

Medium: M5200 Medium parameters used:  $f = 5180 \text{ MHz}$ ;  $\sigma = 5.34 \text{ mho/m}$ ;  $\epsilon_r = 48$ ;  $\rho = 1000 \text{ kg/m}^3$


Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 - SN3566; ConvF(3.53, 3.53, 3.53); Calibrated: 21.08.2009
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn413; Calibrated: 04.01.2010
- Phantom: SAM right; Type: SAM; Serial: 1042
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 146

**Rear position - Low/Area Scan (81x151x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$   
 Maximum value of SAR (interpolated) = 0.189 mW/g

**Rear position - Low/Zoom Scan (7x7x7) (8x8x8)/Cube 0:** Measurement grid:  
 $dx=4.3\text{mm}$ ,  $dy=4.3\text{mm}$ ,  $dz=3\text{mm}$   
 Reference Value = 3.11 V/m; Power Drift = -0.80 dB  
 Peak SAR (extrapolated) = 0.256 W/kg  
**SAR(1 g) = 0.014 mW/g; SAR(10 g) = 0.00589 mW/g**  
 Maximum value of SAR (measured) = 0.256 mW/g

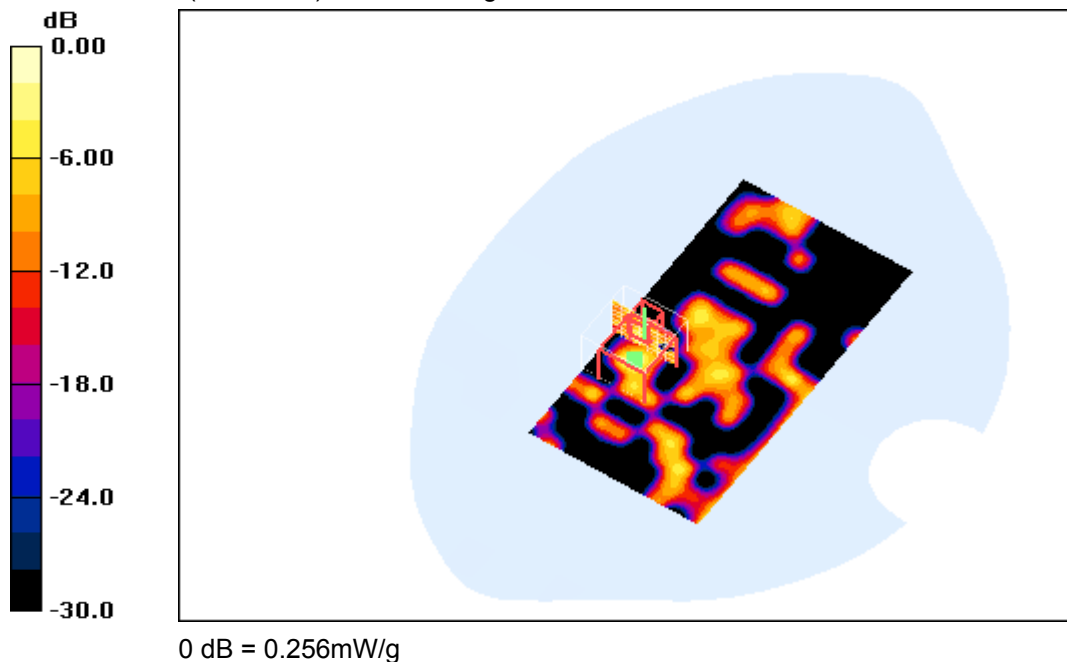

**Additional information:**  
 position or distance of DUT to SAM: DUT touching SAM  
 ambient temperature: 23.5°C; liquid temperature: 22.5°C

Date/Time: 29.04.2010 18:59:15 Date/Time: 29.04.2010 19:13:06

**IEEE1528\_OET65\_EN62209-2-Body-WLAN 5GHz**

**DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107**

Communication System: WLAN 5200; Frequency: 5180 MHz; Duty Cycle: 1:1

Medium: M5200 Medium parameters used:  $f = 5180 \text{ MHz}$ ;  $\sigma = 5.34 \text{ mho/m}$ ;  $\epsilon_r = 48$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 - SN3566; ConvF(3.53, 3.53, 3.53); Calibrated: 21.08.2009
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn413; Calibrated: 04.01.2010
- Phantom: SAM right; Type: SAM; Serial: 1042
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 146

**Front position - Low 10 mm/Area Scan (81x151x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$

Maximum value of SAR (interpolated) = 0.297 mW/g


**Front position - Low 10 mm/Zoom Scan (7x7x7) (8x8x8)/Cube 0:** Measurement grid:  $dx=4.3\text{mm}$ ,  $dy=4.3\text{mm}$ ,  $dz=3\text{mm}$

Reference Value = 6.89 V/m; Power Drift = 0.073 dB

Peak SAR (extrapolated) = 0.412 W/kg

**SAR(1 g) = 0.190 mW/g; SAR(10 g) = 0.110 mW/g**

Maximum value of SAR (measured) = 0.283 mW/g

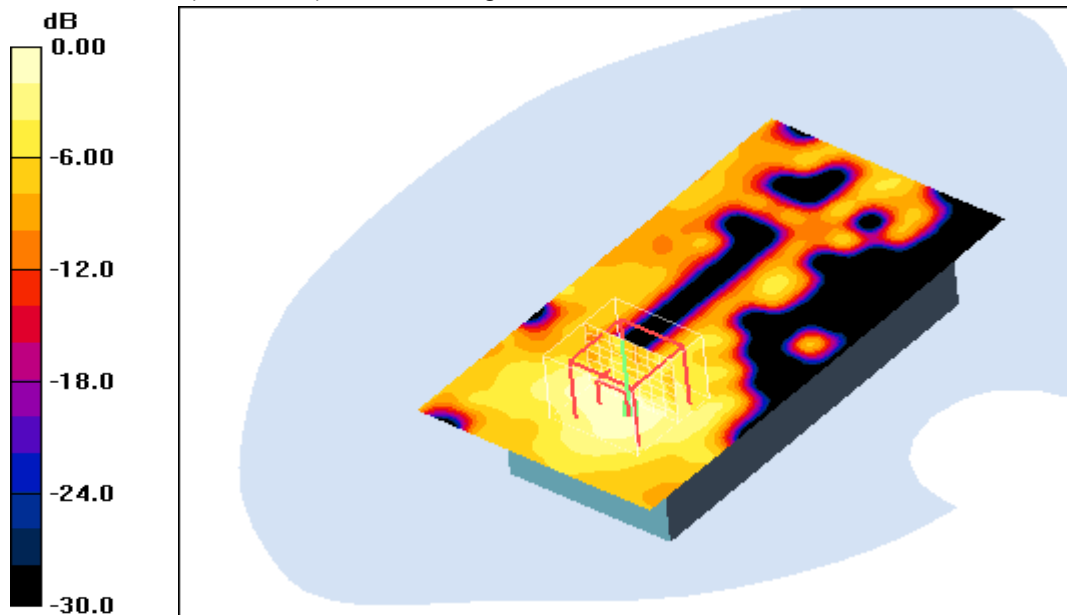

0 dB = 0.283mW/g

**Additional information:**

position or distance of DUT to SAM: 10 mm

ambient temperature: 24.5°C; liquid temperature: 22.8°C

Date/Time: 29.04.2010 20:37:57 Date/Time: 29.04.2010 20:57:22 Date/Time: 29.04.2010 21:14:59

**IEEE1528\_OET65\_EN62209-2-Body-WLAN 5GHz**

**DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107**

Communication System: WLAN 5200; Frequency: 5320 MHz; Duty Cycle: 1:1

Medium: M5200 Medium parameters used:  $f = 5320 \text{ MHz}$ ;  $\sigma = 5.46 \text{ mho/m}$ ;  $\epsilon_r = 47.8$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section


DASY4 Configuration:

- Probe: EX3DV4 - SN3566; ConvF(3.42, 3.42, 3.42); Calibrated: 21.08.2009
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn413; Calibrated: 04.01.2010
- Phantom: SAM right; Type: SAM; Serial: 1042
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 146

**Rear position - High/Area Scan (81x151x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$   
 Maximum value of SAR (interpolated) = 0.334 mW/g

**Rear position - High/Zoom Scan (7x7x7) (8x8x8)/Cube 0:** Measurement grid:  
 $dx=4.3\text{mm}$ ,  $dy=4.3\text{mm}$ ,  $dz=3\text{mm}$   
 Reference Value = 4.59 V/m; Power Drift = -0.106 dB  
 Peak SAR (extrapolated) = 0.265 W/kg  
**SAR(1 g) = 0.022 mW/g; SAR(10 g) = 0.012 mW/g**  
 Maximum value of SAR (measured) = 0.145 mW/g

**Rear position - High/Zoom Scan (7x7x7) (8x8x8)/Cube 1:** Measurement grid:  
 $dx=4.3\text{mm}$ ,  $dy=4.3\text{mm}$ ,  $dz=3\text{mm}$   
 Reference Value = 4.59 V/m; Power Drift = -0.106 dB  
 Peak SAR (extrapolated) = 0.241 W/kg  
**SAR(1 g) = 0.054 mW/g; SAR(10 g) = 0.030 mW/g**  
 Maximum value of SAR (measured) = 0.212 mW/g

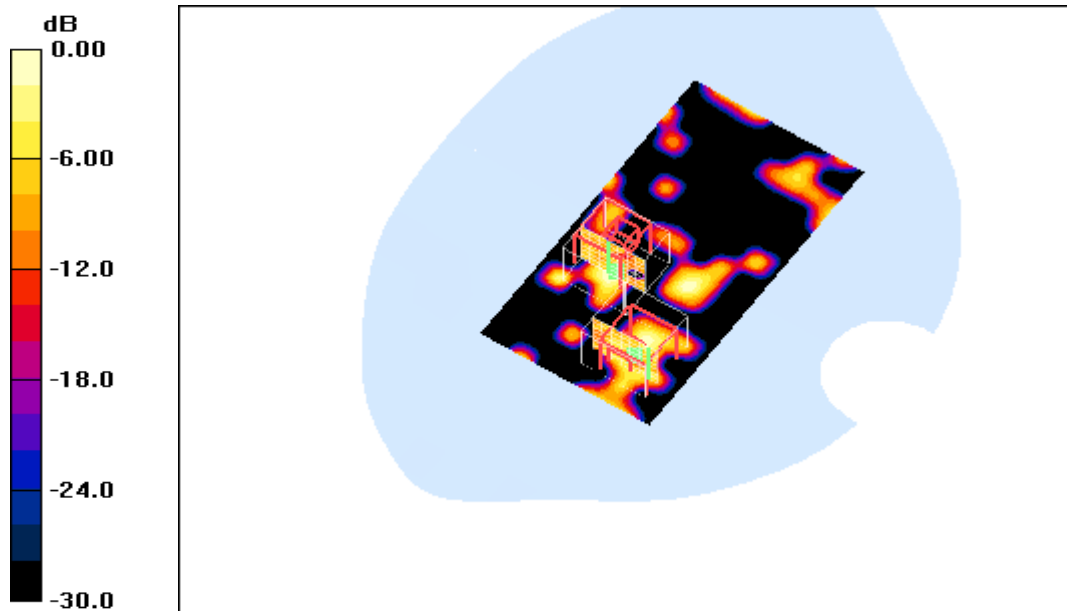

0 dB = 0.212mW/g

**Additional information:**

position or distance of DUT to SAM: DUT touching SAM  
 ambient temperature: 24.7°C; liquid temperature: 23.9°C

Date/Time: 29.04.2010 19:41:36 Date/Time: 29.04.2010 19:55:43

**IEEE1528\_OET65\_EN62209-2-Body-WLAN 5GHz**

**DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107**

Communication System: WLAN 5200; Frequency: 5320 MHz; Duty Cycle: 1:1

Medium: M5200 Medium parameters used:  $f = 5320 \text{ MHz}$ ;  $\sigma = 5.46 \text{ mho/m}$ ;  $\epsilon_r = 47.8$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 - SN3566; ConvF(3.42, 3.42, 3.42); Calibrated: 21.08.2009
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn413; Calibrated: 04.01.2010
- Phantom: SAM right; Type: SAM; Serial: 1042
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 146

**Front position - High 10 mm/Area Scan (81x151x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$

Maximum value of SAR (interpolated) = 0.491 mW/g


**Front position - High 10 mm/Zoom Scan (7x7x7) (8x8x8)/Cube 0:** Measurement grid:  $dx=4.3\text{mm}$ ,  $dy=4.3\text{mm}$ ,  $dz=3\text{mm}$

Reference Value = 9.44 V/m; Power Drift = -0.105 dB

Peak SAR (extrapolated) = 0.808 W/kg

**SAR(1 g) = 0.270 mW/g; SAR(10 g) = 0.136 mW/g**

Maximum value of SAR (measured) = 0.451 mW/g

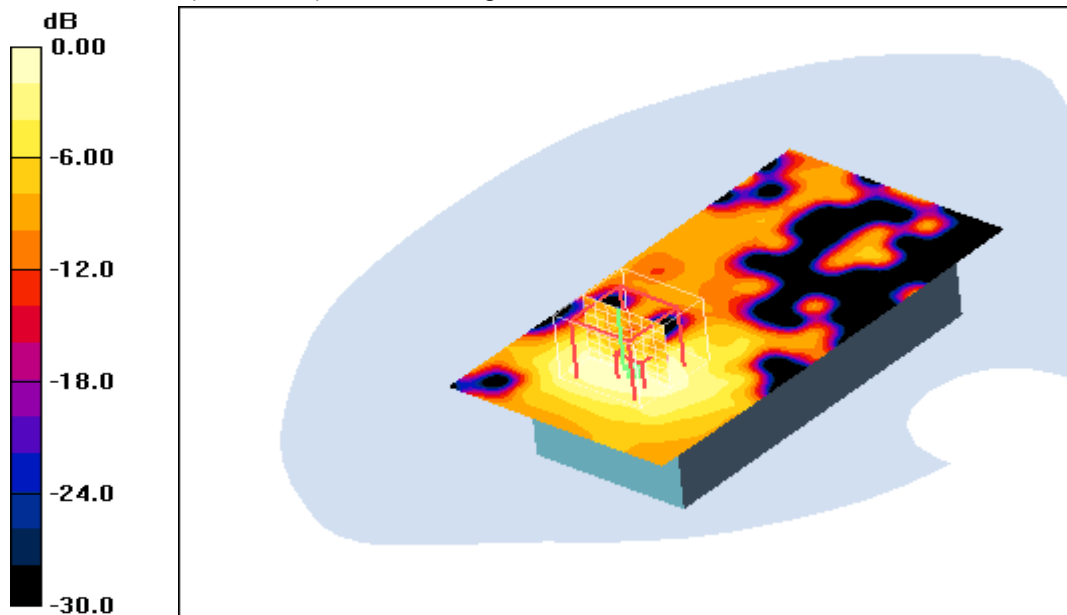

0 dB = 0.451mW/g

**Additional information:**

position or distance of DUT to SAM: DUT touching SAM

ambient temperature: 24.6°C; liquid temperature: 22.8°C

Date/Time: 30.04.2010 11:23:26 Date/Time: 30.04.2010 11:37:33

**IEEE1528\_OET65\_EN62209-2-Body-WLAN 5.8GHz**

**DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107**

Communication System: WLAN 5GHz; Frequency: 5745 MHz; Duty Cycle: 1:1

Medium: M5200 Medium parameters used (interpolated):  $f = 5745 \text{ MHz}$ ;  $\sigma = 5.99 \text{ mho/m}$ ;  $\epsilon_r = 46.8$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 - SN3566; ConvF(3.3, 3.3, 3.3); Calibrated: 21.08.2009

- Sensor-Surface: 2mm (Mechanical Surface Detection)

- Electronics: DAE3 Sn413; Calibrated: 04.01.2010

- Phantom: SAM right; Type: SAM; Serial: 1042

- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 146

**Rear position - Middle/Area Scan (81x151x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$

Maximum value of SAR (interpolated) = 0.212 mW/g

**Rear position - Middle/Zoom Scan (7x7x7) (8x8x8)/Cube 0:** Measurement grid:


$dx=4.3\text{mm}$ ,  $dy=4.3\text{mm}$ ,  $dz=3\text{mm}$

Reference Value = 5.28 V/m; Power Drift = 0.105 dB

Peak SAR (extrapolated) = 0.422 W/kg

**SAR(1 g) = 0.079 mW/g; SAR(10 g) = 0.025 mW/g**

Maximum value of SAR (measured) = 0.310 mW/g

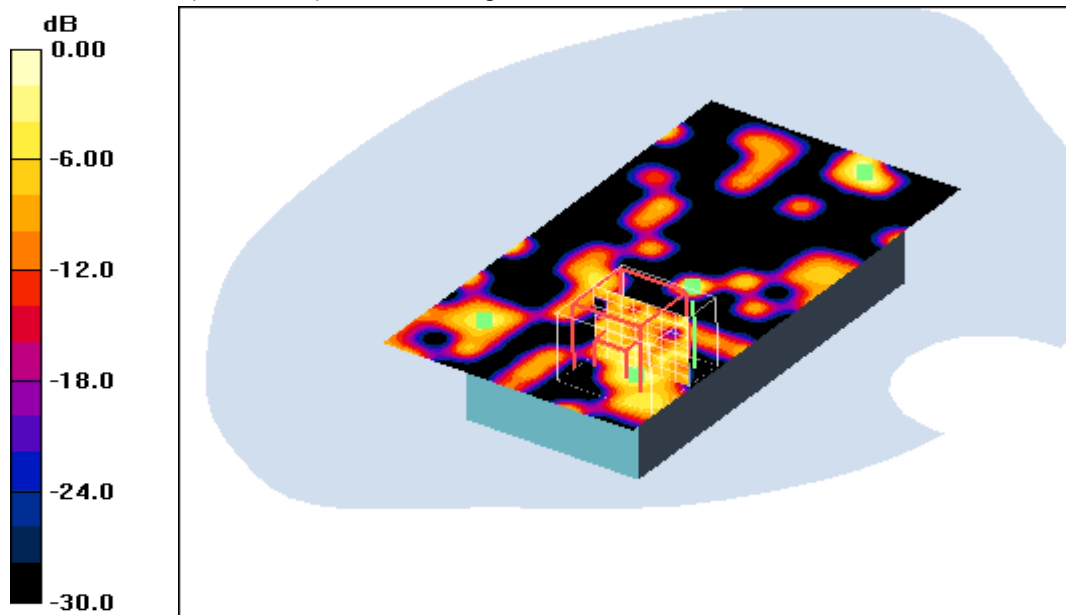

0 dB = 0.310mW/g

**Additional information:**

position or distance of DUT to SAM: DUT touching SAM

ambient temperature: 23.5°C; liquid temperature: 22.5°C



Date/Time: 29.04.2010 17:07:11 Date/Time: 29.04.2010 17:21:10

**IEEE1528\_OET65\_EN62209-2-Body-WLAN 5.8GHz**

**DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107**

Communication System: WLAN 5GHz; Frequency: 5745 MHz; Duty Cycle: 1:1

Medium: M5200 Medium parameters used (interpolated):  $f = 5745 \text{ MHz}$ ;  $\sigma = 5.99 \text{ mho/m}$ ;  $\epsilon_r = 46.8$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 - SN3566; ConvF(3.3, 3.3, 3.3); Calibrated: 21.08.2009

- Sensor-Surface: 2mm (Mechanical Surface Detection)

- Electronics: DAE3 Sn413; Calibrated: 04.01.2010

- Phantom: SAM right; Type: SAM; Serial: 1042

- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 146

**Front position - Low/Area Scan (81x151x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$

Maximum value of SAR (interpolated) = 1.84 mW/g

**Front position - Low/Zoom Scan (7x7x7) (8x8x8)/Cube 0:** Measurement grid:


$dx=4.3\text{mm}$ ,  $dy=4.3\text{mm}$ ,  $dz=3\text{mm}$

Reference Value = 19.3 V/m; Power Drift = 0.116 dB

Peak SAR (extrapolated) = 3.18 W/kg

**SAR(1 g) = 1.04 mW/g; SAR(10 g) = 0.361 mW/g**

Maximum value of SAR (measured) = 1.94 mW/g

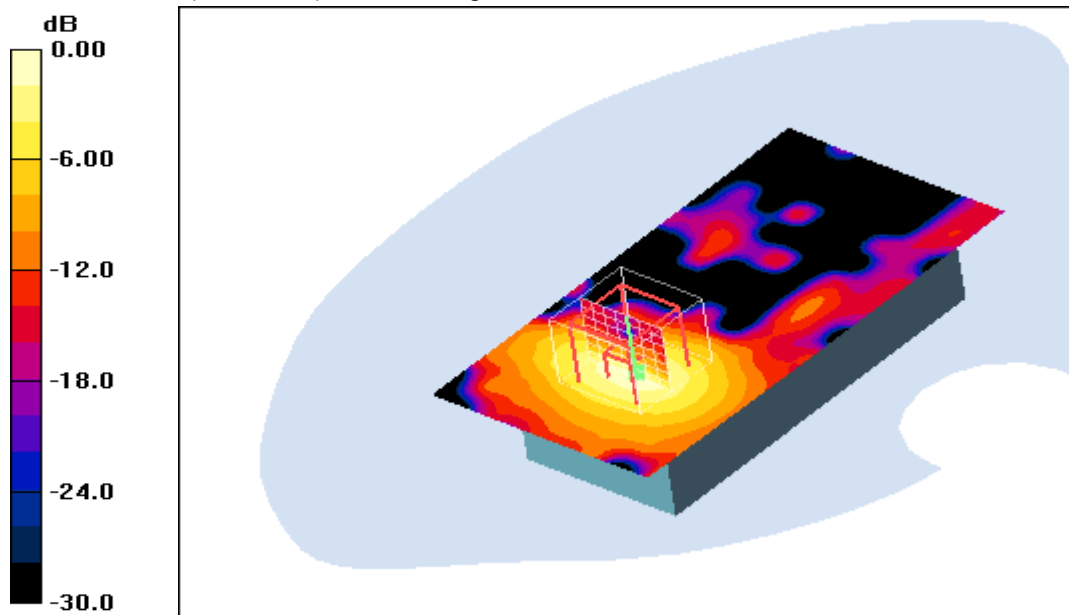

0 dB = 1.94mW/g

**Additional information:**

position or distance of DUT to SAM: 10 mm

ambient temperature: 24.4°C; liquid temperature: 22.7°C

Date/Time: 29.04.2010 17:45:33 Date/Time: 29.04.2010 17:59:32

**IEEE1528\_OET65\_EN62209-2-Body-WLAN 5.8GHz**

**DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107**

Communication System: WLAN 5GHz; Frequency: 5785 MHz; Duty Cycle: 1:1

Medium: M5200 Medium parameters used (interpolated):  $f = 5785 \text{ MHz}$ ;  $\sigma = 6.07 \text{ mho/m}$ ;  $\epsilon_r = 46.7$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 - SN3566; ConvF(3.3, 3.3, 3.3); Calibrated: 21.08.2009

- Sensor-Surface: 2mm (Mechanical Surface Detection)

- Electronics: DAE3 Sn413; Calibrated: 04.01.2010

- Phantom: SAM right; Type: SAM; Serial: 1042

- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 146

**Front position - Middle/Area Scan (81x151x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$

Maximum value of SAR (interpolated) = 1.55 mW/g

**Front position - Middle/Zoom Scan (7x7x7) (8x8x8)/Cube 0:** Measurement grid:


$dx=4.3\text{mm}$ ,  $dy=4.3\text{mm}$ ,  $dz=3\text{mm}$

Reference Value = 17.5 V/m; Power Drift = 0.030 dB

Peak SAR (extrapolated) = 4.51 W/kg

**SAR(1 g) = 0.841 mW/g; SAR(10 g) = 0.318 mW/g**

Maximum value of SAR (measured) = 1.56 mW/g

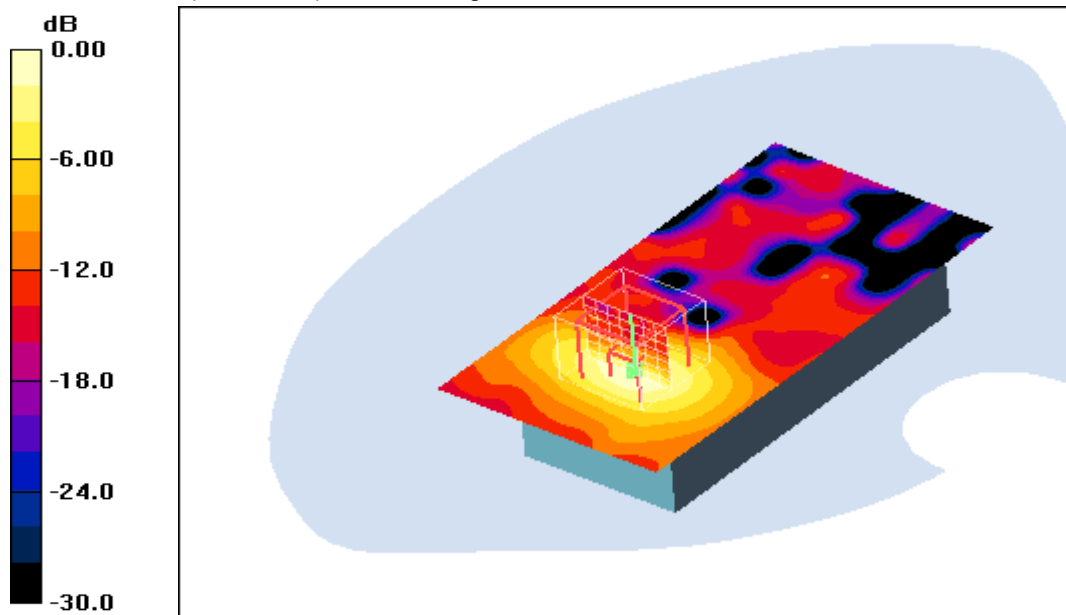

0 dB = 1.56mW/g

**Additional information:**

position or distance of DUT to SAM: 10 mm

ambient temperature: 24.4°C; liquid temperature: 22.7°C

Date/Time: 29.04.2010 18:23:04 Date/Time: 29.04.2010 18:36:53

**IEEE1528\_OET65\_EN62209-2-Body-WLAN 5.8GHz****DUT: Philips; Type: IntelliVue CL Transmitter; Serial: PN: 865221 / DE932Y0107**

Communication System: WLAN 5GHz; Frequency: 5825 MHz; Duty Cycle: 1:1

Medium: M5200 Medium parameters used:  $f = 5800$  MHz;  $\sigma = 6.1$  mho/m;  $\epsilon_r = 46.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV4 - SN3566; ConvF(3.3, 3.3, 3.3); Calibrated: 21.08.2009

- Sensor-Surface: 2mm (Mechanical Surface Detection)

- Electronics: DAE3 Sn413; Calibrated: 04.01.2010

- Phantom: SAM right; Type: SAM; Serial: 1042

- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 146

**Front position - High/Area Scan (81x151x1):** Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 1.30 mW/g

**Front position - High/Zoom Scan (7x7x7) (8x8x8)/Cube 0:** Measurement grid:


dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 16.0 V/m; Power Drift = -0.039 dB

Peak SAR (extrapolated) = 2.32 W/kg

**SAR(1 g) = 0.694 mW/g; SAR(10 g) = 0.289 mW/g**

Maximum value of SAR (measured) = 1.27 mW/g

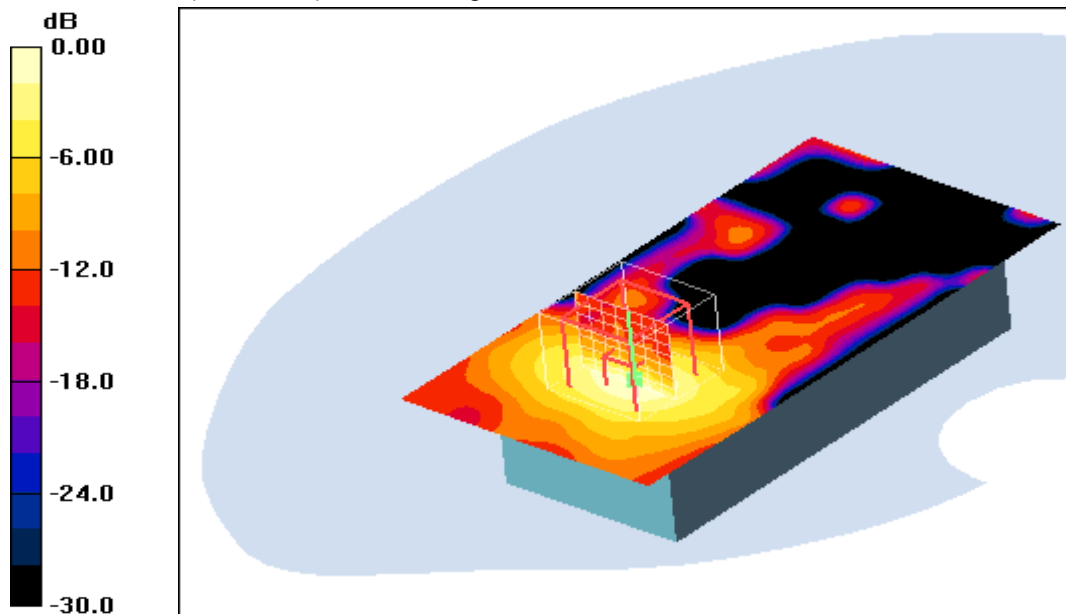


0 dB = 1.27mW/g

**Additional information:**


position or distance of DUT to SAM: 10 mm

ambient temperature: 24.4°C; liquid temperature: 22.7°C

**Annex B.3: Z-axis scan**

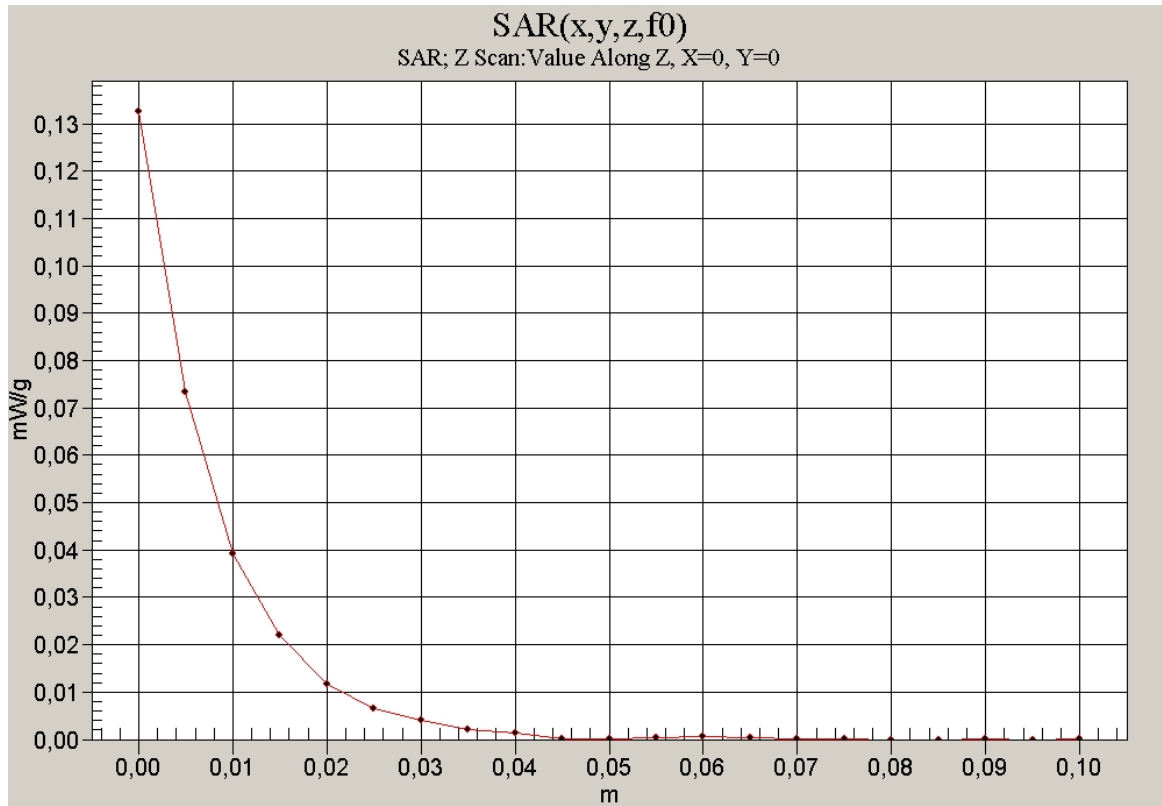

2450 MHz body

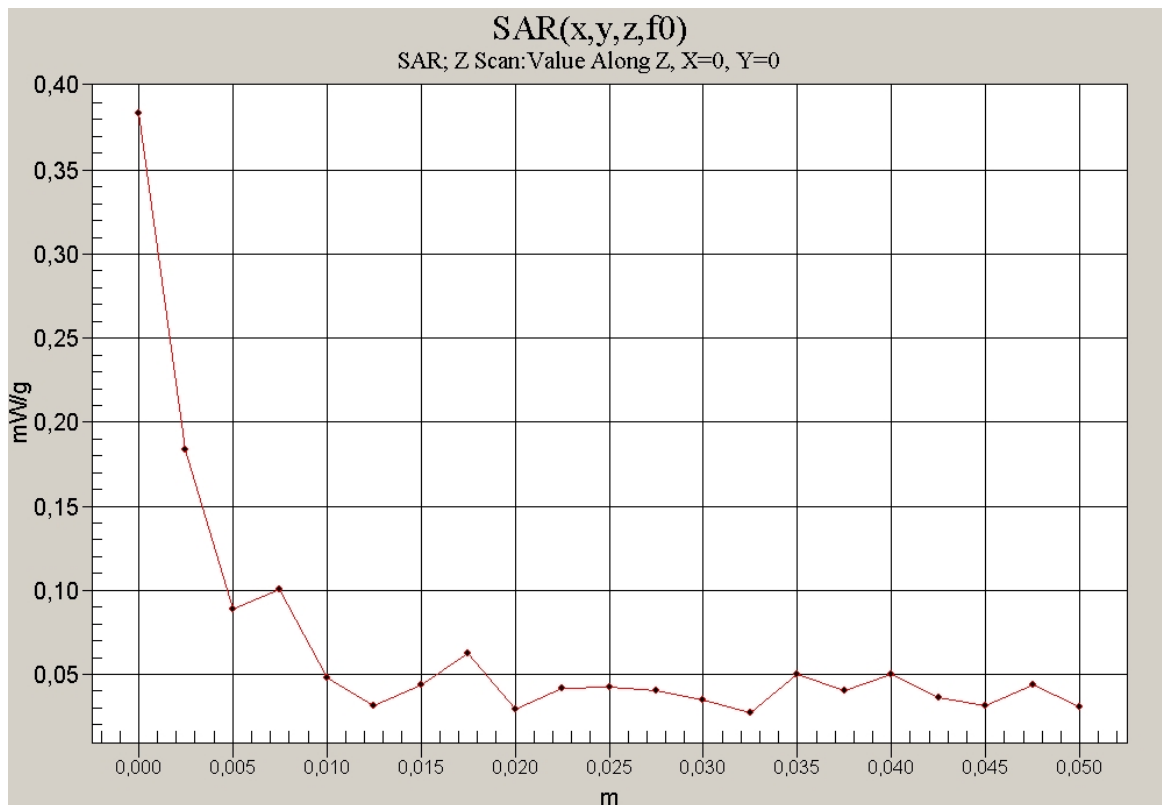

5 GHz body

**Annex D: RF Technical Brief Cover Sheet acc. to RSS-102 Annex A**

1. COMPANY NUMBER: 3549C
2. MODEL NUMBER: WLANBV1
3. MANUFACTURER: **Philips Medizin Systeme Böblingen GmbH**
4. TYPE OF EVALUATION:

SAR Evaluation: Body-worn Device

- Multiple transmitters: Yes  No
- Evaluated against exposure limits: General Public Use  Controlled Use
- Duty cycle used in evaluation: 100 %
- Standard used for evaluation: RSS-102 Issue 4 (2010-03)
- SAR value: **1.340 W/kg.**                      Measured  Computed  Calculated

**Annex D.5: Declaration of RF Exposure Compliance**

ATTESTATION: I attest that the information provided in Annex D: is correct; that a Technical Brief was prepared and the information it contains is correct; that the device evaluation was performed or supervised by me; that applicable measurement methods and evaluation methodologies have been followed and that the device meets the SAR and/or RF exposure limits of RSS-102.

Signature: 

Date: **2010-09-09**

NAME : **Thomas Vogler**

TITLE : Dipl.-Ing. (FH)

COMPANY : CETECOM ICT Services GmbH

## Annex E: Calibration parameters

Calibration parameters are described in the additional document :

### Appendix to test report no. 1-1775-01-14/09 Calibration data, Phantom certificate and detail information of the DASY4 System

## Annex F: Document History

| Version | Applied Changes  | Date of Release |
|---------|--|-----------------|
|         | Initial Release  | 2010-06-21      |
| A       | Model name updated, WLAN conducted power updated,<br>Conducted Power Settings updated<br>Test item details included. | 2010-09-09      |

## Annex G: Further Information

### Glossary

|          |   |                                  |
|----------|---|----------------------------------|
| DUT      | - | Device under Test                |
| EUT      | - | Equipment under Test             |
| FCC      | - | Federal Communication Commission |
| FCC ID   | - | Company Identifier at FCC        |
| HW       | - | Hardware                         |
| IC       | - | Industry Canada                  |
| Inv. No. | - | Inventory number                 |
| N/A      | - | not applicable                   |
| SAR      | - | Specific Absorption Rate         |
| S/N      | - | Serial Number                    |
| SW       | - | Software                         |