


M2720A Cordless Fetal Transducer System Labeling

Transducer top




Parameter
 * Toco
 * US
 * ECG

All other labels moved to bottom

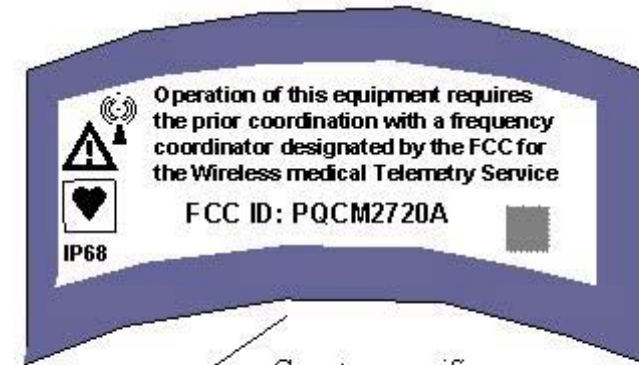

Country specific regulatory labels

Transducer bottom

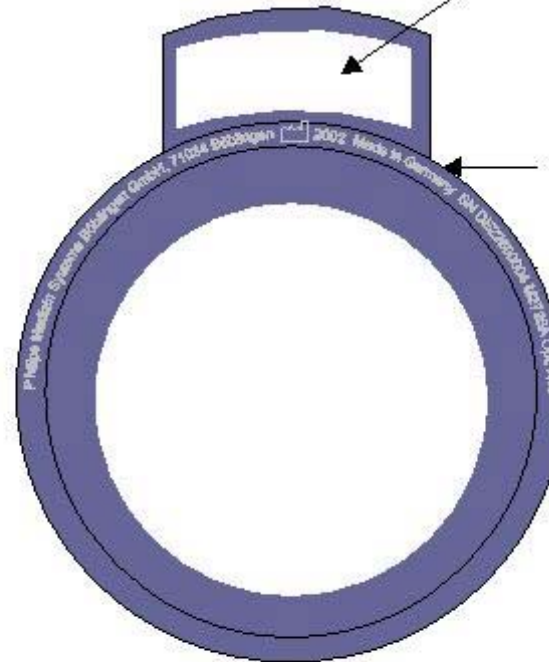


Manufacturing address, date, country of origin, serial number, product number (M2725A, M2726A, M2727A) and RF version (Laser printed)

For manufacturing:
 2D barcode (3mm*3 mm)

Print 1 slide/page for correct size

Labels and symbols are not scaled!

M2720A Base Station Labeling

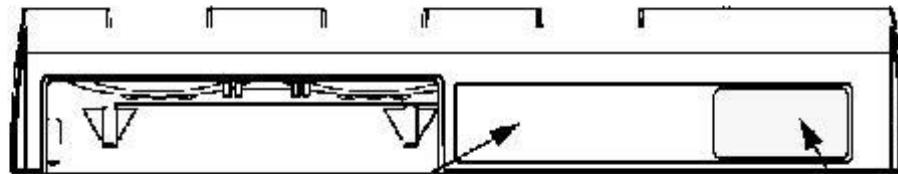


SN label

PTT and Warning label

 <p>Philips Medizin Systeme Boeblingen GmbH 71034 Boeblingen Germany</p> <p>REF M2720A *M2720A* SN DE22400001 *DE22400001* Opt.: A15 Made in Germany</p>	 0388  IPX1 	<p>M2720A  Tested To Comply With FCC Standards FOR HOME OR OFFICE USE</p> <p>IC: 123456789</p> <p>CAUTION: SHOCK HAZARD. DO NOT REMOVE COVER. SERVICE BY QUALIFIED PERSONNEL ONLY.</p> <p>THIS ISM DEVICE COMPLIES WITH CANADIAN ICES-001. CET APPAREIL ISM EST CONFORME A LA NORME NMB-001 DU CANADA.</p>
------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------	-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------	-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

*Manufacturing date
being updated every month*

*Print 1 slide/page for correct size of rear label
(3 of 9 Barcode and Philips fonts required)*

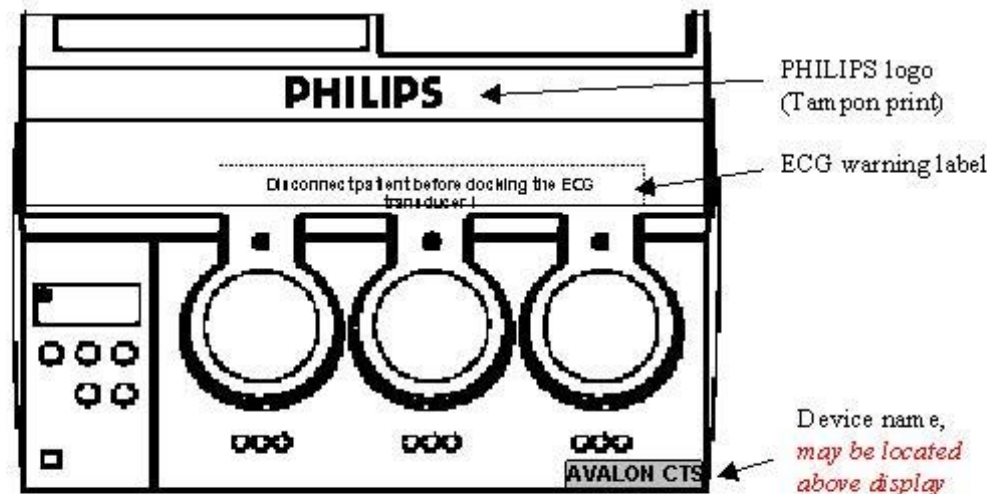

Labels and symbols are not scaled!