

M3814A

SN: US00000000 Proper To UID: 00108351ABCD

This device complies with part 15 of the FCC rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference and (2) this device must accept any interference received, including interference that may cause undesired operation. Except for batteries, no user serviceable parts inside. Made in USA of foreign and domestic components. Property of Philips Medical Systems, Andover, MA. Rx Only.

To return unit, please call toll free 866-246-7316

entela


FC FCC ID: POCM38 14

Certified

A-M3814-80002-1 Rev: A

PHILIPS MEDICAL SYSTEMS RESTRICTED
THIS DOCUMENT AND ANY ASSOCIATED DATA
CONTAIN RESTRICTED INFORMATION THAT IS
PHILIPS MEDICAL SYSTEMS PROPERTY.
ONLY DISCLOSE OR DUPLICATE FOR OTHERS
AS AUTHORIZED BY PHILIPS MEDICAL SYSTEMS.

ENG	GINEERING RESPONSIBILI	B-M3810-80008-1			
REV	REF	REVISION DESCRIPTION		CHANGED BY	DATE
Α	29C4-2002-10-00980	AS ISSUED		S J BLACKER	21-0CT-02

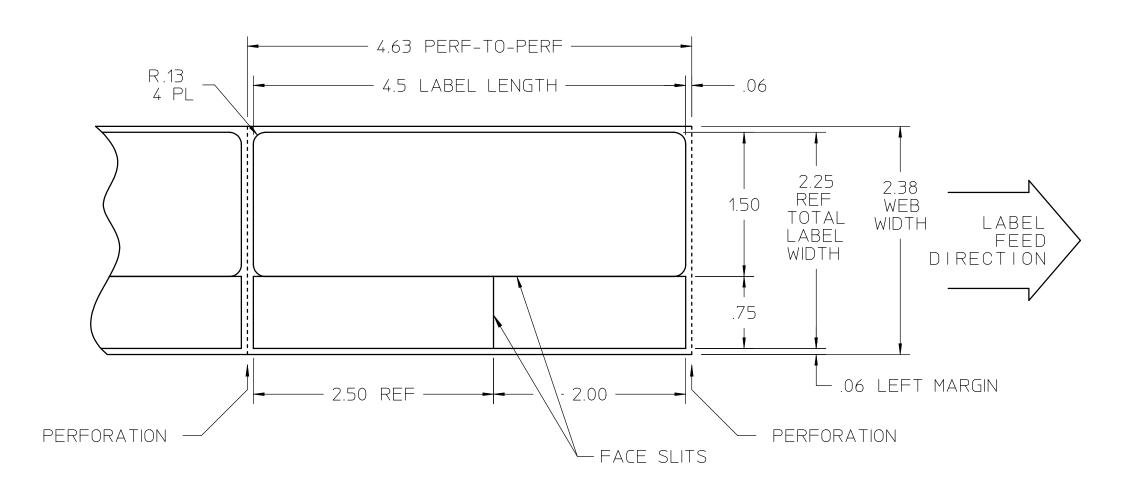

<u>NOTES</u>

1. MATERIAL: CSA ACCEPTED ZEBRA Z-ULTIMATE 3000 WHITE, GLOSS POLYESTER WITH PERMANENT ACRYLIC ADHESIVE ON PERFORATED RELEASE LINER.

2. LABELS ROLLED ON 3 IN I.D. CORE SO THAT THE LABELS UNWIND FROM THE OUTSIDE

3. 1350 LABELS PER ROLL (ROLL O.D. 7.9 INCHES)

4. VENDOR: ZEBRA TECHNOLOGIES

333 CORPORATE WOODS PARKWAY VERNON HILLS, ILLINOIS 60061

TEL: 847-634-6700

UNLESS OTHERWISE SPECIFIED							
ODIMENSIONS ARE IN INCHES OTHERD ANGLE PROJECTION	ITEM	QTY	U/M	MATERIAL DESCRIPTION			MATL-PART NO
• TOLERANCES X.X ± .020 ANGLES ± 1°	NAME		DATE	MODEL RATING &		PHILIPS	
X.XX ± .010	ACT Inc		07 – JUN – 02	SN/UID			
X.XXX ± .005 FEATURES PER NOTES	GIL LEMKE		07 – JUN – 02				
O ADHERENCE TO DWG A-5951-1561-1 (CORP STD SECTION 608) REQUIRED					LABEL STOCK	PART NUMBER	M3810-80008
• ADHERENCE TO ASME SPEC. Y14.5M REVISION 1994 REQUIRED	DO NO	T TAKE	3810-80008-1				