

Contents

10.APPENDIX.....	127
10.1 Photographs of Test Setup.....	127
10.2 Photographs of the EUT	131

10.APPENDIX

10.1 Photographs of Test Setup

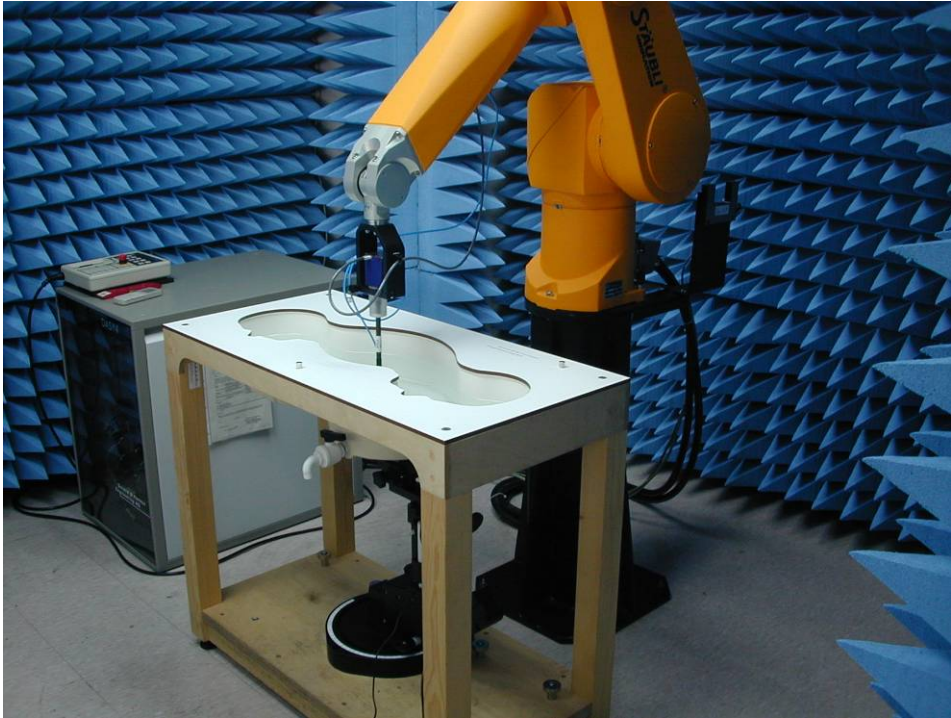


Fig.1 Photograph of the SAR measurement System

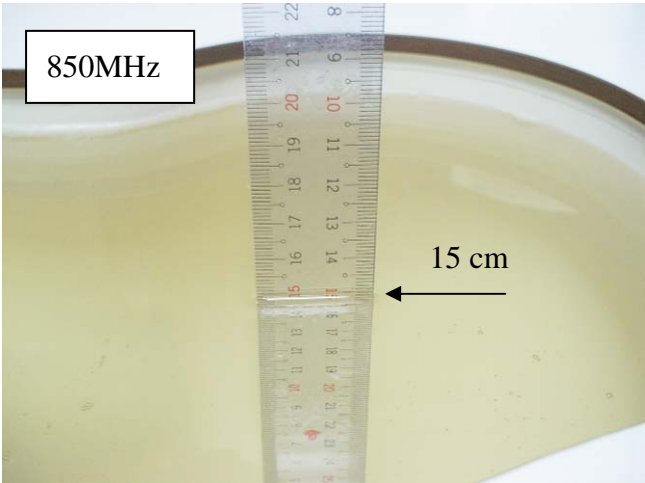


Fig.2.1 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Left-head Side

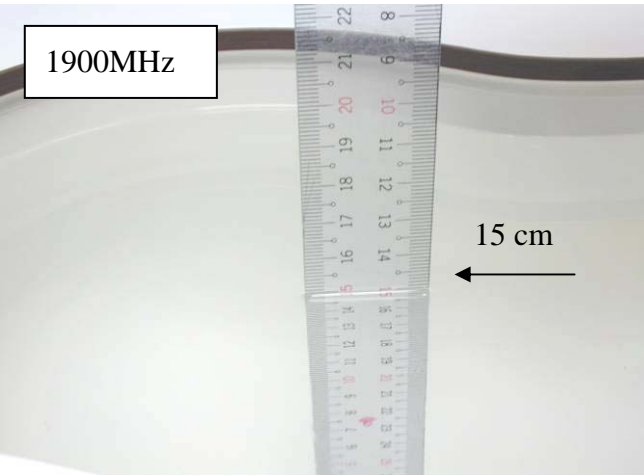


Fig.2.2 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Right-head Side

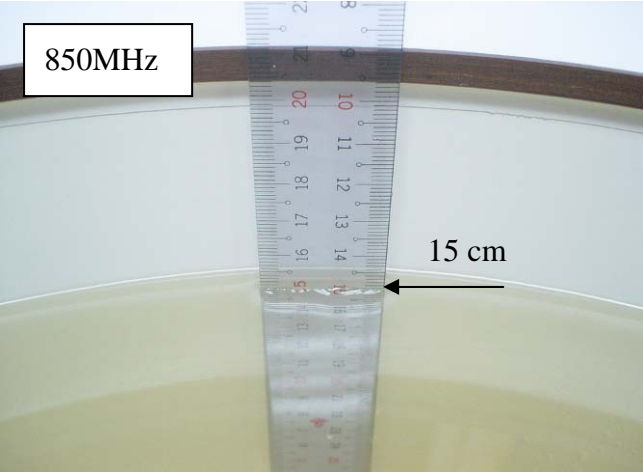


Fig.2.3 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

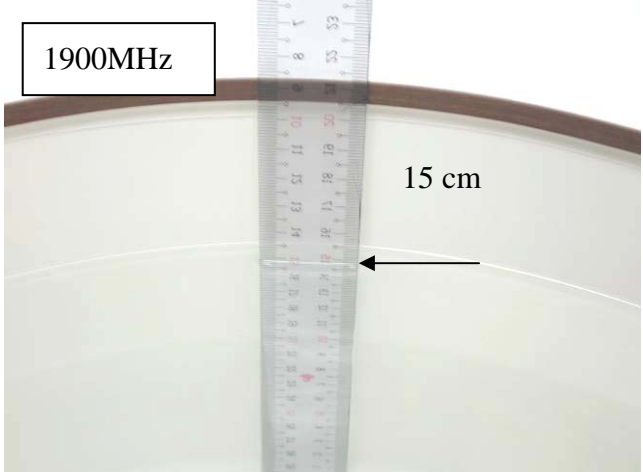


Fig.2.4 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

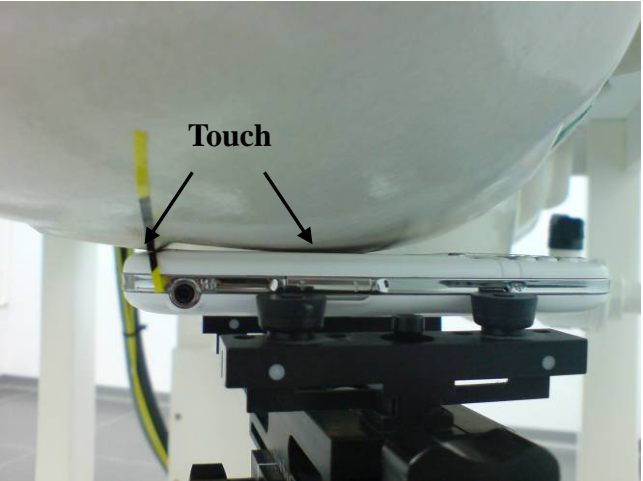


Fig.3 Right Head Section / Cheek-Touch Position

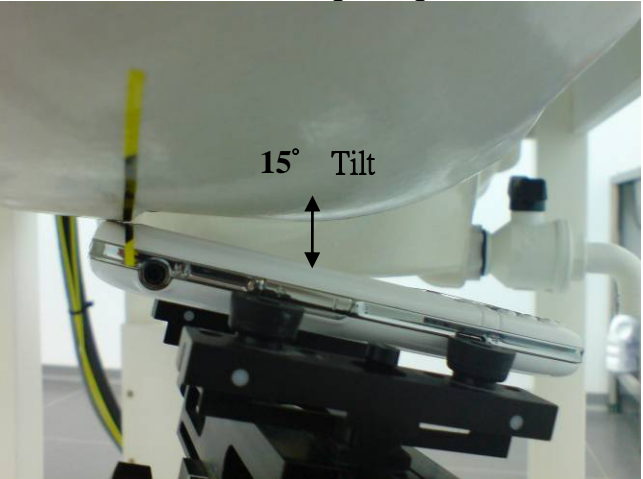
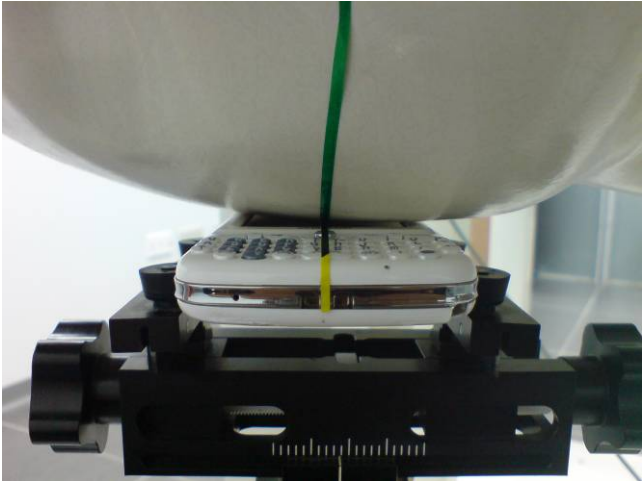
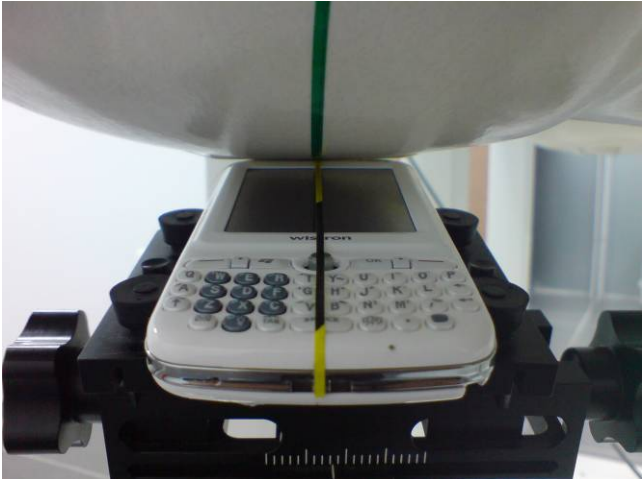


Fig.4 Right Head Section / Ear-Tilt Position(15°)



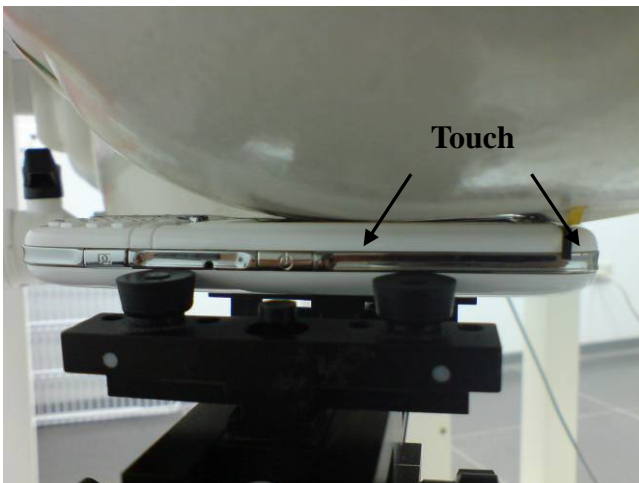


Fig.5 Left Head Section / Cheek-Touch Position

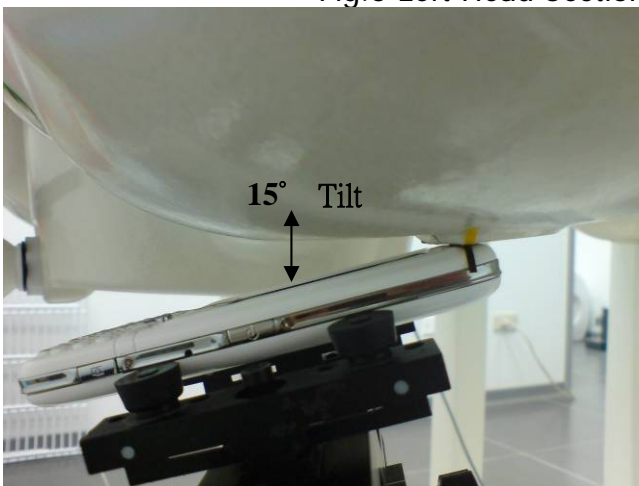
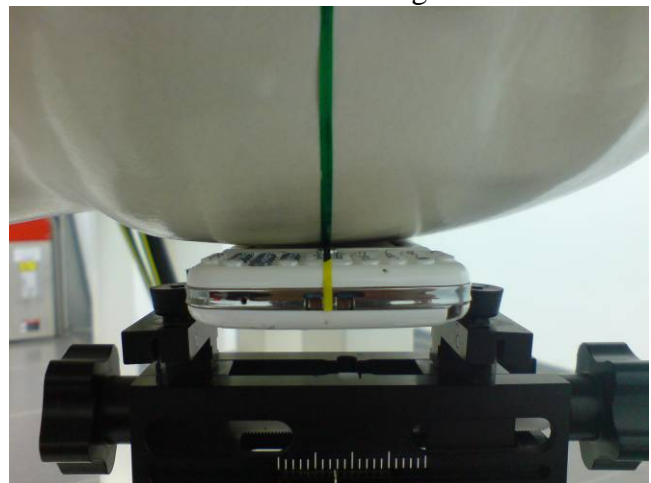


Fig.6 Left Head Section / Ear-Tilt Position(15°)

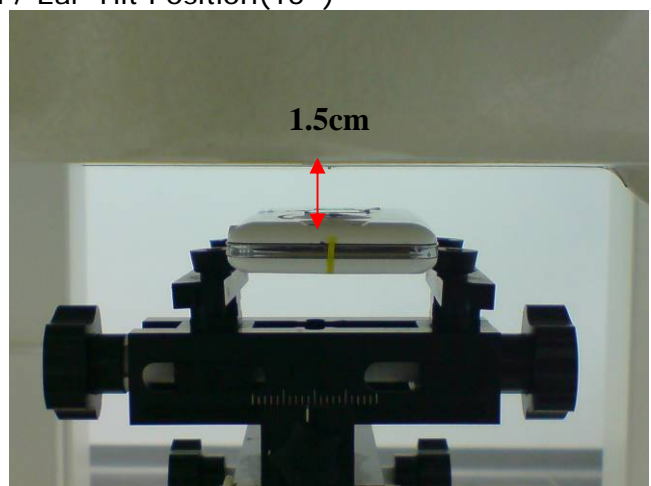


Fig.7 Body worn- EUT back to flat phantom and distance between flat phantom and mobile phone is 1.5 cm

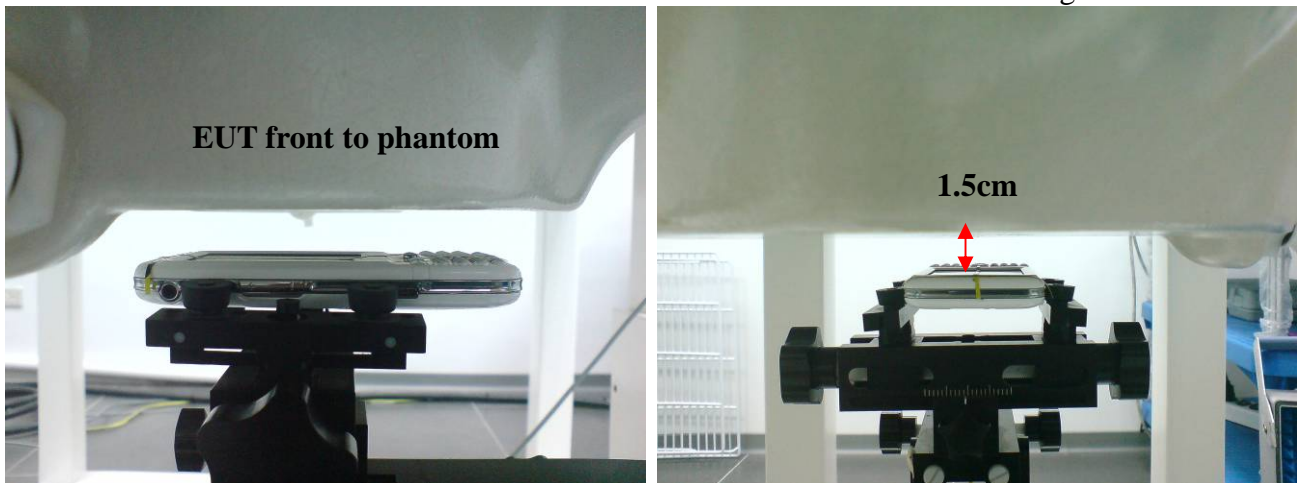


Fig.8 Body worn- EUT front to flat phantom and distance between flat phantom and mobile phone is 1.5 cm

10.2 Photographs of the EUT



Fig.9 Front view of device

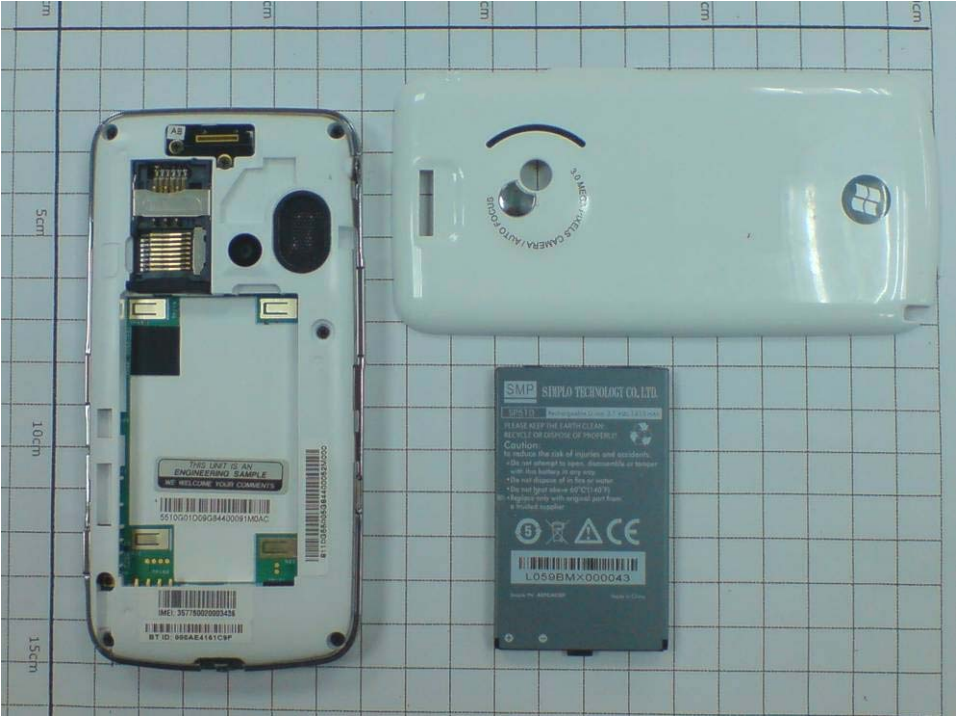


Fig.10 Back view of device



Fig.11 Left view of device

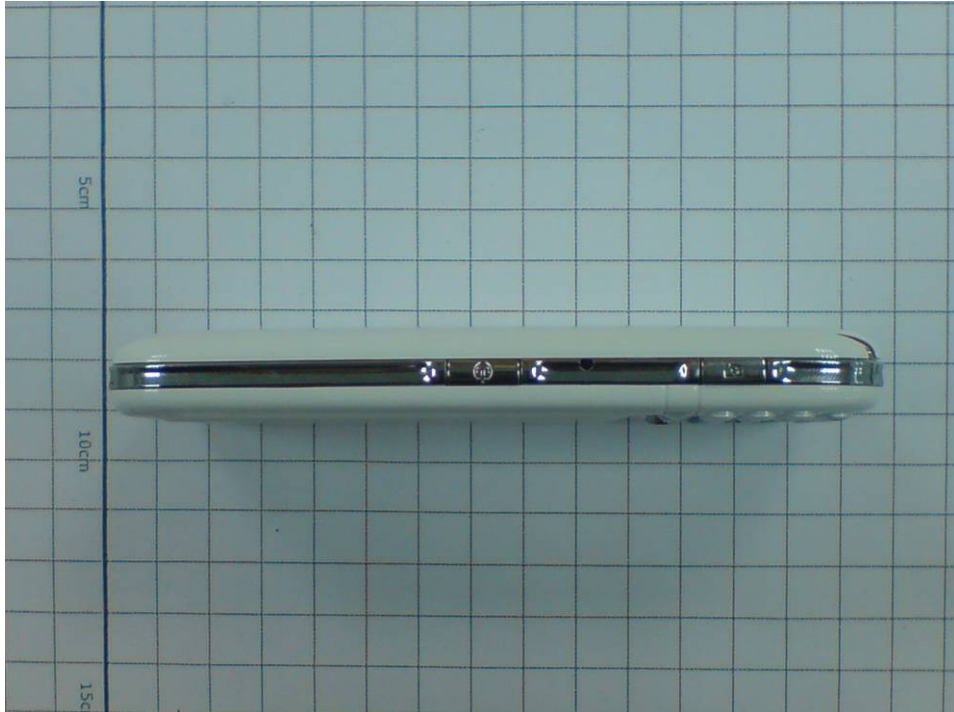


Fig.12 Right view of device



Fig.13 Front view of Battery



Fig.14 Back view of Battery



Fig.15 AC Charger

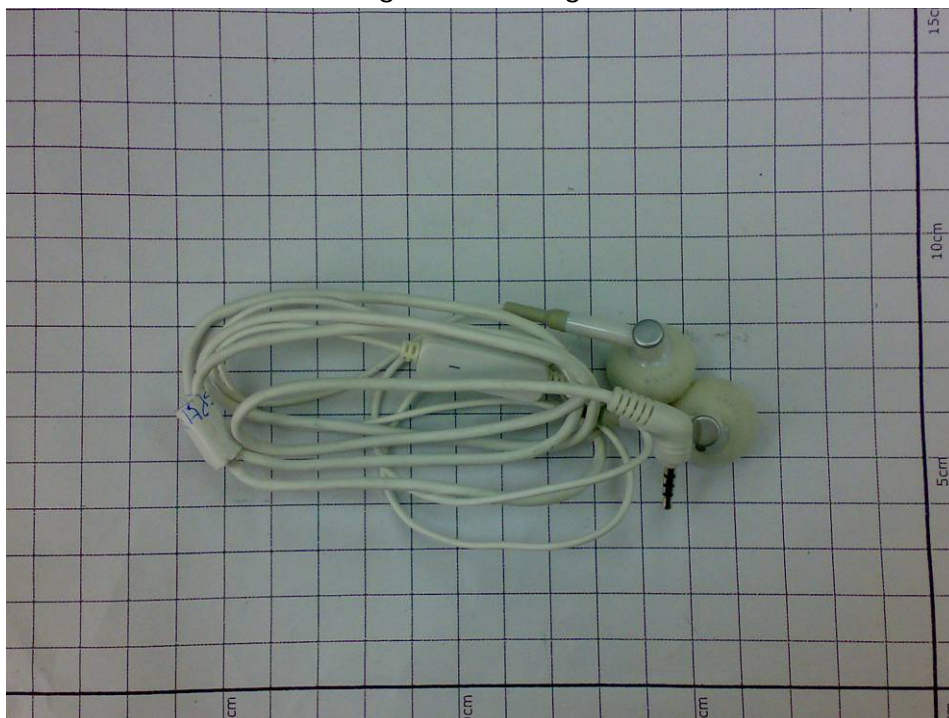


Fig.16 Headset

End of Report