

## System Check\_Head\_750MHz

**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: HSL\_750\_240111 Medium parameters used:  $f = 750.000$  MHz;  $\sigma = 0.894$  S/m;  $\epsilon_r = 43.1$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.84, 9.43, 10.43); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.448 W/kg; SAR (10g) = 0.299 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.07 dB

SAR (1g) = 0.440 W/kg; SAR (8g) = 0.312 W/kg; SAR (10g) = 0.296 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 90.1 %

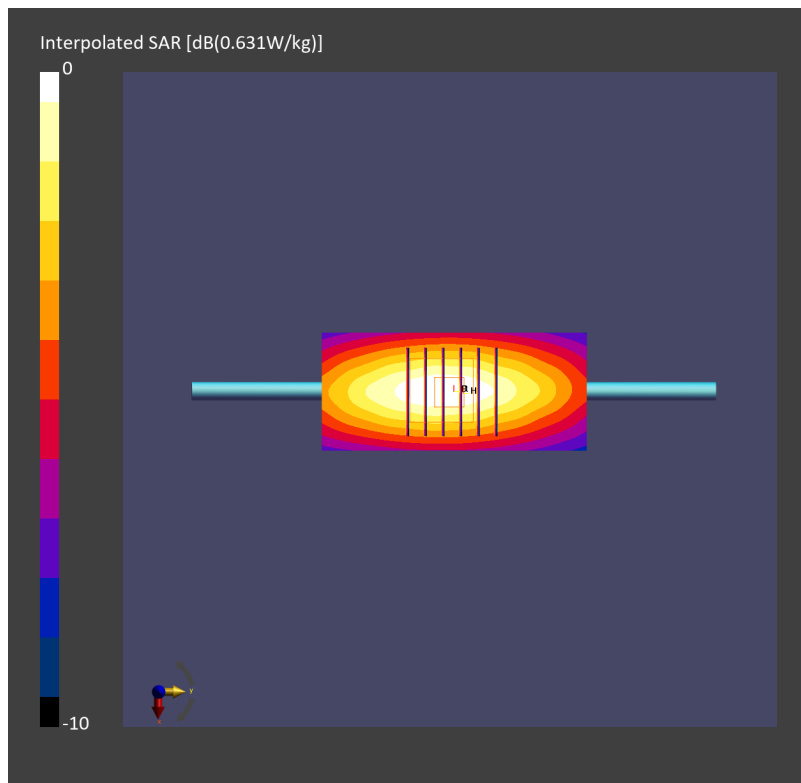

## System Check\_Head\_835MHz

**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: HSL\_850\_240109 Medium parameters used:  $f=835.000$  MHz;  $\sigma=0.930$  S/m;  $\epsilon_r=42.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.35, 9.19, 10.14); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.512 W/kg; SAR (10g) = 0.338 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 0.517 W/kg; SAR (8g) = 0.363 W/kg; SAR (10g) = 0.344 W/kg

Smallest distance from peaks to all points 3 dB below = 22.1 mm

Ratio of SAR at M2 to SAR at M1 = 89.8 %

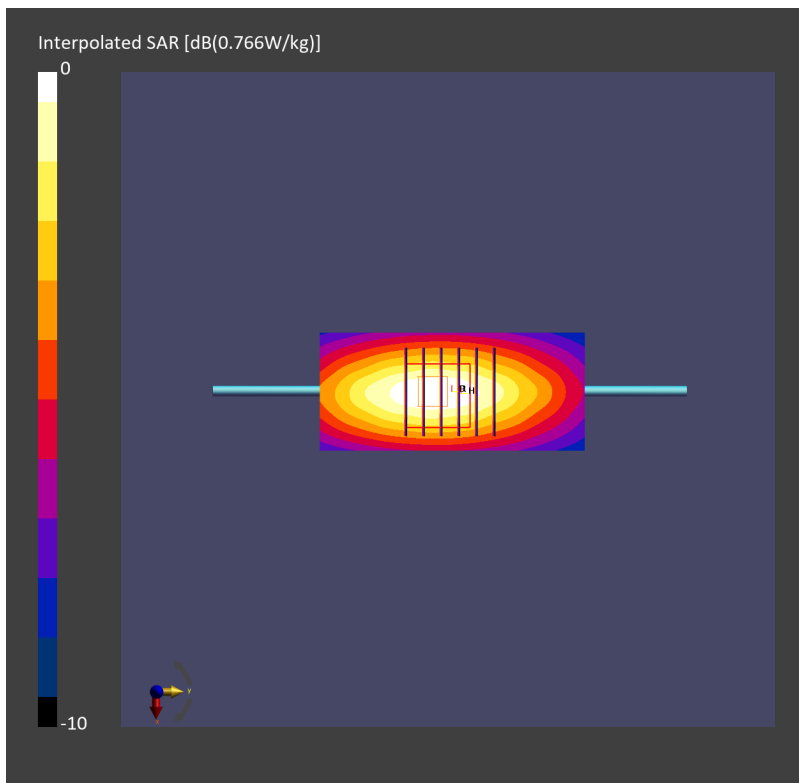

## System Check\_Head\_1750MHz

### DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1

Medium: HSL\_1750\_240110 Medium parameters used:  $f=1750.000$  MHz;  $\sigma=1.35$  S/m;  $\epsilon_r=40.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(8.66, 8.71, 9.35); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.69 W/kg; SAR (10g) = 0.897 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.72 W/kg; SAR (8g) = 1.00 W/kg; SAR (10g) = 0.927 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 82.5 %

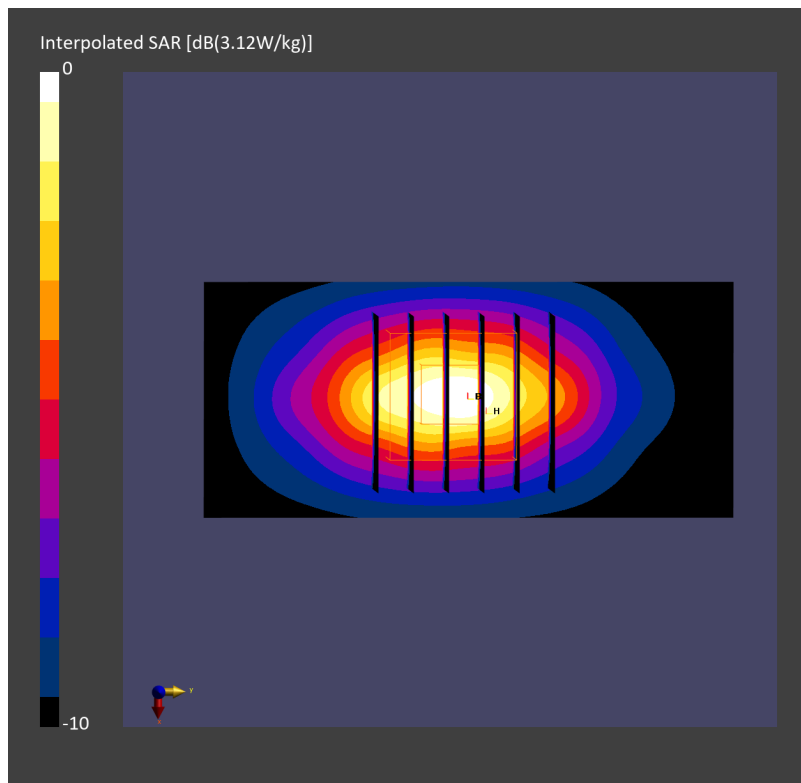

## System Check\_Head\_1900MHz

### DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: HSL\_1900\_240109 Medium parameters used:  $f=1900.000$  MHz;  $\sigma=1.42$  S/m;  $\epsilon_r=40.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(8.0, 8.07, 8.72); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.77 W/kg; SAR (10g) = 0.912 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.03 dB

SAR (1g) = 1.77 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.945 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 85.8 %

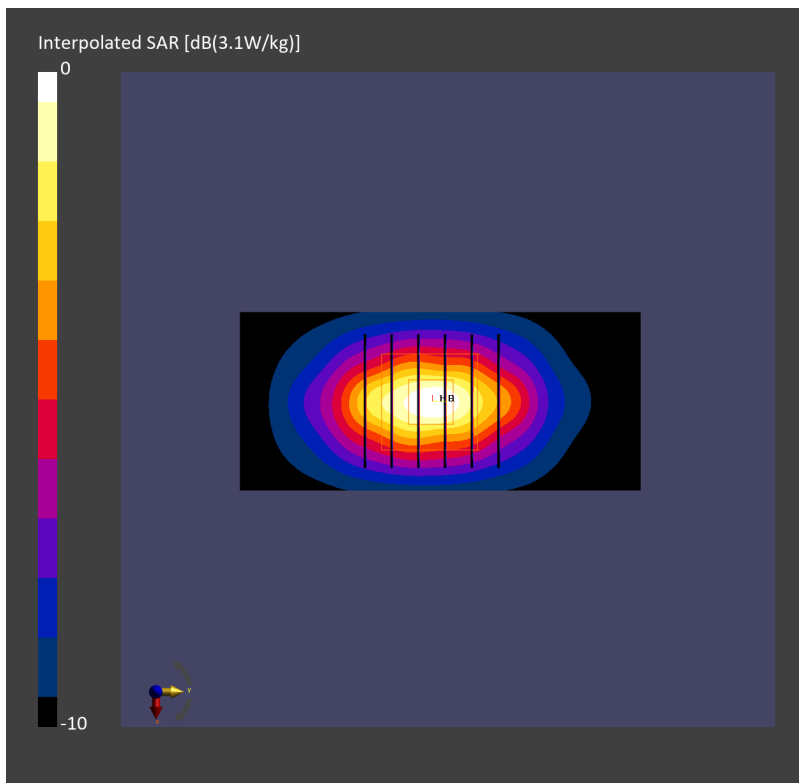

## System Check\_Head\_2300MHz

### DUT: D2300V2 - SN1006

Communication System: CW; Frequency: 2300.000 MHz; Duty Cycle: 1:1

Medium: HSL\_2300\_240109 Medium parameters used:  $f=2300.000$  MHz;  $\sigma=1.64$  S/m;  $\epsilon_r=39.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.71, 7.81, 8.42); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.46 W/kg; SAR (10g) = 1.14 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.48 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.0 %

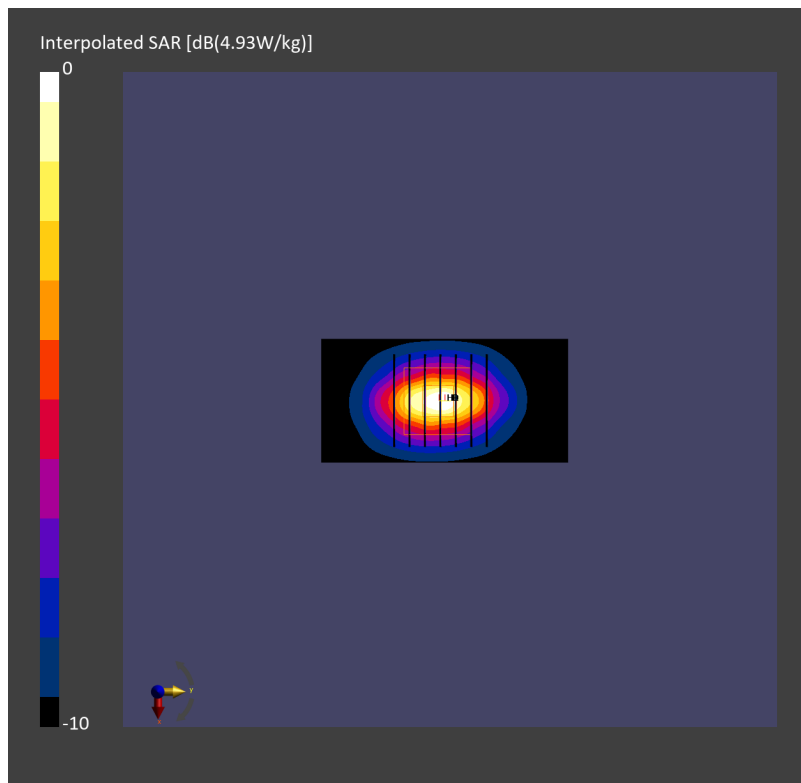

## System Check\_Head\_2600MHz

### DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: HSL\_2600\_240110 Medium parameters used:  $f=2600.000$  MHz;  $\sigma=2.00$  S/m;  $\epsilon_r=39.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.5, 7.6, 8.24); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.52 W/kg; SAR (10g) = 1.14 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.56 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.0 %

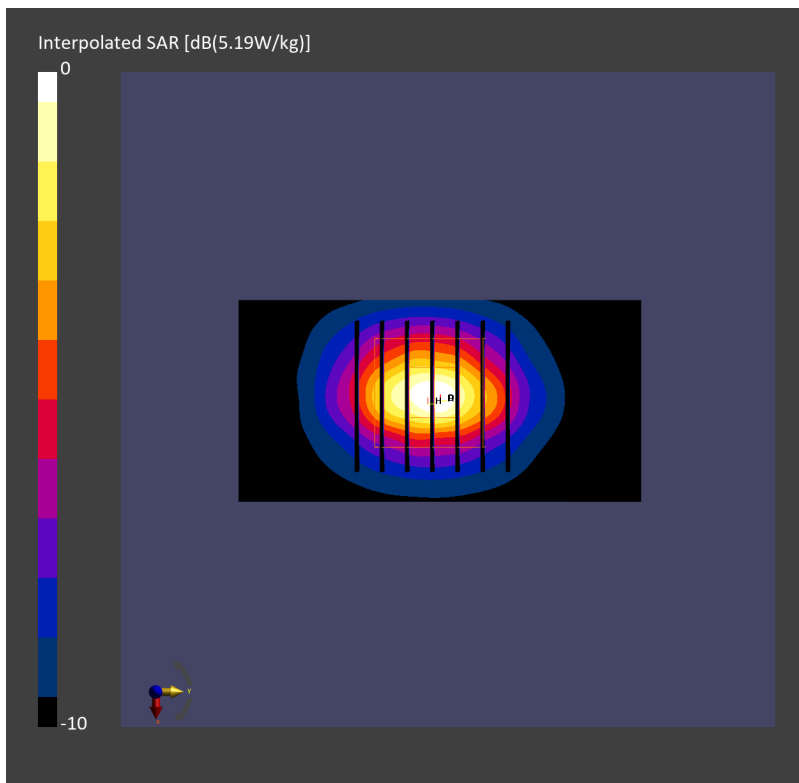

## System Check\_Head\_2600MHz

### DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1  
Medium: HSL\_2600\_240113 Medium parameters used:  $f=2600.000$  MHz;  $\sigma=1.98$  S/m;  $\epsilon_r=38.1$   
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.5, 7.6, 8.24); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm  
SAR (1g) = 2.59 W/kg; SAR (10g) = 1.16 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.08 dB

SAR (1g) = 2.57 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.7 %

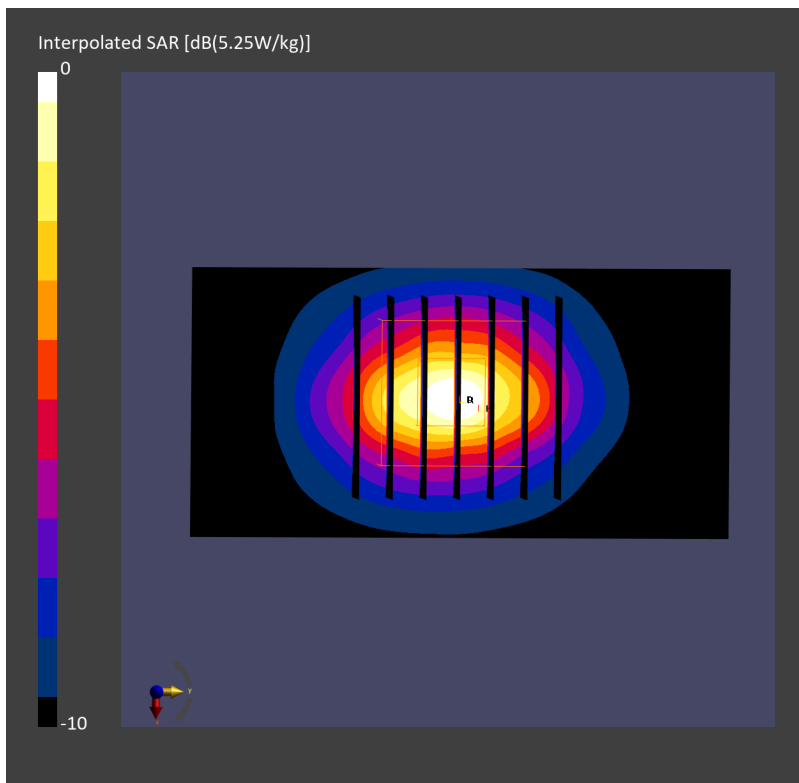

## System Check\_Head\_3500MHz

### DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: HSL\_3500\_240112 Medium parameters used:  $f=3500.000$  MHz;  $\sigma=3.03$  S/m;  $\epsilon_r=38.0$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.07, 7.19, 7.75); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.07 W/kg; SAR (10g) = 1.17 W/kg;


**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.14 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

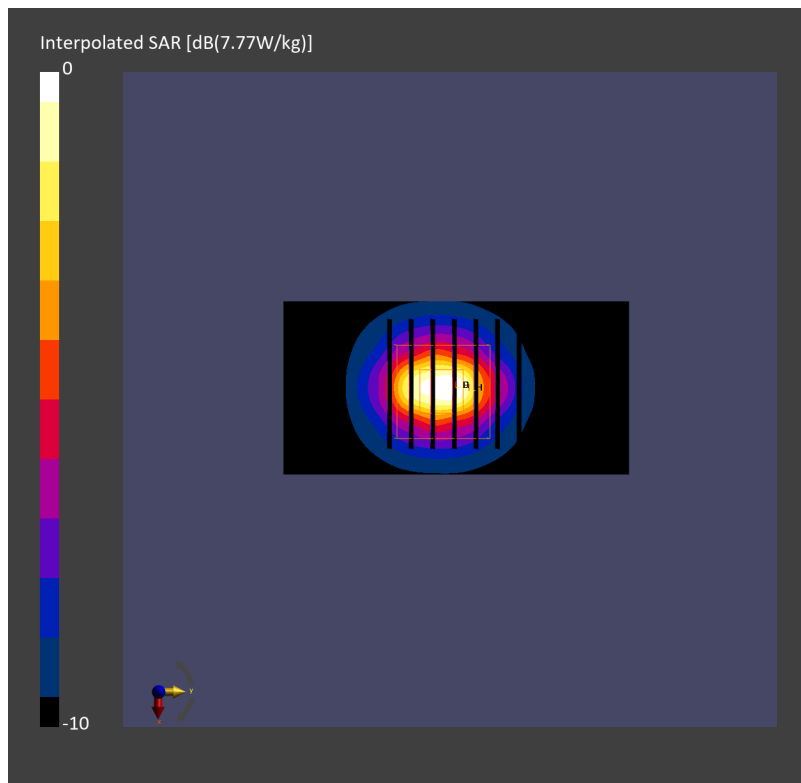



## System Check\_Head\_3700MHz

### DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz; Duty Cycle: 1:1

Medium: HSL\_3700\_240112 Medium parameters used:  $f=3700.000$  MHz;  $\sigma=3.22$  S/m;  $\epsilon_r=37.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.89, 7.01, 7.57); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.07 W/kg; SAR (10g) = 1.14 W/kg;

**Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.14 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.6 %

