

**Test Report**

**Conducted Output Power GSM850/PCS1900**

**SIEMENS A31a**

**Report No: Finch LAM\_Conducted\_Power.doc**

**Issue date: Jan 19, 2006**

**Test Sites: ST-HWC BEJ**

**Phone: +86 10 64748800-7305**

Ma Xin     *Ma Xin*  
RF Test Engineer, System Test  
Zhou Li Dong  
EMC Test Engineer

**Contents**

1 Objective and Method .....3

2 Device under test.....3

3 Measurement Set-up .....3

4 Test Result .....5

Annex 1 Calibration Certificate.....7

### 1 Objective and Method


FCC approval for mobile phone requires reporting output power at RF output terminal pursuant to title 47 CFR part 2.1046. BenQ SIEMENS devices use special test fixtures with 50 Ohm connection suitable for such measurements. Using a special adapter and connecting the phone to an appropriate load in terms of the input port of the measurement equipment used, we hereby report the values for highest power setting.

### 2 Device under test

Mobile Phone: Siemens A31a (GSM850/PCS1900)  
 Frequency Range GSM 850: 824– 894MHz  
 Frequency Range PCS 1900: 1850 – 1990 MHz

There are 10 devices has been tested listed in “Chapter 4 Test Result”.

### 3 Measurement Set-up

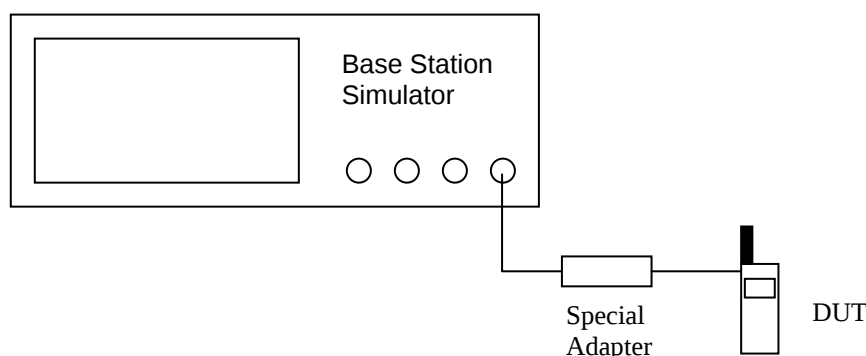

**Figure 1: Block Diagram of set-up for conducted power measurement**

|                           |                      |
|---------------------------|----------------------|
| Base Station Simulator    | CMU 200              |
| Serial Number             | 105851               |
| Software Version          | Base 3.81 / GSM 3.80 |
| Calibration Certification | Annex 1              |

Test Voltage: 4.0 V  
 Temperature: Room Temperature



Figure 2: Set-up for conducted power measurement

#### 4 Test Result

##### Conducted Output Power (GSM850 Band)

| EUTs       |              | Average Power during burst at phone connector (dBm) |                      |                      |
|------------|--------------|-----------------------------------------------------|----------------------|----------------------|
| A31a       | IMEI         | Ch. 128<br>824.2 MHz                                | Ch. 190<br>836.6 MHz | Ch. 251<br>848.8 MHz |
| Sample #1  | 004400043312 | 31.5                                                | 31.5                 | 31.6                 |
| Sample #2  | 004400043023 | 31.5                                                | 31.6                 | 31.6                 |
| Sample #3  | 004400042991 | 31.6                                                | 31.6                 | 31.6                 |
| Sample #4  | 004400043080 | 31.4                                                | 31.5                 | 31.5                 |
| Sample #5  | 004400043049 | 31.5                                                | 31.6                 | 31.6                 |
| Sample #6  | 004400042975 | 31.5                                                | 31.6                 | 31.5                 |
| Sample #7  | 004400043189 | 31.6                                                | 31.7                 | 31.7                 |
| Sample # 8 | 004400043163 | 31.5                                                | 31.5                 | 31.5                 |
| Sample # 9 | 004400043452 | 31.6                                                | 31.6                 | 31.6                 |
| Sample #10 | 004400043031 | 31.4                                                | 31.5                 | 31.5                 |

**Conducted Output Power (PCS1900 Band)**

| <b>EUTs</b> |              | <b>Average Power during burst at phone connector (dBm)</b> |                               |                               |
|-------------|--------------|------------------------------------------------------------|-------------------------------|-------------------------------|
| <b>A31a</b> | <b>IMEI</b>  | <b>Ch. 512<br/>1850.2 MHz</b>                              | <b>Ch. 661<br/>1880.0 MHz</b> | <b>Ch. 810<br/>1909.8 MHz</b> |
| Sample #1   | 004400043312 | 28.7                                                       | 28.5                          | 29.1                          |
| Sample #2   | 004400043023 | 28.9                                                       | 28.7                          | 29.3                          |
| Sample #3   | 004400042991 | 28.9                                                       | 28.6                          | 29.3                          |
| Sample #4   | 004400043080 | 28.9                                                       | 28.7                          | 29.3                          |
| Sample #5   | 004400043049 | 28.7                                                       | 28.5                          | 29.1                          |
| Sample #6   | 004400042975 | 28.9                                                       | 28.6                          | 29.3                          |
| Sample #7   | 004400043189 | 28.8                                                       | 28.6                          | 29.2                          |
| Sample # 8  | 004400043163 | 28.8                                                       | 28.5                          | 29.2                          |
| Sample # 9  | 004400043452 | 28.8                                                       | 28.5                          | 29.2                          |
| Sample #10  | 004400043031 | 28.9                                                       | 28.7                          | 29.3                          |

### Annex 1 Calibration Certificate



**ROHDE & SCHWARZ**

Messgerätebau GmbH

#### Kalibrierschein

#### Calibration Certificate

Nummer 20-137411

Number

Gegenstand  
Item CMU200 UNIV.RADIOCOMM.

Hersteller  
Manufacturer ROHDE & SCHWARZ

Typ  
Type CMU200

Material Nr.  
Material No. 1100.0008K02

Serial Nr.  
Serial No. 105851

Auftraggeber  
Customer

Bestellung Nr.  
Order No.

Ort u. Datum d. Kalibrierung  
Place and date of calibration Memmingen, 2004-08-11

Umfang der Kalibrierung  
Scope of calibration Standard Calibration


Eingangsprüfung  
Performance on receipt

Kalibrierergebnis  
Result of calibration Measurement results within specifications

Umfang des Kalibrierscheins  
Extent of the certificate 3 pages  
60 pages test report

Dieser Kalibrierschein dokumentiert, daß der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Meßwerte lagen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95 % im zugeordneten Werteintervall (Erweiterte Meßunsicherheit mit  $k = 2$ ). Die Kalibrierung erfolgte mit Meßmitteln und Normen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriertechniken rückgeführt sind auf Normale der PTB/DKD oder anderer nationaler/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugsnormale der R&S-Laboratorien. Grundsätze und Verfahren der Kalibrierung entsprechen IEC/ISO 17025. Das Bestätigungssystem für die verwendeten Meßmittel entspricht DIN ISO 10012-1. Das angewandte Qualitätsmanagement-System ist zertifiziert nach DIN EN ISO 9001. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Signifizierungen sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95 % (coverage factor  $k = 2$ ). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national/international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no national standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with IEC/ISO 17025. The metrological confirmation system for the measuring equipment used is in compliance with DIN ISO 10012-1. The applied quality system is certified to DIN EN ISO 9001. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the item recalibrated at appropriate intervals.



Ausstellungsdatum  
Date of issue

2004-08-11

Laborleitung  
Head of laboratory

Steigmüller

Bearbeiter  
Person responsible

Wolfgang Schöning

Page 1/63