





Appendix D






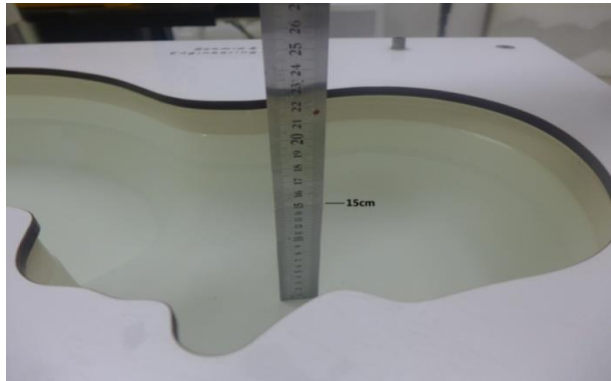
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details


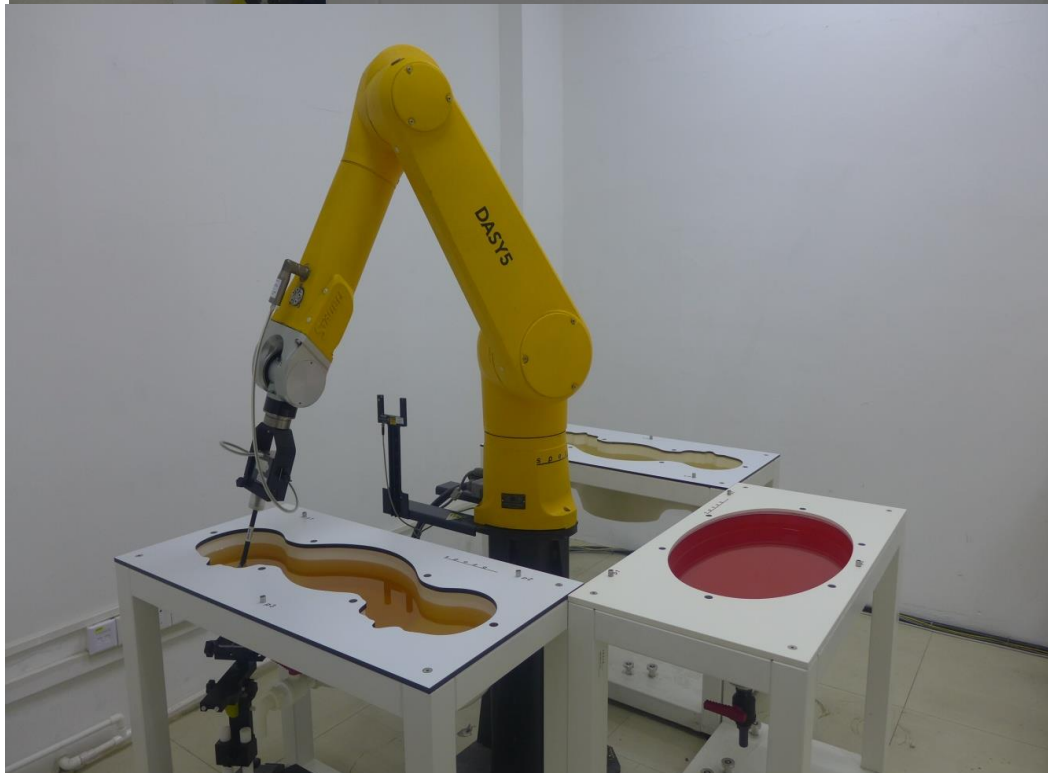
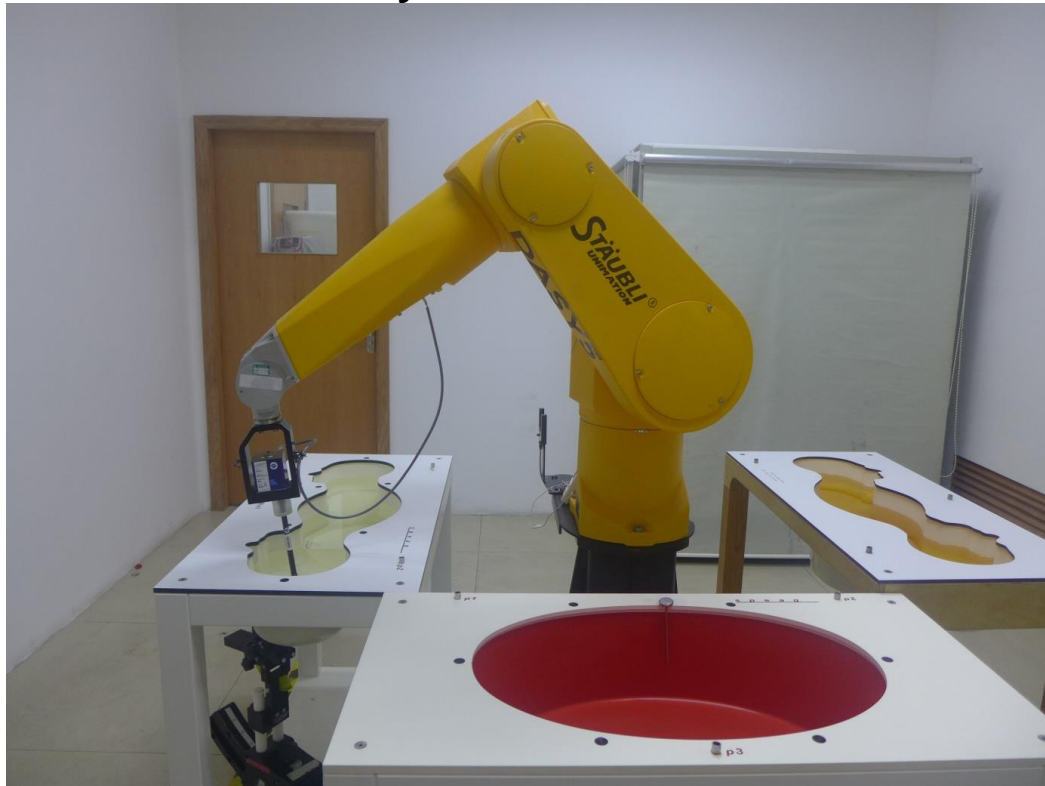



1. SAR measurement System



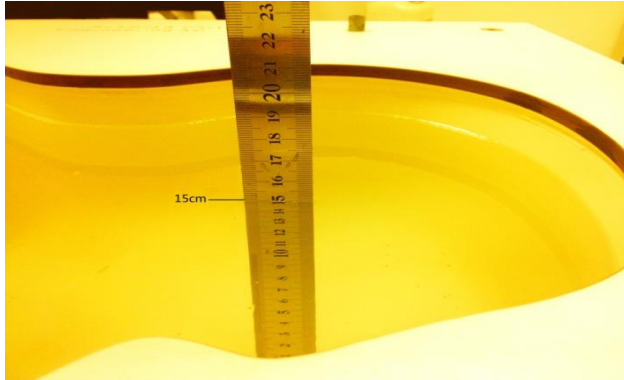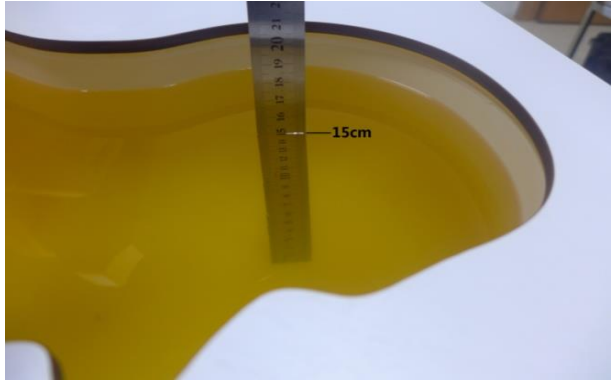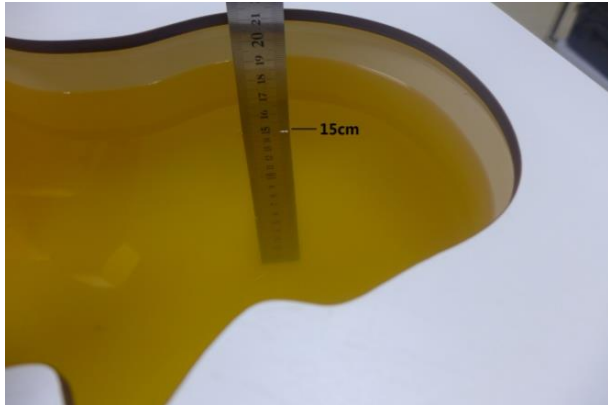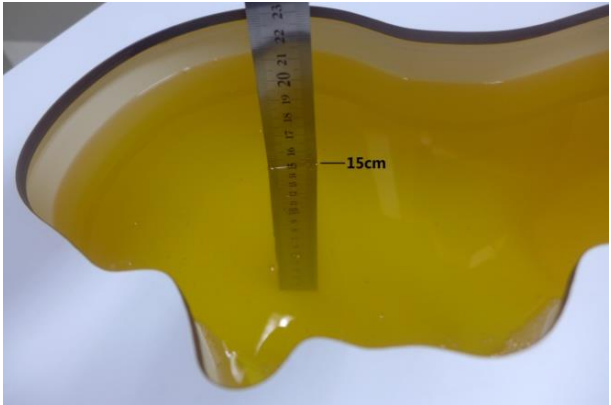



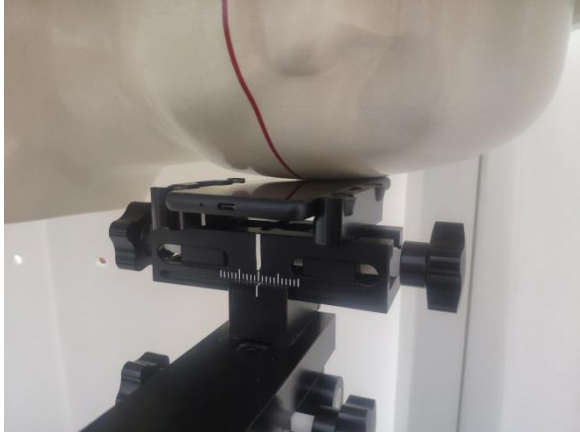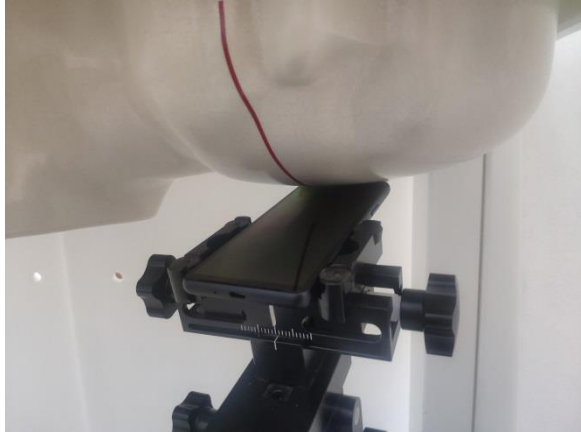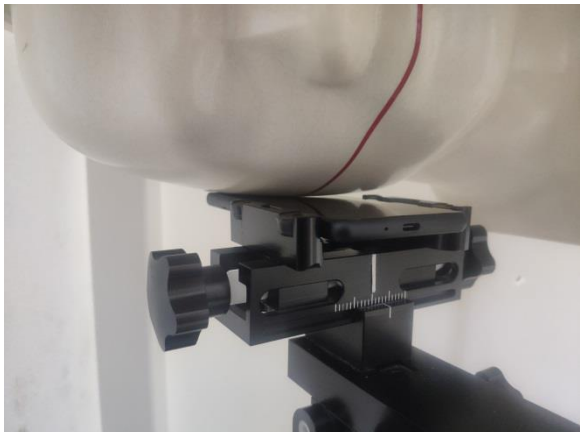


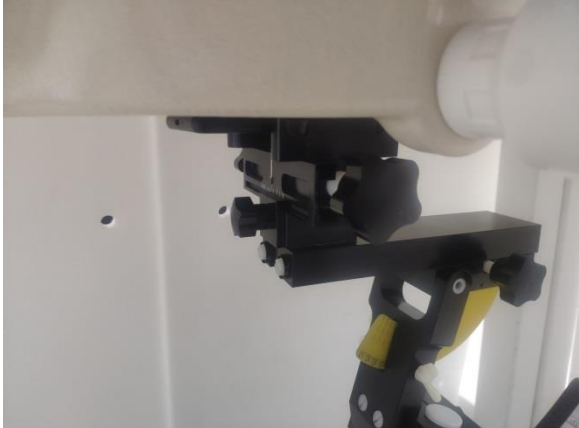




2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 835</p>	<p>Photo 2: Tissue Simulant Liquid for Head 1750</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1900</p>	<p>Photo 4: Tissue Simulant Liquid for Head 2450</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2600</p>	<p>Photo 6: Tissue Simulant Liquid for Head 5G</p>
	

3. Photographs of EUT test position

<p>Photo 7: Left cheek</p>	<p>Photo 8: Left tilted</p>
	
<p>Photo 9: Right cheek</p>	<p>Photo 10: Right tilted</p>
	
<p>Photo 11: Front side 15mm</p>	<p>Photo 12: Back side 15mm</p>
	

<p>Photo 13: Front side 10mm</p>	<p>Photo 14: Back side 10mm</p>
	
<p>Photo 15: Left side 10mm</p>	<p>Photo 16: Right side 10mm</p>
	
<p>Photo 17: Top side 10mm</p>	<p>Photo 18: Bottom side 10mm</p>
	

<p align="center">Photo 19: Front side 0mm</p>	<p align="center">Photo 20: Back side 0mm</p>
	
<p align="center">Photo 21: Left side 0mm</p>	<p align="center">Photo 22: Right side 0mm</p>
	
<p align="center">Photo 23: Top side 0mm</p>	<p align="center">Photo 24: Bottom side 0mm</p>
	

4. Constructional Details

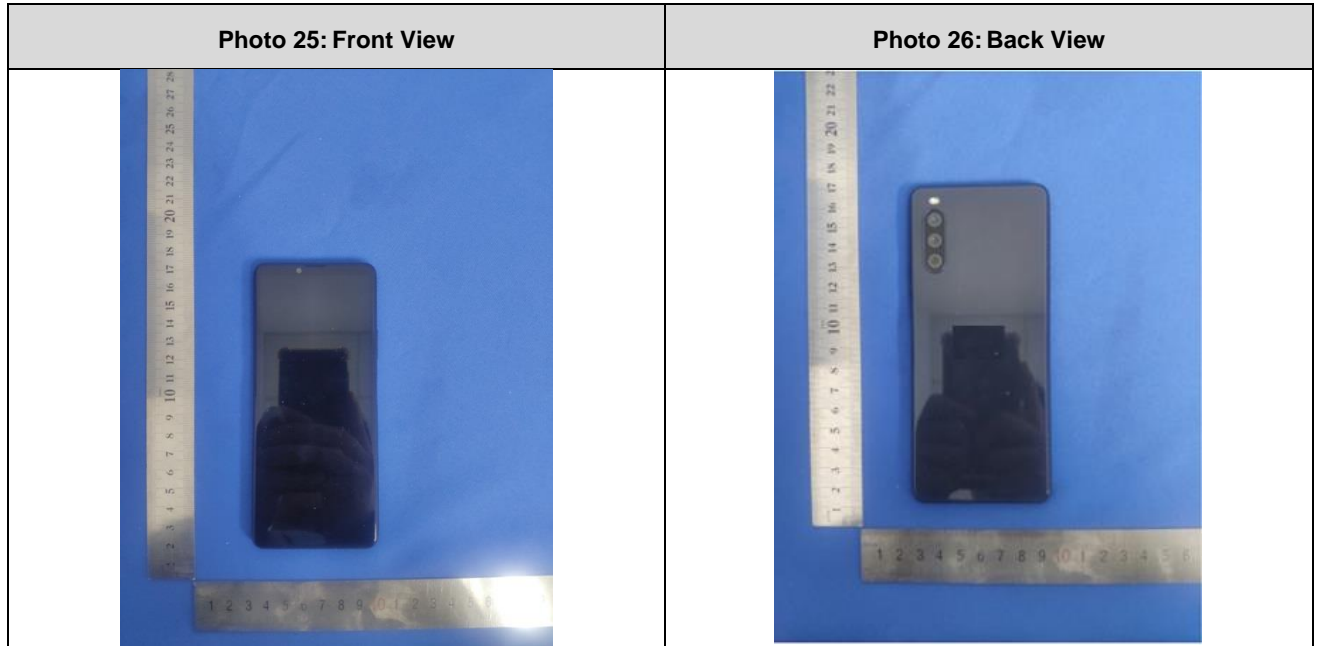


Photo 27: DUT Antenna Locations

