

APPENDIX B: SYSTEM VERIFICATION PLOTS

ELEMENT

DUT: Dipole 6500.0 MHz; Type: D6.5GHzV2 - SN1019

Communication System: UID: 0, CW; Frequency: 6500.0 MHz
Medium: 6000 Head; Medium parameters used:
f = 6500.0 MHz; cond = 6.23 S/m; perm = 33.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 5 mm

Test Date: 03/01/2023; Ambient Temp: 22.5°C; Tissue Temp: 20.8°C

Probe: EX3DV4 - SN7416; ConvF:(5.25,5.25,5.25); Calibrated: 2022-05-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn701; Calibrated: 2022-05-16
Phantom: Twin-SAM V8.0; Serial: 2071
Measurement SW: DASY Module SAR V16.2.0.1425

6500.0 MHz System Verification at 14.0 dBm (25 mW)

Area Scan (51.0 x 85.0): Measurement grid: dx=8.5 mm, dy=8.5 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=3.4 mm, dy=3.4 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 47.3 W/kg

SAR(1 g) = 7.55 W/kg; SAR(10 g) = 1.40 W/kg; APD(4 cm²) = 34.10 W/m²

Deviation (1 g) = 2.37%; Deviation (10 g) = 3.70%; Deviation (4 cm²) = 4.12%



ELEMENT

Date: 03/02/2023

10 GHz System Verification

Device Under Test Properties

DUT	Serial Number	DUT Type
10 GHz Verification Source	1004	10 GHz Verification Source

Exposure Conditions

Phantom Section	Position	Test Distance [mm]	Band	Frequency [MHz]
5G	FRONT	10.00	CW	10000.0

Hardware/Software Setup


Probe, Calibration Date	DAE, Calibration Date	Software	Software Version
EUmmWV3 - SN9407, 10/17/2022	DAE4ip - SN1638, 10/13/2022	cDASY6 Module mmWave	3.2.0.1840

Scans Setup


Scan Type	5G Scan
Grid Extents [mm]	120.0 x 120.0
Grid Steps [lambda]	0.25 x 0.25
Sensor Surface [mm]	10.0

Measurement Results

Scan Type	5G Scan
Avg. Area [cm ²]	4.00
pS _{tot} avg [W/m ²]	47.6
pS _n avg [W/m ²]	47.4
E _{peak} [V/m]	141
pS _{tot} Deviation [dB]	-0.16
pS _n Deviation [dB]	-0.18

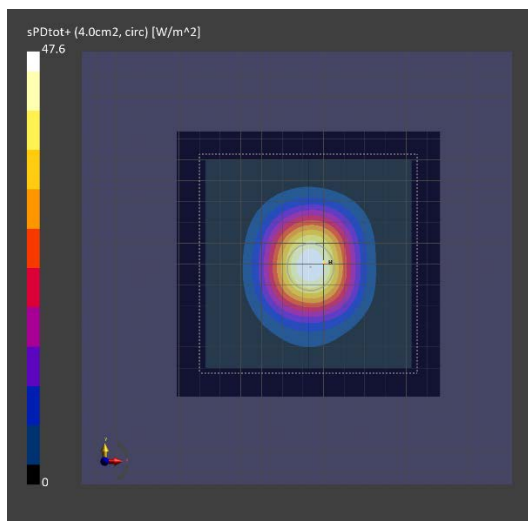

10 GHz System Verification

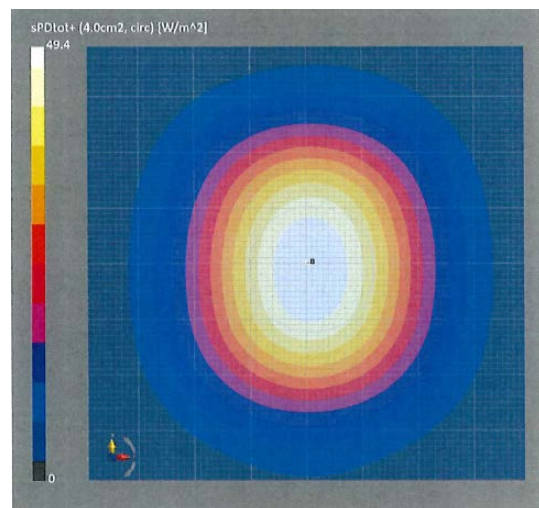

Calibration Certificate