

**APPENDIX B: SAR DIPOLE VERIFICATION PLOTS**

# ELEMENT

**DUT: Dipole 13.0 MHz; Type: CLA-13 - SN1002**

Communication System: UID: 0, CW; Frequency: 13.0 MHz  
Medium: 30 Head; Medium parameters used:  
f = 13.0 MHz; cond = 0.745 S/m; perm = 55.5; density = 1000 kg/m3  
Phantom Section: Flat; Space: 0 mm

Test Date: 02/28/2023; Ambient Temp: 23.2°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN7417; ConvF:(18.67,18.67,18.67); Calibrated: 2023-02-08  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn665; Calibrated: 2023-02-15  
Phantom: ELI V8.0 (20deg probe tilt); Serial: xxxx  
Measurement SW: DASY Module SAR V16.2.0.1425

## 13.0 MHz System Verification at 30.0 dBm (1 W)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 0.996 W/kg

**SAR(1 g) = 0.503 W/kg; SAR(10 g) = 0.313 W/kg**

Deviation (1 g) = -9.69%; Deviation (10 g) = -9.54%;

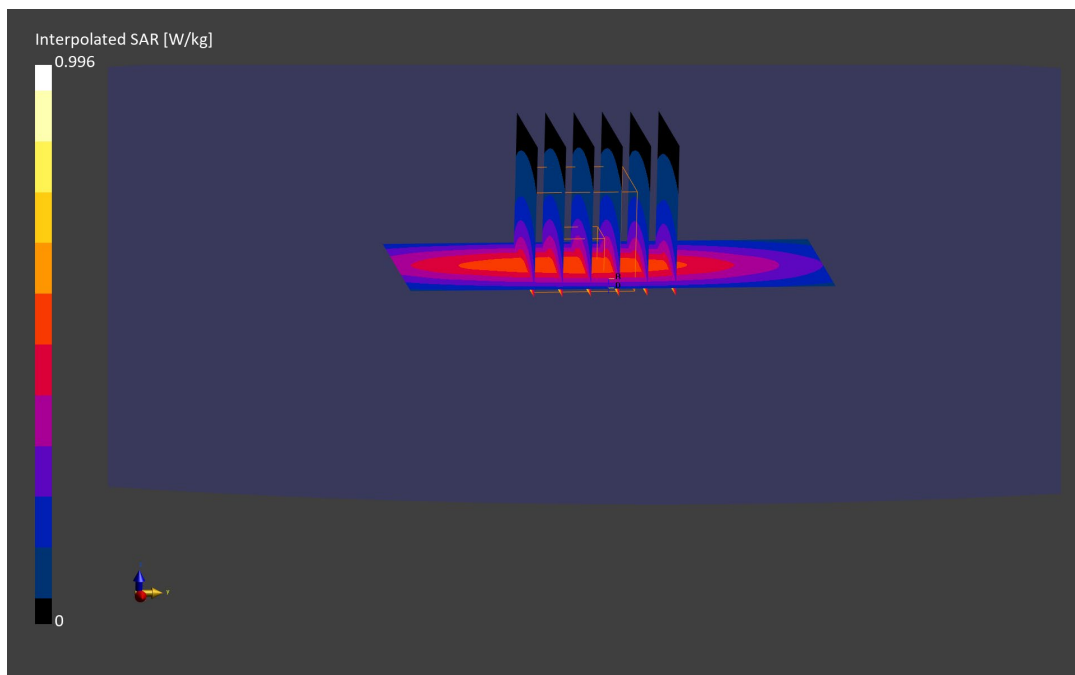

# ELEMENT

**DUT: Dipole 750.0 MHz; Type: D750V3 - SN1161**

Communication System: UID: 0, CW; Frequency: 750.0 MHz  
Medium: 750 Head; Medium parameters used:  
f = 750.0 MHz; cond = 0.860 S/m; perm = 41.0; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 03/09/2023; Ambient Temp: 22.3°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN7406; ConvF:(10.13,10.13,10.13); Calibrated: 2022-07-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1677; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 2064  
Measurement SW: DASY Module SAR V16.2.0.1425

## 750 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.68 W/kg

**SAR(1 g) = 1.69 W/kg; SAR(10 g) = 1.11 W/kg**

Deviation (1 g) = 0.12%; Deviation (10 g) = 0.73%;

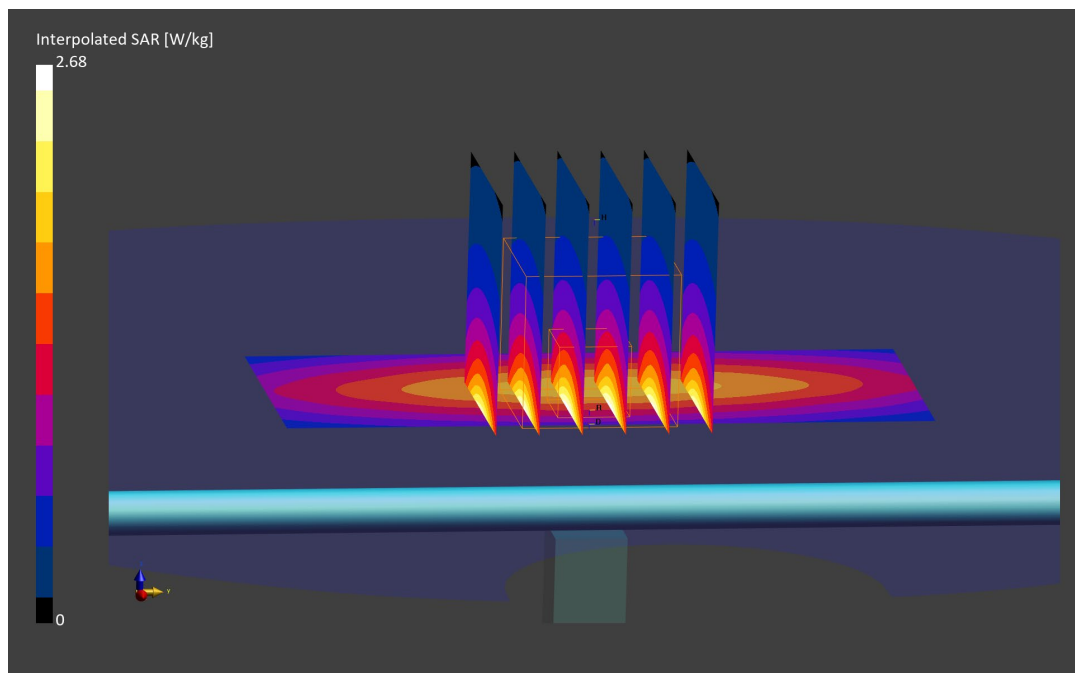

# ELEMENT

**DUT: Dipole 750.0 MHz; Type: D750V3 - SN1161**

Communication System: UID: 0, CW; Frequency: 750.0 MHz  
Medium: 750 Head; Medium parameters used:  
f = 750.0 MHz; cond = 0.920 S/m; perm = 41.9; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 03/20/2023; Ambient Temp: 22.3°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7659; ConvF:(10.93,10.93,10.93); Calibrated: 2022-04-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1407; Calibrated: 2022-04-13  
Phantom: Twin-SAM V5.0; Serial: 1873  
Measurement SW: DASYS Module SAR V16.2.0.1425

## 750 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.69 W/kg

**SAR(1 g) = 1.77 W/kg; SAR(10 g) = 1.16 W/kg**

Deviation (1 g) = 4.86%; Deviation (10 g) = 5.26%;

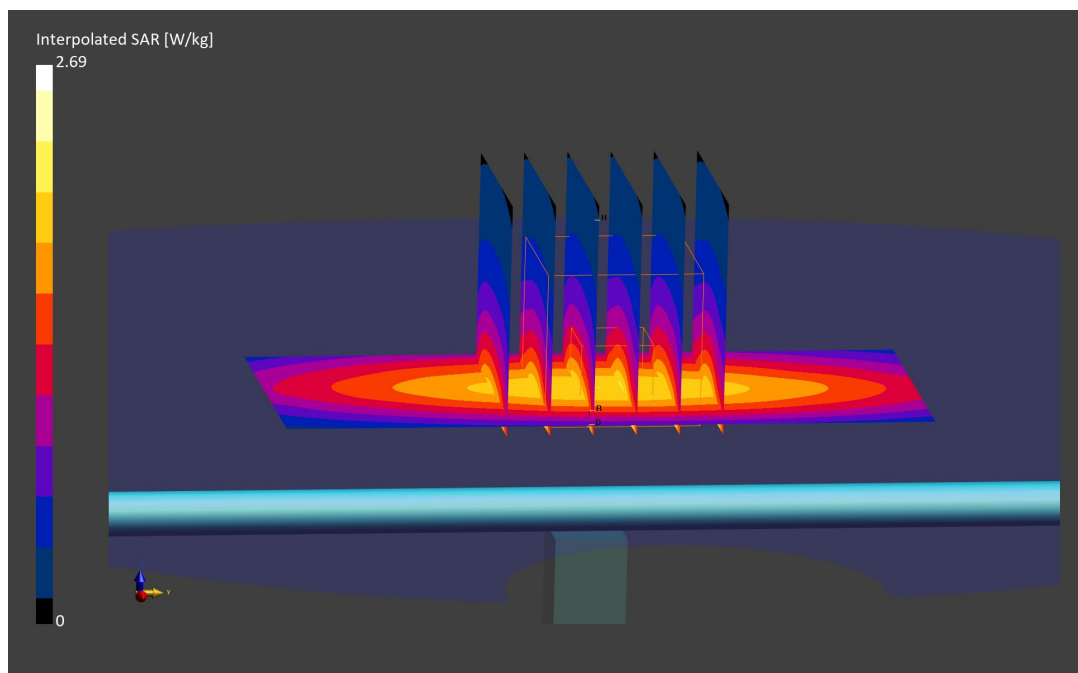

# ELEMENT

**DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d132**

Communication System: UID: 0, CW; Frequency: 835.0 MHz  
Medium: 835 Head; Medium parameters used:  
f = 835.0 MHz; cond = 0.891 S/m; perm = 40.8; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 03/07/2023; Ambient Temp: 22°C; Tissue Temp: 20.1°C

Probe: EX3DV4 - SN7406; ConvF:(9.86,9.86,9.86); Calibrated: 2022-07-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1677; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 2064  
Measurement SW: DASY Module SAR V16.2.0.1425

## 835 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.27 W/kg

**SAR(1 g) = 2.02 W/kg; SAR(10 g) = 1.31 W/kg**

Deviation (1 g) = 4.55%; Deviation (10 g) = 4.47%

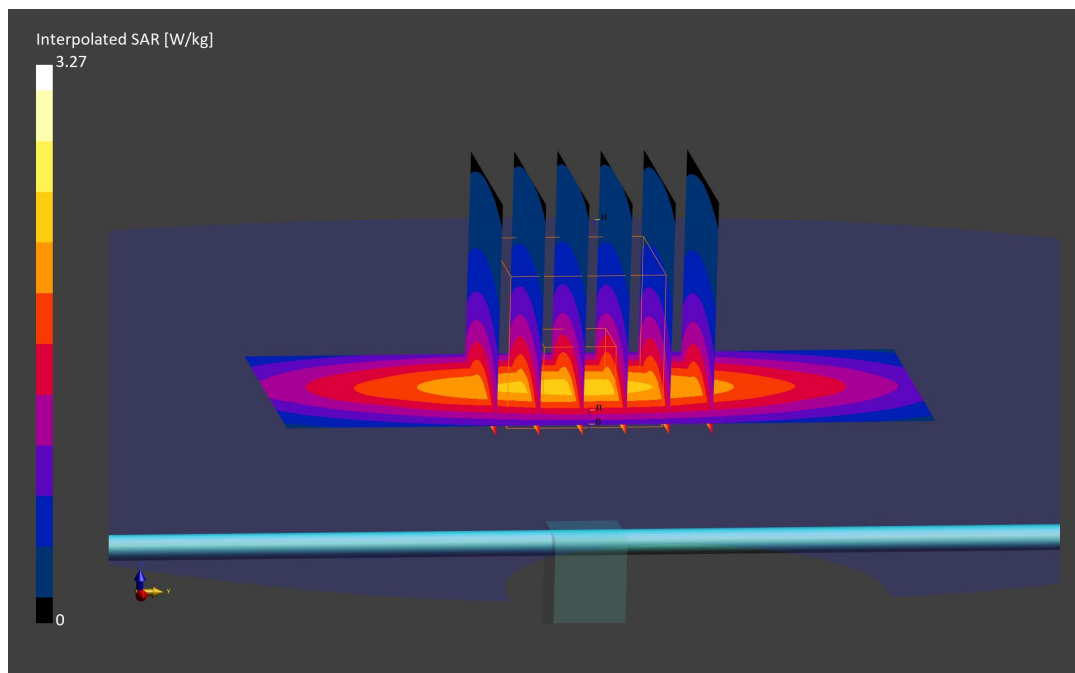

# ELEMENT

**DUT: Dipole 835.0 MHz; Type: D835V2 - SN460**

Communication System: UID: 0, CW; Frequency: 835.0 MHz  
Medium: 835 Head; Medium parameters used:  
f = 835.0 MHz; cond = 0.933 S/m; perm = 40.0; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 03/10/2023; Ambient Temp: 22.2°C; Tissue Temp: 21.8°C

Probe: EX3DV4 - SN7639; ConvF:(10.75,10.75,10.75); Calibrated: 2022-11-14  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1646; Calibrated: 2022-11-10  
Phantom: Twin-SAM V8.0; Serial: 1936  
Measurement SW: DASY Module SAR V16.2.0.1425

## 835 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.26 W/kg

**SAR(1 g) = 2.03 W/kg; SAR(10 g) = 1.31 W/kg**

Deviation (1 g) = 4.42%; Deviation (10 g) = 3.31%

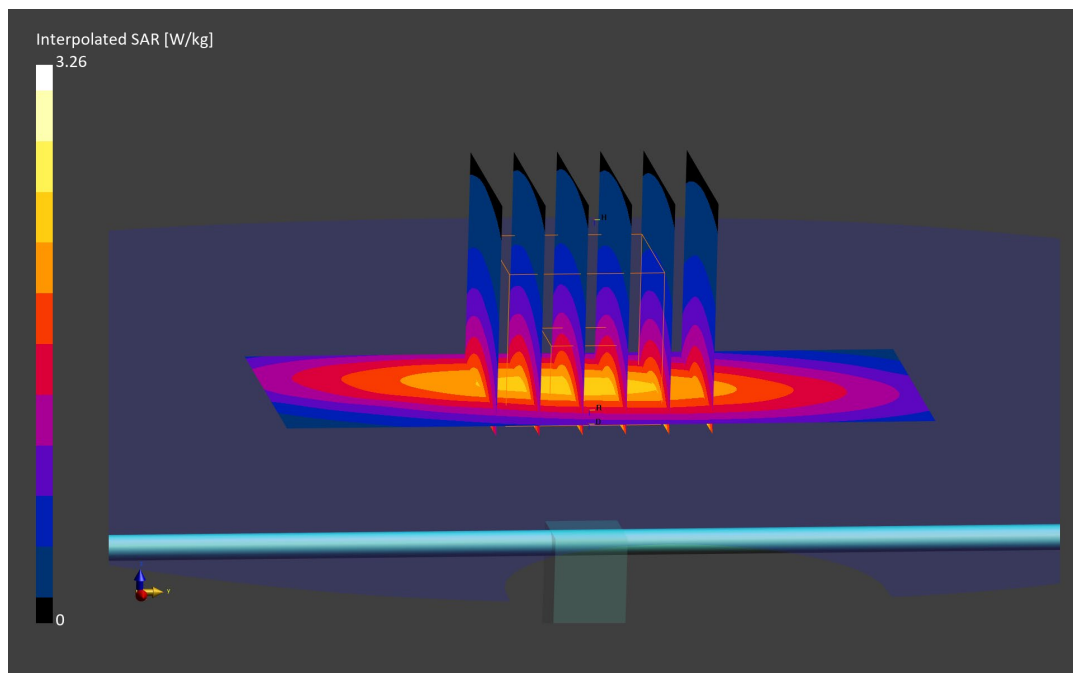

# ELEMENT

**DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d132**

Communication System: UID: 0, CW; Frequency: 835.0 MHz  
Medium: 835 Head; Medium parameters used:  
f = 835.0 MHz; cond = 0.869 S/m; perm = 42.6; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 03/14/2023; Ambient Temp: 19.6°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN7410; ConvF:(9.6,9.6,9.6); Calibrated: 2022-07-19  
Sensor-Surface: 1.4mm (All points)  
Electronics: DAE4 Sn1583; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 1630  
Measurement SW: DASY Module SAR V16.2.0.1425

## 835 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.15 W/kg

**SAR(1 g) = 2.04 W/kg; SAR(10 g) = 1.34 W/kg**

Deviation (1 g) = 5.59%; Deviation (10 g) = 6.86%

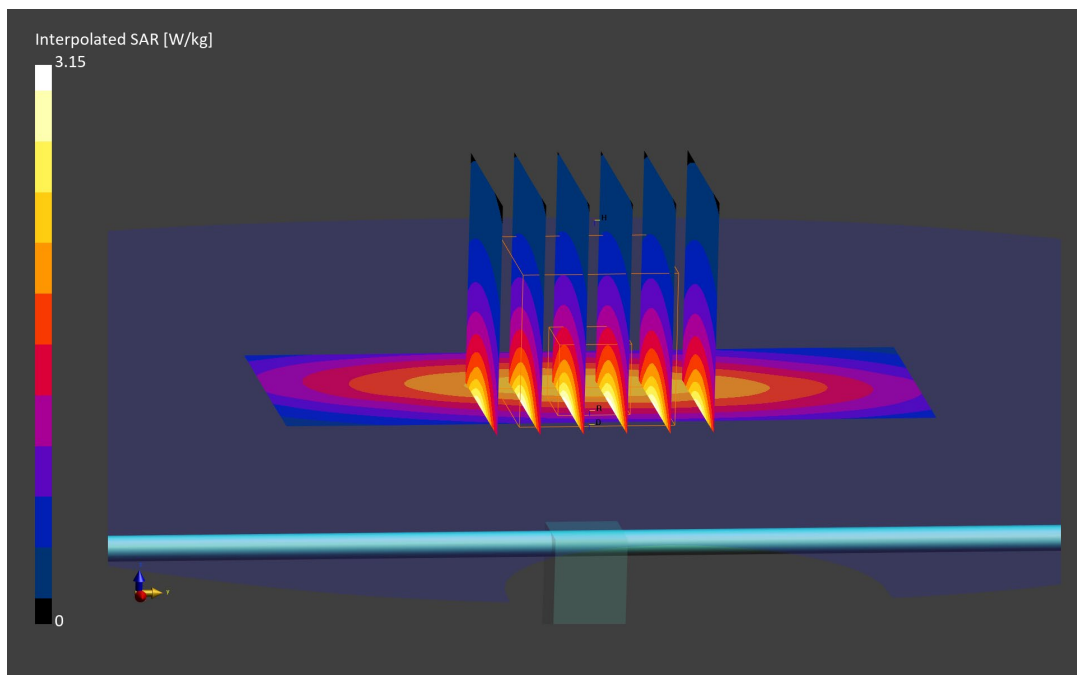

# ELEMENT

**DUT: Dipole 1750.0 MHz; Type: D1765V2 - SN1008**

Communication System: UID: 0, CW; Frequency: 1750.0 MHz  
Medium: 1750 Head; Medium parameters used:  
f = 1750.0 MHz; cond = 1.31 S/m; perm = 41.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/13/2023; Ambient Temp: 19.1°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7409; ConvF:(8.33,8.33,8.33); Calibrated: 2022-06-16  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1334; Calibrated: 2022-06-14  
Phantom: Twin-SAM V5.0; Serial: 1792  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1750 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.30 W/kg

**SAR(1 g) = 3.48 W/kg; SAR(10 g) = 1.87 W/kg**

Deviation (1 g) = -6.95%; Deviation (10 g) = -4.59%;

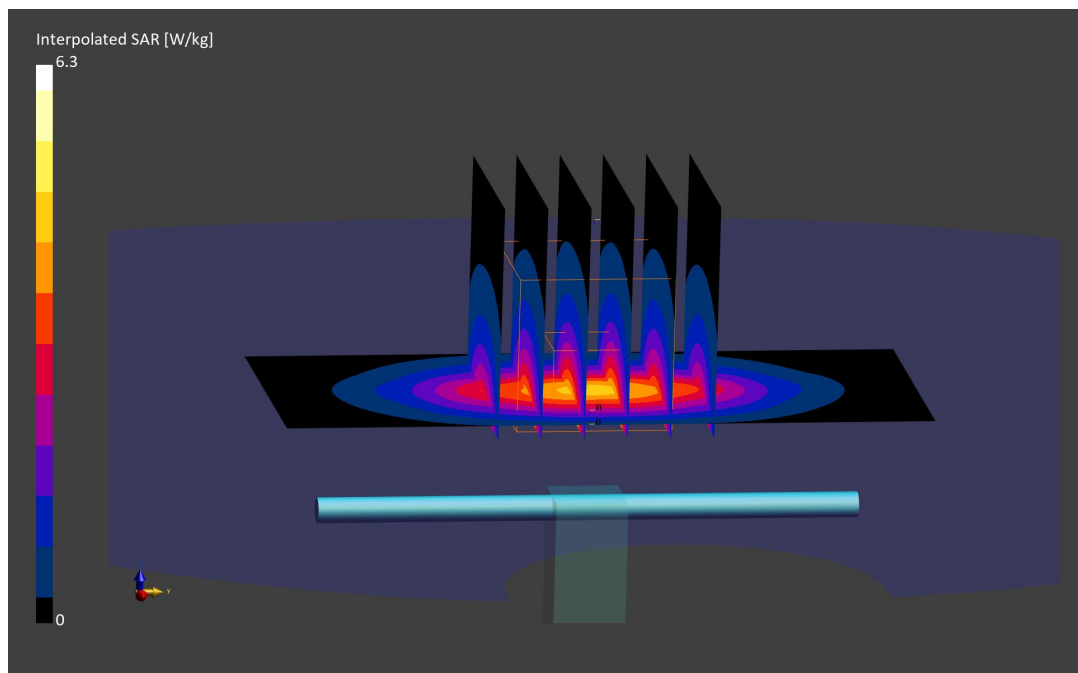



# ELEMENT

**DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1148**

Communication System: UID: 0, CW; Frequency: 1750.0 MHz  
Medium: 1750 Head; Medium parameters used:  
f = 1750.0 MHz; cond = 1.40 S/m; perm = 40.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/16/2023; Ambient Temp: 22.3°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7659; ConvF:(9.43,9.43,9.43); Calibrated: 2022-04-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1407; Calibrated: 2022-04-13  
Phantom: Twin-SAM V5.0; Serial: 1873  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1750 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.01 W/kg

**SAR(1 g) = 3.69 W/kg; SAR(10 g) = 1.96 W/kg**

Deviation (1 g) = -0.81%; Deviation (10 g) = 1.03%;

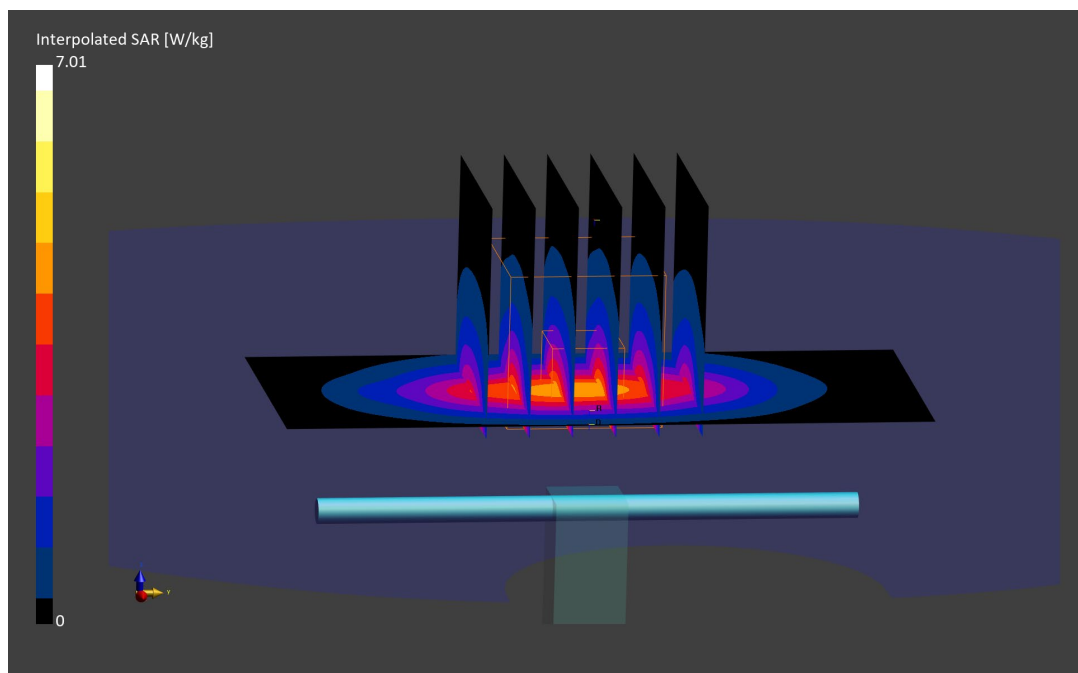

# ELEMENT

**DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d149**

Communication System: UID: 0, CW; Frequency: 1900.0 MHz  
Medium: 1900 Head; Medium parameters used:  
f = 1900.0 MHz; cond = 1.41 S/m; perm = 40.2; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/10/2023; Ambient Temp: 21.4°C; Tissue Temp: 19.3°C

Probe: EX3DV4 - SN7409; ConvF:(8.13,8.13,8.13); Calibrated: 2022-06-16  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1334; Calibrated: 2022-06-14  
Phantom: Twin-SAM V5.0; Serial: 1792  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1900 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.55 W/kg

**SAR(1 g) = 3.98 W/kg; SAR(10 g) = 2.08 W/kg**

Deviation (1 g) = -1.73%; Deviation (10 g) = -1.89%;

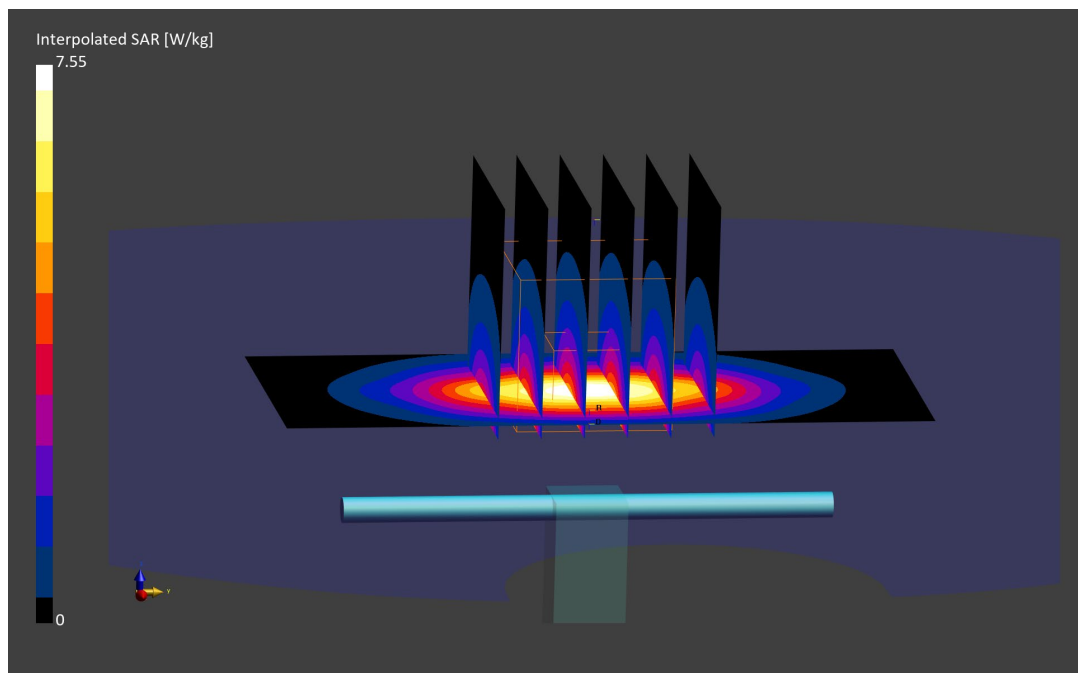

# ELEMENT

**DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d149**

Communication System: UID: 0, CW; Frequency: 1900.0 MHz  
Medium: 1900 Head; Medium parameters used:  
f = 1900.0 MHz; cond = 1.41 S/m; perm = 41.2; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/13/2023; Ambient Temp: 19.1°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7409; ConvF:(8.13,8.13,8.13); Calibrated: 2022-06-16  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1334; Calibrated: 2022-06-14  
Phantom: Twin-SAM V5.0; Serial: 1792  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1900 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.38 W/kg

**SAR(1 g) = 3.94 W/kg; SAR(10 g) = 2.05 W/kg**

Deviation (1 g) = -2.72%; Deviation (10 g) = -3.30%;

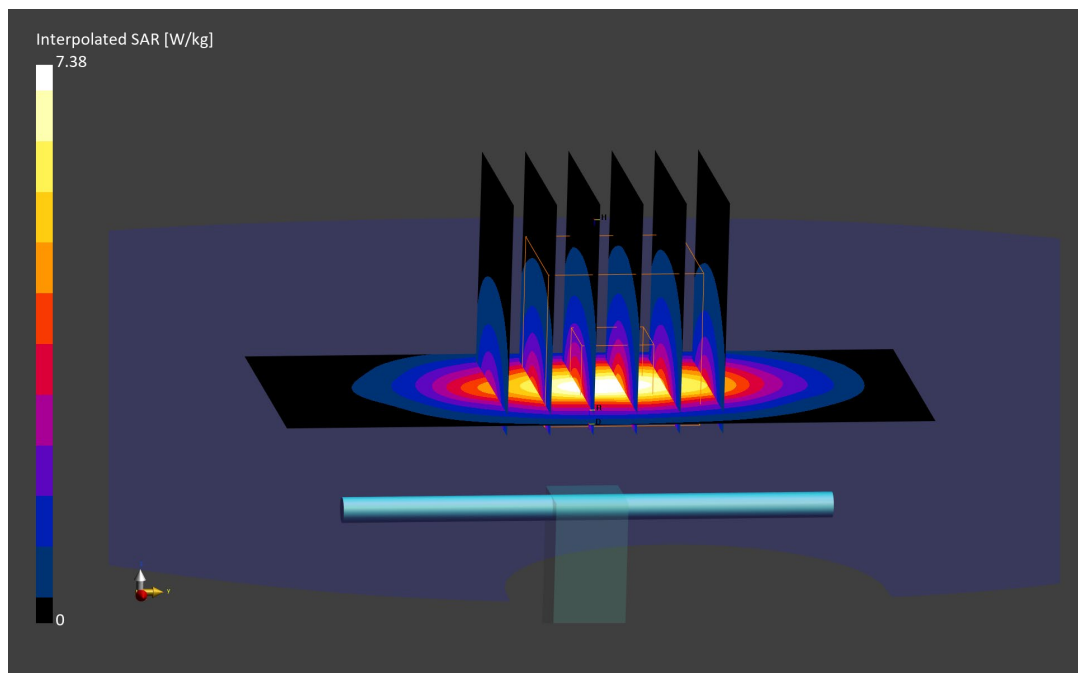

# ELEMENT

**DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d148**

Communication System: UID: 0, CW; Frequency: 1900.0 MHz  
Medium: 1900 Head; Medium parameters used:  
f = 1900.0 MHz; cond = 1.40 S/m; perm = 40.8; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/15/2023; Ambient Temp: 19.1°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7713; ConvF:(8.68,8.68,8.68); Calibrated: 2023-01-11  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1530; Calibrated: 2023-01-18  
Phantom: Twin-SAM V8.0; Serial: 2065  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1900 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 8.04 W/kg

**SAR(1 g) = 4.26 W/kg; SAR(10 g) = 2.23 W/kg**

Deviation (1 g) = 6.23%; Deviation (10 g) = 6.19%;

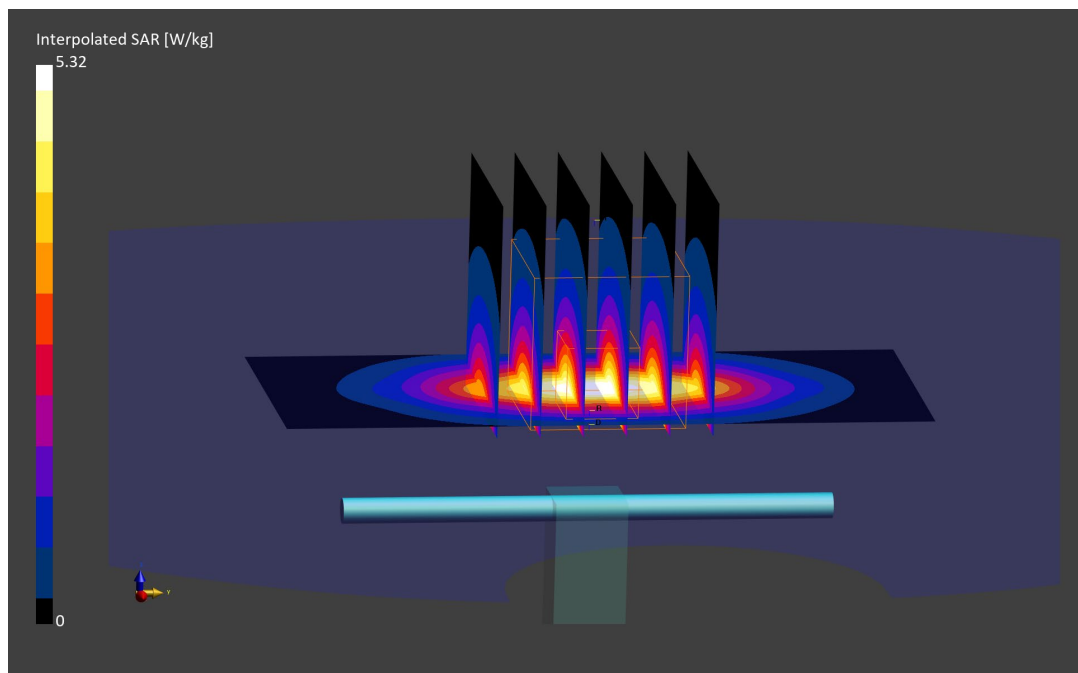

# ELEMENT

**DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1064**

Communication System: UID: 0, CW; Frequency: 2300.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2300.0 MHz; cond = 1.75 S/m; perm = 40.9; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/10/2023; Ambient Temp: 21.0°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN3837; ConvF:(7.47,7.47,7.47); Calibrated: 2023-01-17  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn793; Calibrated: 2023-01-17  
Phantom: Twin-SAM V8.0; Serial: 1944  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2300 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.5 W/kg

**SAR(1 g) = 4.82 W/kg; SAR(10 g) = 2.28 W/kg**

Deviation (1 g) = -1.43%; Deviation (10 g) = -2.56%;

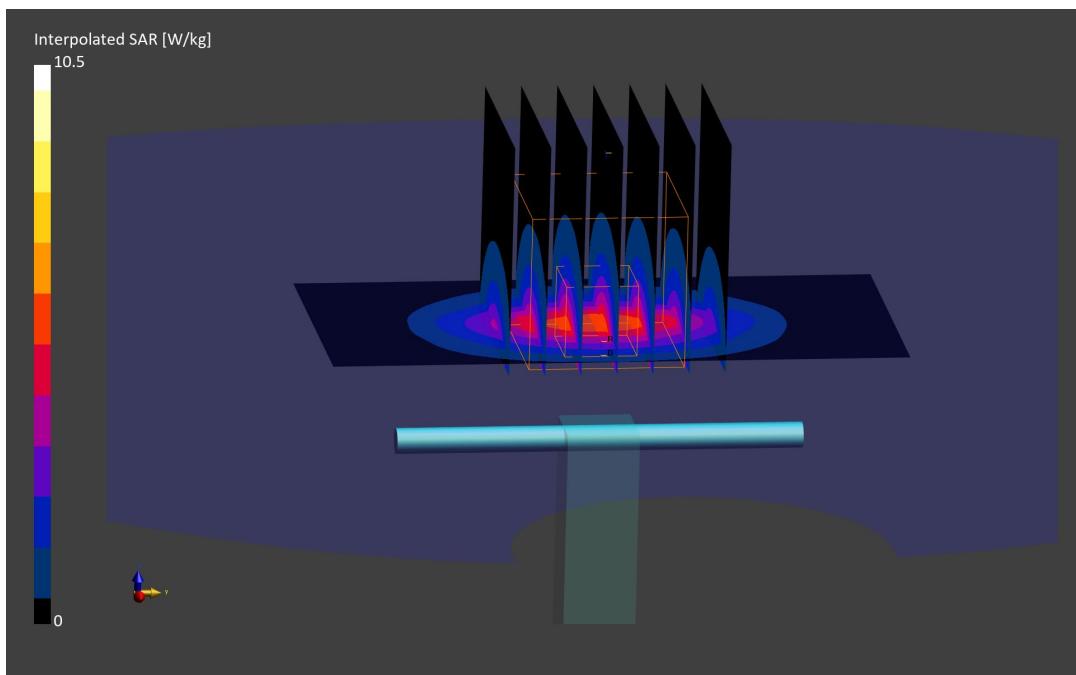

# ELEMENT

**DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1073**

Communication System: UID: 0, CW; Frequency: 2300.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2300.0 MHz; cond = 1.68 S/m; perm = 40.6; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/13/2023; Ambient Temp: 19.1°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7409; ConvF:(7.52,7.52,7.52); Calibrated: 2022-06-16  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1334; Calibrated: 2022-06-14  
Phantom: Twin-SAM V5.0; Serial: 1792  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2300 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.1 W/kg

**SAR(1 g) = 5.10 W/kg; SAR(10 g) = 2.45 W/kg**

Deviation (1 g) = 4.94%; Deviation (10 g) = 3.38%;

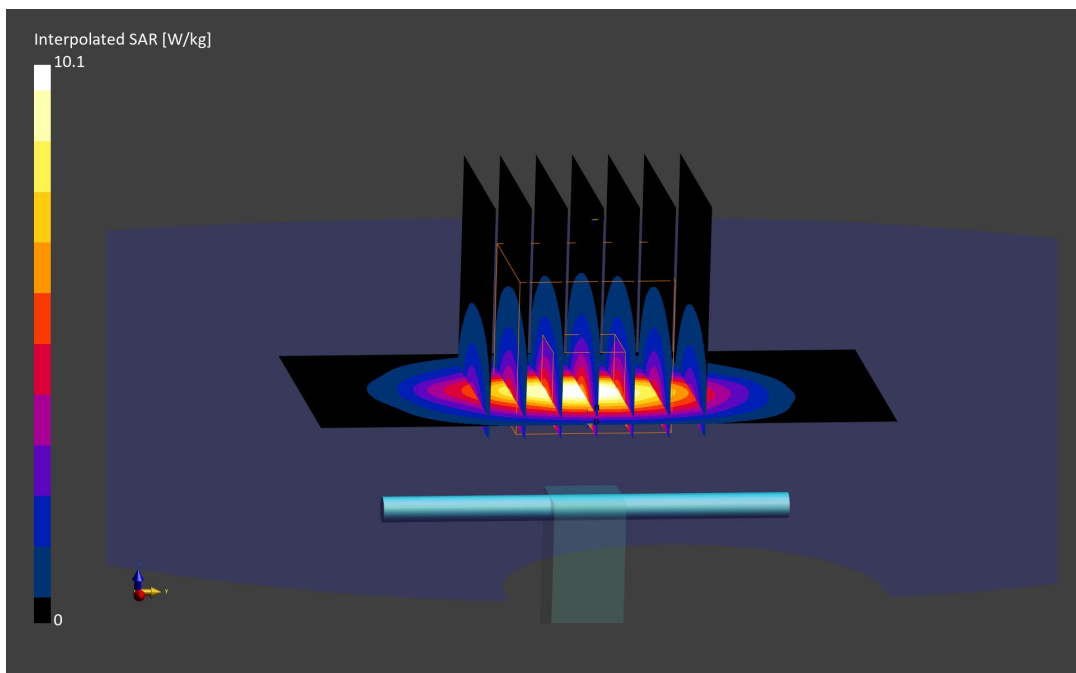

# ELEMENT

**DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN981**

Communication System: UID: 0, CW; Frequency: 2450.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2450.0 MHz; cond = 1.80 S/m; perm = 38.5; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/02/2023; Ambient Temp: 21.5°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7406; ConvF:(7.72,7.72,7.72); Calibrated: 2022-07-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1677; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 2064  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2450 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.8 W/kg

**SAR(1 g) = 5.09 W/kg; SAR(10 g) = 2.39 W/kg**

Deviation (1 g) = -5.57%; Deviation (10 g) = -5.91%

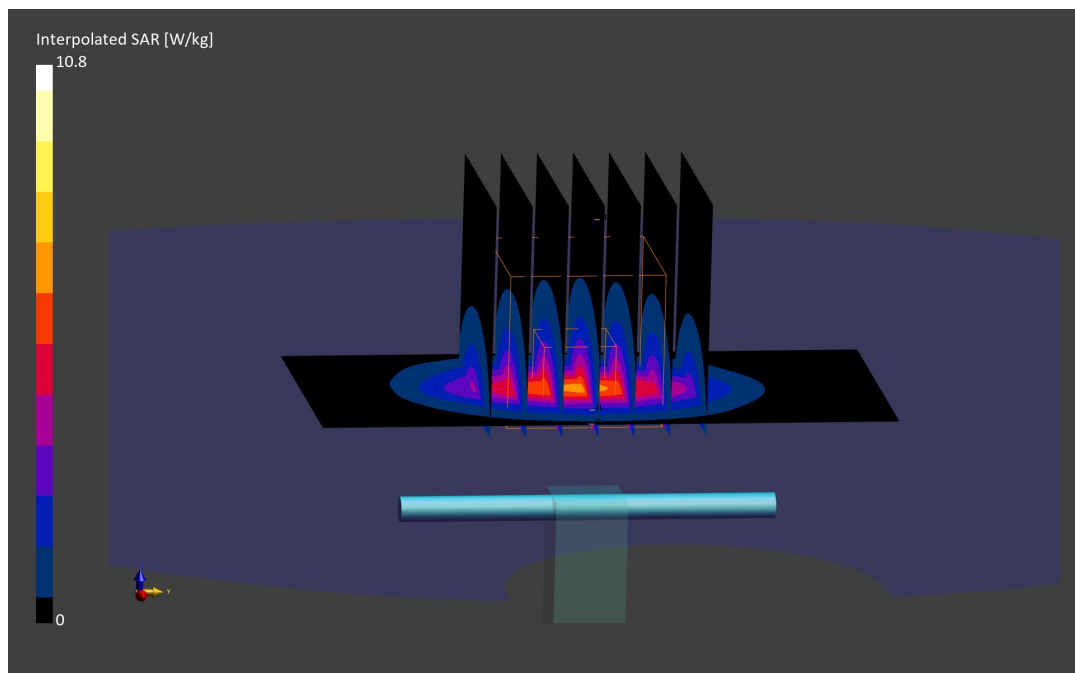

# ELEMENT

**DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1069**

Communication System: UID: 0, CW; Frequency: 2600.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2600.0 MHz; cond = 1.93 S/m; perm = 38.6; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/20/2023; Ambient Temp: 22.1°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7420; ConvF:(7.2,7.2,7.2); Calibrated: 2022-10-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1333; Calibrated: 2022-10-13  
Phantom: Twin-SAM V8.0; Serial: 1736  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2600 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.7 W/kg

**SAR(1 g) = 5.46 W/kg; SAR(10 g) = 2.45 W/kg**

Deviation (1 g) = -1.8%; Deviation (10 g) = -1.61%;

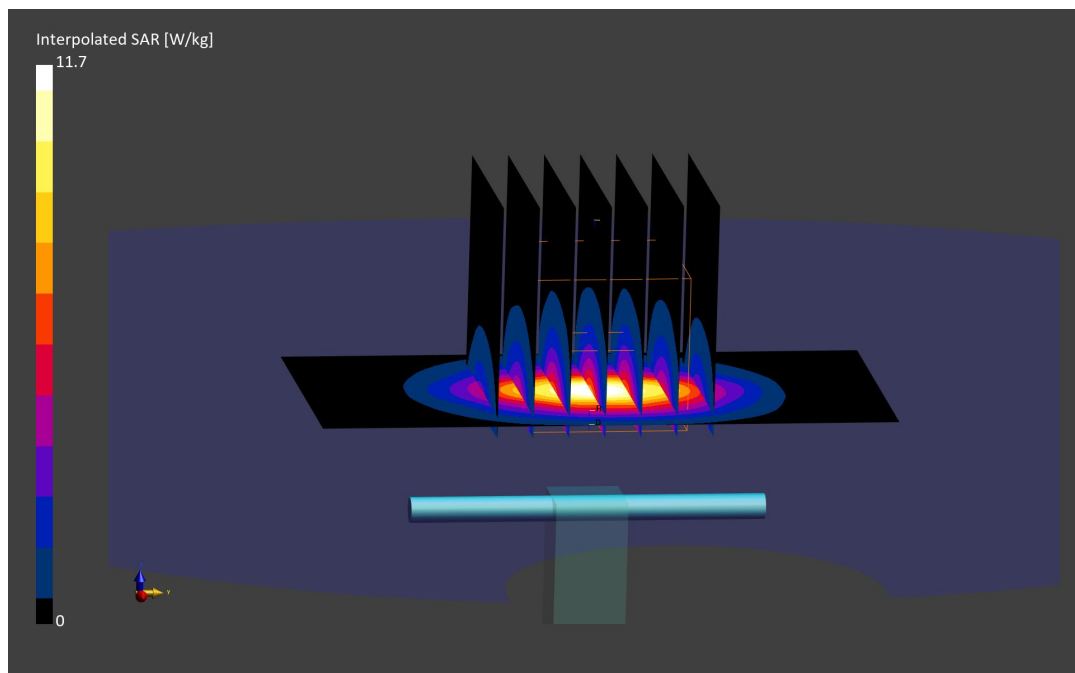



# ELEMENT

**DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN797**

Communication System: UID: 0, CW; Frequency: 2450.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2450.0 MHz; cond = 1.79 S/m; perm = 39.1; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/06/2023; Ambient Temp: 21.7°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7410; ConvF:(7.46,7.46,7.46); Calibrated: 2022-07-19  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1583; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 1630  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2450 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.0 W/kg

**SAR(1 g) = 5.29 W/kg; SAR(10 g) = 2.47 W/kg**

Deviation (1 g) = 1.73%; Deviation (10 g) = 1.23%;

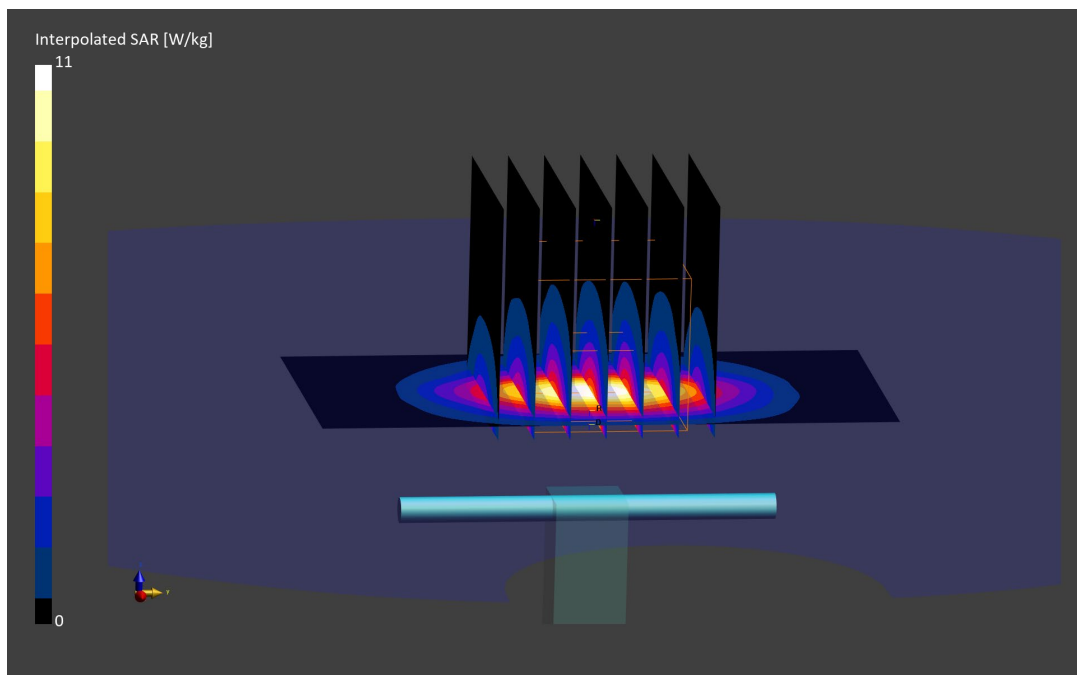

# ELEMENT

**DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1064**

Communication System: UID: 0, CW; Frequency: 2600.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2600.0 MHz; cond = 1.91 S/m; perm = 38.8; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/06/2023; Ambient Temp: 21.7°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7410; ConvF:(7.33,7.33,7.33); Calibrated: 2022-07-19  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1583; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 1630  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2600 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.9 W/kg

**SAR(1 g) = 5.56 W/kg; SAR(10 g) = 2.49 W/kg**

Deviation (1 g) = -1.42%; Deviation (10 g) = -1.19%;

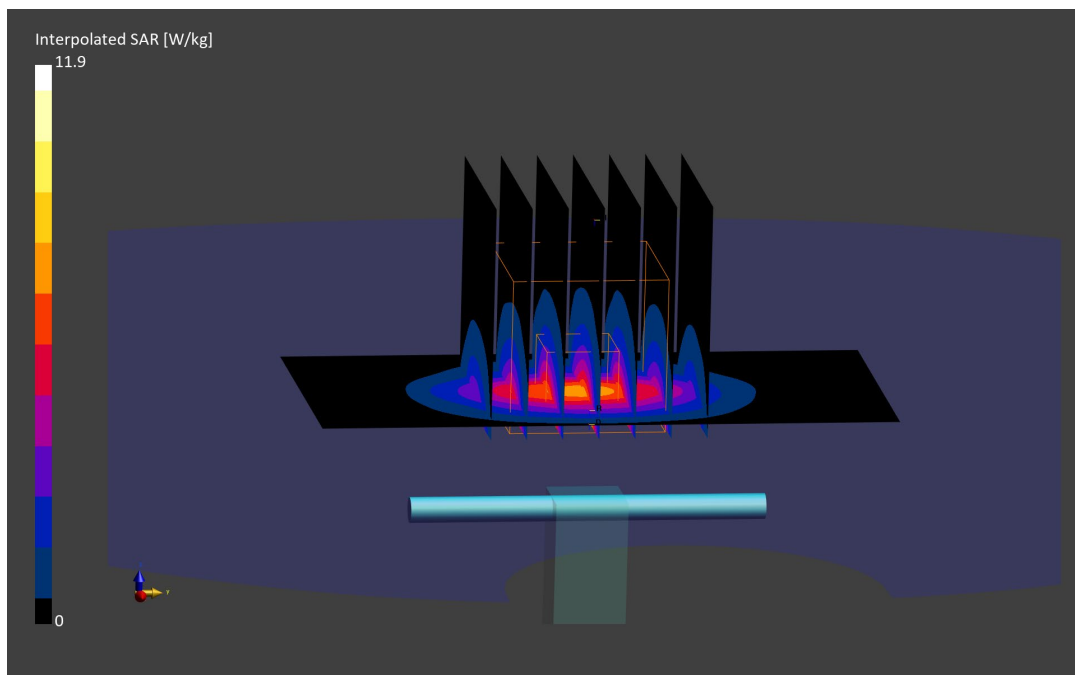

# ELEMENT

**DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1055**

Communication System: UID: 0, CW; Frequency: 3500.0 MHz  
Medium: 3600 Head; Medium parameters used:  
f = 3500.0 MHz; cond = 2.79 S/m; perm = 39.1; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/15/2023; Ambient Temp: 21.6°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7416; ConvF:(6.67,6.67,6.67); Calibrated: 2022-05-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn701; Calibrated: 2022-05-16  
Phantom: Twin-SAM V8.0; Serial: 2067  
Measurement SW: DASY Module SAR V16.2.0.1425

## 3500 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (28.0 x 28.0 x 28.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 17.4 W/kg

**SAR(1 g) = 6.86 W/kg; SAR(10 g) = 2.64 W/kg**

Deviation (1 g) = 3.94%; Deviation (10 g) = 6.02%;

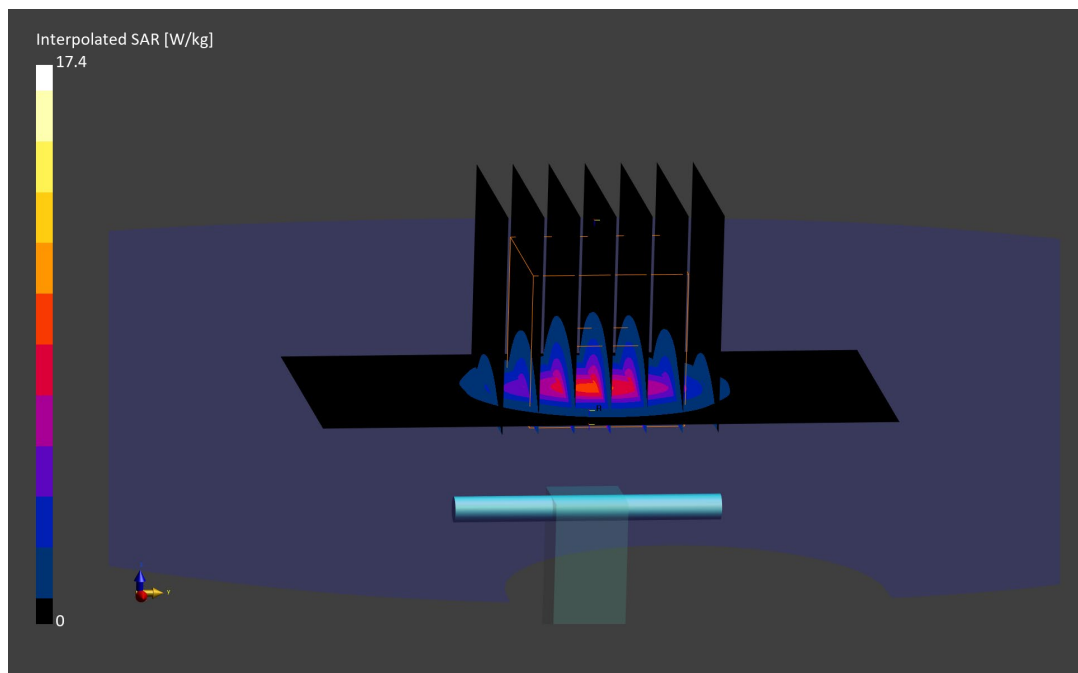

# ELEMENT

**DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1097**

Communication System: UID: 0, CW; Frequency: 3500.0 MHz  
Medium: 3600 Head; Medium parameters used:  
f = 3500.0 MHz; cond = 2.87 S/m; perm = 38.2; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/20/2023; Ambient Temp: 21.7°C; Tissue Temp: 19°C

Probe: EX3DV4 - SN7406; ConvF:(7.06,7.06,7.06); Calibrated: 2022-07-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1677; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 2064  
Measurement SW: DASY Module SAR V16.2.0.1425

## 3500 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (28.0 x 28.0 x 28.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 16.1 W/kg

**SAR(1 g) = 6.20 W/kg; SAR(10 g) = 2.36 W/kg**

Deviation (1 g) = -5.20%; Deviation (10 g) = -4.45%;

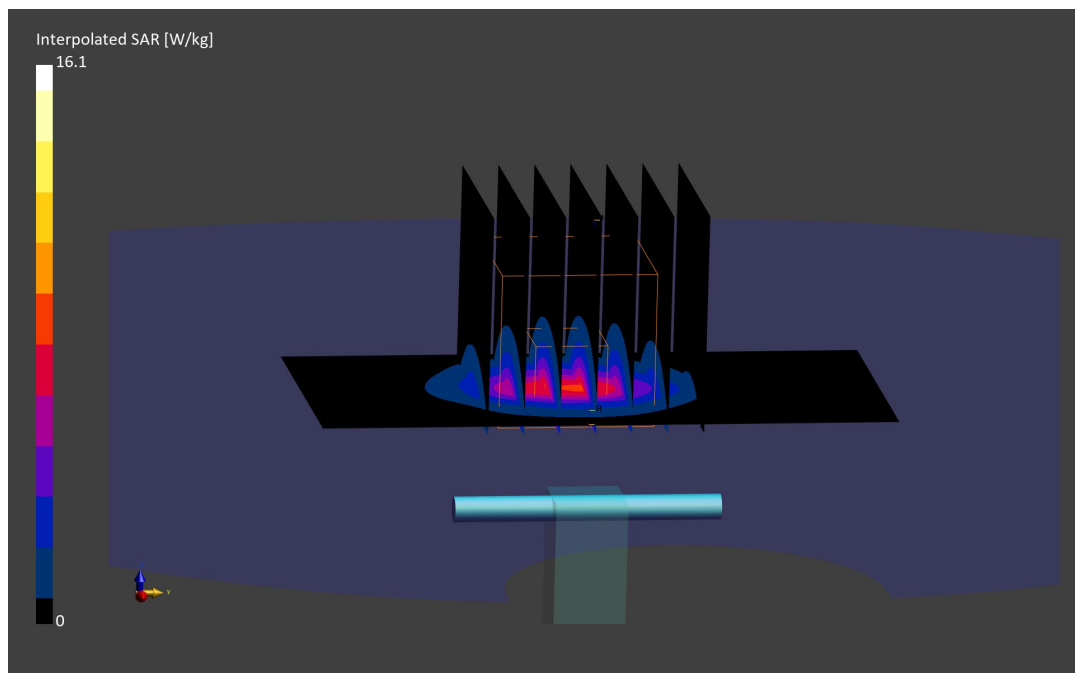

# ELEMENT

**DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1097**

Communication System: UID: 0, CW; Frequency: 3700.0 MHz  
Medium: 3600 Head; Medium parameters used:  
f = 3700.0 MHz; cond = 2.98 S/m; perm = 38.8; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/15/2023; Ambient Temp: 21.6°C; Tissue Temp: 20.1°C

Probe: EX3DV4 - SN7416; ConvF:(6.43,6.43,6.43); Calibrated: 2022-05-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn701; Calibrated: 2022-05-16  
Phantom: Twin-SAM V8.0; Serial: 2067  
Measurement SW: DASY Module SAR V16.2.0.1425

## 3700 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (28.0 x 28.0 x 28.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 17.2 W/kg

**SAR(1 g) = 6.40 W/kg; SAR(10 g) = 2.37 W/kg**

Deviation (1 g) = -6.02%; Deviation (10 g) = -3.27%;

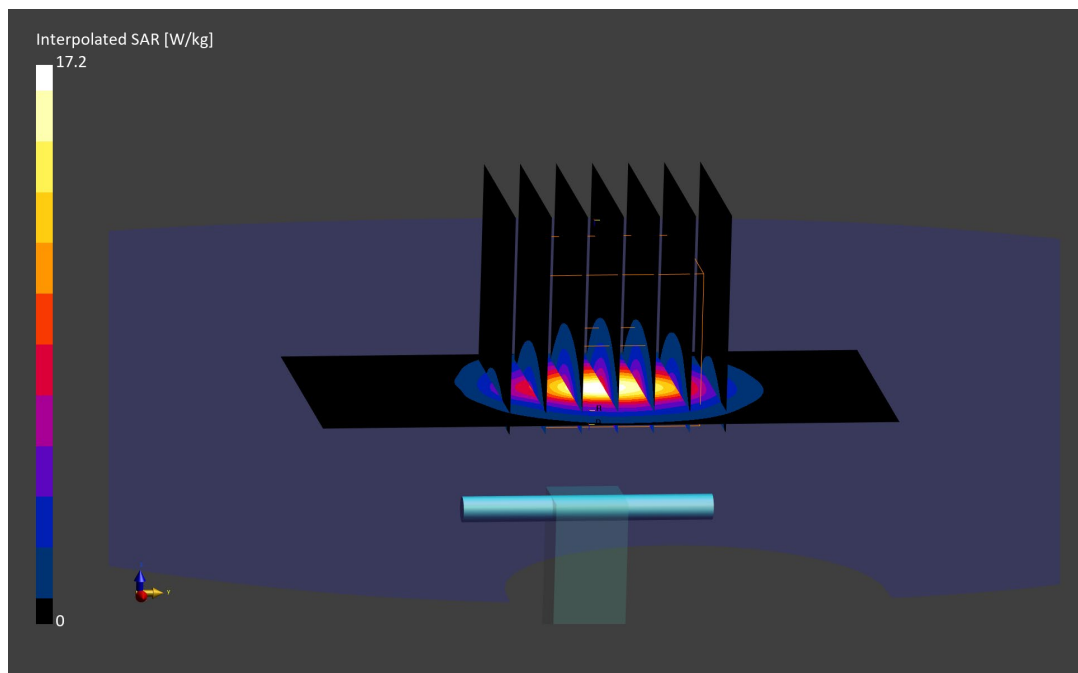

# ELEMENT

**DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1018**

Communication System: UID: 0, CW; Frequency: 3700.0 MHz  
Medium: 3600 Head; Medium parameters used:  
f = 3700.0 MHz; cond = 3.08 S/m; perm = 37.9; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/20/2023; Ambient Temp: 21.7°C; Tissue Temp: 19°C

Probe: EX3DV4 - SN7406; ConvF:(7.02,7.02,7.02); Calibrated: 2022-07-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1677; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 2064  
Measurement SW: DASY Module SAR V16.2.0.1425

## 3700 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (28.0 x 28.0 x 28.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 17.3 W/kg

**SAR(1 g) = 6.56 W/kg; SAR(10 g) = 2.46 W/kg**

Deviation (1 g) = -2.09%; Deviation (10 g) = 1.65%;

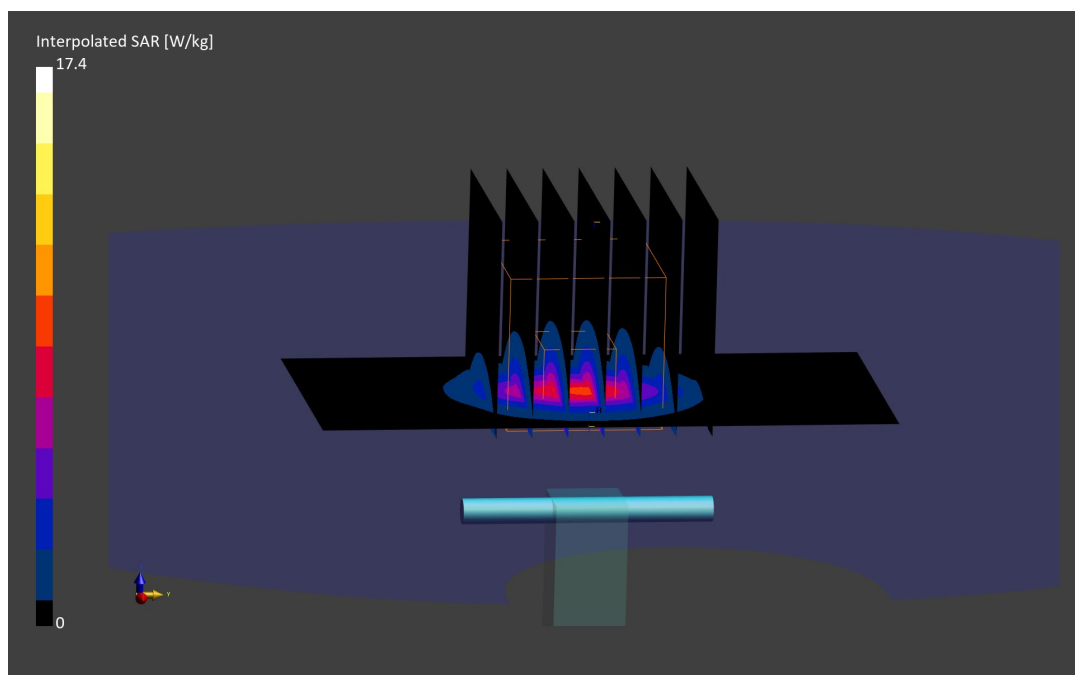

# ELEMENT

**DUT: Dipole 3900.0 MHz; Type: D3900V2 - SN1062**

Communication System: UID: 0, CW; Frequency: 3900.0 MHz  
Medium: 3600 Head; Medium parameters used:  
f = 3900.0 MHz; cond = 3.18 S/m; perm = 38.5; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/15/2023; Ambient Temp: 21.6°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7416; ConvF:(6.4,6.4,6.4); Calibrated: 2022-05-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn701; Calibrated: 2022-05-16  
Phantom: Twin-SAM V8.0; Serial: 2067  
Measurement SW: DASY Module SAR V16.2.0.1425

## 3900 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (28.0 x 28.0 x 28.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 16.9 W/kg

**SAR(1 g) = 6.43 W/kg; SAR(10 g) = 2.29 W/kg**

Deviation (1 g) = -6.27%; Deviation (10 g) = -3.78%;

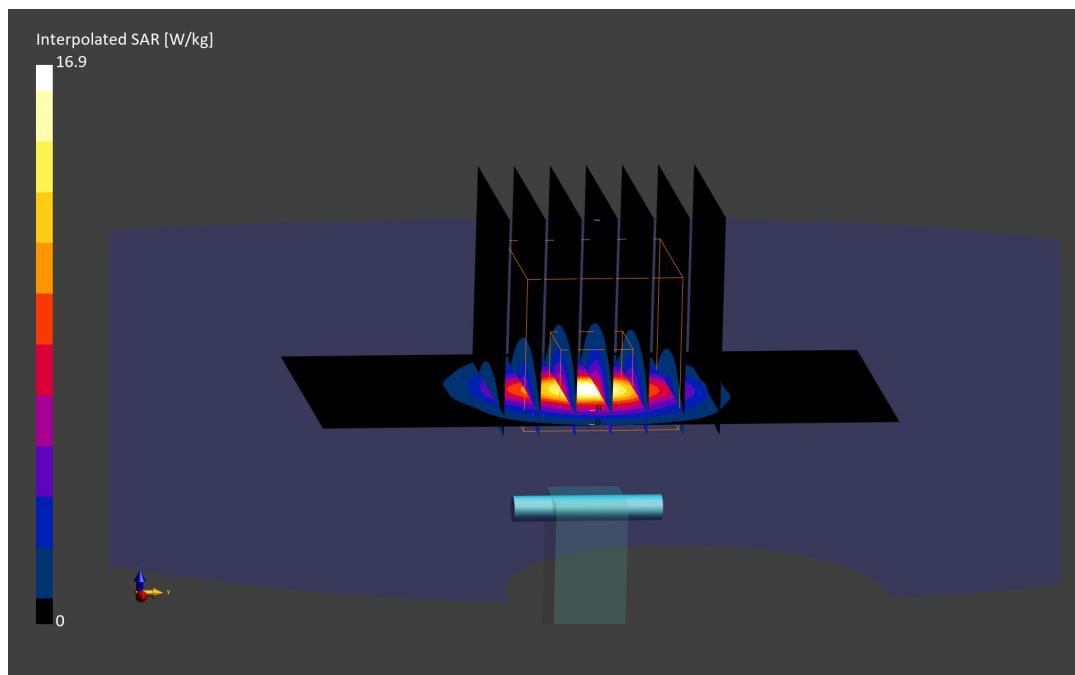

# ELEMENT

**DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1057**

Communication System: UID: 0, CW; Frequency: 5250.0 MHz  
Medium: 5200-5800 Head; Medium parameters used:  
f = 5250.0 MHz; cond = 4.79 S/m; perm = 35.6; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/12/2023; Ambient Temp: 19.1°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7570; ConvF:(5.52,5.52,5.52); Calibrated: 2023-01-11  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1558; Calibrated: 2023-01-17  
Phantom: Twin-SAM V8.0; Serial: 2060  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5250 MHz System Verification at 17 dBm (50 mW)

**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.1 W/kg

**SAR(1 g) = 3.86 W/kg; SAR(10 g) = 1.12 W/kg**

Deviation (1 g) = -4.93%; Deviation (10 g) = -3.45%





# ELEMENT

**DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1057**

Communication System: UID: 0, CW; Frequency: 5600.0 MHz  
Medium: 5200-5800 Head; Medium parameters used:  
f = 5600.0 MHz; cond = 5.22 S/m; perm = 34.8; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/12/2023; Ambient Temp: 19.1°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7570; ConvF:(4.84,4.84,4.84); Calibrated: 2023-01-11  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1558; Calibrated: 2023-01-17  
Phantom: Twin-SAM V8.0; Serial: 2060  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5600 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.7 W/kg

**SAR(1 g) = 4.19 W/kg; SAR(10 g) = 1.20 W/kg**

Deviation (1 g) = -0.48%; Deviation (10 g) = 0.42%

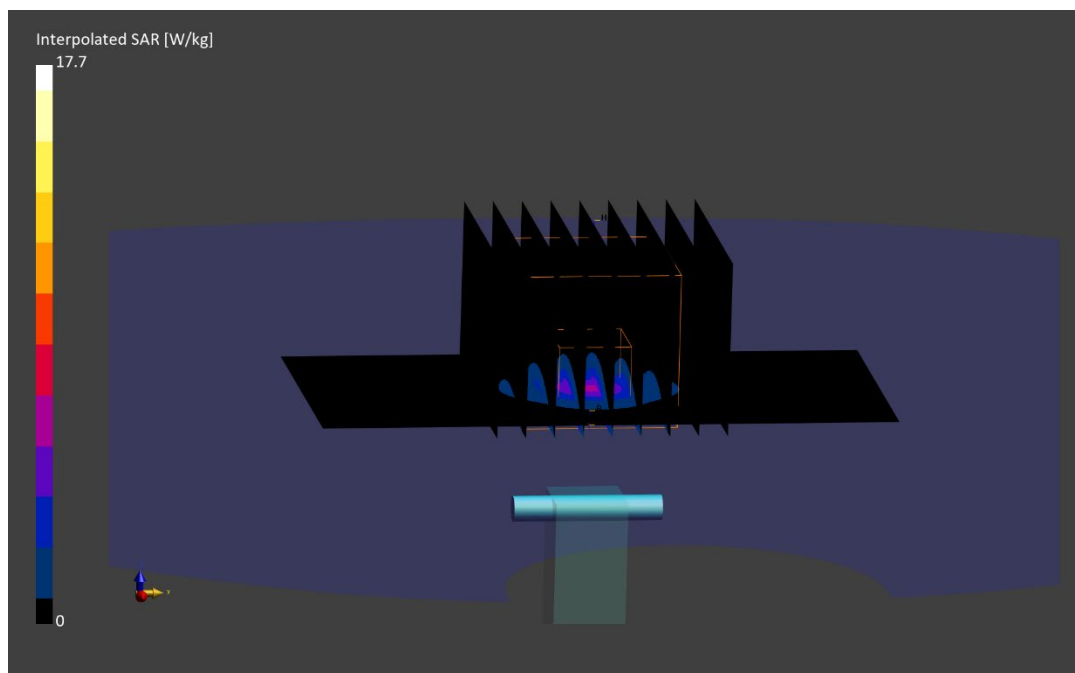

# ELEMENT

**DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1057**

Communication System: UID: 0, CW; Frequency: 5750.0 MHz  
Medium: 5200-5800 Head; Medium parameters used:  
f = 5750.0 MHz; cond = 5.40 S/m; perm = 34.5; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/12/2023; Ambient Temp: 19.1°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7570; ConvF:(4.92,4.92,4.92); Calibrated: 2023-01-11  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1558; Calibrated: 2023-01-17  
Phantom: Twin-SAM V8.0; Serial: 2060  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5750 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.3 W/kg

**SAR(1 g) = 3.99 W/kg; SAR(10 g) = 1.13 W/kg**

Deviation (1 g) = -1.24%; Deviation (10 g) = -1.31%

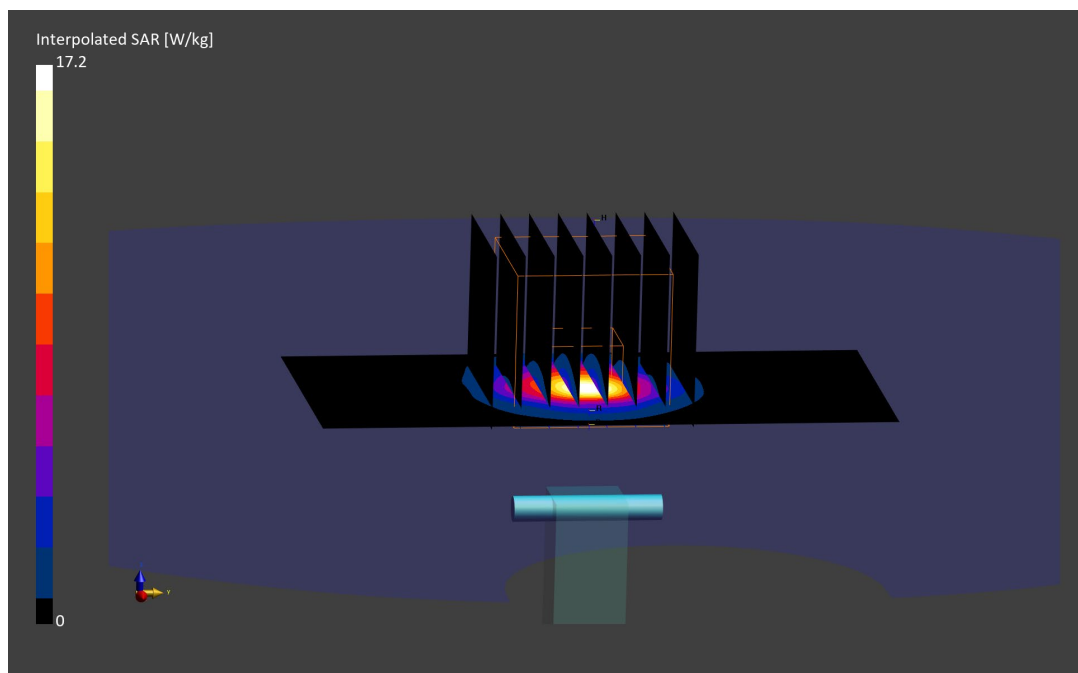

# ELEMENT

**DUT: Dipole 5800.0 MHz; Type: D5GHzV2 - SN1057**

Communication System: UID: 0, CW; Frequency: 5800.0 MHz  
Medium: 5200-5800 Head; Medium parameters used:  
f = 5800.0 MHz; cond = 5.47 S/m; perm = 34.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/12/2023; Ambient Temp: 19.1°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7570; ConvF:(4.92,4.92,4.92); Calibrated: 2023-01-11  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1558; Calibrated: 2023-01-17  
Phantom: Twin-SAM V8.0; Serial: 2060  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5800 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.3 W/kg

**SAR(1 g) = 3.96 W/kg; SAR(10 g) = 1.12 W/kg**

Deviation (1 g) = -3.53%; Deviation (10 g) = -2.61%

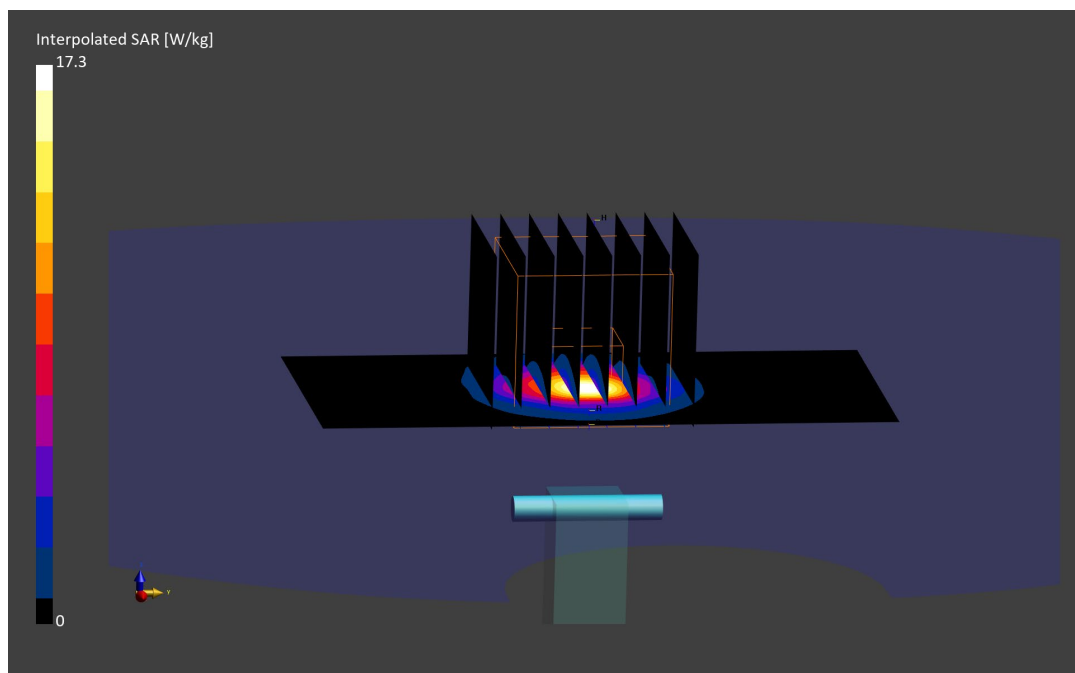

# ELEMENT

**DUT: Dipole 750.0 MHz; Type: D750V3 - SN1161**

Communication System: UID: 0, CW; Frequency: 750.0 MHz  
Medium: 750 Body; Medium parameters used:  
f = 750.0 MHz; cond = 0.939 S/m; perm = 54.0; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 03/06/2023; Ambient Temp: 22.7°C; Tissue Temp: 20.3°C

Probe: EX3DV4 - SN7570; ConvF:(10.26,10.26,10.26); Calibrated: 2023-01-11  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1558; Calibrated: 2023-01-17  
Phantom: Twin-SAM V8.0; Serial: 2060  
Measurement SW: DASY Module SAR V16.2.0.1425

## 750 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.68 W/kg

**SAR(1 g) = 1.73 W/kg; SAR(10 g) = 1.15 W/kg**

Deviation (1 g) = -1.59%; Deviation (10 g) = -1.54%;

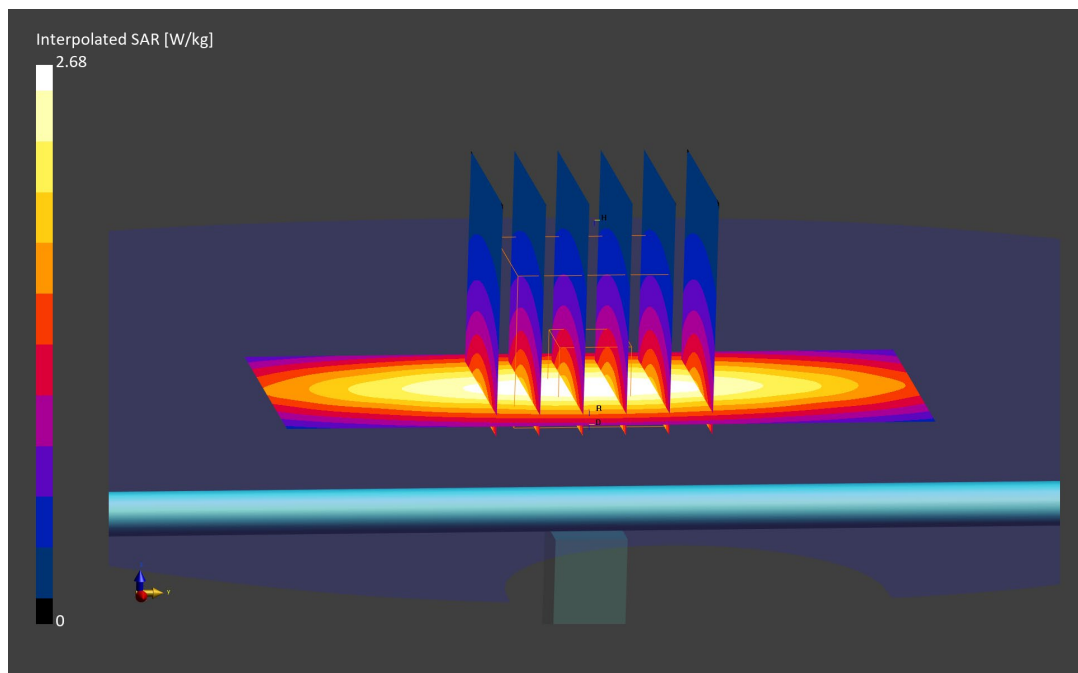

# ELEMENT

**DUT: Dipole 750.0 MHz; Type: D750V3 - SN1034**

Communication System: UID: 0, CW; Frequency: 750.0 MHz  
Medium: 750 Body; Medium parameters used:  
f = 750.0 MHz; cond = 0.955 S/m; perm = 55.7; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 03/07/2023; Ambient Temp: 21.4°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7639; ConvF:(10.83,10.83,10.83); Calibrated: 2022-11-14  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1646; Calibrated: 2022-11-10  
Phantom: Twin-SAM V8.0; Serial: 1936  
Measurement SW: DASY Module SAR V16.2.0.1425

## 750 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.68 W/kg

**SAR(1 g) = 1.72 W/kg; SAR(10 g) = 1.14 W/kg**

Deviation (1 g) = -0.81%; Deviation (10 g) = -0.35%

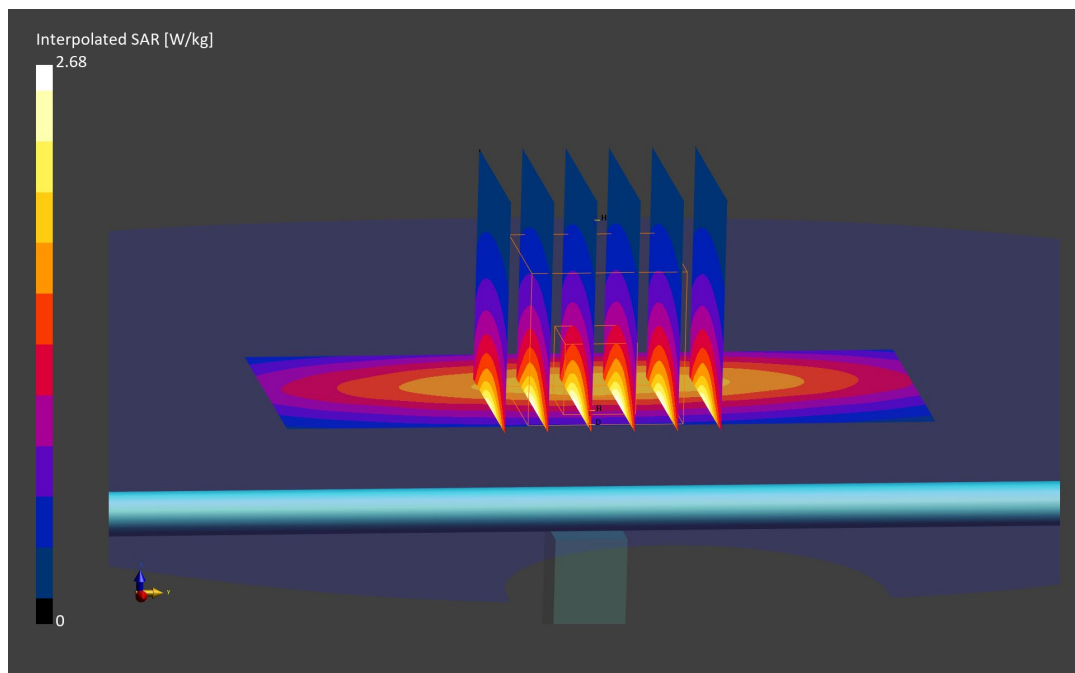

# ELEMENT

**DUT: Dipole 750.0 MHz; Type: D750V3 - SN1161**

Communication System: UID: 0, CW; Frequency: 750.0 MHz  
Medium: 750 Body; Medium parameters used:  
f = 750.0 MHz; cond = 0.950 S/m; perm = 54.9; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 03/09/2023; Ambient Temp: 20.7°C; Tissue Temp: 19.6°C

Probe: EX3DV4 - SN7570; ConvF:(10.26,10.26,10.26); Calibrated: 2023-01-11  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1558; Calibrated: 2023-01-17  
Phantom: Twin-SAM V8.0; Serial: 2060  
Measurement SW: DASY Module SAR V16.0.2.83

## 750 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.71 W/kg

**SAR(1 g) = W/kg; SAR(10 g) = W/kg**

Deviation (1 g) = -0.46%; Deviation (10 g) = -0.68%;

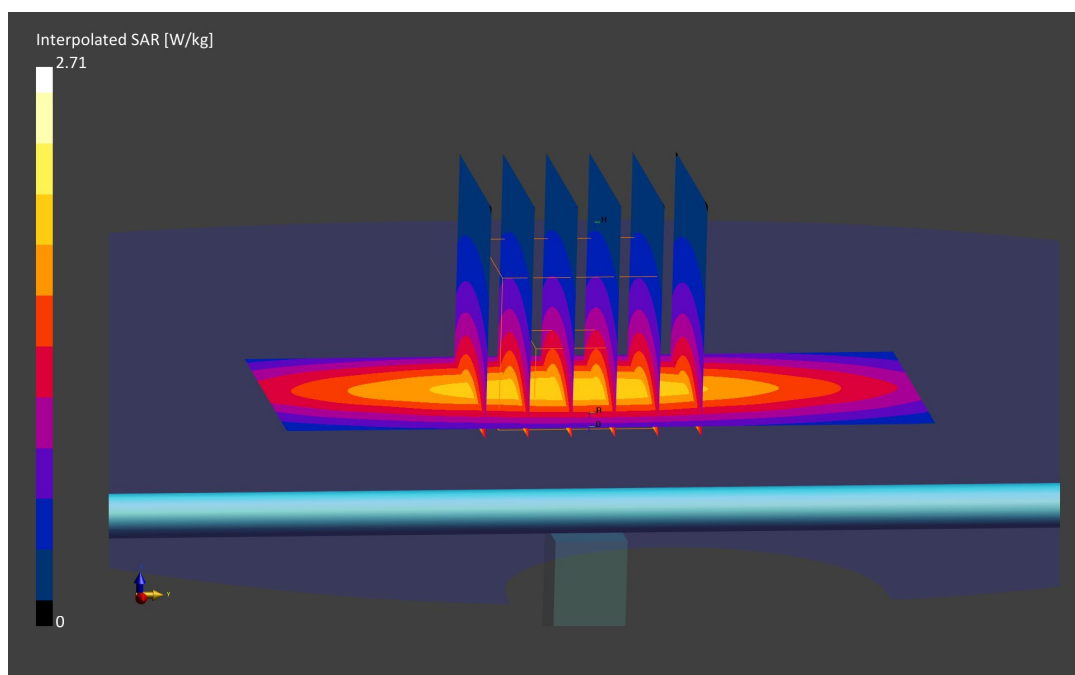

# ELEMENT

**DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d132**

Communication System: UID: 0, CW; Frequency: 835.0 MHz  
Medium: 835 Body; Medium parameters used:  
f = 835.0 MHz; cond = 0.955 S/m; perm = 55.1; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 03/06/2023; Ambient Temp: 23.7°C; Tissue Temp: 20.1°C

Probe: EX3DV4 - SN7406; ConvF:(9.48,9.48,9.48); Calibrated: 2022-07-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1677; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 2064  
Measurement SW: DASY Module SAR V16.2.0.1425

## 835 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.24 W/kg

**SAR(1 g) = 2.02 W/kg; SAR(10 g) = 1.33 W/kg**

Deviation (1 g) = 2.96%; Deviation (10 g) = 3.26%

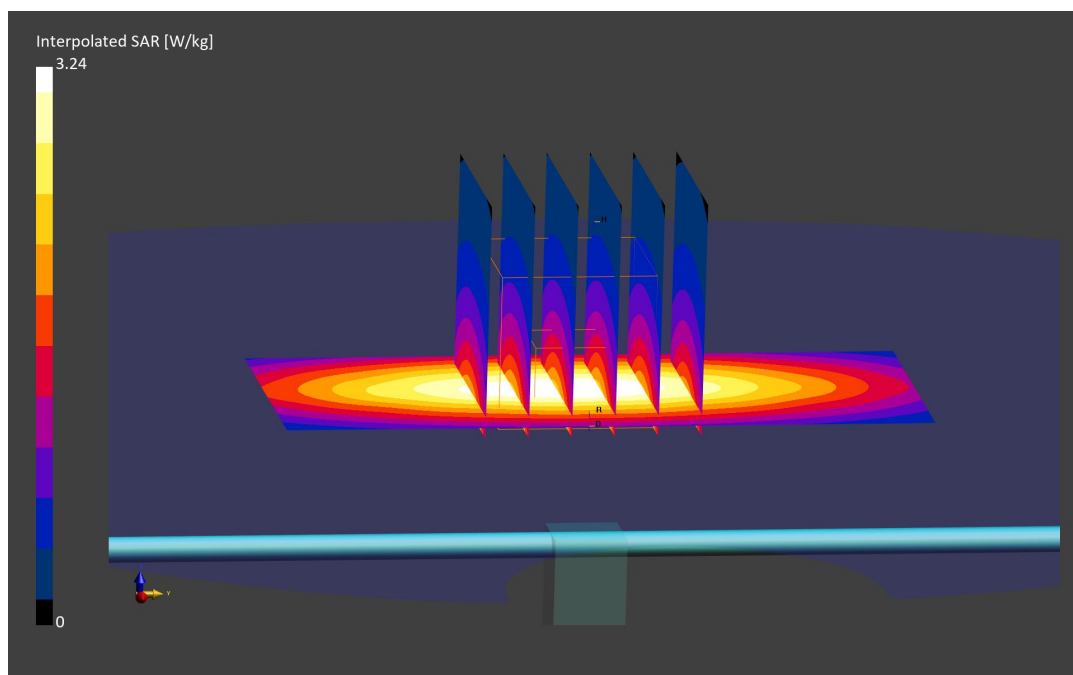

# ELEMENT

**DUT: Dipole 835.0 MHz; Type: D835V2 - SN460**

Communication System: UID: 0, CW; Frequency: 835.0 MHz  
Medium: 835 Body; Medium parameters used:  
f = 835.0 MHz; cond = 0.948 S/m; perm = 56.0; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 03/09/2023; Ambient Temp: 22.0°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN7639; ConvF:(10.6,10.6,10.6); Calibrated: 2022-11-14  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1646; Calibrated: 2022-11-10  
Phantom: Twin-SAM V8.0; Serial: 1936  
Measurement SW: DASY Module SAR V16.2.0.1425

## 835 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.08 W/kg

**SAR(1 g) = 1.99 W/kg; SAR(10 g) = 1.32 W/kg**

Deviation (1 g) = 1.63%; Deviation (10 g) = 2.17%

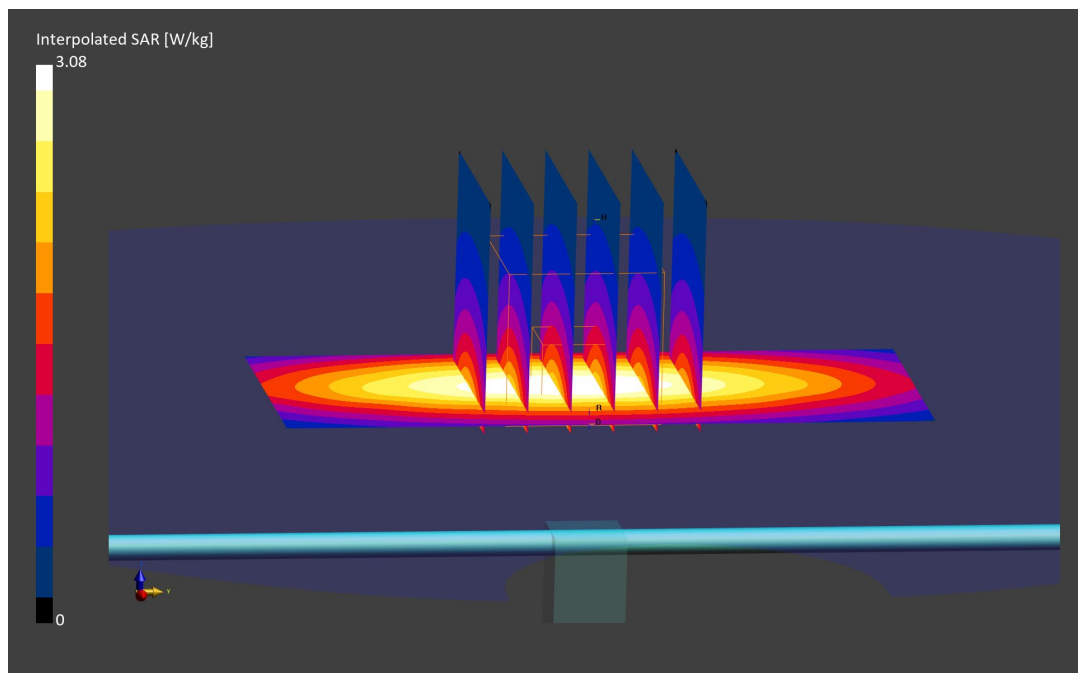



# ELEMENT

**DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d132**

Communication System: UID: 0, CW; Frequency: 835.0 MHz  
Medium: 835 Body; Medium parameters used:  
f = 835.0 MHz; cond = 0.942 S/m; perm = 54.9; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 03/14/2023; Ambient Temp: 22.9°C; Tissue Temp: 19.7°C

Probe: EX3DV4 - SN7406; ConvF:(9.48,9.48,9.48); Calibrated: 2022-07-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1677; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 2064  
Measurement SW: DASY Module SAR V16.2.0.1425

## 835 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.08 W/kg

**SAR(1 g) = 1.86 W/kg; SAR(10 g) = 1.22 W/kg**

Deviation (1 g) = -5.20%; Deviation (10 g) = -5.28%

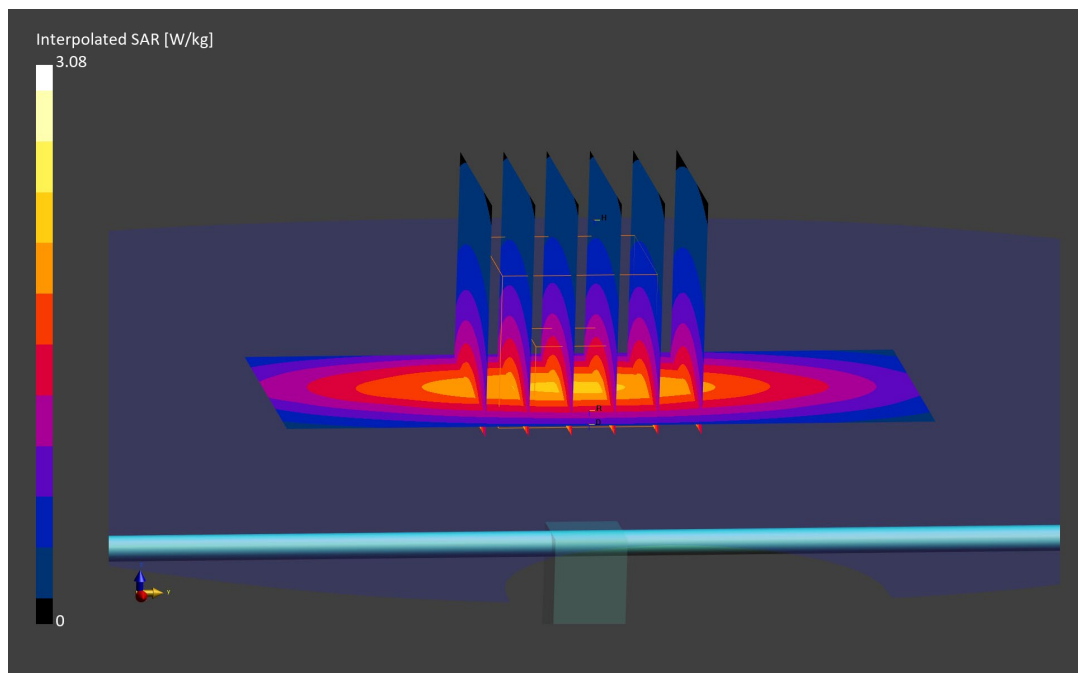

# ELEMENT

**DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1104**

Communication System: UID: 0, CW; Frequency: 1750.0 MHz  
Medium: 1750 Body; Medium parameters used:  
f = 1750.0 MHz; cond = 1.42 S/m; perm = 52.8; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/13/2023; Ambient Temp: 21.9°C; Tissue Temp: 20.8°C

Probe: EX3DV4 - SN7639; ConvF:(9.36,9.36,9.36); Calibrated: 2022-11-14  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1646; Calibrated: 2022-11-10  
Phantom: Twin-SAM V8.0; Serial: 1936  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1750 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.70 W/kg

**SAR(1 g) = 3.49 W/kg; SAR(10 g) = 1.85 W/kg**

Deviation (1 g) = -3.86%; Deviation (10 g) = -4.15%;

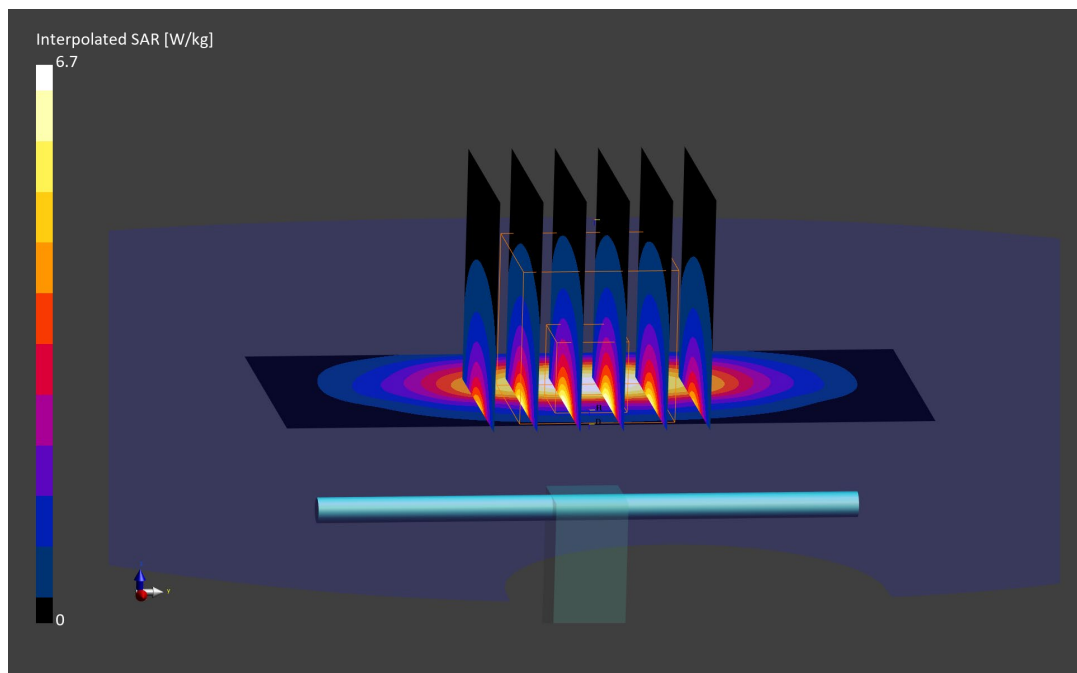

# ELEMENT

**DUT: Dipole 1750.0 MHz; Type: D1765V2 - SN1008**

Communication System: UID: 0, CW; Frequency: 1750.0 MHz  
Medium: 1750 Body; Medium parameters used:  
f = 1750.0 MHz; cond = 1.46 S/m; perm = 53.3; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/14/2023; Ambient Temp: 21.7°C; Tissue Temp: 19.7°C

Probe: EX3DV4 - SN7406; ConvF:(8.06,8.06,8.06); Calibrated: 2022-07-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1677; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 2064  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1750 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.26 W/kg

**SAR(1 g) = 3.82 W/kg; SAR(10 g) = 2.03 W/kg**

Deviation (1 g) = 1.06%; Deviation (10 g) = 2.01%;

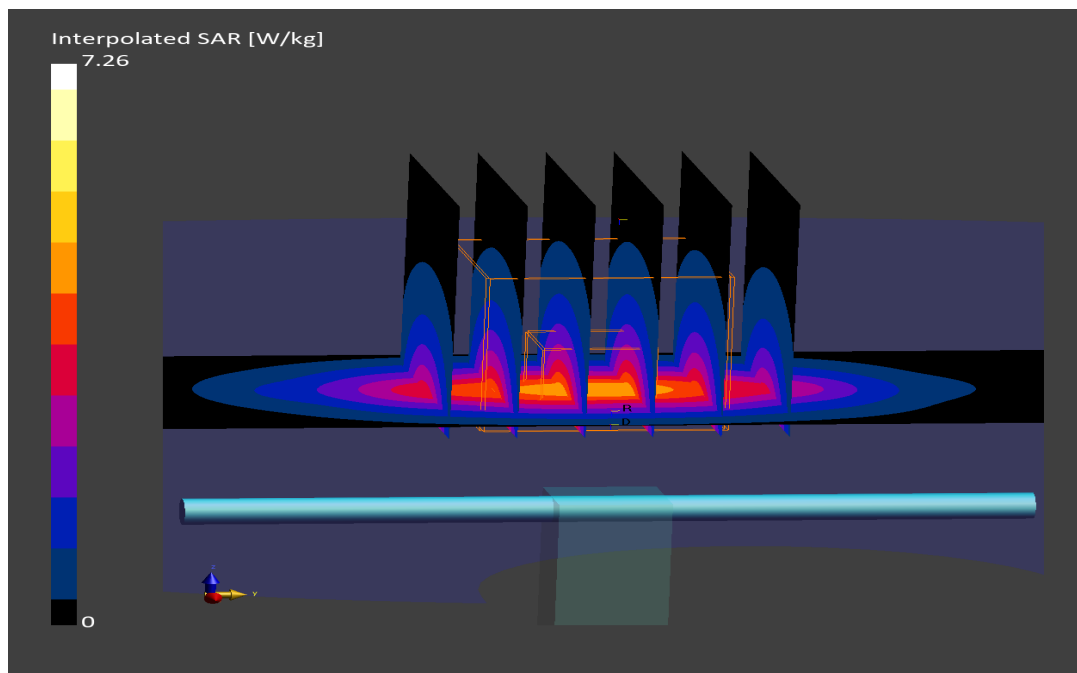

# ELEMENT

**DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1150**

Communication System: UID: 0, CW; Frequency: 1750.0 MHz  
Medium: 1750 Body; Medium parameters used:  
f = 1750.0 MHz; cond = 1.52 S/m; perm = 53.1; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/15/2023; Ambient Temp: 19.1°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7409; ConvF:(8.01,8.01,8.01); Calibrated: 2022-06-16  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1334; Calibrated: 2022-06-14  
Phantom: Twin-SAM V5.0; Serial: 1792  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1750 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.92 W/kg

**SAR(1 g) = 3.84 W/kg; SAR(10 g) = 2.07 W/kg**

Deviation (1 g) = 1.59%; Deviation (10 g) = 3.50%;

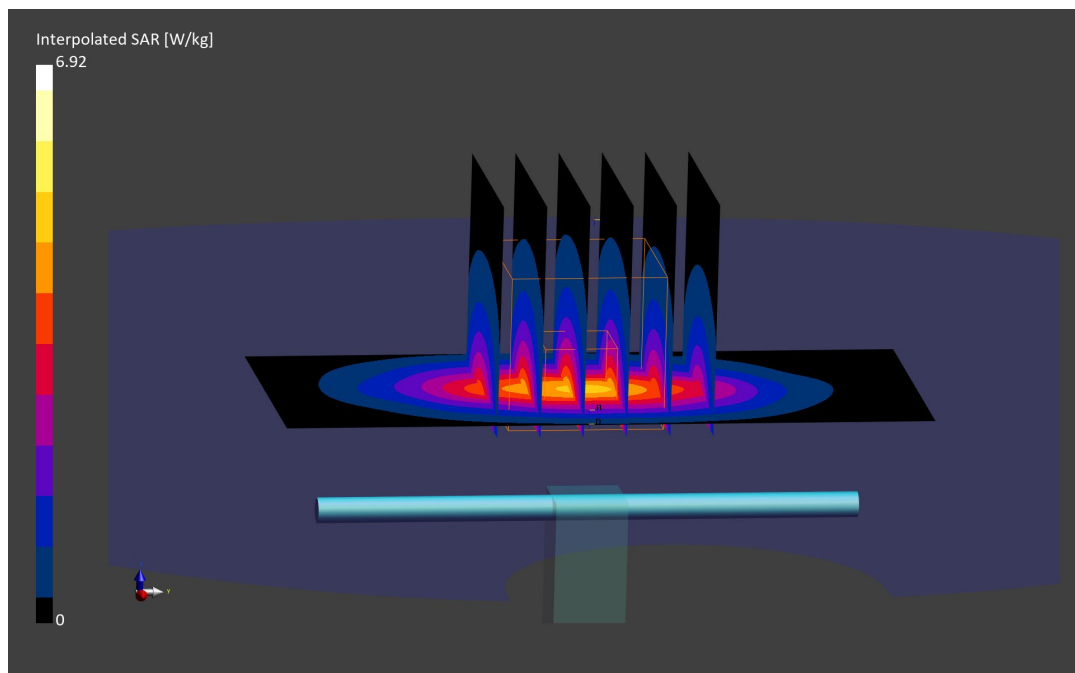

# ELEMENT

**DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1150**

Communication System: UID: 0, CW; Frequency: 1750.0 MHz  
Medium: 1750 Body; Medium parameters used:  
f = 1750.0 MHz; cond = 1.49 S/m; perm = 53.7; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/19/2023; Ambient Temp: 21.9°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7409; ConvF:(8.01,8.01,8.01); Calibrated: 2022-06-16  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1334; Calibrated: 2022-06-14  
Phantom: Twin-SAM V5.0; Serial: 1792  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1750 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.97 W/kg

**SAR(1 g) = 3.89 W/kg; SAR(10 g) = 2.09 W/kg**

Deviation (1 g) = 2.91%; Deviation (10 g) = 4.50%;

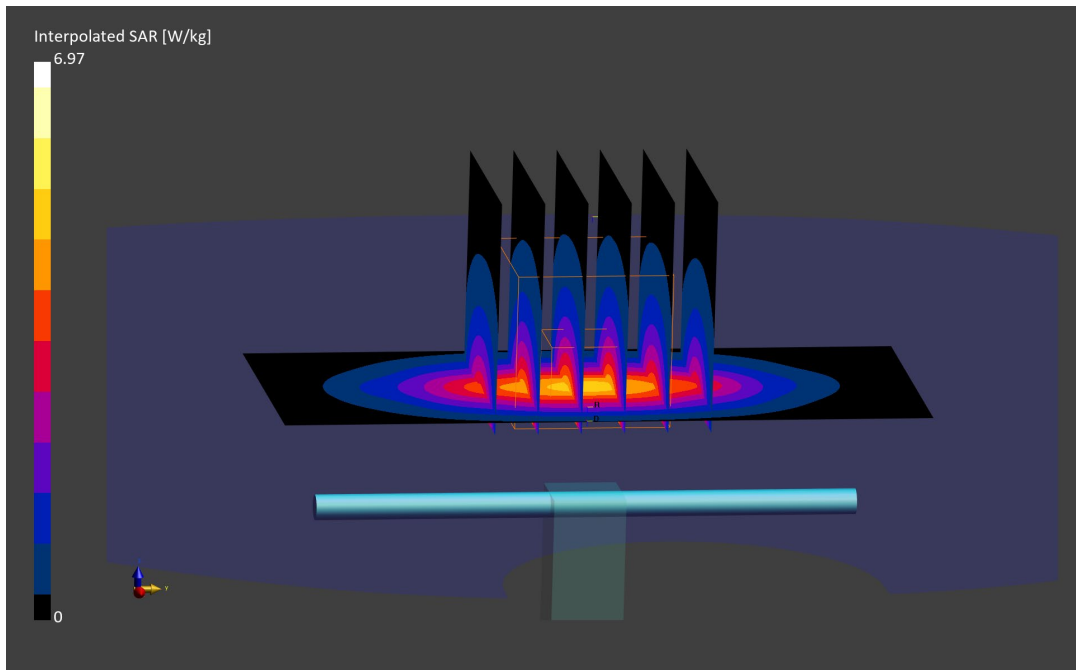

# ELEMENT

**DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d181**

Communication System: UID: 0, CW; Frequency: 1900.0 MHz  
Medium: 1900 Body; Medium parameters used:  
f = 1900.0 MHz; cond = 1.53 S/m; perm = 52.6; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/13/2023; Ambient Temp: 21.9°C; Tissue Temp: 20.8°C

Probe: EX3DV4 - SN7639; ConvF:(8.96,8.96,8.96); Calibrated: 2022-11-14  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1646; Calibrated: 2022-11-10  
Phantom: Twin-SAM V8.0; Serial: 1936  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1900 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.86 W/kg

**SAR(1 g) = 4.04 W/kg; SAR(10 g) = 2.08 W/kg**

Deviation (1 g) = 1.76%; Deviation (10 g) = -0.95%;

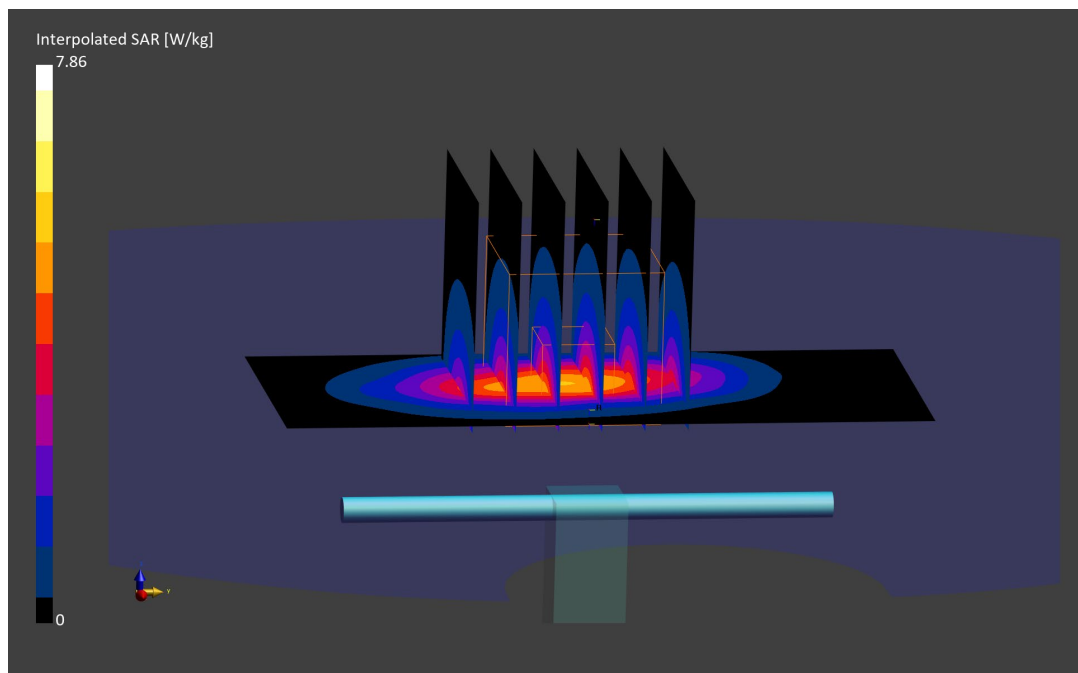

# ELEMENT

**DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d148**

Communication System: UID: 0, CW; Frequency: 1900.0 MHz  
Medium: 1900 Body; Medium parameters used:  
f = 1900.0 MHz; cond = 1.56 S/m; perm = 53.0; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/15/2023; Ambient Temp: 19.1°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7409; ConvF:(7.66,7.66,7.66); Calibrated: 2022-06-16  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1334; Calibrated: 2022-06-14  
Phantom: Twin-SAM V5.0; Serial: 1792  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1900 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.57 W/kg

**SAR(1 g) = 4.32 W/kg; SAR(10 g) = 2.25 W/kg**

Deviation (1 g) = 8.27%; Deviation (10 g) = 7.66%;

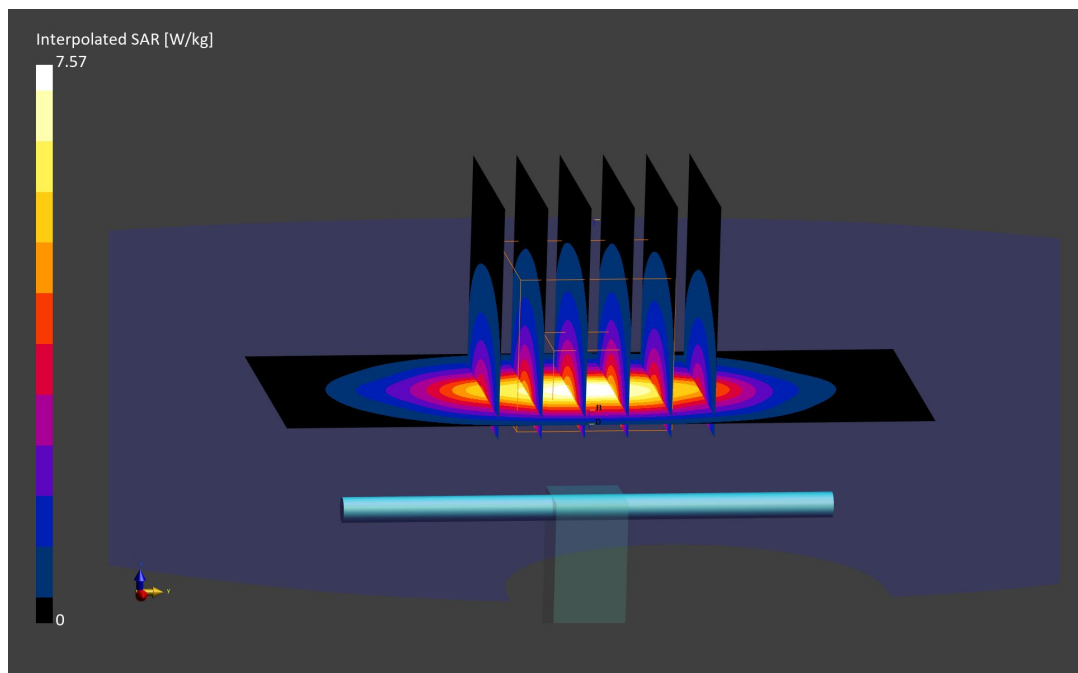

# ELEMENT

**DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d148**

Communication System: UID: 0, CW; Frequency: 1900.0 MHz  
Medium: 1900 Body; Medium parameters used:  
f = 1900.0 MHz; cond = 1.57 S/m; perm = 51.7; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/17/2023; Ambient Temp: 21.1°C; Tissue Temp: 19.3°C

Probe: EX3DV4 - SN7409; ConvF:(7.66,7.66,7.66); Calibrated: 2022-06-16  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1334; Calibrated: 2022-06-14  
Phantom: Twin-SAM V5.0; Serial: 1792  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1900 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.32 W/kg

**SAR(1 g) = 4.17 W/kg; SAR(10 g) = 2.18 W/kg**

Deviation (1 g) = 4.51%; Deviation (10 g) = 4.31%;

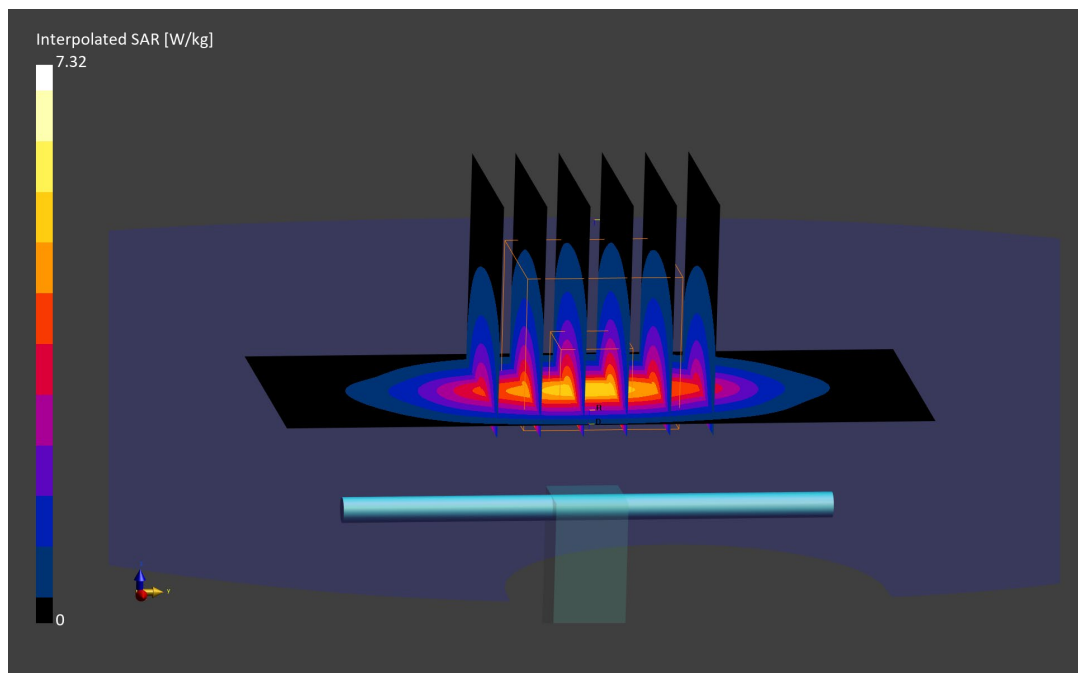



# ELEMENT

**DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d149**

Communication System: UID: 0, CW; Frequency: 1900.0 MHz  
Medium: 1900 Body; Medium parameters used:  
f = 1900.0 MHz; cond = 1.53 S/m; perm = 52.2; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/20/2023; Ambient Temp: 22.1°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7551; ConvF:(7.83,7.83,7.83); Calibrated: 2022-11-11  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1323; Calibrated: 2022-11-10  
Phantom: Twin-SAM V8.0; Serial: 2057  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1900 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.97 W/kg

**SAR(1 g) = 3.95 W/kg; SAR(10 g) = 2.05 W/kg**

Deviation (1 g) = -2.23%; Deviation (10 g) = -2.84%

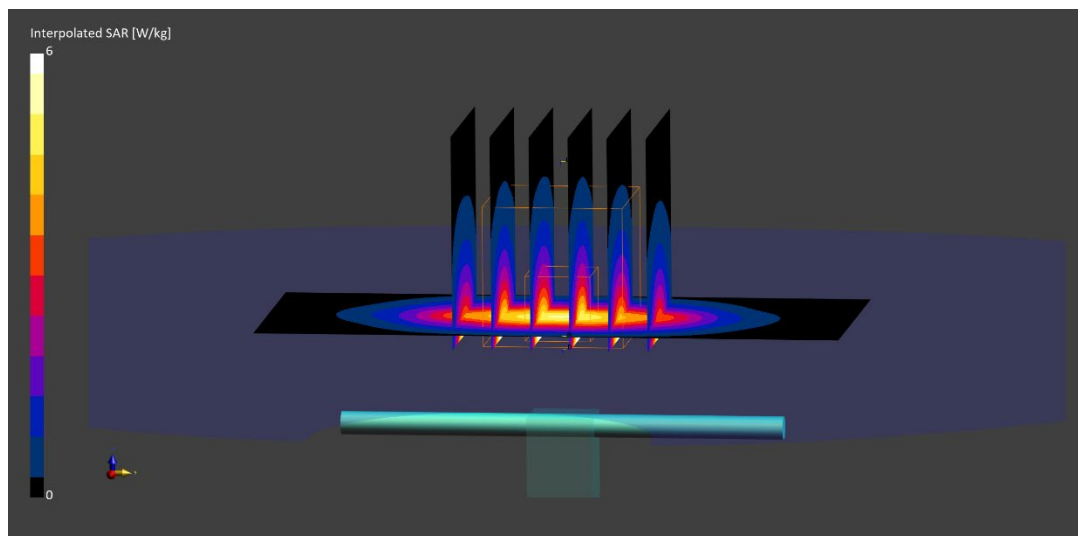

# ELEMENT

**DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1038**

Communication System: UID: 0, CW; Frequency: 2300.0 MHz  
Medium: 2450 Body; Medium parameters used:  
f = 2300.0 MHz; cond = 1.84 S/m; perm = 52.1; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/13/2023; Ambient Temp: 22.3°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7420; ConvF:(7.6,7.6,7.6); Calibrated: 2022-10-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1333; Calibrated: 2022-10-13  
Phantom: Twin-SAM V8.0; Serial: 1736  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2300 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.1 W/kg

**SAR(1 g) = 5.01 W/kg; SAR(10 g) = 2.37 W/kg**

Deviation (1 g) = 5.92%; Deviation (10 g) = 3.95%;

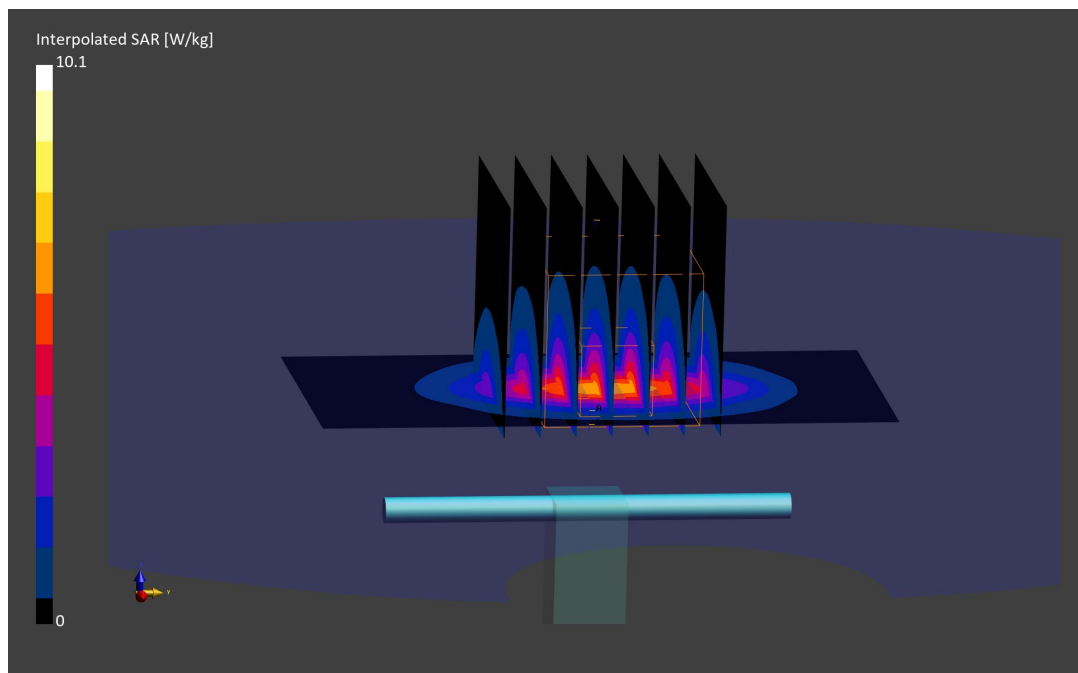

# ELEMENT

**DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1073**

Communication System: UID: 0, CW; Frequency: 2300.0 MHz  
Medium: 2450 Body; Medium parameters used:  
f = 2300.0 MHz; cond = 1.80 S/m; perm = 53.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/13/2023; Ambient Temp: 22.3°C; Tissue Temp: 21.7°C

Probe: EX3DV4 - SN7551; ConvF:(7.75,7.75,7.75); Calibrated: 2022-11-11  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1323; Calibrated: 2022-11-10  
Phantom: Twin-SAM V8.0; Serial: 2057  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2300 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.05 W/kg

**SAR(1 g) = 4.66 W/kg; SAR(10 g) = 2.21 W/kg**

Deviation (1 g) = -3.12%; Deviation (10 g) = -6.36%

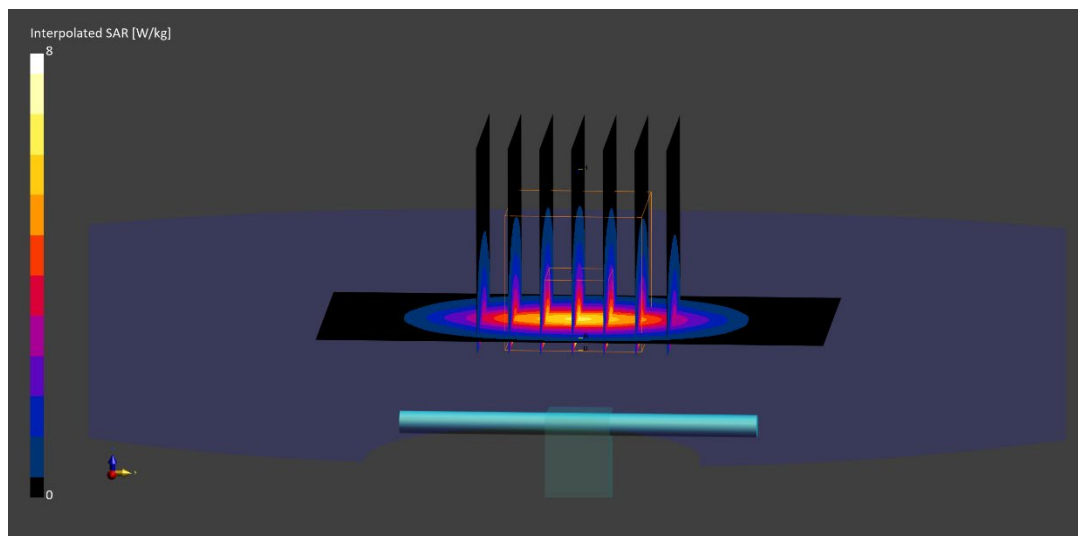

# ELEMENT

**DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1064**

Communication System: UID: 0, CW; Frequency: 2300.0 MHz  
Medium: 2450 Body; Medium parameters used:  
f = 2300.0 MHz; cond = 1.82 S/m; perm = 51.5; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/15/2023; Ambient Temp: 22.1°C; Tissue Temp: 22.3°C

Probe: EX3DV4 - SN7420; ConvF:(7.6,7.6,7.6); Calibrated: 2022-10-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1333; Calibrated: 2022-10-13  
Phantom: Twin-SAM V8.0; Serial: 1736  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2300 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.94 W/kg

**SAR(1 g) = 4.92 W/kg; SAR(10 g) = 2.37 W/kg**

Deviation (1 g) = 1.65%; Deviation (10 g) = 1.72%

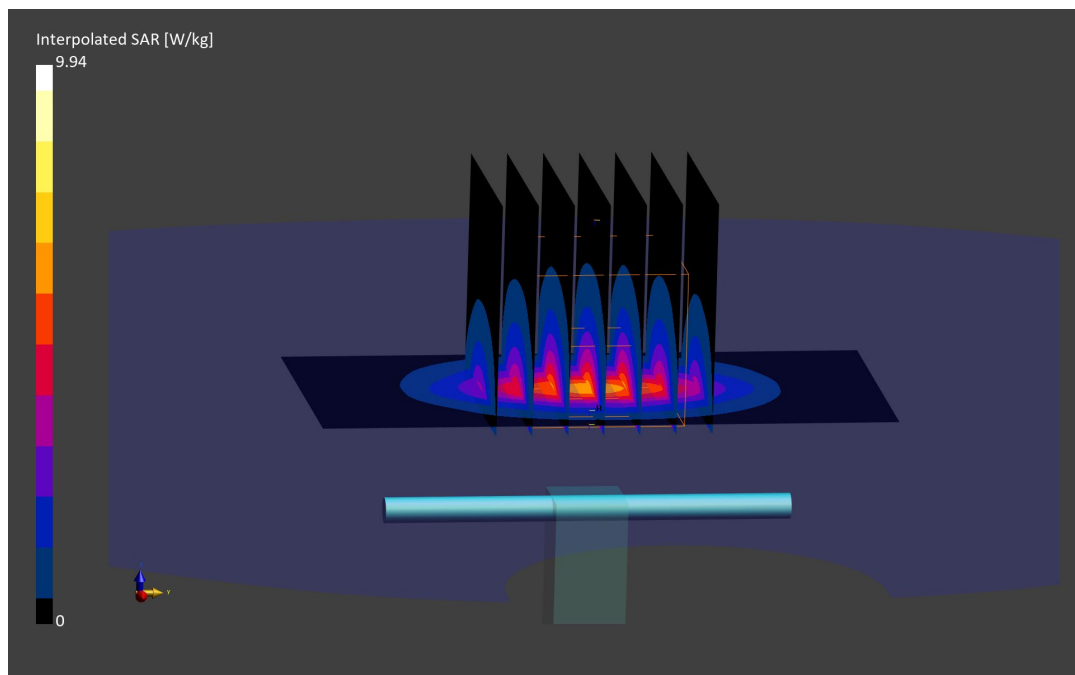

# ELEMENT

**DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN981**

Communication System: UID: 0, CW; Frequency: 2450.0 MHz  
Medium: 2450 Body; Medium parameters used:  
f = 2450.0 MHz; cond = 2.01 S/m; perm = 51.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/01/2023; Ambient Temp: 22.3°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7410; ConvF:(7.52,7.52,7.52); Calibrated: 2022-07-19  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1583; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 1966  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2450 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.9 W/kg

**SAR(1 g) = 5.14 W/kg; SAR(10 g) = 2.38 W/kg**

Deviation (1 g) = 2.19%; Deviation (10 g) = 0.42%

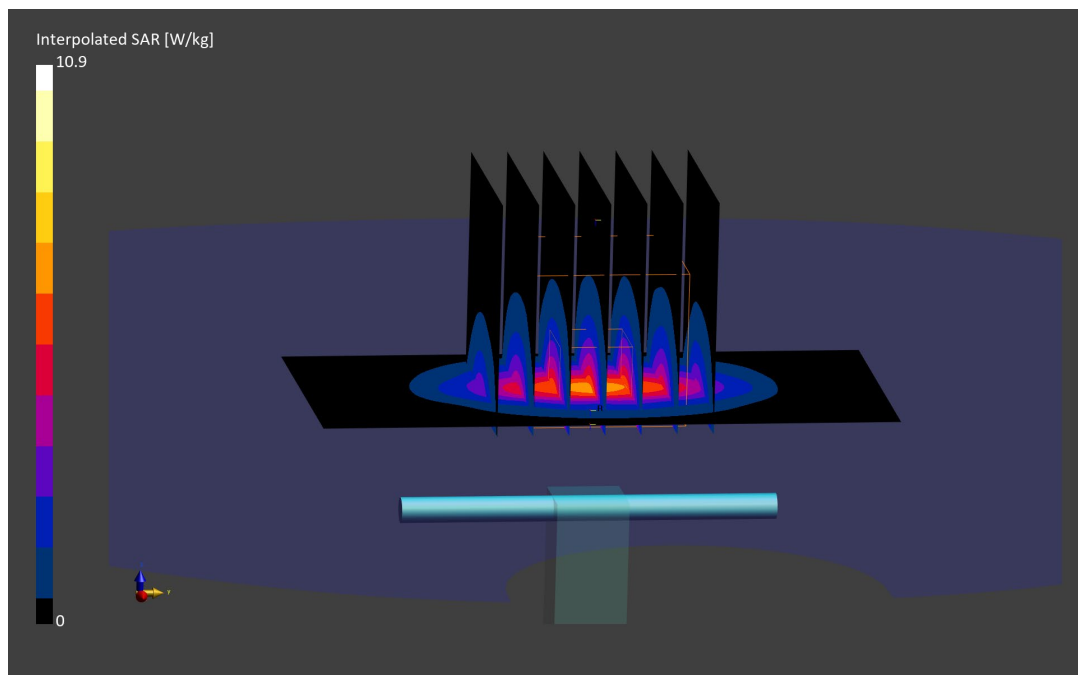

# ELEMENT

**DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN981**

Communication System: UID: 0, CW; Frequency: 2450.0 MHz  
Medium: 2450 Body; Medium parameters used:  
f = 2450.0 MHz; cond = 2.01 S/m; perm = 52.9; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/13/2023; Ambient Temp: 22.3°C; Tissue Temp: 21.7°C

Probe: EX3DV4 - SN7551; ConvF:(7.6,7.6,7.6); Calibrated: 2022-11-11  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1323; Calibrated: 2022-11-10  
Phantom: Twin-SAM V8.0; Serial: 2057  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2450 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.2 W/kg

**SAR(1 g) = 4.83 W/kg; SAR(10 g) = 2.19 W/kg**

Deviation (1 g) = -3.98%; Deviation (10 g) = -7.59%

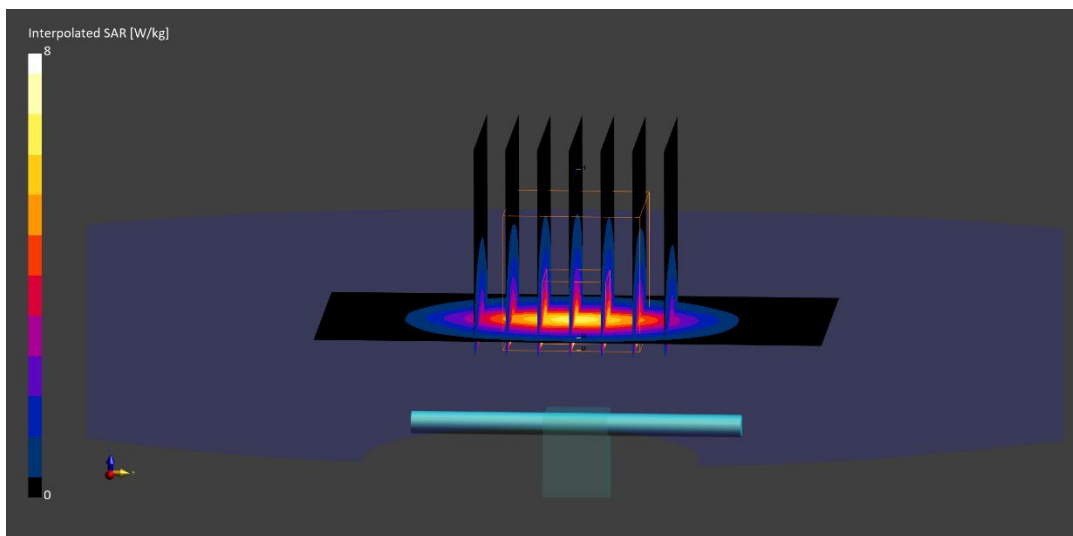

# ELEMENT

**DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750**

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Body; Medium parameters used:

f = 2450.0 MHz; cond = 2.02 S/m; perm = 50.9; density = 1000 kg/m<sup>3</sup>

Phantom Section: Flat; Space: 10 mm

Test Date: 03/15/2023; Ambient Temp: 22.1°C; Tissue Temp: 22.3°C

Probe: EX3DV4 - SN7420; ConvF:(7.47,7.47,7.47); Calibrated: 2022-10-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1333; Calibrated: 2022-10-13

Phantom: Twin-SAM V8.0; Serial: 1736

Measurement SW: DASY Module SAR V16.2.0.1425

## 2450 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.8 W/kg

**SAR(1 g) = 5.20 W/kg; SAR(10 g) = 2.39 W/kg**

Deviation (1 g) = 2.97%; Deviation (10 g) = 0.00%

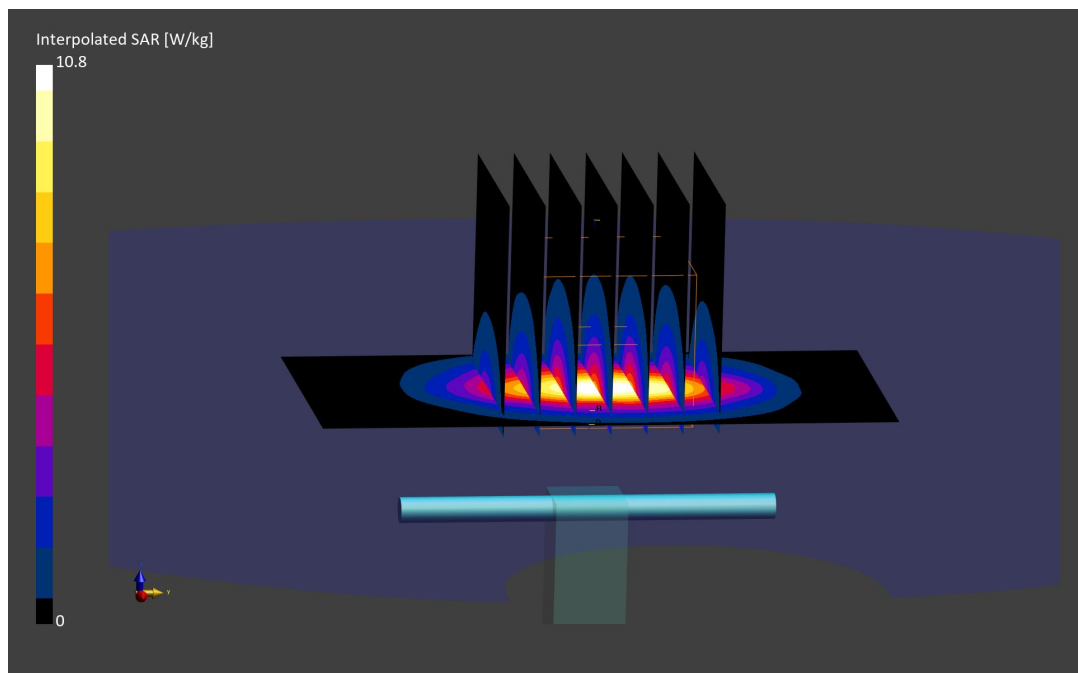

# ELEMENT

**DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1071**

Communication System: UID: 0, CW; Frequency: 2600.0 MHz  
Medium: 2450 Body; Medium parameters used:  
f = 2600.0 MHz; cond = 2.22 S/m; perm = 52.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/13/2023; Ambient Temp: 22.3°C; Tissue Temp: 21.7°C

Probe: EX3DV4 - SN7551; ConvF:(7.45,7.45,7.45); Calibrated: 2022-11-11  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1323; Calibrated: 2022-11-10  
Phantom: Twin-SAM V8.0; Serial: 2057  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2600 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.7 W/kg

**SAR(1 g) = 5.28 W/kg; SAR(10 g) = 2.30 W/kg**

Deviation (1 g) = -2.76%; Deviation (10 g) = -5.35%

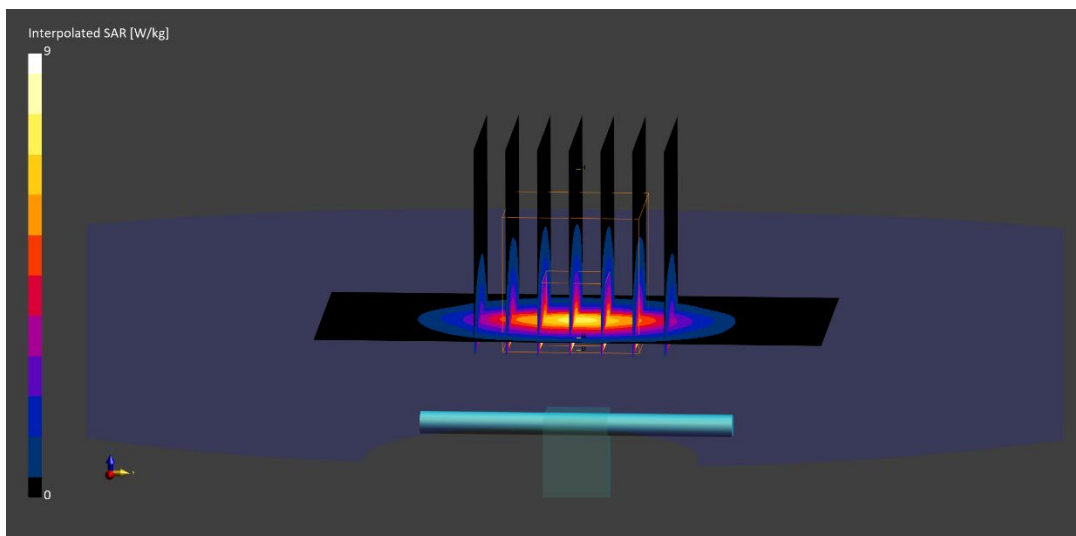



# ELEMENT

**DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1069**

Communication System: UID: 0, CW; Frequency: 2600.0 MHz  
Medium: 2450 Body; Medium parameters used:  
f = 2600.0 MHz; cond = 2.22 S/m; perm = 50.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/15/2023; Ambient Temp: 22.1°C; Tissue Temp: 22.3°C

Probe: EX3DV4 - SN7420; ConvF:(7.27,7.27,7.27); Calibrated: 2022-10-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1333; Calibrated: 2022-10-13  
Phantom: Twin-SAM V8.0; Serial: 1736  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2600 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.4 W/kg

**SAR(1 g) = 5.53 W/kg; SAR(10 g) = 2.42 W/kg**

Deviation (1 g) = 1.65%; Deviation (10 g) = 0.00%

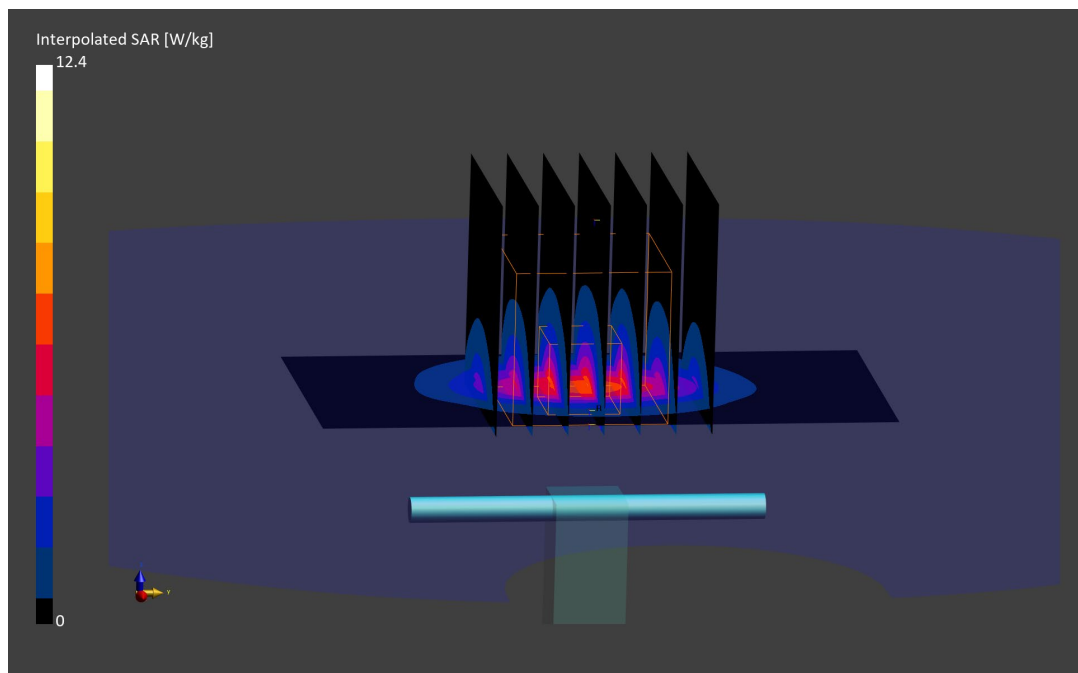

# ELEMENT

**DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1126**

Communication System: UID: 0, CW; Frequency: 3500.0 MHz  
Medium: 3600 Body; Medium parameters used:  
f = 3500.0 MHz; cond = 3.41 S/m; perm = 51.3; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/14/2023; Ambient Temp: 22.1°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN3837; ConvF:(6.19,6.19,6.19); Calibrated: 2023-01-17  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn793; Calibrated: 2023-01-17  
Phantom: Twin-SAM V8.0; Serial: 1944  
Measurement SW: DASY Module SAR V16.2.0.1425

## 3500 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (28.0 x 28.0 x 28.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 16.1 W/kg

**SAR(1 g) = 6.05 W/kg; SAR(10 g) = 2.23 W/kg**

Deviation (1 g) = -4.87%; Deviation (10 g) = -5.51%;

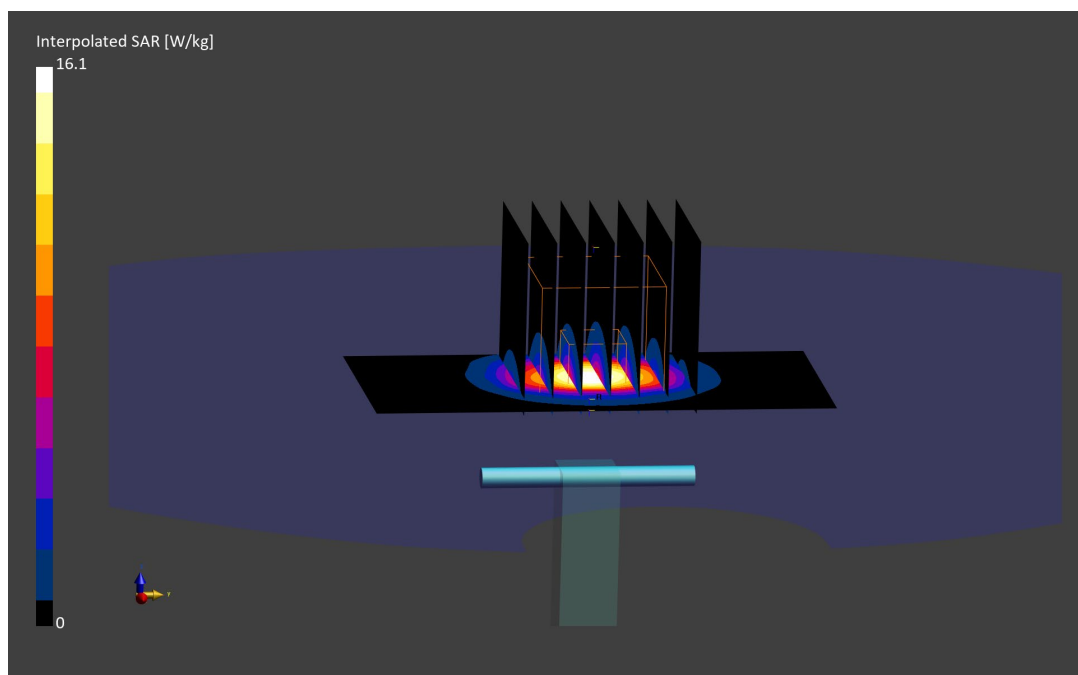

# ELEMENT

**DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1059**

Communication System: UID: 0, CW; Frequency: 3500.0 MHz  
Medium: 3600 Body; Medium parameters used:  
f = 3500.0 MHz; cond = 3.17 S/m; perm = 49.7; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/16/2023; Ambient Temp: 21.3°C; Tissue Temp: 19.7°C

Probe: EX3DV4 - SN7410; ConvF:(6.65,6.65,6.65); Calibrated: 2022-07-19  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1583; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 1966  
Measurement SW: DASY Module SAR V16.2.0.1425

## 3500 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (28.0 x 28.0 x 28.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 15.1 W/kg

**SAR(1 g) = 5.97 W/kg; SAR(10 g) = 2.26 W/kg**

Deviation (1 g) = -5.24%; Deviation (10 g) = -3%;

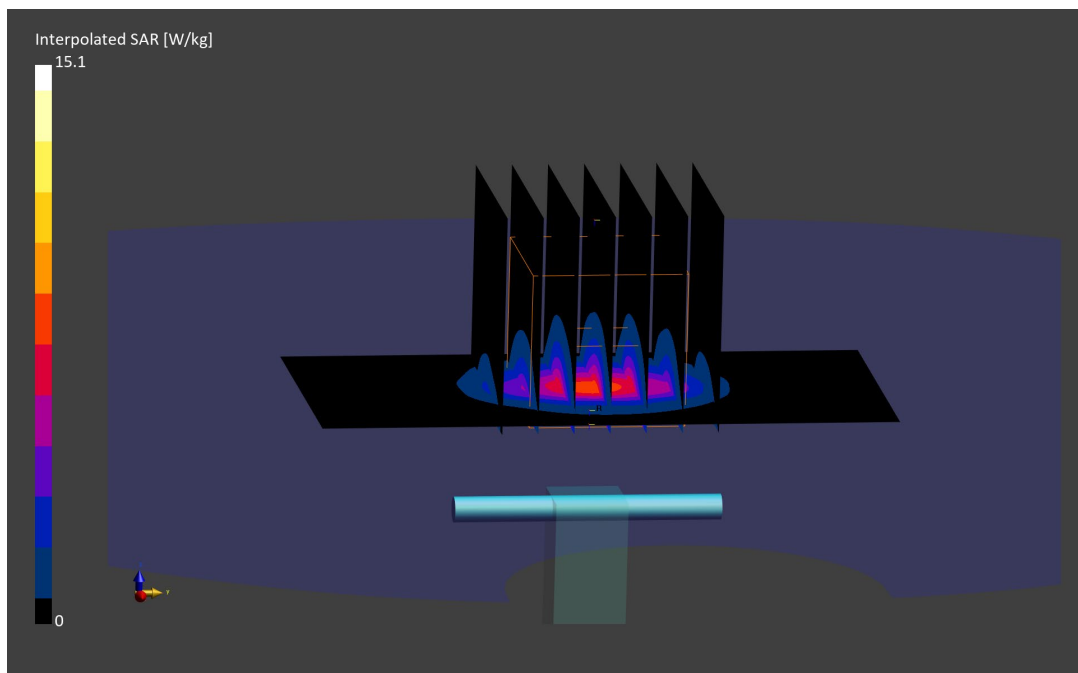

# ELEMENT

**DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1126**

Communication System: UID: 0, CW; Frequency: 3500.0 MHz  
Medium: 3600 Body; Medium parameters used:  
f = 3500.0 MHz; cond = 3.43 S/m; perm = 49.5; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/20/2023; Ambient Temp: 21.7°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN3837; ConvF:(6.19,6.19,6.19); Calibrated: 2023-01-17  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn793; Calibrated: 2023-01-17  
Phantom: Twin-SAM V8.0; Serial: 1944  
Measurement SW: DASY Module SAR V16.2.0.1425

## 3500 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (28.0 x 28.0 x 28.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 17.9 W/kg

**SAR(1 g) = 6.76 W/kg; SAR(10 g) = 2.49 W/kg**

Deviation (1 g) = 6.29%; Deviation (10 g) = 5.51%;

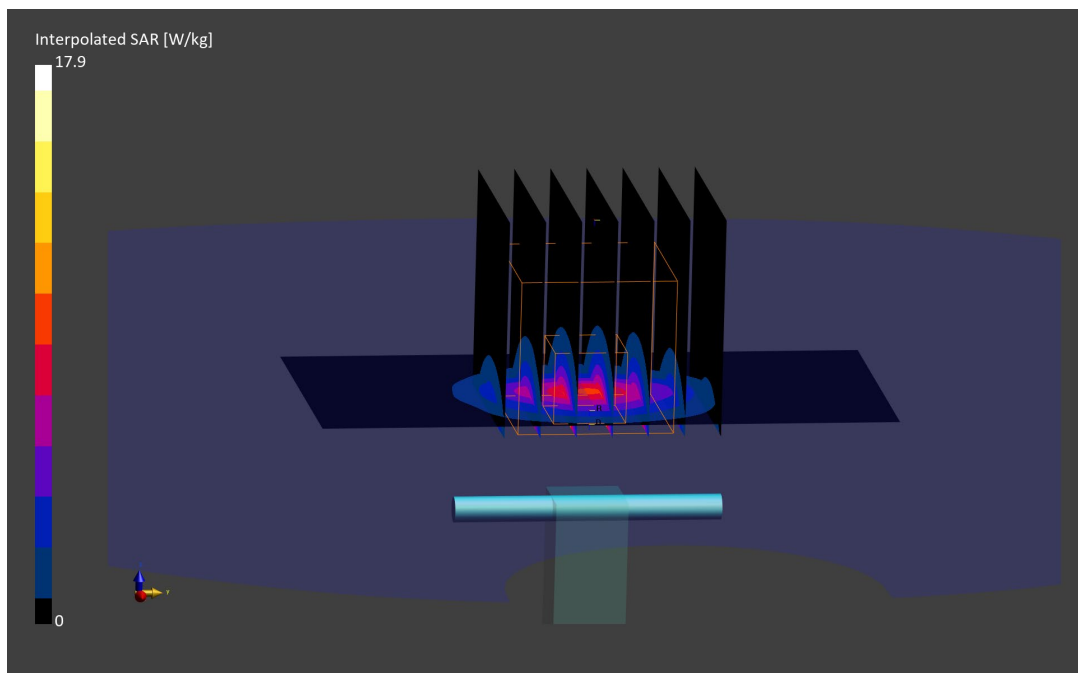

# ELEMENT

**DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1097**

Communication System: UID: 0, CW; Frequency: 3700.0 MHz  
Medium: 3600 Body; Medium parameters used:  
f = 3700.0 MHz; cond = 3.63 S/m; perm = 51.0; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/14/2023; Ambient Temp: 22.1°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN3837; ConvF:(6.04,6.04,6.04); Calibrated: 2023-01-17  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn793; Calibrated: 2023-01-17  
Phantom: Twin-SAM V8.0; Serial: 1944  
Measurement SW: DASY Module SAR V16.2.0.1425

## 3700 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (28.0 x 28.0 x 28.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 16.3 W/kg

**SAR(1 g) = 5.94 W/kg; SAR(10 g) = 2.13 W/kg**

Deviation (1 g) = -4.65%; Deviation (10 g) = -4.05%;

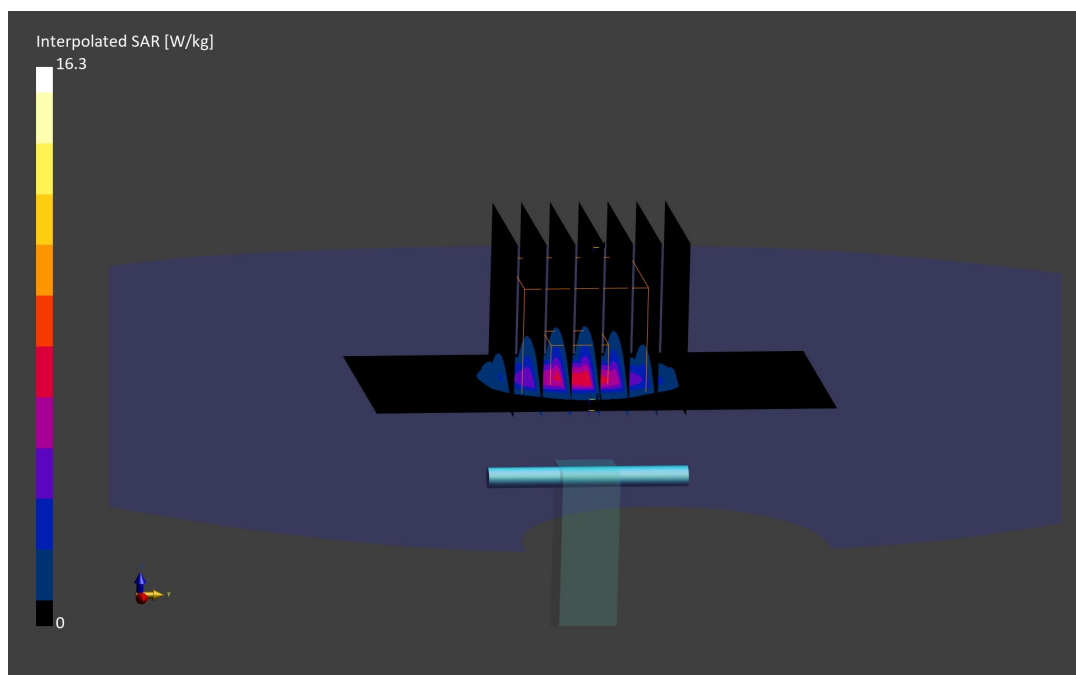

# ELEMENT

**DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1067**

Communication System: UID: 0, CW; Frequency: 3700.0 MHz  
Medium: 3600 Body; Medium parameters used:  
f = 3700.0 MHz; cond = 3.41 S/m; perm = 49.3; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/16/2023; Ambient Temp: 21.3°C; Tissue Temp: 19.7°C

Probe: EX3DV4 - SN7410; ConvF:(6.45,6.45,6.45); Calibrated: 2022-07-19  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1583; Calibrated: 2022-07-18  
Phantom: Twin-SAM V8.0; Serial: 1966  
Measurement SW: DASY Module SAR V16.2.0.1425

## 3700 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (28.0 x 28.0 x 28.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 16.8 W/kg

**SAR(1 g) = 6.31 W/kg; SAR(10 g) = 2.32 W/kg**

Deviation (1 g) = -1.71%; Deviation (10 g) = 0.87%;

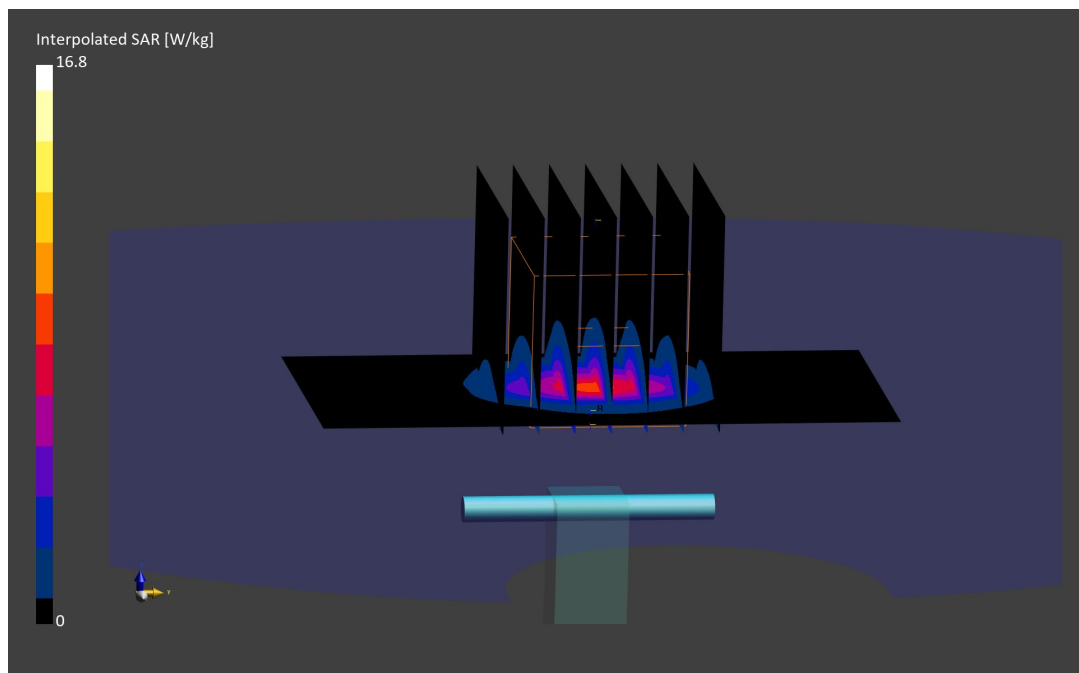

# ELEMENT

**DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1097**

Communication System: UID: 0, CW; Frequency: 3700.0 MHz  
Medium: 3600 Body; Medium parameters used:  
f = 3700.0 MHz; cond = 3.65 S/m; perm = 49.3; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/20/2023; Ambient Temp: 21.7°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN3837; ConvF:(6.04,6.04,6.04); Calibrated: 2023-01-17  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn793; Calibrated: 2023-01-17  
Phantom: Twin-SAM V8.0; Serial: 1944  
Measurement SW: DASY Module SAR V16.2.0.1425

## 3700 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (28.0 x 28.0 x 28.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 18.2 W/kg

**SAR(1 g) = 6.57 W/kg; SAR(10 g) = 2.34 W/kg**

Deviation (1 g) = 5.46%; Deviation (10 g) = 5.41%;

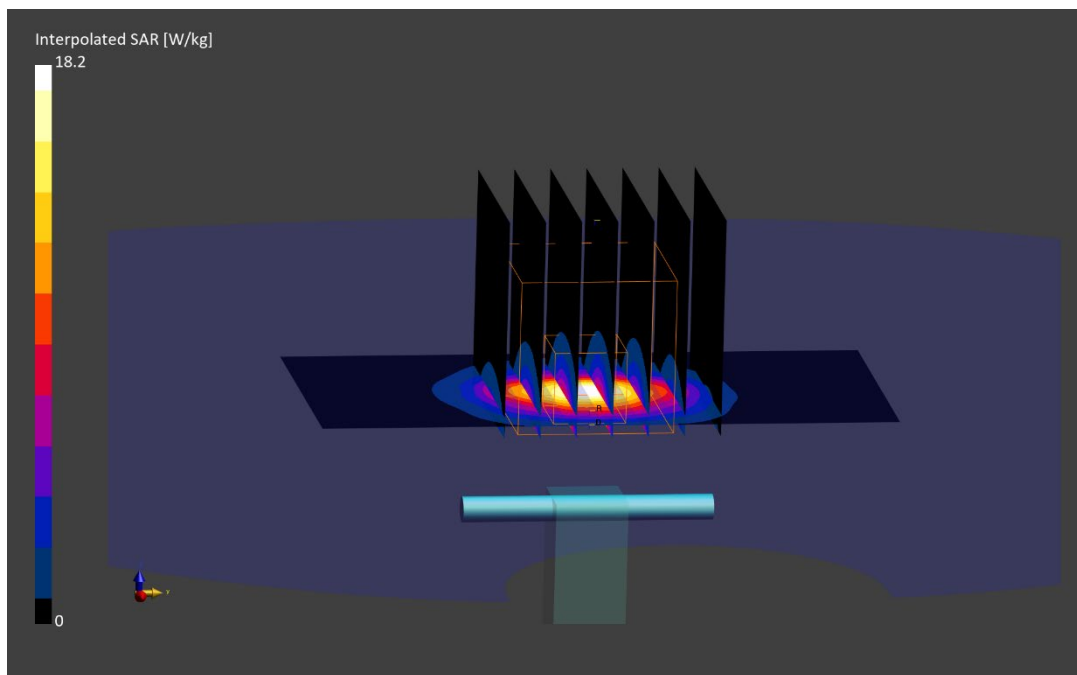

# ELEMENT

**DUT: Dipole 3900.0 MHz; Type: D3900V2 - SN1062**

Communication System: UID: 0, CW; Frequency: 3900.0 MHz  
Medium: 3600 Body; Medium parameters used:  
f = 3900.0 MHz; cond = 3.86 S/m; perm = 50.7; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/14/2023; Ambient Temp: 22.1°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN3837; ConvF:(5.98,5.98,5.98); Calibrated: 2023-01-17  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn793; Calibrated: 2023-01-17  
Phantom: Twin-SAM V8.0; Serial: 1944  
Measurement SW: DASY Module SAR V16.2.0.1425

## 3900 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (28.0 x 28.0 x 28.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 20.2 W/kg

**SAR(1 g) = 6.92 W/kg; SAR(10 g) = 2.37 W/kg**

Deviation (1 g) = 4.37%; Deviation (10 g) = 2.6%;

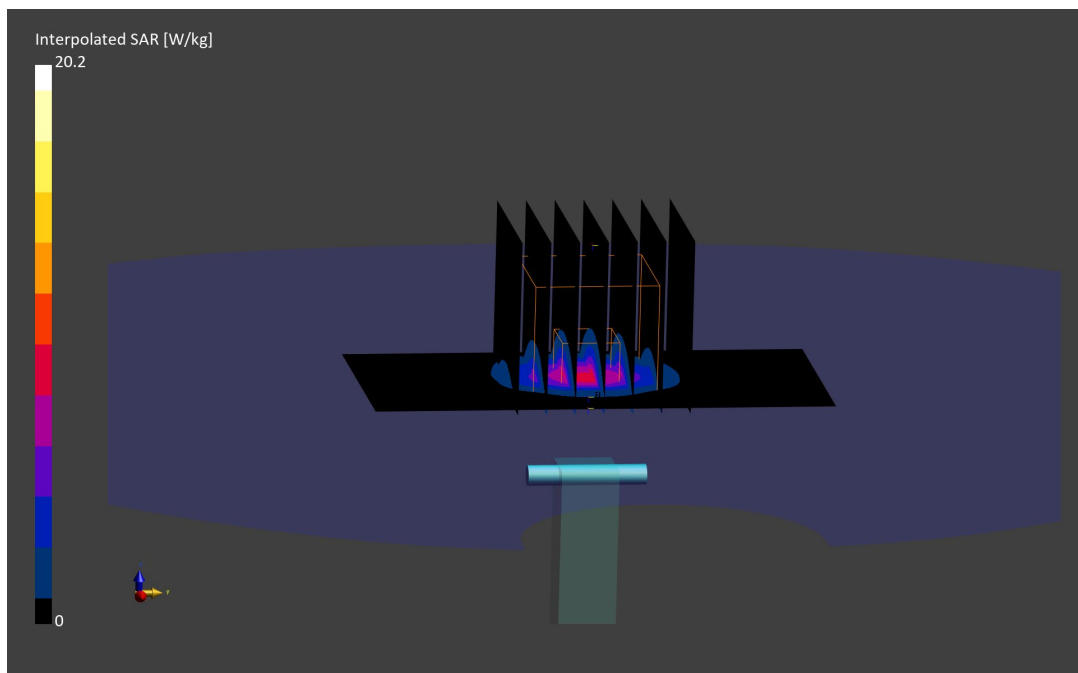



# ELEMENT

**DUT: Dipole 3900.0 MHz; Type: D3900V2 - SN1062**

Communication System: UID: 0, CW; Frequency: 3900.0 MHz  
Medium: 3600 Body; Medium parameters used:  
f = 3900.0 MHz; cond = 3.87 S/m; perm = 49.0; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/20/2023; Ambient Temp: 21.7°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN3837; ConvF:(5.98,5.98,5.98); Calibrated: 2023-01-17  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn793; Calibrated: 2023-01-17  
Phantom: Twin-SAM V8.0; Serial: 1944  
Measurement SW: DASY Module SAR V16.2.0.1425

## 3900 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (28.0 x 28.0 x 28.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 20.9 W/kg

**SAR(1 g) = 7.15 W/kg; SAR(10 g) = 2.45 W/kg**

Deviation (1 g) = 7.84%; Deviation (10 g) = 6.06%;

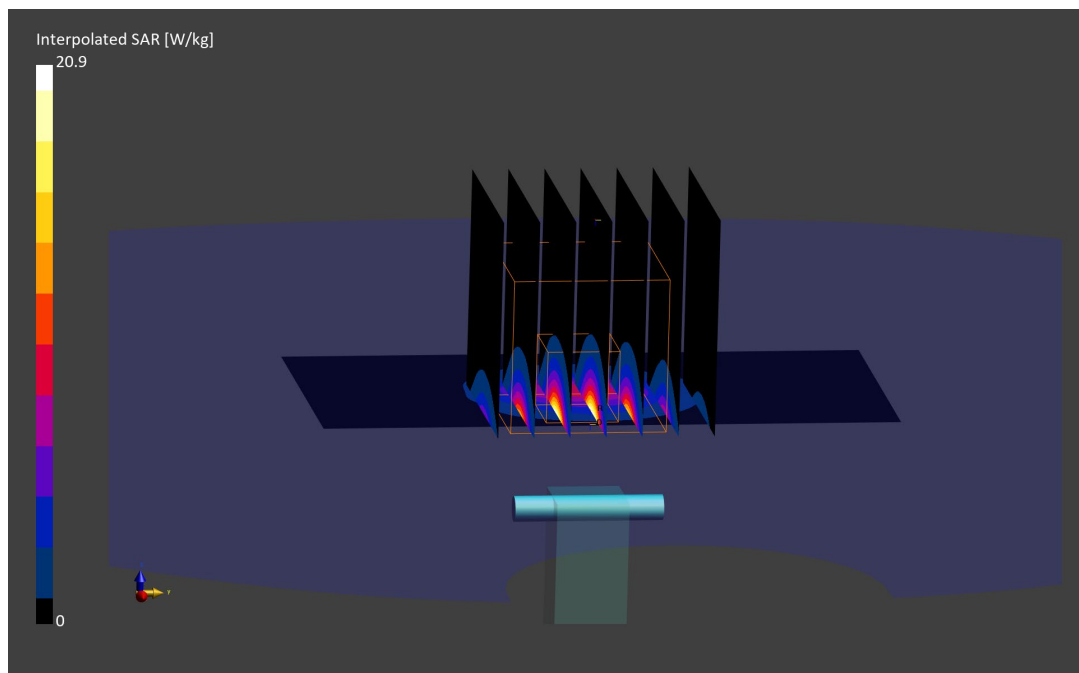

# ELEMENT

**DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1191**

Communication System: UID: 0, CW; Frequency: 5250.0 MHz  
Medium: 5200-5800 Body; Medium parameters used:  
f = 5250.0 MHz; cond = 5.19 S/m; perm = 48.6; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 02/28/2023; Ambient Temp: 22.3°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7659; ConvF:(5.21,5.21,5.21); Calibrated: 2022-04-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1407; Calibrated: 2022-04-13  
Phantom: Twin-SAM V5.0; Serial: 1873  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5250 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 12.8 W/kg

**SAR(1 g) = 3.54 W/kg; SAR(10 g) = 1.01 W/kg**

Deviation (1 g) = -5.09%; Deviation (10 g) = -2.42%;

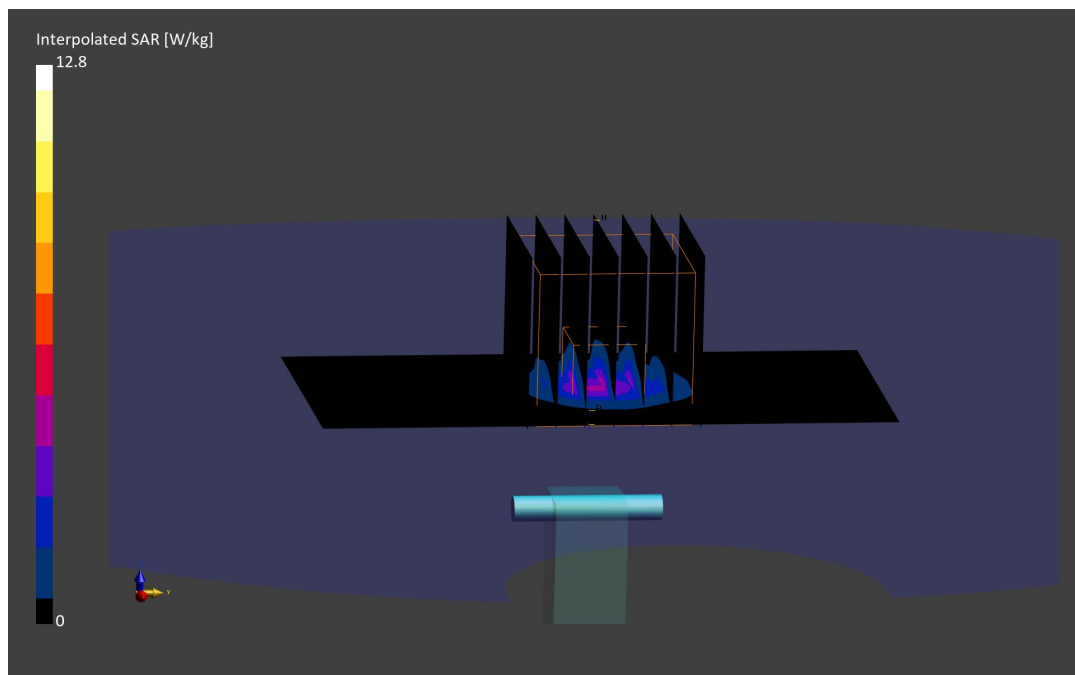

# ELEMENT

**DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1057**

Communication System: UID: 0, CW; Frequency: 5250.0 MHz  
Medium: 5200-5800 Body; Medium parameters used:  
f = 5250.0 MHz; cond = 5.17 S/m; perm = 47.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/06/2023; Ambient Temp: 23.0°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7659; ConvF:(5.21,5.21,5.21); Calibrated: 2022-04-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1407; Calibrated: 2022-04-13  
Phantom: Twin-SAM V5.0; Serial: 1873  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5250 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 12.4 W/kg

**SAR(1 g) = 3.46 W/kg; SAR(10 g) = 0.992 W/kg**

Deviation (1 g) = -6.74%; Deviation (10 g) = -3.69%;

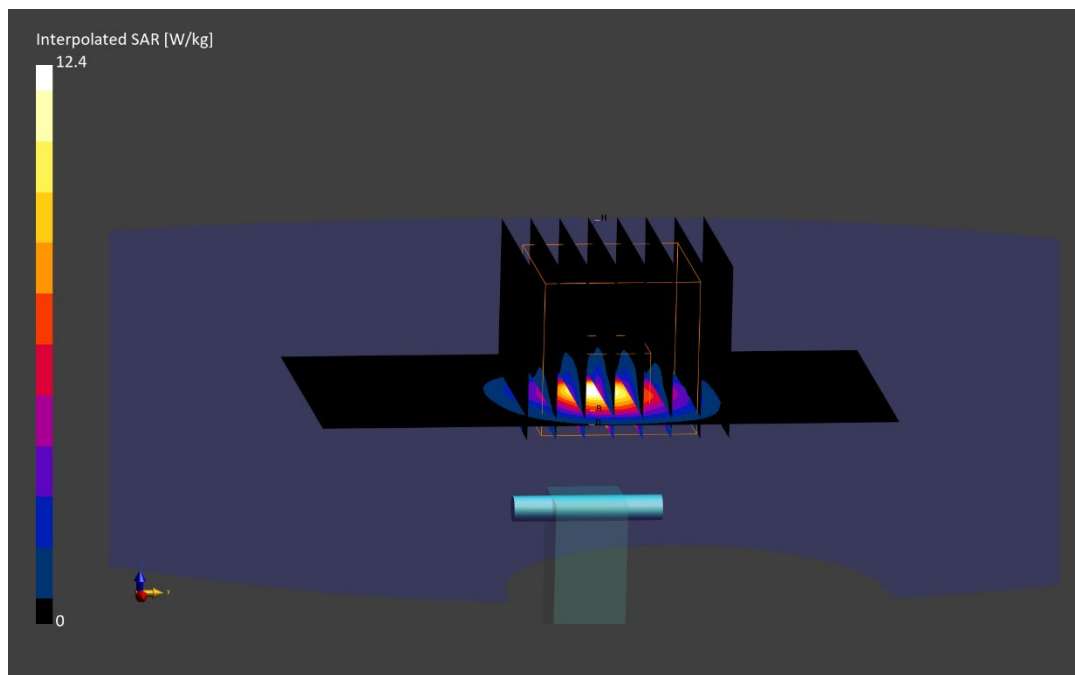

# ELEMENT

**DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1191**

Communication System: UID: 0, CW; Frequency: 5600.0 MHz  
Medium: 5200-5800 Body; Medium parameters used:  
f = 5600.0 MHz; cond = 5.69 S/m; perm = 47.9; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 02/28/2023; Ambient Temp: 22.3°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7659; ConvF:(4.6,4.6,4.6); Calibrated: 2022-04-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1407; Calibrated: 2022-04-13  
Phantom: Twin-SAM V5.0; Serial: 1873  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5600 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.9 W/kg

**SAR(1 g) = 3.76 W/kg; SAR(10 g) = 1.07 W/kg**

Deviation (1 g) = -4.33%; Deviation (10 g) = -1.83%;

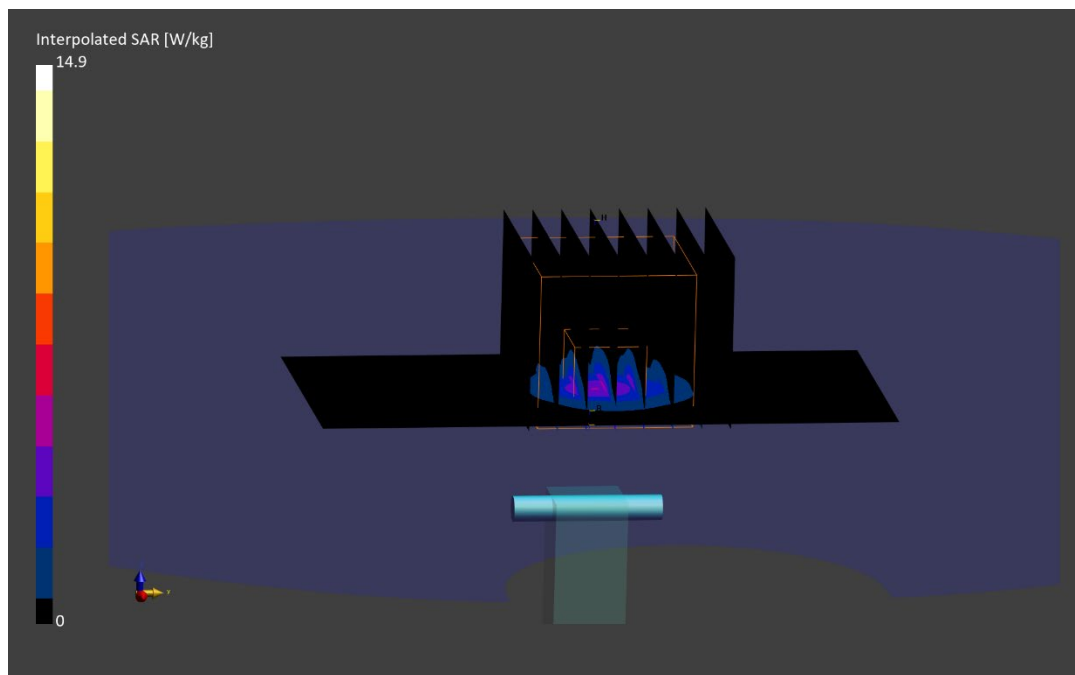

# ELEMENT

**DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1057**

Communication System: UID: 0, CW; Frequency: 5600.0 MHz  
Medium: 5200-5800 Body; Medium parameters used:  
f = 5600.0 MHz; cond = 5.66 S/m; perm = 46.8; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/06/2023; Ambient Temp: 23.0°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7659; ConvF:(4.6,4.6,4.6); Calibrated: 2022-04-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1407; Calibrated: 2022-04-13  
Phantom: Twin-SAM V5.0; Serial: 1873  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5600 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.5 W/kg

**SAR(1 g) = 3.94 W/kg; SAR(10 g) = 1.11 W/kg**

Deviation (1 g) = 2.34%; Deviation (10 g) = 4.72%;

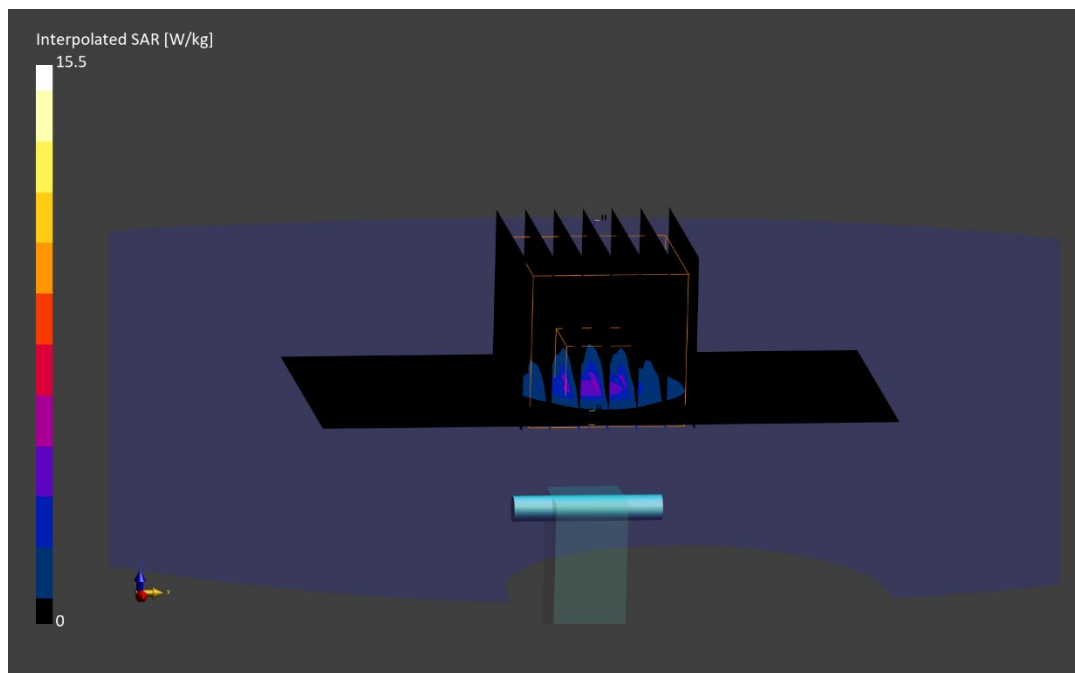

# ELEMENT

**DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1191**

Communication System: UID: 0, CW; Frequency: 5750.0 MHz  
Medium: 5200-5800 Body; Medium parameters used:  
f = 5750.0 MHz; cond = 5.91 S/m; perm = 47.7; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 02/28/2023; Ambient Temp: 22.3°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7659; ConvF:(4.67,4.67,4.67); Calibrated: 2022-04-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1407; Calibrated: 2022-04-13  
Phantom: Twin-SAM V5.0; Serial: 1873  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5750 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.0 W/kg

**SAR(1 g) = 3.50 W/kg; SAR(10 g) = 0.993 W/kg**

Deviation (1 g) = -6.54%; Deviation (10 g) = -4.06%;

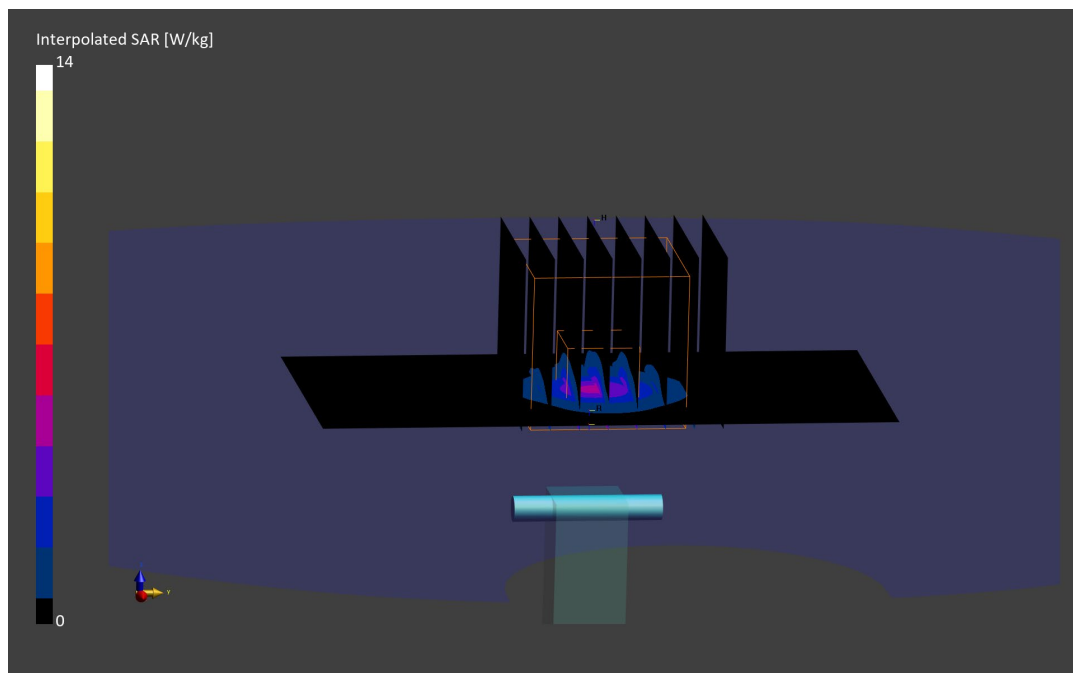

# ELEMENT

**DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1057**

Communication System: UID: 0, CW; Frequency: 5750.0 MHz  
Medium: 5200-5800 Body; Medium parameters used:  
f = 5750.0 MHz; cond = 5.89 S/m; perm = 46.5; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/06/2023; Ambient Temp: 23.0°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7659; ConvF:(4.67,4.67,4.67); Calibrated: 2022-04-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1407; Calibrated: 2022-04-13  
Phantom: Twin-SAM V5.0; Serial: 1873  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5750 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.5 W/kg

**SAR(1 g) = 3.57 W/kg; SAR(10 g) = 1.01 W/kg**

Deviation (1 g) = -4.67%; Deviation (10 g) = -2.42%;

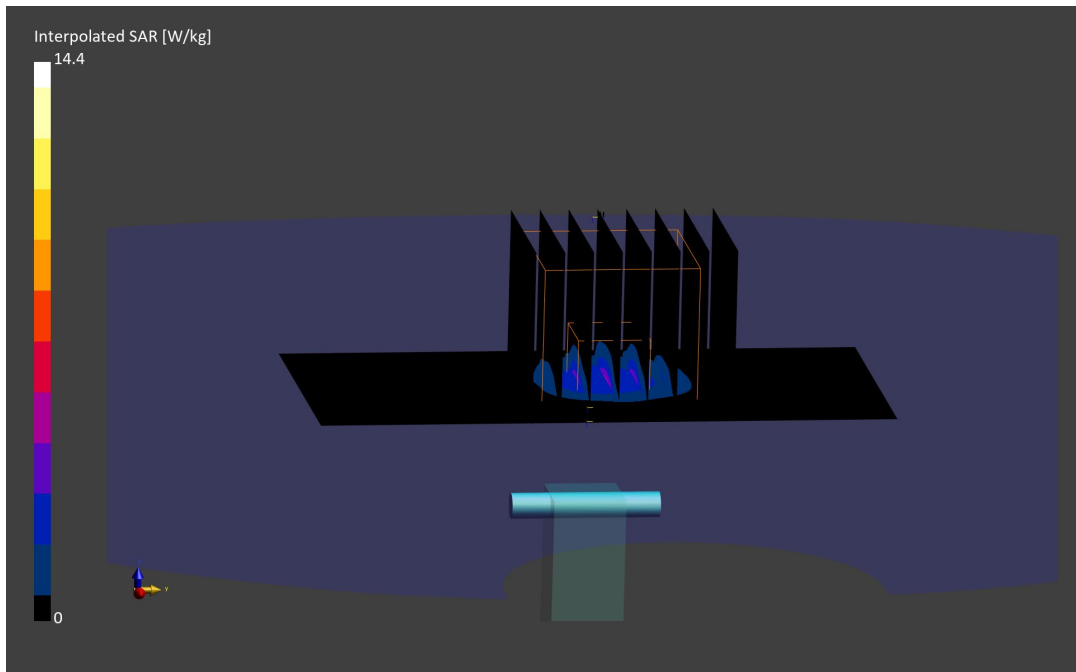

# ELEMENT

**DUT: Dipole 5800.0 MHz; Type: D5GHzV2 - SN1191**

Communication System: UID: 0, CW; Frequency: 5800.0 MHz  
Medium: 5200-5800 Body; Medium parameters used:  
f = 5800.0 MHz; cond = 5.98 S/m; perm = 47.5; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 02/28/2023; Ambient Temp: 22.3°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7659; ConvF:(4.67,4.67,4.67); Calibrated: 2022-04-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1407; Calibrated: 2022-04-13  
Phantom: Twin-SAM V5.0; Serial: 1873  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5800 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.3 W/kg

**SAR(1 g) = 3.53 W/kg; SAR(10 g) = 1.00 W/kg**

Deviation (1 g) = -2.22%; Deviation (10 g) = 0.00%;

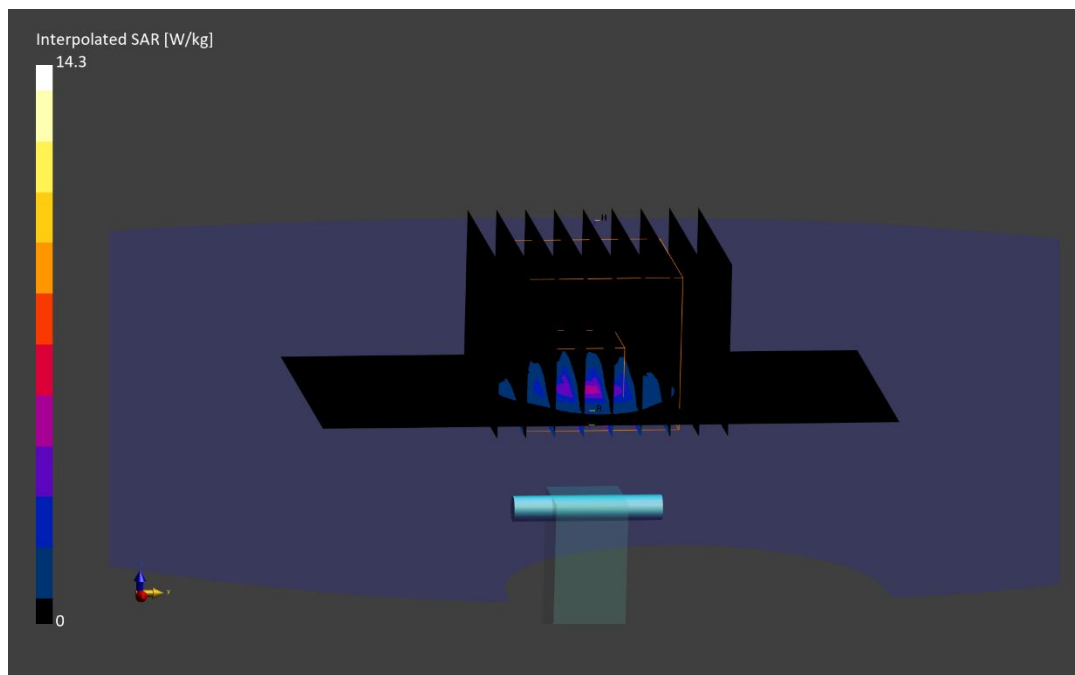



# ELEMENT

**DUT: Dipole 5800.0 MHz; Type: D5GHzV2 - SN1057**

Communication System: UID: 0, CW; Frequency: 5800.0 MHz  
Medium: 5200-5800 Body; Medium parameters used:  
f = 5800.0 MHz; cond = 5.96 S/m; perm = 46.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 03/06/2023; Ambient Temp: 23.0°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7659; ConvF:(4.67,4.67,4.67); Calibrated: 2022-04-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1407; Calibrated: 2022-04-13  
Phantom: Twin-SAM V5.0; Serial: 1873  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5800 MHz System Verification at 17 dBm (50 mW)

**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.2 W/kg

**SAR(1 g) = 3.97 W/kg; SAR(10 g) = 1.11 W/kg**

Deviation (1 g) = 6.15%; Deviation (10 g) = 8.29%;

