

# HAC RF TEST REPORT

## No. I15Z40514-SEM03

## For

Sony Mobile Communications Inc.

**GSM/WCDMA/LTE** device

With

Hardware Version: A

Software Version: 28.0.A.0.684

FCC ID: PY7-PM0796

Results Summary: M Category = M4

Issued Date: 2015-05-19



#### Note:

The test results in this test report relate only to the devices specified in this report. This report shall not be reproduced except in full without the written approval of CTTL.

#### Test Laboratory:

CTTL, Telecommunication Technology Labs, Academy of Telecommunication Research, MIIT No. 51 Shouxiang Science Building, Xueyuan Road, Haidian District, Beijing, P. R. China100191 Tel:+86(0)10-62304633-2512,Fax:+86(0)10-62304633-2504 Email:<u>cttl\_terminals@catr.cn</u>, website:<u>www.chinattl.com</u>

©Copyright. All rights reserved by CTTL.



## **REPORT HISTORY**

Report Number	Revision	Issue Date	Description
I15Z40514-SEM03	Rev.0	2015-04-30	Initial creation of test report
I15Z40514-SEM03	Rev.1	2015-05-19	Remove the type number and marketing name



## TABLE OF CONTENT

1 TEST LABORATORY	4
1.1 TESTING LOCATION	
1.2 TESTING ENVIRONMENT 1.3 PROJECT DATA	
1.4 Signature	
2 CLIENT INFORMATION	
2.1 Applicant Information 2.2 Manufacturer Information	5 5
3 EQUIPMENT UNDER TEST (EUT) AND ANCILLARY EQUIPMENT (AE)	6
3.1 About EUT	
3.2 INTERNAL IDENTIFICATION OF EUT USED DURING THE TEST	
3.4 AIR INTERFACES / BANDS INDICATING OPERATING MODES	6
4 CONDUCTED OUTPUT POWER MEASUREMENT	
4.1 SUMMARY 4.2 Conducted Power	
5. REFERENCE DOCUMENTS	7
5.1 Reference Documents for testing	7
6 OPERATIONAL CONDITIONS DURING TEST	8
6.1 HAC MEASUREMENT SET-UP	
6.2 PROBE SPECIFICATION 6.3 TEST ARCH PHANTOM & PHONE POSITIONER	9
6.4 ROBOTIC SYSTEM SPECIFICATIONS	.10
7 EUT ARRANGEMENT	.11
7.1 WD RF EMISSION MEASUREMENTS REFERENCE AND PLANE	. 11
8 SYSTEM VALIDATION	12
8.1 VALIDATION PROCEDURE	
9 EVALUATION OF MIF	13
9.1 INTRODUCTION	
9.2 MIF measurement with the AIA 9.3 Test equipment for the MIF measurement	. 14 . 14
9.4 Test signal validation 9.5 DUT MIF results	. 14
10 EVALUATION FOR LOW-POWER EXEMPTION	
10.1 PRODUCT TESTING THRESHOLD	
10.2 Conducted power	. 16
10.3 Conclusion	
11 RF TEST PROCEDUERES	
12 MEASUREMENT RESULTS (E-FIELD)	
13 ANSI C 63.19-2011 LIMITS	-
	-
15 MAIN TEST INSTRUMENTS	
ANNEX C SYSTEM VALIDATION RESULT	-
ANNEX E DIPOLE CALIBRATION CERTIFICATE	
©Copyright. All rights reserved by CT	IL.



## **1 Test Laboratory**

#### **1.1 Testing Location**

Company Name:	CTTL(Shouxiang)
Address:	No. 51 Shouxiang Science Building, Xueyuan Road, Haidian District,
	Beijing, P. R. China100191

#### **1.2 Testing Environment**


Temperature:	18°C~25 °C,		
Relative humidity:	30%~ 70%		
Ground system resistance:	< 0.5 Ω		
Ambient noise is checked and found very low and in compliance with requirement of standards.			
Reflection of surrounding objects is minimized and in compliance with requirement of standards			

#### 1.3 Project Data

Project Leader:	Qi Dianyuan
Test Engineer:	Lin Hao
Testing Start Date:	April 13, 2015
Testing End Date:	April 13, 2015

## 1.4 Signature

Lin Hao (Prepared this test report)



Qi Dianyuan (Reviewed this test report)



Deputy Director of the laboratory (Approved this test report)



## **2 Client Information**

#### **2.1 Applicant Information**

Company Name:	Sony Mobile Communications (China) Co. Ltd		
Address /Post:	Sony Mobile R&D Center, No. 16, Guangshun South Street,		
Address / Post.	Chaoyang District		
City:	Beijing		
Postal Code:	100102		
Country:	China		
Contact:	Ma, Gang		
Telephone:	+86-10-58656312		
Fax:	+86-10-58659049		

#### **2.2 Manufacturer Information**

Company Name:	Sony Mobile Communications Inc.		
Address /Post:	1-8-15 Konan, Minato-ku, Tokyo, 108-0075, Japan		
City:	Токуо		
Postal Code:	108-0075		
Country:	Japan		



## 3 Equipment Under Test (EUT) and Ancillary Equipment (AE)

#### 3.1 About EUT

Description	GSM/WCDMA/LTE device
Operating mode(s)	GSM 850/900/1800/1900, WCDMA 850/900/1700/1900/2100, BT, WiFi
	LTE Band 1/2/3/4/5/7/8/17/20/38/39/40/41

#### 3.2 Internal Identification of EUT used during the test

EUT ID*	IMEI	HW Version	SW Version
EUT1	004402148059805	А	28.0.A.0.684
EUT2	004402148058435	А	28.0.A.0.684

\*EUT ID: is used to identify the test sample in the lab internally.

Note: It is performed to test HAC with the EUT1 and conducted power with the EUT2.

#### 3.3 Internal Identification of AE used during the test

AE ID*	Description	Model	SN	Manufacturer
AE1	Battery	1288-9125	/	Sony Mobile

\*AE ID: is used to identify the test sample in the lab internally.

#### 3.4 Air Interfaces / Bands Indicating Operating Modes

Air-interface	Band(MHz)	Туре	C63.19/tested	Simultaneous Transmissions	отт	Power Reduction
GSM	850	VO	Yes			NA
93M	1900	V	res	BT, WiFi	NA	NA
GPRS/EDGE	850	DT	NA			No
GFK3/EDGE	1900	וט	NA			
	850					
WCDMA	1700	VO	Yes	BT, WiFi	NA	Yes for W1700
(UMTS)	1900				NA	
	HSPA	DT	NA			
LTE	Band	DT	NA		NA	Yes for Band
LIE	2/4/5/7/17/38	וט	NA	BT, WiFi		4/7
BT	2450	DT	NA	GSM, WCDMA, LTE	NA	NA
WLAN	2450	DT	NA	GSM, WCDMA, LTE	NA	NA

VO: Voice CMRS/PSTN Service Only

V/D: Voice CMRS/PSTN and Data Service

DT: Digital Transport

\* HAC Rating was not based on concurrent voice and data modes, Non current mode was found to represent worst case rating for both M and T rating



## 4 CONDUCTED OUTPUT POWER MEASUREMENT

#### 4.1 Summary

During the process of testing, the EUT was controlled via Agilent Digital Radio Communication tester (E5515C) to ensure the maximum power transmission and proper modulation. This result contains conducted output power for the EUT. In all cases, the measured output power should be greater and within 5% than EMI measurement.

#### 4.2 Conducted Power

GSM		Conducted Power (dBm)			
850MHz	Channel 251(848.8MHz)	Channel 190(836.6MHz)	Channel 128(824.2MHz)		
ODUIVITIZ	32.95	33.06	33.00		
GSM		Conducted Power (dBm)			
1900MHz	Channel 810(1909.8MHz)	Channel 661(1880MHz)	Channel 512(1850.2MHz)		
ISOUINILIZ	29.25	29.47	29.41		
WCDMA		Conducted Power (dBm)			
850MHz	Channel 4233(846.6MHz)	Channel 4182(836.4MHz)	Channel 4132(826.4MHz)		
820INIHZ	22.95	23.56	23.29		
	Conducted Power (dBm)				
WCDMA 1700MHz	Channel 1513(1752.6MHz)	Channel 1412(1732.4MHz)	Channel 1312(1712.4MHz)		
	22.94	22.89	23.43		
WCDMA	Conducted Power (dBm)				
	Channel 9538(1907.6MHz)	Channel 9400(1880MHz)	Channel 9262(1852.4MHz)		
1900MHz	21.57	22.64	22.42		

### **5. Reference Documents**

#### 5.1 Reference Documents for testing

The following document listed in this section is referred for testing.


Reference	Title	Version
ANSI C63.19-2011	American National Standard for Methods of Measurement	2011
	of Compatibility between Wireless Communication Devices	Edition
	and Hearing Aids	
FCC 47 CFR §20.19	Hearing Aid Compatible Mobile Headsets	/
KDB 285076 D01	Equipment Authorization Guidance for Hearing Aid	v04
	Compatibility	



## **6 OPERATIONAL CONDITIONS DURING TEST**

#### 6.1 HAC MEASUREMENT SET-UP

These measurements are performed using the DASY5 NEO automated dosimetric assessment system. It is made by Schmid & Partner Engineering AG (SPEAG) in Zurich, Switzerland. It consists of high precision robotics system (Stäubli), robot controller, Intel Core2 computer, near-field probe, probe alignment sensor. The robot is a six-axis industrial robot performing precise movements. A cell controller system contains the power supply, robot controller, teach pendant (Joystick), and remote control, is used to drive the robot motors. The PC consists of the HP Intel Core2 1.86 GHz computer with Windows XP system and HAC Measurement Software DASY5 NEO, A/D interface card, monitor, mouse, and keyboard. The Stäubli Robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE) circuit performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. is connected to the Electro-optical coupler (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the PC plug-in card.

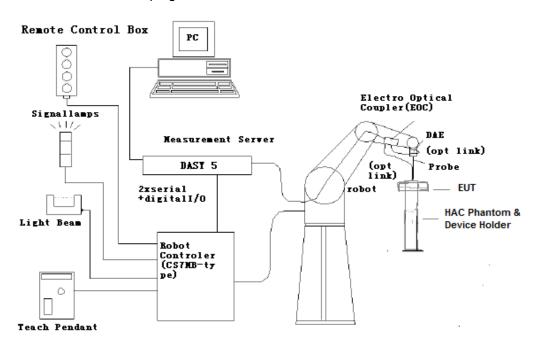



The DAE4 consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the PC-card is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe mounting device includes two different sensor systems for frontal and sidewise probe contacts. They are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built in VME-bus computer.



#### 6.2 Probe Specification

#### E-Field Probe Description

Construction	One dipole parallel, two dipoles normal to probe axis Built-in shielding against static charges PEEK enclosure material In air from 100 MHz to 3.0 GHz (absolute accuracy ±6.0%,	ALE.
	k=2)	
Frequency	40 MHz to > 6 GHz (can be extended to < 20 MHz) Linearity: ± 0.2 dB (100 MHz to 3 GHz)	[ER3DV6]
Directivity	$\pm$ 0.2 dB in air (rotation around probe axis) $\pm$ 0.4 dB in air (rotation normal to probe axis)	
Dynamic Range	2 V/m to > 1000 V/m; Linearity: $\pm$ 0.2 dB	
Dimensions	Overall length: 330 mm (Tip: 16 mm) Tip diameter: 8 mm (Body: 12 mm) Distance from probe tip to dipole centers: 2.5 mm	
Application	General near-field measurements up to 6 GHz Field component measurements Fast automatic scanning in phantoms	



## 6.3 Test Arch Phantom & Phone Positioner

The Test Arch phantom should be positioned horizontally on a stable surface. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot. It enables easy and well defined positioning of the phone and validation dipoles as well as simple teaching of the robot (Dimensions: 370 x 370 x 370 mm).

The Phone Positioner supports accurate and reliable positioning of any phone with effect on near field < $\pm$ 0.5 dB.



Fig. 2 HAC Phantom & Device Holder

### 6.4 Robotic System Specifications

#### **Specifications**

Positioner: Stäubli Unimation Corp. Robot Model: RX160L Repeatability: ±0.02 mm No. of Axis: 6 Data Acquisition Electronic (DAE) System Cell Controller Processor: Intel Core2 Clock Speed: 1.86 GHz Operating System: Windows XP Data Converter Features:Signal Amplifier, multiplexer, A/D converter, and control logic Software: DASY5 software Connecting Lines: Optical downlink for data and status info. Optical uplink for commands and clock



## 7 EUT ARRANGEMENT

#### 7.1 WD RF Emission Measurements Reference and Plane

Figure 4 illustrates the references and reference plane that shall be used in the WD emissions measurement.

- The grid is 5 cm by 5 cm area that is divided into 9 evenly sized blocks or sub-grids.
- The grid is centered on the audio frequency output transducer of the WD (speaker or T-coil).

• The grid is located by reference to a reference plane. This reference plane is the planar area that contains the highest point in the area of the WD that normally rests against the user's ear

• The measurement plane is located parallel to the reference plane and 15 mm from it, out from the phone. The grid is located in the measurement plane.

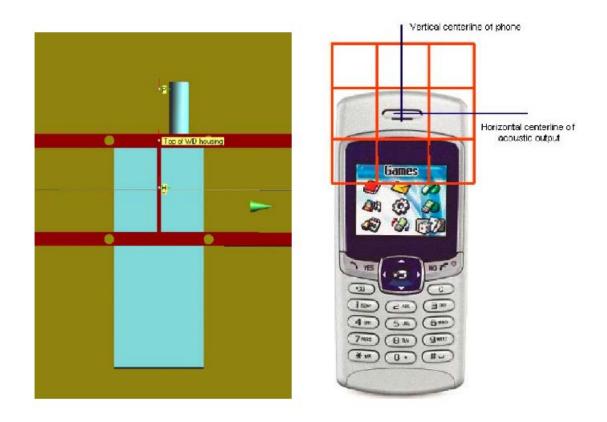


Fig. 3 WD reference and plane for RF emission measurements



## **8 SYSTEM VALIDATION**

#### 8.1 Validation Procedure

Place a dipole antenna meeting the requirements given in ANSI C63.19 in the position normally occupied by the WD. The dipole antenna serves as a known source for an electrical output. Position the E-field probes so that:

· The probes and their cables are parallel to the coaxial feed of the dipole antenna

• The probe cables and the coaxial feed of the dipole antenna approach the measurement area from opposite directions

• The center point of the probe element(s) are 15 mm from the closest surface of the dipole elements.

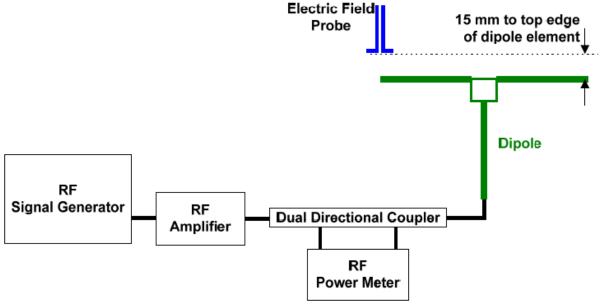


Fig. 4 Dipole Validation Setup

#### 8.2 Validation Result

E-Field Scan								
Mode	ModeFrequencyInput PowerMeasured1Target2Deviation3Limit4							
	(MHz)	(mW)	Value(dBV/m)	Value(dBV/m)	(%)	(%)		
CW	835	100	40.56	40.70	-1.60	±25		
CW	1880	100	39.31	39.04	3.16	±25		

Notes:

1. Please refer to the attachment for detailed measurement data and plot.

2. Target value is provided by SPEAD in the calibration certificate of specific dipoles.

3. Deviation (%) = 100 \* (Measured value minus Target value) divided by Target value.

4. ANSI C63.19 requires values within  $\pm$  25% are acceptable, of which 12% is deviation and 13% is measurement uncertainty. Values independently validated for the dipole actually used in the measurements should be used, when available.



## 9 Evaluation of MIF

#### 9.1 Introduction

The MIF (Modulation Interference Factor) is used to classify E-field emission to determine Hearing Aid Compatibility (HAC). It scales the power-averaged signal to the RF audio interference level and is characteristic to a modulation scheme. The HAC standard preferred "indirect" measurement method is based on average field measurement with separate scaling by the MIF. With an Audio Interference Analyzer (AIA) designed by SPEAG specifically for the MIF measurement, these values have been verified by practical measurements on an RF signal modulated with each of the waveforms. The resulting deviations from the simulated values are within the requirements of the HAC standard.

The AIA (Audio Interference Analyzer) is an USB powered electronic sensor to evaluate signals in the frequency range 698 MHz - 6 GHz. It contains RMS detector and audio frequency circuits for sampling of the RF envelope.



Fig. 5 AIA Front View



#### 9.2 MIF measurement with the AIA

The MIF is measured with the AIA as follows:

- 1. Connect the AIA via USB to the DASY5 PC and verify the configuration settings.
- 2. Couple the RF signal to be evaluated to an AIA via cable or antenna.
- 3. Generate a MIF measurement job for the unknown signal and select the measurement port and timing settings.
- 4. Document the results via the post processor in a report.

#### 9.3 Test equipment for the MIF measurement

No.	Name	Туре	Serial Number	Manufacturer
01	Signal Generator	E4438C	MY49071430	Agilent
02	AIA	SE UMS 170 CB	1029	SPEAG
03	BTS	E5515C	MY50263375	Agilent

#### 9.4 Test signal validation

The signal generator (E4438C) is used to generate a 1GHz signal with different modulation in the below table based on the ANSI C63.19-2011. The measured MIF with AIA are compared with the target values given in ANSI C63.19-2011 table D.3, D.4 and D5.

Pulse modulation	Target MIF	Measured MIF	Deviation
0.5ms pulse, 1000Hz repetition rate	-0.9 dB	-0.9 dB	0 dB
1ms pulse, 100Hz repetition rate	+3.9 dB	+3.7 dB	0.2 dB
0.1ms pulse, 100Hz repetition rate	+10.1 dB	+10.0 dB	0.1 dB
10ms pulse, 10Hz repetition rate	+1.6 dB	+1.7 dB	0.1 dB
Sine-wave modulation	Target MIF	Measured MIF	Deviation
1 kHz, 80% AM	-1.2 dB	-1.3 dB	0.1 dB
1 kHz, 10% AM	-9.1 dB	-9.0 dB	0.1 dB
1 kHz, 1% AM	-19.1 dB	-18.9 dB	0.2 dB
100 Hz, 10% AM	-16.1 dB	-16.0 dB	0.1 dB
10 kHz, 10% AM	-21.5 dB	-21.6 dB	0.1 dB
Transmission protocol	Target MIF	Measured MIF	Deviation
GSM; full-rate version 2; speech codec/handset low	+3.5 dB	+3.47 dB	0.03 dB
WCDMA; speech; speech codec low; AMR 12.2 kb/s	-20.0 dB	-19.8 dB	0.2 dB
CDMA; speech; SO3; RC3; full frame rate; 8kEVRC	-19.0 dB	-19.1 dB	0.1 dB
CDMA; speech; SO3; RC1; 1/8 <sup>th</sup> frame rate; 8kEVRC	+3.3 dB	+3.44 dB	0.14 dB



#### 9.5 DUT MIF results

Typical MIF levels in ANSI C63.19-2011					
Transmission protocol	Modulation interference factor				
GSM; full-rate version 2; speech codec/handset low	+3.5 dB				
WCDMA; speech; speech codec low; AMR 12.2 kb/s	-20.0 dB				

	Measured MIF lev	els
Band	Channel	Modulation interference factor
	251	+3.40 dB
GSM 850	190	+3.44 dB
	128	+3.42 dB
	810	+3.37 dB
GSM 1900	661	+3.38 dB
	512	+3.38 dB
	4233	-19.78 dB
WCDMA 850	4182	-19.75 dB
	4132	-19.74 dB
	1513	-19.69 dB
WCDMA 1700	1412	-19.70 dB
	1312	-19.72 dB
	9538	-19.73 dB
WCDMA 1900	9400	-19.68 dB
	9262	-19.69 dB



## 10 Evaluation for low-power exemption

#### **10.1 Product testing threshold**

There are two methods for exempting an RF air interface technology from testing. The first method requires evaluation of the MIF for the worst-case operating mode. An RF air interface technology of a device is exempt from testing when its average antenna input power plus its MIF is  $\leq$ 17 dBm for any of its operating modes. The second method does not require determination of the MIF. The RF emissions testing exemption shall be applied to an RF air interface technology in a device whose peak antenna input power, averaged over intervals  $\leq$ 50 µ s20, is  $\leq$ 23 dBm. An RF air interface technology that is exempted from testing by either method shall be rated as M4. The first method is used to be exempt from testing for the RF air interface technology in this report.

Band	Average power (dBm)	MIF (dB)	Sum (dBm)
GSM 850	33.06	3.44	36.50
GSM 1900	29.47	3.38	32.85
WCDMA 850	23.56	-19.74	3.82
WCDMA 1700	23.43	-19.69	3.74
WCDMA 1900	22.64	-19.68	2.96

#### **10.2 Conducted power**

#### 10.3 Conclusion

According to the above table, the sums of average power and MIF for UMTS are less than 17dBm. So it is only measured for GSM bands. The UMTS bands are exempt from testing and rated as M4.



## **11 RF TEST PROCEDUERES**

#### The evaluation was performed with the following procedure:

- 1) Confirm proper operation of the field probe, probe measurement system and other instrumentation and the positioning system.
- 2) Position the WD in its intended test position. The gauge block can simplify this positioning.
- 3) Configure the WD normal operation for maximum rated RF output power, at the desired channel and other operating parameters (e.g., test mode), as intended for the test.
- 4) The center sub-grid shall centered on the center of the T-Coil mode axial measurement point or the acoustic output, as appropriate. Locate the field probe at the initial test position in the 50 mm by 50 mm grid, which is contained in the measurement plane. If the field alignment method is used, align the probe for maximum field reception.
- 5) Record the reading.
- 6) Scan the entire 50 mm by 50 mm region in equally spaced increments and record the reading at each measurement point. The distance between measurement points shall be sufficient to assure the identification of the maximum reading.
- 7) Identify the five contiguous sub-grids around the center sub-grid whose maximum reading is the lowest of all available choices. This eliminates the three sub-grids with the maximum readings. Thus, the six areas to be used to determine the WD's highest emissions are identified.
- 8) Identify the maximum field reading within the non-excluded sub-grids identified in Step 7)
- 9) Evaluate the MIF and add to the maximum steady-state rms field-strength reading to obtain the RF audio interference level..
- 10) Compare this RF audio interference level with the categories and record the resulting WD category rating.



## 12 Measurement Results (E-Field)

Freq	luency	Measured Value	Power Drift	Category					
MHz	Channel	(dBV/m)	(dB)						
	GSM 850								
848.8	251	36.63	-0.00	M4 (see Fig B.1)					
836.6	190	37.03	-0.13	M4 (see Fig B.2)					
824.2	128	36.86	-0.05	M4 (see Fig B.3)					
		GSM 19	00						
1909.8	810	27.88	-0.10	<b>M4</b> (see Fig B.4)					
1880	661	27.16	-0.06	M4 (see Fig B.5)					
1850.2	512	26.24	0.01	M4 (see Fig B.6)					

## 13 ANSI C 63.19-2011 LIMITS

#### WD RF audio interference level categories in logarithmic units


Emission categories	< 960 MHz				
	E-field emissions				
Category M1	50 to 55 dB (V/m)				
Category M2	45 to 50	dB (V/m)			
Category M3	40 to 45	dB (V/m)			
Category M4	< 40	dB (V/m)			
Emission categories	> 96	0 MHz			
	E-field e	missions			
Category M1	40 to 45	dB (V/m)			
Category M2	35 to 40	dB (V/m)			
Category M3	30 to 35 dB (V/m)				
Category M4	< 30	dB (V/m)			



## **14 MEASUREMENT UNCERTAINTY**

No.	Error source	Туре	Uncertainty Value (%)	Prob. Dist.	k	Ci E	Standard Uncertainty (%) $u_i^{(*)}$ E	Degree of freedom V <sub>eff</sub> or <i>v</i> i
Meas	urement System							
1	Probe Calibration	В	5.	Ν	1	1	5.1	∞
2	Axial Isotropy	В	4.7	R	$\sqrt{3}$	1	2.7	œ
3	Sensor Displacement	В	16.5	R	$\sqrt{3}$	1	9.5	∞
4	Boundary Effects	В	2.4	R	$\sqrt{3}$	1	1.4	×
5	Linearity	В	4.7	R	$\sqrt{3}$	1	2.7	∞
6	Scaling to Peak Envelope Power	В	2.0	R	$\sqrt{3}$	1	1.2	ø
7	System Detection Limit	В	1.0	R	$\sqrt{3}$	1	0.6	8
8	Readout Electronics	В	0.3	N	1	1	0.3	∞
9	Response Time	В	0.8	R	$\sqrt{3}$	1	0.5	8
10	Integration Time	В	2.6	R	$\sqrt{3}$	1	1.5	∞
11	RF Ambient Conditions	В	3.0	R	$\sqrt{3}$	1	1.7	∞
12	RF Reflections	В	12.0	R	$\sqrt{3}$	1	6.9	∞
13	Probe Positioner	В	1.2	R	$\sqrt{3}$	1	0.7	∞
14	Probe Positioning	A	4.7	R	$\sqrt{3}$	1	2.7	∞
15	Extra. And Interpolation	В	1.0	R	$\sqrt{3}$	1	0.6	∞
Test	Sample Related							
16	Device Positioning Vertical	В	4.7	R	$\sqrt{3}$	1	2.7	œ
17	Device Positioning Lateral	В	1.0	R	$\sqrt{3}$	1	0.6	œ
18	Device Holder and Phantom	В	2.4	R	$\sqrt{3}$	1	1.4	œ
19	Power Drift	В	5.0	R	$\sqrt{3}$	1	2.9	∞

©Copyright. All rights reserved by CTTL.





20	AIA measurement	В	12	R	$\sqrt{3}$	1	6.9	∞
Pha	Phantom and Setup related							
21	Phantom Thickness	В	2.4	R	$\sqrt{3}$	1	1.4	∞
Comb	Combined standard uncertainty(%) 16.2							
Expanded uncertainty (confidence interval of 95 %)		ı	$u_e = 2u_c$	Ν	k=:	2	32.4	

## **15 MAIN TEST INSTRUMENTS**

#### Table 1: List of Main Instruments

No.	Name	Туре	Serial Number	Calibration Date	Valid Period
01	Signal Generator	E4438C	MY49071430	February 02, 2015	One Year
02	Power meter	NRVD	102196	March 03, 2015	One year
03	Power sensor	NRV-Z5	100596	March 05, 2015	One year
04	Amplifier	60S1G4	0331848	No Calibration Re	quested
05	E-Field Probe	ER3DV6	2428	January 23, 2015	One year
06	HAC Dipole	CD835V3	1023	September 17, 2014	One year
07	HAC Dipole	CD1880V3	1018	September 17, 2014	One year
08	BTS	E5515C	MY50263375	January 30, 2015	One year
09	DAE	SPEAG DAE4	771	January 27, 2015	One year
10	AIA	SE UMS 170 CB	1029	No Calibration Requested	


## **16 CONCLUSION**

The HAC measurement indicates that the EUT complies with the HAC limits of the ANSI C63.19-2011. The total M-rating is **M4.** 

\*\*\*END OF REPORT BODY\*\*\*



## ANNEX A TEST LAYOUT

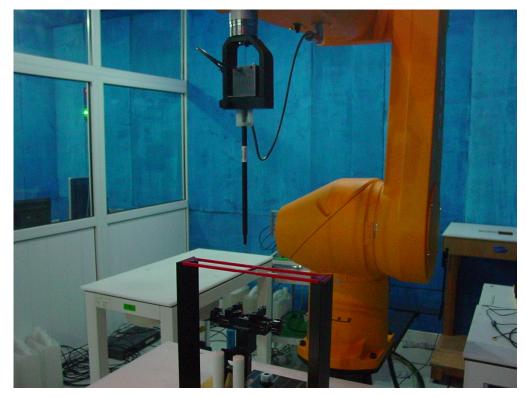

Picture A1: HAC RF System Layout




## ANNEX B TEST PLOTS

### HAC RF E-Field GSM 850 High

Date: 2015-4-13 Electronics: DAE4 Sn771 Medium: Air Medium parameters used:  $\sigma = 0$  mho/m,  $\epsilon_r = 1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature:22.5°C Communication System: GSM 850; Frequency: 848.8 MHz; Duty Cycle: 1:8.3 Probe: ER3DV6 - SN2428;ConvF(1, 1, 1) **E Scan - ER3DV6 - 2011: 15 mm from Probe Center to the Device/Hearing Aid Compatibility Test (101x101x1):** Interpolated grid: dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm Reference Value = 55.95 V/m; Power Drift = -0.00 dB Applied MIF = 3.40 dB RF audio interference level = 36.63 dBV/m **Emission category: M4** 

MIF scaled E-field

Grid 1 <b>M4</b>	Grid 2 <b>M4</b>	Grid 3 <b>M4</b>
35.45 dBV/m	35.78 dBV/m	34.95 dBV/m
Grid 4 <b>M4</b>	Grid 5 M4	Grid 6 <b>M4</b>
36.46 dBV/m	36.63 dBV/m	35.6 dBV/m
Grid 7 M4	Grid 8 <b>M4</b>	Grid 9 <b>M4</b>
37.3 dBV/m	37.42 dBV/m	35.85 dBV/m

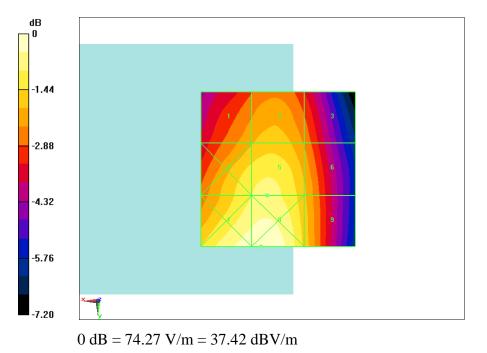

#### Fig B.1 HAC RF E-Field GSM 850 High




## HAC RF E-Field GSM 850 Middle

Date: 2015-4-13 Electronics: DAE4 Sn771 Medium: Air Medium parameters used:  $\sigma = 0$  mho/m,  $\varepsilon_r = 1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature:22.5°C Communication System: GSM 850; Frequency: 836.6 MHz; Duty Cycle: 1:8.3 Probe: ER3DV6 - SN2428;ConvF(1, 1, 1)

E Scan - ER3DV6 - 2011: 15 mm from Probe Center to the Device 2/Hearing Aid Compatibility Test (101x101x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm Reference Value = 59.60 V/m; Power Drift = -0.13 dB Applied MIF = 3.44 dB RF audio interference level = 37.03 dBV/m Emission category: M4

Grid 1 <b>M4</b>	Grid 2 <b>M4</b>	Grid 3 <b>M4</b>
36.01 dBV/m	36.34 dBV/m	35.47 dBV/m
Grid 4 M4	Grid 5 M4	Grid 6 <b>M4</b>
36.78 dBV/m	37.03 dBV/m	35.99 dBV/m
Grid 7 M4	Grid 8 M4	Grid 9 <b>M4</b>
37.51 dBV/m	37.6 dBV/m	36.17 dBV/m

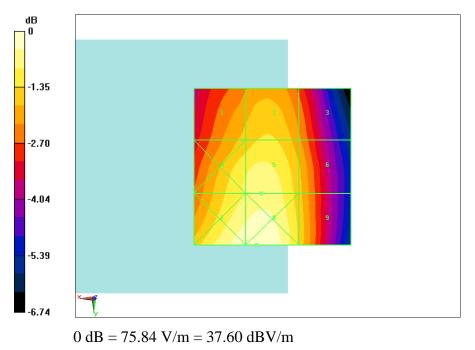






## HAC RF E-Field GSM 850 Low

Date: 2015-4-13 Electronics: DAE4 Sn771 Medium: Air Medium parameters used:  $\sigma = 0$  mho/m,  $\epsilon_r = 1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature:22.5°C Communication System: GSM 850; Frequency: 824.2 MHz; Duty Cycle: 1:8.3 Probe: ER3DV6 - SN2428;ConvF(1, 1, 1)

E Scan - ER3DV6 - 2011: 15 mm from Probe Center to the Device 3/Hearing Aid Compatibility Test (101x101x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm Reference Value = 57.74 V/m; Power Drift = -0.05 dB Applied MIF = 3.42 dB RF audio interference level = 36.86 dBV/m Emission category: M4

Grid 1 <b>M4</b>	Grid 2 <b>M4</b>	Grid 3 <b>M4</b>
35.91 dBV/m	36.13 dBV/m	35.18 dBV/m
Grid 4 <b>M4</b>	Grid 5 M4	Grid 6 <b>M4</b>
36.67 dBV/m	36.86 dBV/m	35.65 dBV/m
Grid 7 M4	Grid 8 M4	Grid 9 <b>M4</b>
37.37 dBV/m	37.49 dBV/m	35.82 dBV/m

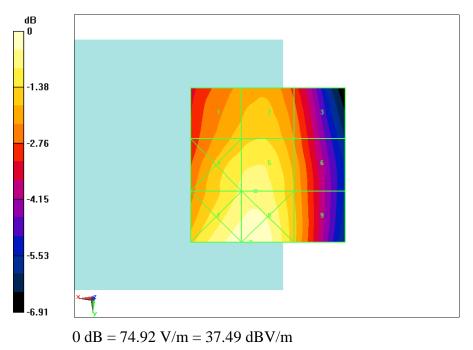






## HAC RF E-Field GSM 1900 High

Date: 2015-4-13 Electronics: DAE4 Sn771 Medium: Air Medium parameters used:  $\sigma = 0$  mho/m,  $\varepsilon_r = 1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature:22.5°C Communication System: DCS 1900; Frequency: 1909.8 MHz; Duty Cycle: 1:8.3 Probe: ER3DV6 - SN2428;ConvF(1, 1, 1)

E Scan - ER3DV6 - 2011: 15 mm from Probe Center to the Device/Hearing Aid Compatibility Test (101x101x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm Reference Value = 20.94 V/m; Power Drift = -0.10 dB Applied MIF = 3.37 dB RF audio interference level = 27.88 dBV/m Emission category: M4

Grid 1 <b>M4</b>	Grid 2 M4	Grid 3 <b>M4</b>
29.01 dBV/m	29.02 dBV/m	27.36 dBV/m
Grid 4 <b>M4</b>	Grid 5 M4	Grid 6 <b>M4</b>
27.42 dBV/m	27.88 dBV/m	27.71 dBV/m
Grid 7 <b>M4</b>	Grid 8 <b>M4</b>	Grid 9 <b>M4</b>
26.12 dBV/m	27.79 dBV/m	27.67 dBV/m

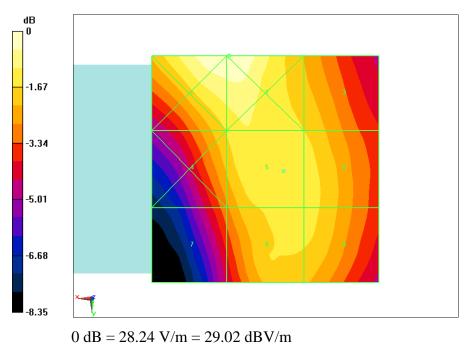






## HAC RF E-Field GSM 1900 Middle

Date: 2015-4-13 Electronics: DAE4 Sn771 Medium: Air Medium parameters used:  $\sigma = 0$  mho/m,  $\varepsilon_r = 1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature:22.5°C Communication System: DCS 1900; Frequency: 1880 MHz; Duty Cycle: 1:8.3 Probe: ER3DV6 - SN2428;ConvF(1, 1, 1)

E Scan - ER3DV6 - 2011: 15 mm from Probe Center to the Device 2/Hearing Aid Compatibility Test (101x101x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm Reference Value = 18.38 V/m; Power Drift = -0.06 dB Applied MIF = 3.38 dB RF audio interference level = 27.16 dBV/m Emission category: M4

MIF scaled E-field

Grid 1 M4	Grid 2 M4	Grid 3 M4
28.44 dBV/m	28.41 dBV/m	26.55 dBV/m
Grid 4 <b>M4</b>	Grid 5 M4	Grid 6 <b>M4</b>
26.45 dBV/m	27.16 dBV/m	27.02 dBV/m
Grid 7 <b>M4</b>	Grid 8 <b>M4</b>	Grid 9 <b>M4</b>
25.15 dBV/m	27.08 dBV/m	27.01 dBV/m

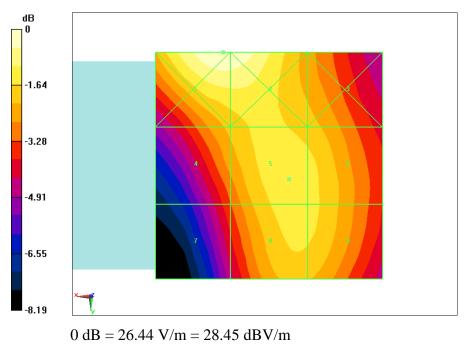

#### Fig B.5 HAC RF E-Field GSM 1900 Middle





## HAC RF E-Field GSM 1900 Low

Date: 2015-4-13 Electronics: DAE4 Sn771 Medium: Air Medium parameters used:  $\sigma = 0$  mho/m,  $\varepsilon_r = 1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature:22.5°C Communication System: DCS 1900; Frequency: 1850.2 MHz; Duty Cycle: 1:8.3 Probe: ER3DV6 - SN2428;ConvF(1, 1, 1)

E Scan - ER3DV6 - 2011: 15 mm from Probe Center to the Device 3/Hearing Aid Compatibility Test (101x101x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm Reference Value = 16.67 V/m; Power Drift = 0.01 dB Applied MIF = 3.38 dB RF audio interference level = 26.24 dBV/m Emission category: M4

Grid 1 M4	Grid 2 M4	Grid 3 M4
27.32 dBV/m	27.2 dBV/m	25.65 dBV/m
Grid 4 <b>M4</b>	Grid 5 M4	Grid 6 <b>M4</b>
25.28 dBV/m	26.24 dBV/m	26.08 dBV/m
Grid 7 <b>M4</b>	Grid 8 <b>M4</b>	Grid 9 <b>M4</b>
24.06 dBV/m	26.15 dBV/m	26.05 dBV/m

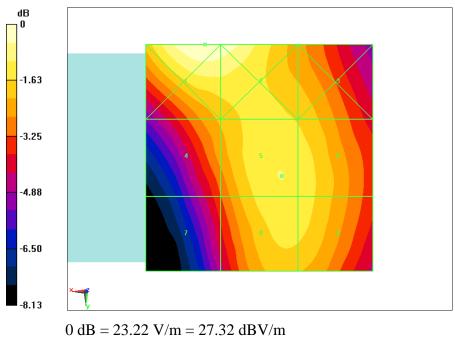






## ANNEX C SYSTEM VALIDATION RESULT

E SCAN of Dipole 835 MHz

**Date: 2015-4-13** Electronics: DAE4 Sn771 Medium: Air Medium parameters used:  $\sigma = 0$  mho/m,  $\epsilon r = 1$ ;  $\rho = 1000$  kg/m3 Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1 Probe: ER3DV6 - SN2428;ConvF(1, 1, 1) **E Scan - measurement distance from the probe sensor center to CD835 Dipole = 15mm/Hearing Aid Compatibility Test (41x361x1):** Interpolated grid: dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm Reference Value = 118.5 V/m; Power Drift = 0.07 dB Applied MIF = 0.00 dB RF audio interference level = 40.56 dBV/m **Emission category: M3** 

MIF scaled E-field

Grid 1 <b>M3</b>	Grid 2 <b>M3</b>	Grid 3 <b>M3</b>
40.37 dBV/m	40.56 dBV/m	40.45 dBV/m
Grid 4 <b>M4</b>	Grid 5 M4	Grid 6 <b>M4</b>
35.58 dBV/m	35.89 dBV/m	35.86 dBV/m
Grid 7 <b>M3</b>	Grid 8 <b>M3</b>	Grid 9 <b>M3</b>
40.01 dBV/m	40.28 dBV/m	40.22 dBV/m

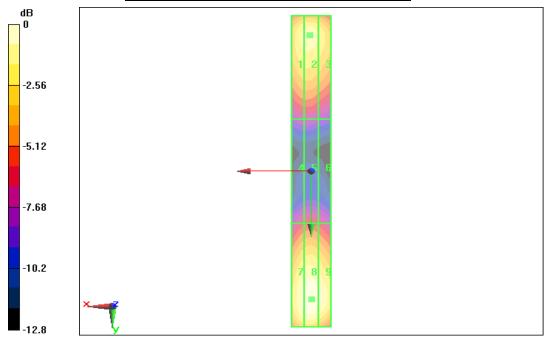


0 dB = 40.56 dBV/m



#### E SCAN of Dipole 1880 MHz Date: 2015-4-13

Electronics: DAE4 Sn771 Medium: Air Medium parameters used:  $\sigma = 0$  mho/m,  $\varepsilon_r = 1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1 Probe: ER3DV6 - SN2428;ConvF(1, 1, 1) **E Scan - measurement distance from the probe sensor center to CD1880 Dipole = 15mm/Hearing Aid Compatibility Test (41x181x1):** Interpolated grid: dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm Reference Value = 142.9 V/m; Power Drift = -0.02 dB Applied MIF = 0.00 dB RF audio interference level = 39.31 dBV/m **Emission category: M2** MIE scaled E-field

	in Source E nore				
Grid 1 <b>M2</b>	Grid 2 <b>M2</b>	Grid 3 <b>M2</b>			
39.08 dBV/m	39.31 dBV/m	39.18 dBV/m			
Grid 4 <b>M2</b>	Grid 5 <b>M2</b>	Grid 6 <b>M2</b>			
36.73 dBV/m	36.92 dBV/m	36.87 dBV/m			
Grid 7 <b>M2</b>	Grid 8 <b>M2</b>	Grid 9 <b>M2</b>			
39.10 dBV/m	39.24 dB V/m	39.14 dBV/m			

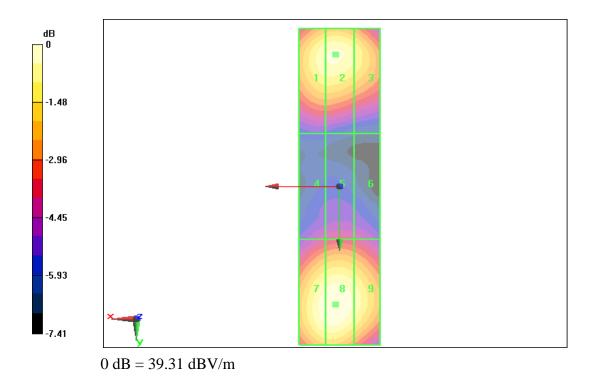



## ANNEX D PROBE CALIBRATION CERTIFICATE

#### E\_Probe ER3DV6

eughausstrasse 43, 8004 Zur	ich, Switzerland	S Statement	Servizio svizzero di taratura Swiss Calibration Service
ccredited by the Swiss Accredit he Swiss Accreditation Servi		2.00 B	reditation No.: SCS 0108
lultilateral Agreement for the			
lient CTTL (Auden)	)	Certificate No:	ER3-2428 Jan15
CALIBRATION	CERTIFICATE		
Object	ER3DV6 - SN:24	28	
Calibration procedure(s)	QA CAL-02.v8, C	)A CAL-25 v6	
	Calibration proce	dure for E-field probes optimized f	or close near field
	evaluations in air		
Calibration date:	January 23, 2015		
		onal standards, which realize the physical units obability are given on the following pages and	
The measurements and the unc All calibrations have been condu	certainties with confidence pr ucted in the closed laborator	and the second	are part of the certificate.
The measurements and the unc All calibrations have been condu Calibration Equipment used (M&	certainties with confidence pr ucted in the closed laborator \$TE critical for calibration)	obability are given on the following pages and y facility: environment temperature (22 ± 3)°C a	are part of the certificate. and humidity < 70%.
The measurements and the unc All calibrations have been condu- Calibration Equipment used (M& Primary Standards	certainties with confidence pr ucted in the closed laborator	obability are given on the following pages and y facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.)	are part of the certificate. and humidity < 70%.
The measurements and the unc All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E4419B	ertainties with confidence pr ucted in the closed laborator &TE critical for calibration)	obability are given on the following pages and         y facility: environment temperature (22 ± 3)°C a         Cal Date (Certificate No.)         03-Apr-14 (No. 217-01911)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15
The measurements and the unc All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A	ertainties with confidence pr ucted in the closed laborator &TE critical for calibration) ID GB41293874	Cal Date (Certificate No.) 03-Apr-14 (No. 217-01911) 03-Apr-14 (No. 217-01911)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15
The measurements and the unc All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator	ertainties with confidence pr ucted in the closed laborator &TE critical for calibration) ID GB41293874 MY41498087	obability are given on the following pages and         y facility: environment temperature (22 ± 3)°C a         Cal Date (Certificate No.)         03-Apr-14 (No. 217-01911)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15
The measurements and the unc All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	ertainties with confidence pr ucted in the closed laborator &TE critical for calibration) ID GB41293874 MY41498087 SN: S5054 (3c)	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15
The measurements and the unc All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator	ertainties with confidence pr ucted in the closed laborator &TE critical for calibration) ID GB41293874 MY41498087 SN: \$5054 (3c) SN: \$5277 (20x)	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01919)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15
The measurements and the unc All calibrations have been condu- Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4419A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator Reference Probe ER3DV6	ertainties with confidence pr ucted in the closed laborator &TE critical for calibration) ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5277 (20x) SN: S5129 (30b)	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01915)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15
The measurements and the unc All calibrations have been condu- Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 70 dB Attenuator Reference Probe ER3DV6 DAE4	ertainties with confidence pr ucted in the closed laborator &TE critical for calibration) ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5277 (20x) SN: S5129 (30b) SN: 2328	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01920)           08-Oct-14 (No. ER3-2328_Oct14)           30-Apr-14 (No. DAE4-789_Apr14)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Oct-15 Oct-15 Apr-15
The measurements and the unc All calibrations have been condu- Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ER3DV6 DAE4 Secondary Standards	Artainties with confidence pr ucted in the closed laborator ATE critical for calibration) ID GB41293874 MY41498087 SN: 55054 (3c) SN: 55054 (3c) SN: 55277 (20x) SN: 55129 (30b) SN: 55129 (30b) SN: 789	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01920)           08-Oct-14 (No. ER3-2328_Oct14)           30-Apr-14 (No. DAE4-789_Apr14)           Check Date (in house)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Oct-15 Oct-15 Apr-15 Scheduled Check
The measurements and the unc All calibrations have been condu- Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ER3DV6 DAE4 Secondary Standards RF generator HP 8648C	ertainties with confidence pr ucted in the closed laborator &TE critical for calibration) ID GB41293874 MY41498087 SN: 55054 (3c) SN: 55054 (3c) SN: 55277 (20x) SN: 55129 (30b) SN: 55128 SN: 789 ID	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01920)           08-Oct-14 (No. ER3-2328_Oct14)           30-Apr-14 (No. DAE4-789_Apr14)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Oct-15 Oct-15 Apr-15
The measurements and the unc All calibrations have been condu- Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference Probe ER3DV6 DAE4	ertainties with confidence pr ucted in the closed laborator &TE critical for calibration) ID GB41293874 MY41498087 SN: \$5054 (3c) SN: \$5054 (3c) SN: \$55277 (20x) SN: \$5129 (30b) SN: 3228 SN: 789 ID US3642U01700 US3642U01700 US37390585	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01920)           08-Oct-14 (No. DAE4-789_Apr14)           Check Date (in house)           4-Aug-99 (in house check Apr-13)           18-Oct-01 (in house check Oct-14)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Oct-15 Oct-15 Apr-15 Scheduled Check In house check: Apr-16 In house check: Oct-15
The measurements and the unc All calibrations have been condu- Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4419A Reference 3 dB Attenuator Reference 9 robe ER3DV6 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	Artainties with confidence pr ucted in the closed laborator BTE critical for calibration) ID GB41293874 MY41498087 SN: \$5054 (3c) SN: \$5129 (30b) SN: \$5129 (30b) SN: \$2328 SN: 789 ID US3642U01700 US37390585 Name	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01920)           08-Oct-14 (No. ER3-2328_Oct14)           30-Apr-14 (No. DAE4-789_Apr14)           Check Date (in house)           4-Aug-99 (in house check Apr-13)           18-Oct-01 (in house check Oct-14)           Function	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Oct-15 Apr-15 Oct-15 Apr-15 Scheduled Check In house check: Apr-16
The measurements and the unc All calibrations have been condu- Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4419A Reference 3 dB Attenuator Reference 9 robe ER3DV6 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	ertainties with confidence pr ucted in the closed laborator &TE critical for calibration) ID GB41293874 MY41498087 SN: \$5054 (3c) SN: \$5054 (3c) SN: \$55277 (20x) SN: \$5129 (30b) SN: 3228 SN: 789 ID US3642U01700 US3642U01700 US37390585	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01920)           08-Oct-14 (No. DAE4-789_Apr14)           Check Date (in house)           4-Aug-99 (in house check Apr-13)           18-Oct-01 (in house check Oct-14)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Oct-15 Oct-15 Apr-15 Scheduled Check In house check: Apr-16 In house check: Oct-15
The measurements and the unc All calibrations have been condu- Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ER3DV6 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E Calibrated by:	Artainties with confidence pr ucted in the closed laborator ATE critical for calibration) ID GB41293874 MY41498087 SN: 55054 (3c) SN: 55277 (20x) SN: 55129 (30b) SN: 2328 SN: 789 ID US3642U01700 US37390585 Name Leif Klysner	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01920)           08-Oct-14 (No. ER3-2328_Oct14)           30-Apr-14 (No. DAE4-789_Apr14)           Check Date (in house)           4-Aug-99 (in house check Apr-13)           18-Oct-01 (in house check Oct-14)           Function           Laboratory Technician	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Oct-15 Oct-15 Apr-15 Scheduled Check In house check: Apr-16 In house check: Oct-15
The measurements and the unc All calibrations have been condu- Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ER3DV6 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E Calibrated by:	Artainties with confidence pr ucted in the closed laborator BTE critical for calibration) ID GB41293874 MY41498087 SN: \$5054 (3c) SN: \$5129 (30b) SN: \$5129 (30b) SN: \$2328 SN: 789 ID US3642U01700 US37390585 Name	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01920)           08-Oct-14 (No. ER3-2328_Oct14)           30-Apr-14 (No. DAE4-789_Apr14)           Check Date (in house)           4-Aug-99 (in house check Apr-13)           18-Oct-01 (in house check Oct-14)           Function	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Oct-15 Oct-15 Apr-15 Scheduled Check In house check: Apr-16 In house check: Oct-15
The measurements and the unc All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ER3DV6 DAE4 Secondary Standards RF generator HP 8648C	Artainties with confidence pr ucted in the closed laborator ATE critical for calibration) ID GB41293874 MY41498087 SN: 55054 (3c) SN: 55277 (20x) SN: 55129 (30b) SN: 2328 SN: 789 ID US3642U01700 US37390585 Name Leif Klysner	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01920)           08-Oct-14 (No. ER3-2328_Oct14)           30-Apr-14 (No. DAE4-789_Apr14)           Check Date (in house)           4-Aug-99 (in house check Apr-13)           18-Oct-01 (in house check Oct-14)           Function           Laboratory Technician	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Oct-15 Oct-15 Apr-15 Scheduled Check In house check: Apr-16 In house check: Oct-15

Certificate No: ER3-2428\_Jan15

Page 1 of 10



#### No. 115Z40514-SEM03 Page 31 of 56

#### Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

S

C

S

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary

Glossaly.	
NORMx,y,z	sensitivity in free space
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization $\phi$	φ rotation around probe axis
Polarization 9	9 rotation around an axis that is in the plane normal to probe axis (at measurement center),
Connector Angle	i.e., 9 = 0 is normal to probe axis information used in DASY system to align probe sensor X to the robot coordinate system
	and the second of the second o

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1309-2005, " IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", December 2005
- b) CTIA Test Plan for Hearing Aid Compatibility, April 2010.

#### Methods Applied and Interpretation of Parameters:

- NORMx, y,z: Assessed for E-field polarization 9 = 0 for XY sensors and 9 = 90 for Z sensor (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). .
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW . signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal ٠ characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- Spherical isotropy (3D deviation from isotropy): in a locally homogeneous field realized using an open waveguide setup.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: ER3-2428\_Jan15

Page 2 of 10



No. I15Z40514-SEM03 Page 32 of 56

ER3DV6 - SN:2428

January 23, 2015

# Probe ER3DV6

# SN:2428

Calibrated:

Manufactured: September 11, 2007 January 23, 2015

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: ER3-2428\_Jan15

Page 3 of 10



ER3DV6 - SN:2428

January 23, 2015

#### DASY/EASY - Parameters of Probe: ER3DV6 - SN:2428

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)$	1.51	1.58	1.83	± 10.1 %
DCP (mV) <sup>B</sup>	101.6	99.5	102.3	

## Modulation Calibration Parameters

UID	Communication System Name		A dB	B dBõV	С	dB	VR mV	Unc <sup>c</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	189.0	±3.8 %
		Y	0.0	0.0	1.0		207.2	
		Z	0.0	0.0	1.0		199.4	
10011- CAB	UMTS-FDD (WCDMA)	X	3.18	66.7	18.9	2.91	112.3	±0.7 %
		Y	3.14	66.0	18.2		123.4	
		Z	3.14	66.4	18.4		116.3	
10021- DAB	GSM-FDD (TDMA, GMSK)	x	16.25	97.6	28.0	9.39	106.6	±1.7 %
		Y	9.84	90.3	25.6		112.7	
		Z	18.91	97.3	27.6		121.7	
10039- CAB	CDMA2000 (1xRTT, RC1)	X	4.67	66.4	19.2	4.57	113.6	±0.9 %
		Y	4.71	66.5	19.1		125.0	
		Z	4.49	66.0	18.8		115.6	
10081- CAB	CDMA2000 (1xRTT, RC3)	×	3.75	65.2	18.3	3.97	110.4	±0.7 %
		Y	3.78	65.2	18.2		122.0	
		Z	3.69	65.3	18.3		113.2	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>8</sup> Numerical linearization parameter: uncertainty not required.
<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: ER3-2428\_Jan15


Page 4 of 10



ER3DV6 - SN:2428

January 23, 2015

#### Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

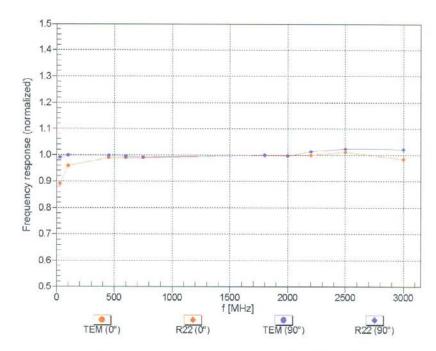

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Certificate No: ER3-2428\_Jan15

Page 5 of 10




ER3DV6 - SN:2428

January 23, 2015

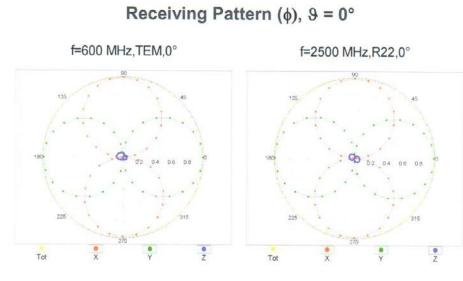


Receiving Pattern ( $\phi$ ),  $\vartheta$  = 90°

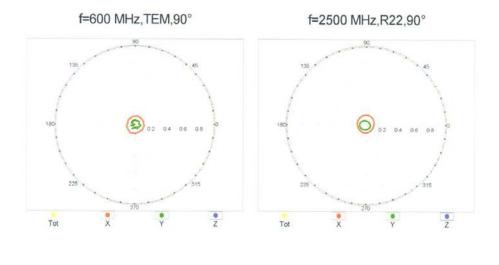

Certificate No: ER3-2428\_Jan15

Page 6 of 10



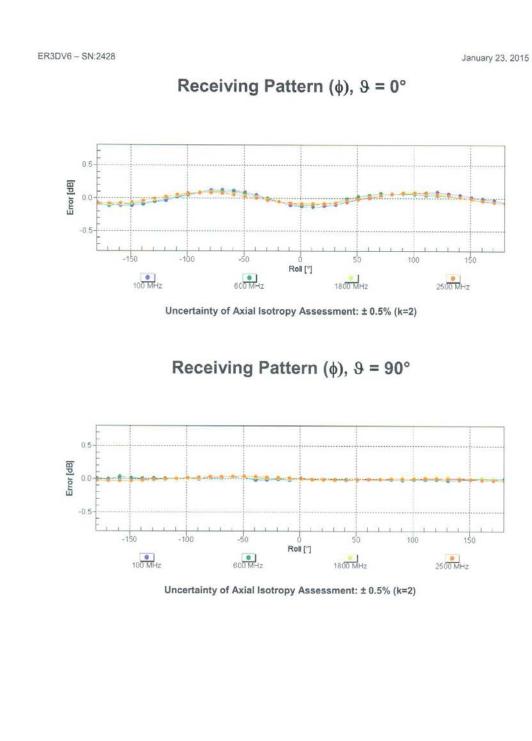


Page 7 of 10



ER3DV6 - SN:2428

January 23, 2015

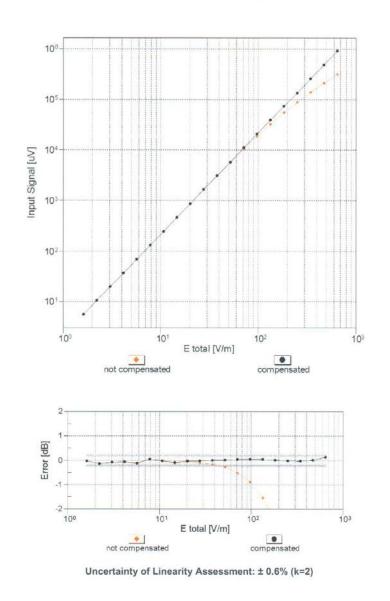

Dynamic Range f(E-field) (TEM cell , f = 900 MHz)

Certificate No: ER3-2428\_Jan15


Page 8 of 10



# No. I15Z40514-SEM03 Page 38 of 56

ER3DV6 - SN:2428

January 23, 2015

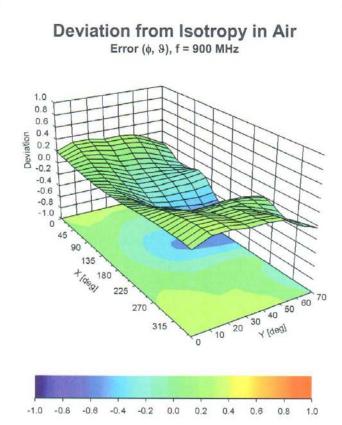

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ER3-2428\_Jan15

Page 9 of 10



ER3DV6 - SN:2428

January 23, 2015

# DASY/EASY - Parameters of Probe: ER3DV6 - SN:2428

## **Other Probe Parameters**

Sensor Arrangement	Rectangular
Connector Angle (°)	-39.1
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	8 mm
Probe Tip to Sensor X Calibration Point	2.5 mm
Probe Tip to Sensor Y Calibration Point	2.5 mm
Probe Tip to Sensor Z Calibration Point	2.5 mm

Certificate No: ER3-2428\_Jan15

Page 10 of 10



# ANNEX E DIPOLE CALIBRATION CERTIFICATE

## Dipole 835 MHz

**Calibration Laboratory of** SWISS Schweizerischer Kalibrierdienst S Schmid & Partner Service suisse d'étalonnage C CRUBRATIO **Engineering AG** Servizio svizzero di taratura S Zeughausstrasse 43, 8004 Zurich, Switzerland Swiss Calibration Service Accredited by the Swiss Accreditation Service (SAS) Accreditation No.: SCS 108 The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Client CTTL (Auden) Certificate No: CD835V3-1023\_Sep14 **CALIBRATION CERTIFICATE** CD835V3 - SN: 1023 Object QA CAL-20.v6 Calibration procedure(s) Calibration procedure for dipoles in air September 17, 2014 Calibration date: This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID # Cal Date (Certificate No.) Scheduled Calibration GB37480704 Power meter EPM-442A 09-Oct-13 (No. 217-01827) Oct-14 Power sensor HP 8481A US37292783 09-Oct-13 (No. 217-01827) Oct-14 Power sensor HP 8481A MY41092317 09-Oct-13 (No. 217-01828) Oct-14 Type-N mismatch combination SN: 5047.2 / 06327 03-Apr-14 (No. 217-01921) Apr-15 Probe ER3DV6 SN: 2336 30-Dec-13 (No. ER3-2336\_Dec13) Dec-14 Probe H3DV6 SN: 6065 30-Dec-13 (No. H3-6065\_Dec13) Dec-14 DAE4 SN: 781 12-Sep-14 (No. DAE4-781\_Sep14) Sep-15 Secondary Standards ID # Check Date (in house) Scheduled Check Power meter Agilent 4419B SN: GB40202831 29-Oct-13 (in house check Oct-13) In house check: Oct-15 Power sensor HP E4412A SN: MY41498700 11-Oct-13 (in house check Oct-13) In house check: Oct-15 Power sensor HP E4412A SN: MY41502623 11-Oct-13 (in house check Oct-13) In house check: Oct-15 Network Analyzer HP 8753E US37390585 18-Oct-01 (in house check Oct-13) In house check: Oct-14 RF generator R&S SMT-06 SN: 832283/011 27-Aug-12 (in house check Oct-13) In house check: Oct-16 Name Function Signature Calibrated by: Leif Klysner Laboratory Technician Lei Approved by: Fin Bomholt Deputy Technical Manager Issued: September 22, 2014 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: CD835V3-1023\_Sep14

Page 1 of 8



# No. I15Z40514-SEM03 Page 41 of 56

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S

C

S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### References

- [1] ANSI-C63.19-2007
  - American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids. ANSI-C63.19-2011
- [2]
  - American National Standard, Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.

#### Methods Applied and Interpretation of Parameters:

- Coordinate System: y-axis is in the direction of the dipole arms. z-axis is from the basis of the antenna (mounted on the table) towards its feed point between the two dipole arms. x-axis is normal to the other axes. In coincidence with the standards [1], the measurement planes (probe sensor center) are selected to be at a distance of 10 mm (15 mm for [2]) above the top metal edge of the dipole arms.
- Measurement Conditions: Further details are available from the hardcopies at the end of the certificate. All
  figures stated in the certificate are valid at the frequency indicated. The forward power to the dipole connector
  is set with a calibrated power meter connected and monitored with an auxiliary power meter connected to a
  directional coupler. While the dipole under test is connected, the forward power is adjusted to the same level.
- Antenna Positioning: The dipole is mounted on a HAC Test Arch phantom using the matching dipole positioner with the arms horizontal and the feeding cable coming from the floor. The measurements are performed in a shielded room with absorbers around the setup to reduce the reflections. It is verified before the mounting of the dipole under the Test Arch phantom, that its arms are perfectly in a line. It is installed on the HAC dipole positioner with its arms parallel below the dielectric reference wire and able to move elastically in vertical direction without changing its relative position to the top center of the Test Arch phantom. The vertical distance to the probe is adjusted after dipole mounting with a DASY5 Surface Check job. Before the measurement, the distance between phantom surface and probe tip is verified. The proper measurement distance is selected by choosing the matching section of the HAC Test Arch phantom with the proper device reference point (upper surface of the dipole) and the matching grid reference point (tip of the probe) considering the probe sensor offset. The vertical distance to the probe is essential for the accuracy.
- Feed Point Impedance and Return Loss: These parameters are measured using a HP 8753E Vector Network Analyzer. The impedance is specified at the SMA connector of the dipole. The influence of reflections was eliminating by applying the averaging function while moving the dipole in the air, at least 70cm away from any obstacles.
- *E-field distribution:* E field is measured in the x-y-plane with an isotropic ER3D-field probe with 100 mW forward power to the antenna feed point. In accordance with [1] and [2], the scan area is 20mm wide, its length exceeds the dipole arm length (180 or 90mm). The sensor center is 10 mm (15 mm for [2]) (in z) above the metal top of the dipole arms. Two 3D maxima are available near the end of the dipole arms. Assuming the dipole arms are perfectly in one line, the average of these two maxima (in subgrid 2 and subgrid 8) is determined to compensate for any non-parallelity to the measurement plane as well as the sensor displacement. The E-field value stated as calibration value represents the maximum of the interpolated 3D-E-field, in the plane above the dipole surface.
- H-field distribution: H-field is measured with an isotropic H-field probe with 100mW forward power to the
  antenna feed point, in the x-y-plane. The scan area and sensor distance is equivalent to the E-field scan. The
  maximum of the field is available at the center (subgrid 5) above the feed point. The H-field value stated as
  calibration value represents the maximum of the interpolated H-field, 10mm above the dipole surface at the
  feed point.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: CD835V3-1023\_Sep14

Page 2 of 8



## Measurement Conditions


DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Phantom	HAC Test Arch	
Distance Dipole Top - Probe Center	10 mm	
Scan resolution	dx, dy = 5 mm	
Frequency	835 MHz ± 1 MHz	
Input power drift	< 0.05 dB	

## Maximum Field values at 835 MHz

H-field 10 mm above dipole surface	condition	interpolated maximum
Maximum measured	100 mW input power	0.459 A/m ± 8.2 % (k=2)
E-field 10 mm above dipole surface	condition	Interpolated maximum
Maximum measured above high end	100 mW input power	170.0 V/m = 44.61 dBV/m
Maximum measured above low end	100 mW input power	158.3 V/m = 43.99 dBV/m
Averaged maximum above arm	100 mW input power	164.2 V/m ± 12.8 % (k=2)
E-field 15 mm above dipole surface	condition	Interpolated maximum
Maximum measured above high end	100 mW input power	108.3 V/m = 40.69 dBV/m
Maximum measured above low end	100 mW input power	104.9 V/m = 40.41 dBV/m
Averaged maximum above arm	100 mW input power	106.6 V/m ± 12.8 % (k=2)

Page 3 of 8





## Appendix (Additional assessments outside the scope of SCS108)

#### Antenna Parameters

Frequency	Return Loss	Impedance
800 MHz	16.7 dB	48.6 Ω - 14.4 jΩ
835 MHz	24.0 dB	45.5 Ω + 4.0 jΩ
900 MHz	16.5 dB	51.6 Ω + 15.4 jΩ
950 MHz	20.3 dB	51.4 Ω - 9.7 jΩ
960 MHz	16.5 dB	42.9 Ω - 12.1 jΩ

#### 3.2 Antenna Design and Handling


The calibration dipole has a symmetric geometry with a built-in two stub matching network, which leads to the enhanced bandwidth.

The dipole is built of standard semirigid coaxial cable. The internal matching line is open ended. The antenna is therefore open for DC signals.


Do not apply force to dipole arms, as they are liable to bend. The soldered connections near the feedpoint may be damaged. After excessive mechanical stress or overheating, check the impedance characteristics to ensure that the internal matching network is not affected.

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

Page 4 of 8





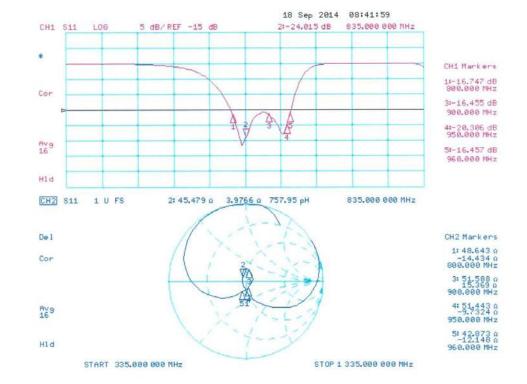

## Impedance Measurement Plot

Page 5 of 8



#### **DASY5 H-field Result**

Date: 17.09.2014

Test Laboratory: SPEAG Lab2

#### DUT: HAC-Dipole 835 MHz; Type: CD835V3; Serial: CD835V3 - SN: 1023

Communication System: UID 0 - CW ; Frequency: 835 MHz Medium parameters used:  $\sigma = 0$  S/m,  $\varepsilon_r = 1$ ;  $\rho = 1$  kg/m<sup>3</sup> Phantom section: RF Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:


- Probe: H3DV6 SN6065; ; Calibrated: 30.12.2013
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn781; Calibrated: 12.09.2014
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole H-Field measurement @ 835MHz/H-Scan - 835MHz d=10mm/Hearing Aid Compatibility Test (41x361x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm Reference Value = 0.4880 A/m; Power Drift = -0.02 dB PMR not calibrated. PMF = 1.000 is applied. H-field emissions = 0.4587 A/m

Near-field category: M4 (AWF 0 dB)

PMF scaled H-field

Grid 1 M4	Grid 2 M4	Grid 3 M4
0.378 A/m	0.400 A/m	0.383 A/m
Grid 4 M4	Grid 5 M4	Grid 6 M4
0.427 A/m	0.459 A/m	0.441 A/m
Grid 7 M4	Grid 8 M4	Grid 9 M4
0.379 A/m	0.410 A/m	0.394 A/m

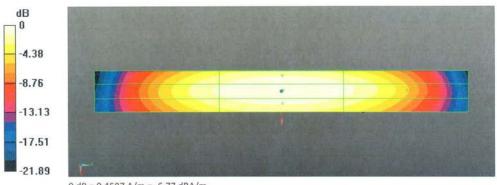

0 dB = 0.4587 A/m = -6.77 dBA/m

Certificate No: CD835V3-1023\_Sep14

Page 6 of 8



# No. I15Z40514-SEM03 Page 46 of 56

## **DASY5 E-field Result**

Date: 17.09.2014

Test Laboratory: SPEAG Lab2

#### DUT: HAC-Dipole 835 MHz; Type: CD835V3; Serial: CD835V3 - SN: 1023

Communication System: UID 0 - CW ; Frequency: 835 MHz Medium parameters used:  $\sigma = 0$  S/m,  $\varepsilon_r = 1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: RF Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ER3DV6 SN2336; ConvF(1, 1, 1); Calibrated: 30.12.2013;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn781; Calibrated: 12.09.2014
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole E-Field measurement @ 835MHz/E-Scan - 835MHz d=10mm/Hearing Aid Compatibility Test (41x361x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm Reference Value = 121.3 V/m; Power Drift = -0.02 dB Applied MIF = 0.00 dB

RF audio interference level = 44.61 dBV/m Emission category: M3

MIF scaled E-field

2012/2012	Grid 2 M3 44.61 dBV/m	
	Grid 5 M4 38.91 dBV/m	Grid 6 M4 38.82 dBV/m
	Grid 8 M3 43.99 dBV/m	and the second second



# No. I15Z40514-SEM03 Page 47 of 56

Dipole E-Field measurement @ 835MHz/E-Scan - 835MHz d=15mm/Hearing Aid Compatibility Test (41x361x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm


Device Reference Point: 0, 0, -6.3 mm

Reference Value = 120.8 V/m; Power Drift = 0.00 dB Applied MIF = 0.00 dB RF audio interference level = 40.70 dBV/m

Emission category: M3

MIF scaled E-field

Grid 1 M3	Grid 2 M3	Grid 3 M3
40.42 dBV/m	40.69 dBV/m	40.6 dBV/m
	Grid 5 M4 36.03 dBV/m	Grid 6 M4 36 dBV/m
1.221.0222.02010.0222.0	Grid 8 M3 40.41 dBV/m	Grid 9 M3 40.35 dBV/m

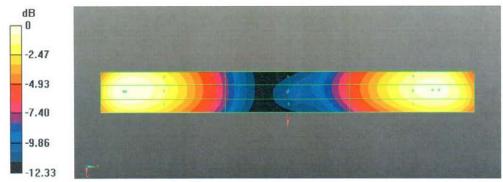

0 dB = 170.0 V/m = 44.61 dBV/m



## Dipole 1880 MHz

Engineering AG ughausstrasse 43, 8004 Zurich	y of n, Switzerland	HAC MRA	Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
credited by the Swiss Accreditation Service	is one of the signatories	to the EA	No.: SCS 108
ultilateral Agreement for the re- ient CTTL (Auden)	cognition of calibration of		CD1880V3-1018_Sep14
CALIBRATION C	CERTIFICATI		
Dbject	CD1880V3 - SN:	1018	
Calibration procedure(s)	QA CAL-20.v6 Calibration proce	dure for dipoles in air	
Calibration date:	September 17, 2	014	
The measurements and the unce	rtainties with confidence p	onal standards, which realize the physical unit robability are given on the following pages and ry facility: environment temperature $(22 \pm 3)^{\circ}C$	d are part of the certificate.
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&	rtainties with confidence p	robability are given on the following pages and	d are part of the certificate.
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards	rtainties with confidence p cted in the closed laborator TE critical for calibration)	robability are given on the following pages and ry facility: environment temperature (22 $\pm$ 3)°C	d are part of the certificate.
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID #	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.)	d are part of the certificate. and humidity < 70%. Scheduled Calibration
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 MY41092317	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01828)	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-14 Oct-14 Oct-14 Oct-14
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Type-N mismatch combination	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5047.2 / 06327	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01828) 03-Apr-14 (No. 217-01921)	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-14 Oct-14 Oct-14 Oct-14 Apr-15
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Fype-N mismatch combination Probe ER3DV6	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5047.2 / 06327 SN: 2336	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01828) 03-Apr-14 (No. 217-01921) 30-Dec-13 (No. ER3-2336_Dec13)	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-14 Oct-14 Oct-14 Oct-14 Apr-15 Dec-14
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Type-N mismatch combination Probe ER3DV6 Probe H3DV6	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5047.2 / 06327	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01828) 03-Apr-14 (No. 217-01921)	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-14 Oct-14 Oct-14 Oct-14 Apr-15
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Type-N mismatch combination Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards	rtainties with confidence p cted in the closed laborator ID # GB37480704 US37292783 MY41092317 SN: 5047.2 / 06327 SN: 2336 SN: 6065 SN: 781 ID #	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01828) Og-Apr-14 (No. 217-01921) 30-Dec-13 (No. ER3-2336_Dec13) 30-Dec-13 (No. ER3-2336_Dec13) 12-Sep-14 (No. DAE4-781_Sep14) Check Date (in house)	d are part of the certificate. c and humidity < 70%. <u>Scheduled Calibration</u> Oct-14 Oct-14 Oct-14 Oct-14 Oct-14 Apr-15 Dec-14 Dec-14 Dec-14 Sep-15 Scheduled Check
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Type-N mismatch combination Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B	rtainties with confidence p cted in the closed laborator ID # GB37480704 US37292783 MY41092317 SN: 5047.2 / 06327 SN: 2036 SN: 0605 SN: 781 ID # ID # SN: GB40202831	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01921) 30-Dec-13 (No. ER3-2336_Dec13) 30-Dec-13 (No. ER3-2336_Dec13) 12-Sep-14 (No. DAE4-781_Sep14) Check Date (in house) 29-Oct-13 (in house check Oct-13)	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-14 Oct-14 Oct-14 Oct-14 Oct-14 Dec-14 Dec-14 Dec-14 Dec-14 Sep-15 Scheduled Check In house check: Oct-15
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Type-N mismatch combination Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP E4412A	rtainties with confidence p cted in the closed laborator ID # GB37480704 US37292783 MY41092317 SN: 5047.2 / 06327 SN: 2336 SN: 6065 SN: 781 ID # ID # SN: GB40202831 SN: MY41498700	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01921) 30-Dec-13 (No. 217-01921) 30-Dec-13 (No. ER3-2336_Dec13) 30-Dec-13 (No. H3-6065_Dec13) 12-Sep-14 (No. DAE4-781_Sep14) Check Date (in house) 29-Oct-13 (in house check Oct-13) 11-Oct-13 (in house check Oct-13)	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-14 Oct-14 Oct-14 Oct-14 Oct-14 Apr-15 Dec-14 Dec-14 Dec-14 Sep-15 Scheduled Check In house check: Oct-15 In house check: Oct-15
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Type-N mismatch combination Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP E4412A Power sensor HP E4412A	rtainties with confidence p cted in the closed laborator ID # GB37480704 US37292783 MY41092317 SN: 5047.2 / 06327 SN: 2036 SN: 0605 SN: 781 ID # ID # SN: GB40202831	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01921) 30-Dec-13 (No. ER3-2336_Dec13) 30-Dec-13 (No. ER3-2336_Dec13) 12-Sep-14 (No. DAE4-781_Sep14) Check Date (in house) 29-Oct-13 (in house check Oct-13)	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-14 Oct-14 Oct-14 Oct-14 Oct-14 Dec-14 Dec-14 Dec-14 Dec-14 Sep-15 Scheduled Check In house check: Oct-15
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Type-N mismatch combination Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP E4412A Power sensor HP E4412A Network Analyzer HP 8753E	rtainties with confidence p cted in the closed laborator ID # GB37480704 US37292783 MY41092317 SN: 5047.2 / 06327 SN: 6065 SN: 761 ID # ID # SN: GB40202831 SN: MY41498700 SN: MY41502623	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01827) Og-Oct-13 (No. 217-01828) Og-Apr-14 (No. 217-01921) 30-Dec-13 (No. ER3-2336_Dec13) 30-Dec-13 (No. H3-6065_Dec13) 12-Sep-14 (No. DAE4-781_Sep14) Check Date (in house) 29-Oct-13 (in house check Oct-13) 11-Oct-13 (in house check Oct-13) 11-Oct-13 (in house check Oct-13)	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-14 Oct-14 Oct-14 Oct-14 Apr-15 Dec-14 Dec-14 Sep-15 Scheduled Check In house check: Oct-15 In house check: Oct-15 In house check: Oct-15
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Type-N mismatch combination Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP E4412A Power sensor HP E4412A Power sensor HP E4412A Network Analyzer HP 8753E RF generator R&S SMT-06	rtainties with confidence p cted in the closed laborator ID # GB37480704 US37292783 MY41092317 SN: 5047.2 / 06327 SN: 5047.2 / 06327 SN: 6065 SN: 781 ID # SN: GB40202831 SN: MY41498700 SN: MY41502623 US37390585 SN: 832283/011 Name	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01828) 03-Apr-14 (No. 217-01921) 30-Dec-13 (No. H3-6065_Dec13) 30-Dec-13 (No. H3-6065_Dec13) 12-Sep-14 (No. DAE4-781_Sep14) Check Date (in house) 29-Oct-13 (in house check Oct-13) 11-Oct-13 (in house check Oct-13) 11-Oct-13 (in house check Oct-13) 18-Oct-01 (in house check Oct-13) 27-Aug-12 (in house check Oct-13)	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-14 Oct-14 Oct-14 Oct-14 Apr-15 Dec-14 Dec-14 Sep-15 Scheduled Check In house check: Oct-15 In house check: Oct-14
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Type-N mismatch combination Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP E4412A Power sensor HP E4412A Power sensor HP E4412A Network Analyzer HP 8753E RF generator R&S SMT-06	rtainties with confidence p cted in the closed laborator ID # GB37480704 US37292783 MY41092317 SN: 5047.2 / 06327 SN: 2336 SN: 6065 SN: 781 ID # SN: GB40202831 SN: MY41498700 SN: MY41502623 US37390585 SN: 832283/011	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01828) 03-Apr-14 (No. 217-01828) 03-Apr-14 (No. 217-01921) 30-Dec-13 (No. H3-6065_Dec13) 12-Sep-14 (No. DAE4-781_Sep14) Check Date (in house) 29-Oct-13 (in house check Oct-13) 11-Oct-13 (in house check Oct-13) 11-Oct-13 (in house check Oct-13) 11-Oct-13 (in house check Oct-13) 18-Oct-01 (in house check Oct-13) 27-Aug-12 (in house check Oct-13)	d are part of the certificate. c and humidity < 70%. C and humidit
The measurements and the unce	rtainties with confidence p cted in the closed laborator ID # GB37480704 US37292783 MY41092317 SN: 5047.2 / 06327 SN: 5047.2 / 06327 SN: 6065 SN: 781 ID # SN: GB40202831 SN: MY41498700 SN: MY41502623 US37390585 SN: 832283/011 Name	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01828) 03-Apr-14 (No. 217-01921) 30-Dec-13 (No. H3-6065_Dec13) 30-Dec-13 (No. H3-6065_Dec13) 12-Sep-14 (No. DAE4-781_Sep14) Check Date (in house) 29-Oct-13 (in house check Oct-13) 11-Oct-13 (in house check Oct-13) 11-Oct-13 (in house check Oct-13) 18-Oct-01 (in house check Oct-13) 27-Aug-12 (in house check Oct-13)	d are part of the certificate. c and humidity < 70%. C and humidit

Certificate No: CD1880V3-1018\_Sep14

Page 1 of 8



## No. I15Z40514-SEM03 Page 49 of 56

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



SWISS

BRA

S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### References

- [1] ANSI-C63.19-2007
  - American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids. ANSI-C63.19-2011
- [2]
  - American National Standard, Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.

#### Methods Applied and Interpretation of Parameters:

- Coordinate System: y-axis is in the direction of the dipole arms. z-axis is from the basis of the antenna (mounted on the table) towards its feed point between the two dipole arms. x-axis is normal to the other axes. In coincidence with the standards [1], the measurement planes (probe sensor center) are selected to be at a distance of 10 mm (15 mm for [2]) above the top metal edge of the dipole arms.
- Measurement Conditions: Further details are available from the hardcopies at the end of the certificate. All
  figures stated in the certificate are valid at the frequency indicated. The forward power to the dipole connector
  is set with a calibrated power meter connected and monitored with an auxiliary power meter connected to a
  directional coupler. While the dipole under test is connected, the forward power is adjusted to the same level.
- Antenna Positioning: The dipole is mounted on a HAC Test Arch phantom using the matching dipole positioner with the arms horizontal and the feeding cable coming from the floor. The measurements are performed in a shielded room with absorbers around the setup to reduce the reflections. It is verified before the mounting of the dipole under the Test Arch phantom, that its arms are perfectly in a line. It is installed on the HAC dipole positioner with its arms parallel below the dielectric reference wire and able to move elastically in vertical direction without changing its relative position to the top center of the Test Arch phantom. The vertical distance to the probe is adjusted after dipole mounting with a DASY5 Surface Check job. Before the measurement, the distance between phantom surface and probe tip is verified. The proper measurement distance is selected by choosing the matching section of the HAC Test Arch phantom with the proper device reference point (upper surface of the dipole) and the matching grid reference point (tip of the probe) considering the probe sensor offset. The vertical distance to the probe is essential for the accuracy.
- Feed Point Impedance and Return Loss: These parameters are measured using a HP 8753E Vector Network Analyzer. The impedance is specified at the SMA connector of the dipole. The influence of reflections was eliminating by applying the averaging function while moving the dipole in the air, at least 70cm away from any obstacles.
- E-field distribution: E field is measured in the x-y-plane with an isotropic ER3D-field probe with 100 mW forward power to the antenna feed point. In accordance with [1] and [2], the scan area is 20mm wide, its length exceeds the dipole arm length (180 or 90mm). The sensor center is 10 mm (15 mm for [2]) (in z) above the metal top of the dipole arms. Two 3D maxima are available near the end of the dipole arms. Assuming the dipole arms are perfectly in one line, the average of these two maxima (in subgrid 2 and subgrid 8) is determined to compensate for any non-parallelity to the measurement plane as well as the sensor displacement. The E-field value stated as calibration value represents the maximum of the interpolated 3D-E-field, in the plane above the dipole surface.
- H-field distribution: H-field is measured with an isotropic H-field probe with 100mW forward power to the
  antenna feed point, in the x-y-plane. The scan area and sensor distance is equivalent to the E-field scan. The
  maximum of the field is available at the center (subgrid 5) above the feed point. The H-field value stated as
  calibration value represents the maximum of the interpolated H-field, 10mm above the dipole surface at the
  feed point.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: CD1880V3-1018\_Sep14



## **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Phantom	HAC Test Arch	
Distance Dipole Top - Probe Center	10 mm	
Scan resolution	dx, dy = 5 mm	
Frequency	1880 MHz ± 1 MHz	
Input power drift	< 0.05 dB	

## Maximum Field values at 1880 MHz

H-field 10 mm above dipole surface	condition	interpolated maximum
Maximum measured	100 mW input power	0.456 A/m ± 8.2 % (k=2)
E-field 10 mm above dipole surface	condition	Interpolated maximum
Maximum measured above high end	100 mW input power	143.0 V/m = 43.11 dBV/m
Maximum measured above low end	100 mW input power	134.6 V/m = 42.58 dBV/m
Averaged maximum above arm	100 mW input power	138.8 V/m ± 12.8 % (k=2)
E-field 15 mm above dipole surface	condition	Interpolated maximum
Maximum measured above high end	100 mW input power	89.5 V/m = 39.04 dBV/m
Maximum measured above low end	100 mW input power	88.9 V/m = 38.97 dBV/m
Averaged maximum above arm	100 mW input power	89.2 V/m ± 12.8 % (k=2)

Page 3 of 8



#### Appendix (Additional assessments outside the scope of SCS108)

#### **Antenna Parameters**

Frequency	Return Loss	Impedance
1730 MHz	27.1 dB	53.3 Ω + 3.2 jΩ
1880 MHz	21.6 dB	49.2 Ω + 8.3 jΩ
1900 MHz	22.9 dB	51.6 Ω + 7.1 jΩ
1950 MHz	32.8 dB	51.4 Ω + 1.9 jΩ
2000 MHz	19.2 dB	41.4 Ω + 5.3 jΩ

#### 3.2 Antenna Design and Handling

The calibration dipole has a symmetric geometry with a built-in two stub matching network, which leads to the enhanced bandwidth.


The dipole is built of standard semirigid coaxial cable. The internal matching line is open ended. The antenna is therefore open for DC signals.

Do not apply force to dipole arms, as they are liable to bend. The soldered connections near the feedpoint may be damaged. After excessive mechanical stress or overheating, check the impedance characteristics to ensure that the internal matching network is not affected.

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.



## Impedance Measurement Plot

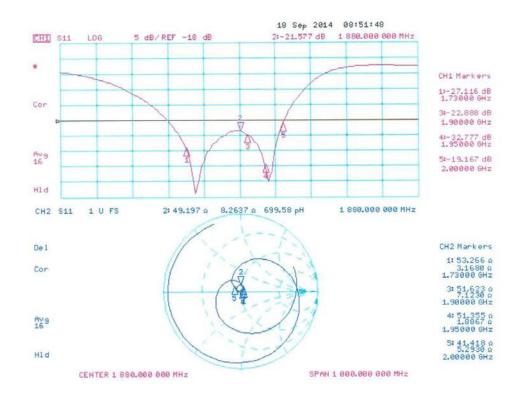

Page 5 of 8



## **DASY5 H-field Result**

Date: 17.09.2014

Test Laboratory: SPEAG Lab2

#### DUT: HAC Dipole 1880 MHz; Type: CD1880V3; Serial: CD1880V3 - SN: 1018

Communication System: UID 0 - CW ; Frequency: 1880 MHz Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 1$  kg/m<sup>3</sup> Phantom section: RF Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:


- Probe: H3DV6 SN6065; ; Calibrated: 30.12.2013
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn781; Calibrated: 12.09.2014
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole H-Field measurement @ 1880MHz/H-Scan - 1880MHz d=10mm/Hearing Aid Compatibility Test (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm Reference Value = 0.4820 A/m; Power Drift = 0.02 dB PMR not calibrated. PMF = 1.000 is applied. H-field emissions = 0.4565 A/m Near-field category: M2 (AWF 0 dB)

PMF scaled H-field

Grid 1 M2	Grid 2 M2	Grid 3 M2
0.394 A/m	0.416 A/m	0.400 A/m
Grid 4 M2	Grid 5 M2	Grid 6 M2
0.431 A/m	0.456 A/m	0.439 A/m
Grid 7 M2	Grid 8 M2	Grid 9 M2
0.394 A/m	0.422 A/m	0.405 A/m

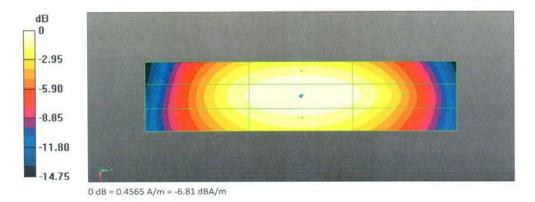

Certificate No: CD1880V3-1018\_Sep14

Page 6 of 8



## **DASY5 E-field Result**

Date: 17.09.2014

Test Laboratory: SPEAG Lab2

## DUT: HAC Dipole 1880 MHz; Type: CD1880V3; Serial: CD1880V3 - SN: 1018

Communication System: UID 0 - CW ; Frequency: 1880 MHz Medium parameters used:  $\sigma = 0$  S/m,  $\varepsilon_r = 1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: RF Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ER3DV6 SN2336; ConvF(1, 1, 1); Calibrated: 30.12.2013;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn781; Calibrated: 12.09.2014
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

# Dipole E-Field measurement @ 1880MHz/E-Scan - 1880MHz d=10mm/Hearing Aid Compatibility Test (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm Reference Value = 141.0 V/m; Power Drift = -0.01 dB Applied MIF = 0.00 dB RF audio interference level = 43.11 dBV/m Emission category: M1

MIF scaled E-field

100000000000000000000000000000000000000	Grid 2 M1 43.11 dBV/m	Grid 3 M1 42.82 dBV/m
	Grid 5 M2 38.77 dBV/m	Grid 6 M2 38.69 dBV/m
	Grid 8 M1 4 <b>2.58 dBV/m</b>	Grid 9 M1 42.44 dBV/m



# No. I15Z40514-SEM03 Page 55 of 56

Dipole E-Field measurement @ 1880MHz/E-Scan - 1880MHz d=15mm/Hearing Aid Compatibility Test (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm


Device Reference Point: 0, 0, -6.3 mm

Reference Value = 140.9 V/m; Power Drift = -0.02 dB Applied MIF = 0.00 dB RF audio interference level = 39.04 dBV/m

Emission category: M2

MIF scaled E-field

	Grid 2 M2 39.04 dBV/m	Grid 3 M2 38.91 dBV/m
and the second se	Grid 5 M2 36.65 dBV/m	Grid 6 M2 36.61 dBV/m
	Grid 8 M2 38.97 dBV/m	Grid 9 M2 38.87 dBV/m

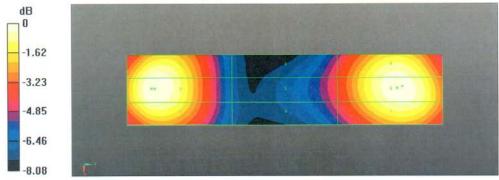

0 dB = 143.0 V/m = 43.11 dBV/m

Page 8 of 8



# The photos of HAC test are presented in the additional document:

Appendix to test report no. I15Z40514-SEM03/04

The photos of HAC test