

# DASY

## Dipole Validation Kit

Type: D5GHzV2

Serial: 1019

Manufactured: February 5, 2004

Calibrated: February 23, 2004

## 1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **head simulating solution** of the following electrical parameters:

Frequency:	<b>5200 MHz</b>	
Relative Dielectricity	<b>36.3</b>	$\pm 5\%$
Conductivity	<b>4.57 mho/m</b>	$\pm 5\%$
Frequency:	<b>5800 MHz</b>	
Relative Dielectricity	<b>35.4</b>	$\pm 5\%$
Conductivity	<b>5.20 mho/m</b>	$\pm 5\%$

The DASY4 System with a dosimetric E-field probe EX3DV3 - SN:3503 was used for the measurements. The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. Lossless spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. Special 8x8x8 fine cube was chosen for cube integration ( $dx=dy=4.3\text{mm}$ ,  $dz=3\text{mm}$ ). Distance between probe sensors and phantom surface was set to 2.5 mm. The dipole input power (forward power) was  $250\text{ mW} \pm 3\%$ . The results are normalized to 1W input power.

## 2. SAR Measurement with DASY System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figures supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured at **5200 MHz (Head Tissue)** with the dosimetric probe EX3DV3 SN:3503 and applying the advanced extrapolation are:

averaged over $1\text{ cm}^3$ (1 g) of tissue:	<b>86.0 mW/g</b> $\pm 20.3\%$ (k=2) <sup>1</sup>
averaged over $10\text{ cm}^3$ (10 g) of tissue:	<b>24.1 mW/g</b> $\pm 19.8\%$ (k=2) <sup>1</sup>

The resulting averaged SAR-values measured at **5800 MHz (Head Tissue)** with the dosimetric probe EX3DV3 SN:3503 and applying the advanced extrapolation are:

averaged over $1\text{ cm}^3$ (1 g) of tissue:	<b>86.8 mW/g</b> $\pm 20.3\%$ (k=2) <sup>2</sup>
averaged over $10\text{ cm}^3$ (10 g) of tissue:	<b>24.4 mW/g</b> $\pm 19.8\%$ (k=2) <sup>2</sup>

<sup>1</sup> Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR\_1g=76.5 mW/g, SAR\_10g=21.6 mW/g and SAR\_peak=310.3 mW/g.

<sup>2</sup> Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR\_1g=78.0 mW/g, SAR\_10g=21.9 mW/g and SAR\_peak=340.9 mW/g.

### 3. Dipole Transformation Parameters

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint (please refer to the graphics attached to this document). The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:	<b>1.200 ns</b>	(one direction)
Transmission factor:	<b>0.974</b>	(voltage transmission, one direction)

### 4. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **body simulating solution** of the following electrical parameters:

Frequency:	<b>5200 MHz</b>	
Relative Dielectricity	<b>49.7</b>	$\pm 5\%$
Conductivity	<b>5.18 mho/m</b>	$\pm 5\%$
Frequency:	<b>5800 MHz</b>	
Relative Dielectricity	<b>48.5</b>	$\pm 5\%$
Conductivity	<b>6.01 mho/m</b>	$\pm 5\%$

The DASY3 System with a dosimetric E-field probe EX3DV3 - SN:3503 was used for the measurements. The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. Lossless spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 8x8x8 fine cube was chosen for cube integration ( $dx=dy=4.3\text{mm}$ ,  $dz=3\text{mm}$ ). Distance between probe sensors and phantom surface was set to 2.5 mm. The dipole input power (forward power) was  $250\text{ mW} \pm 3\%$ . The results are normalized to 1W input power.

## 5. SAR Measurement with DASY System

Standard SAR-measurements were performed according to the measurement conditions described in section 4. The results (see figures supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured at **5200 MHz (Body Tissue)** with the dosimetric probe EX3DV3 SN:3503 and applying the advanced extrapolation are:

averaged over 1 cm<sup>3</sup> (1 g) of tissue: **77.6 mW/g ± 20.3 % (k=2)<sup>3</sup>**

averaged over 10 cm<sup>3</sup> (10 g) of tissue: **21.8 mW/g ± 19.8 % (k=2)<sup>3</sup>**

The resulting averaged SAR-values measured at **5800 MHz (Body Tissue)** with the dosimetric probe EX3DV3 SN:3503 and applying the advanced extrapolation are:

averaged over 1 cm<sup>3</sup> (1 g) of tissue: **75.6 mW/g ± 20.3 % (k=2)<sup>4</sup>**

averaged over 10 cm<sup>3</sup> (10 g) of tissue: **21.0 mW/g ± 19.8 % (k=2)<sup>4</sup>**

## 6. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

## 7. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Small end caps have been added to the dipole arms in order to increase frequency bandwidth at the position as explained in Sections 1 and 4.

## 8. Power Test

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

---

<sup>3</sup> Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR\_1g=71.8 mW/g, SAR\_10g=20.1 mW/g and SAR\_peak=284.7 mW/g.

<sup>4</sup> Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR\_1g=74.1 mW/g, SAR\_10g=20.5 mW/g and SAR\_peak=324.7 mW/g.



Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 5GHz; Serial: D5GHzV2 - SN:1019**

Communication System: CW-5GHz;Duty Cycle: 1:1;Medium: HSL5800

Medium parameters used:  $f = 5200$  MHz;  $\sigma = 4.57$  mho/m;  $\epsilon_r = 36.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Medium parameters used:  $f = 5800$  MHz;  $\sigma = 5.2$  mho/m;  $\epsilon_r = 35.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

DASY4 Configuration:

- Probe: EX3DV3 - SN3503; ConvF(5.7, 5.7, 5.7)  
ConvF(5, 5, 5); Calibrated: 6/27/2003
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Electronics: DAE4 600; Calibrated: 9/30/2003
- Phantom: SAM with CRP - TP:1312; Phantom section: Flat Section
- Measurement SW: DASY4, V4.2 Build 30; Postprocessing SW: SEMCAD, V1.8 Build 98

**d=10mm, Pin=250mW, f=5200 MHz/Area Scan (91x91x1):** Measurement grid: dx=10mm, dy=10mm

Reference Value = 96.8 V/m

Power Drift = 0.0 dB

Maximum value of SAR = 39.6 mW/g

**d=10mm, Pin=250mW, f=5800 MHz 2/Zoom Scan (8x8x8), dist=2.5mm (7x7x8)/Cube 0:**

Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Peak SAR (extrapolated) = 90.4 W/kg


SAR(1 g) = 21.7 mW/g; SAR(10 g) = 6.09 mW/g

**d=10mm, Pin=250mW, f=5200 MHz/Zoom Scan (8x8x8), dist=2.5mm (7x7x8)/Cube 0:**

Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Peak SAR (extrapolated) = 83.1 W/kg

SAR(1 g) = 21.5 mW/g; SAR(10 g) = 6.03 mW/g

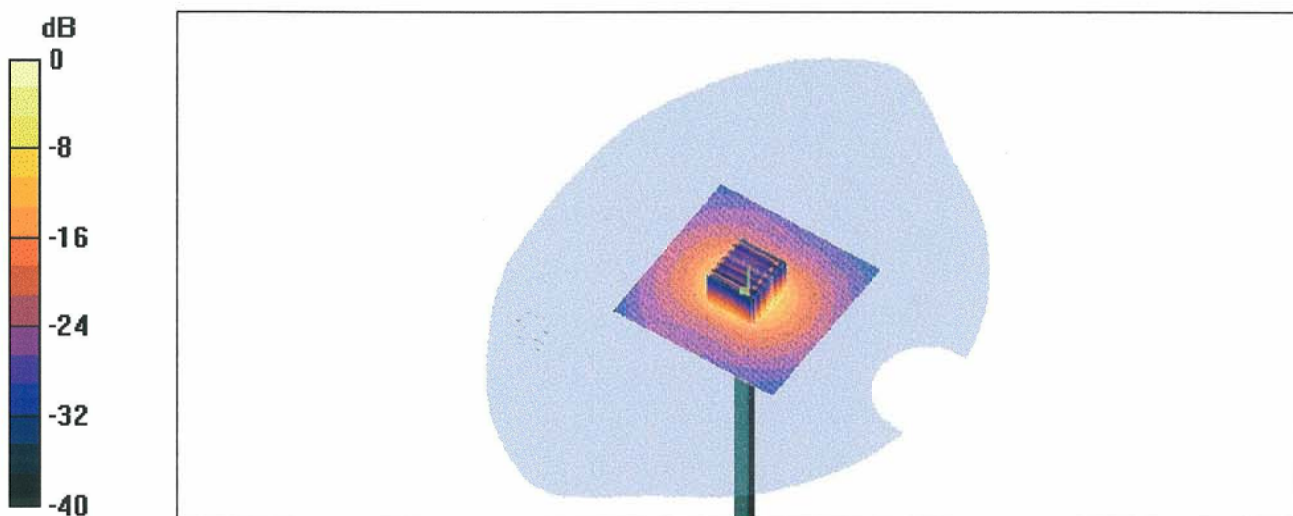


0 dB = 36mW/g

1019  
Head

20 Feb 2004 11:18:09

CH1 S11 1 U FS 2: 47.818  $\Omega$  6.8516  $\Omega$  209.70 pF 5 200.000 000 MHz

De1  
Smo  
Cor

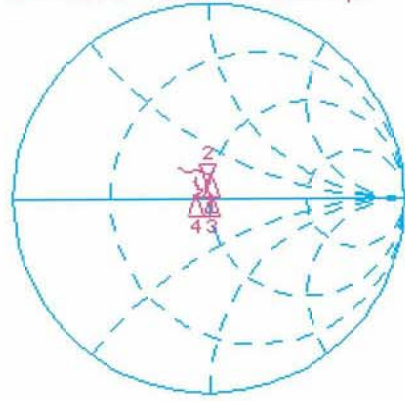

CH1 Markers

- 1: 49.475  $\Omega$   
11.139  $\Omega$   
5.10000 GHz
- 3: 50.738  $\Omega$   
1.1973  $\Omega$   
5.50000 GHz
- 4: 43.486  $\Omega$   
0.6895  $\Omega$   
5.80000 GHz

Avg  
13

↑

CH2 S11 LOG 5 dB/REF -20 dB 2:-22.670 dB 5 200.000 000 MHz

Smo  
Cor

Avg  
13

↑



CH2 Markers

- 1:-19.043 dB  
5.10000 GHz
- 3:-35.803 dB  
5.50000 GHz
- 4:-23.151 dB  
5.80000 GHz

START 4 800.000 000 MHz

STOP 6 000.000 000 MHz

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 5GHz; Serial: D5GHzV2 - SN:1019**

Communication System: CW-5GHz;Duty Cycle: 1:1;Medium: MSL5800

Medium parameters used:  $f = 5200$  MHz;  $\sigma = 5.18$  mho/m;  $\epsilon_r = 49.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Medium parameters used:  $f = 5800$  MHz;  $\sigma = 6.01$  mho/m;  $\epsilon_r = 48.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

DASY4 Configuration:

- Probe: EX3DV3 - SN3503; ConvF(5, 5, 5)  
ConvF(4.6, 4.6, 4.6); Calibrated: 6/27/2003
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Electronics: DAE4 600; Calibrated: 9/30/2003
- Phantom: SAM with CRP - TP:1312; Phantom section: Flat Section
- Measurement SW: DASY4, V4.2 Build 34; Postprocessing SW: SEMCAD, V1.8 Build 105

**d=10mm, Pin=250mW, f=5200 MHz/Area Scan (91x91x1):** Measurement grid: dx=10mm, dy=10mm

Reference Value = 79.9 V/m; Power Drift = -0.002 dB

Maximum value of SAR (interpolated) = 35.3 mW/g

**d=10mm, Pin=250mW, f=5800 MHz/Zoom Scan (8x8x8), dist=2.5mm (7x7x8)/Cube 0:**

Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Peak SAR (extrapolated) = 75.2 W/kg


SAR(1 g) = 18.9 mW/g; SAR(10 g) = 5.25 mW/g

**d=10mm, Pin=250mW, f=5200 MHz/Zoom Scan (8x8x8), dist=2.5mm (7x7x8)/Cube 0:**

Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Peak SAR (extrapolated) = 69.2 W/kg

SAR(1 g) = 19.4 mW/g; SAR(10 g) = 5.45 mW/g

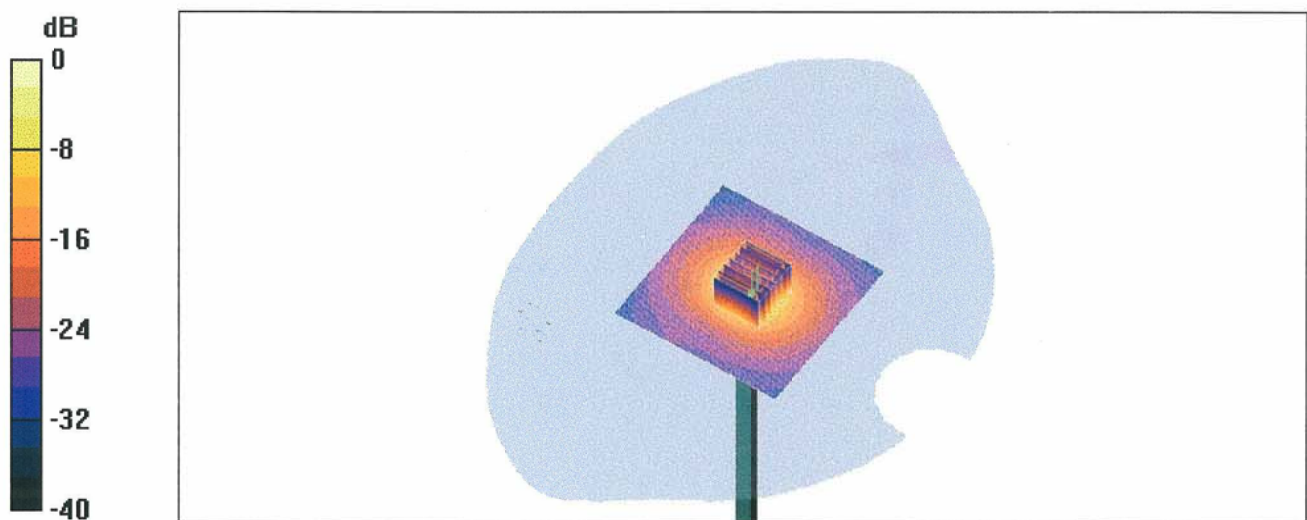

0 dB = 32.6mW/g

1019  
Boody

23 Feb 2004 12:04:44


CH1 S11 1 U FS 3: 49.855  $\Omega$  -916.02 m $\Omega$  33.413 pF 5 200.000 000 MHz

Del

Cor

Avg  
16

↑

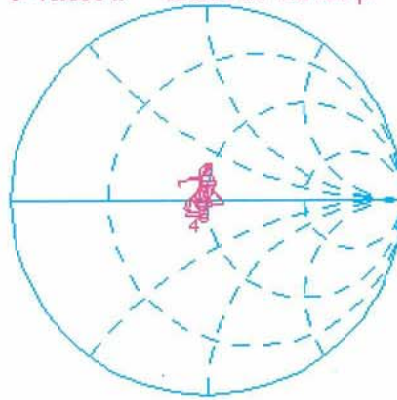

CH1 Markers


- 1: 46.670  $\Omega$   
17.160  $\Omega$   
5.00000 GHz
- 2: 45.758  $\Omega$   
8.1426  $\Omega$   
5.10000 GHz
- 4: 43.258  $\Omega$   
1.5586  $\Omega$   
5.50000 GHz
- 5: 47.248  $\Omega$   
6.5820  $\Omega$   
5.80000 GHz

CH2 S11 L06 5 dB/REF -20 dB 3:-40.131 dB 5 200.000 000 MHz

Cor

Avg  
16

↑

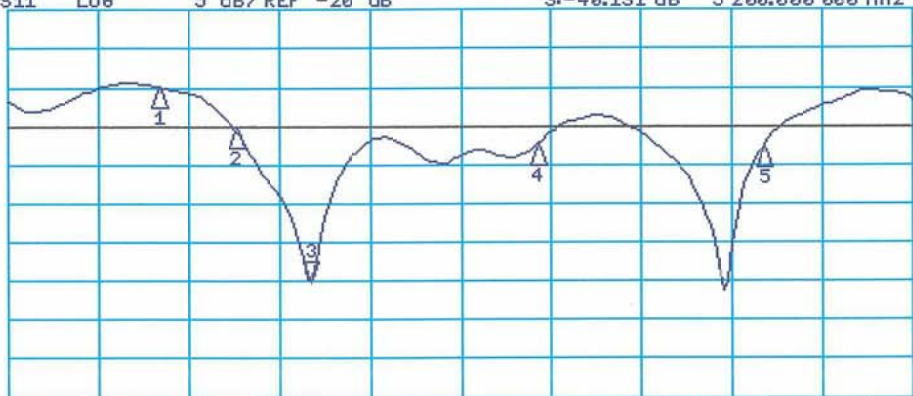

CH2 Markers

- 1:-14.989 dB  
5.00000 GHz
- 2:-20.396 dB  
5.10000 GHz
- 4:-22.588 dB  
5.50000 GHz
- 5:-22.716 dB  
5.80000 GHz





## **D4: 2450MHz SYSTEM VALIDATION DIPOLE**

**Client**      **ADT (Auden)**

**CALIBRATION CERTIFICATE**

**Object(s)**      D2450V2 - SN:716

**Calibration procedure(s)**      QA CAL-05.v2  
Calibration procedure for dipole validation kits

**Calibration date:**      August 23, 2004



**Condition of the calibrated item**      In Tolerance (according to the specific calibration document)

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.

**Calibration Equipment used (M&TE critical for calibration)**

Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter EPM E442	GB37480704	6-Nov-03 (METAS, No. 252-0254)	Nov-04
Power sensor HP 8481A	US37292783	6-Nov-03 (METAS, No. 252-0254)	Nov-04
Power sensor HP 8481A	MY41092317	18-Oct-02 (Agilent, No. 20021018)	Oct-04
RF generator R&S SML-03	100698	27-Mar-2002 (R&S, No. 20-92389)	In house check: Mar-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-03)	In house check: Oct 05

	Name	Function	Signature
<b>Calibrated by:</b>	Judith Mueller	Technician	
<b>Approved by:</b>	Katja Pokovic	Laboratory Director	

Date issued: August 26, 2004

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

# DASY

## Dipole Validation Kit

Type: D2450V2

Serial: 716

Manufactured: September 10, 2002

Calibrated: August 23, 2004